
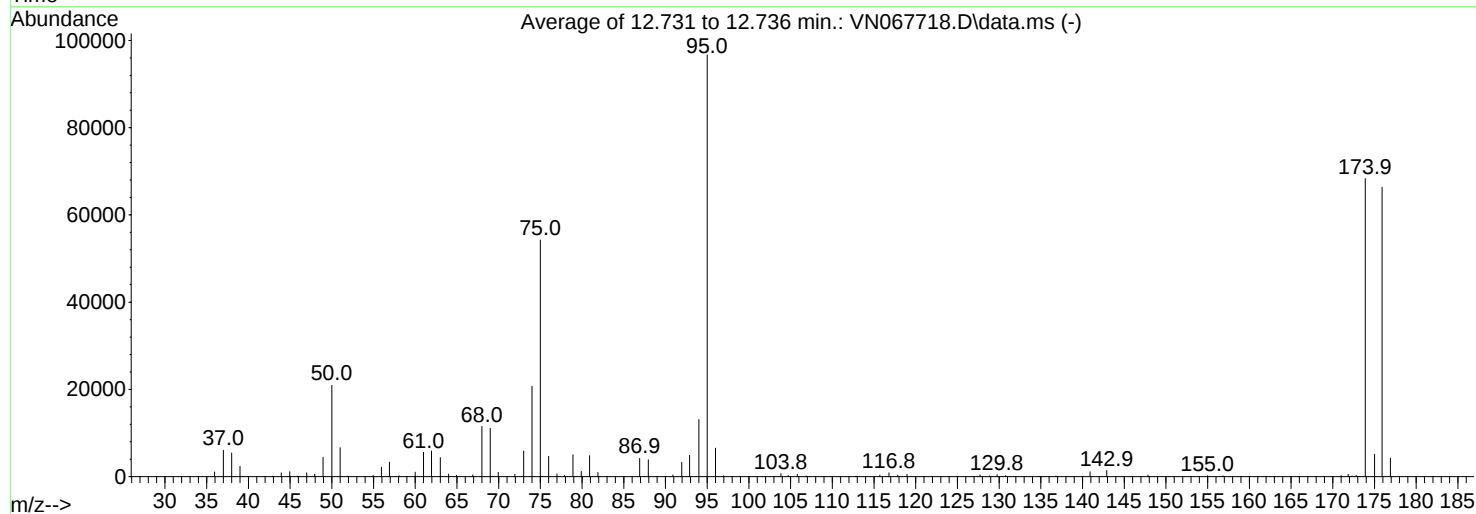


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071421\
 Data File : VN067718.D
 Acq On : 13 Jul 2021 15:34
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N071421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jul 14 01:19:19 2021

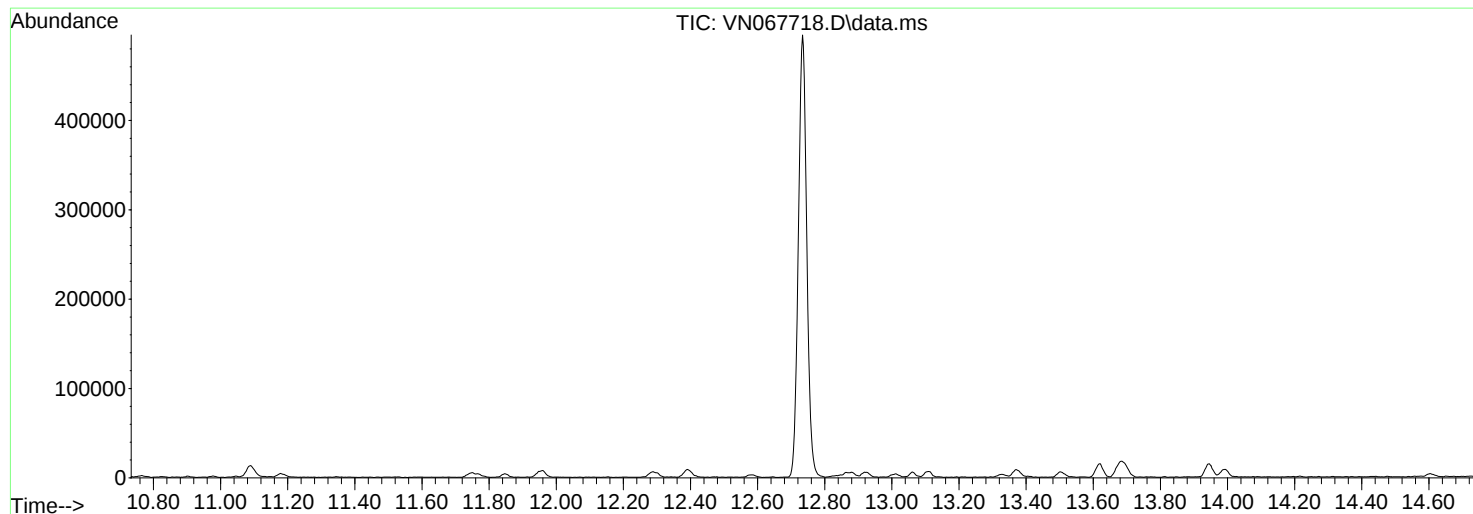

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	20952	PASS
75	95	30	60	56.1	54264	PASS
95	95	100	100	100.0	96699	PASS
96	95	5	9	6.8	6539	PASS
173	174	0.00	2	0.4	306	PASS
174	95	50	100	70.7	68341	PASS
175	174	5	9	7.5	5139	PASS
176	174	95	101	97.1	66373	PASS
177	176	5	9	6.4	4260	PASS