


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071421\
 Data File : VN067732.D
 Acq On : 14 Jul 2021 8:51
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N071421W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Wed Jul 14 01:19:19 2021

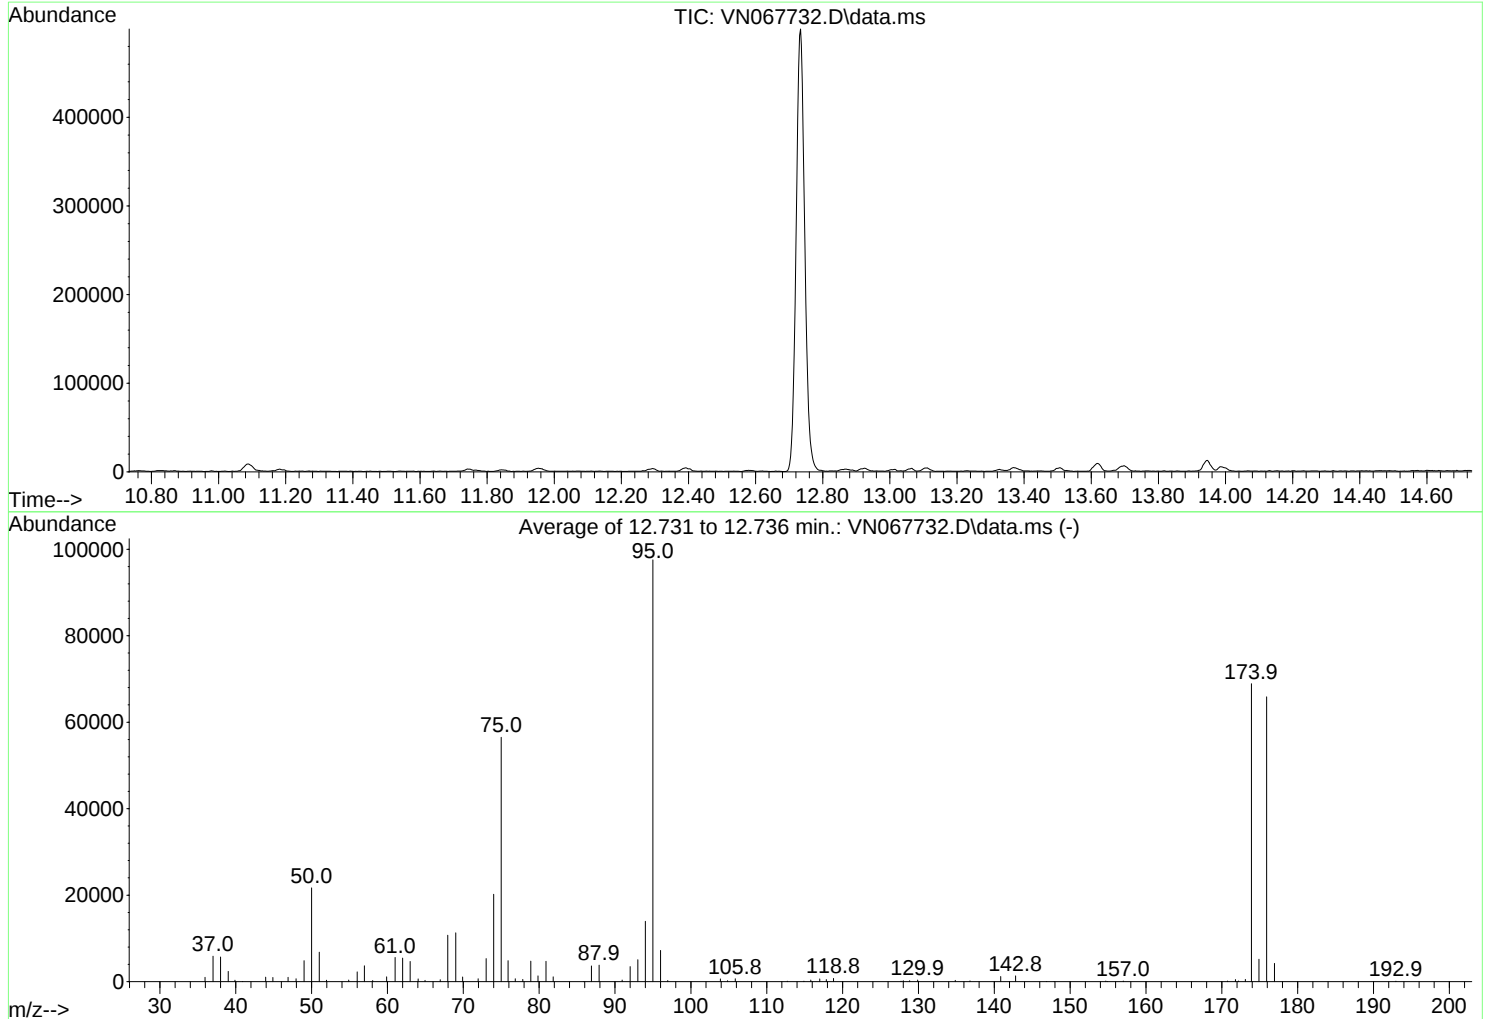

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3989

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	21699	PASS
75	95	30	60	57.9	56517	PASS
95	95	100	100	100.0	97549	PASS
96	95	5	9	7.4	7233	PASS
173	174	0.00	2	0.8	520	PASS
174	95	50	100	70.6	68896	PASS
175	174	5	9	7.5	5201	PASS
176	174	95	101	95.6	65880	PASS
177	176	5	9	6.4	4236	PASS