

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071422\
 Data File : VN073470.D
 Acq On : 14 Jul 2022 19:06
 Operator : JC\MD
 Sample : N3697-02 100X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 CASING-NUMBER-5D-WATERING

Quant Time: Jul 15 02:03:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.016	168	270988	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.904	114	461629	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	428563	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	198306	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	181117	46.298	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	92.600%
35) Dibromofluoromethane	7.951	113	149067	48.536	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.080%
50) Toluene-d8	10.381	98	488120	44.748	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.500%
62) 4-Bromofluorobenzene	12.669	95	207186	49.425	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.840%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071422\
Data File : VN073470.D
Acq On : 14 Jul 2022 19:06
Operator : JC\MD
Sample : N3697-02 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
CASING-NUMBER-5D-WATERING

Quant Time: Jul 15 02:03:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




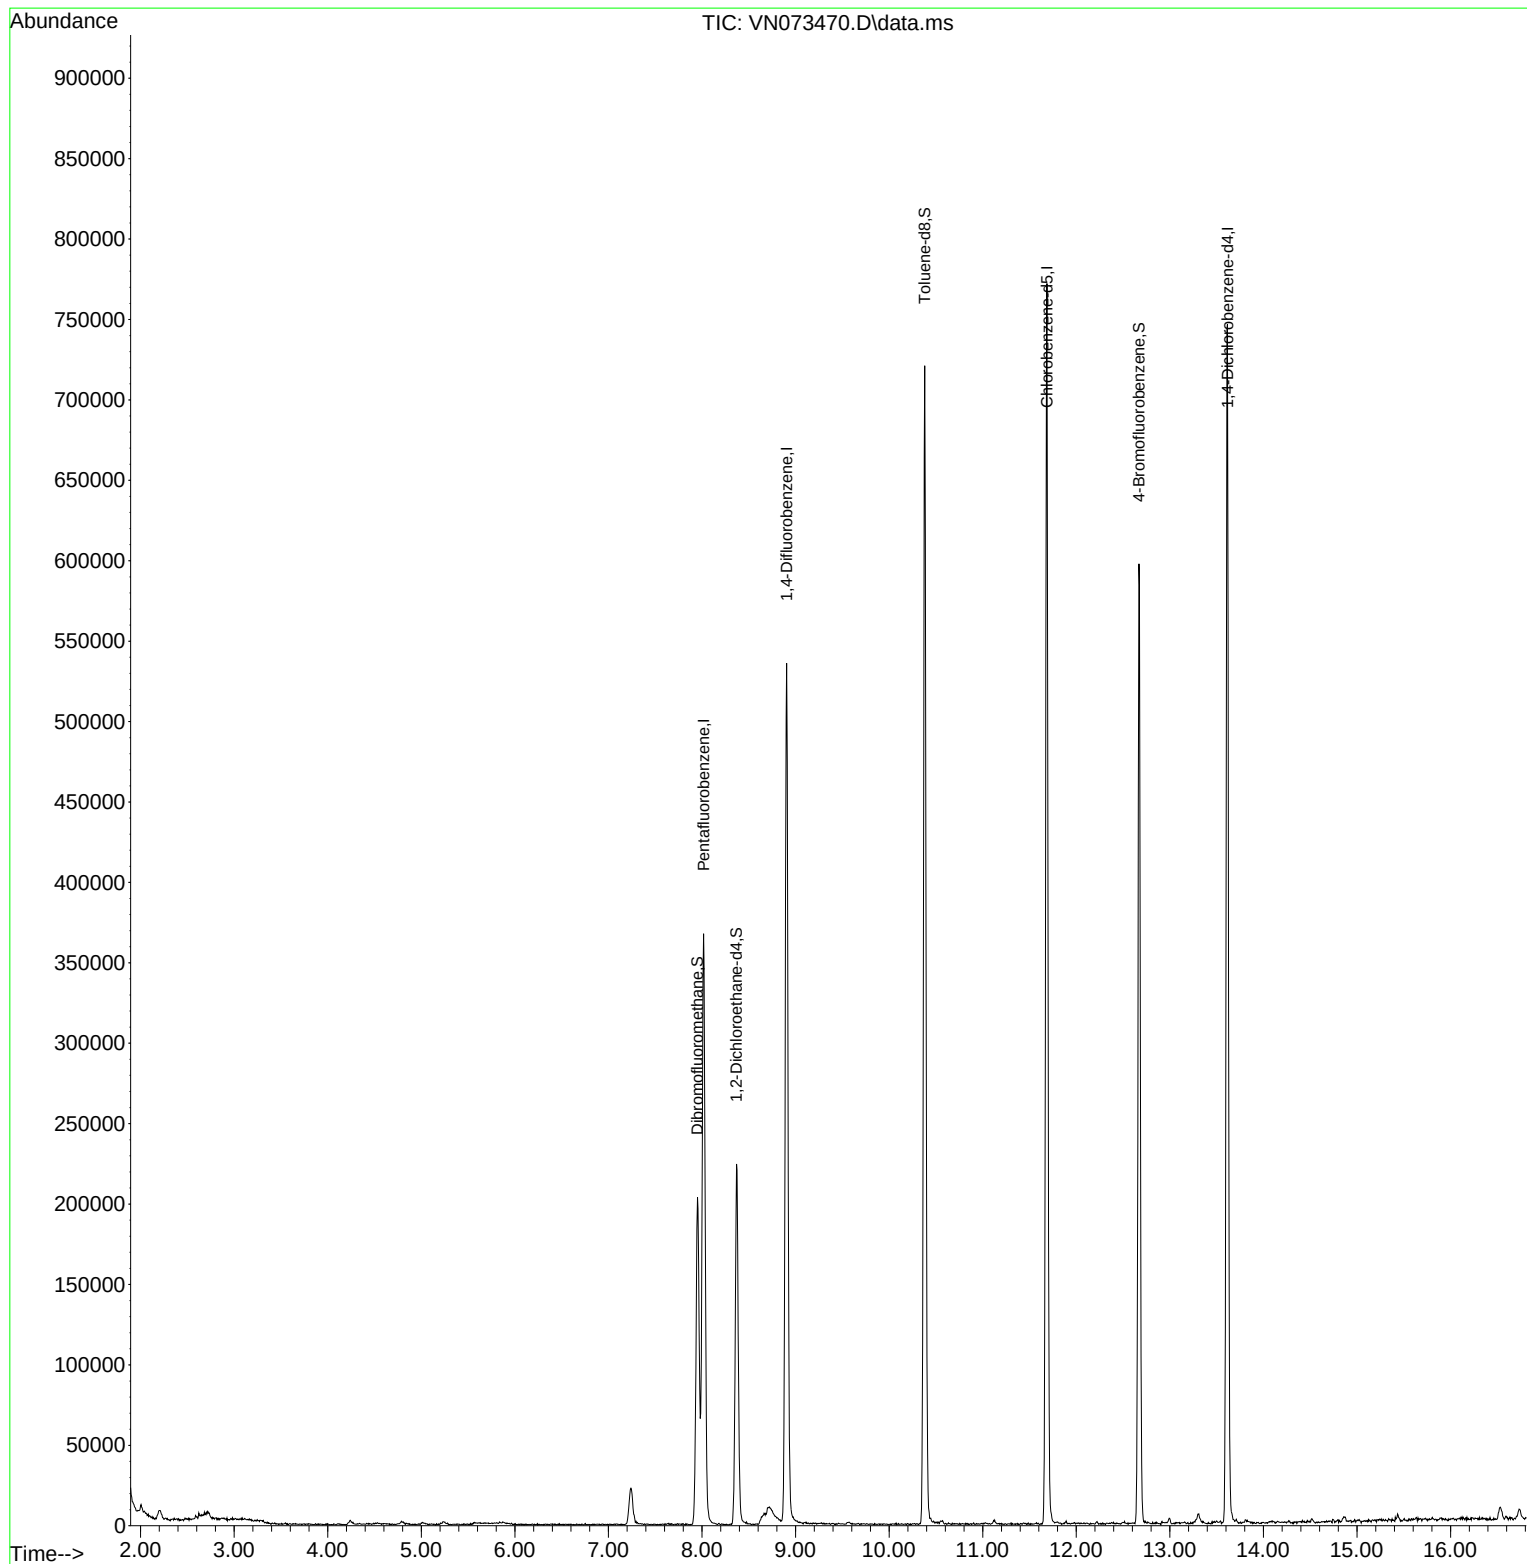


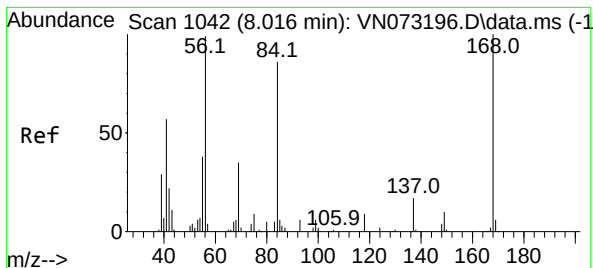

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073470.D
Acq: 14 Jul 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
CASING-NUMBER-5D-WATERING


Tgt Ion:168 Resp: 270988
Ion Ratio Lower Upper
168 100
99 59.9 42.3 63.5

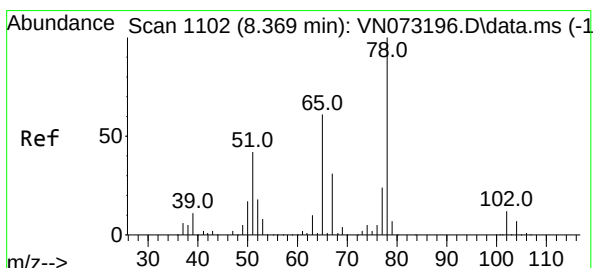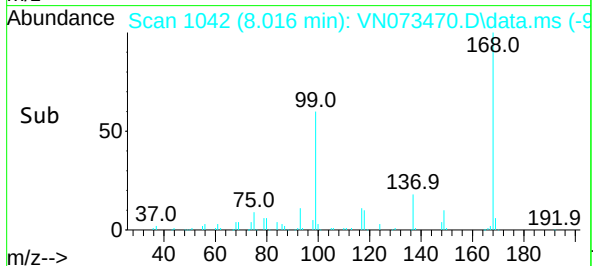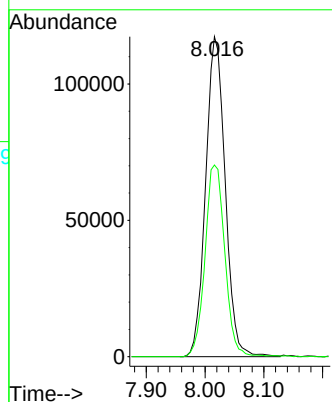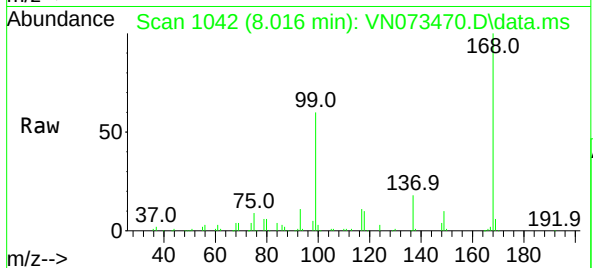

#33
1,2-Dichloroethane-d4
Concen: 46.298 ug/l
RT: 8.369 min Scan# 1102
Delta R.T. -0.000 min
Lab File: VN073470.D
Acq: 14 Jul 2022 19:06

Tgt Ion: 65 Resp: 181117
Ion Ratio Lower Upper
65 100
67 52.9 0.0 104.8

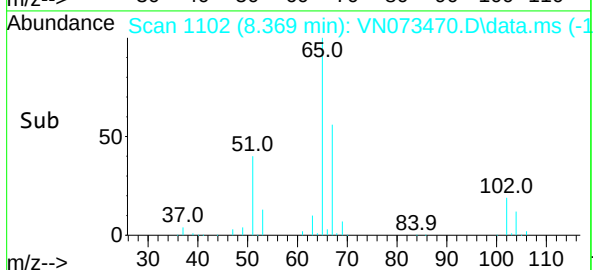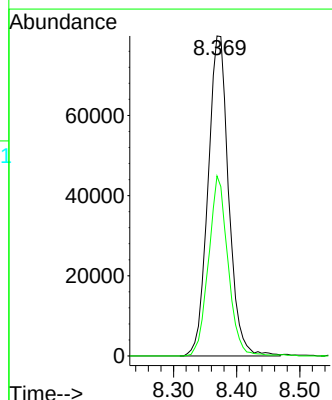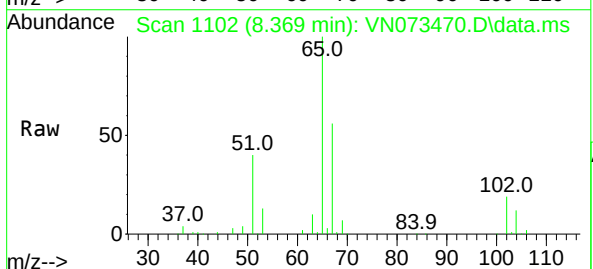

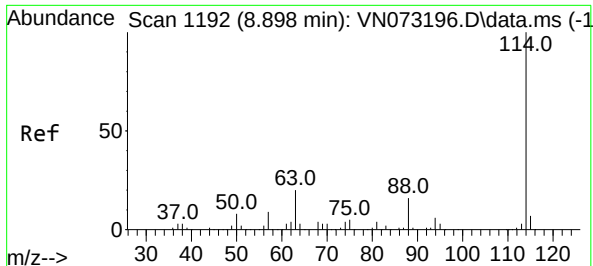

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073470.D

Acq: 14 Jul 2022 19:06

Instrument :

MSVOA_N

ClientSampleId :

CASING-NUMBER-5D-WATERING





Tgt Ion:114 Resp: 461629

Ion Ratio Lower Upper

114 100

63 21.2 0.0 40.0

88 15.5 0.0 32.6

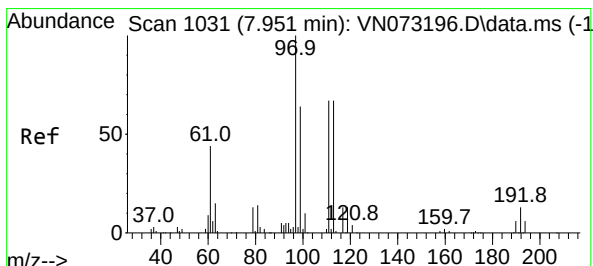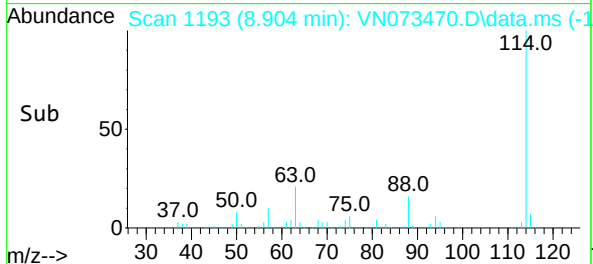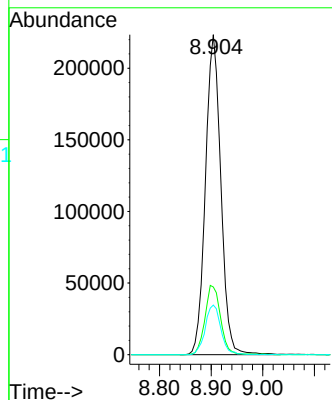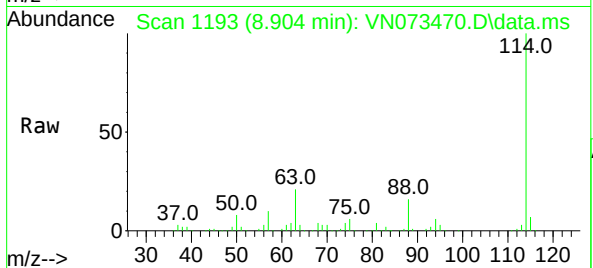

#35

Dibromofluoromethane

Concen: 48.536 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073470.D

Acq: 14 Jul 2022 19:06




Tgt Ion:113 Resp: 149067


Ion Ratio Lower Upper

113 100

111 104.6 81.4 122.0

192 18.7 17.0 25.6


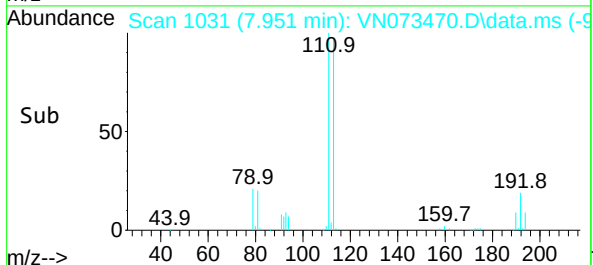
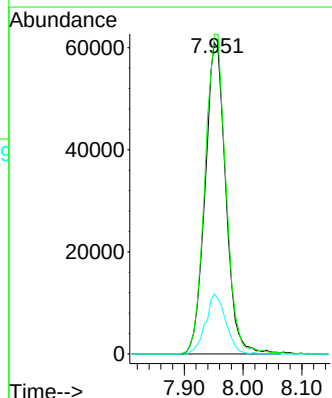
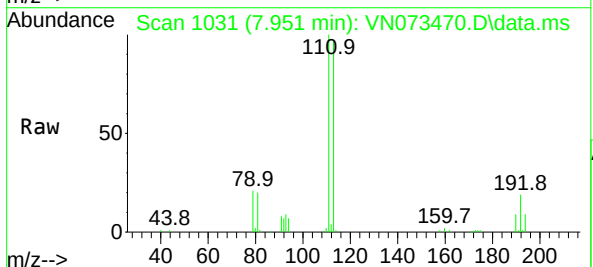


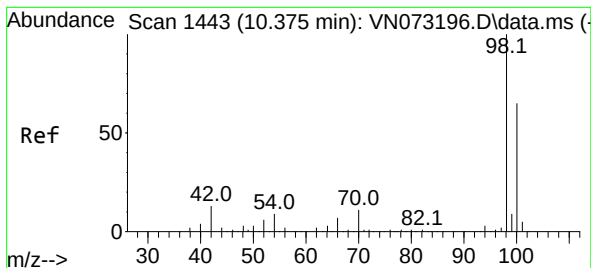

#50
Toluene-d8
Concen: 44.748 ug/l
RT: 10.381 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VN073470.D
Acq: 14 Jul 2022 19:06




Instrument :
MSVOA_N
ClientSampleId :
CASING-NUMBER-5D-WATERING


Tgt Ion: 98 Resp: 488120
Ion Ratio Lower Upper
98 100
100 65.3 52.6 78.8

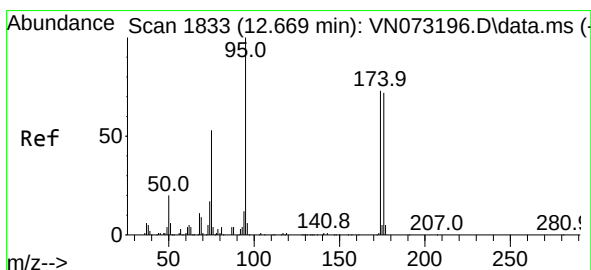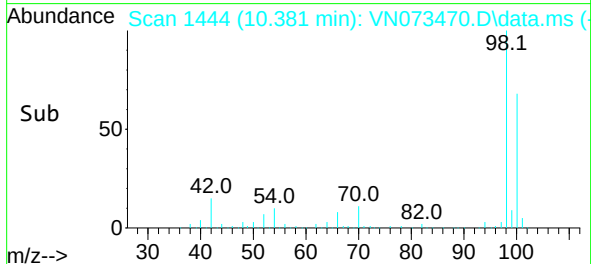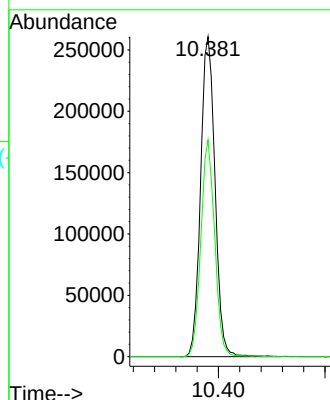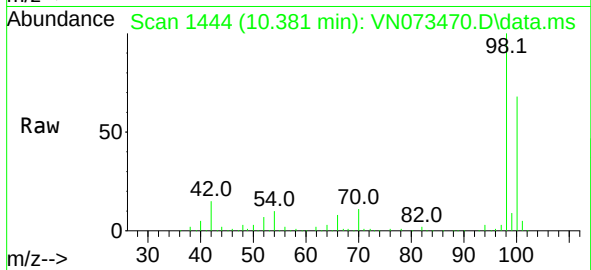

#62
4-Bromofluorobenzene
Concen: 49.425 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073470.D
Acq: 14 Jul 2022 19:06

Tgt Ion: 95 Resp: 207186
Ion Ratio Lower Upper
95 100
174 74.5 0.0 167.6
176 70.0 0.0 163.4


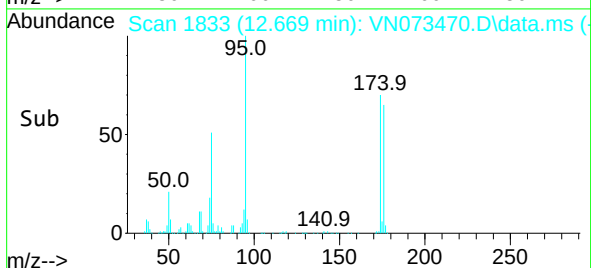
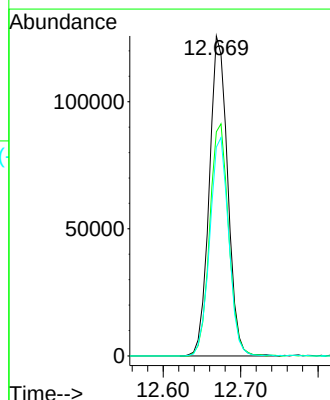
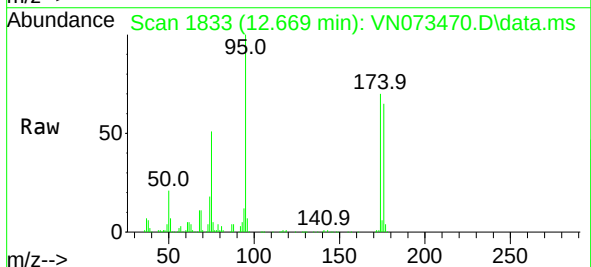


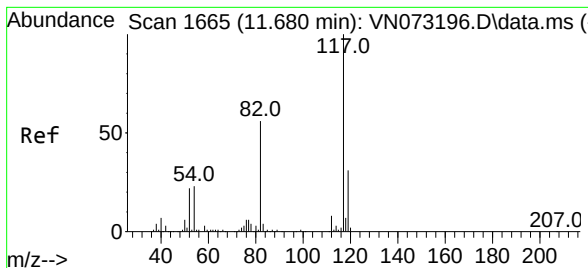

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1166
Delta R.T. 0.006 min
Lab File: VN073470.D
Acq: 14 Jul 2022 19:06

Instrument :
MSVOA_N
ClientSampleId :
CASING-NUMBER-5D-WATERING

Tgt Ion:117 Resp: 428563
Ion Ratio Lower Upper
117 100
82 56.0 44.2 66.2
119 33.0 25.4 38.0

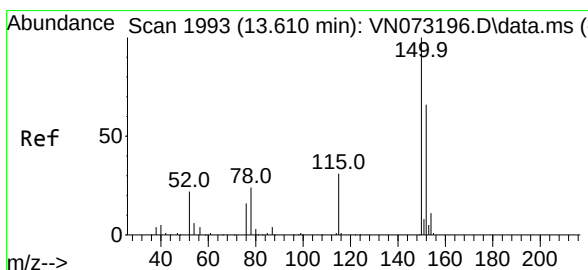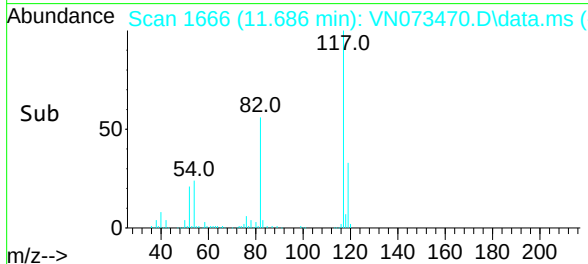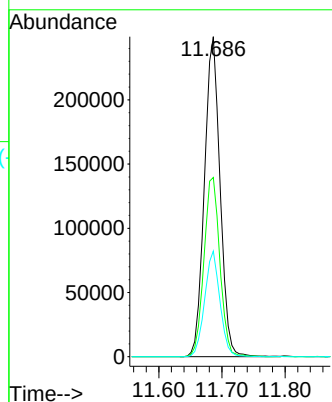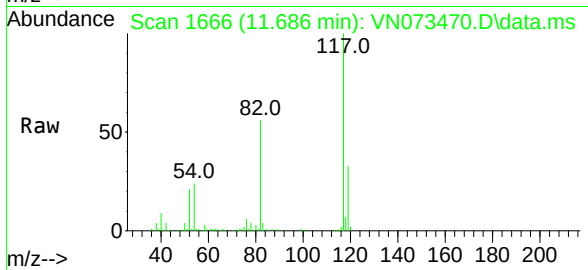

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.006 min
Lab File: VN073470.D
Acq: 14 Jul 2022 19:06

Tgt Ion:152 Resp: 198306
Ion Ratio Lower Upper
152 100
115 61.2 28.9 86.7
150 159.0 0.0 356.2

