
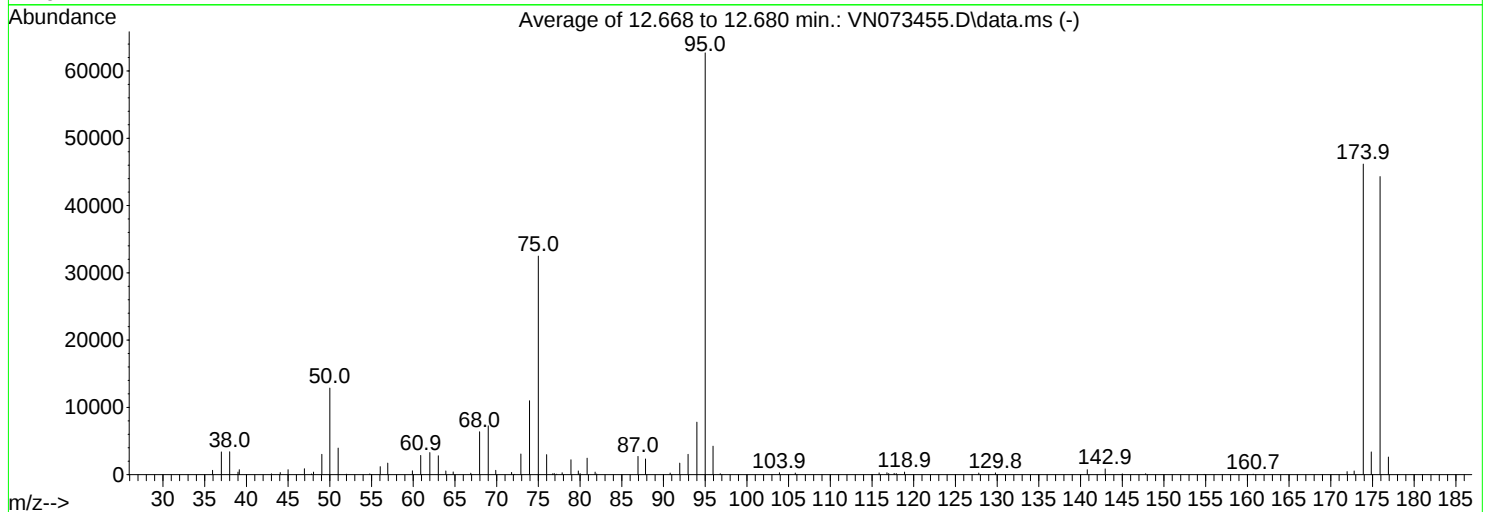


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071422\
Data File : VN073455.D
Acq On : 14 Jul 2022 11:20
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 01:54:03 2022

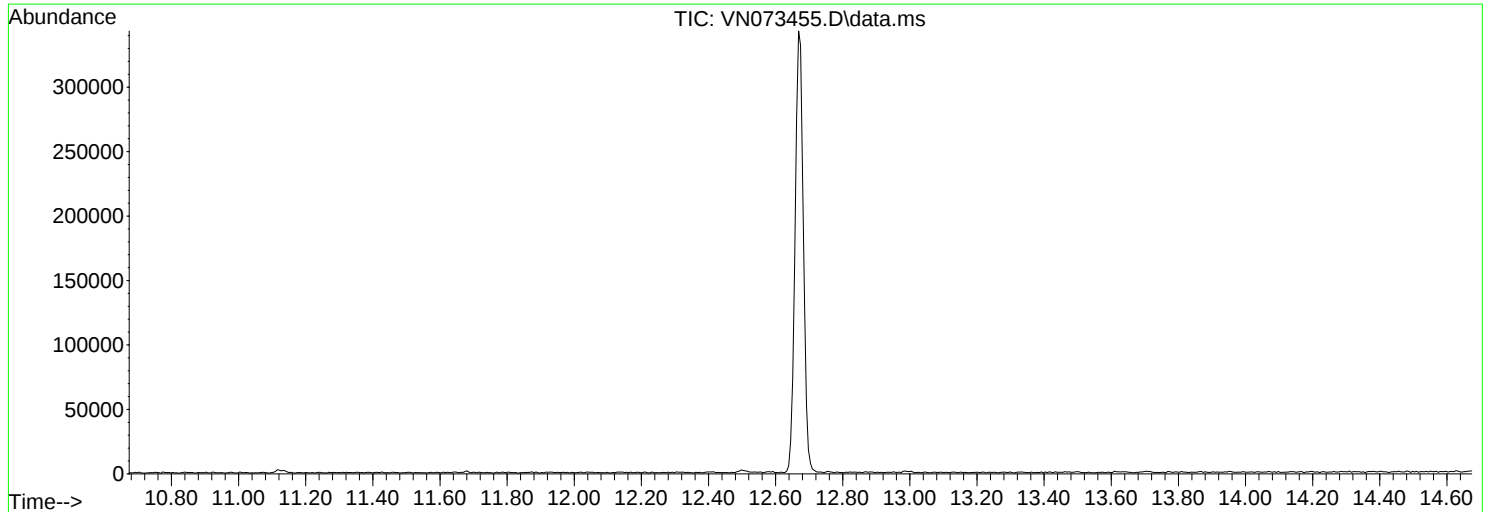

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.5	12864	PASS
75	95	30	60	51.8	32480	PASS
95	95	100	100	100.0	62693	PASS
96	95	5	9	6.7	4230	PASS
173	174	0.00	2	1.2	540	PASS
174	95	50	100	73.6	46152	PASS
175	174	5	9	7.3	3382	PASS
176	174	95	101	96.0	44299	PASS
177	176	5	9	5.9	2615	PASS