
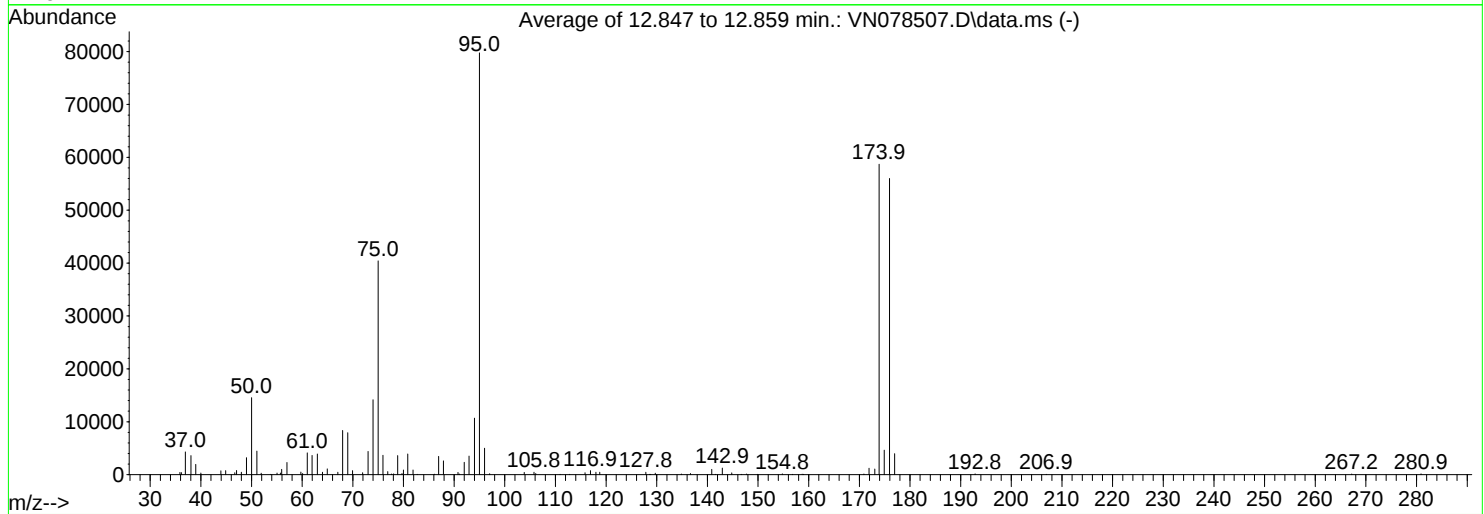


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071423\
Data File : VN078507.D
Acq On : 14 Jul 2023 08:35
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

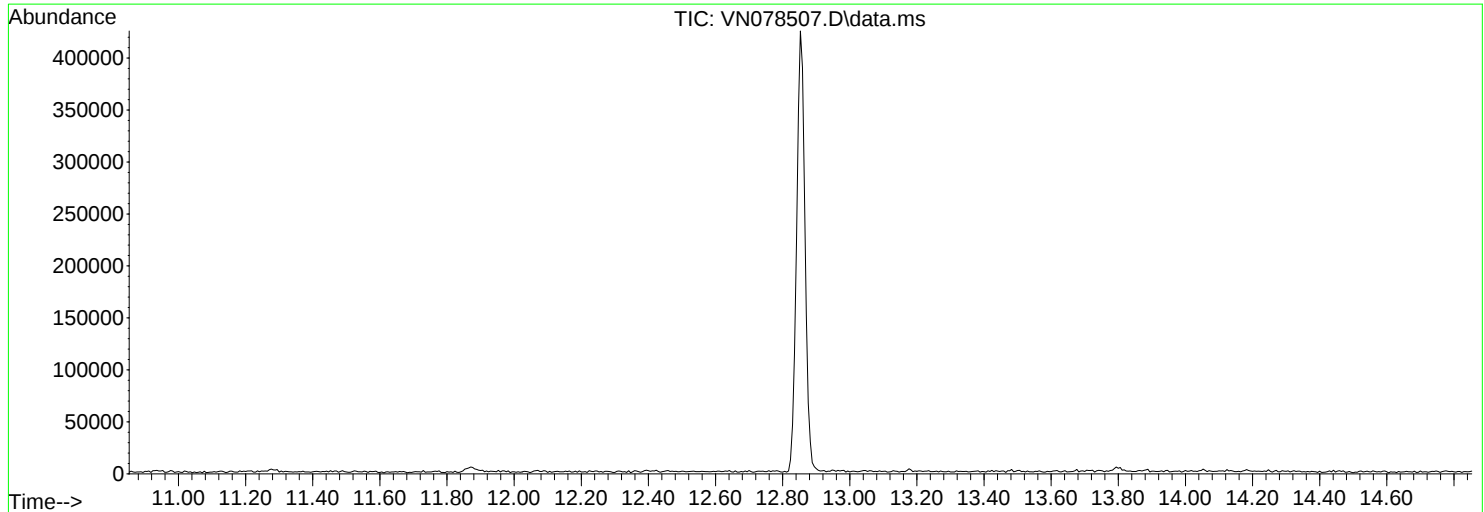

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	14555	PASS
75	95	30	60	50.7	40437	PASS
95	95	100	100	100.0	79763	PASS
96	95	5	9	6.2	4980	PASS
173	174	0.00	2	1.8	1057	PASS
174	95	50	100	73.6	58701	PASS
175	174	5	9	7.9	4631	PASS
176	174	95	101	95.4	55995	PASS
177	176	5	9	7.1	3959	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	417	49.00	3215	61.00	4105	74.00	1416
36.15	388	50.00	14555	61.95	3625	75.00	4043
36.95	4303	51.05	4445	63.00	3901	75.95	365
38.05	3611	51.90	291	64.00	443	76.90	56
39.00	1948	53.80	62	64.95	1083	77.65	130
40.00	293	55.05	302	67.05	467	78.05	152
43.95	742	55.70	303	68.00	8352	78.85	3592
44.90	761	55.95	1010	69.00	7927	79.70	223
46.70	372	57.00	2291	69.95	771	80.00	888
47.05	784	59.75	482	71.95	363	80.85	3898
48.00	458	60.10	208	73.00	4403	81.90	882

Average of 12.847 to 12.859 min.: VN078507.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
82.70	61	97.00	189	128.60	67	149.90	52
86.10	82	103.85	433	128.80	61	154.80	163
86.95	3446	105.75	461	129.70	279	156.80	54
87.90	2598	106.10	219	134.85	114	158.70	97
90.75	422	110.90	52	136.65	210	159.00	56
91.00	116	112.80	52	140.85	1007	170.90	134
92.00	2337	115.85	377	141.60	67	171.90	1219
92.95	3518	116.90	747	142.95	1231	173.05	1057
94.00	10673	118.00	466	144.80	334	173.90	58701
95.00	79763	118.75	459	146.70	58	174.90	4631
96.00	4980	127.85	447	147.75	128	175.95	55995

Average of 12.847 to 12.859 min.: VN078507.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.95	3959						
192.85	140						
206.90	69						
267.20	137						
280.90	146						

Instrument :

MSVOA_N

ClientSampleId :

BFB