



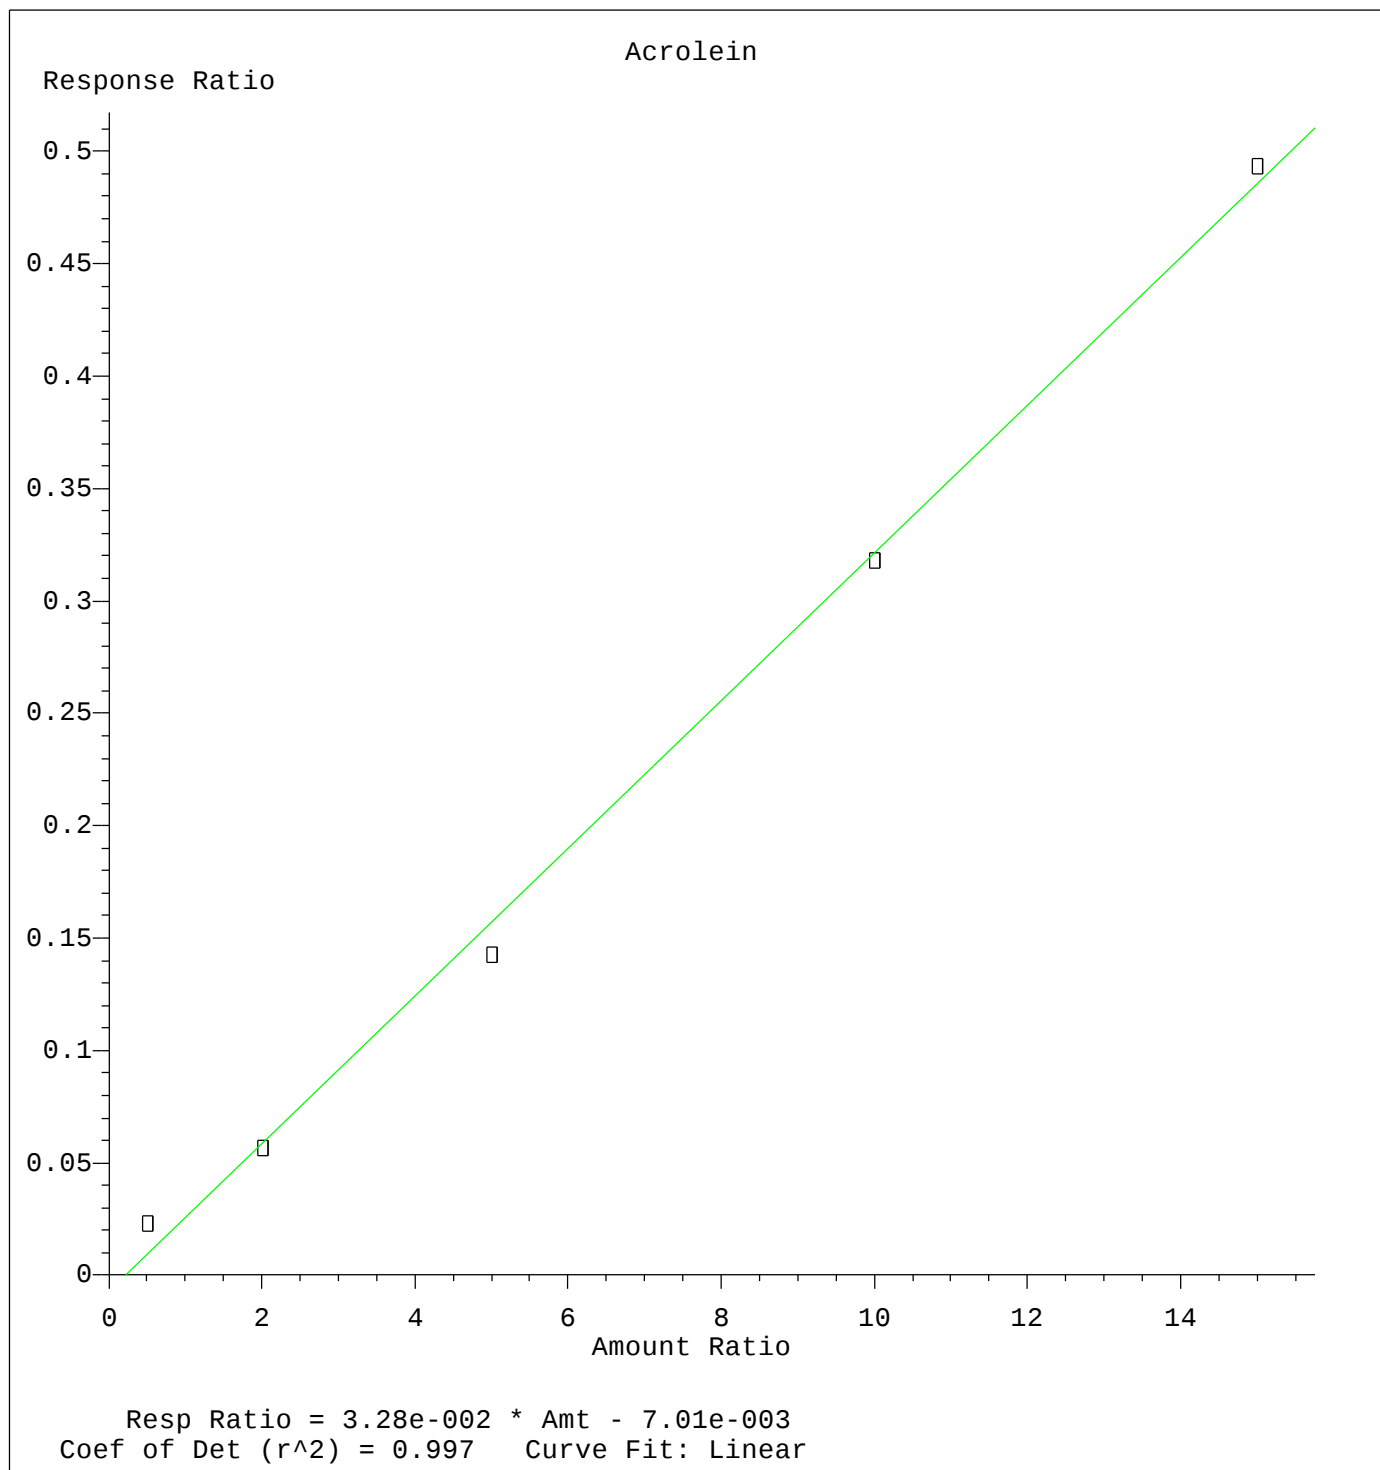


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

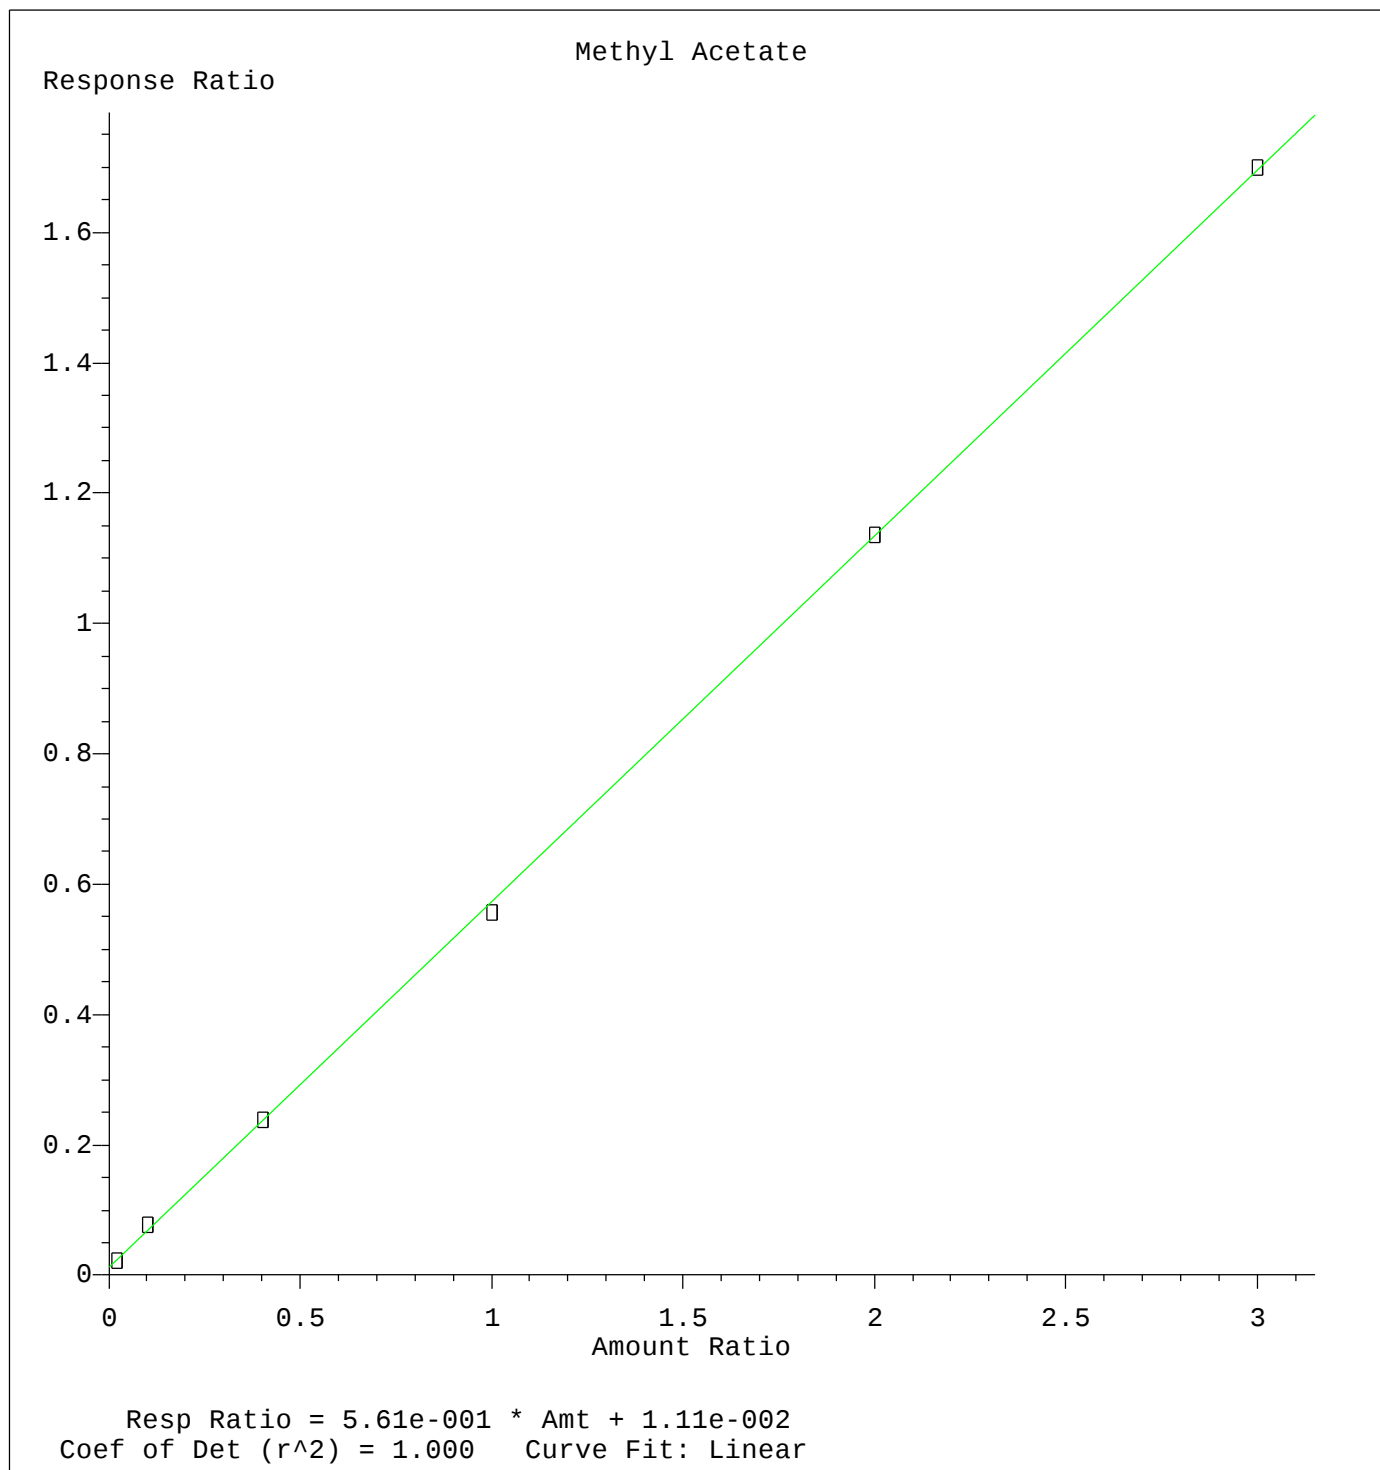

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

1,1,2,2-Tetrachloroethane

Response Ratio

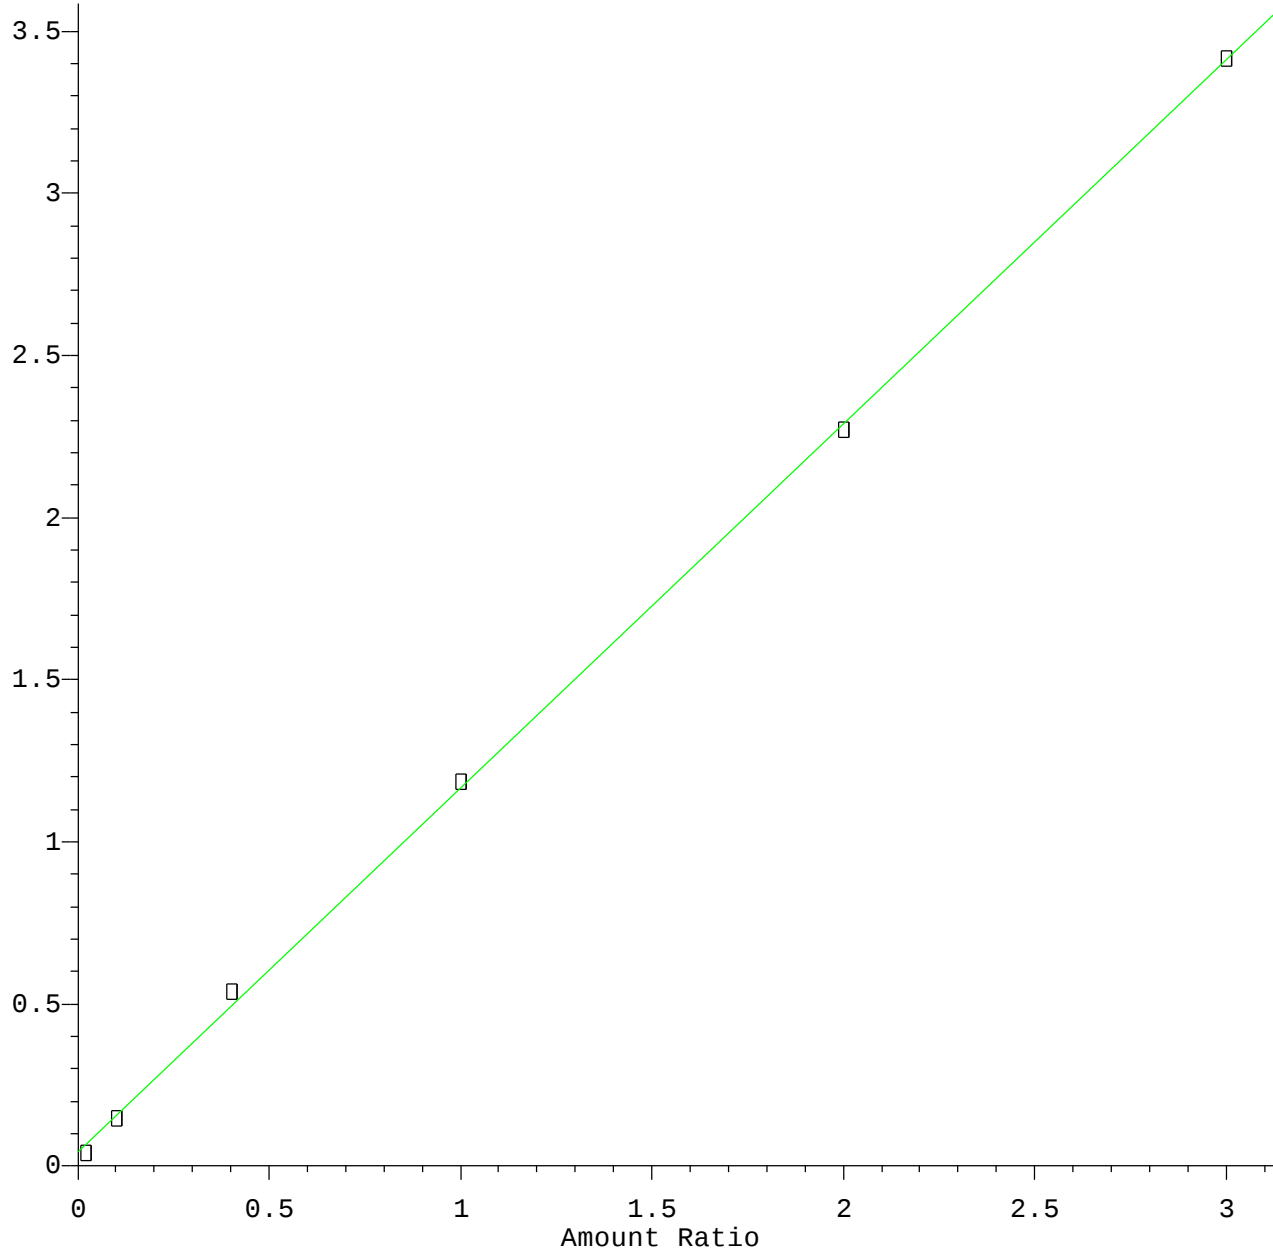


Resp Ratio = 1.12×10^0 * Amt + 4.54×10^{-2}
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

2-Chlorotoluene

Response Ratio

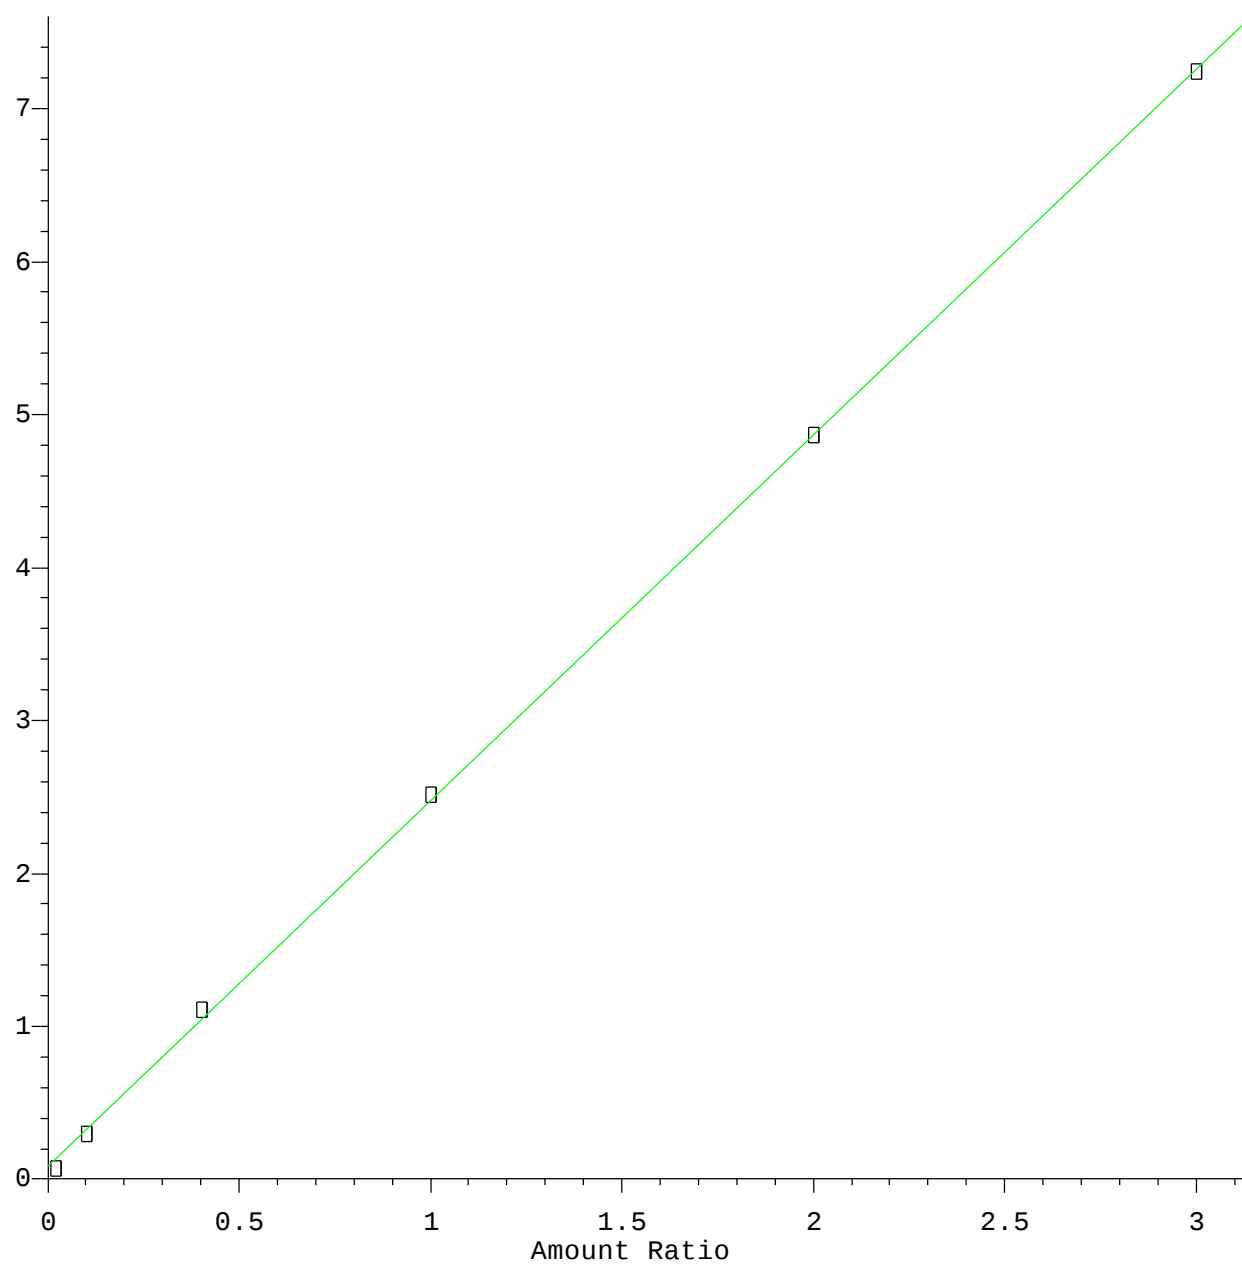


Resp Ratio = 2.39e+000 * Amt + 8.11e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

tert-Butylbenzene

Response Ratio

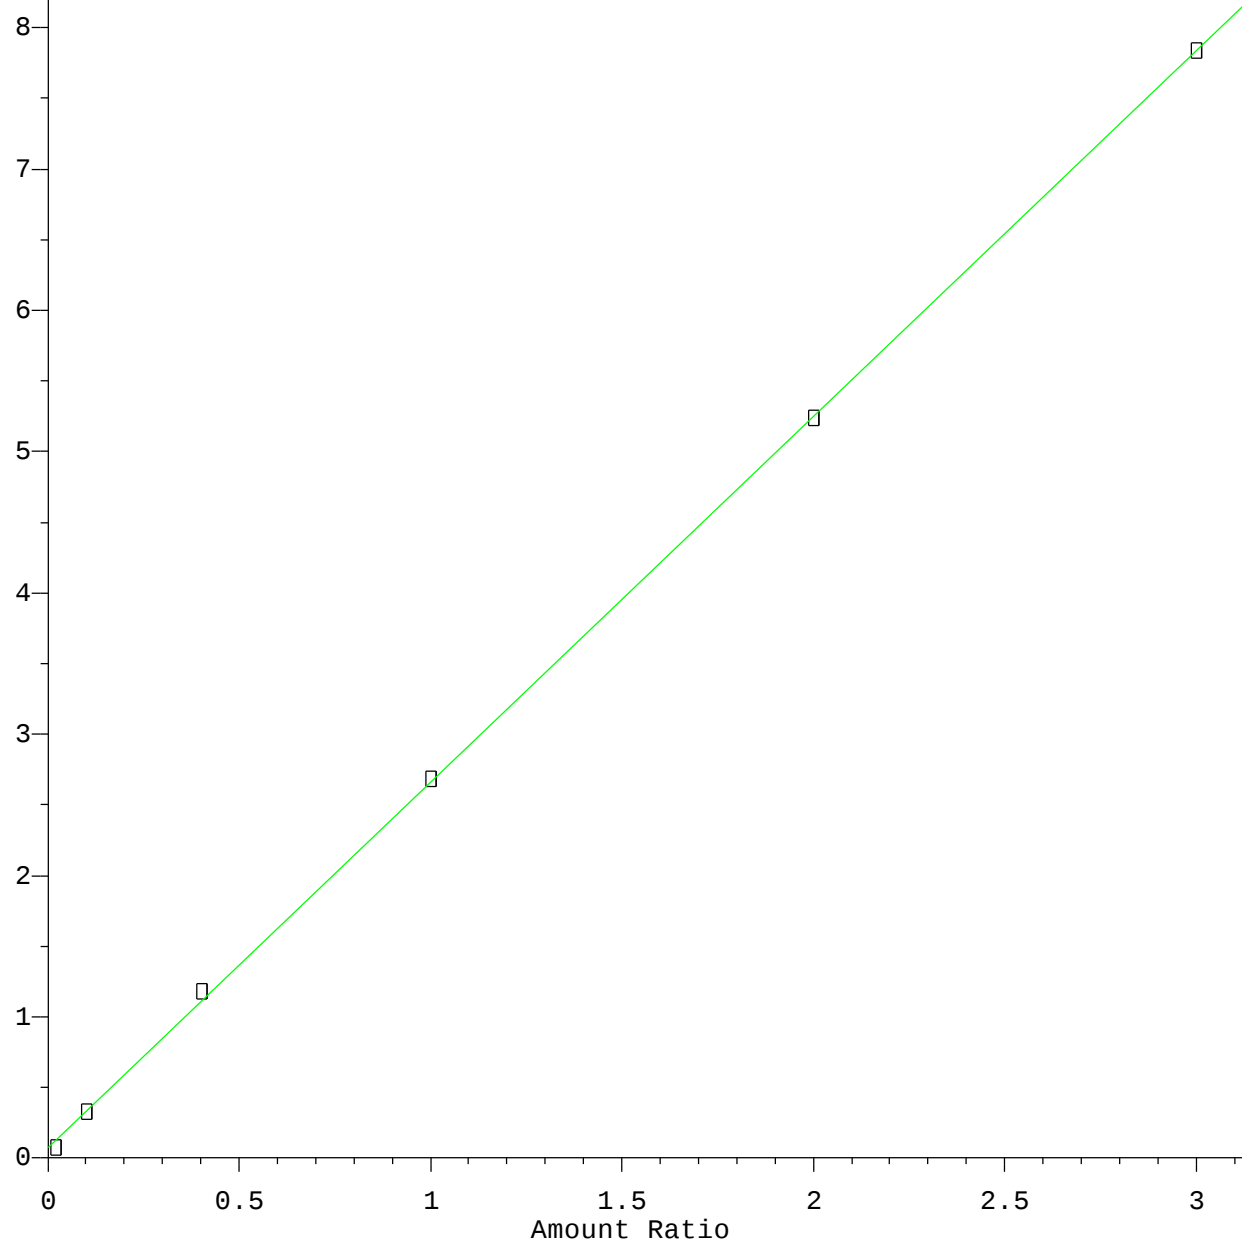


Resp Ratio = 2.59e+000 * Amt + 7.69e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019


1,2,4-Trichlorobenzene

Response Ratio

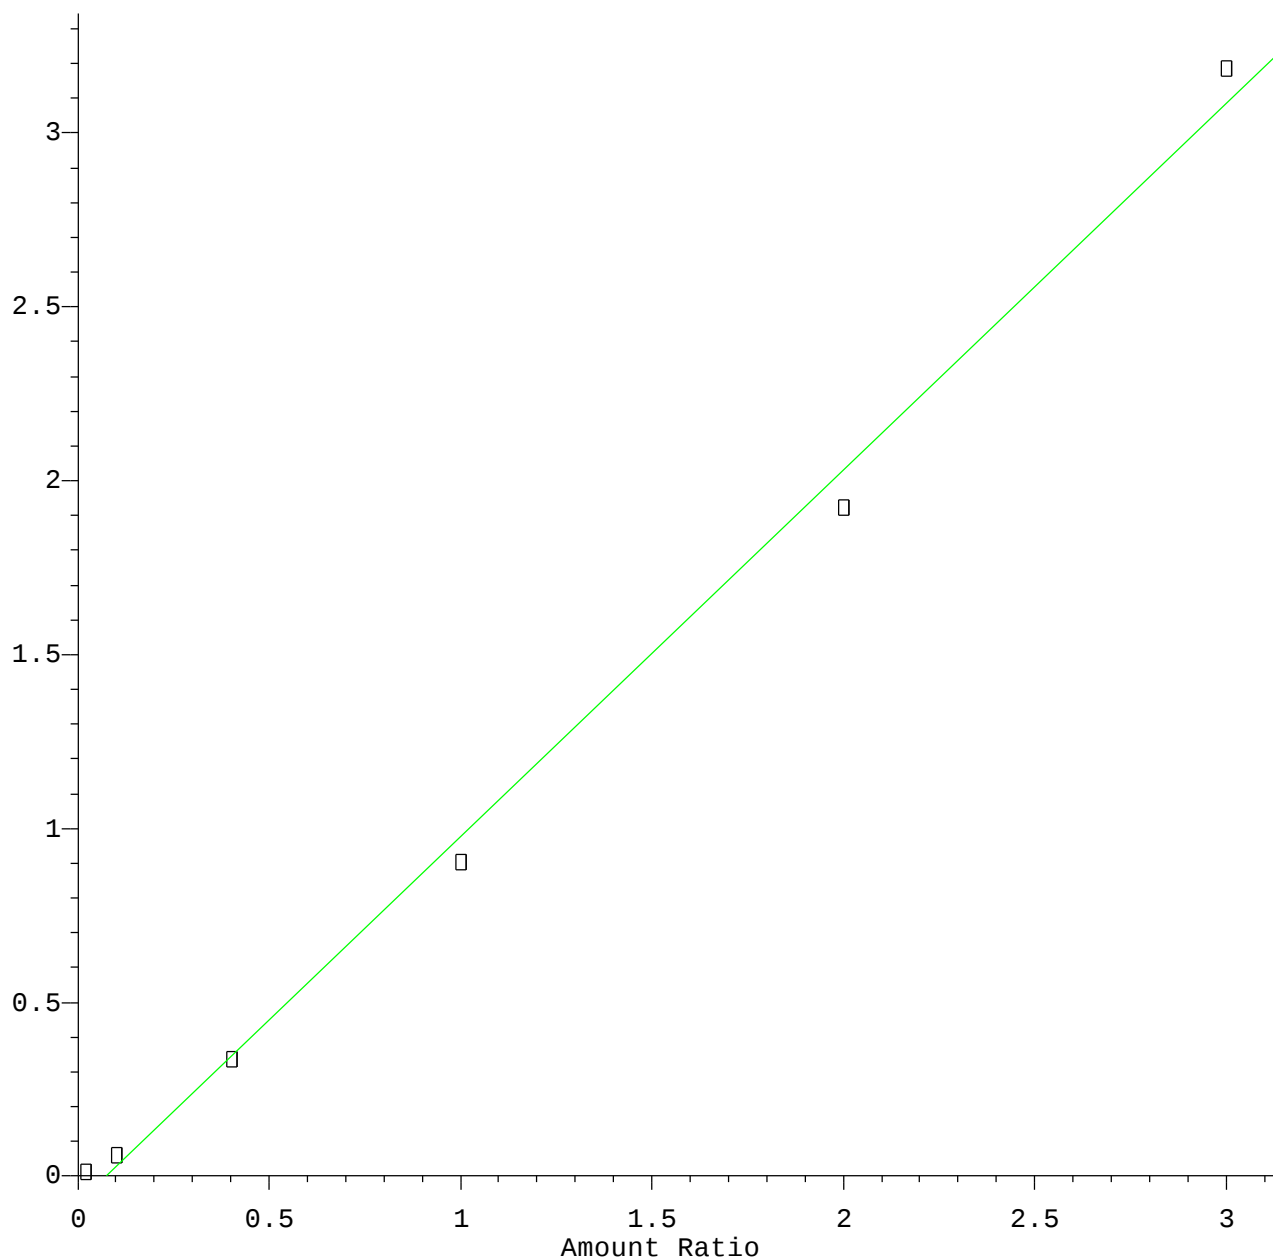

Resp Ratio = $1.05 \times 10^0 \times \text{Amt} - 7.78 \times 10^{-2}$
Coef of Det (r^2) = 0.996 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

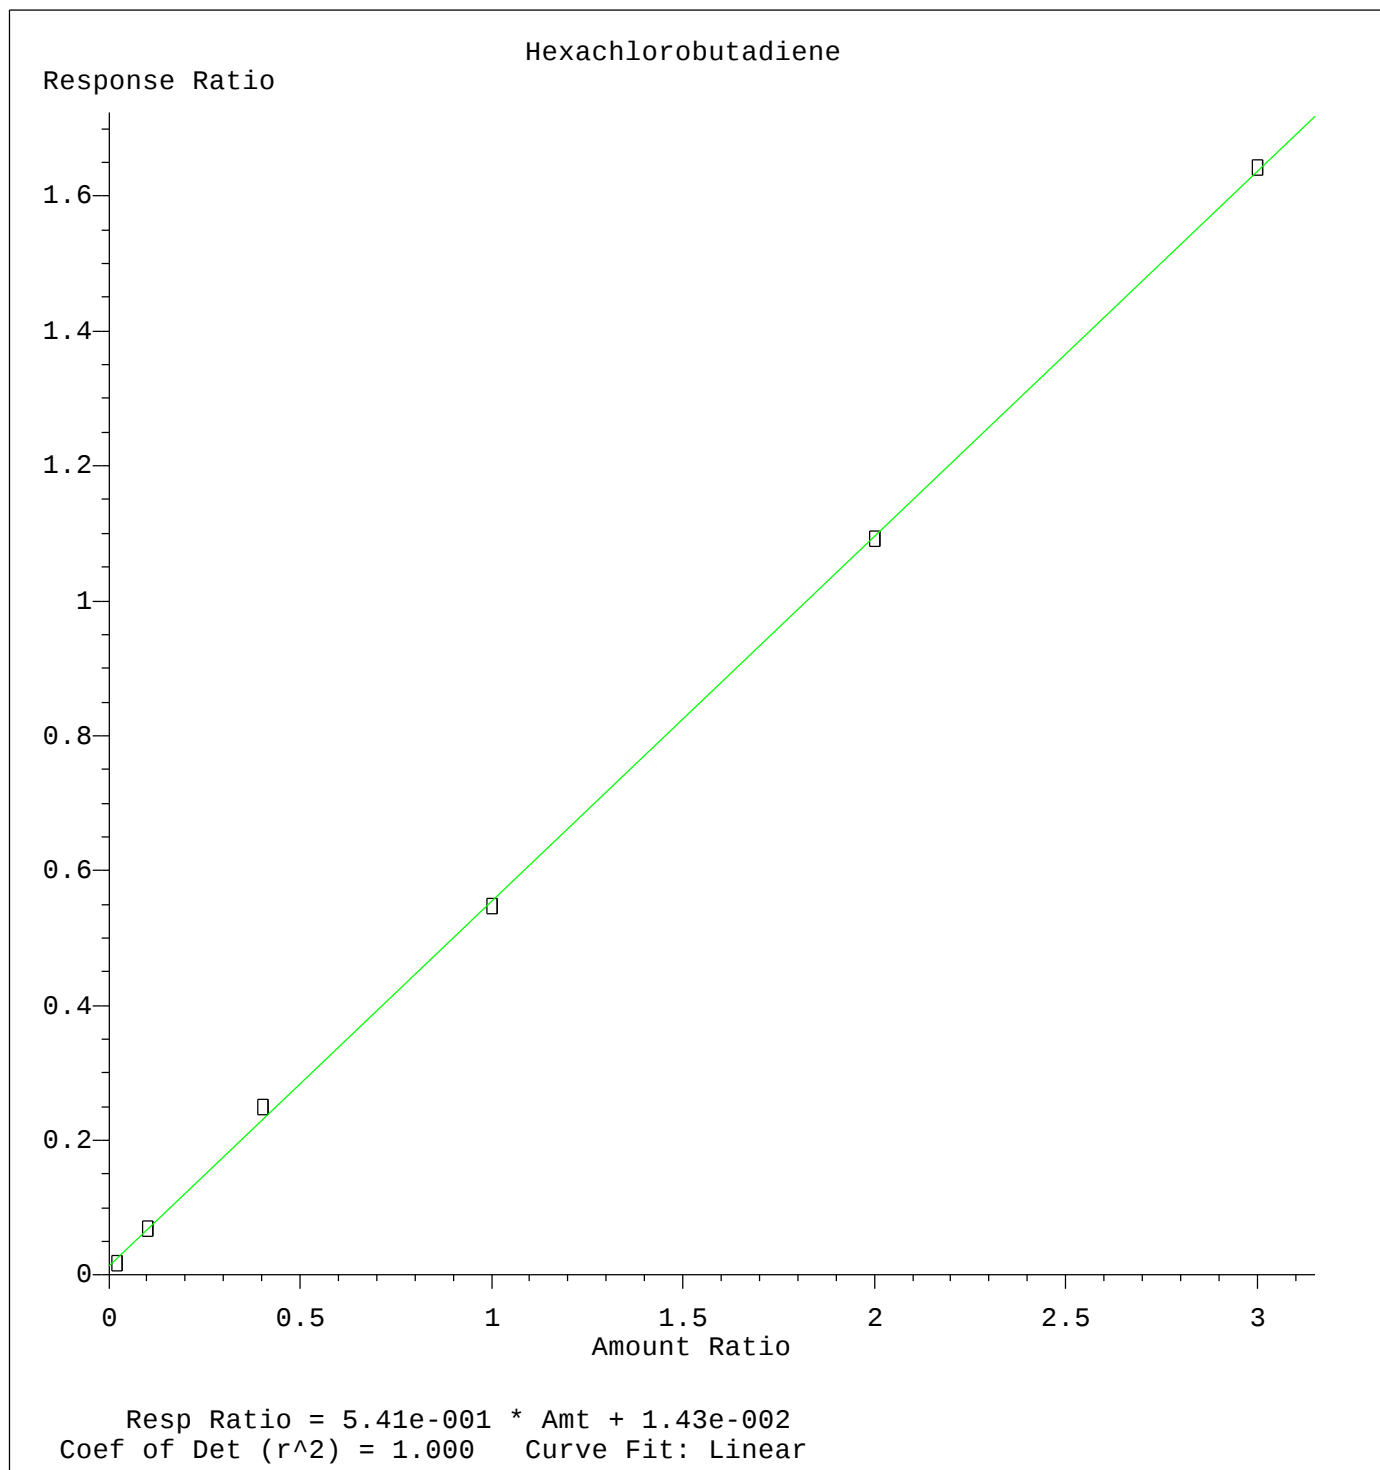

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

Naphthalene

Response Ratio

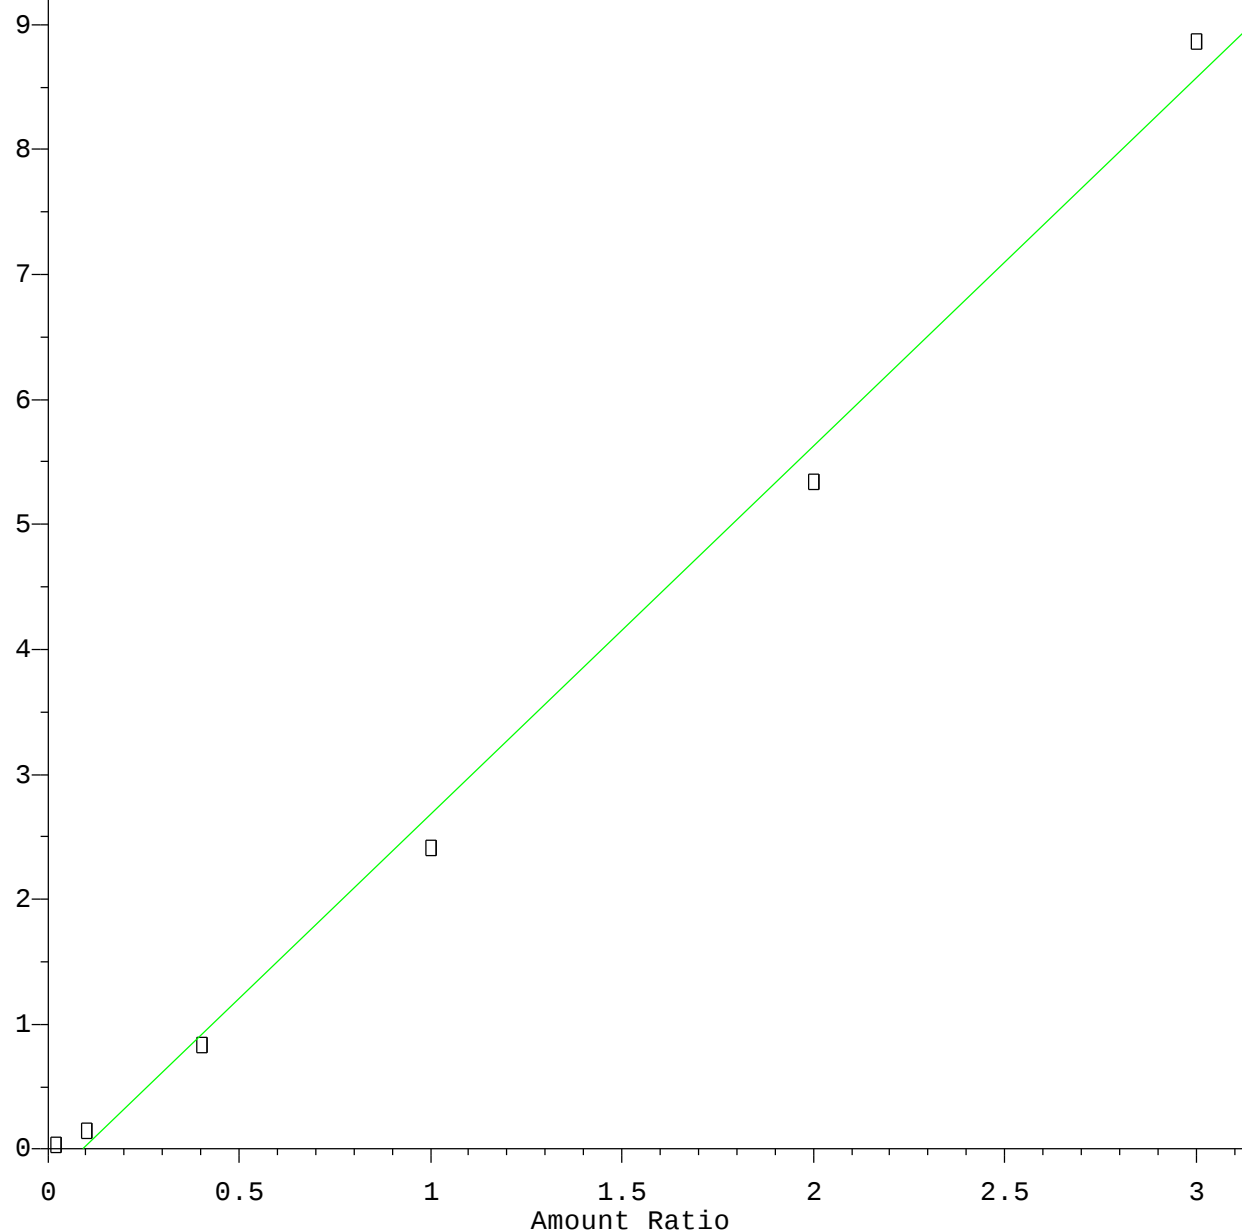


Resp Ratio = 2.95e+000 * Amt - 2.67e-001
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019

1,2,3-Trichlorobenzene

Response Ratio

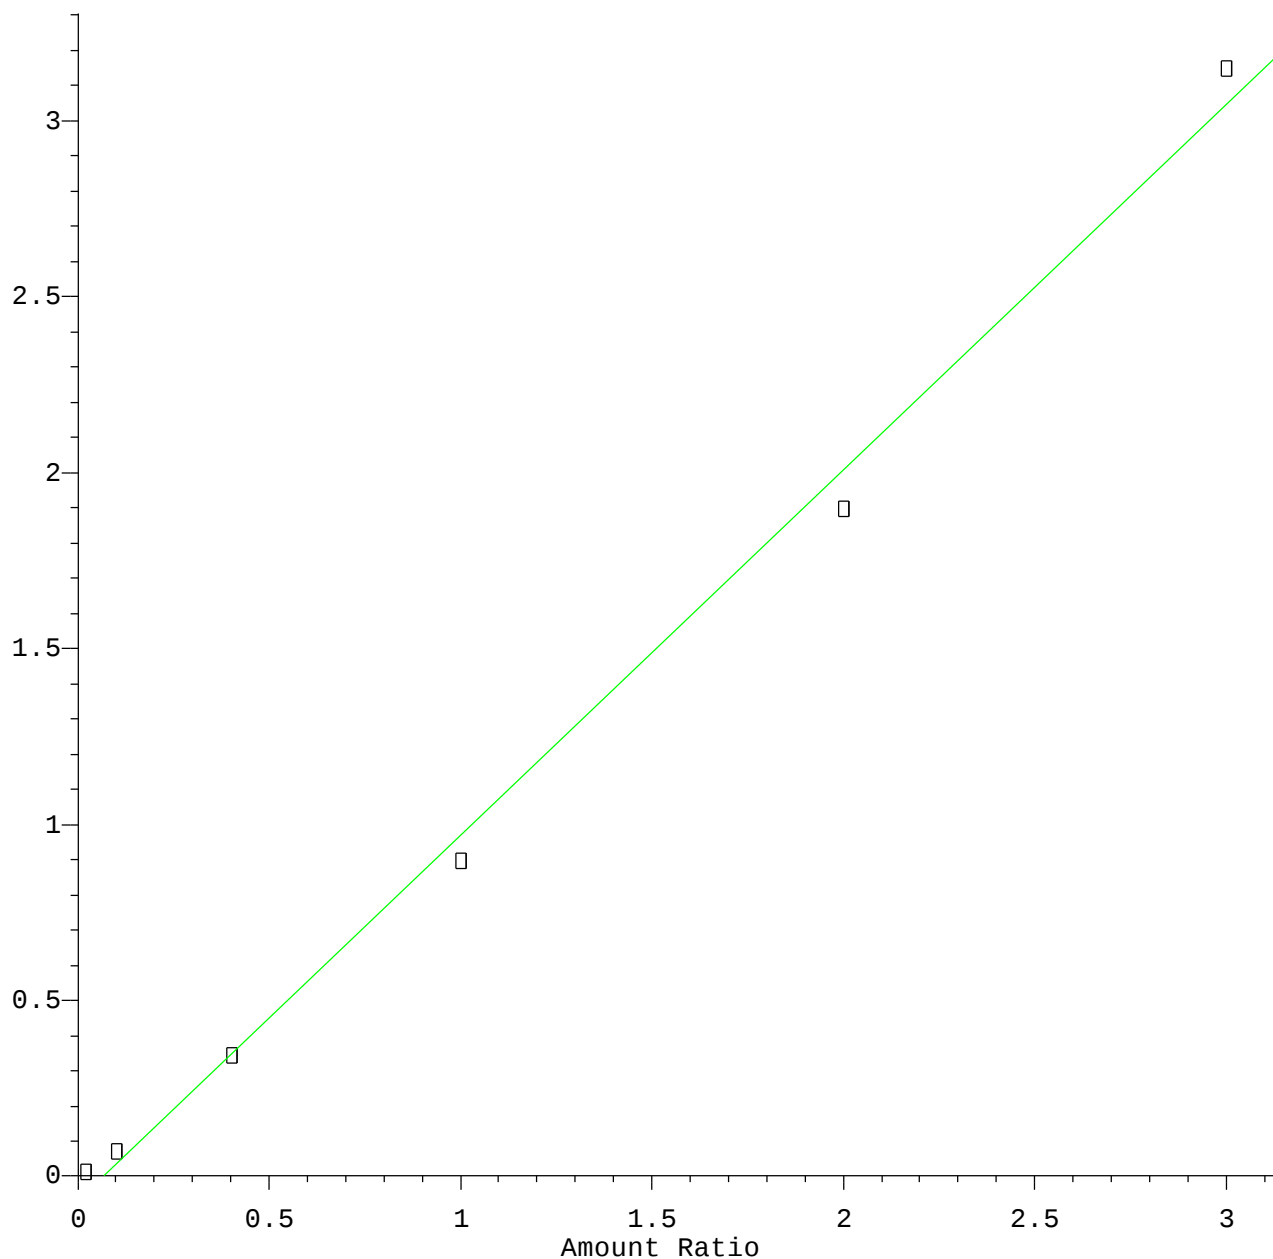

Resp Ratio = 1.04×10^0 * Amt - 6.90×10^{-2}
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Calibration Table Last Updated: Tue Jul 16 07:03:34 2019