


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071519\
Data File : VN056725.D
Acq On : 15 Jul 2019 20:42
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071519W.M
Title : SW846 8260
Last Update : Tue Jul 16 07:03:34 2019

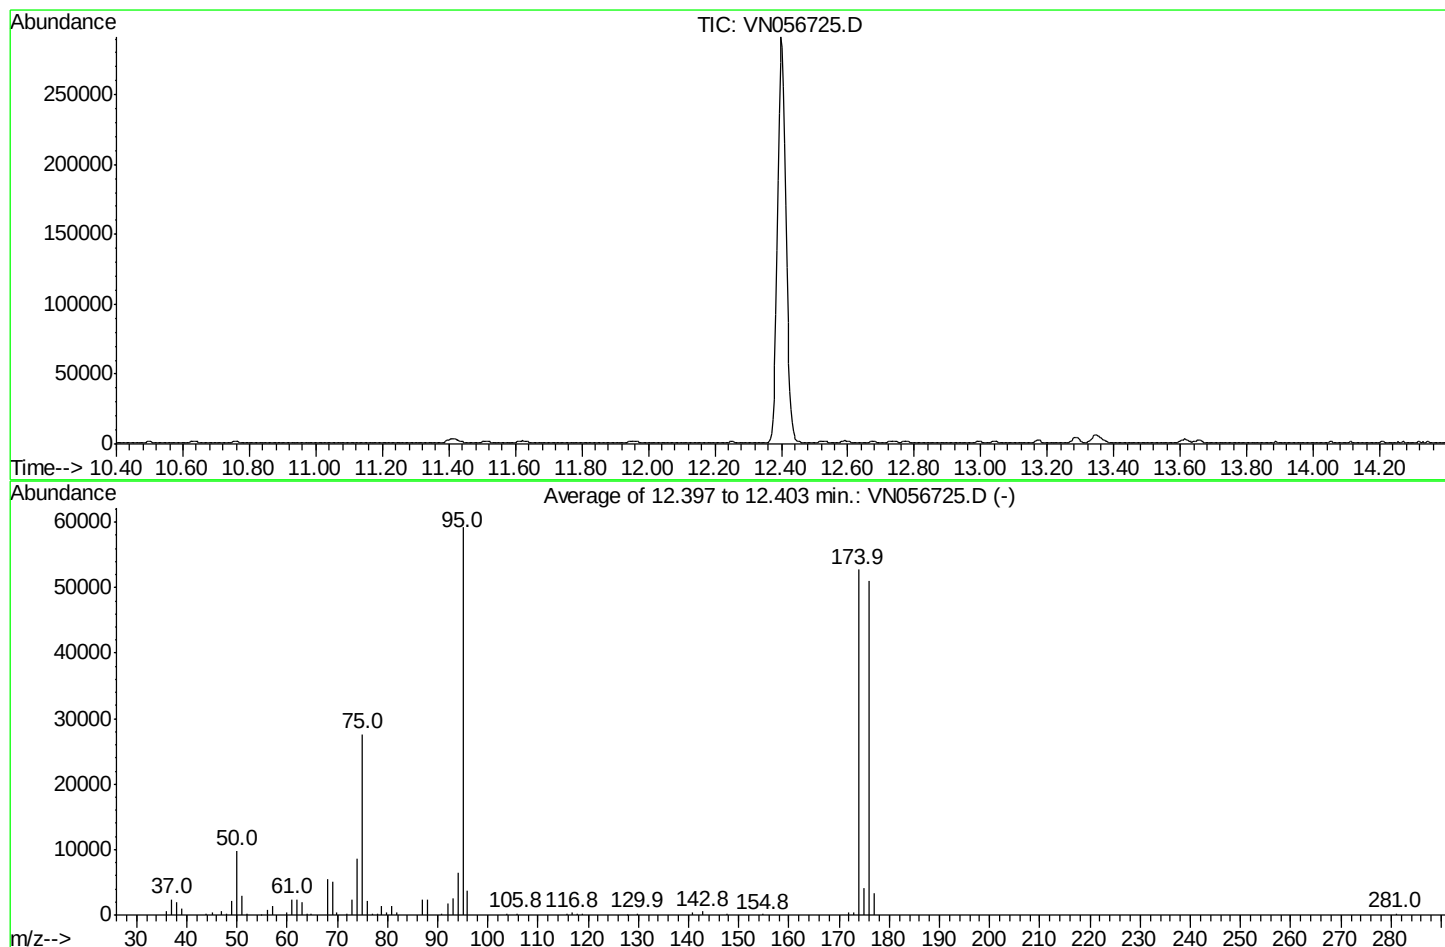

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	9840	PASS
75	95	30	60	46.7	27640	PASS
95	95	100	100	100.0	59221	PASS
96	95	5	9	6.4	3806	PASS
173	174	0.00	2	0.9	479	PASS
174	95	50	100	89.1	52760	PASS
175	174	5	9	7.6	4025	PASS
176	174	95	101	96.9	51125	PASS
177	176	5	9	6.4	3273	PASS