


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071520\
Data File : VN062526.D
Acq On : 15 Jul 2020 9:09
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N070820W.M
Title : SW846 8260
Last Update : Fri Jul 10 00:55:52 2020

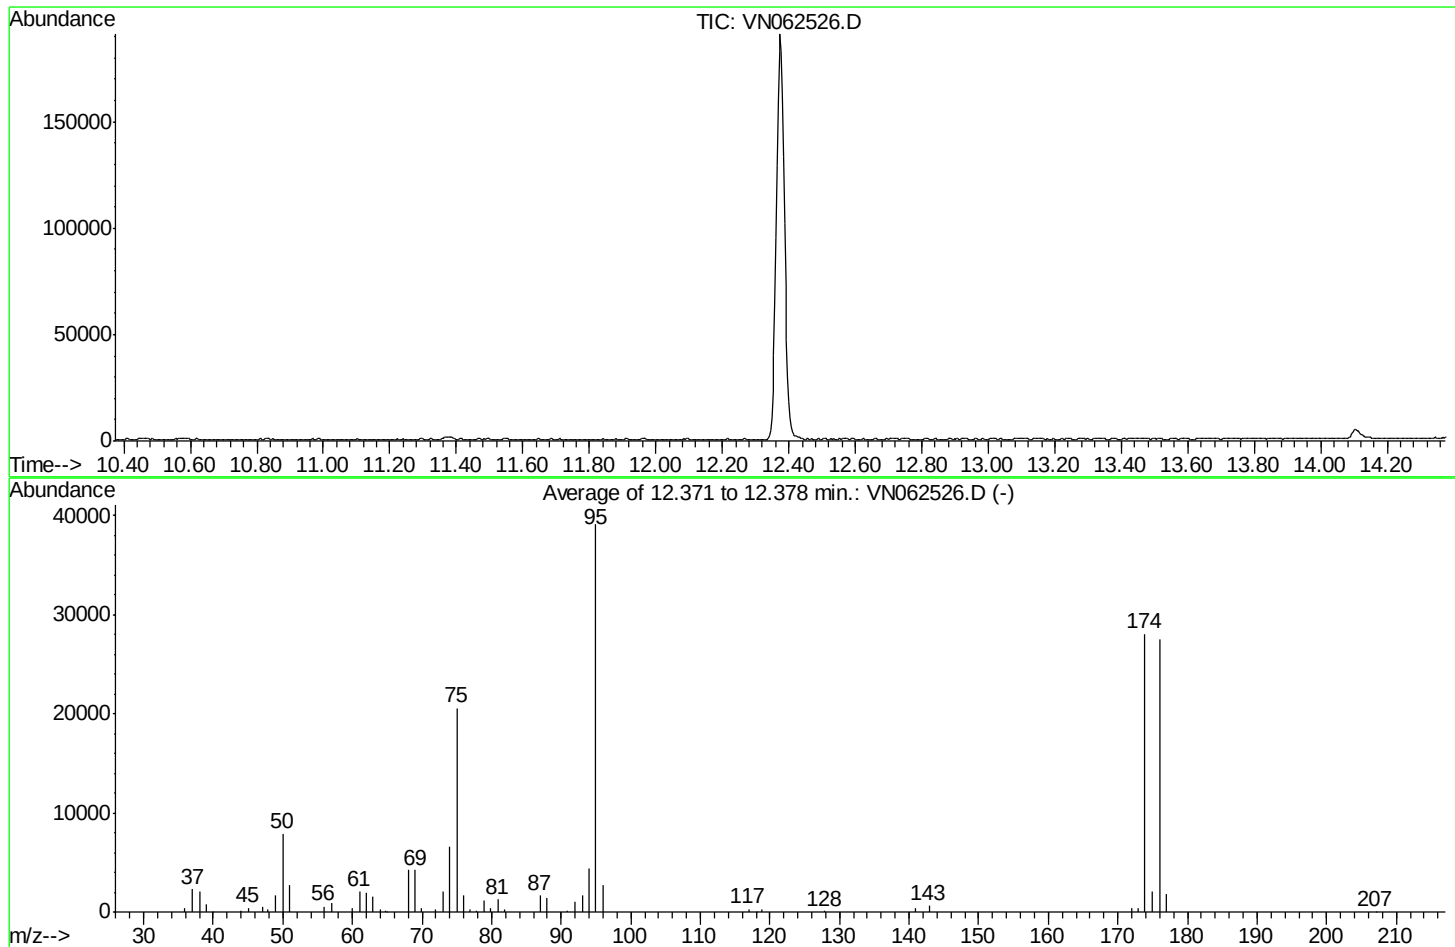

AutoFind: Scans 3296, 3297, 3298; Background Corrected with Scan 3283

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	7943	PASS
75	95	30	60	52.6	20594	PASS
95	95	100	100	100.0	39125	PASS
96	95	5	9	6.9	2696	PASS
173	174	0.00	2	1.3	360	PASS
174	95	50	100	71.7	28066	PASS
175	174	5	9	7.6	2134	PASS
176	174	95	101	98.0	27517	PASS
177	176	5	9	6.4	1757	PASS