

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071522\
 Data File : VN073485.D
 Acq On : 15 Jul 2022 15:01
 Operator : JC\MD
 Sample : N3726-06DL 100X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TW-ANOMDL

Quant Time: Jul 16 04:13:54 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.016	168	264759	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.904	114	451527	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	416605	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	203723	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.369	65	176171	46.093	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery =	92.180%		
35) Dibromofluoromethane	7.951	113	145511	48.438	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	96.880%		
50) Toluene-d8	10.380	98	479966	44.985	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery =	89.980%		
62) 4-Bromofluorobenzene	12.669	95	207282	50.554	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	101.100%		
Target Compounds						
						Qvalue
16) Acetone	4.240	43	2548	1.188	ug/l	# 39
20) Methylene Chloride	5.028	84	1693	0.449	ug/l	# 70
26) 2,2-Dichloropropane	7.251	77	1506	0.257	ug/l	# 53
29) Tetrahydrofuran	7.634	42	767	0.328	ug/l	# 47
31) Cyclohexane	8.016	56	12462	1.991	ug/l	# 45
36) 1,1-Dichloropropene	8.010	75	22366	4.839	ug/l	# 50
38) Carbon Tetrachloride	8.016	117	28612	5.986	ug/l	# 17
39) Methylcyclohexane	9.392	83	5255	0.913	ug/l	89
52) Toluene	10.445	92	58491	6.635	ug/l	95
55) 1,1,2-Trichloroethane	10.816	97	824	0.227	ug/l	# 16
67) Ethyl Benzene	11.786	91	359691	21.028	ug/l	99
68) m/p-Xylenes	11.886	106	569199	88.171	ug/l	94
69) o-Xylene	12.222	106	186706	28.331	ug/l	96
70) Styrene	12.222	104	9878	0.971	ug/l	# 1
71) Bromoform	12.663	173	1636	0.645	ug/l	# 28
73) Isopropylbenzene	12.516	105	19008	1.080	ug/l	98
76) 1,2,3-Trichloropropane	12.669	75	111965	21.019	ug/l	# 1
78) n-propylbenzene	12.857	91	64945	3.323	ug/l	97
79) 2-Chlorotoluene	12.921	91	23803	1.924	ug/l	# 40
80) 1,3,5-Trimethylbenzene	12.998	105	91820	6.403	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.669	75	111965	57.643	ug/l	# 10
82) 4-Chlorotoluene	12.998	91	10568	0.883	ug/l	# 40
83) tert-Butylbenzene	13.498	119	5967	0.464	ug/l	71
84) 1,2,4-Trimethylbenzene	13.310	105	394545	27.559	ug/l	97
85) sec-Butylbenzene	13.310	105	394545	22.856	ug/l	# 56
86) p-Isopropyltoluene	13.498	119	5967	0.428	ug/l	90
89) n-Butylbenzene	13.880	91	4630	0.398	ug/l	# 82
90) Hexachloroethane	14.151	117	2659	1.023	ug/l	# 9
92) 1,2-Dibromo-3-Chloropr...	14.527	75	302	0.213	ug/l	# 1
95) Naphthalene	15.433	128	181248	11.544	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071522\
Data File : VN073485.D
Acq On : 15 Jul 2022 15:01
Operator : JC\MD
Sample : N3726-06DL 100X
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL

Quant Time: Jul 16 04:13:54 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




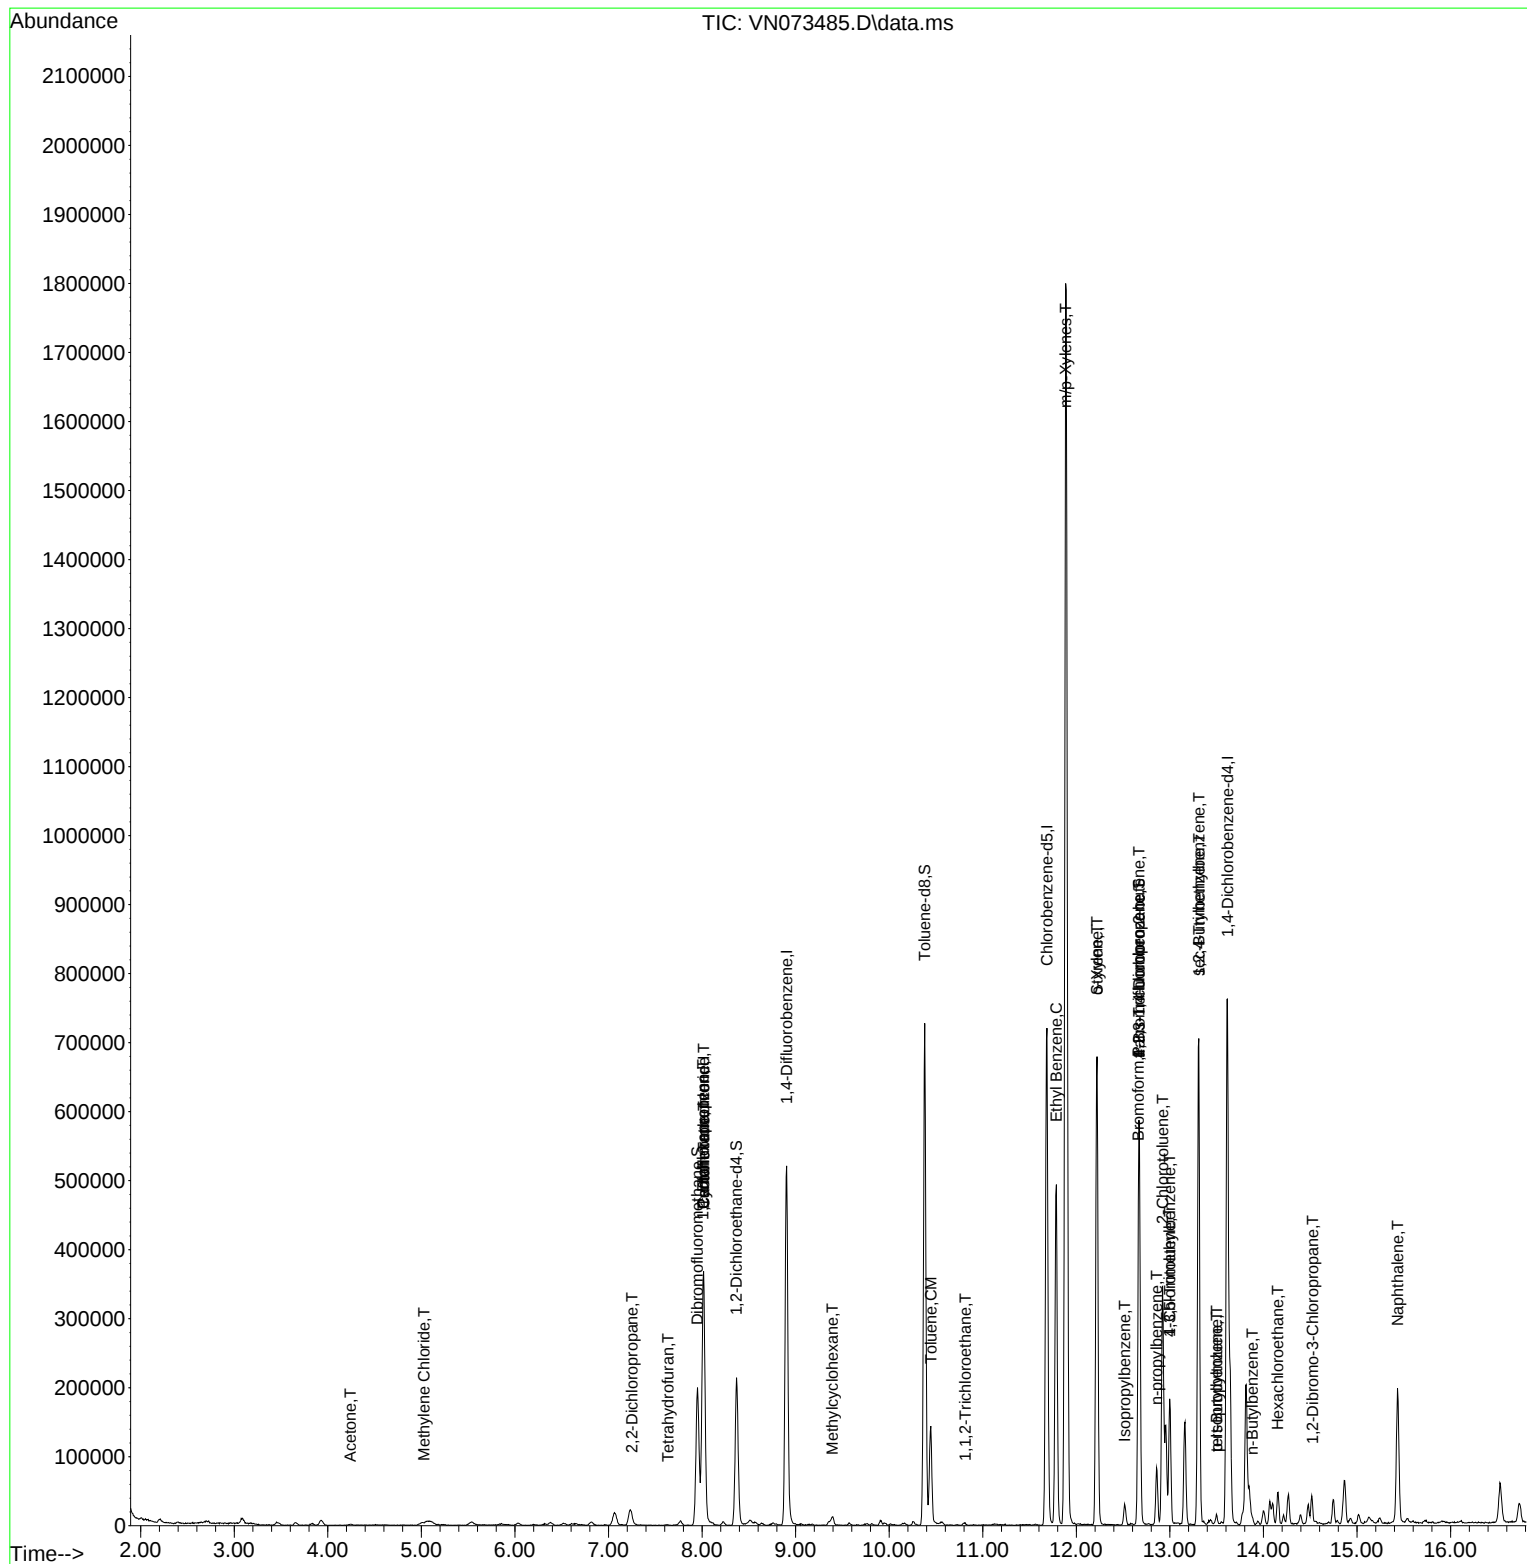


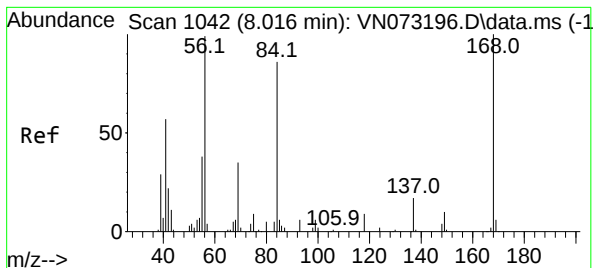

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.000 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion:168 Resp: 264759
Ion Ratio Lower Upper
168 100
99 65.6 42.3 63.5#

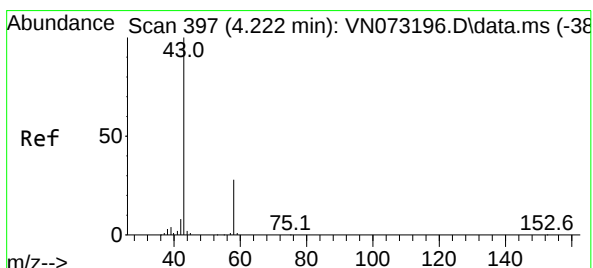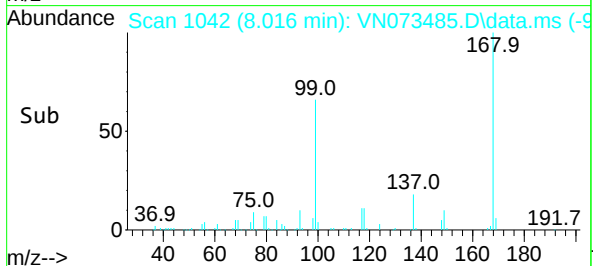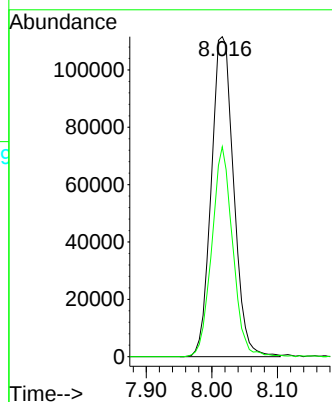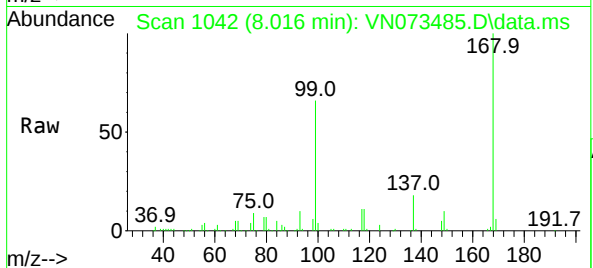

#16
Acetone
Concen: 1.188 ug/l
RT: 4.240 min Scan# 400
Delta R.T. 0.018 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 43 Resp: 2548
Ion Ratio Lower Upper
43 100
58 66.5 26.0 39.0#

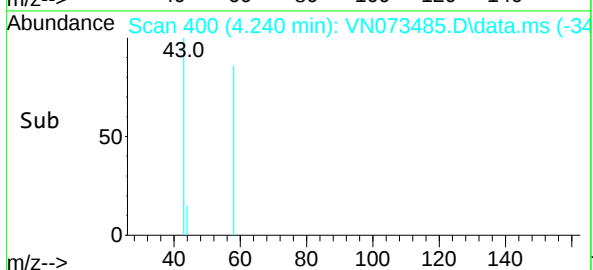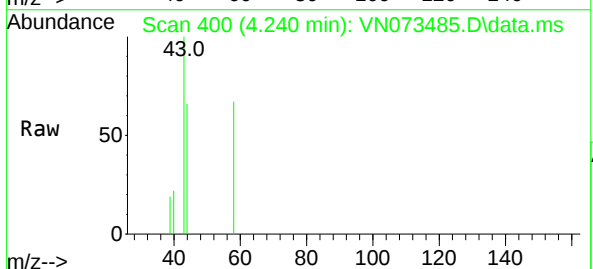




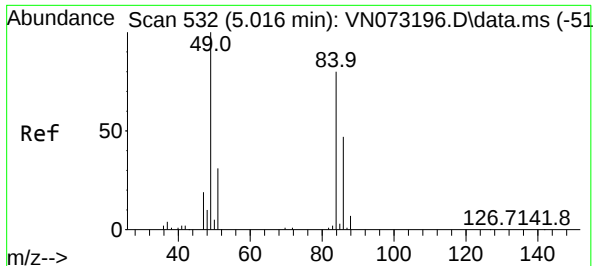


#20
Methylene Chloride
Concen: 0.449 ug/l
RT: 5.028 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL

Tgt Ion: 84 Resp: 1693




Ion	Ratio	Lower	Upper
84	100		
49	57.0	88.3	132.5#
51	28.3	28.2	42.2
86	66.4	50.6	76.0

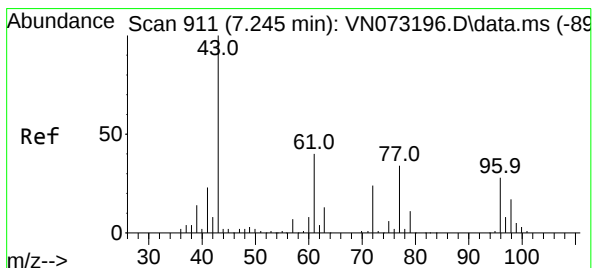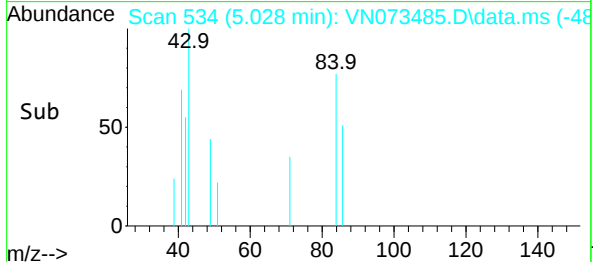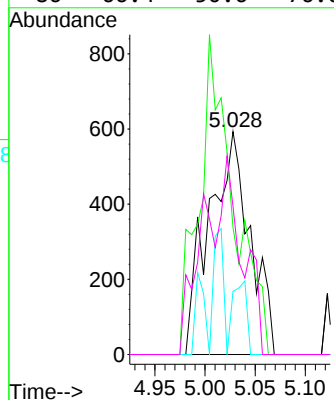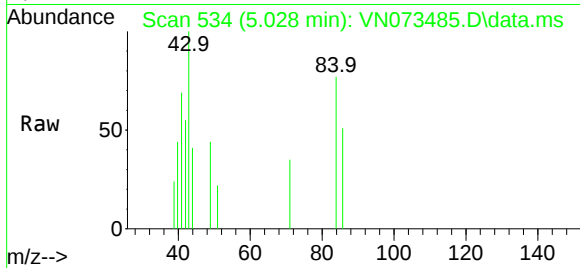


#26
2,2-Dichloropropane
Concen: 0.257 ug/l
RT: 7.251 min Scan# 912
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 77 Resp: 1506

Ion	Ratio	Lower	Upper
77	100		
97	0.0	11.4	34.2#

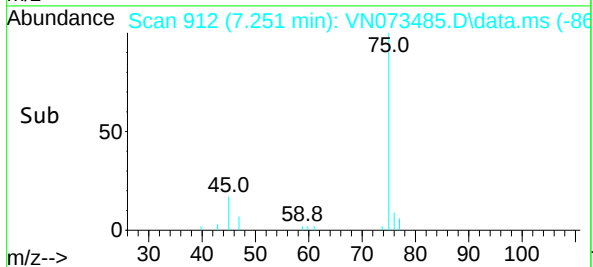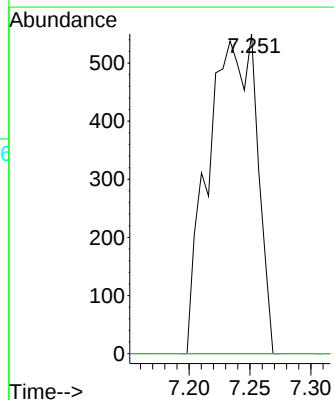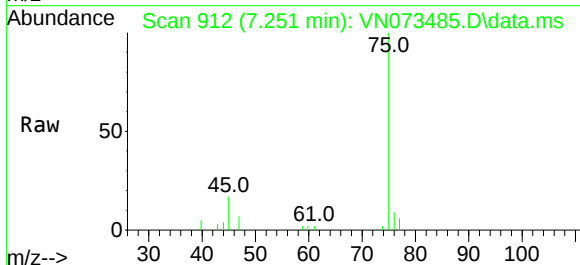

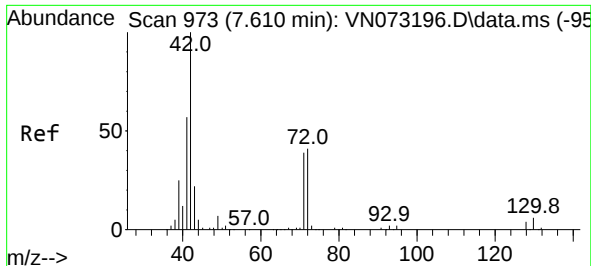

#29

Tetrahydrofuran

Concen: 0.328 ug/l

RT: 7.634 min Scan# 91

Delta R.T. 0.024 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01

Instrument :

MSVOA_N

ClientSampleId :

TW-ANOMDL





Tgt Ion: 42 Resp: 767

Ion Ratio Lower Upper

42 100

72 23.1 39.7 59.5#

71 0.0 36.6 55.0#

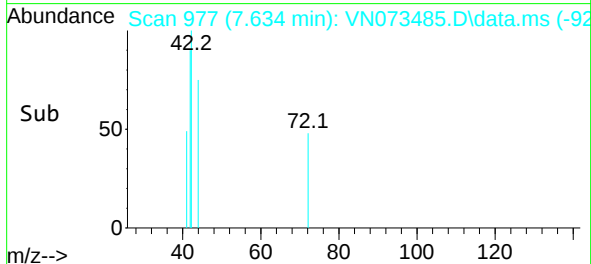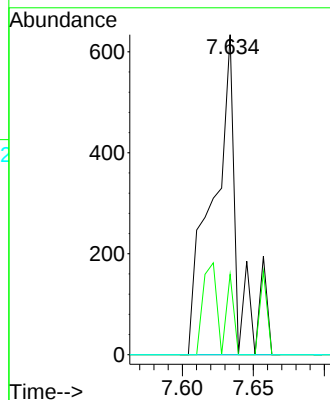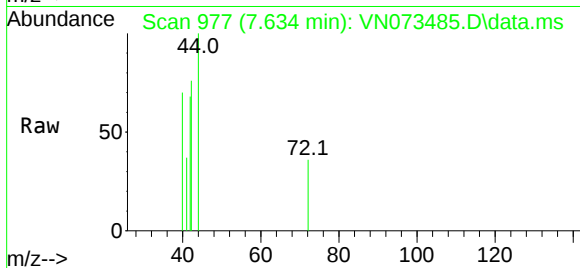

#31

Cyclohexane

Concen: 1.991 ug/l

RT: 8.016 min Scan# 1042

Delta R.T. -0.006 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01




Tgt Ion: 56 Resp: 12462


Ion Ratio Lower Upper

56 100

69 118.2 27.8 41.8#

84 117.9 76.9 115.3#

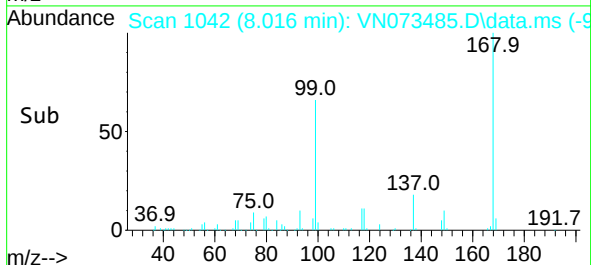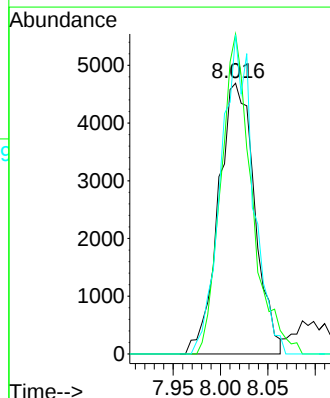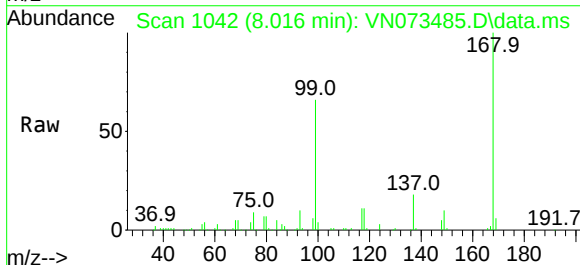

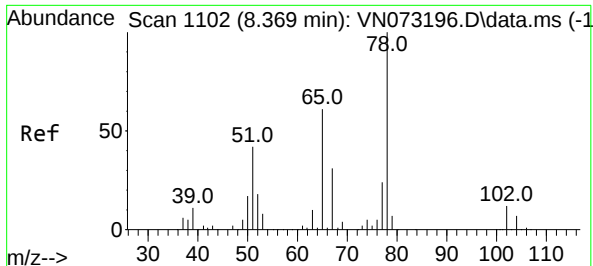

#33

1,2-Dichloroethane-d4

Concen: 46.093 ug/l

RT: 8.369 min Scan# 1102

Delta R.T. -0.000 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01

Instrument :

MSVOA_N

ClientSampleId :





TW-ANOMDL

Tgt Ion: 65 Resp: 176171

Ion Ratio Lower Upper

65 100

67 52.5 0.0 104.8

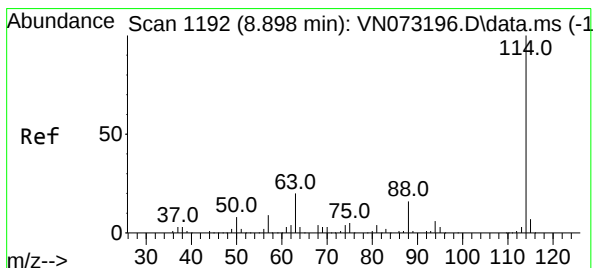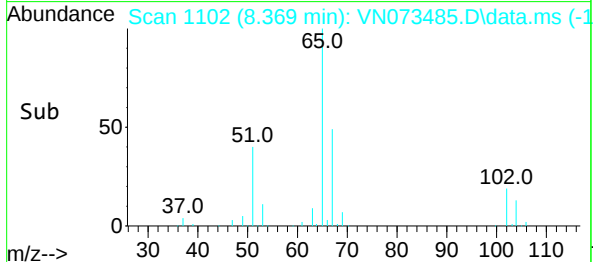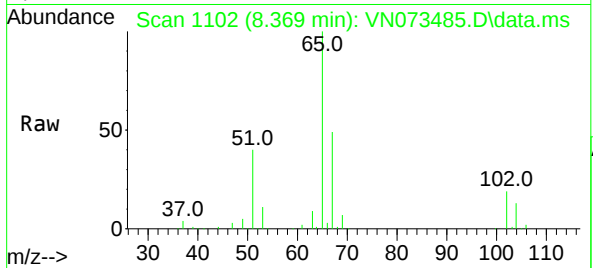

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.904 min Scan# 1193

Delta R.T. 0.006 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01




Tgt Ion: 114 Resp: 451527


Ion Ratio Lower Upper

114 100

63 22.6 0.0 40.0

88 16.9 0.0 32.6

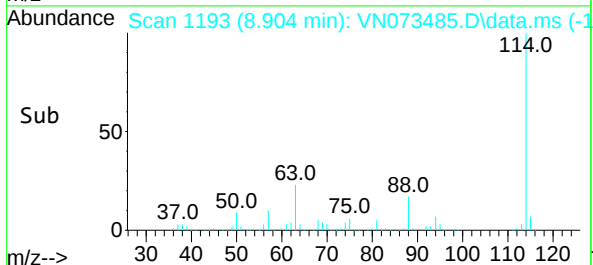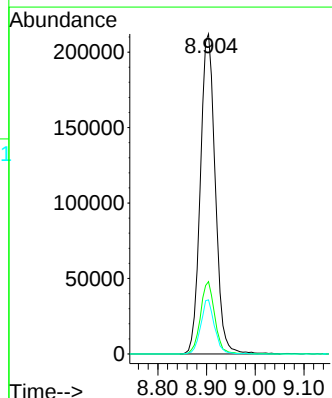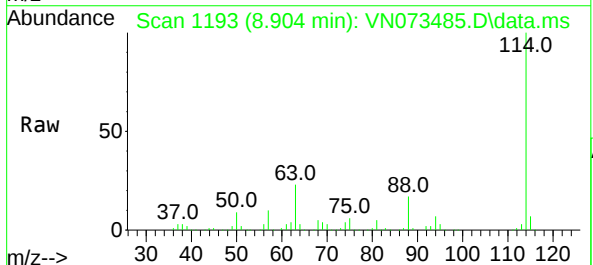

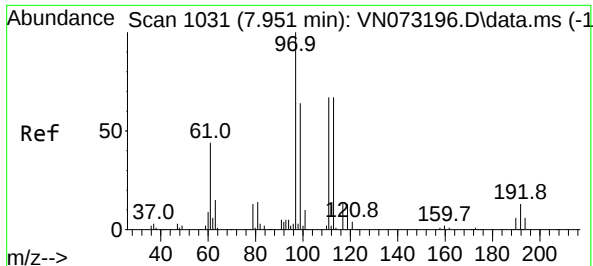

#35

Dibromofluoromethane

Concen: 48.438 ug/l

RT: 7.951 min Scan# 1031

Delta R.T. 0.000 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01

Instrument :

MSVOA_N

ClientSampleId :

TW-ANOMDL





Tgt Ion:113 Resp: 145511

Ion Ratio Lower Upper

113 100

111 104.5 81.4 122.0

192 18.0 17.0 25.6

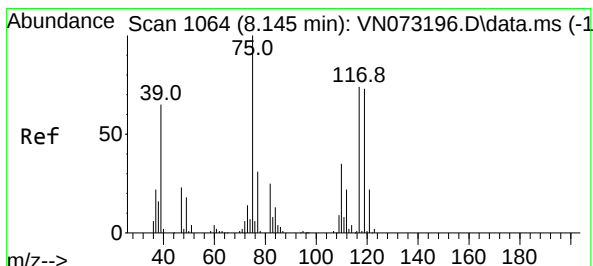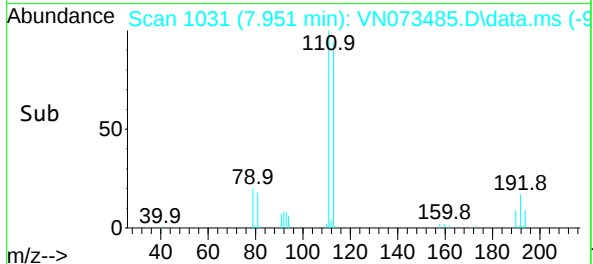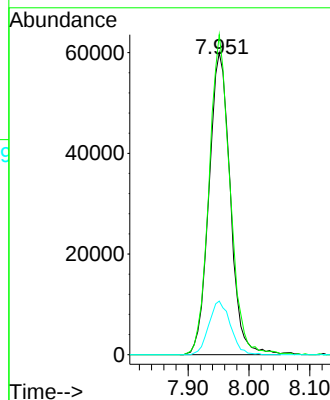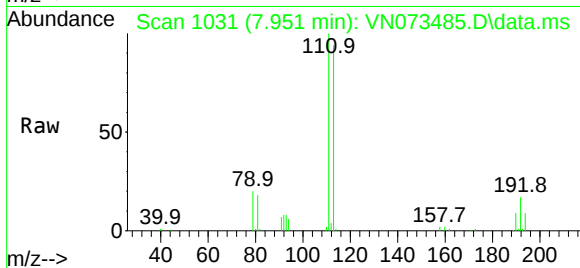

#36

1,1-Dichloropropene

Concen: 4.839 ug/l

RT: 8.010 min Scan# 1041

Delta R.T. -0.135 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01




Tgt Ion: 75 Resp: 22366


Ion Ratio Lower Upper

75 100

110 10.4 18.3 54.8#

77 0.0 25.1 37.7#


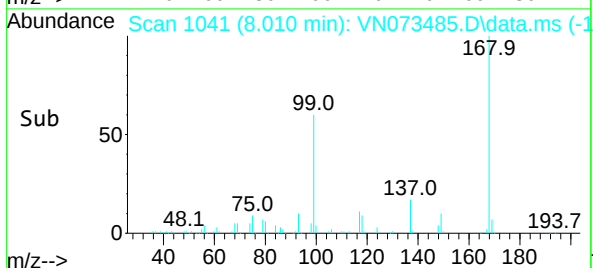
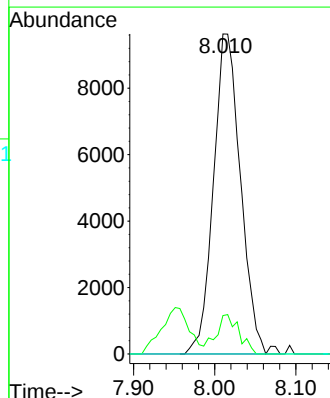
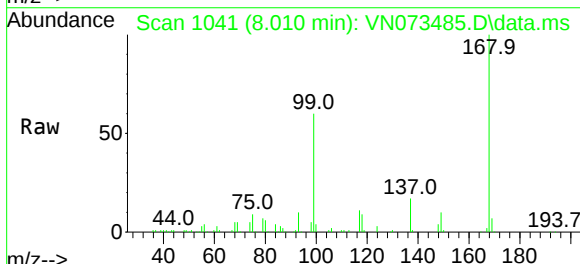


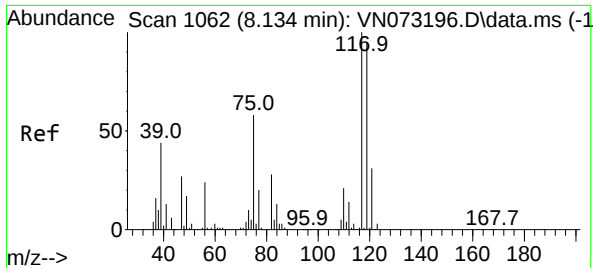

#38
Carbon Tetrachloride
Concen: 5.986 ug/l
RT: 8.016 min Scan# 1042
Delta R.T. -0.118 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion:117 Resp: 28612
Ion Ratio Lower Upper
117 100
119 5.3 75.8 113.8#
121 0.0 24.6 37.0#

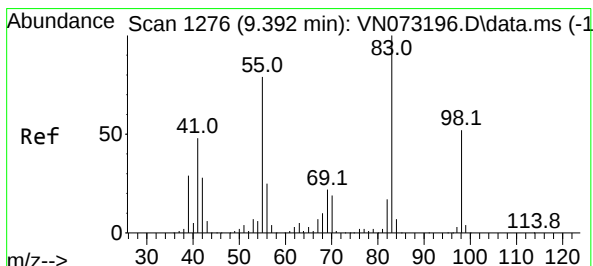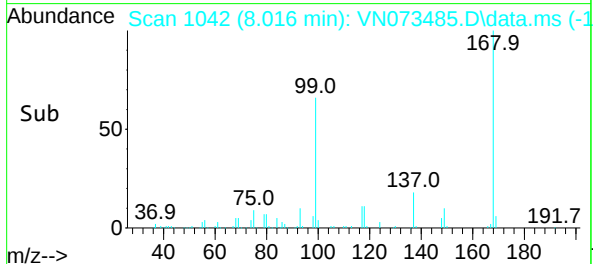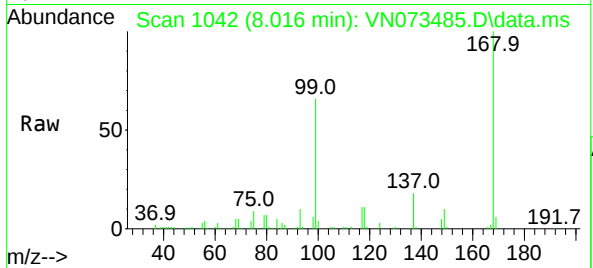

#39
Methylcyclohexane
Concen: 0.913 ug/l
RT: 9.392 min Scan# 1276
Delta R.T. 0.000 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 83 Resp: 5255
Ion Ratio Lower Upper
83 100
55 81.3 57.8 86.8
98 57.1 39.4 59.2


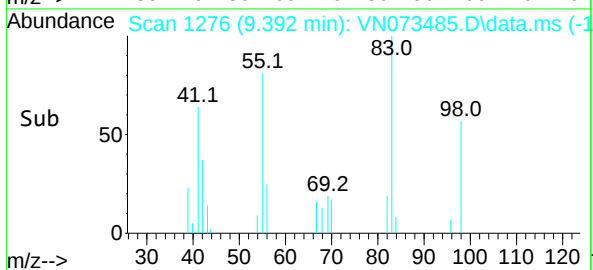

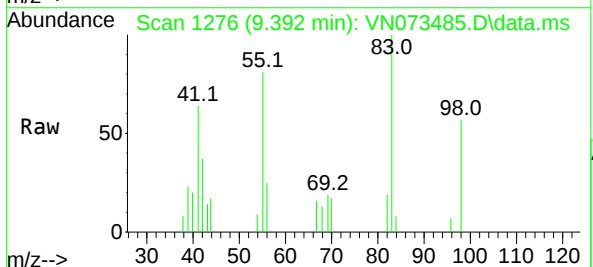




#50
Toluene-d8
Concen: 44.985 ug/l
RT: 10.380 min Scan# 1443
Delta R.T. 0.005 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion: 98 Resp: 479966
Ion Ratio Lower Upper
98 100
100 65.1 52.6 78.8

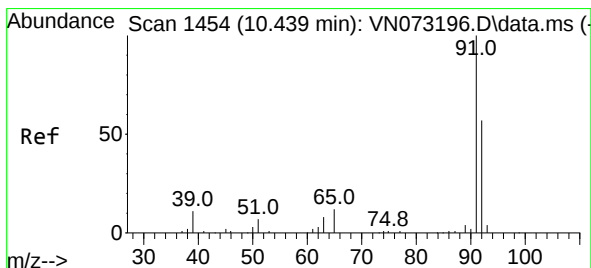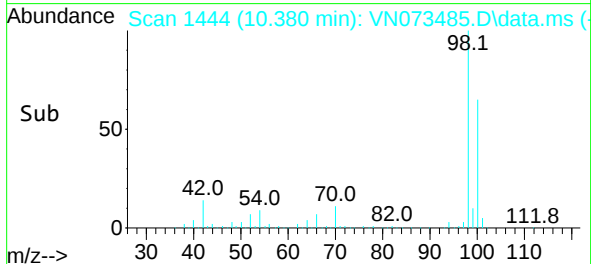

#52
Toluene
Concen: 6.635 ug/l
RT: 10.445 min Scan# 1455
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 92 Resp: 58491
Ion Ratio Lower Upper
92 100
91 180.6 138.6 207.8


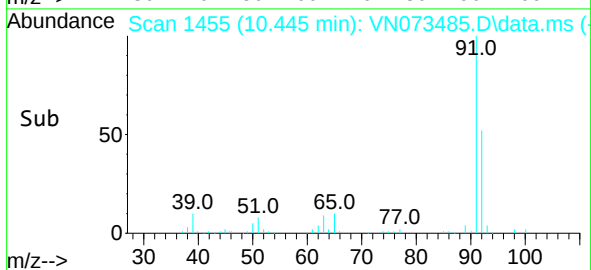

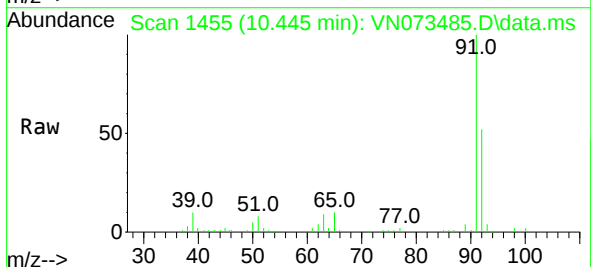


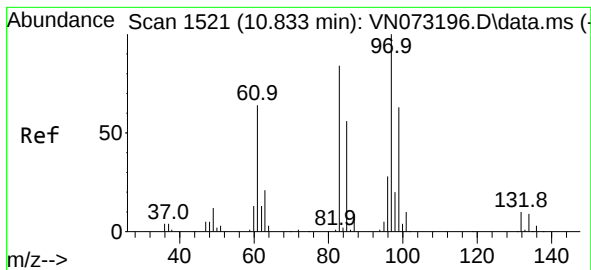

#55
1,1,2-Trichloroethane
Concen: 0.227 ug/l
RT: 10.816 min Scan# 1518
Delta R.T. -0.017 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion: 97	Resp: 824
Ion Ratio	Lower Upper
97 100	
83 0.0	66.2 99.4#
85 0.0	43.9 65.9#
99 0.0	50.6 76.0#

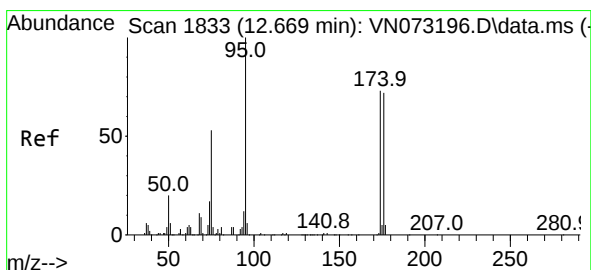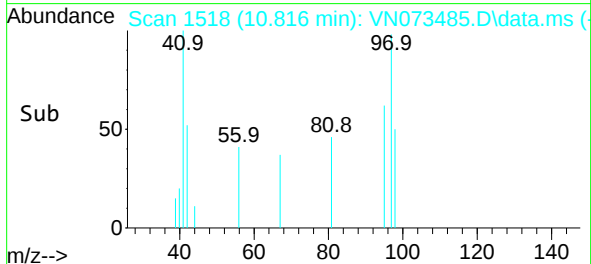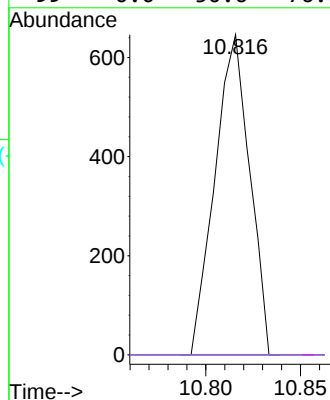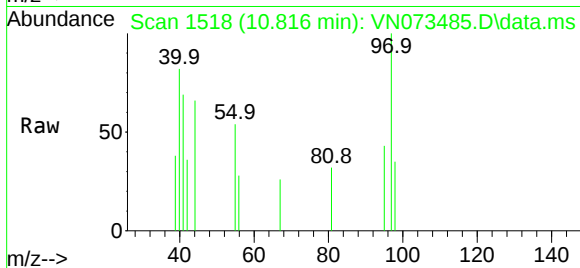

#62
4-Bromofluorobenzene
Concen: 50.554 ug/l
RT: 12.669 min Scan# 1833
Delta R.T. -0.000 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 95	Resp: 207282
Ion Ratio	Lower Upper
95 100	
174 74.1	0.0 167.6
176 72.1	0.0 163.4


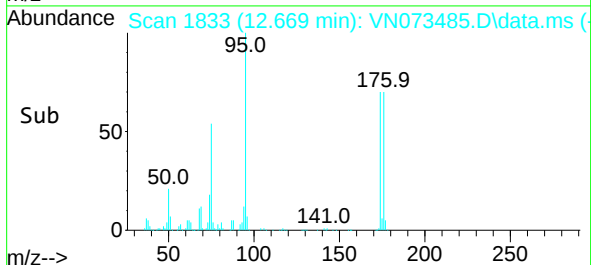
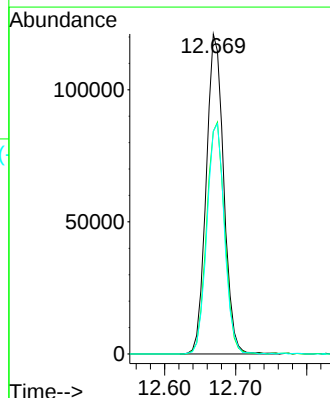
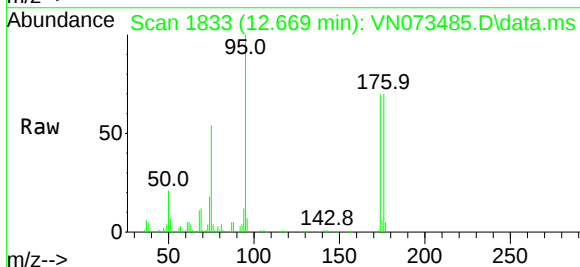


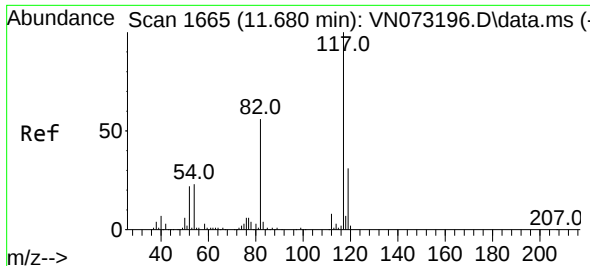

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.686 min Scan# 1666
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion:117 Resp: 416605
Ion Ratio Lower Upper
117 100
82 56.5 44.2 66.2
119 32.4 25.4 38.0

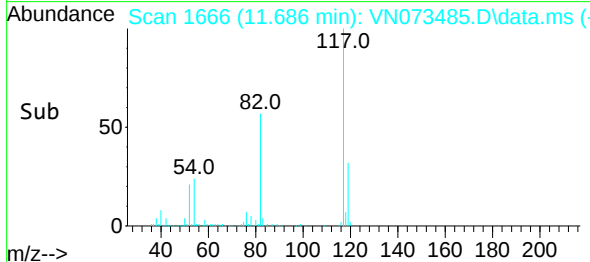

#67
Ethyl Benzene
Concen: 21.028 ug/l
RT: 11.786 min Scan# 1683
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 91 Resp: 359691
Ion Ratio Lower Upper
91 100
106 31.7 24.9 37.3


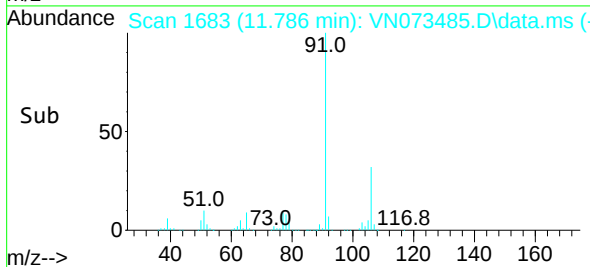

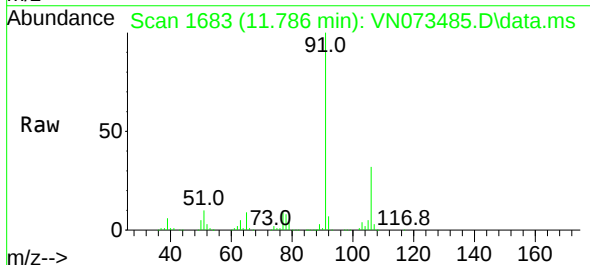


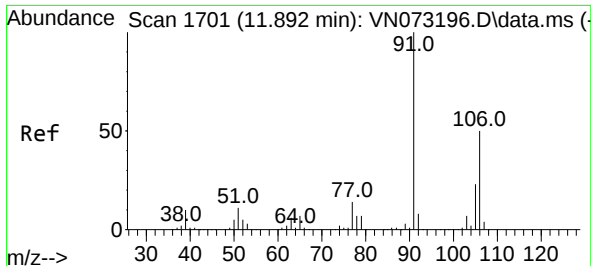

#68
m/p-Xylenes
Concen: 88.171 ug/l
RT: 11.886 min Scan# 11
Delta R.T. -0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion:106 Resp: 569199
Ion Ratio Lower Upper
106 100
91 208.0 158.9 238.3

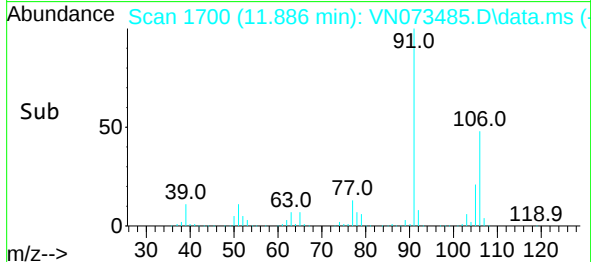

#69
o-Xylene
Concen: 28.331 ug/l
RT: 12.222 min Scan# 1757
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion:106 Resp: 186706
Ion Ratio Lower Upper
106 100
91 218.8 106.0 318.0


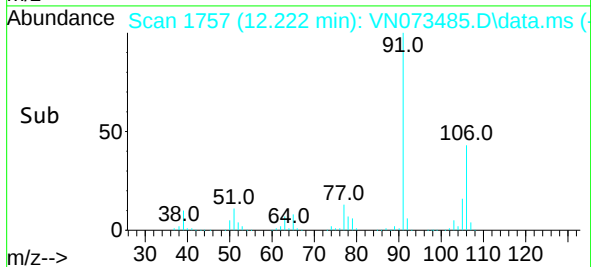

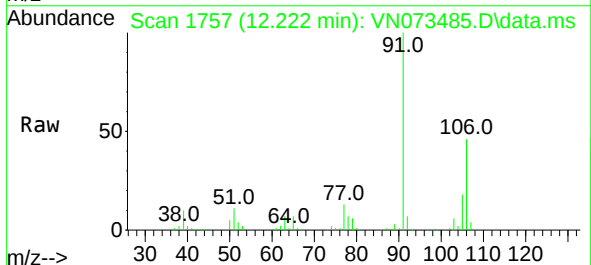




#70
Styrene
Concen: 0.971 ug/l
RT: 12.222 min Scan# 11
Delta R.T. -0.011 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion:104 Resp: 9878
Ion Ratio Lower Upper
104 100
78 302.2 39.5 59.3#
103 254.2 44.0 66.0#

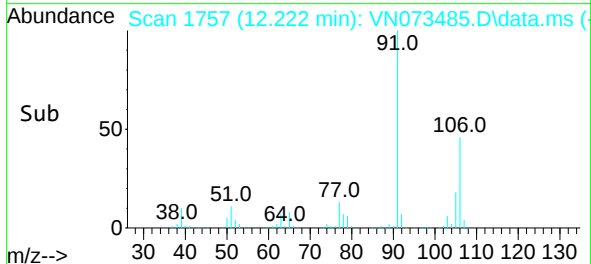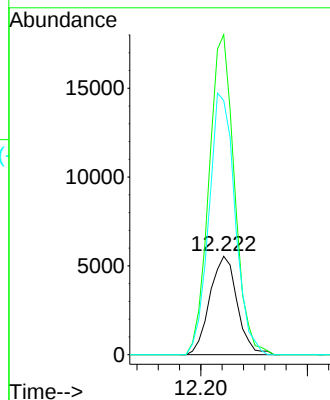

#71
Bromoform
Concen: 0.645 ug/l
RT: 12.663 min Scan# 1832
Delta R.T. 0.265 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion:173 Resp: 1636
Ion Ratio Lower Upper
173 100
175 0.0 24.6 73.6#
254 0.0 0.1 0.1#



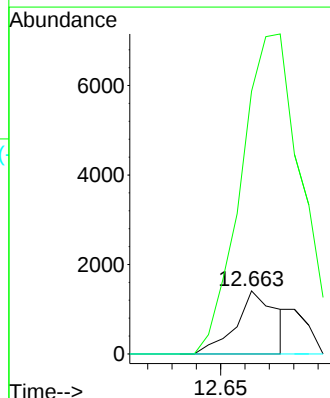
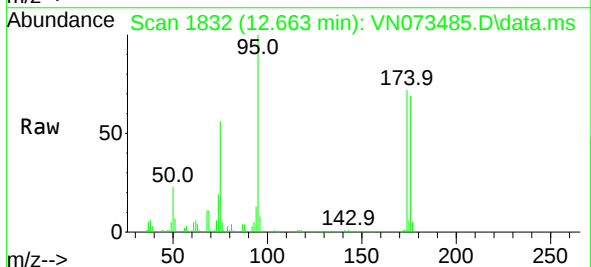


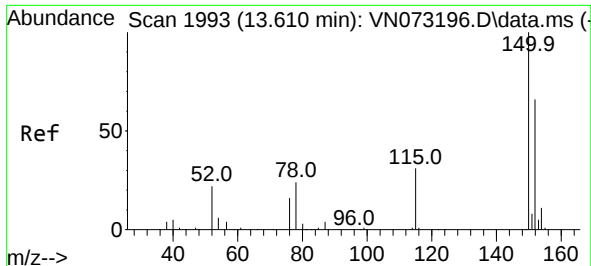

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.616 min Scan# 1994
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion:152 Resp: 203723
Ion Ratio Lower Upper
152 100
115 65.2 28.9 86.7
150 157.3 0.0 356.2

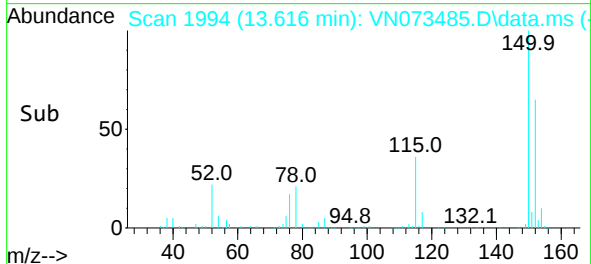

#73
Isopropylbenzene
Concen: 1.080 ug/l
RT: 12.516 min Scan# 1807
Delta R.T. -0.000 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion:105 Resp: 19008
Ion Ratio Lower Upper
105 100
120 26.1 13.5 40.4

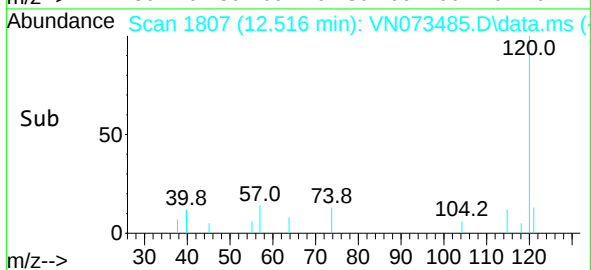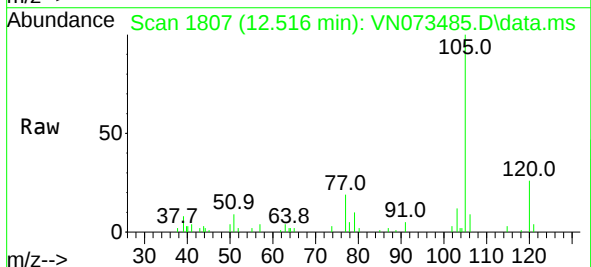



#76

1,2,3-Trichloropropane

Concen: 21.019 ug/l

RT: 12.669 min Scan# 1833

Delta R.T. -0.147 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01

Instrument :

MSVOA_N

ClientSampleId :





TW-ANOMDL

Tgt Ion: 75 Resp: 111965

Ion Ratio Lower Upper

75 100

77 1.6 98.5 295.5#

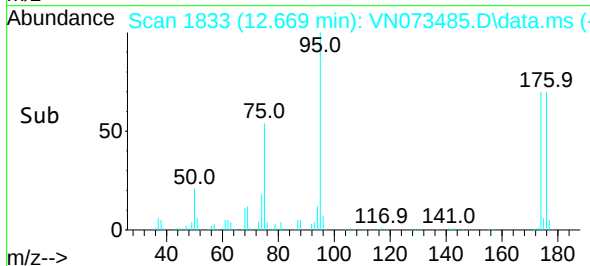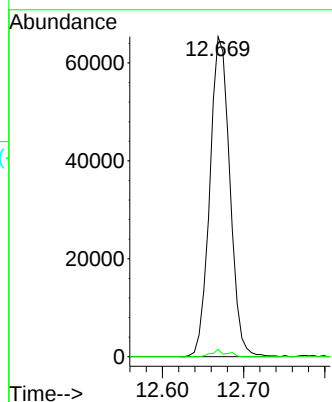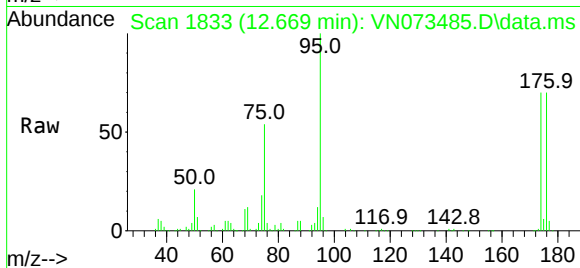

#78

n-propylbenzene

Concen: 3.323 ug/l

RT: 12.857 min Scan# 1865

Delta R.T. -0.000 min

Lab File: VN073485.D




Acq: 15 Jul 2022 15:01


Tgt Ion: 91 Resp: 64945

Ion Ratio Lower Upper

91 100

120 22.0 11.9 35.5


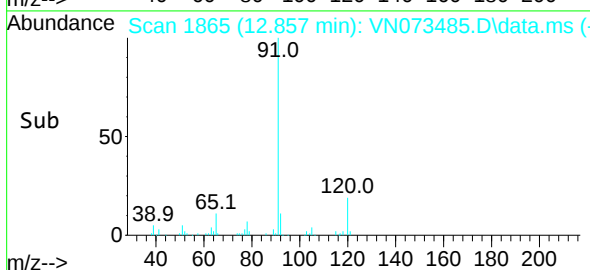

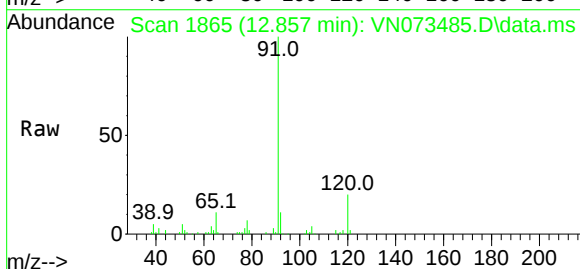


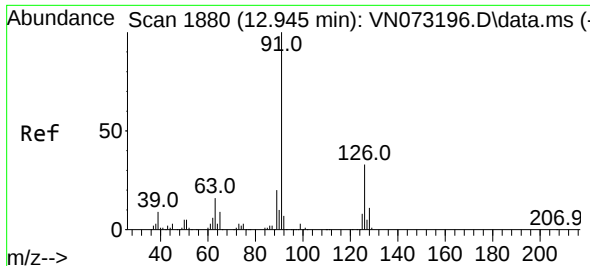

#79
2-Chlorotoluene
Concen: 1.924 ug/l
RT: 12.921 min Scan# 1876
Delta R.T. -0.024 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion: 91 Resp: 23803
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.9#

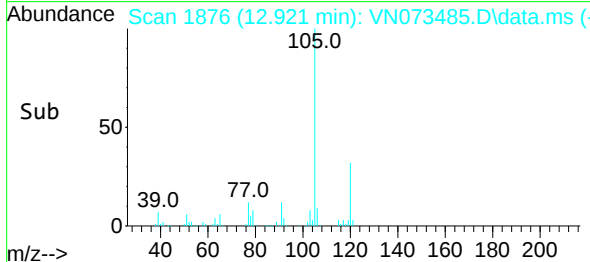

#80
1,3,5-Trimethylbenzene
Concen: 6.403 ug/l
RT: 12.998 min Scan# 1889
Delta R.T. -0.000 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 105 Resp: 91820
Ion Ratio Lower Upper
105 100
120 50.8 24.9 74.7


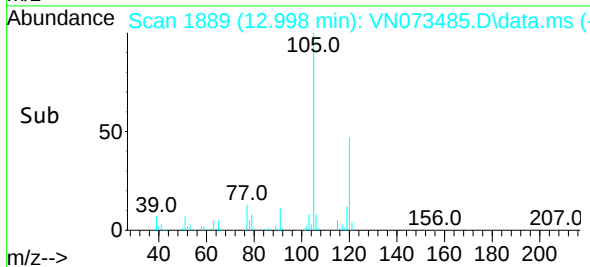

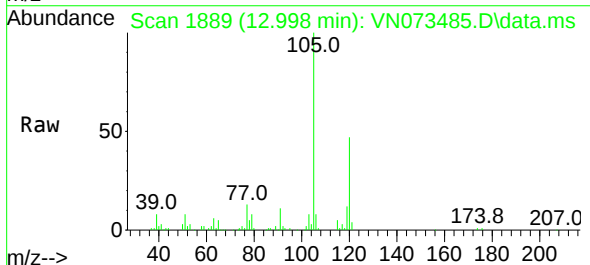




#81
 trans-1,4-Dichloro-2-butene
 Concen: 57.643 ug/l
 RT: 12.669 min Scan# 1833
 Delta R.T. 0.106 min
 Lab File: VN073485.D
 Acq: 15 Jul 2022 15:01




Instrument :
 MSVOA_N
 ClientSampleId :
 TW-ANOMDL


Tgt Ion: 75 Resp: 111965
 Ion Ratio Lower Upper
 75 100
 53 0.0 78.0 117.0#
 89 0.0 37.2 55.8#

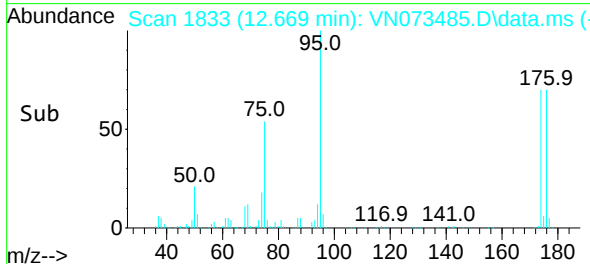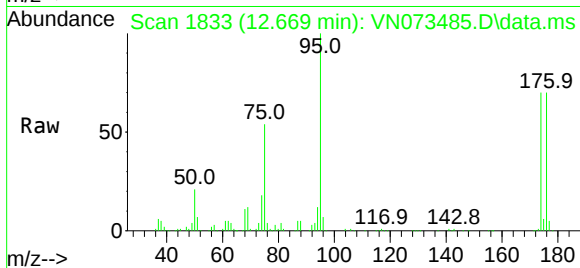

#82
 4-Chlorotoluene
 Concen: 0.883 ug/l
 RT: 12.998 min Scan# 1889
 Delta R.T. -0.041 min
 Lab File: VN073485.D
 Acq: 15 Jul 2022 15:01

Tgt Ion: 91 Resp: 10568
 Ion Ratio Lower Upper
 91 100
 126 0.0 17.2 51.6#

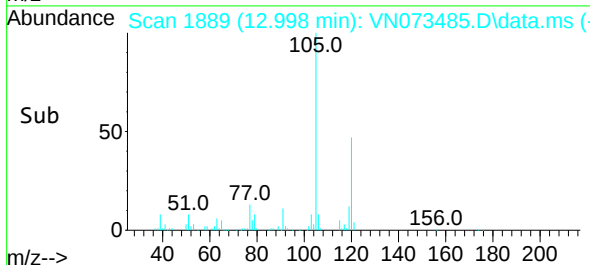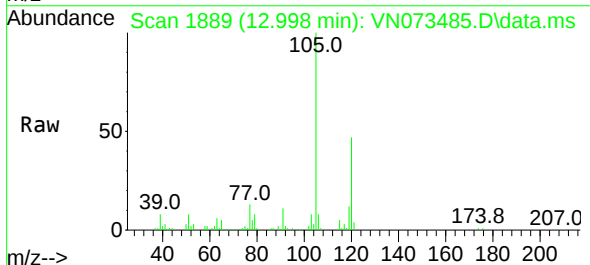



#83

tert-Butylbenzene

Concen: 0.464 ug/l

RT: 13.498 min Scan# 1933

Delta R.T. 0.241 min

Lab File: VN073485.D

Acq: 15 Jul 2022 15:01

Instrument :

MSVOA_N

ClientSampleId :

TW-ANOMDL





Tgt Ion:119 Resp: 5967

Ion Ratio Lower Upper

119 100

91 32.1 31.6 94.8

134 25.8 13.7 41.1

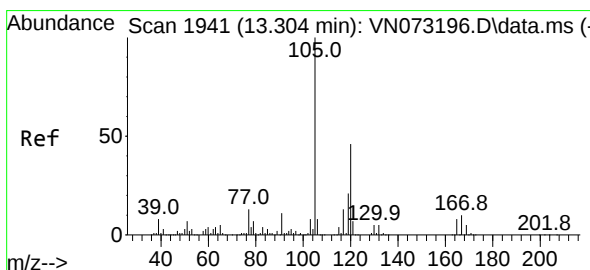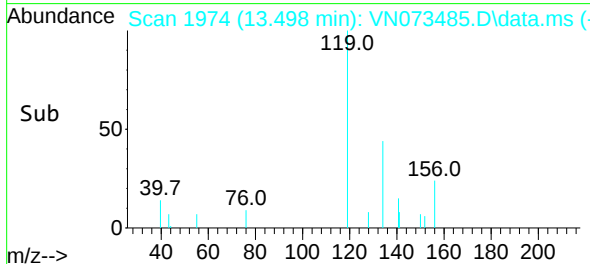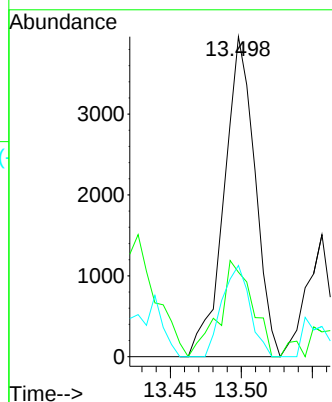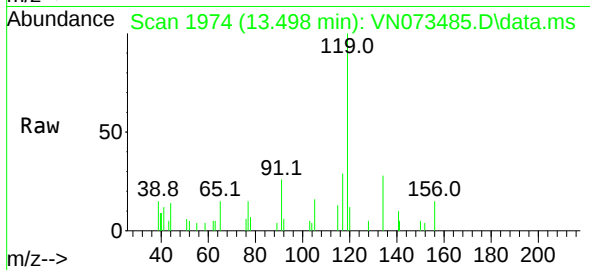

#84

1,2,4-Trimethylbenzene

Concen: 27.559 ug/l

RT: 13.310 min Scan# 1942

Delta R.T. 0.006 min

Lab File: VN073485.D




Acq: 15 Jul 2022 15:01


Tgt Ion:105 Resp: 394545

Ion Ratio Lower Upper

105 100

120 44.7 23.3 69.8




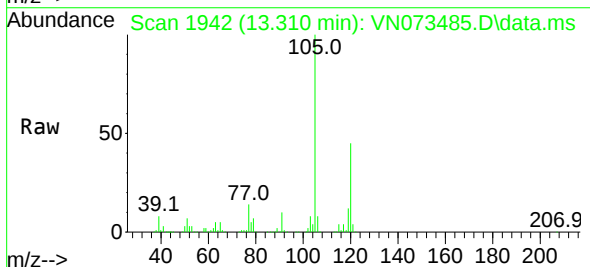




#85
 sec-Butylbenzene
 Concen: 22.856 ug/l
 RT: 13.310 min Scan# 1942
 Delta R.T. -0.129 min
 Lab File: VN073485.D
 Acq: 15 Jul 2022 15:01




Instrument :
 MSVOA_N
 ClientSampleId :
 TW-ANOMDL


Tgt Ion:105 Resp: 394545
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.4 31.1#

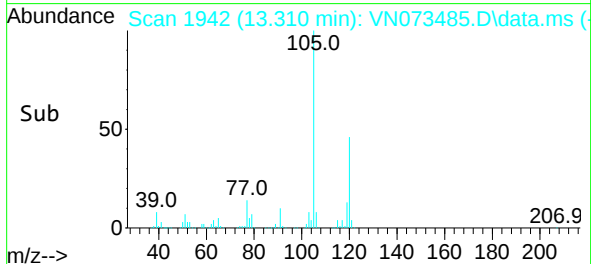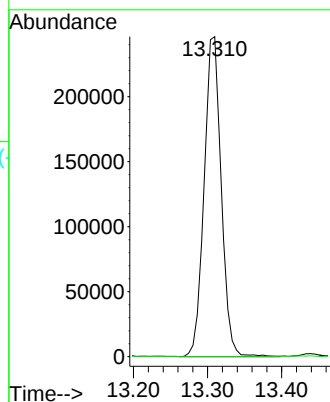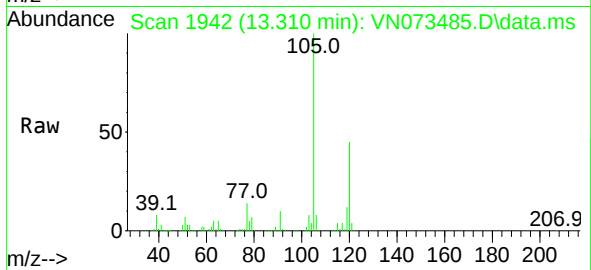

#86
 p-Isopropyltoluene
 Concen: 0.428 ug/l
 RT: 13.498 min Scan# 1974
 Delta R.T. -0.053 min
 Lab File: VN073485.D
 Acq: 15 Jul 2022 15:01

Tgt Ion:119 Resp: 5967
 Ion Ratio Lower Upper
 119 100
 134 25.8 13.3 39.8
 91 32.1 11.3 33.9



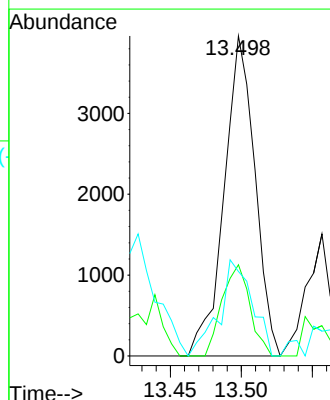
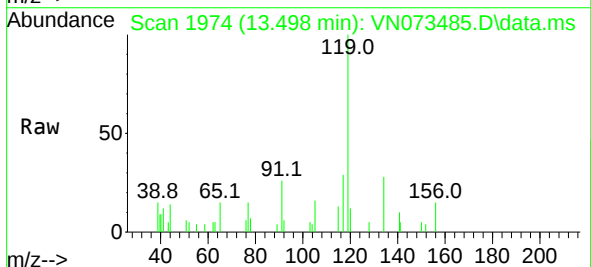




#89
n-Butylbenzene
Concen: 0.398 ug/l
RT: 13.880 min Scan# 2039
Delta R.T. 0.000 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01




Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL


Tgt Ion: 91 Resp: 4630
Ion Ratio Lower Upper
91 100
92 54.1 26.9 80.7
134 0.0 13.6 40.8#

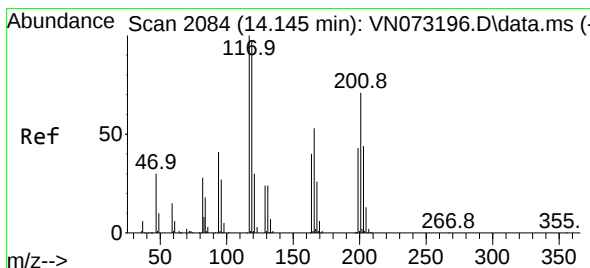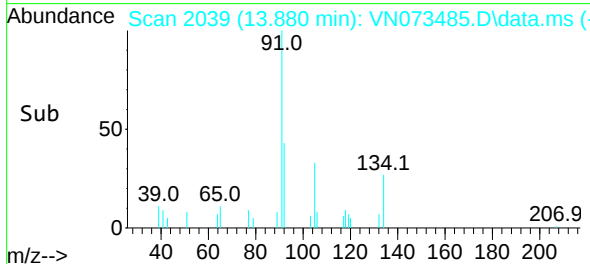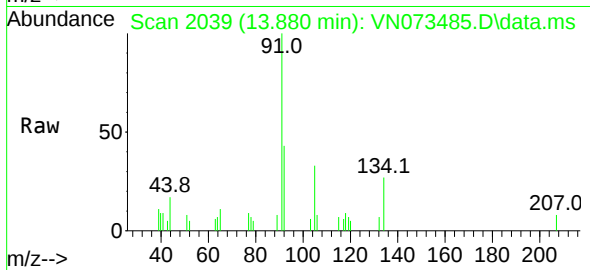

#90
Hexachloroethane
Concen: 1.023 ug/l
RT: 14.151 min Scan# 2085
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 117 Resp: 2659
Ion Ratio Lower Upper
117 100
201 0.0 40.6 122.0#




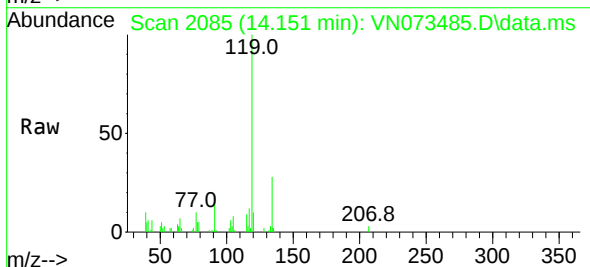


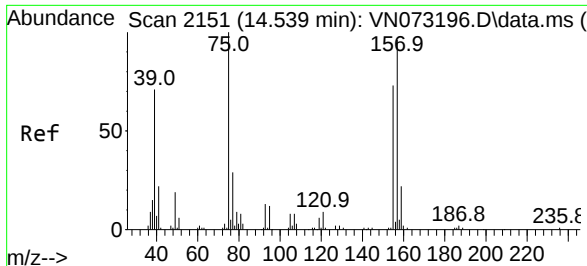

#92
1,2-Dibromo-3-Chloropropane
Concen: 0.213 ug/l
RT: 14.527 min Scan# 2151
Delta R.T. -0.012 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Instrument :
MSVOA_N
ClientSampleId :
TW-ANOMDL

Tgt Ion: 75 Resp: 302
Ion Ratio Lower Upper
75 100
155 0.0 44.9 134.5#
157 0.0 59.0 176.8#

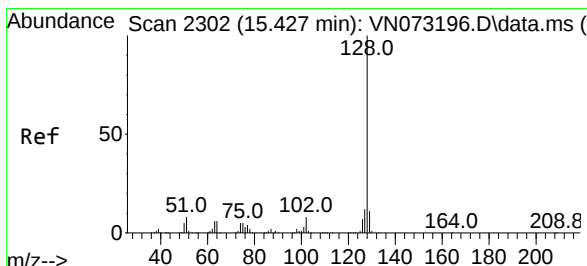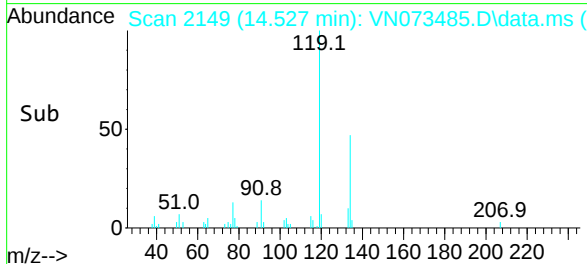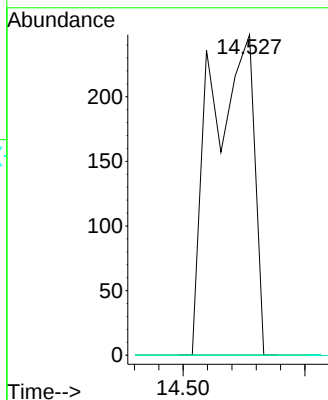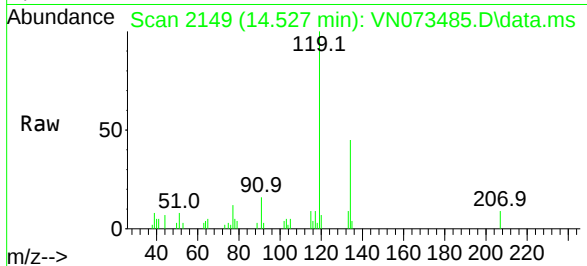

#95
Naphthalene
Concen: 11.544 ug/l
RT: 15.433 min Scan# 2303
Delta R.T. 0.006 min
Lab File: VN073485.D
Acq: 15 Jul 2022 15:01

Tgt Ion: 128 Resp: 181248
Ion Ratio Lower Upper
128 100
127 12.6 10.3 15.5
129 10.8 8.6 13.0

