


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071522\
Data File : VN073473.D
Acq On : 15 Jul 2022 09:24
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 01:54:03 2022

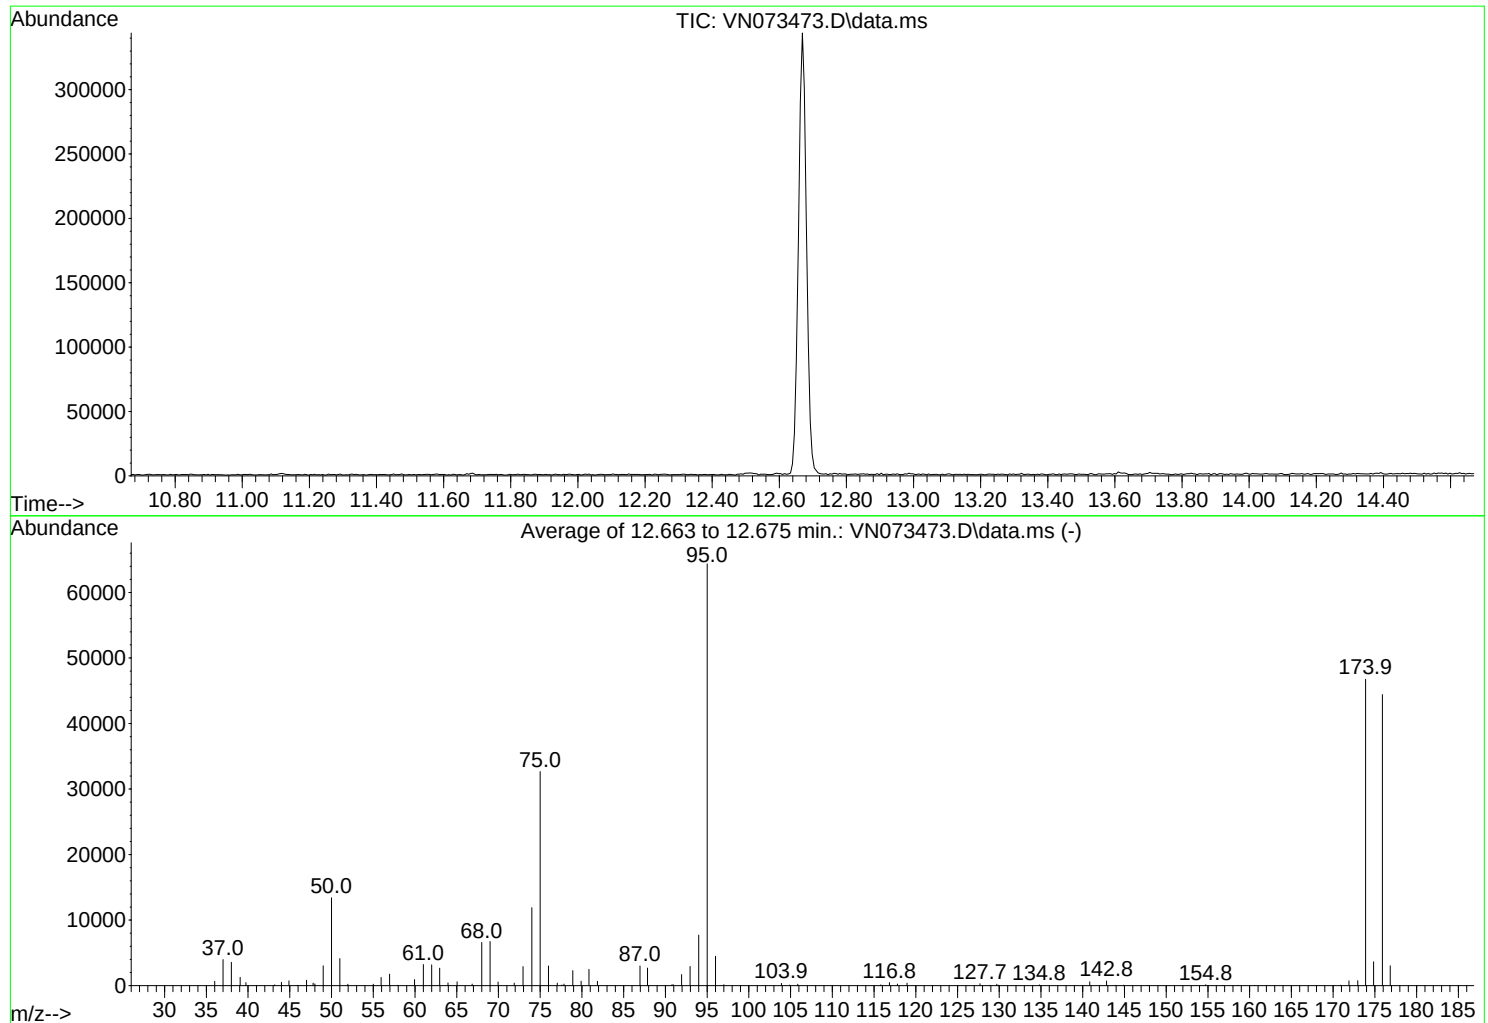

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	13396	PASS
75	95	30	60	50.8	32669	PASS
95	95	100	100	100.0	64371	PASS
96	95	5	9	7.0	4496	PASS
173	174	0.00	2	1.6	760	PASS
174	95	50	100	72.6	46765	PASS
175	174	5	9	7.8	3639	PASS
176	174	95	101	95.0	44424	PASS
177	176	5	9	6.8	3041	PASS