


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071524\
Data File : VN082914.D
Acq On : 15 Jul 2024 11:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

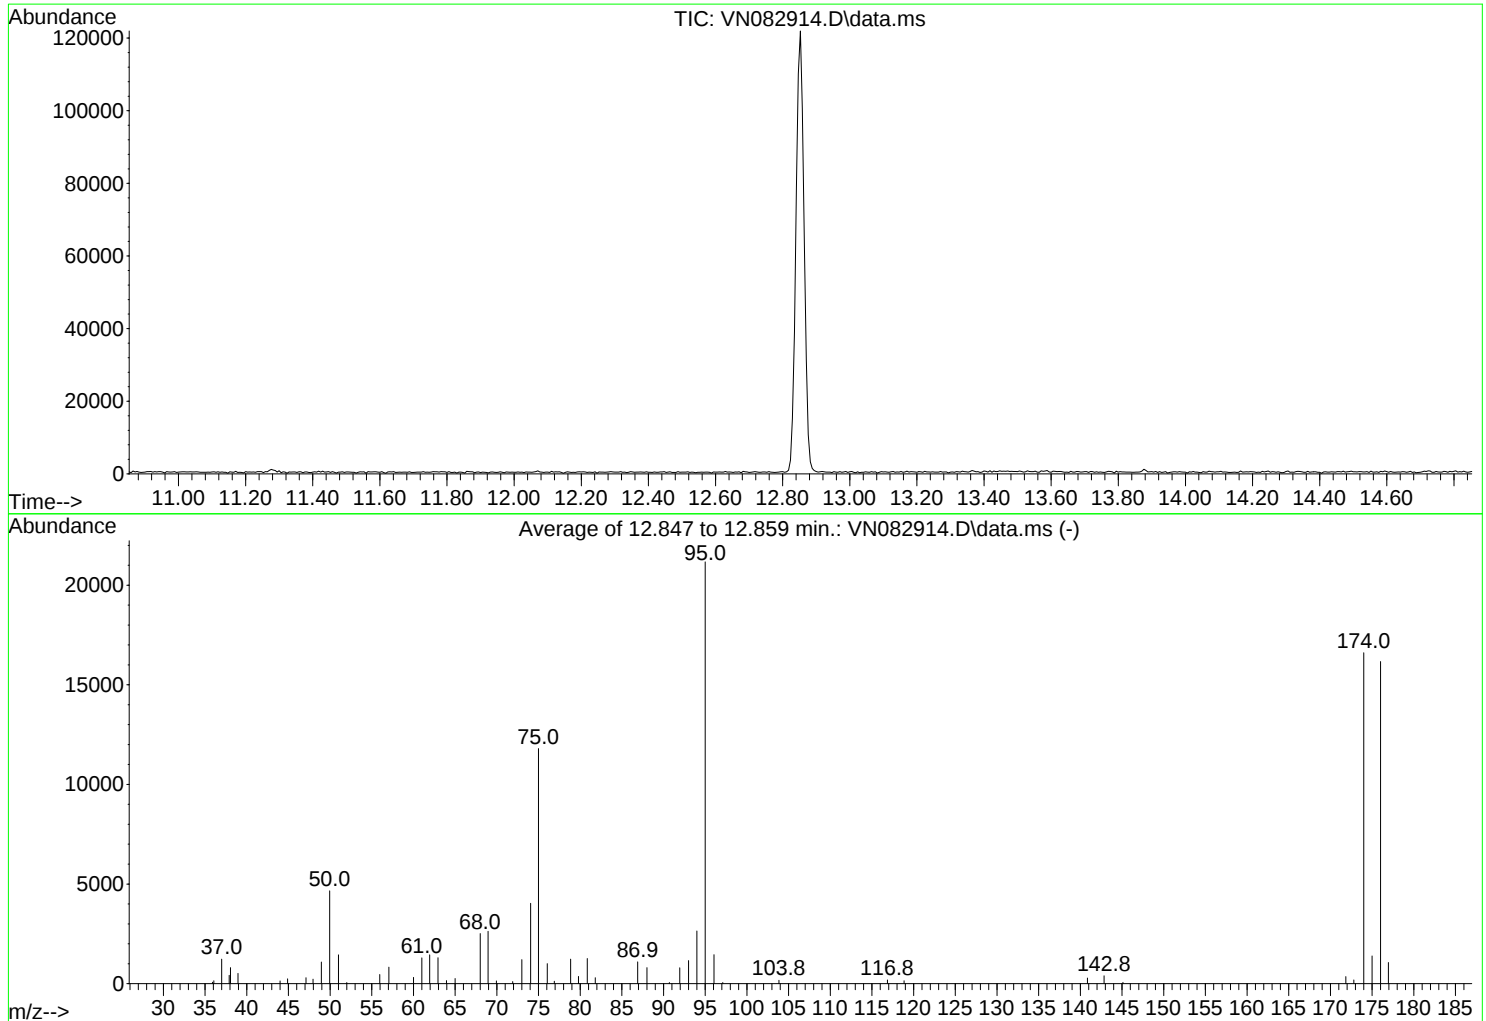

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.0	4657	PASS
75	95	30	60	55.7	11800	PASS
95	95	100	100	100.0	21173	PASS
96	95	5	9	6.9	1451	PASS
173	174	0.00	2	1.1	188	PASS
174	95	50	100	78.4	16606	PASS
175	174	5	9	8.4	1390	PASS
176	174	95	101	97.4	16172	PASS
177	176	5	9	6.6	1060	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	72	49.95	4657	68.00	2518	80.85	1261
36.05	145	51.00	1443	68.95	2623	81.80	291
37.00	1232	52.00	56	69.95	137	86.90	109
37.90	417	55.95	455	71.90	102	88.00	80
38.05	807	57.05	824	73.00	1206	90.70	56
38.95	518	60.00	311	74.05	4030	91.95	799
44.00	137	61.00	1294	75.00	11800	93.00	1153
44.90	241	61.95	1444	76.05	1005	94.00	2644
47.10	294	62.95	1304	76.90	123	95.00	21173
47.95	227	63.95	150	78.85	1233	96.05	1451
48.95	1082	65.00	258	79.80	364	97.10	56

Average of 12.847 to 12.859 min.: VN082914.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
103.85	166	176.95	1060				
116.85	183						
118.85	143						
140.85	283						
142.85	391						
145.10	63						
171.85	353						
172.80	188						
174.00	16606						
175.00	1390						
176.00	16172						

Instrument :

MSVOA_N

ClientSampleId :

BFB