

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071624\
 Data File : VN082935.D
 Acq On : 16 Jul 2024 14:51
 Operator : JC\MD
 Sample : IBLK
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Jul 17 00:55:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	89051	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	171051	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	169197	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	72837	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	60003	48.067	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	96.140%
35) Dibromofluoromethane	8.171	113	49447	45.050	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	90.100%
50) Toluene-d8	10.571	98	181406	44.748	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.500%
62) 4-Bromofluorobenzene	12.853	95	62284	42.771	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	85.540%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071624\
Data File : VN082935.D
Acq On : 16 Jul 2024 14:51
Operator : JC\MD
Sample : IBLK
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Jul 17 00:55:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration




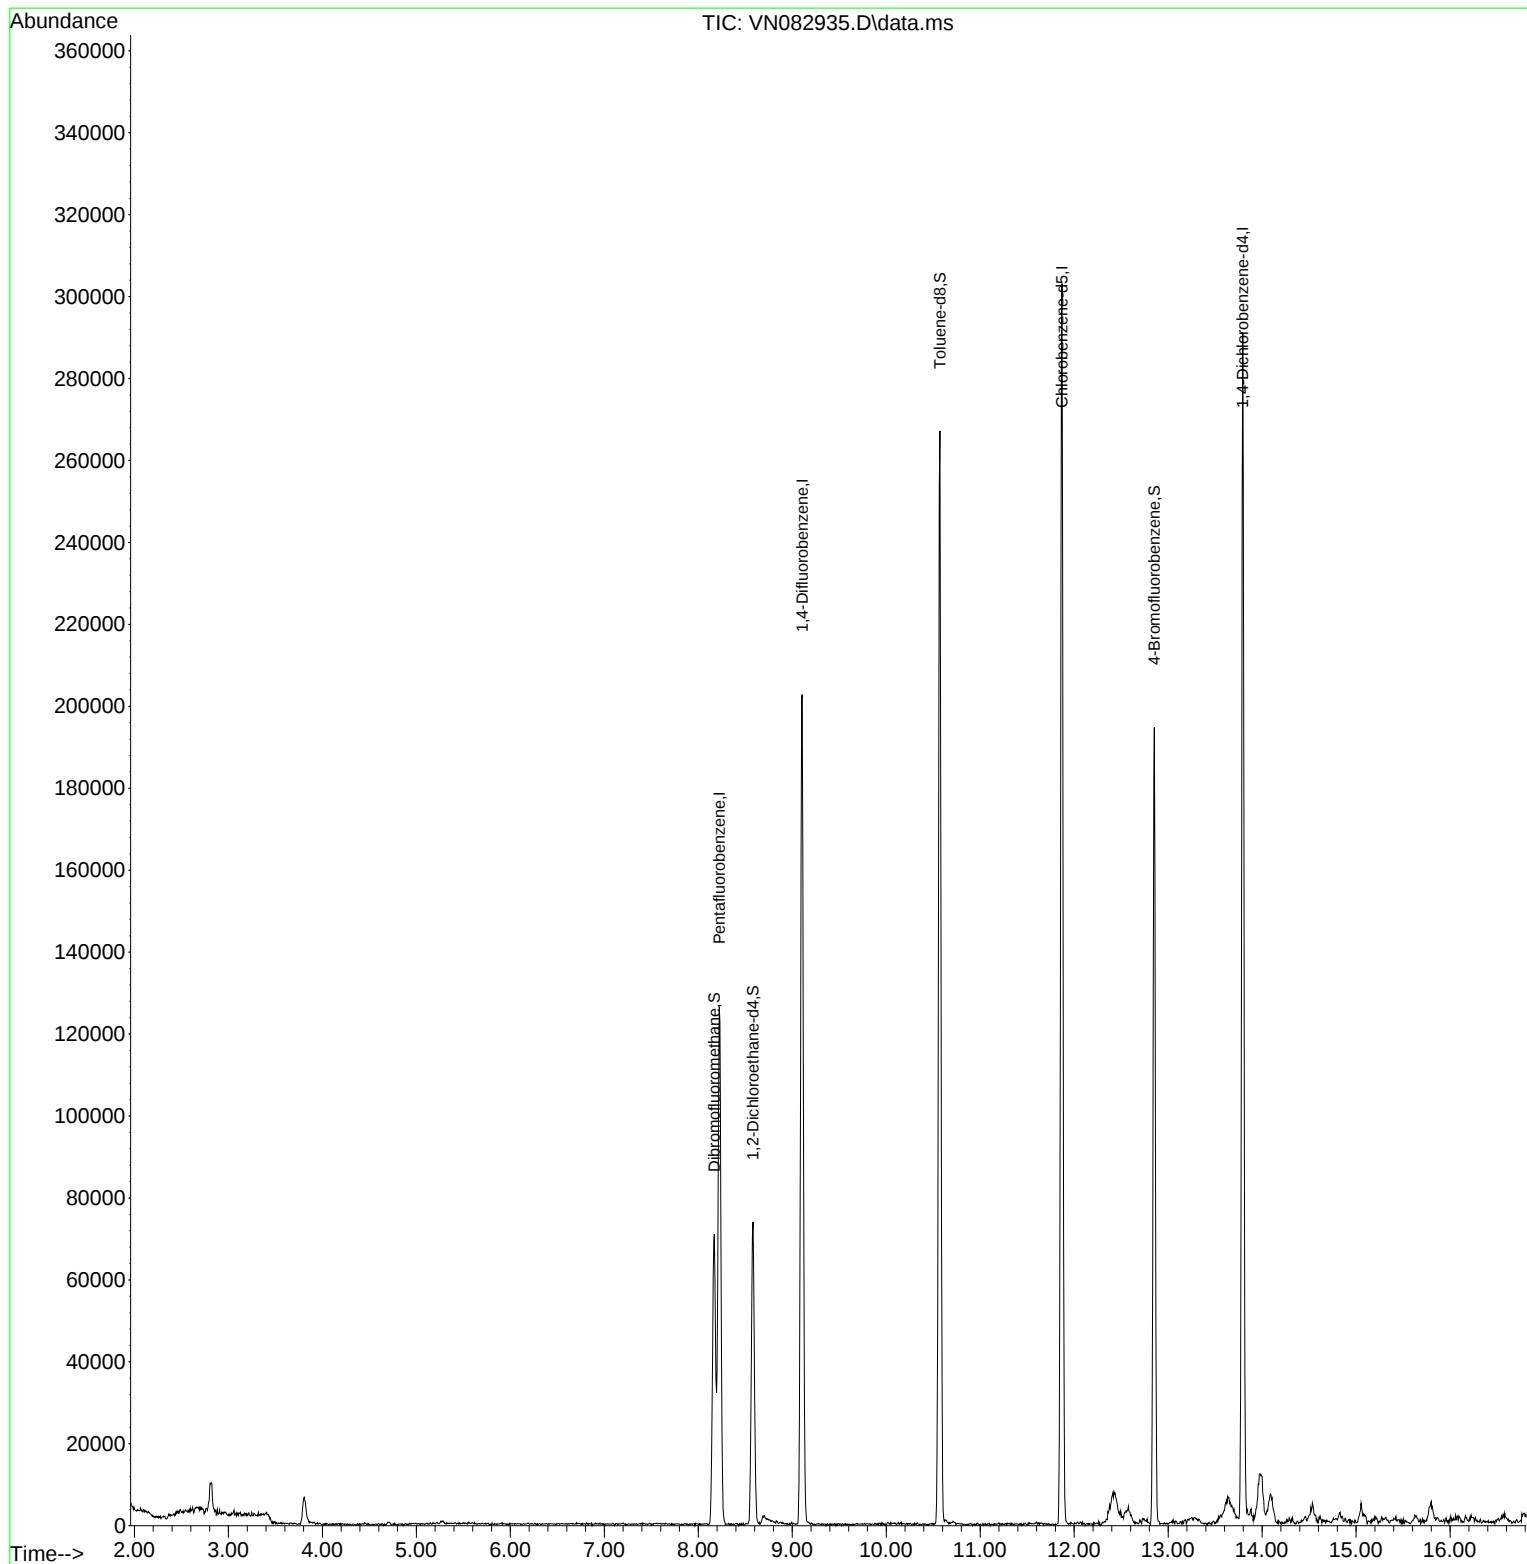


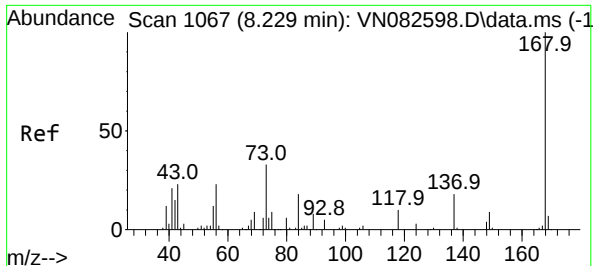

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.005 min
Lab File: VN082935.D
Acq: 16 Jul 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion:168 Resp: 89051
Ion Ratio Lower Upper
168 100
99 58.6 48.2 72.4

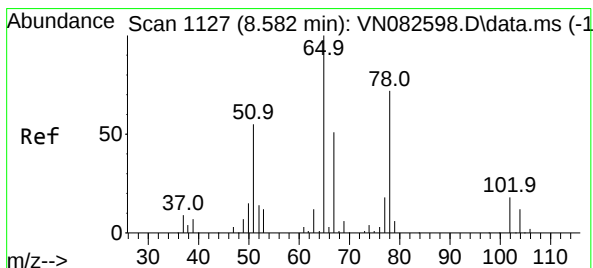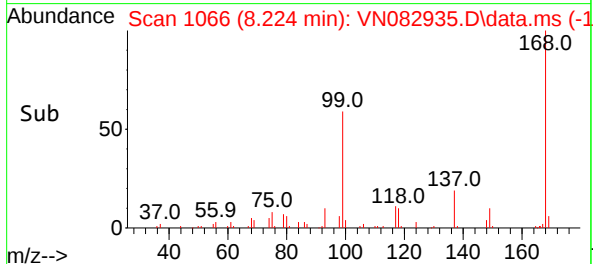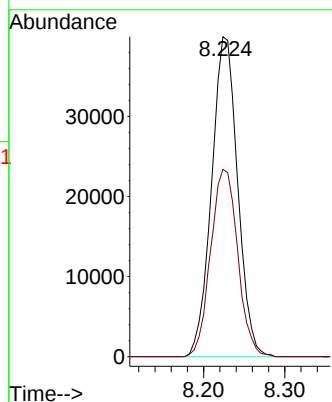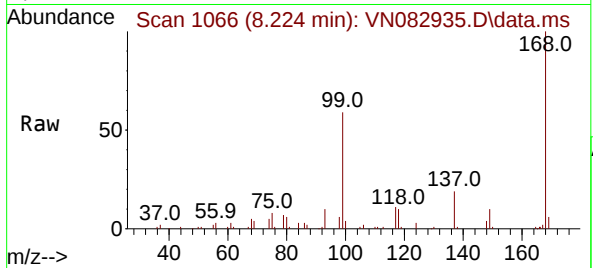

#33
1,2-Dichloroethane-d4
Concen: 48.067 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN082935.D
Acq: 16 Jul 2024 14:51

Tgt Ion: 65 Resp: 60003
Ion Ratio Lower Upper
65 100
67 52.6 0.0 104.4

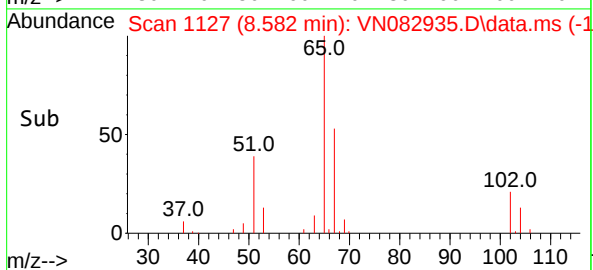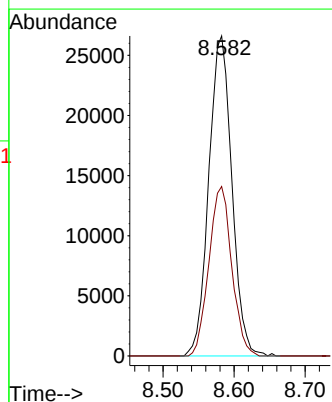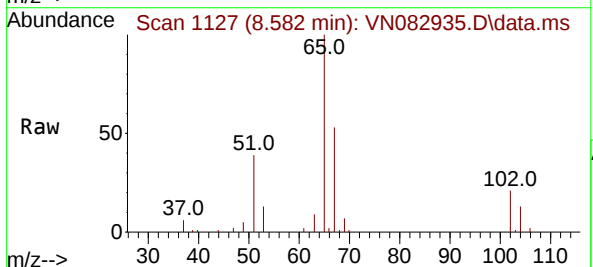

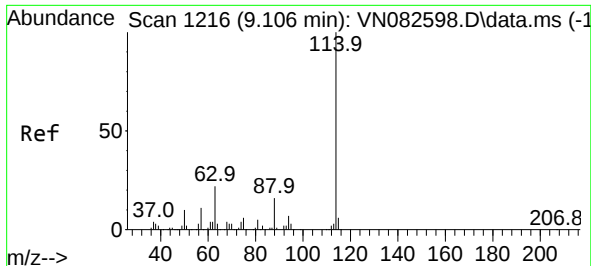

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN082935.D

Acq: 16 Jul 2024 14:51

Instrument :

MSVOA_N

ClientSampleId :

IBLK





Tgt Ion:114 Resp: 171051

Ion Ratio Lower Upper

114 100

63 21.1 0.0 44.6

88 14.9 0.0 31.4

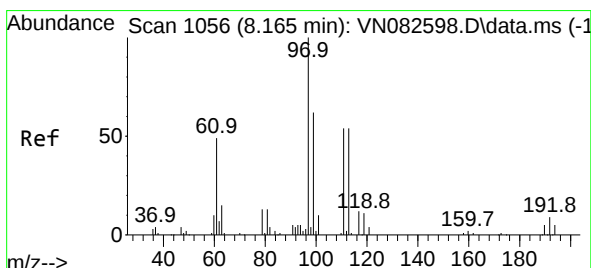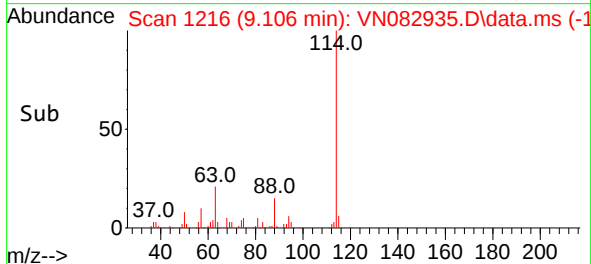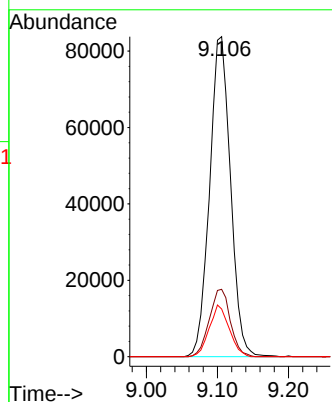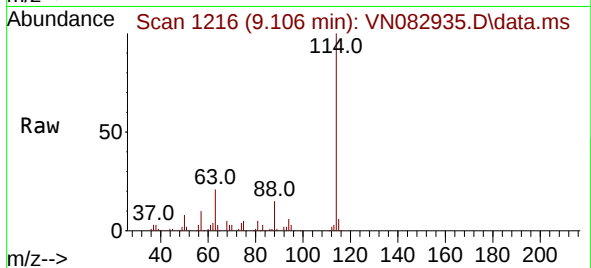

#35

Dibromofluoromethane

Concen: 45.050 ug/l

RT: 8.171 min Scan# 1057

Delta R.T. 0.006 min

Lab File: VN082935.D

Acq: 16 Jul 2024 14:51




Tgt Ion:113 Resp: 49447


Ion Ratio Lower Upper

113 100

111 105.4 82.4 123.6

192 18.2 14.9 22.3


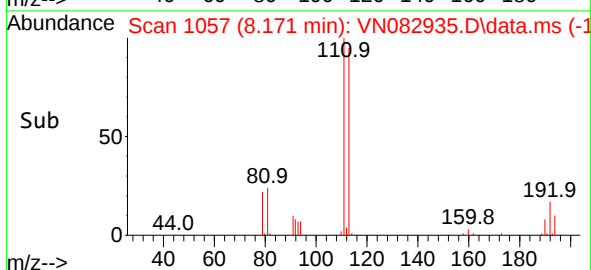
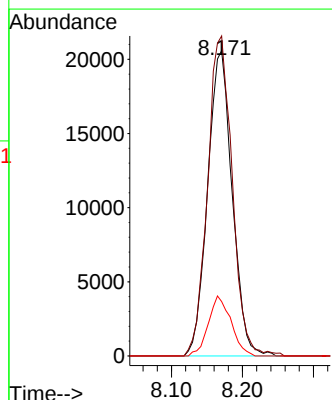
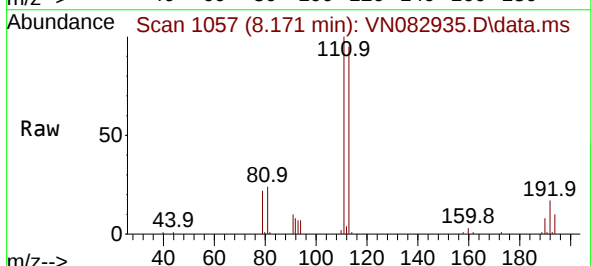


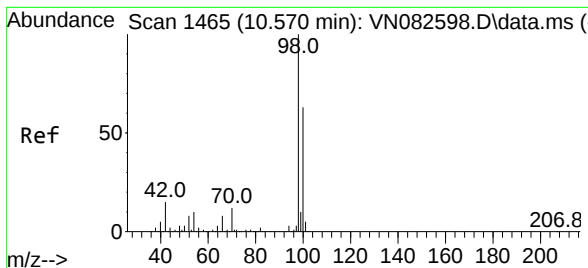

#50
Toluene-d8
Concen: 44.748 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN082935.D
Acq: 16 Jul 2024 14:51




Instrument :
MSVOA_N
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 181406
Ion Ratio Lower Upper
98 100
100 63.8 51.5 77.3

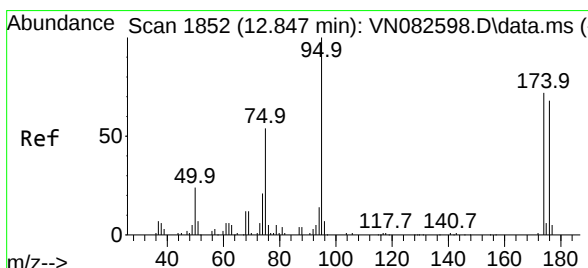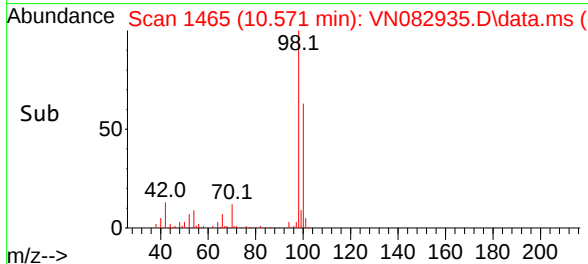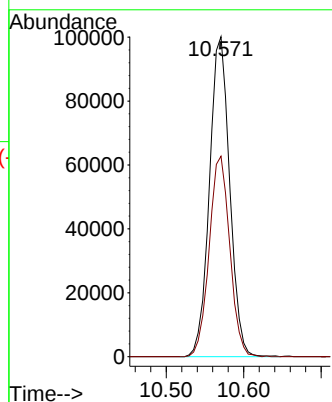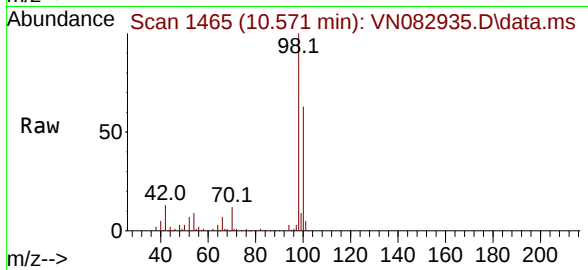

#62
4-Bromofluorobenzene
Concen: 42.771 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082935.D
Acq: 16 Jul 2024 14:51

Tgt Ion: 95 Resp: 62284
Ion Ratio Lower Upper
95 100
174 78.1 0.0 159.2
176 75.7 0.0 147.6


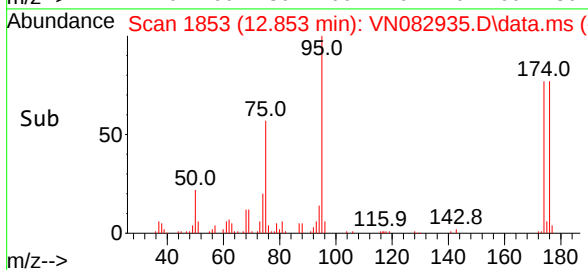
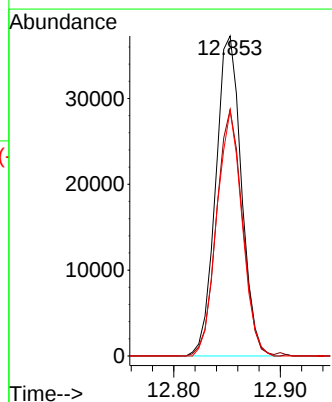
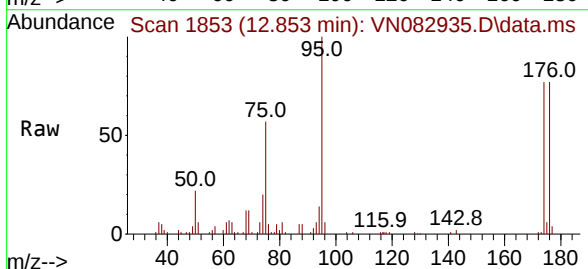


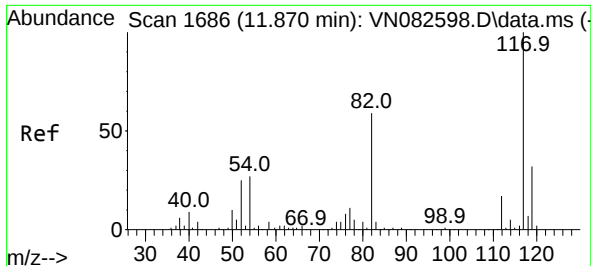

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 1169
Delta R.T. 0.000 min
Lab File: VN082935.D
Acq: 16 Jul 2024 14:51

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Tgt Ion:117 Resp: 169197
Ion Ratio Lower Upper
117 100
82 54.8 47.5 71.3
119 33.1 25.6 38.4

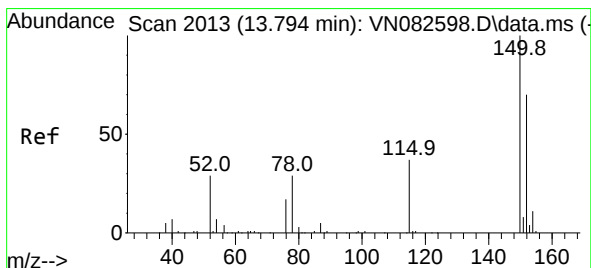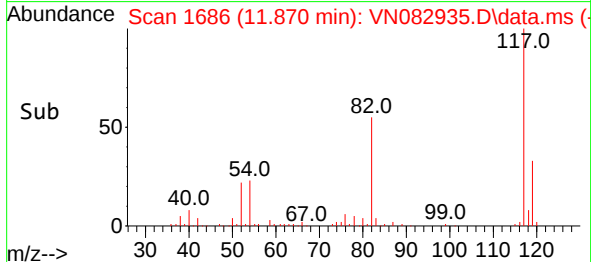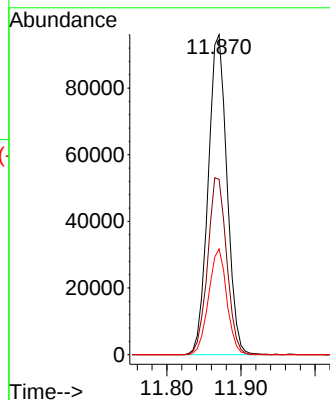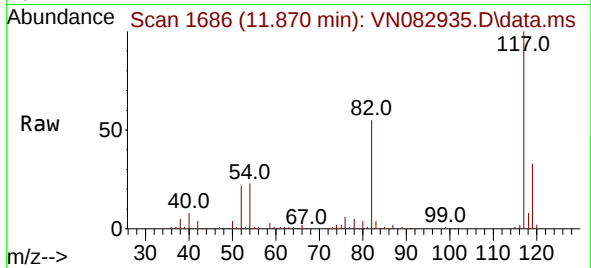

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082935.D
Acq: 16 Jul 2024 14:51

Tgt Ion:152 Resp: 72837
Ion Ratio Lower Upper
152 100
115 63.3 30.6 91.6
150 161.7 0.0 348.6

