
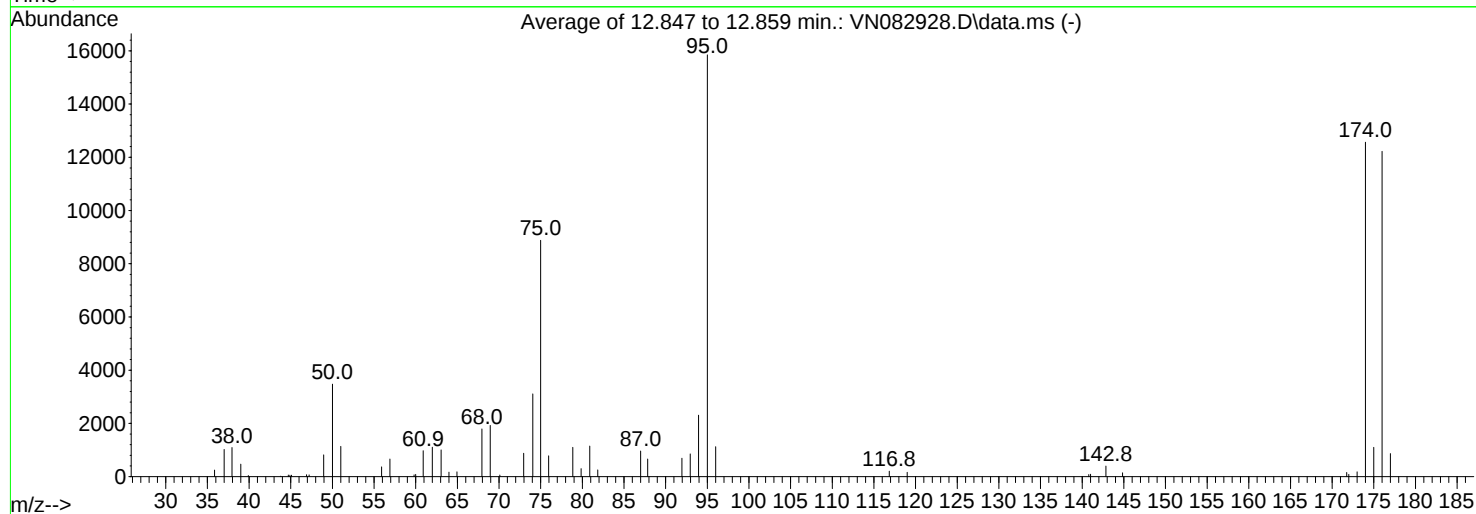


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071624\
Data File : VN082928.D
Acq On : 16 Jul 2024 09:23
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

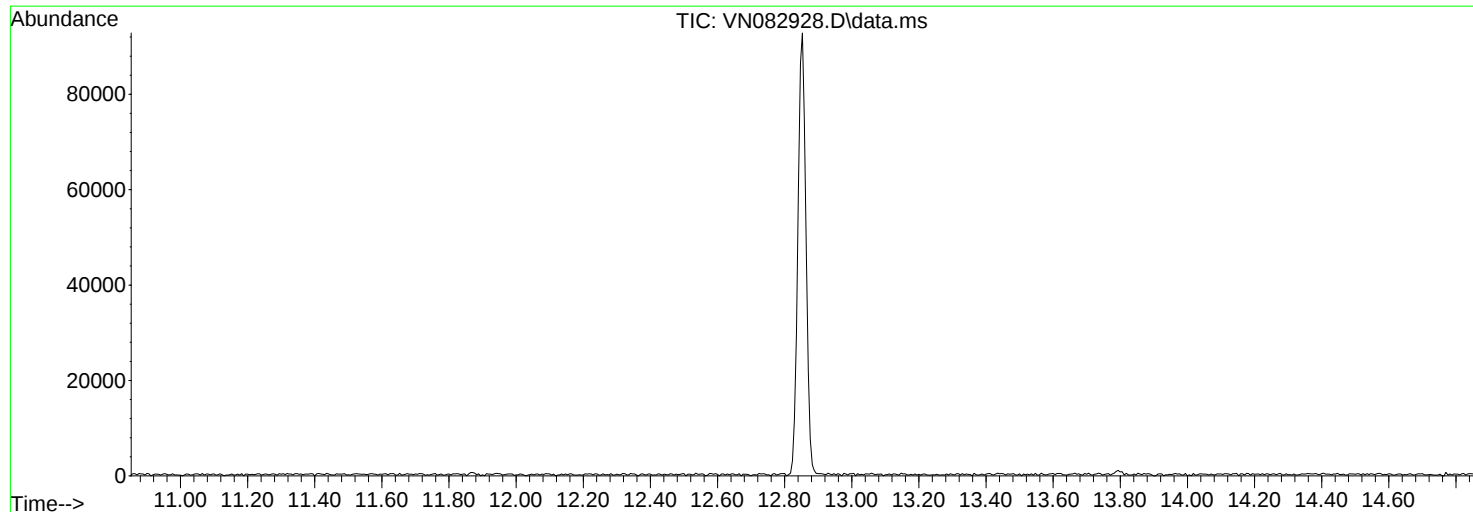

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	3474	PASS
75	95	30	60	56.0	8882	PASS
95	95	100	100	100.0	15849	PASS
96	95	5	9	7.1	1122	PASS
173	174	0.00	2	1.5	183	PASS
174	95	50	100	79.3	12566	PASS
175	174	5	9	8.7	1099	PASS
176	174	95	101	97.3	12222	PASS
177	176	5	9	7.1	868	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	249	48.95	820	64.95	181	81.85	25
37.00	1020	50.00	3474	67.95	1789	87.00	96
37.95	1093	51.00	1134	68.95	1926	87.85	66
39.00	470	55.90	368	70.10	63	91.95	69
39.90	44	56.90	660	72.95	877	92.95	851
43.80	16	59.80	65	74.05	3111	93.95	2308
44.70	61	60.00	85	75.00	8882	95.00	15849
44.90	56	60.90	974	75.95	781	96.00	1122
45.10	55	62.00	1108	78.85	1099	116.85	206
46.90	71	63.05	1006	79.85	300	119.00	165
47.20	66	64.00	169	80.90	1146	140.80	80

Average of 12.847 to 12.859 min.: VN082928.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
141.00	93						
142.85	396						
144.85	144						
171.75	154						
172.00	87						
173.00	183						
174.00	12566						
175.00	1099						
176.00	12222						
177.00	868						

Instrument :

MSVOA_N

ClientSampleId :

BFB