



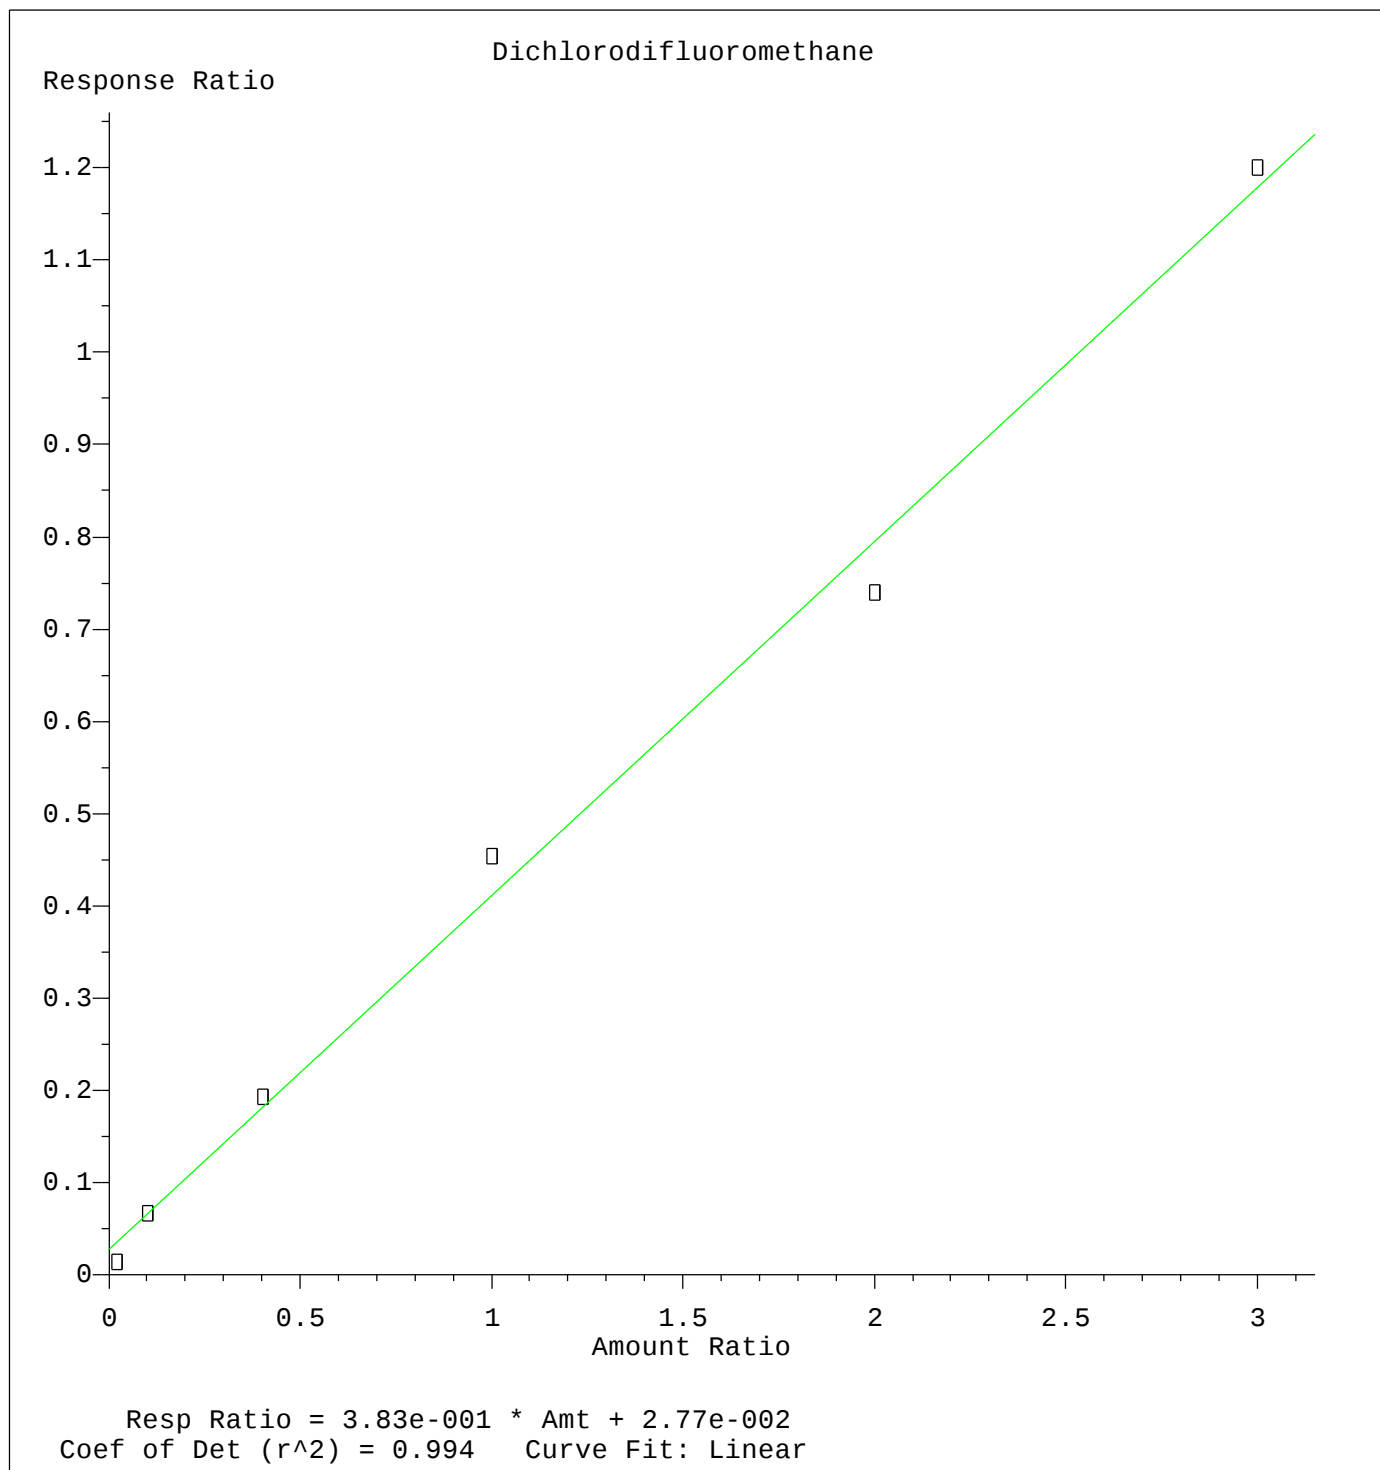

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

Naphthalene

Response Ratio

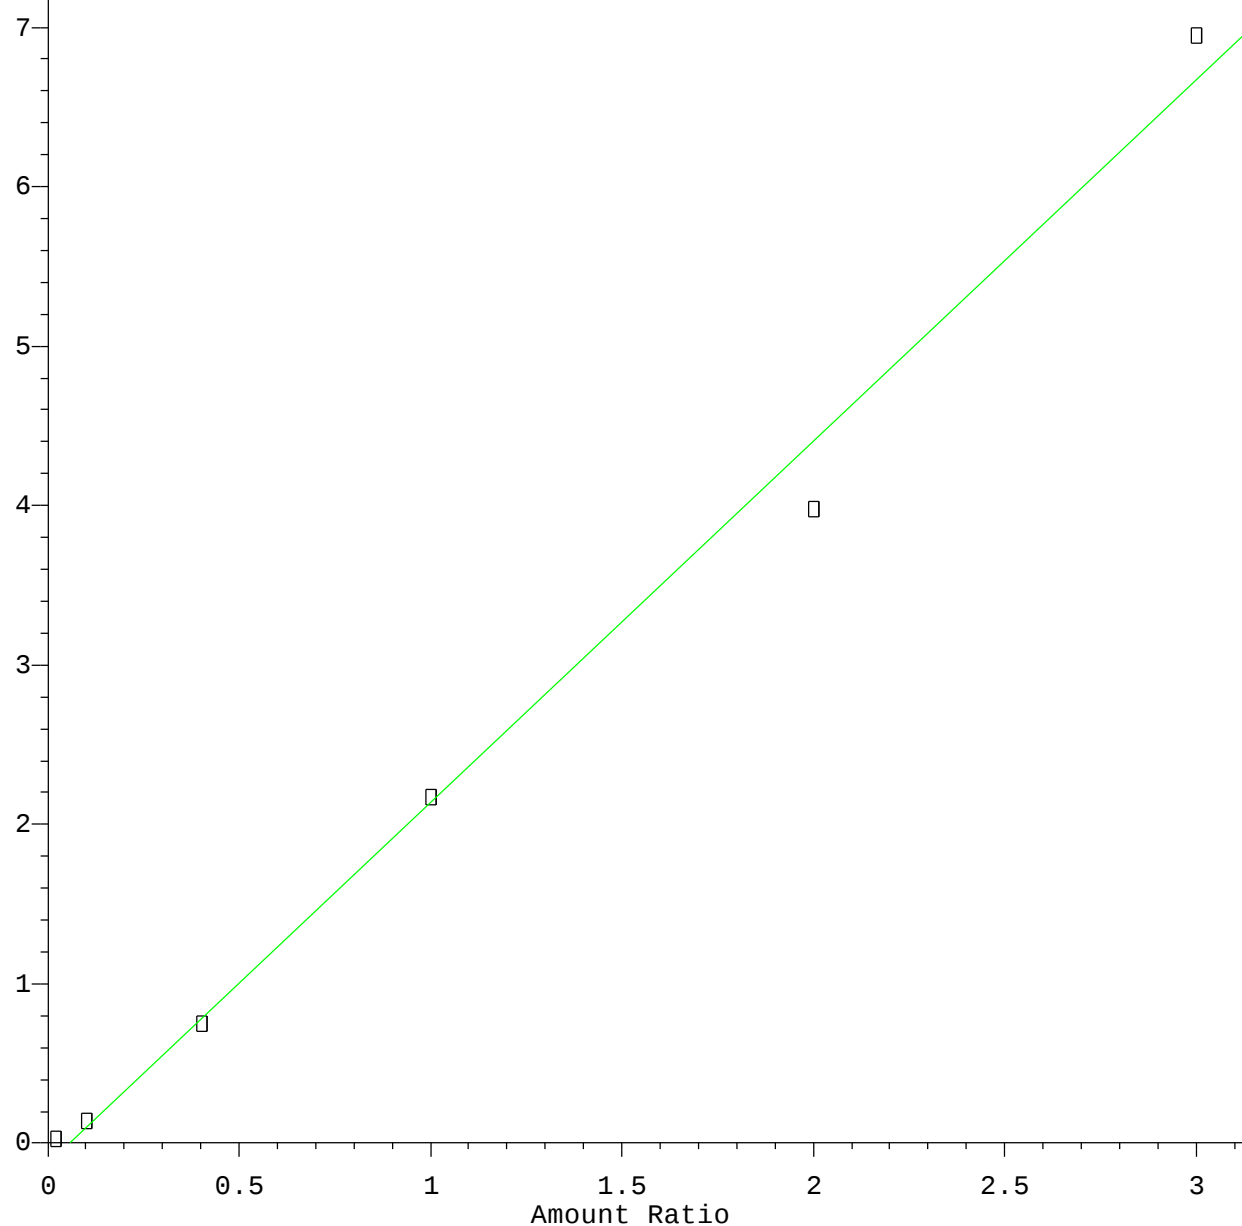


Resp Ratio = 2.26e+000 * Amt - 1.28e-001
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018


1,2-Dibromo-3-Chloropropane

Response Ratio

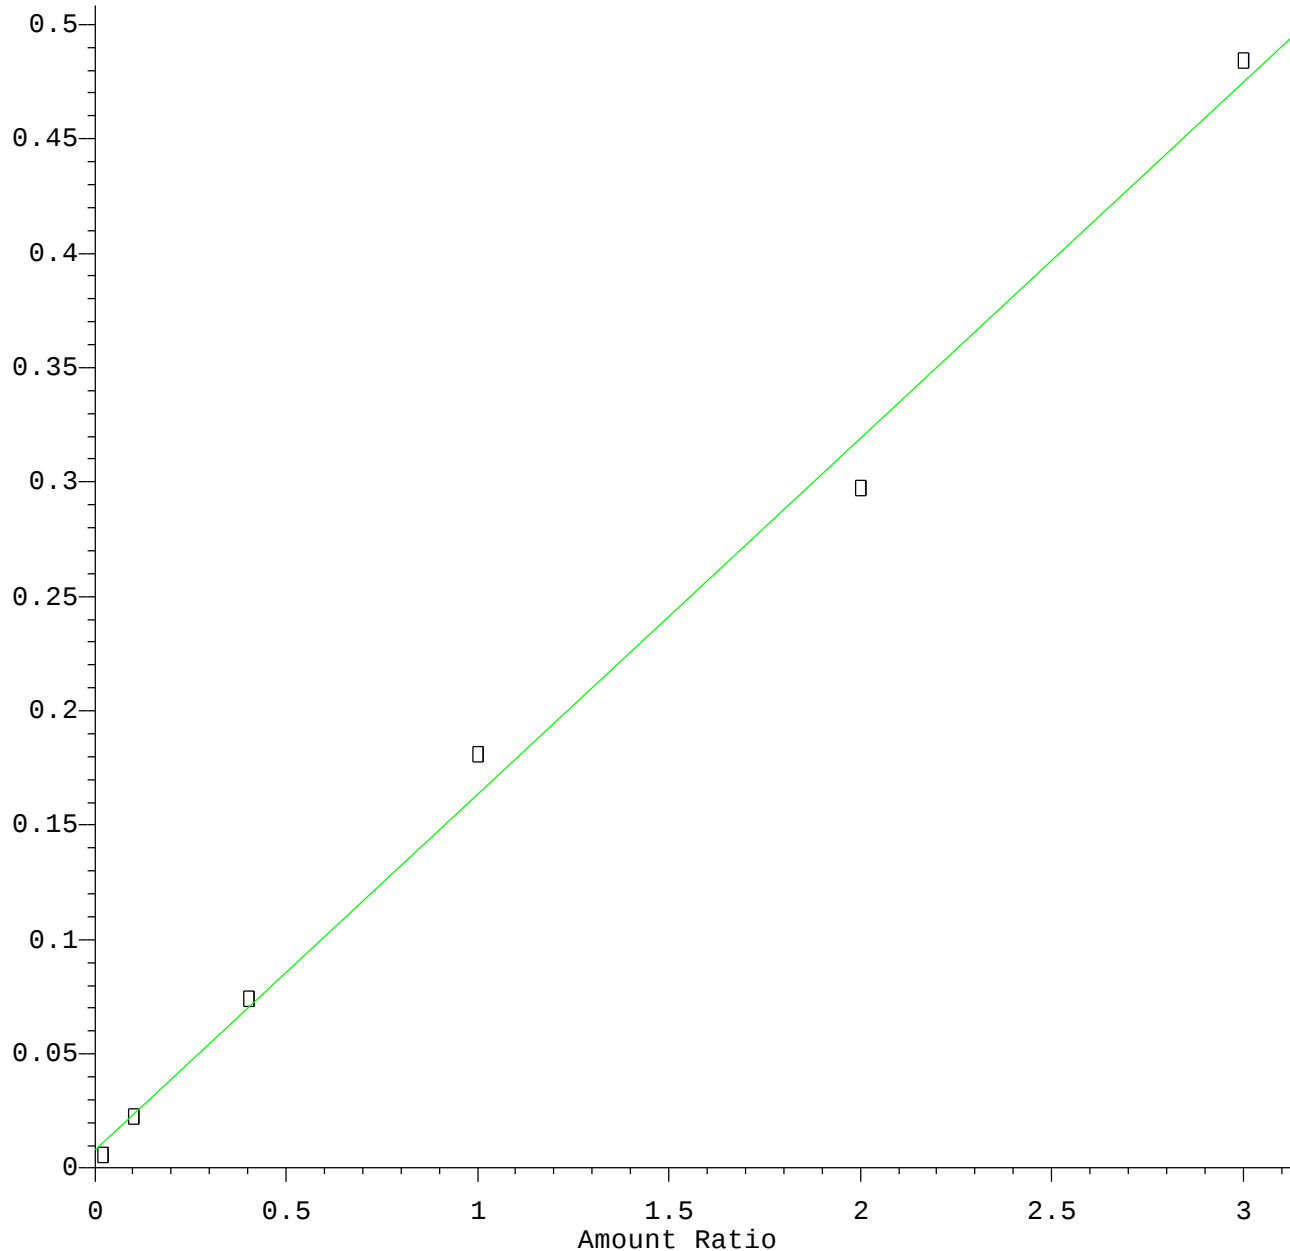


Resp Ratio = $1.56 \times 10^{-1} \times \text{Amt} + 7.98 \times 10^{-3}$
Coef of Det (r^2) = 0.995 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

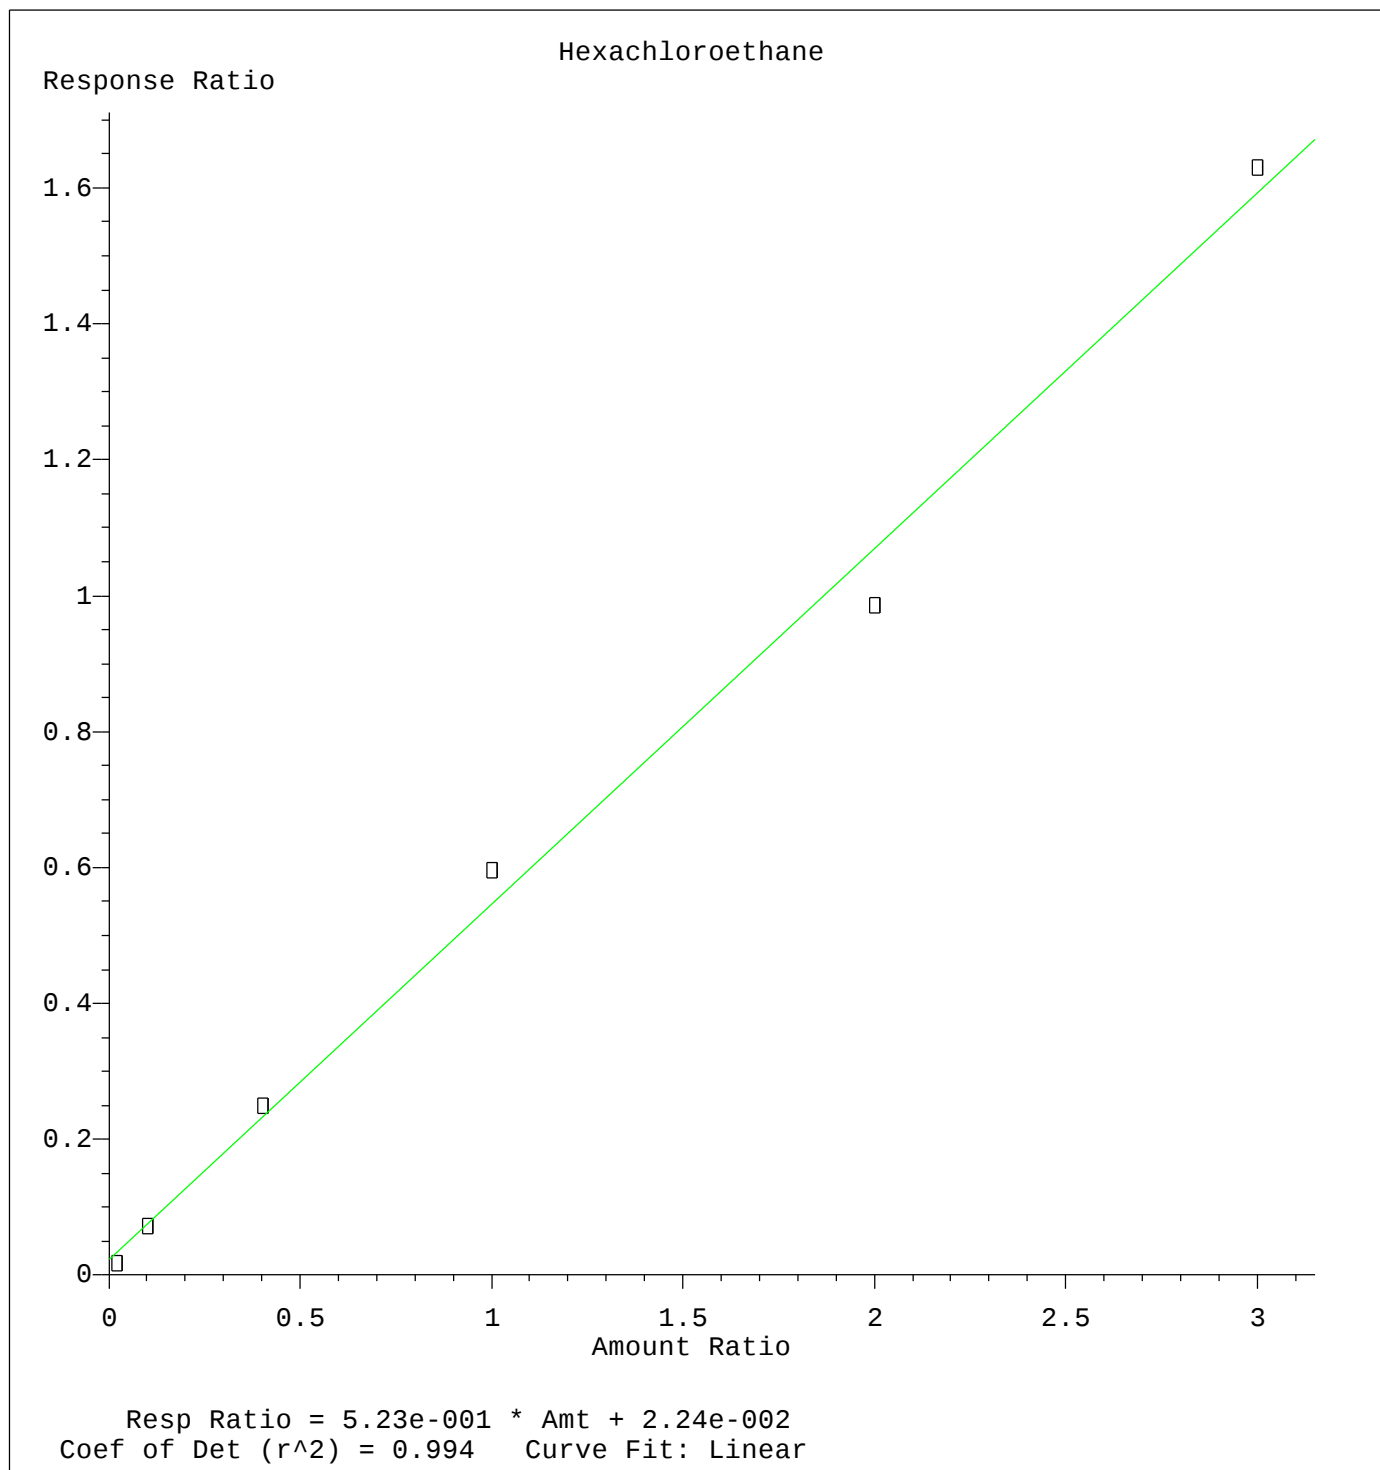


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

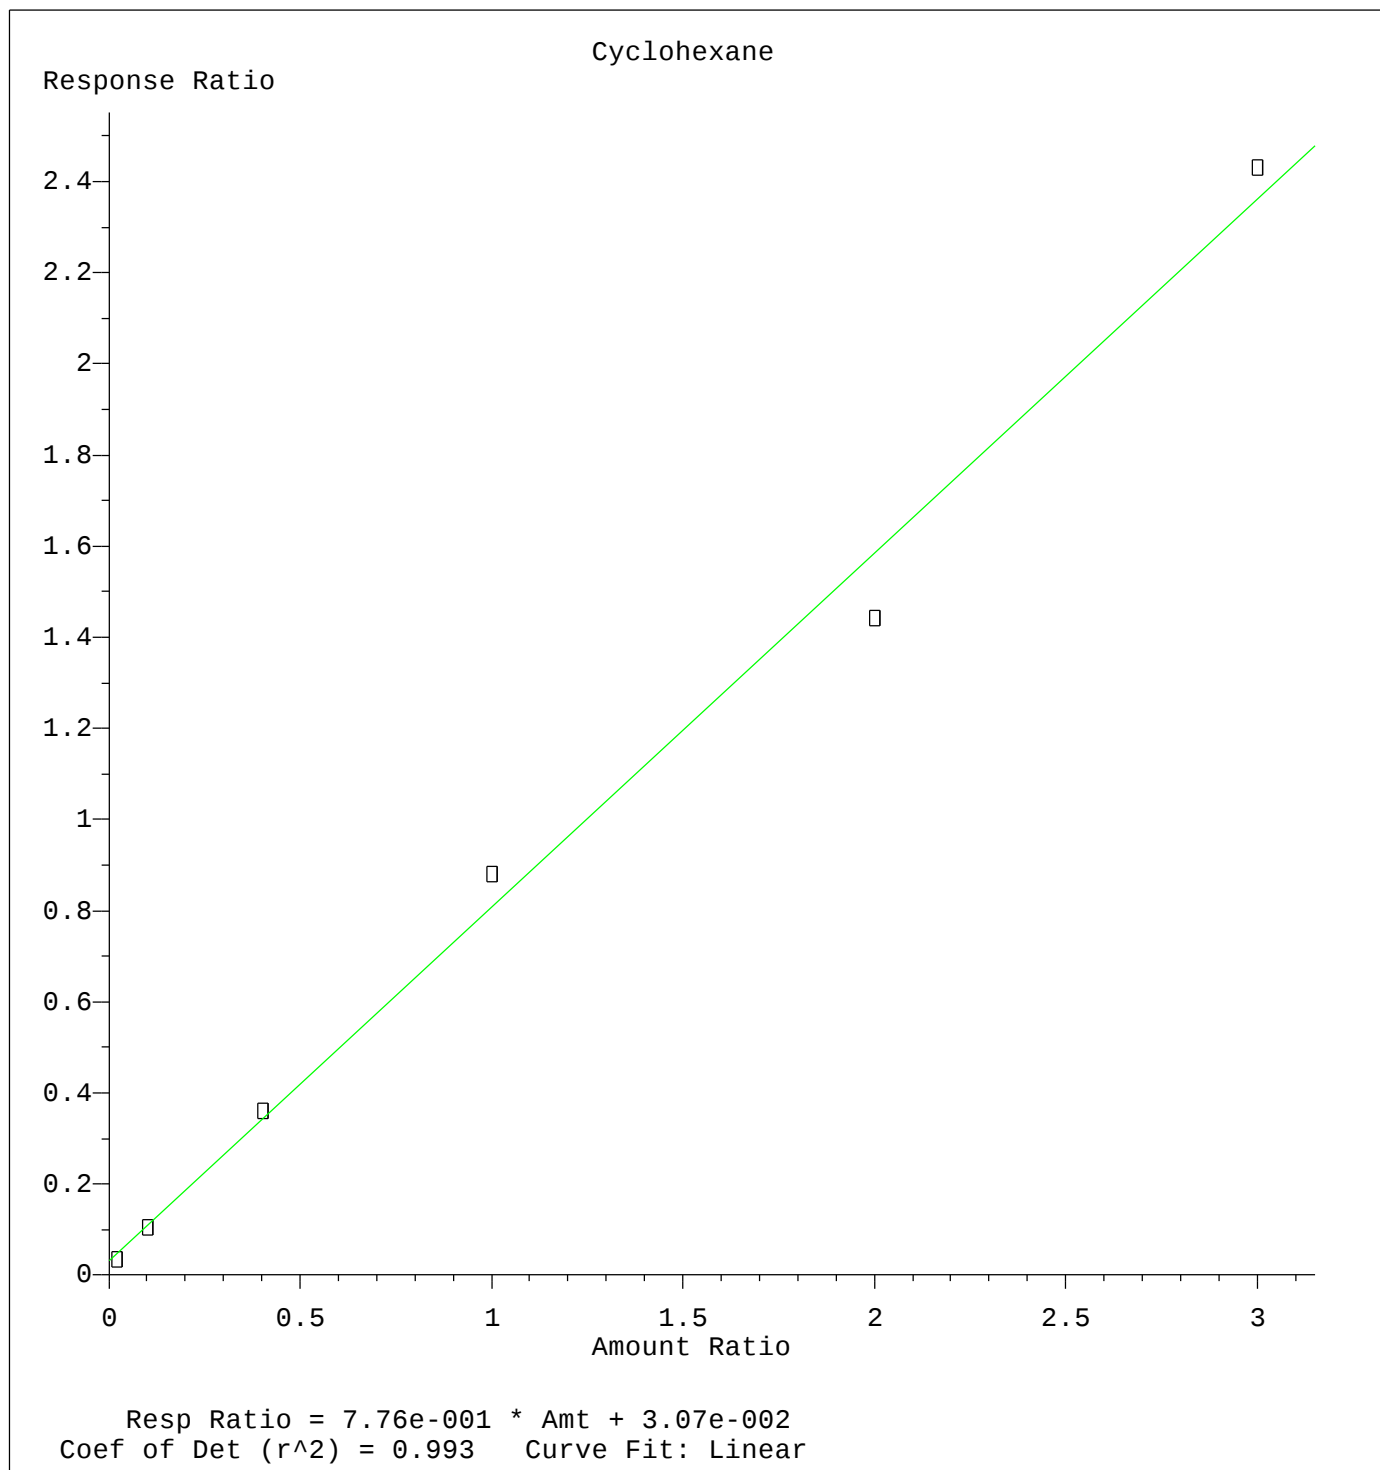

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018


Methylene Chloride

Response Ratio

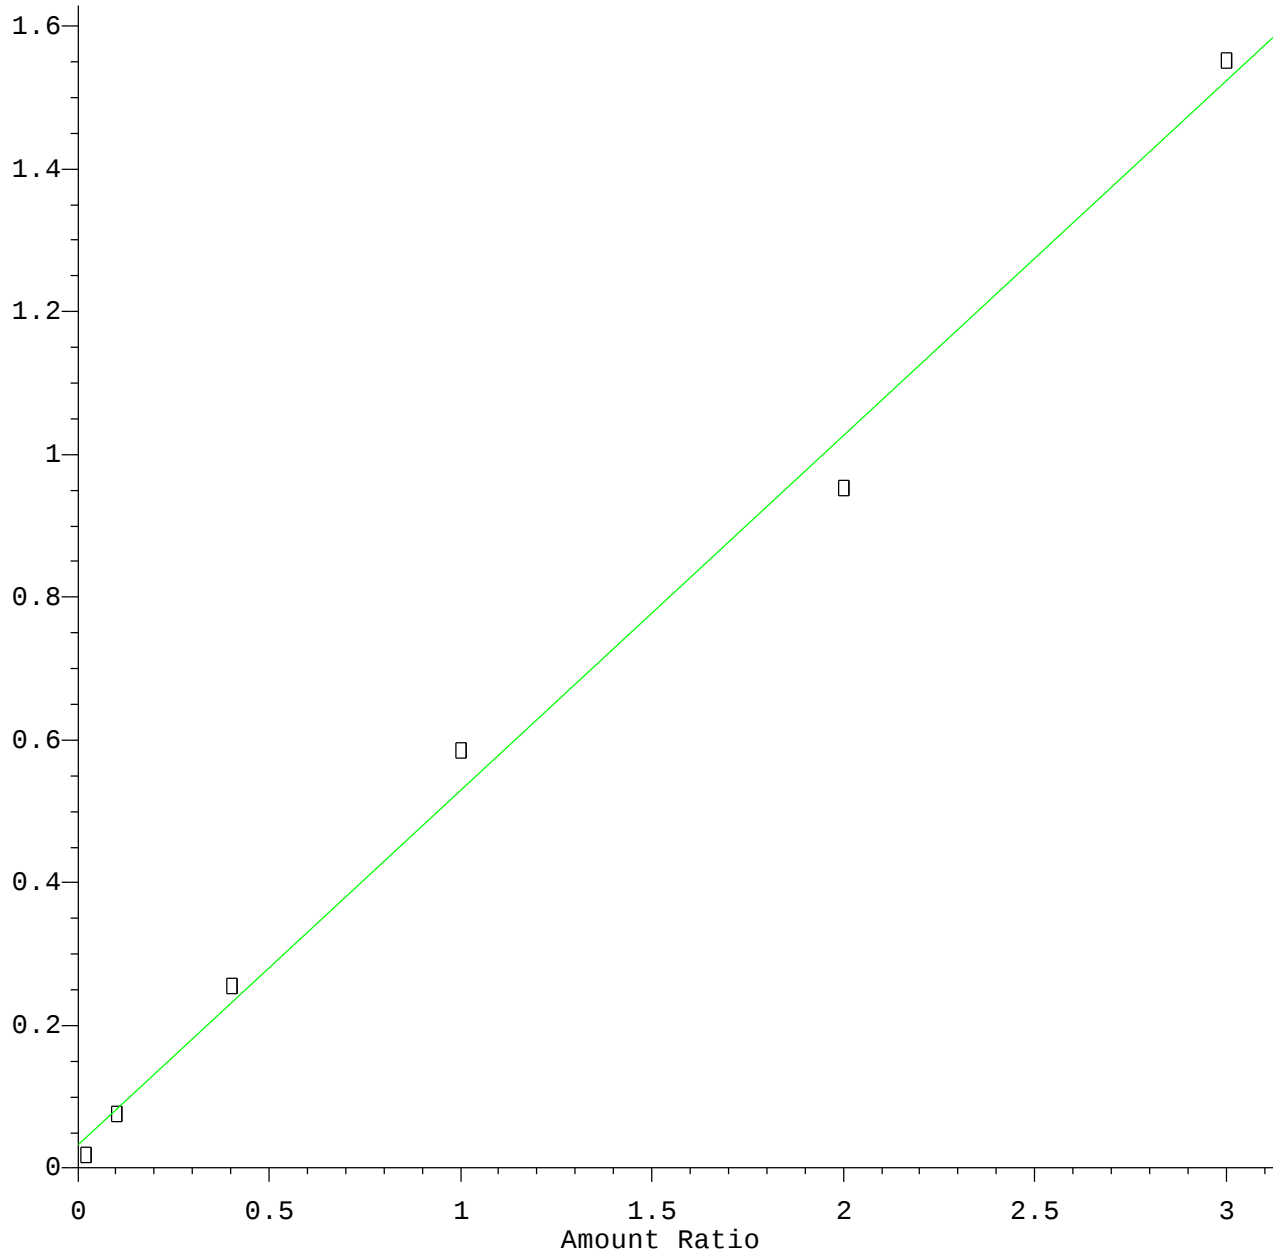


Resp Ratio = $4.96 \times 10^{-1} \times \text{Amt} + 3.29 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

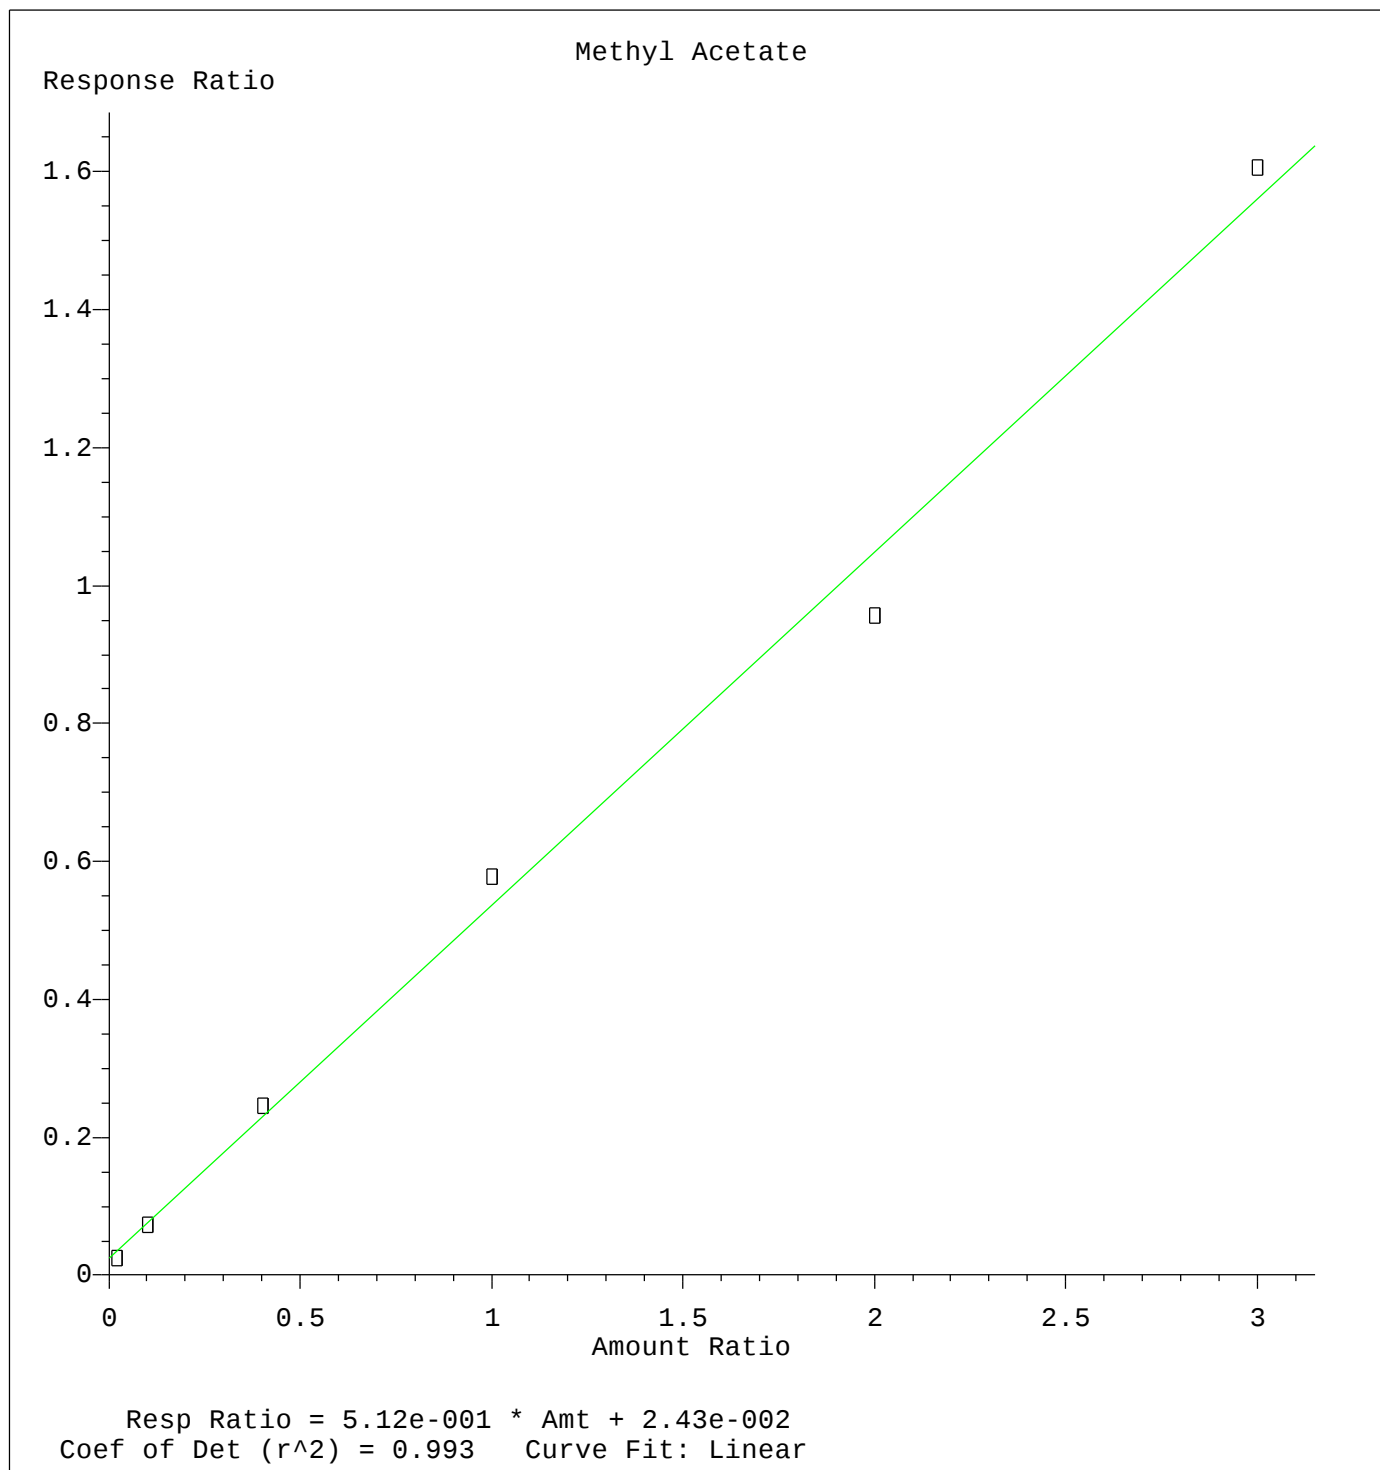

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

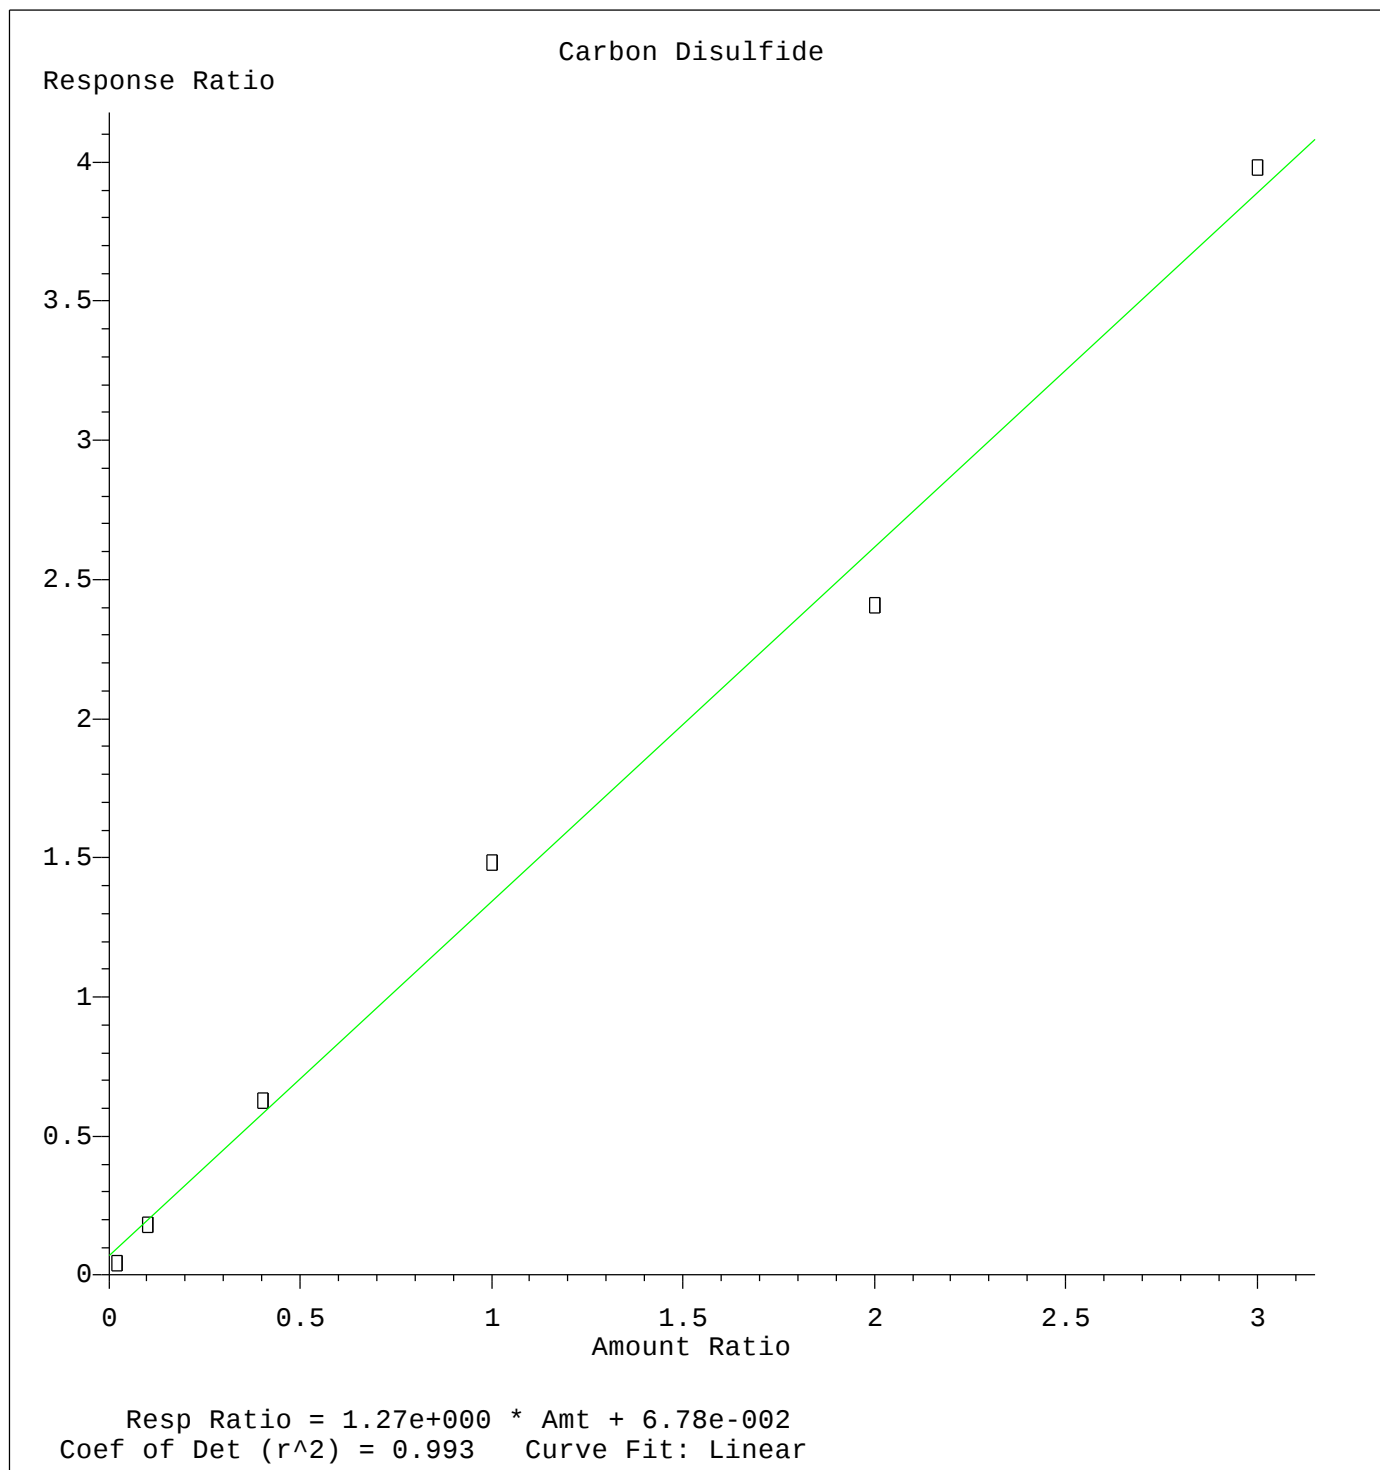


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

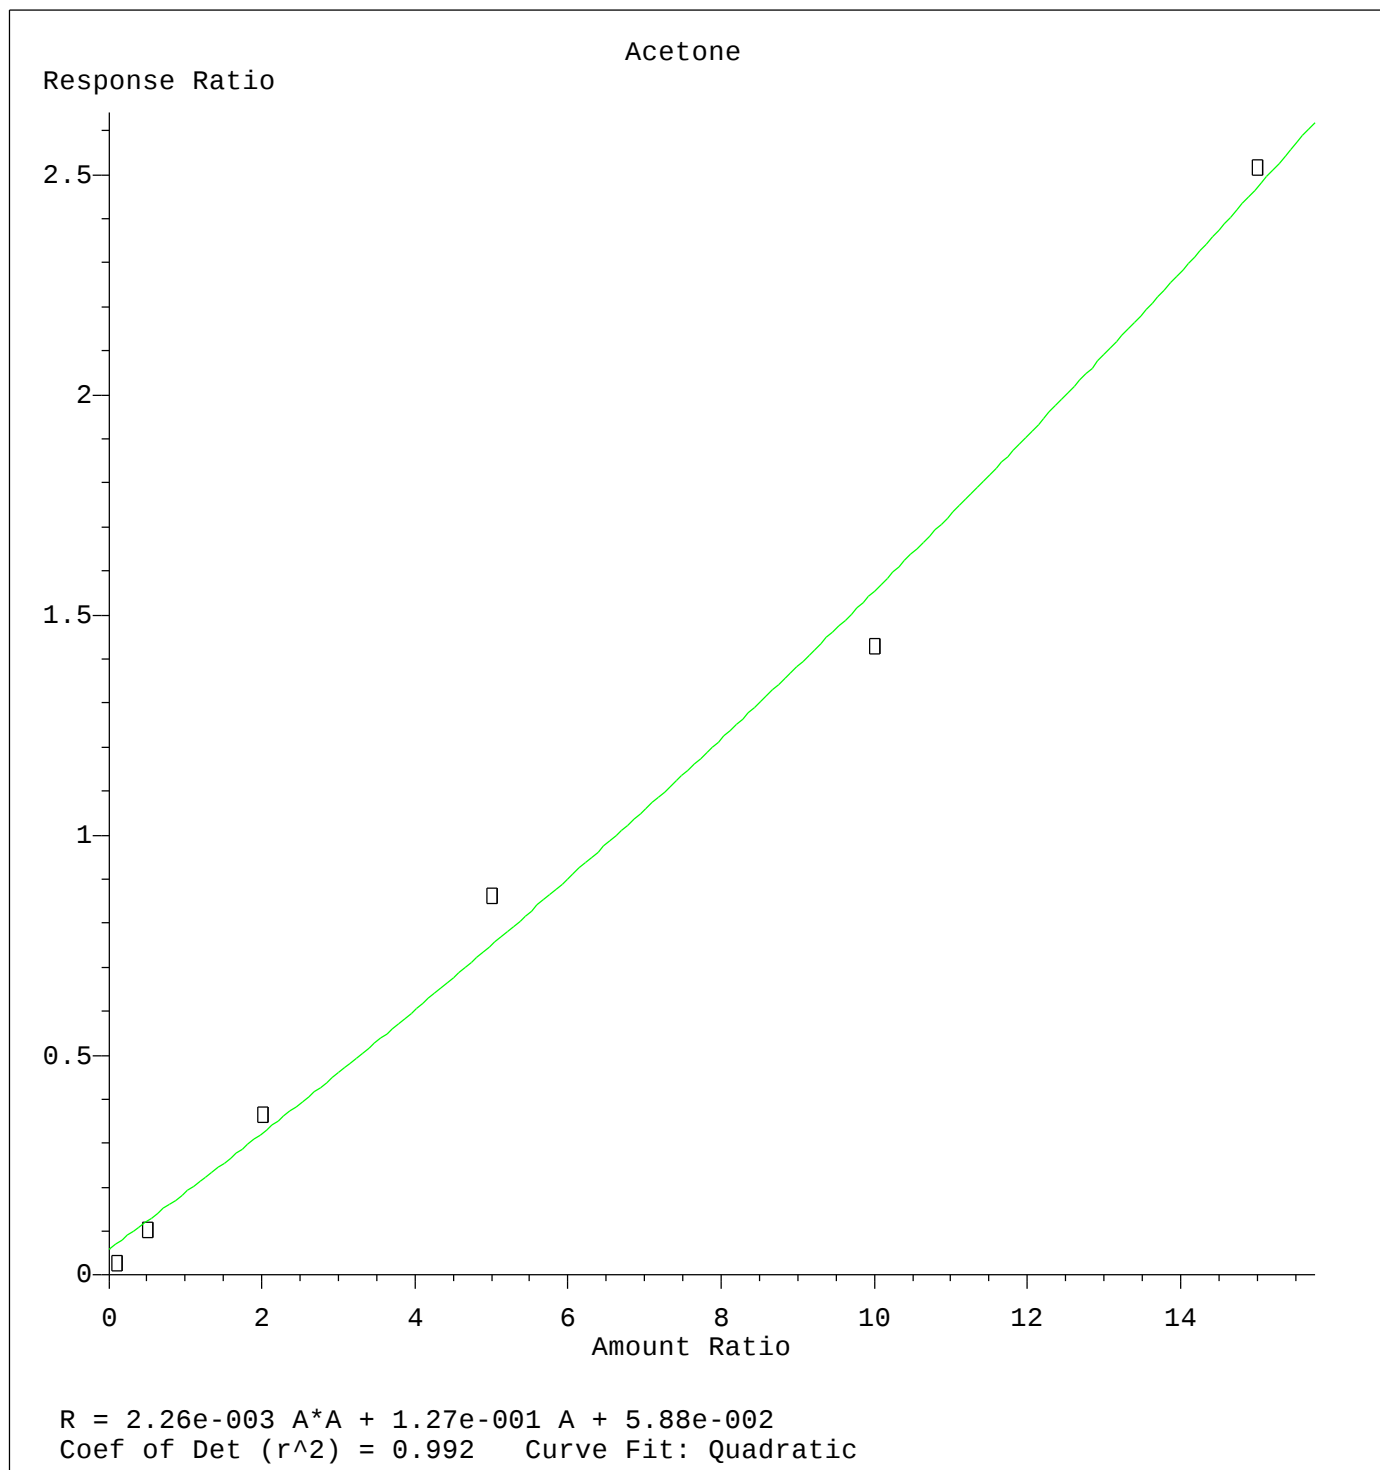

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

Acrolein

Response Ratio

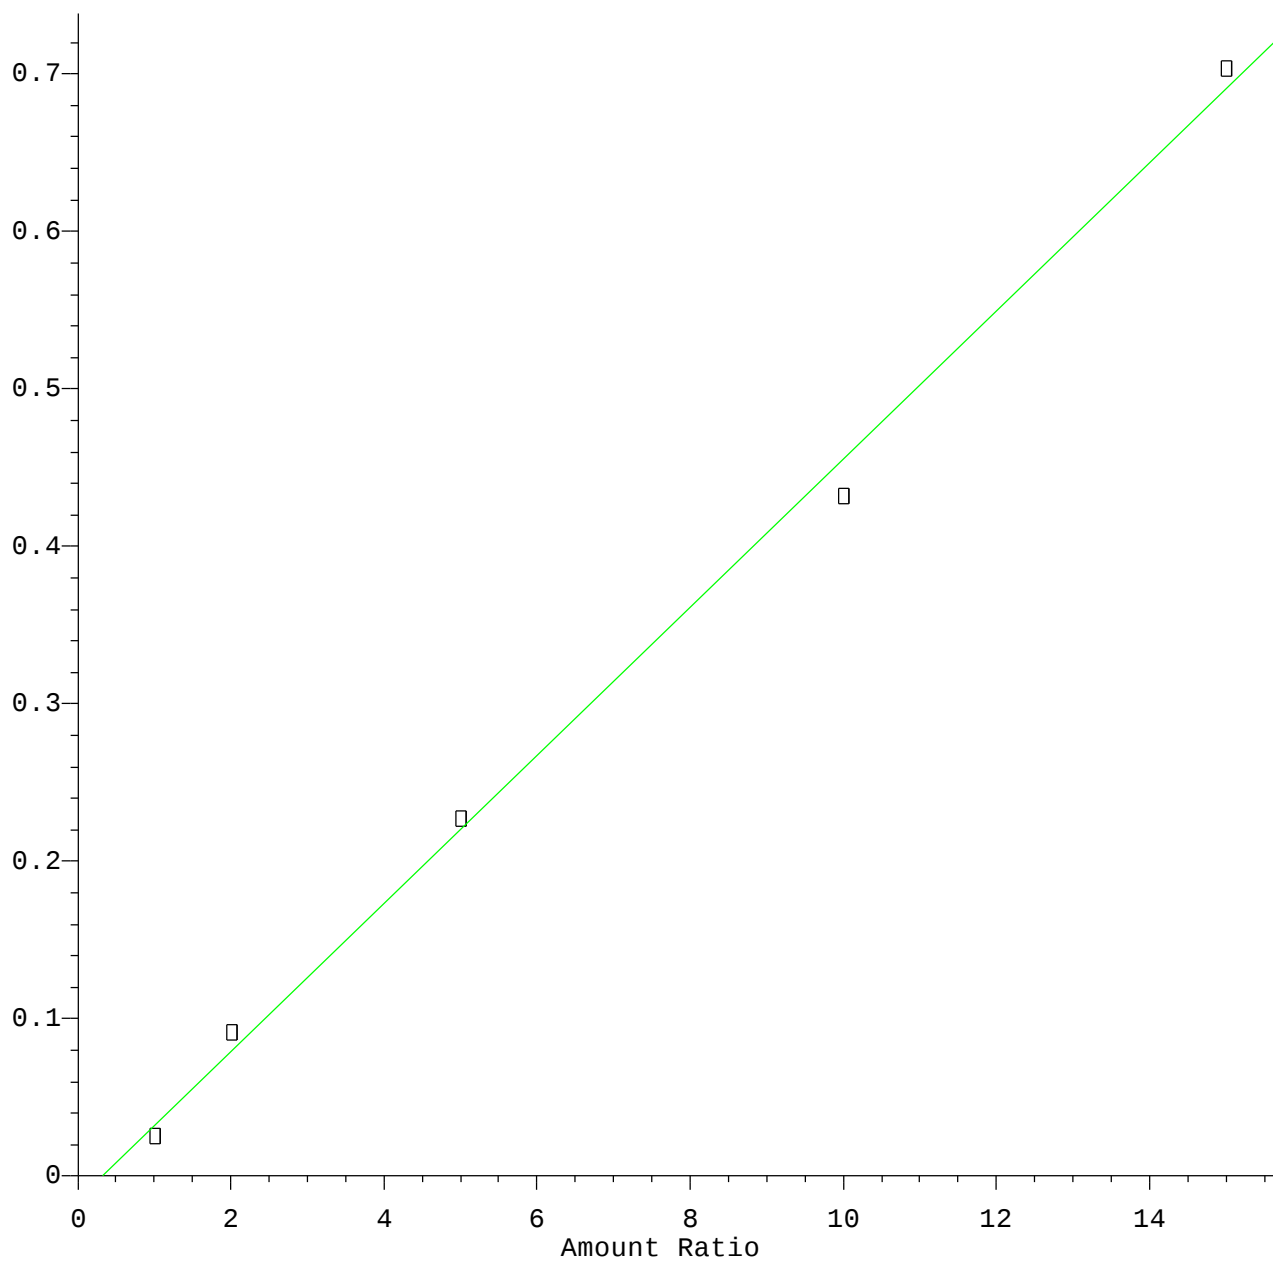


Resp Ratio = $4.70 \times 10^{-2} \times \text{Amt} - 1.48 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

1,1,2-Trichlorotrifluoroethane

Response Ratio

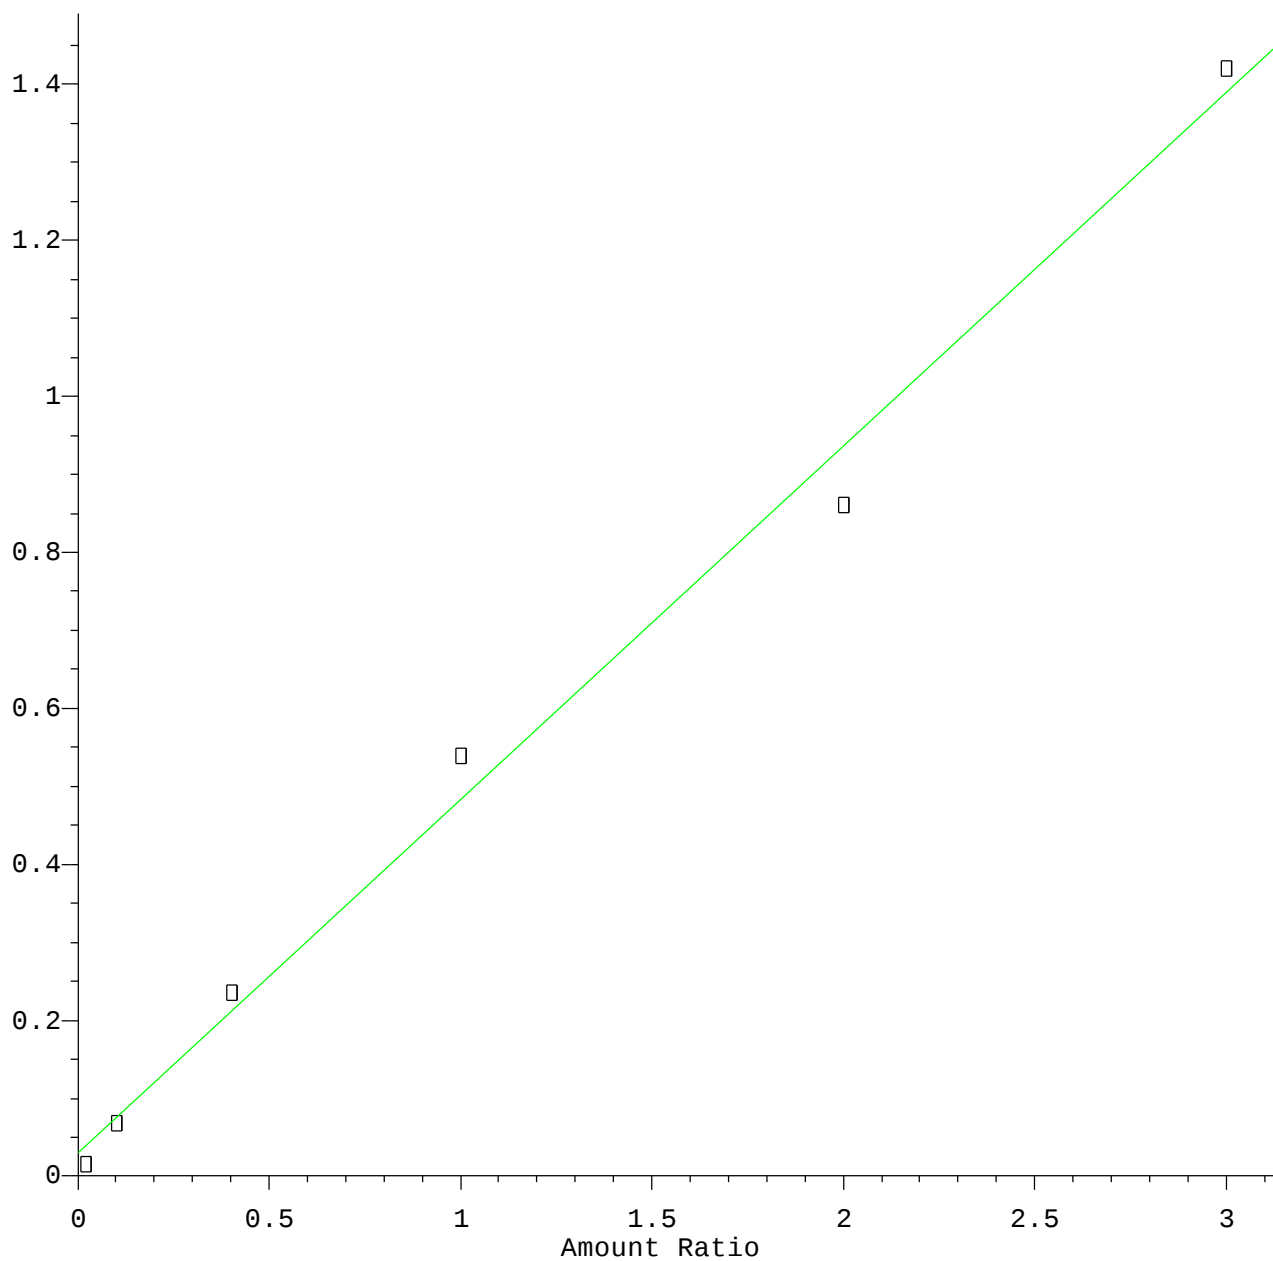


Resp Ratio = $4.53 \times 10^{-1} \times \text{Amt} + 3.01 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

Trichlorofluoromethane

Response Ratio

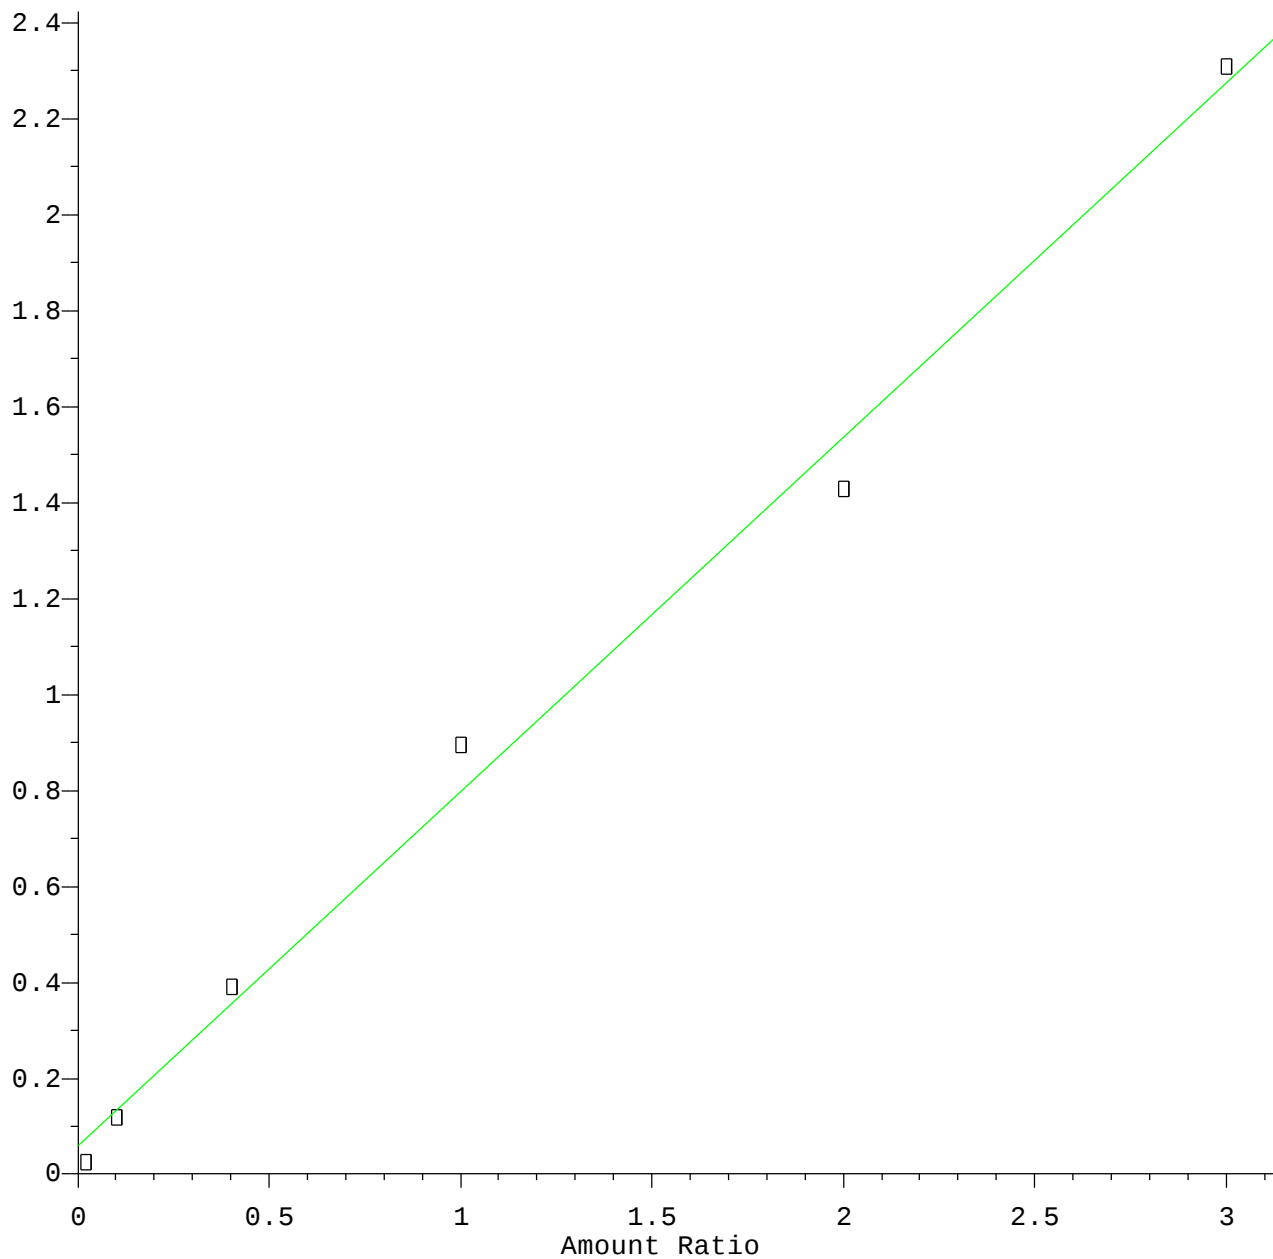


Resp Ratio = $7.38 \times 10^{-1} \times \text{Amt} + 5.78 \times 10^{-2}$
Coef of Det (r^2) = 0.993 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018


Chloroethane

Response Ratio

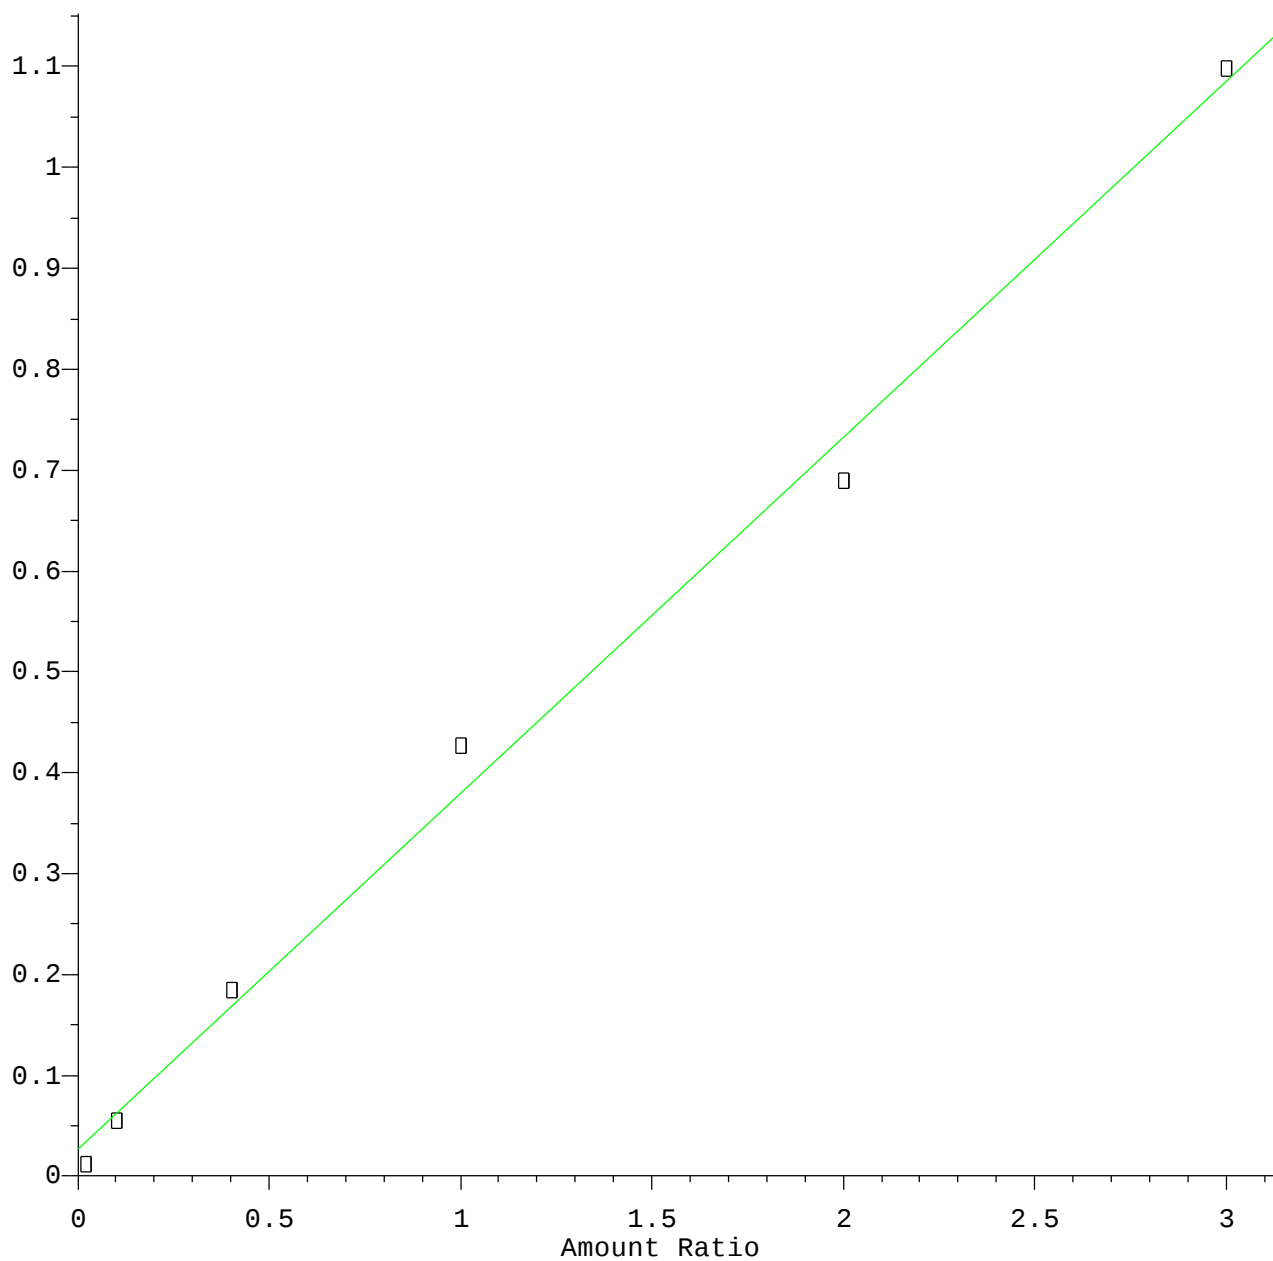


Resp Ratio = $3.53 \times 10^{-1} \times \text{Amt} + 2.70 \times 10^{-2}$
Coef of Det (r^2) = 0.994 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

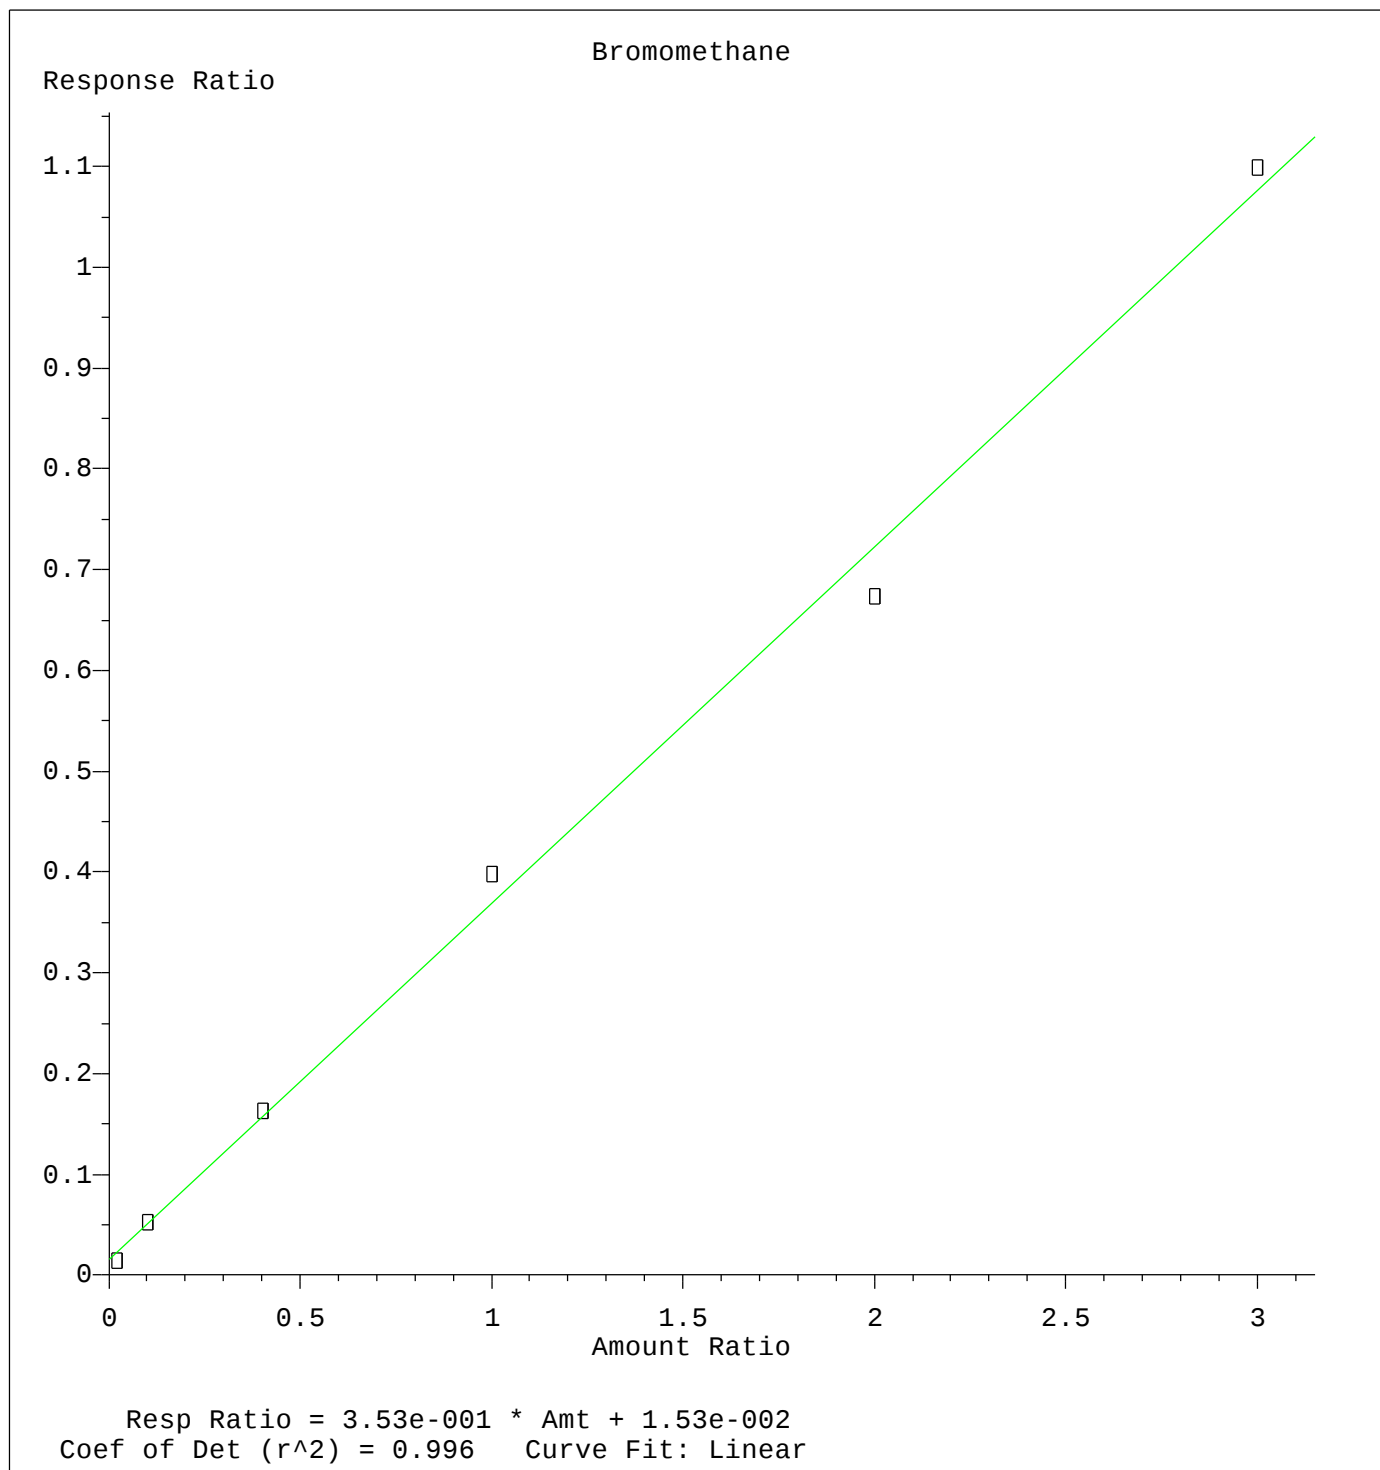

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018

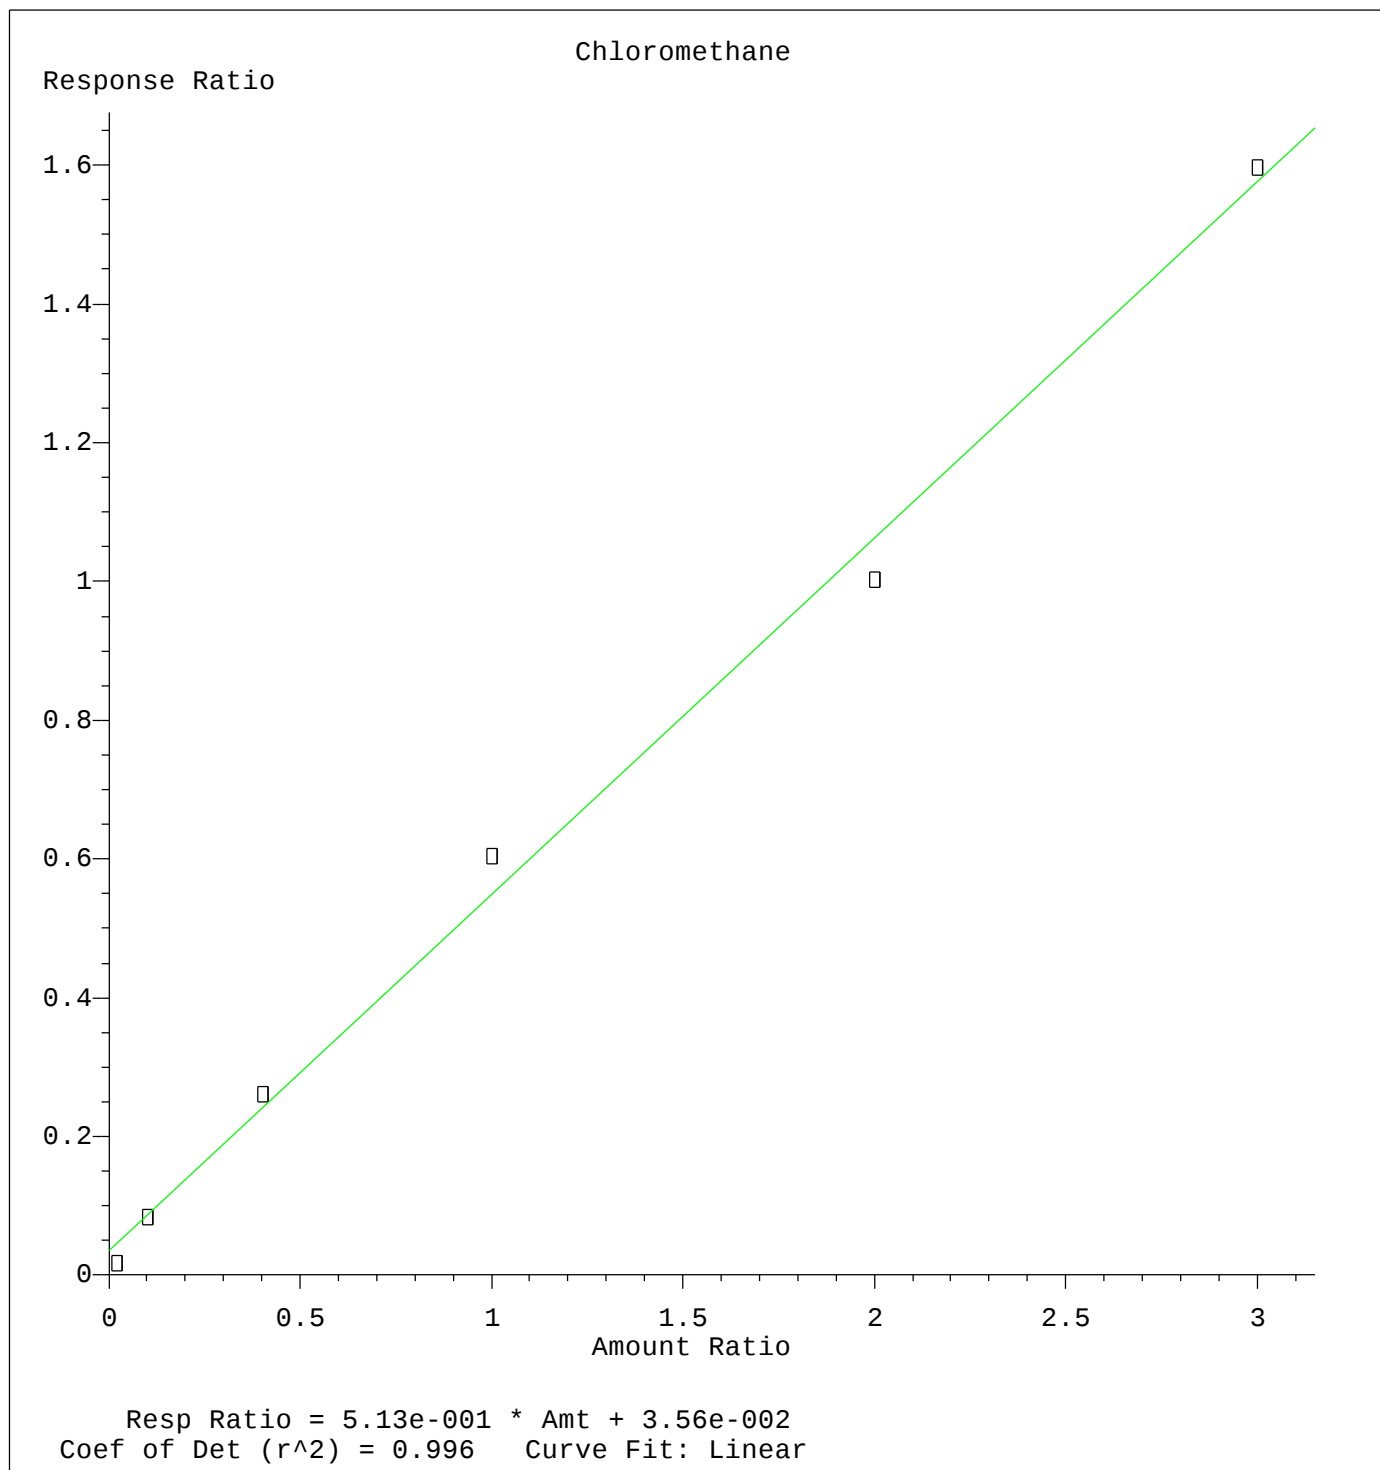

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Calibration Table Last Updated: Wed Jul 18 13:12:02 2018