


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071718\
Data File : VN049837.D
Acq On : 17 Jul 2018 9:55
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071718W.M
Title : SW846 8260
Last Update : Tue Jul 17 13:20:18 2018

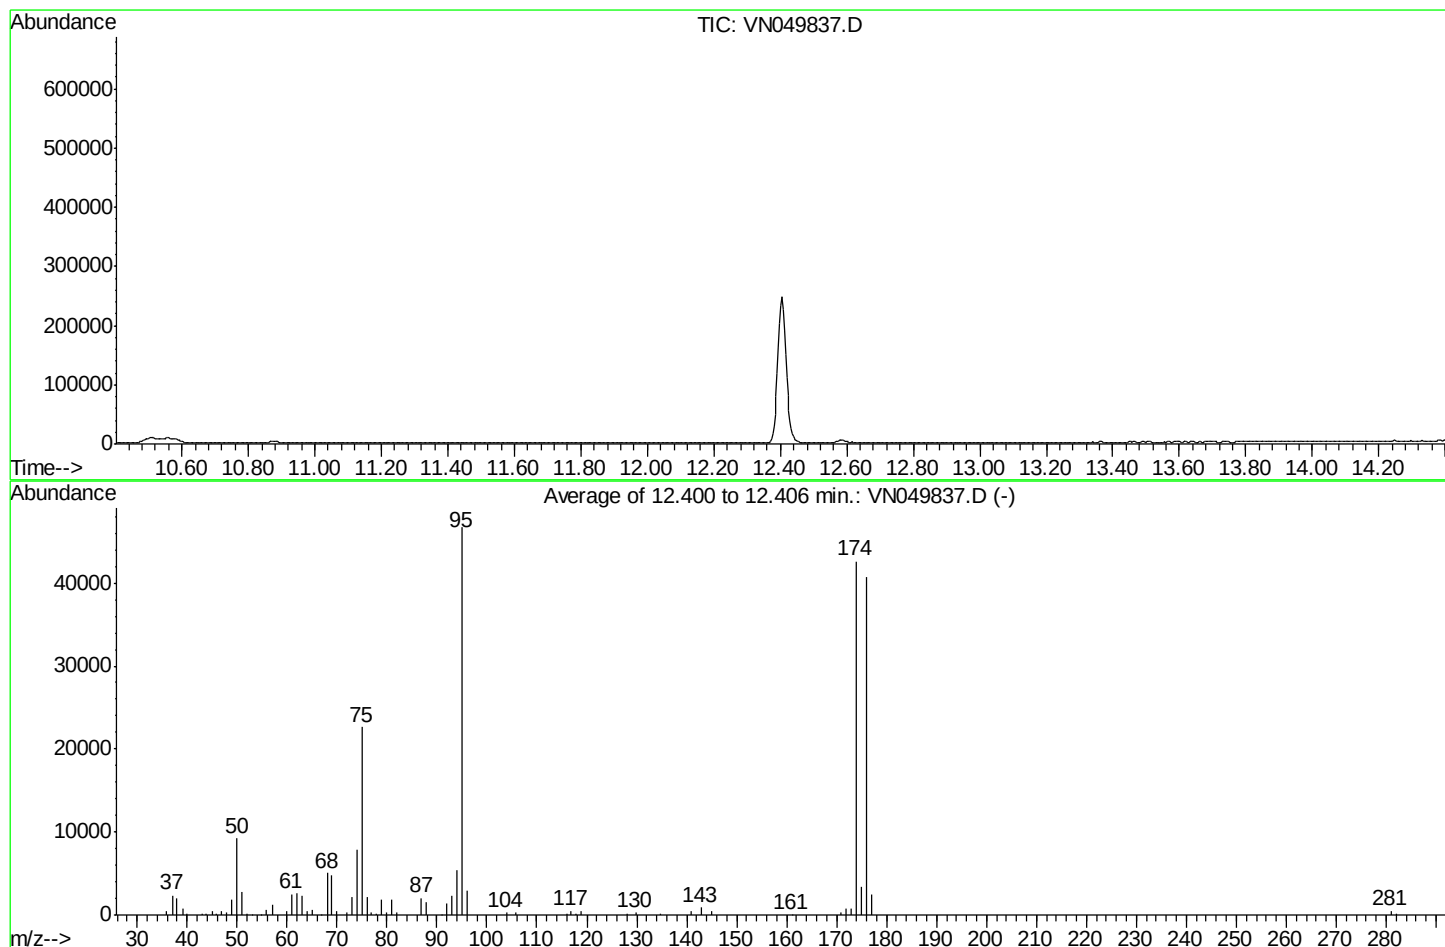

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	9241	PASS
75	95	30	60	48.5	22640	PASS
95	95	100	100	100.0	46712	PASS
96	95	5	9	6.1	2863	PASS
173	174	0.00	2	1.7	739	PASS
174	95	50	100	91.2	42594	PASS
175	174	5	9	7.8	3337	PASS
176	174	95	101	95.8	40797	PASS
177	176	5	9	5.9	2411	PASS