

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071724\
 Data File : VN082954.D
 Acq On : 17 Jul 2024 11:10
 Operator : JC\MD
 Sample : VN0717WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0717WBL01

Quant Time: Jul 18 05:20:32 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 08 13:46:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.230	168	107080	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	211741	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	210883	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	87152	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	85179	56.746	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	113.500%
35) Dibromofluoromethane	8.165	113	70879	52.167	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.340%
50) Toluene-d8	10.571	98	239837	47.793	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	95.580%
62) 4-Bromofluorobenzene	12.853	95	77655	43.079	ug/l	0.00
Spiked Amount	50.000	Range	64 - 133	Recovery	=	86.160%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071724\
Data File : VN082954.D
Acq On : 17 Jul 2024 11:10
Operator : JC\MD
Sample : VN0717WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0717WBL01


Quant Time: Jul 18 05:20:32 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 08 13:46:04 2024
Response via : Initial Calibration

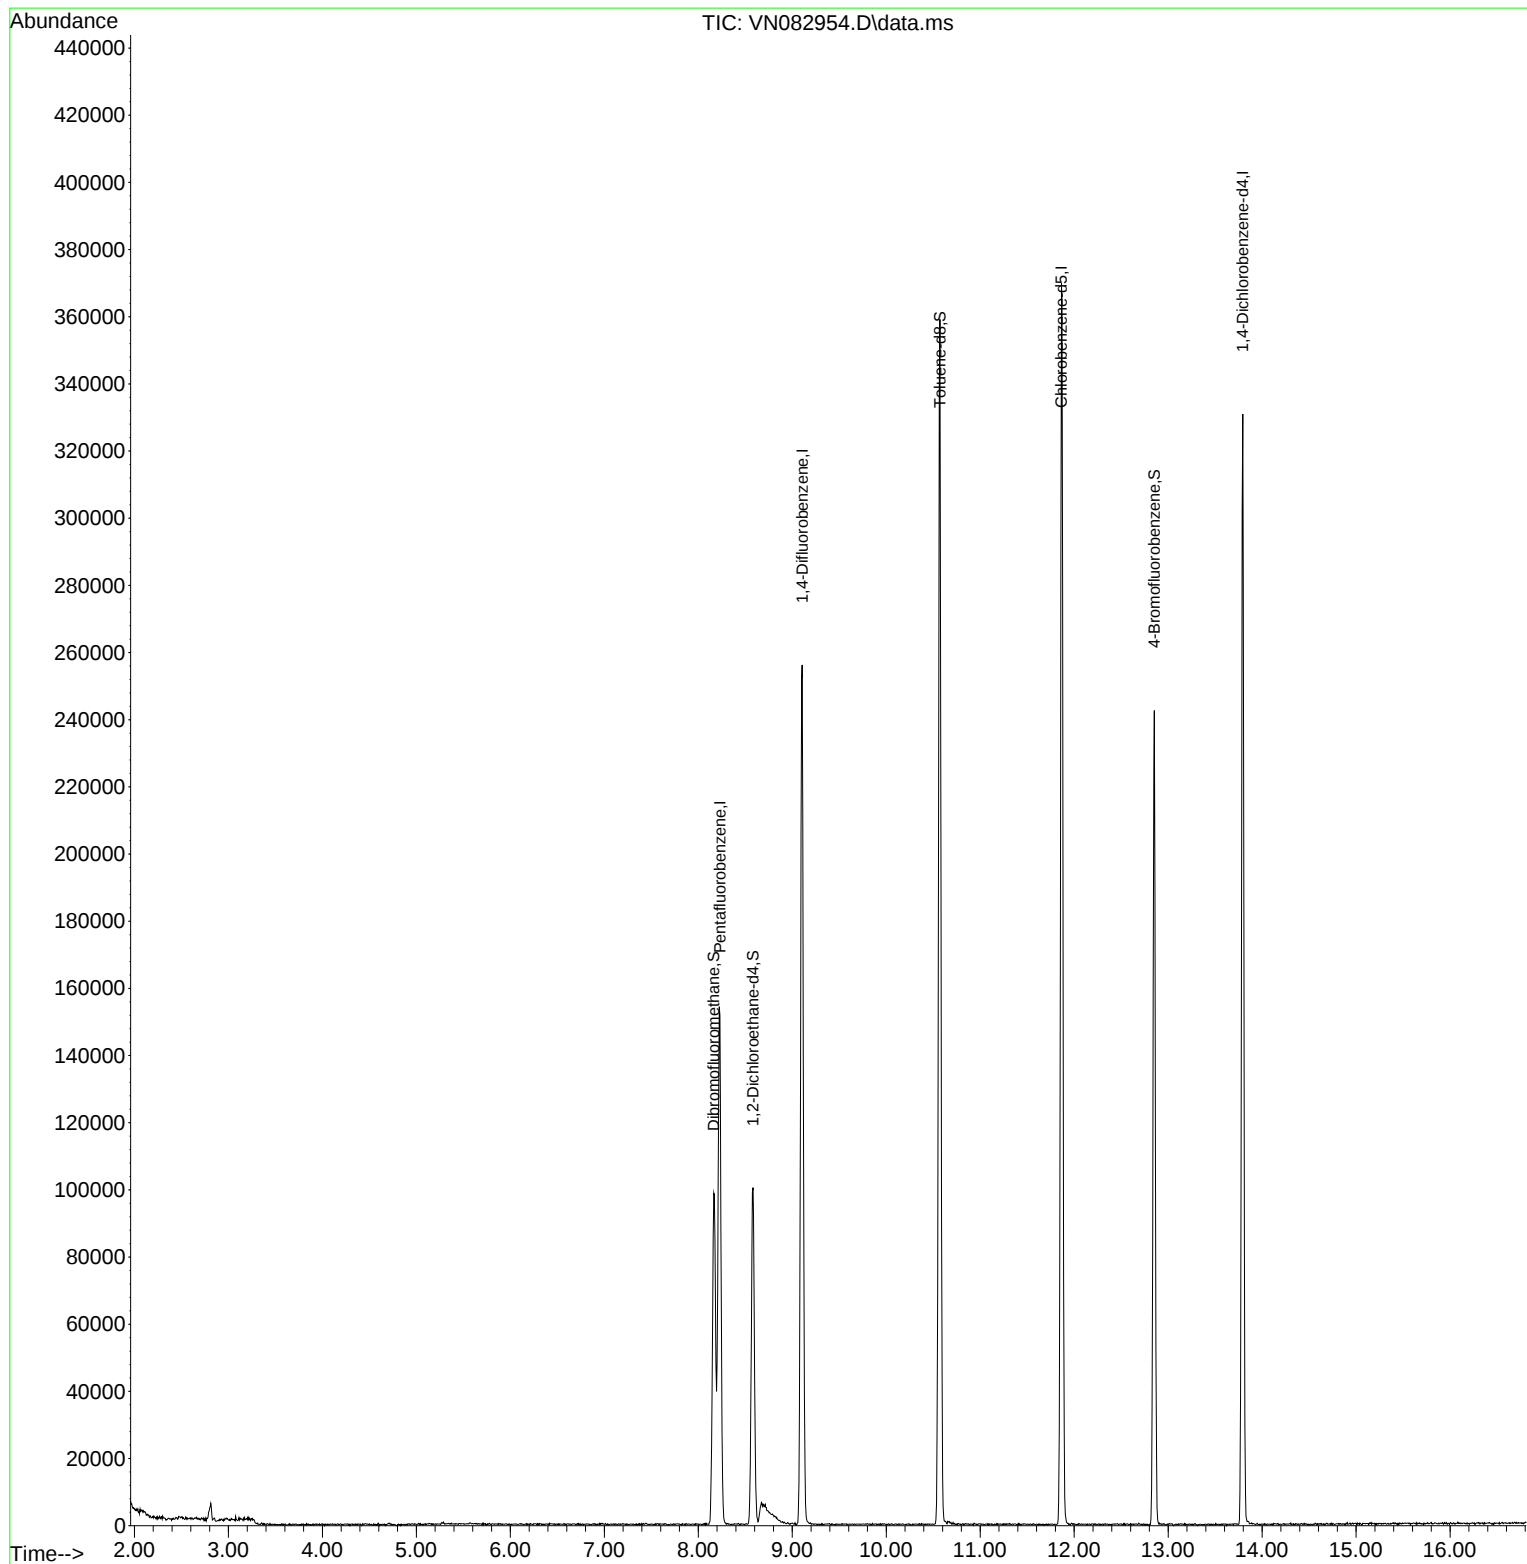



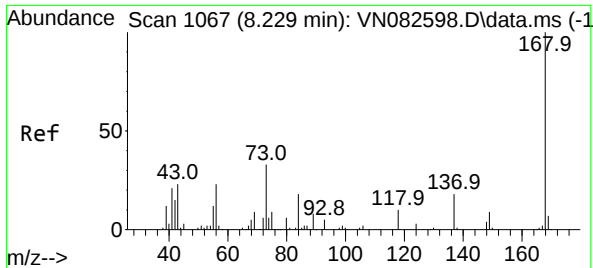


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. 0.001 min
Lab File: VN082954.D
Acq: 17 Jul 2024 11:10

Instrument :
MSVOA_N
ClientSampleId :
VN0717WBL01



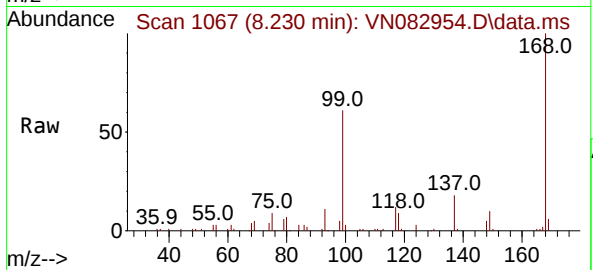



Tgt Ion:168 Resp: 107080
Ion Ratio Lower Upper
168 100
99 61.2 48.2 72.4

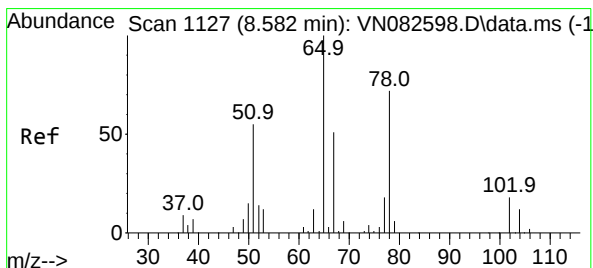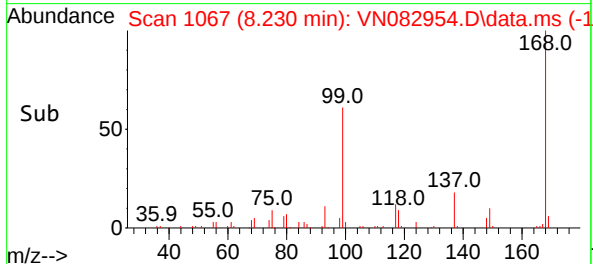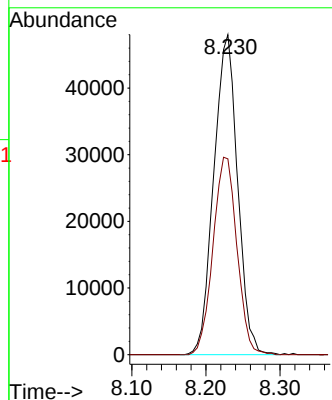

#33
1,2-Dichloroethane-d4
Concen: 56.746 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. 0.000 min
Lab File: VN082954.D
Acq: 17 Jul 2024 11:10

Tgt Ion: 65 Resp: 85179
Ion Ratio Lower Upper
65 100
67 50.2 0.0 104.4

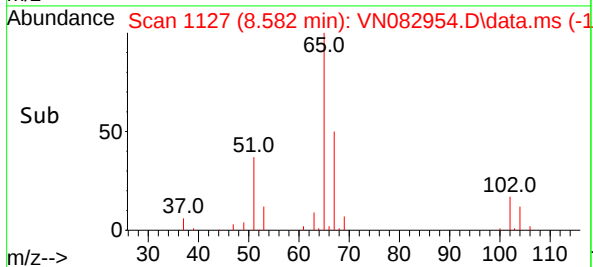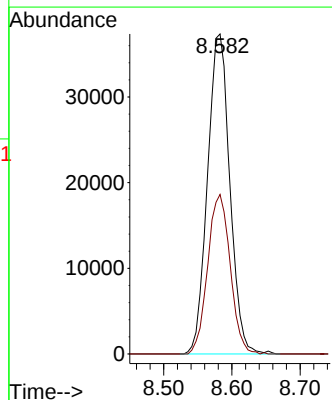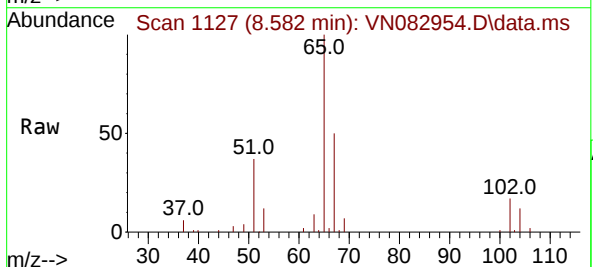

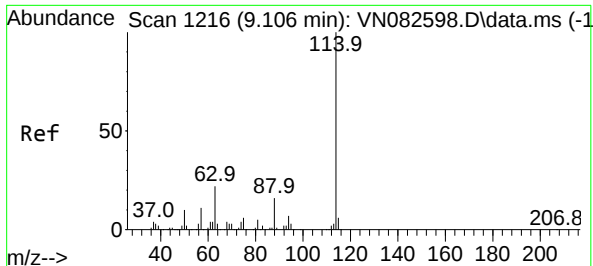

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN082954.D

Acq: 17 Jul 2024 11:10

Instrument :

MSVOA_N

ClientSampleId :

VN0717WBL01





Tgt Ion:114 Resp: 211741

Ion Ratio Lower Upper

114 100

63 20.8 0.0 44.6

88 15.8 0.0 31.4

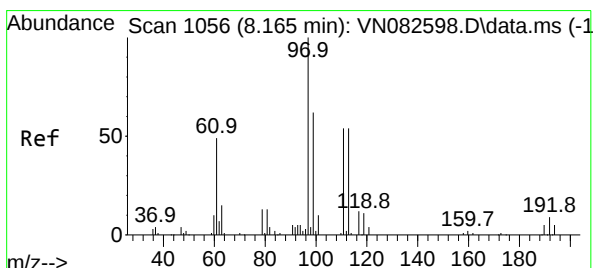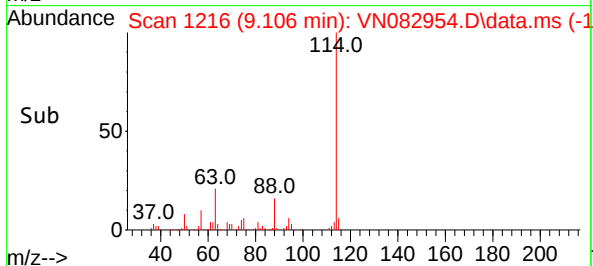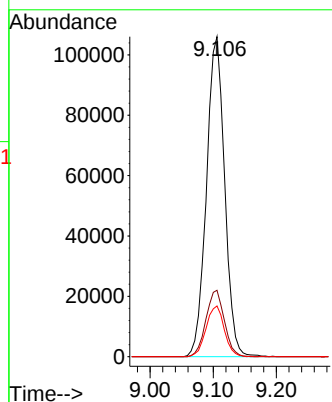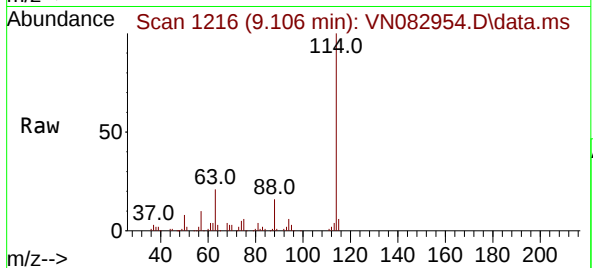

#35

Dibromofluoromethane

Concen: 52.167 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. -0.000 min

Lab File: VN082954.D

Acq: 17 Jul 2024 11:10




Tgt Ion:113 Resp: 70879


Ion Ratio Lower Upper

113 100

111 104.5 82.4 123.6

192 17.8 14.9 22.3


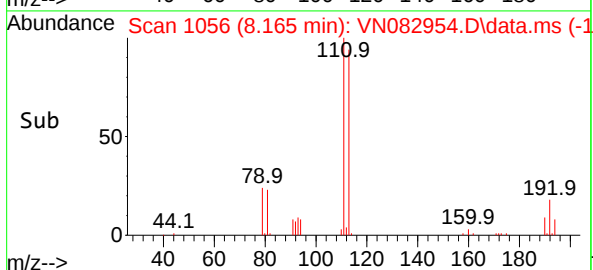
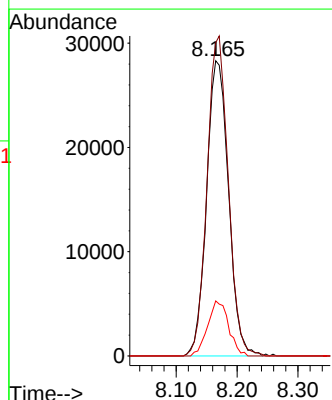
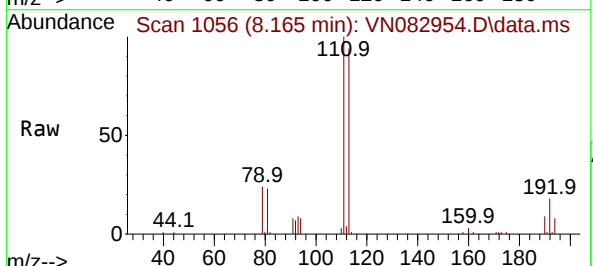


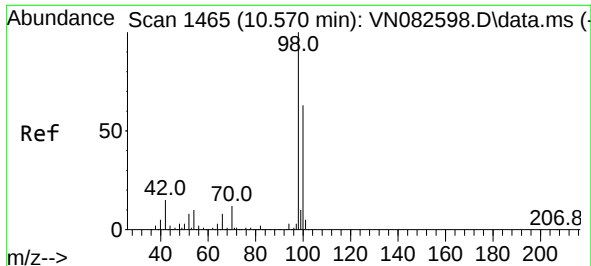

#50
Toluene-d8
Concen: 47.793 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.001 min
Lab File: VN082954.D
Acq: 17 Jul 2024 11:10




Instrument :
MSVOA_N
ClientSampleId :
VN0717WBL01


Tgt Ion: 98 Resp: 239837
Ion Ratio Lower Upper
98 100
100 63.6 51.5 77.3

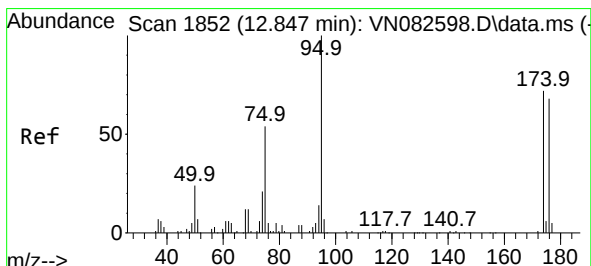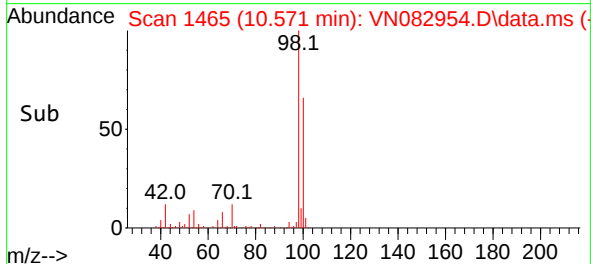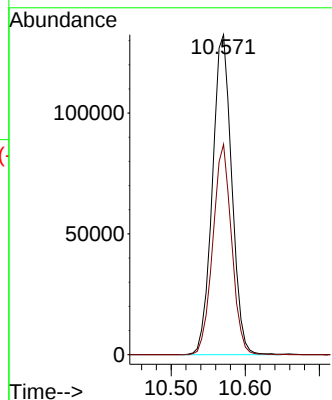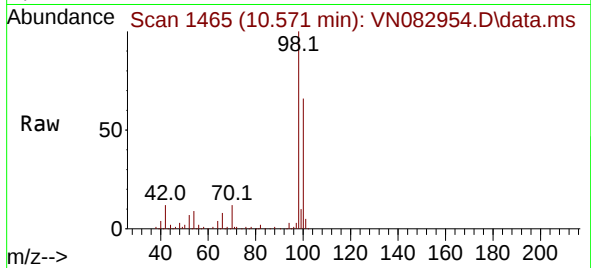

#62
4-Bromofluorobenzene
Concen: 43.079 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN082954.D
Acq: 17 Jul 2024 11:10

Tgt Ion: 95 Resp: 77655
Ion Ratio Lower Upper
95 100
174 78.4 0.0 159.2
176 75.7 0.0 147.6


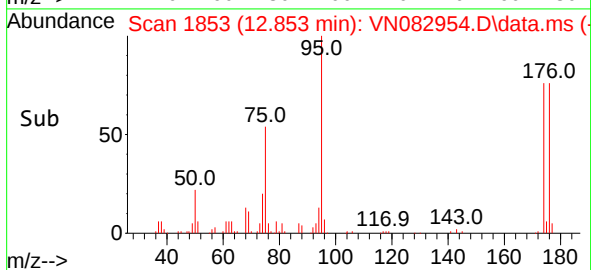
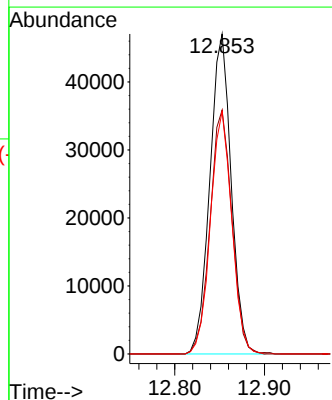
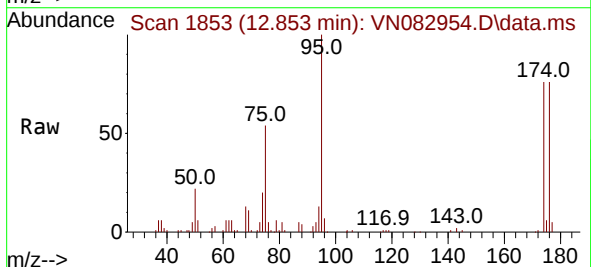


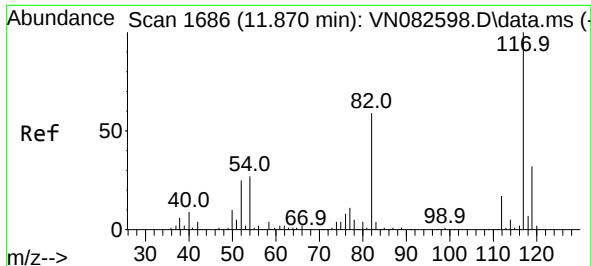

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1170
Delta R.T. -0.005 min
Lab File: VN082954.D
Acq: 17 Jul 2024 11:10

Instrument :
MSVOA_N
ClientSampleId :
VN0717WBL01

Tgt Ion:117 Resp: 210883
Ion Ratio Lower Upper
117 100
82 56.4 47.5 71.3
119 31.1 25.6 38.4

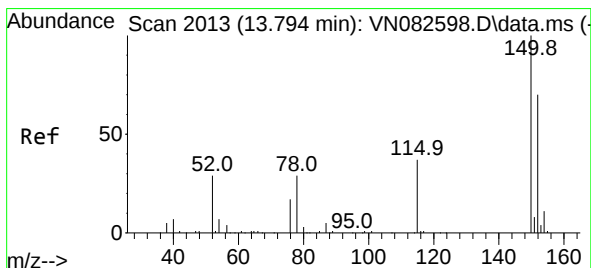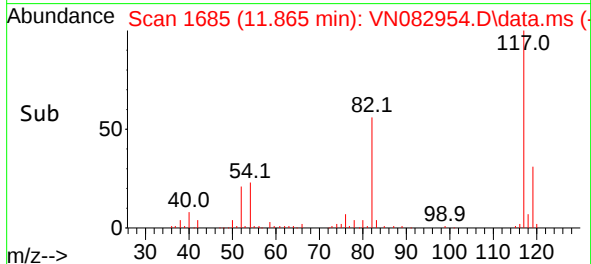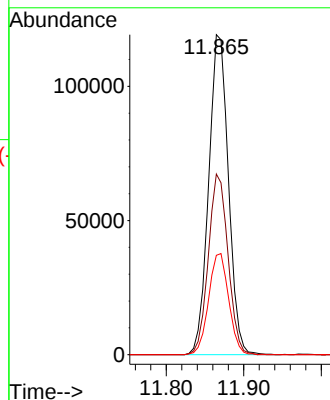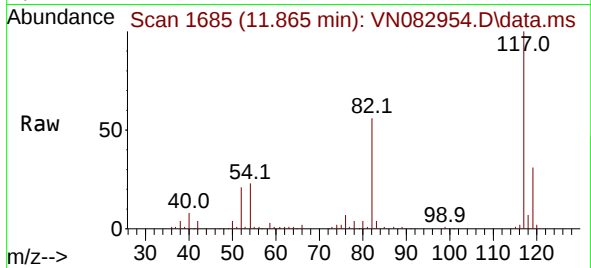

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.000 min
Lab File: VN082954.D
Acq: 17 Jul 2024 11:10

Tgt Ion:152 Resp: 87152
Ion Ratio Lower Upper
152 100
115 60.5 30.6 91.6
150 157.3 0.0 348.6

