
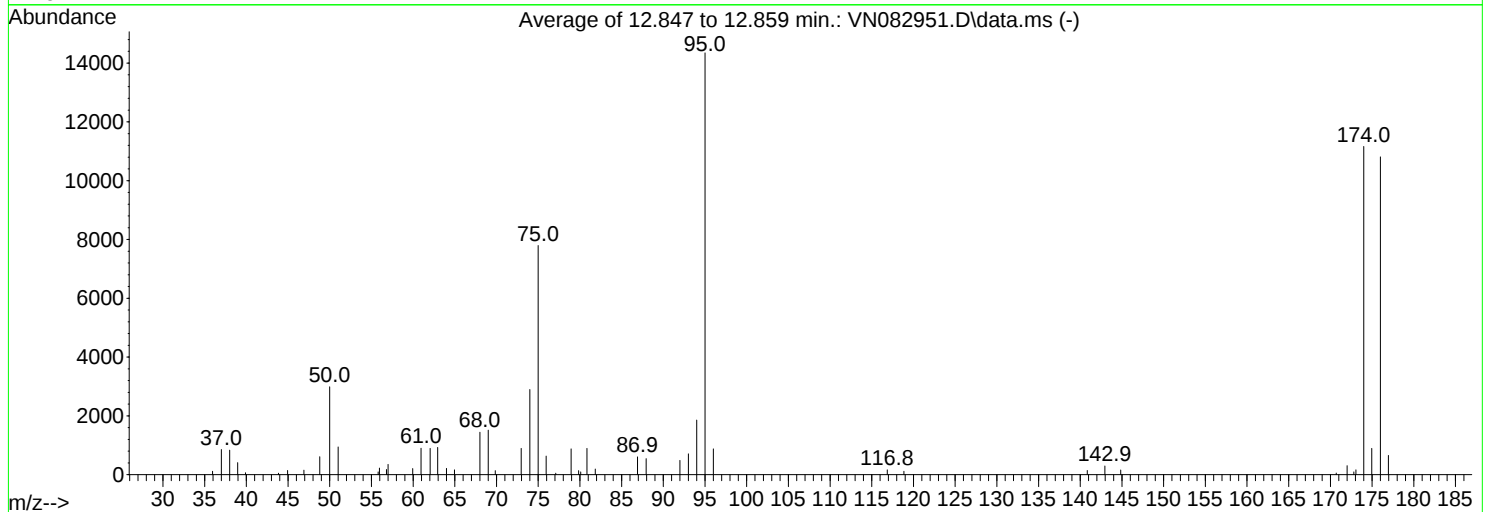


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071724\
Data File : VN082951.D
Acq On : 17 Jul 2024 09:39
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

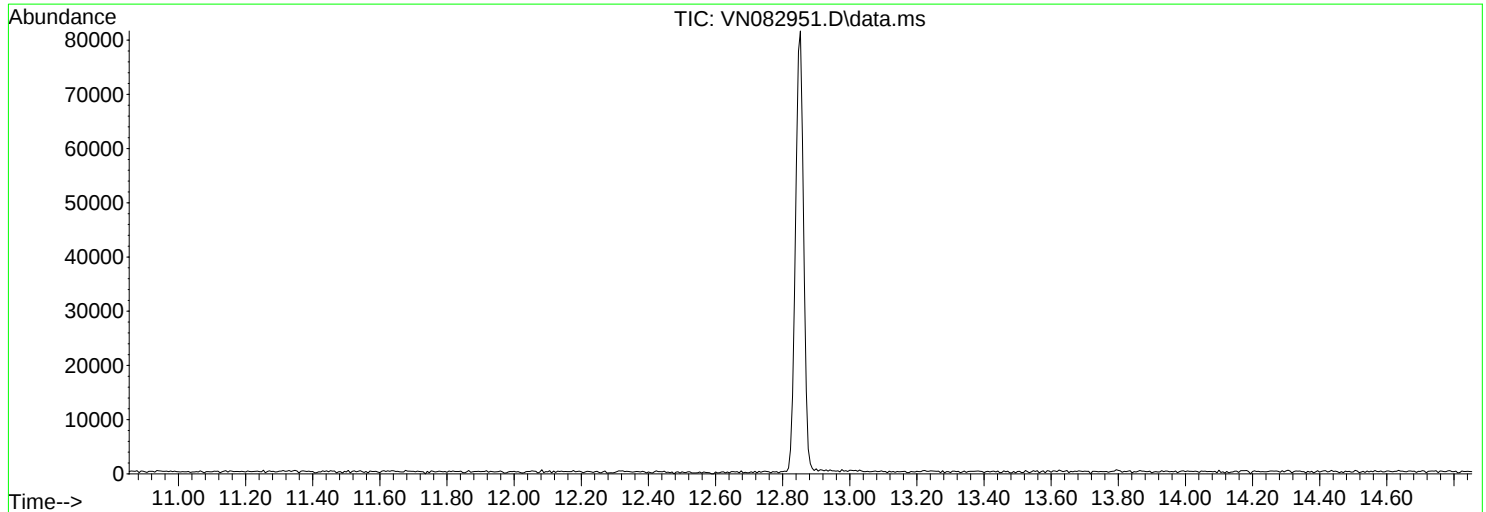

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	2989	PASS
75	95	30	60	54.3	7794	PASS
95	95	100	100	100.0	14347	PASS
96	95	5	9	6.1	877	PASS
173	174	0.00	2	1.5	164	PASS
174	95	50	100	77.8	11160	PASS
175	174	5	9	8.0	891	PASS
176	174	95	101	96.8	10807	PASS
177	176	5	9	6.0	653	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	113	55.80	94	69.00	1511	81.85	1854
37.00	857	55.95	224	69.85	138	86.90	607
38.00	832	56.80	172	72.95	895	87.95	541
38.95	411	57.00	346	74.00	2895	92.00	481
39.90	65	59.95	209	75.00	7794	93.00	708
43.85	51	60.95	896	75.95	632	94.00	1854
44.95	139	62.05	893	77.10	51	95.00	14347
46.90	152	62.95	927	78.95	878	96.00	877
48.80	611	64.00	212	79.85	135	116.85	163
50.00	2989	64.95	163	80.10	95	118.85	116
51.00	942	68.00	1444	80.85	895	140.85	143

Average of 12.847 to 12.859 min.: VN082951.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
142.95	296						
144.85	160						
170.70	57						
172.00	307						
172.80	94						
173.05	164						
174.00	11160						
174.95	891						
176.00	10807						
176.95	653						

Instrument :
MSVOA_N
ClientSampleId :
BFB