

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071725\
 Data File : VN087346.D
 Acq On : 17 Jul 2025 15:47
 Operator : JC\MD
 Sample : Q2633-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 FIBER-GLASS-TANK

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M

Title : SW846 8260

Signal : TIC: VN087346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	8.153	1044	1054	1058	rBV	214043	491298	32.44%	5.714%
2	8.212	1058	1064	1074	rVB	311610	726550	47.97%	8.451%
3	8.565	1114	1124	1137	rBV	241366	547359	36.14%	6.366%
4	9.082	1204	1212	1226	rVB	534000	1093685	72.21%	12.721%
5	10.547	1453	1461	1470	rBV	820493	1514575	100.00%	17.616%
6	11.847	1674	1682	1691	rBV	722666	1299976	85.83%	15.120%
7	12.676	1821	1823	1830	rVB4	11363	16177	1.07%	0.188%
8	12.829	1841	1849	1864	rBV	562043	1009826	66.67%	11.745%
9	13.770	2001	2009	2024	rVB	749428	1298810	85.75%	15.107%
10	13.941	2035	2038	2046	rVB9	8995	22659	1.50%	0.264%
11	15.017	2213	2221	2222	rBV6	15221	25151	1.66%	0.293%
12	15.617	2315	2323	2334	rVB	118391	274442	18.12%	3.192%
13	16.211	2412	2424	2435	rVB3	48097	202076	13.34%	2.350%
14	16.753	2508	2516	2522	rBV3	31179	75073	4.96%	0.873%




Sum of corrected areas: 8597657

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071725\
Data File : VN087346.D
Acq On : 17 Jul 2025 15:47
Operator : JC\MD
Sample : Q2633-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FIBER-GLASS-TANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

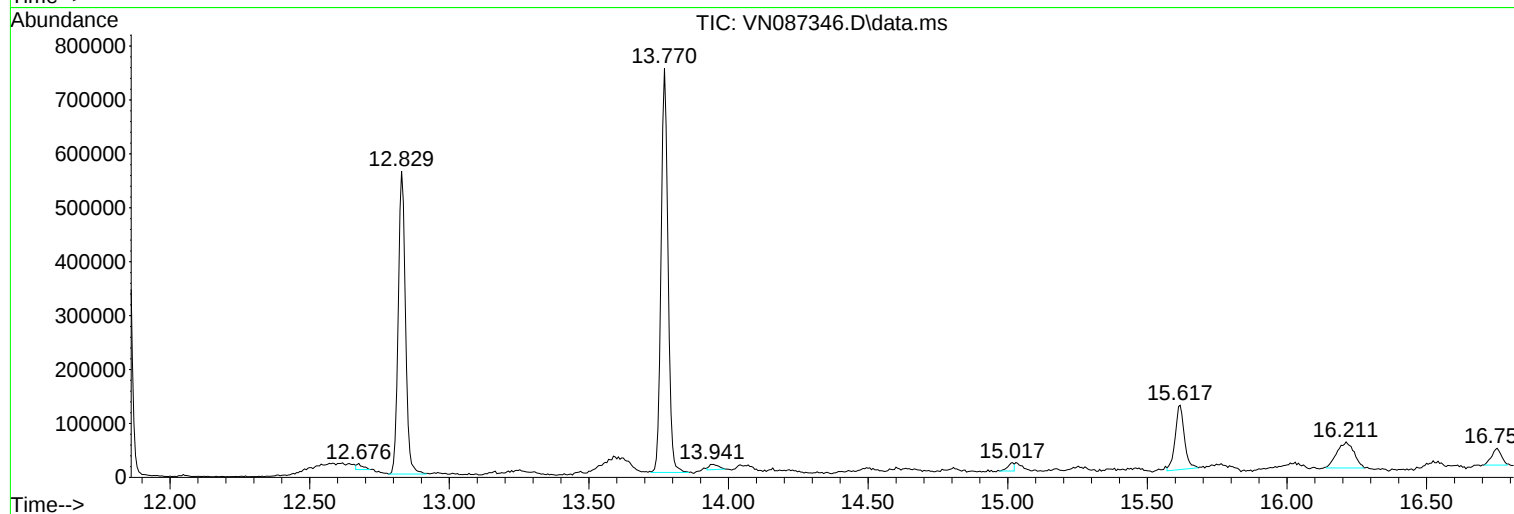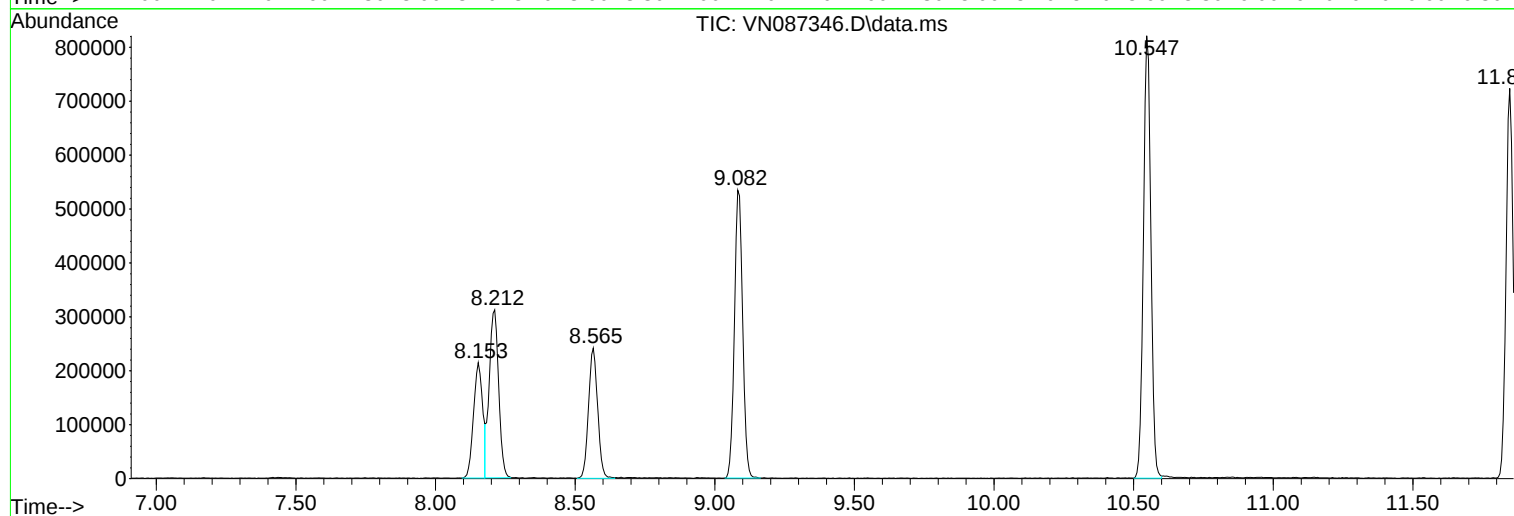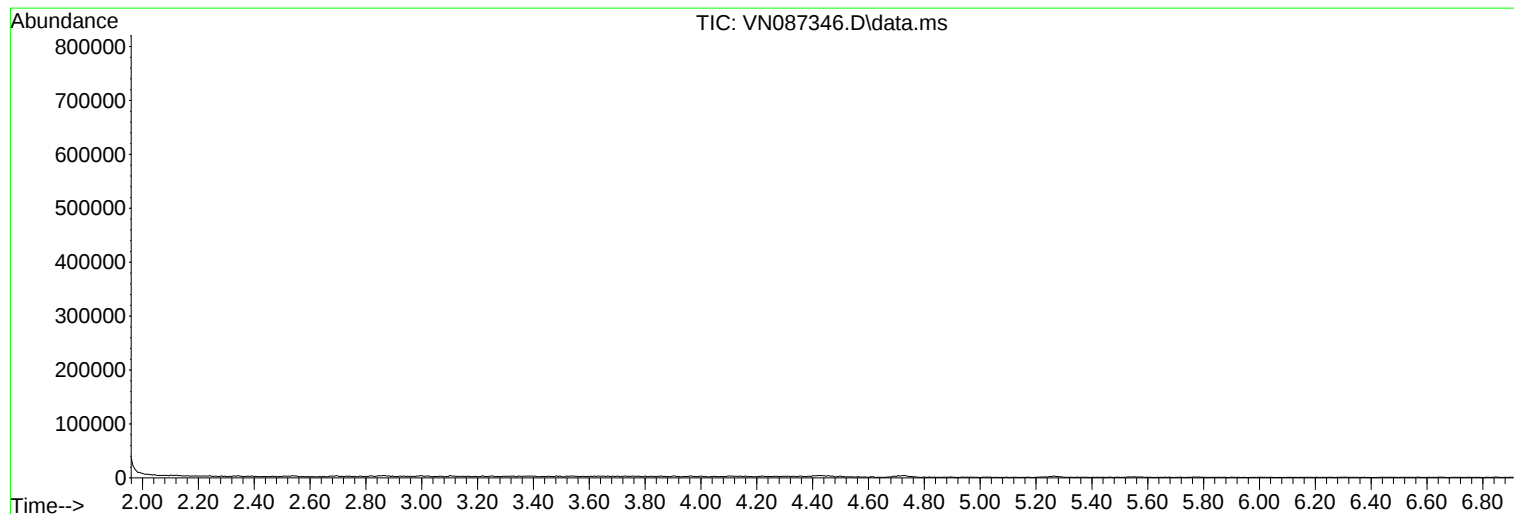

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071725\
Data File : VN087346.D
Acq On : 17 Jul 2025 15:47
Operator : JC\MD
Sample : Q2633-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FIBER-GLASS-TANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071725\
Data File : VN087346.D
Acq On : 17 Jul 2025 15:47
Operator : JC\MD
Sample : Q2633-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
FIBER-GLASS-TANK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------