
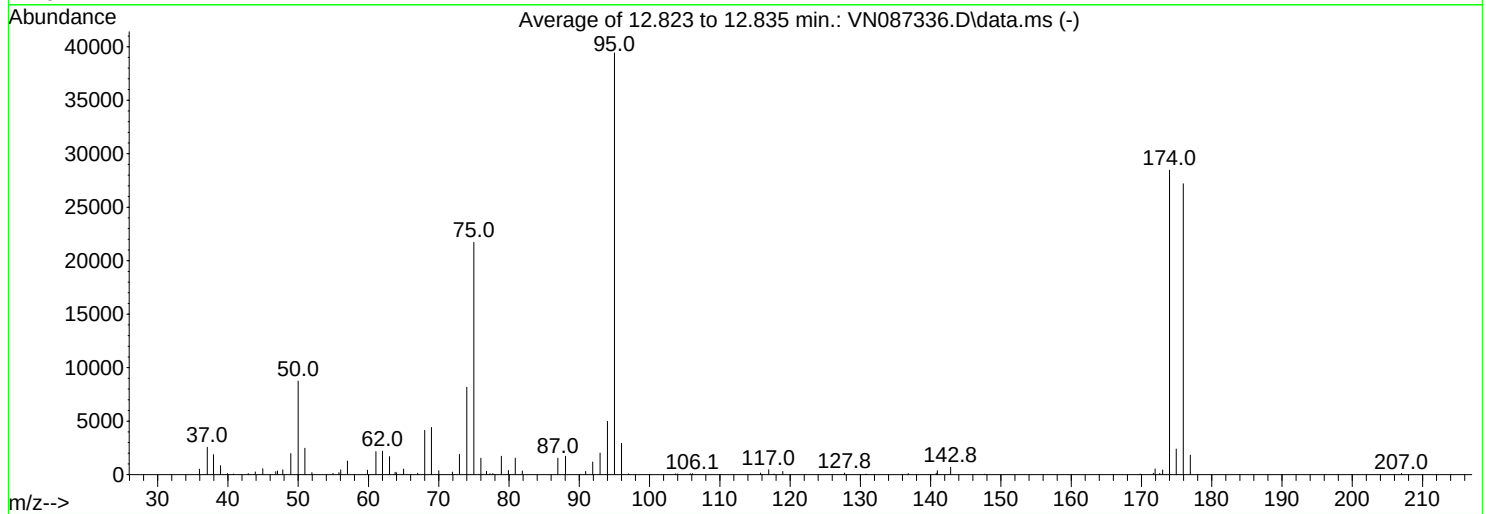


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071725\
Data File : VN087336.D
Acq On : 17 Jul 2025 09:19
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

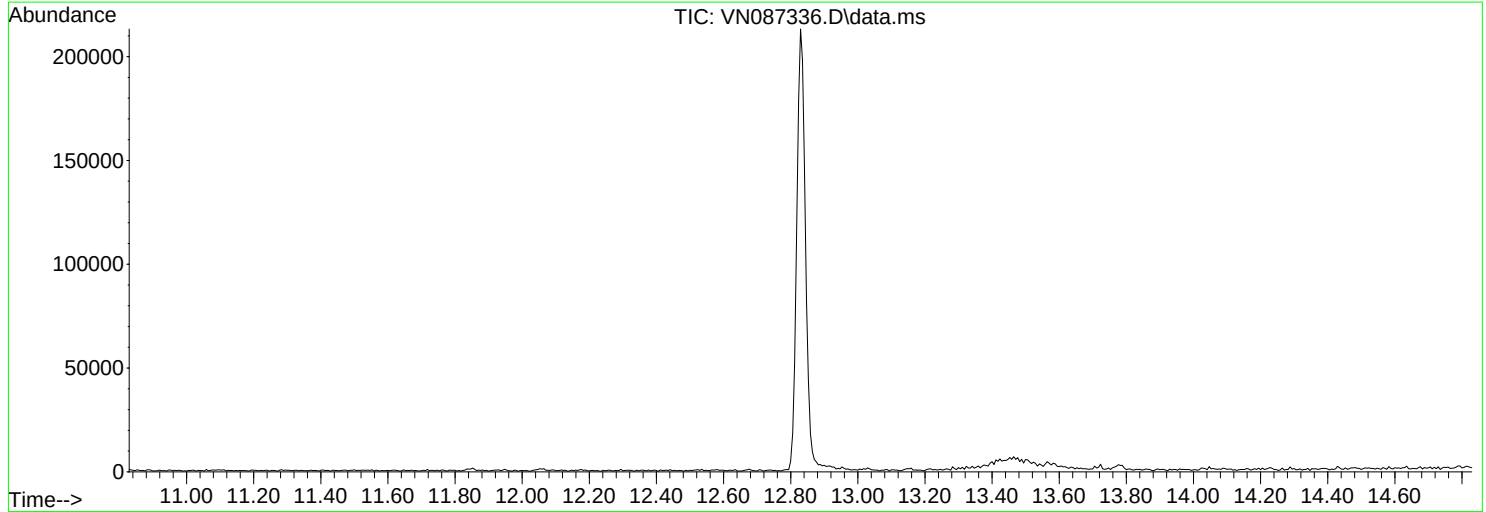

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.2	8748	PASS
75	95	30	60	55.1	21720	PASS
95	95	100	100	100.0	39429	PASS
96	95	5	9	7.4	2926	PASS
173	174	0.00	2	1.5	429	PASS
174	95	50	100	72.2	28461	PASS
175	174	5	9	8.4	2395	PASS
176	174	95	101	95.5	27192	PASS
177	176	5	9	6.7	1832	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	510	47.80	455	62.00	2204	74.00	816
37.05	2565	48.95	1968	63.00	1692	75.00	2172
37.95	1868	50.00	8748	63.80	231	76.00	154
38.95	832	50.95	2469	64.00	180	76.80	31
39.95	98	51.95	189	65.00	529	77.30	88
40.80	63	54.95	121	67.00	140	77.70	100
42.90	108	55.80	199	68.00	4137	78.90	1724
43.90	253	56.05	451	68.95	4417	79.90	397
44.95	554	57.00	1277	70.00	379	80.90	1537
46.80	280	59.85	424	71.95	238	81.90	348
47.05	347	61.05	2150	72.95	1897	86.95	1534

Average of 12.823 to 12.835 min.: VN087336.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
88.05	1714	106.10	104	147.70	52		
90.90	295	115.80	153	169.80	60		
91.90	1180	116.95	465	171.70	143		
92.95	2019	117.70	55	171.95	546		
94.00	4983	118.95	300	172.60	119		
95.00	39429	127.75	146	173.00	429		
96.00	2926	130.80	62	174.00	28461		
97.00	74	136.80	116	174.95	2395		
103.70	73	140.80	129	175.95	27192		
104.00	68	140.95	376	176.95	1832		
105.80	89	142.85	688	207.00	104		

Instrument :

MSVOA_N

ClientSampleId :

BFB