


Dichlorodifluoromethane

Response Ratio

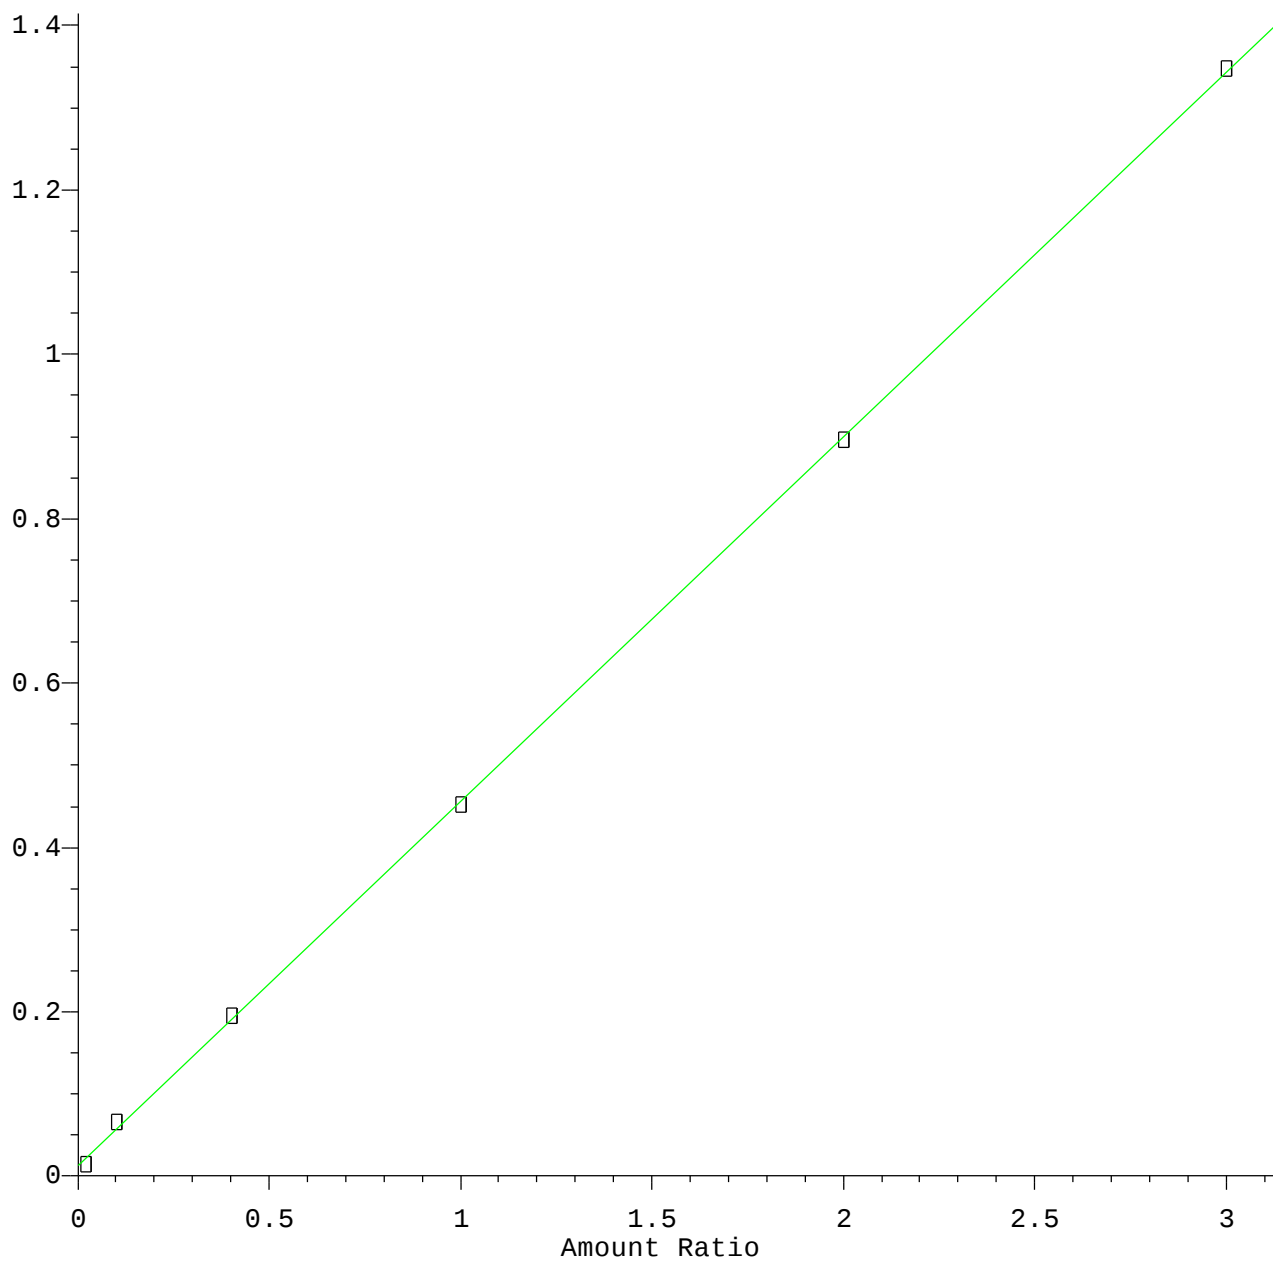


Resp Ratio = $4.43 \times 10^{-1} \times \text{Amt} + 1.29 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018

Naphthalene

Response Ratio

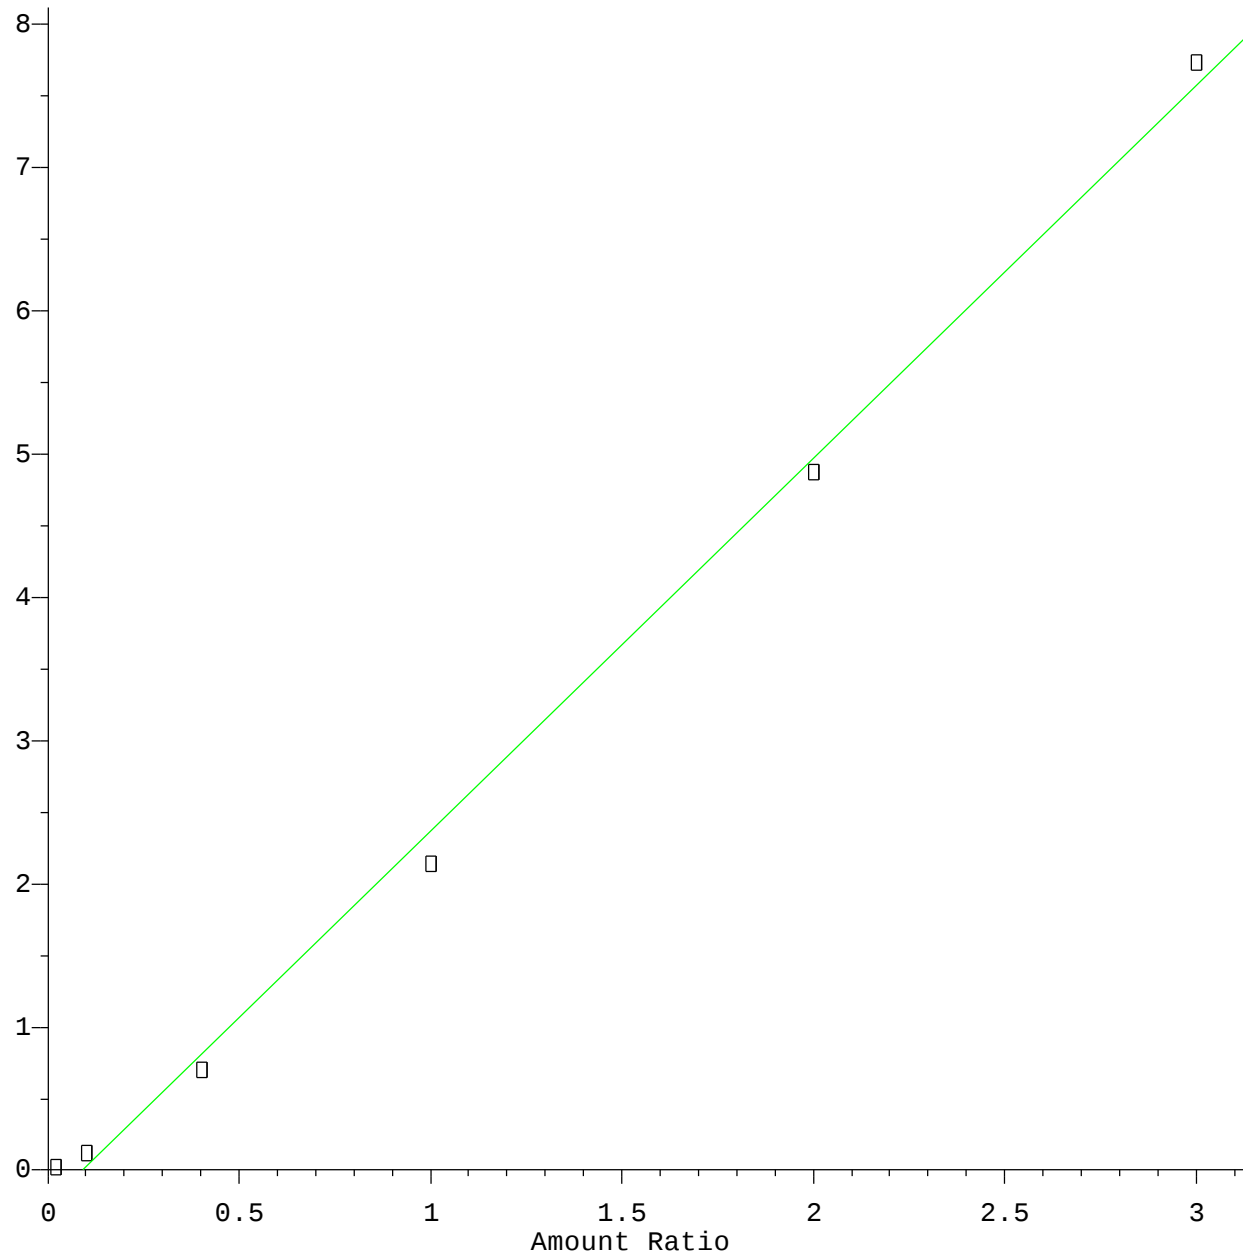


Resp Ratio = 2.60×10^0 * Amt - 2.34×10^{-1}
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018

1,2,4-Trichlorobenzene

Response Ratio

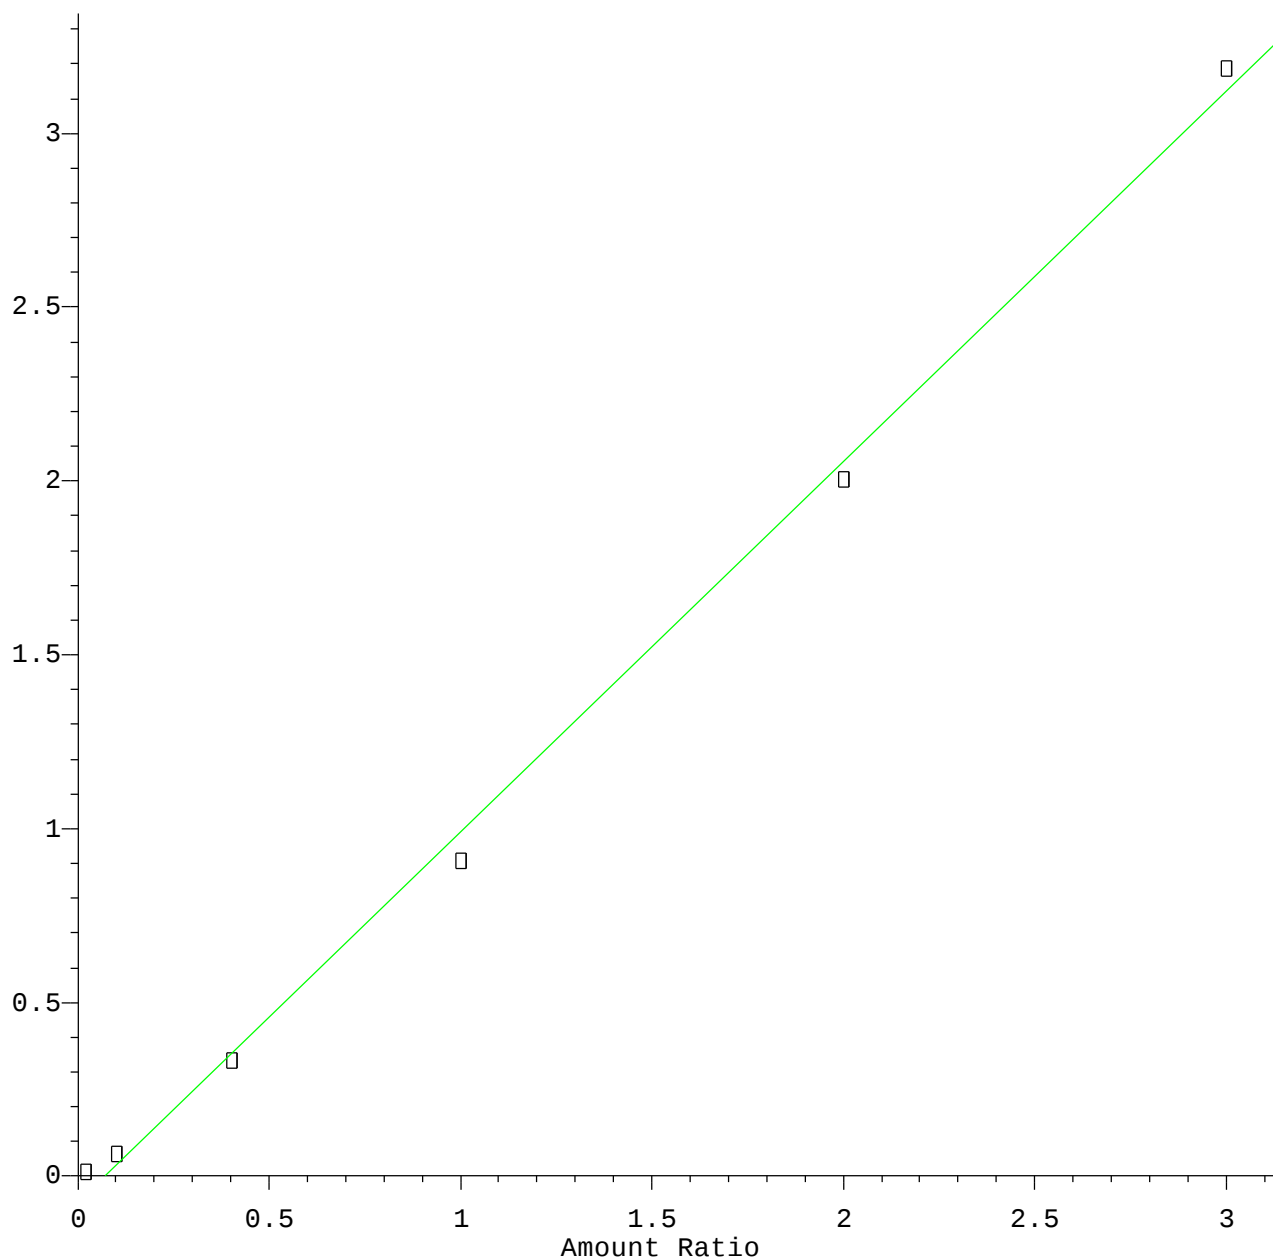


Resp Ratio = 1.06×10^0 * Amt - 7.40×10^{-2}
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018

2-Chloroethyl Vinyl ether

Response Ratio

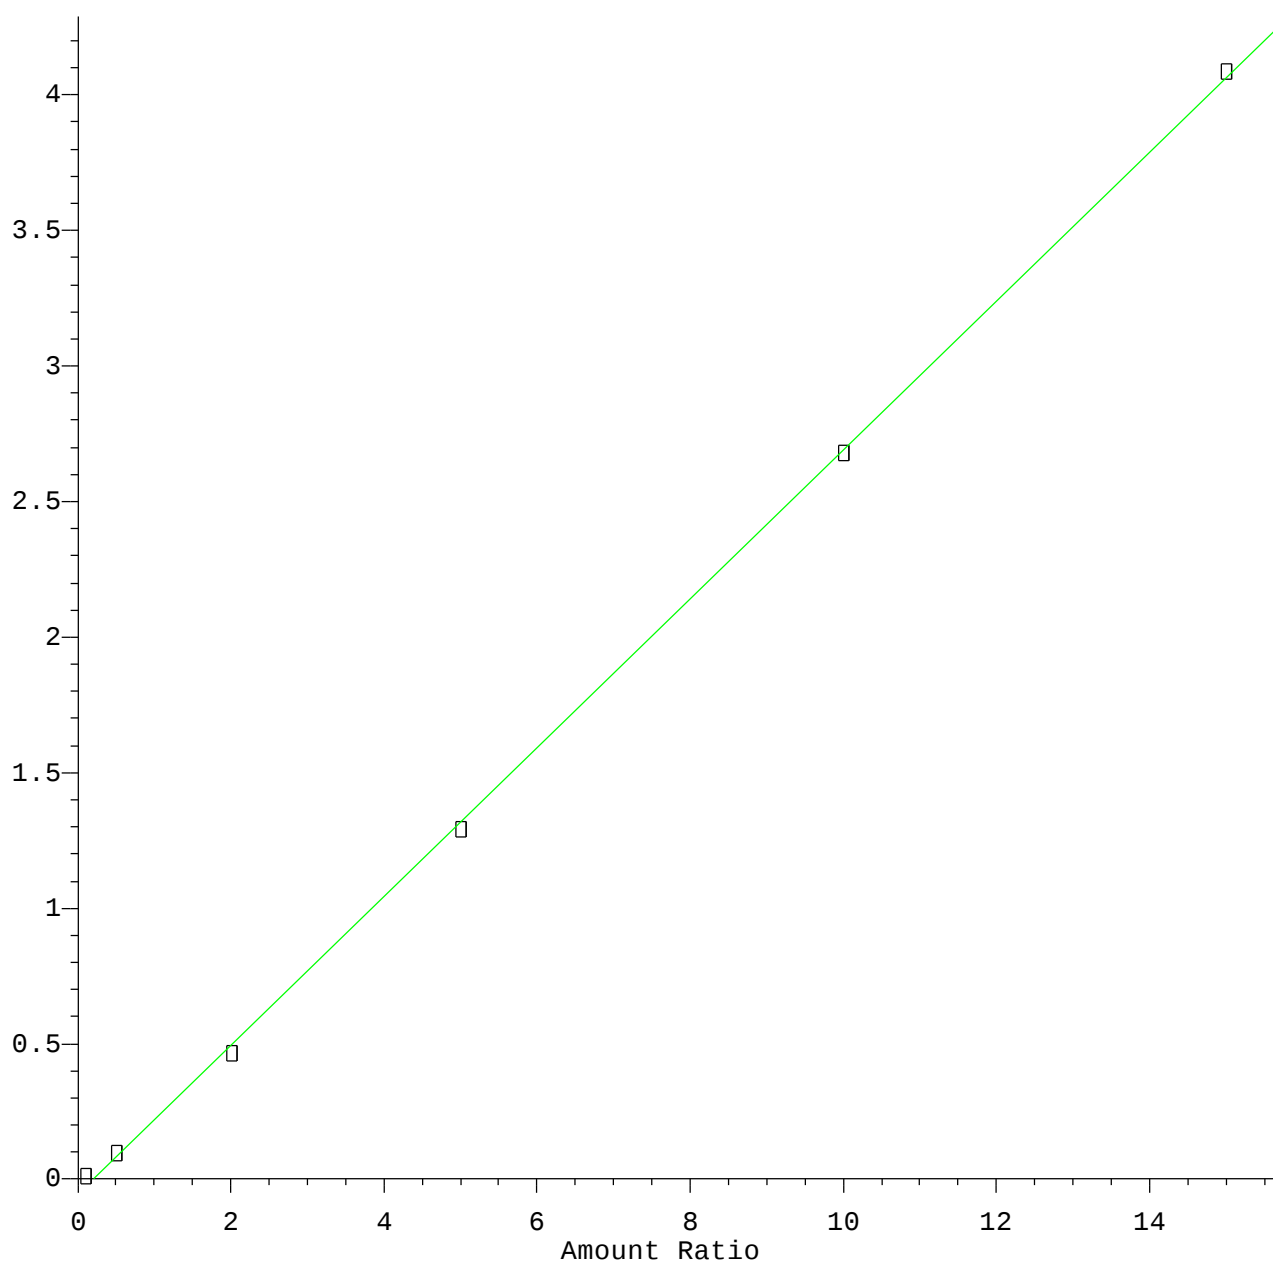


Resp Ratio = 2.74e-001 * Amt - 5.37e-002
Coef of Det (r²) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018


Ethyl methacrylate

Response Ratio

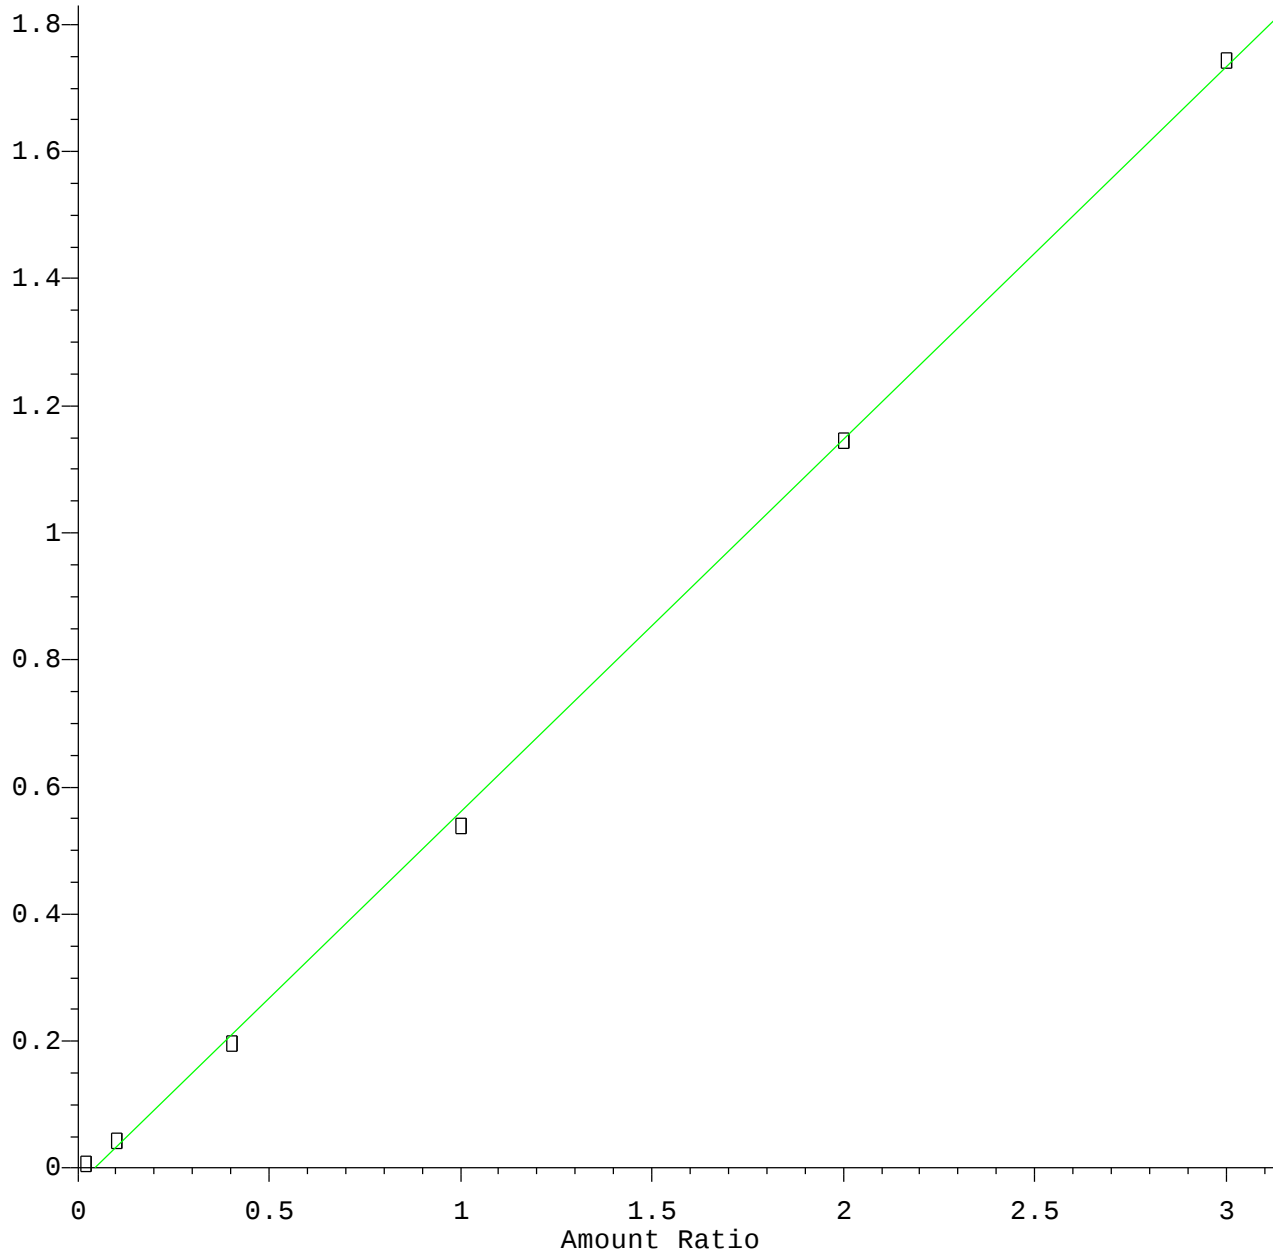


Resp Ratio = 5.86e-001 * Amt - 2.53e-002
Coef of Det (r²) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018

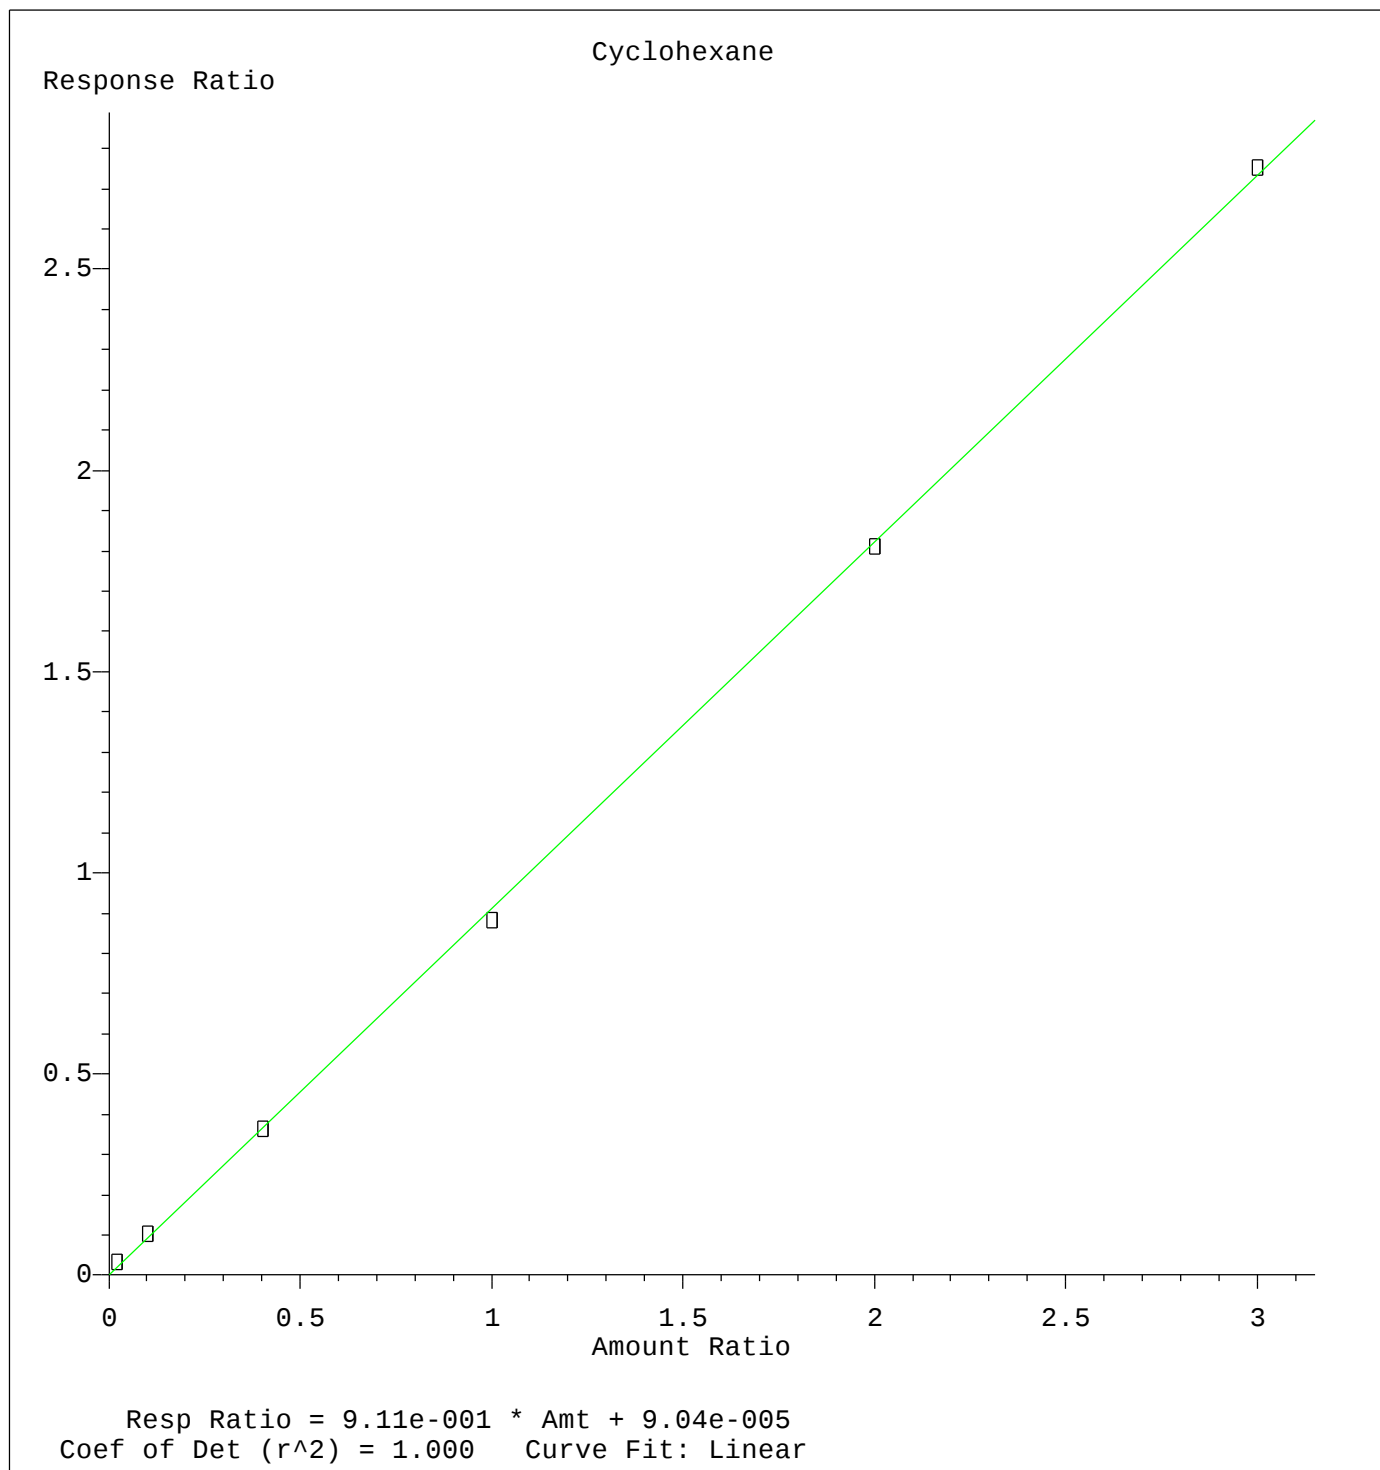

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018

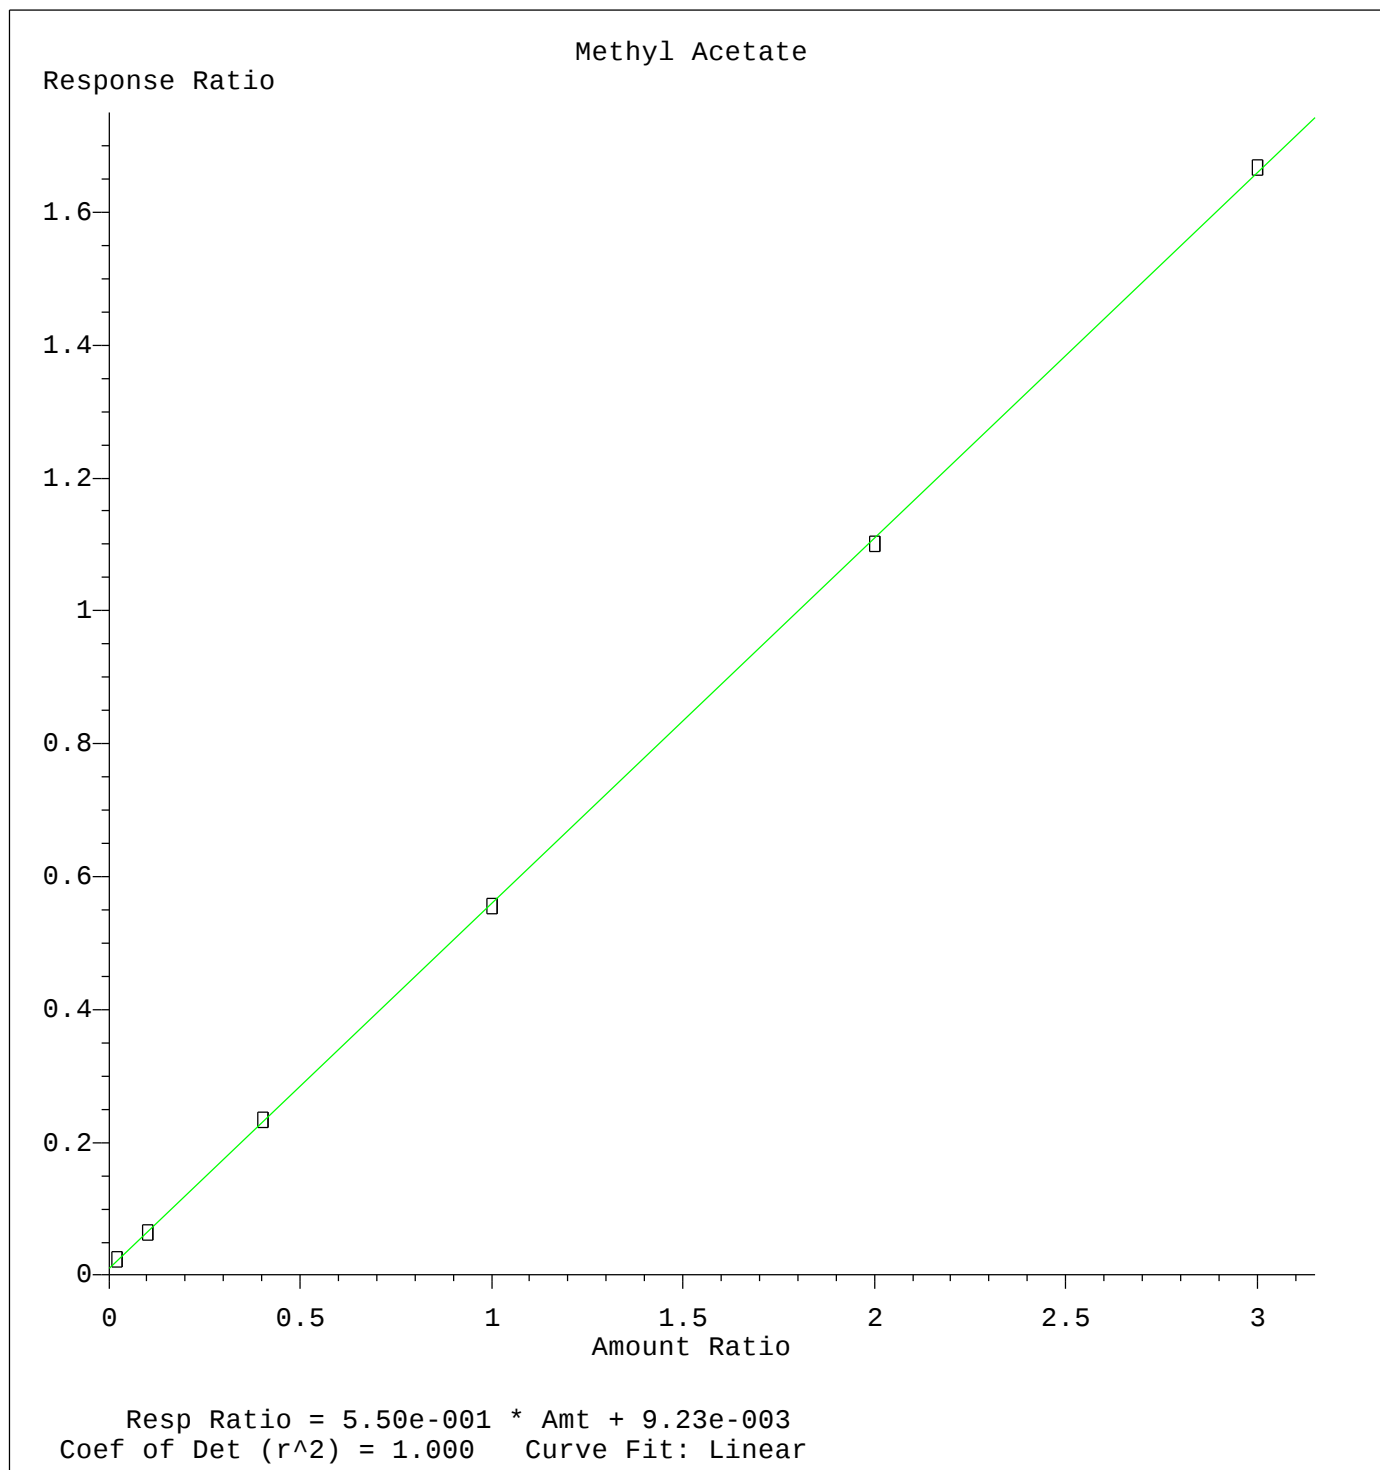

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018

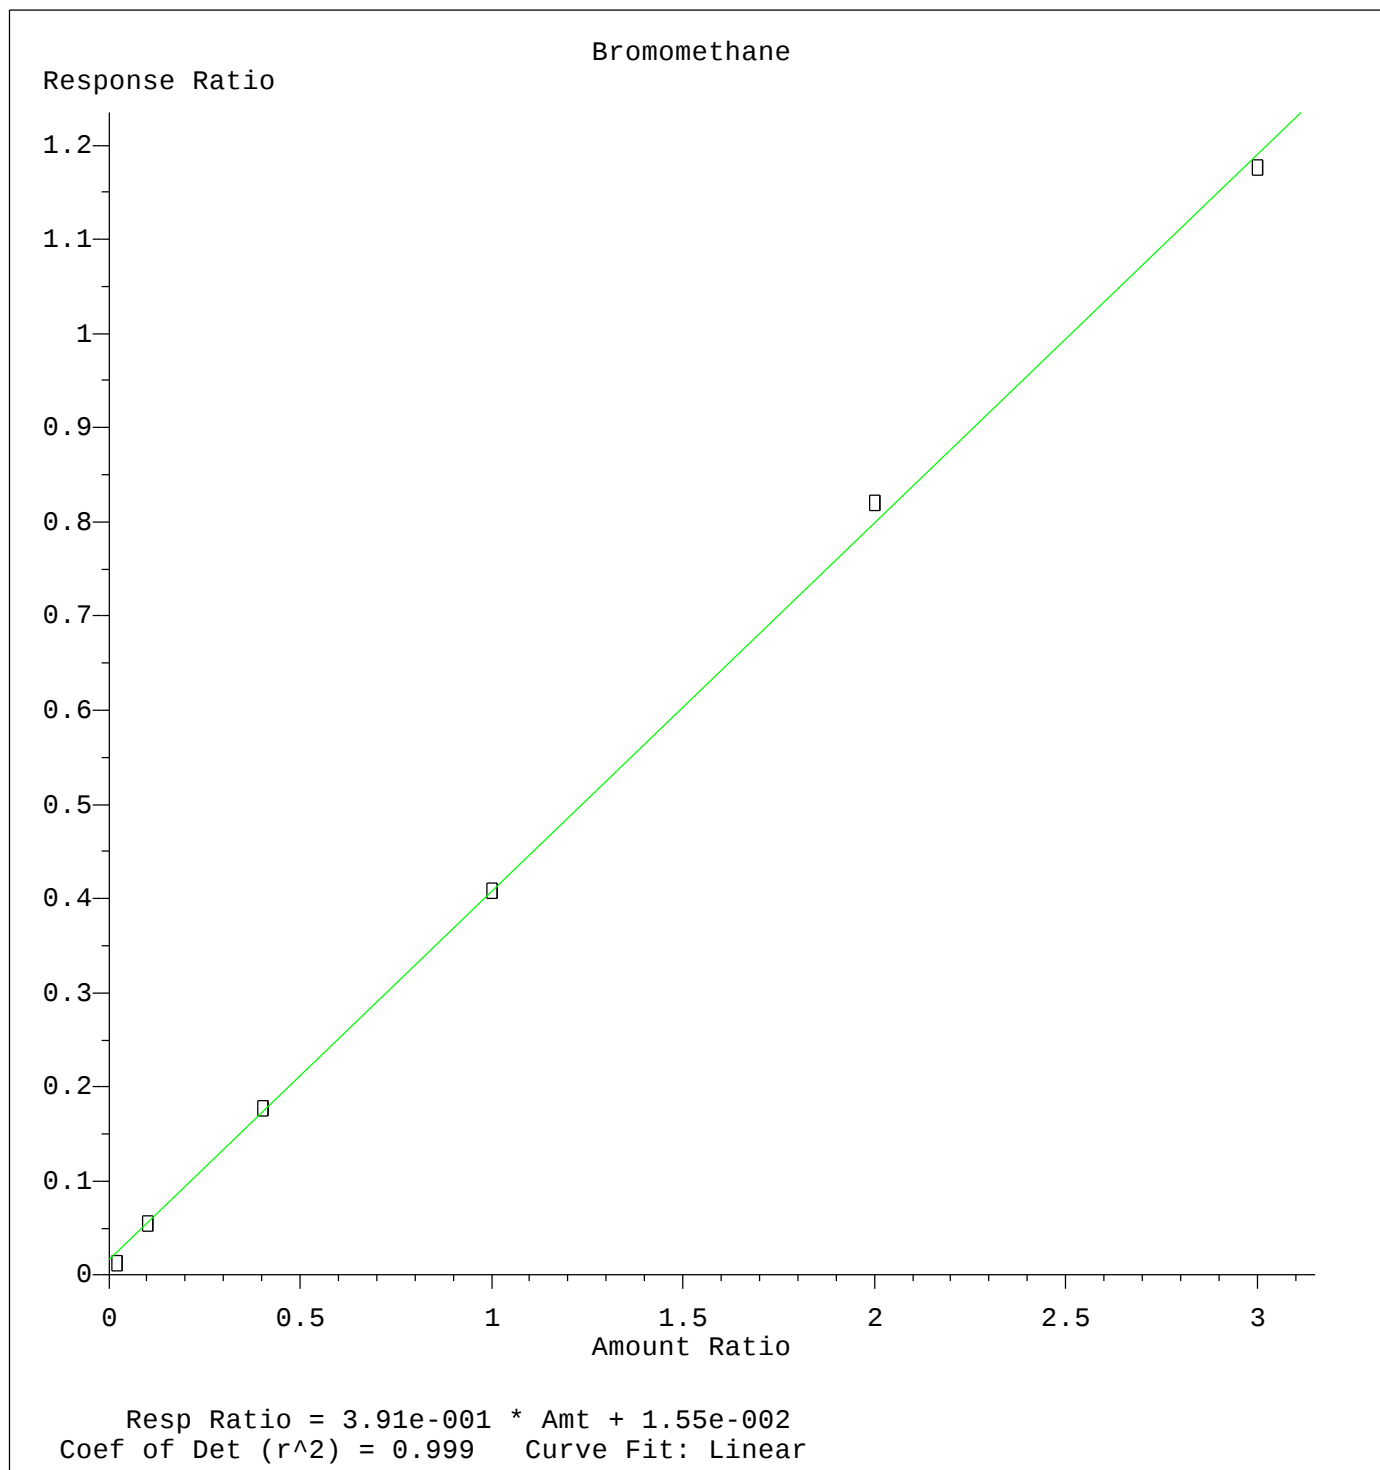

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Calibration Table Last Updated: Thu Jul 19 16:34:06 2018