

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071818\
 Data File : VN049878.D
 Acq On : 18 Jul 2018 17:37
 Operator : MD\SY
 Sample : PB111206ZHE#10
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB111206ZHE#10

Quant Time: Jul 19 04:44:05 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 18 13:09:48 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	584070	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	961223	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	812354	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.35	152	313564	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	411367	51.24	ug/l	0.00
Spiked Amount			Recovery	=	102.48%	
35) Dibromofluoromethane	7.59	113	361287	44.77	ug/l	0.00
Spiked Amount			Recovery	=	89.54%	
50) Toluene-d8	10.09	98	1292772	43.97	ug/l	0.00
Spiked Amount			Recovery	=	87.94%	
62) 4-Bromofluorobenzene	12.40	95	359417	35.50	ug/l	0.00
Spiked Amount			Recovery	=	71.00%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.83	43	24665	11.87	ug/l	97
18) Methyl Acetate	4.34	43	20921	2.42	ug/l	94
20) Methylene Chloride	4.55	84	13525	1.71	ug/l	94
43) Isopropyl Acetate	8.17	43	253573	19.78	ug/l	99
59) 2-Hexanone	10.77	43	22560	4.69	ug/l #	61
95) Naphthalene	15.14	128	6305	4.88	ug/l	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN071818\
Data File : VN049878.D
Acq On : 18 Jul 2018 17:37
Operator : MD\SY
Sample : PB111206ZHE#10
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB111206ZHE#10

Quant Time: Jul 19 04:44:05 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 18 13:09:48 2018
Response via : Initial Calibration

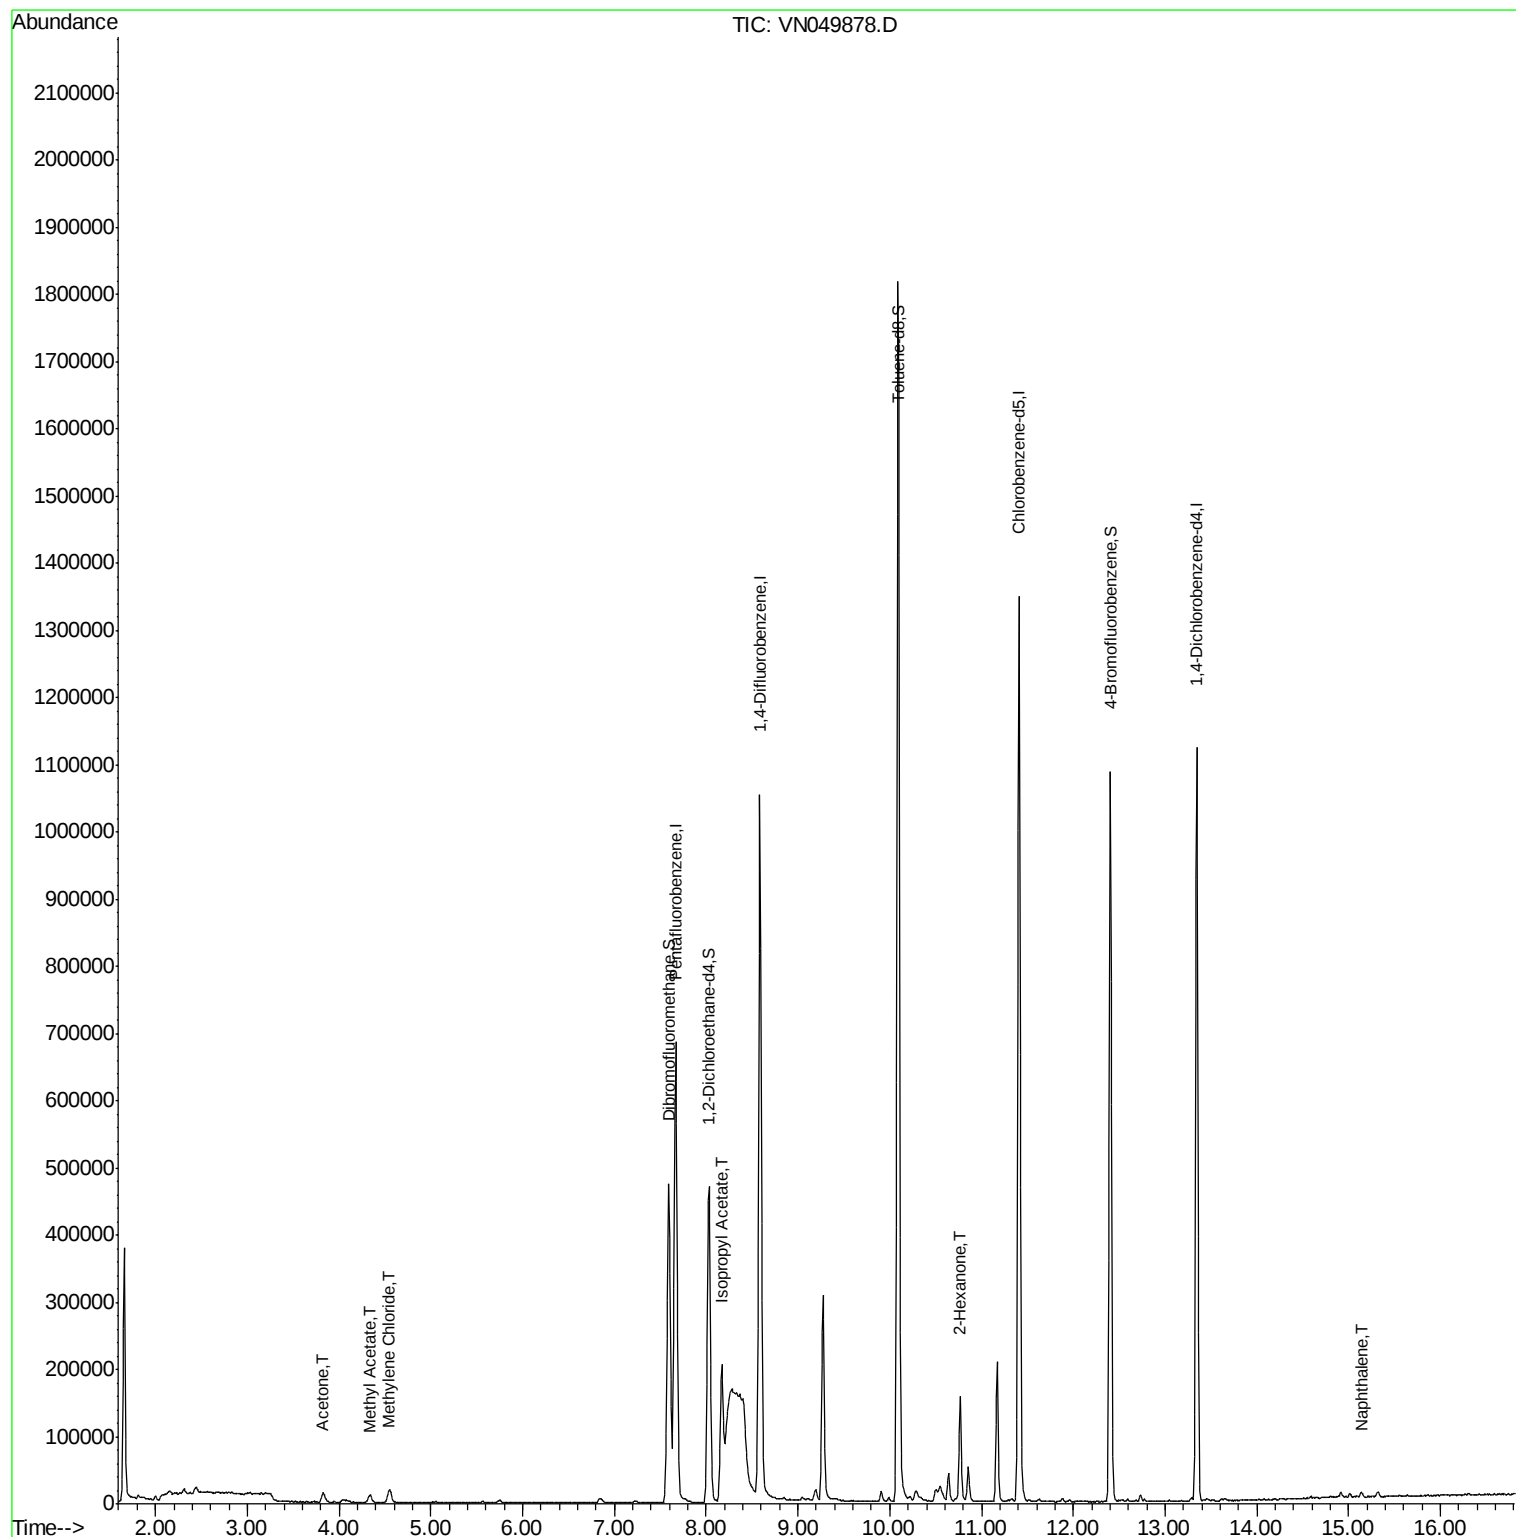

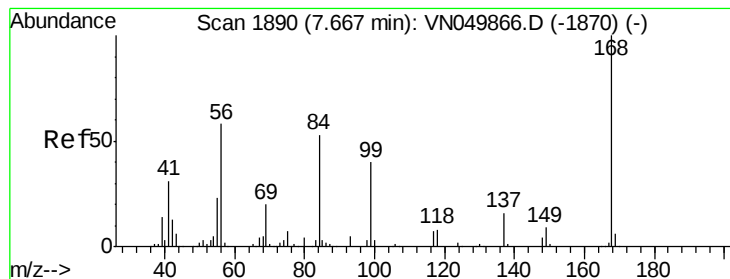

#1

Pentafluorobenzene

Concen: 50.00 ug/l

RT: 7.67 min Scan# 1890

Delta R.T. 0.00 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37

Instrument :

MSVOA_N

ClientSampleId :


PB111206ZHE#10

Tot Ion:168 Resp: 584070

Ion Ratio Lower Upper




168 100

99 51.1 40.6 61.0



Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

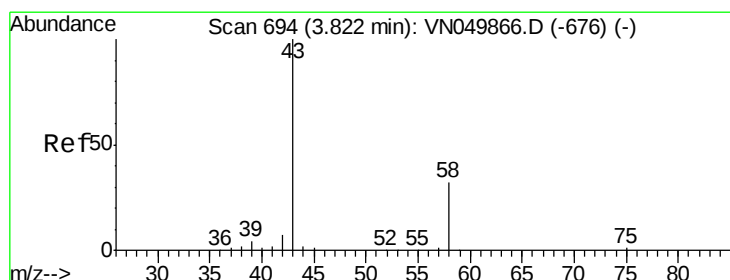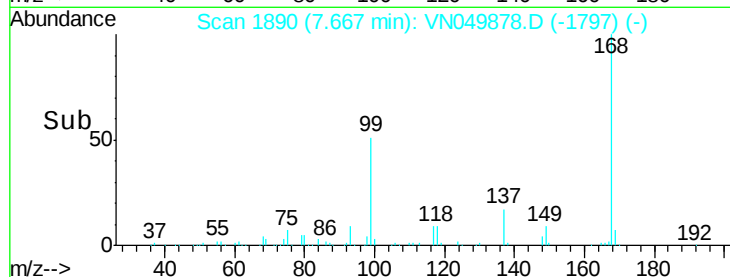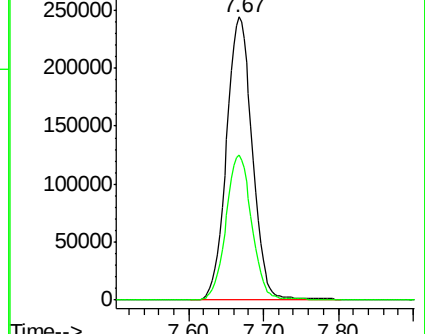

#16

Acetone

Concen: 11.87 ug/l

RT: 3.83 min Scan# 696

Delta R.T. 0.01 min

Lab File: VN049878.D


Acq: 18 Jul 2018 17:37

Tgt Ion: 43 Resp: 24665

Ion Ratio Lower Upper



43 100


58 30.7 25.9 38.9



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

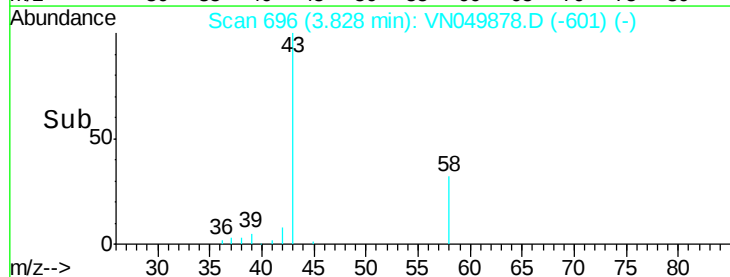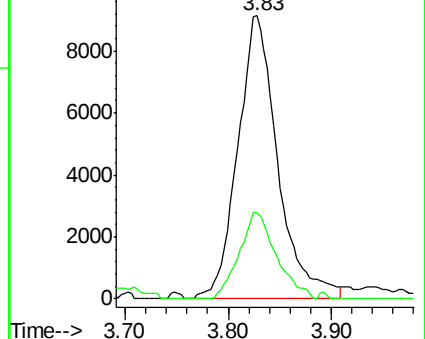

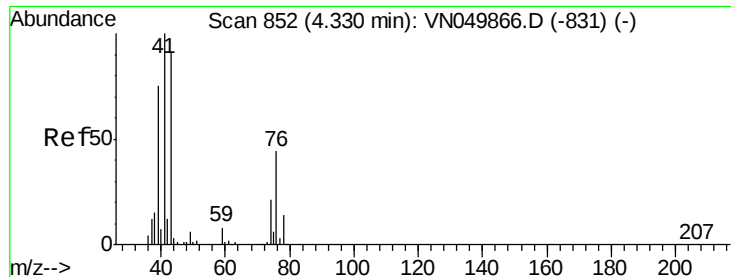

#18

Methyl Acetate

Concen: 2.42 ug/l

RT: 4.34 min Scan# 855

Delta R.T. 0.01 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37

Instrument :

MSVOA_N

ClientSampleId :


PB111206ZHE#10

Tot Ion: 43 Resp: 20921

Ion Ratio Lower Upper




43 100

74 21.9 19.8 29.8

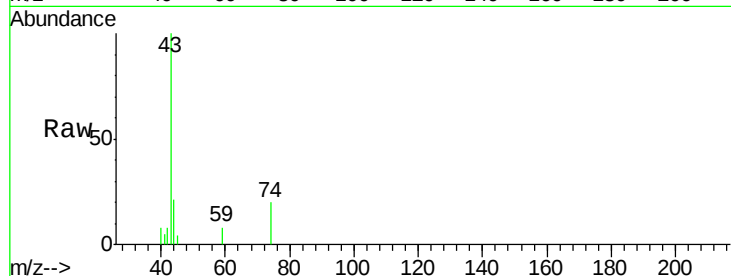

Abundance Ion 43.00 (42.70 to 43.70): VN049866.D (-831) (-)

Ion 74.00 (73.70 to 74.70): VN049866.D (-831) (-)

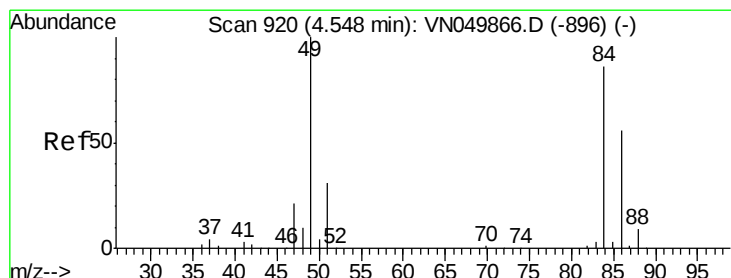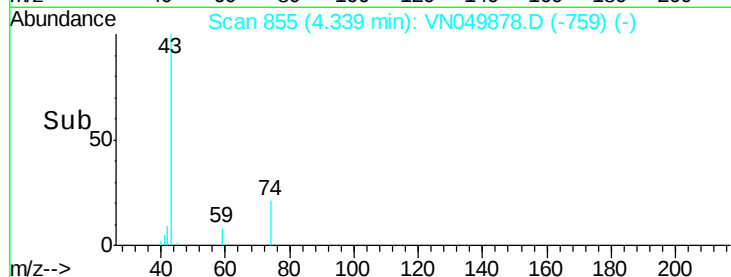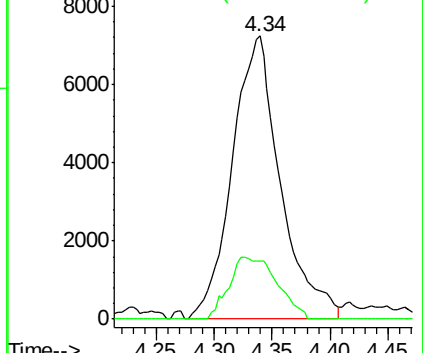

#20

Methylene Chloride

Concen: 1.71 ug/l

RT: 4.55 min Scan# 920

Delta R.T. 0.00 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37

Tgt Ion: 84 Resp: 13525


Ion Ratio Lower Upper

84 100

49 126.0 95.4 143.2

51 32.2 28.4 42.6

86 71.7 52.6 79.0


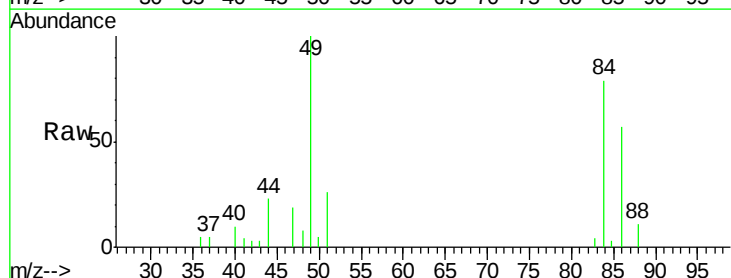



Abundance Ion 83.90 (83.60 to 84.60): VN049866.D (-896) (-)

Ion 48.90 (48.60 to 49.60): VN049866.D (-896) (-)

Ion 50.90 (50.60 to 51.60): VN049866.D (-896) (-)

Ion 85.90 (85.60 to 86.60): VN049866.D (-896) (-)



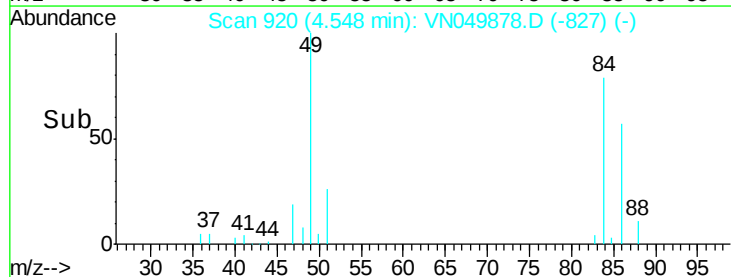
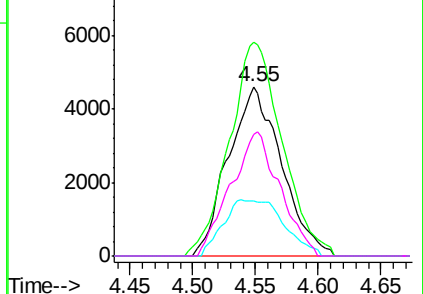


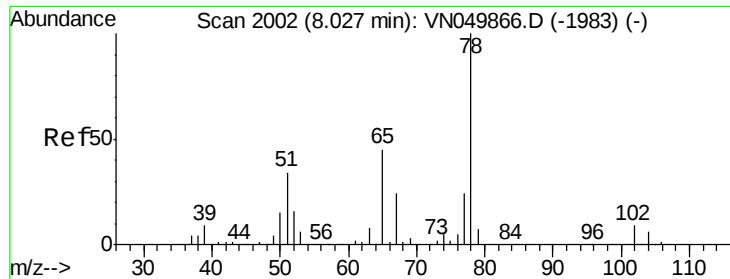

#33
 1,2-Dichloroethane-d4
 Concen: 51.24 ug/l
 RT: 8.03 min Scan# 2002
 Delta R.T. 0.00 min
 Lab File: VN049878.D
 Acq: 18 Jul 2018 17:37




Instrument :
 MSVOA_N
 ClientSampleId :
 PB111206ZHE#10


Tot Ion: 65 Resp: 411367
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 107.2

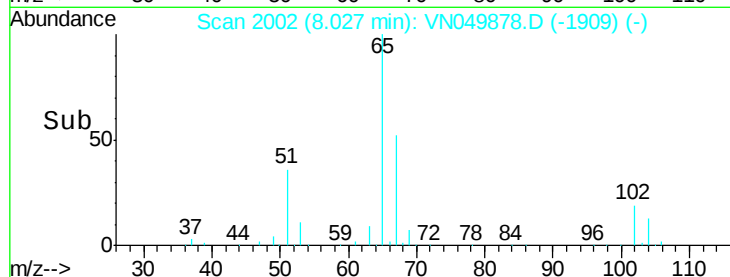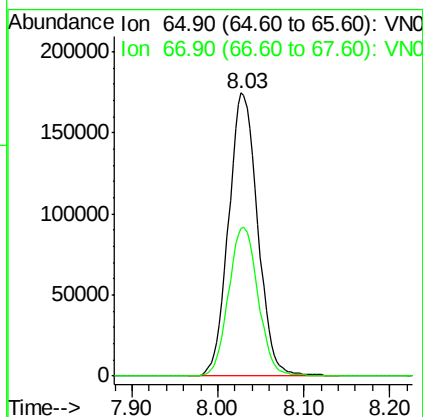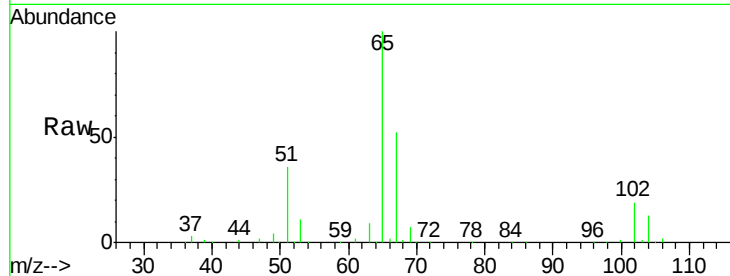

#34
 1,4-Difluorobenzene
 Concen: 50.00 ug/l
 RT: 8.59 min Scan# 2176
 Delta R.T. 0.00 min
 Lab File: VN049878.D
 Acq: 18 Jul 2018 17:37

Tgt Ion: 114 Resp: 961223
 Ion Ratio Lower Upper
 114 100
 63 20.0 0.0 39.8
 88 15.4 0.0 30.6


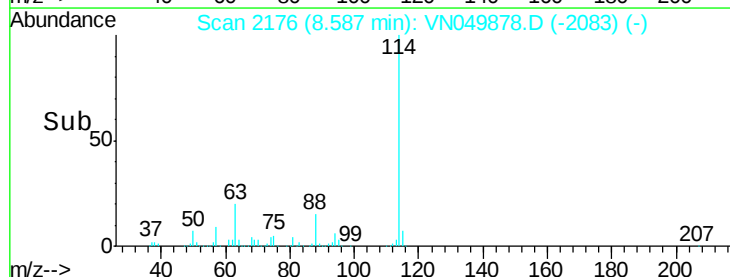
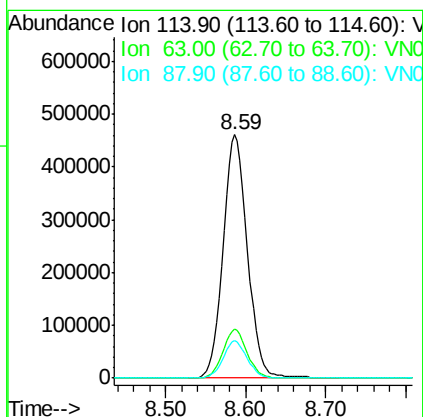



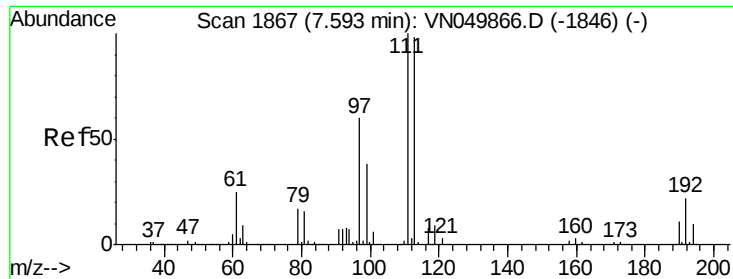

#35
 Dibromofluoromethane
 Concen: 44.77 ug/l
 RT: 7.59 min Scan# 1867
 Delta R.T. 0.00 min
 Lab File: VN049878.D
 Acq: 18 Jul 2018 17:37




Instrument :
 MSVOA_N
 ClientSampleId :
 PB111206ZHE#10


Tot Ion	Ratio	Lower	Upper
113	100		
111	102.5	81.8	122.8
192	21.6	17.8	26.6

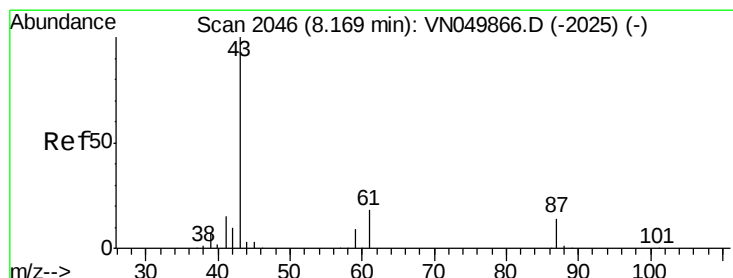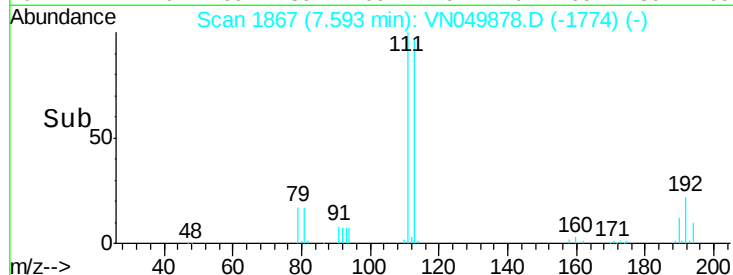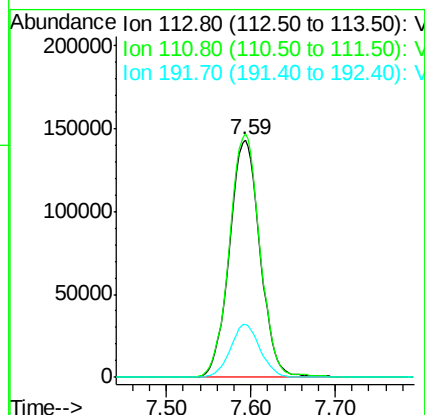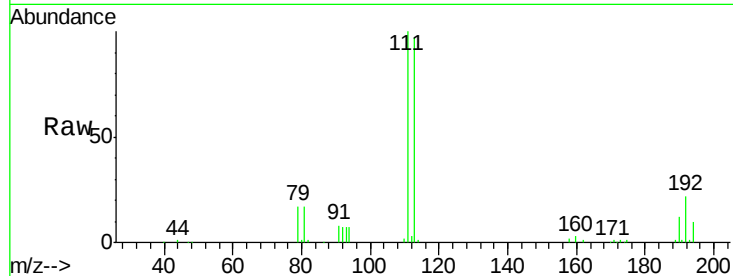

#43
 Isopropyl Acetate
 Concen: 19.78 ug/l
 RT: 8.17 min Scan# 2046
 Delta R.T. 0.00 min
 Lab File: VN049878.D
 Acq: 18 Jul 2018 17:37

Tgt Ion	Ratio	Lower	Upper
43	100		
61	18.3	14.9	22.3
87	12.4	10.0	15.0


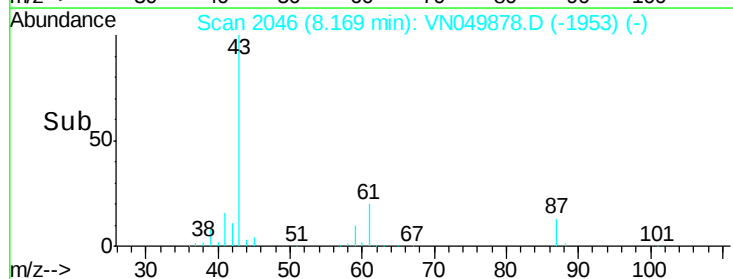
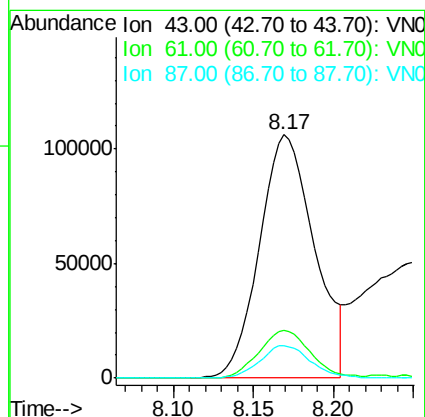
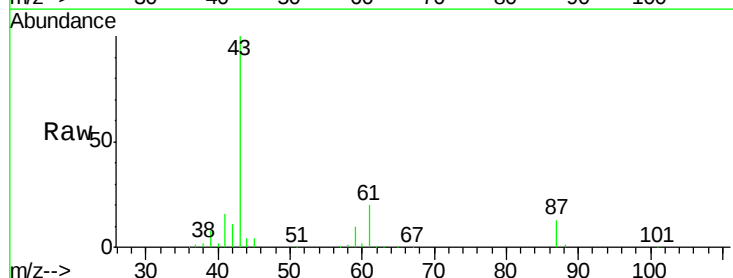


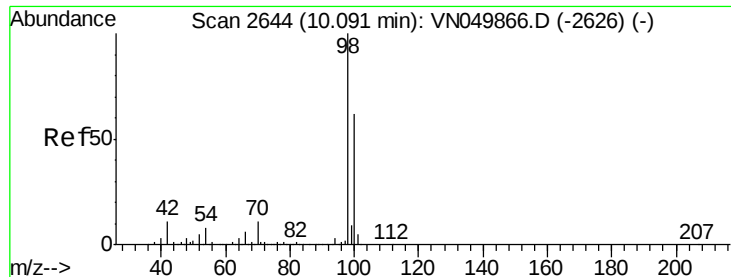

#50
Toluene-d8
Concen: 43.97 ug/l
RT: 10.09 min Scan# 2644
Delta R.T. 0.00 min
Lab File: VN049878.D
Acq: 18 Jul 2018 17:37




Instrument :
MSVOA_N
ClientSampleId :
PB111206ZHE#10


Tot Ion: 98 Resp: 1292772
Ion Ratio Lower Upper
98 100
100 63.2 51.7 77.5

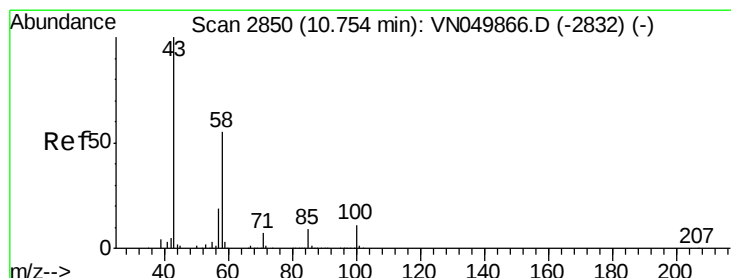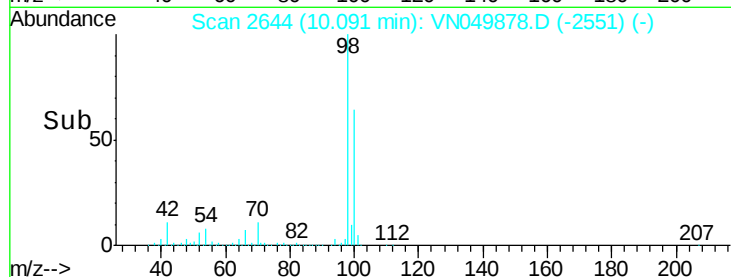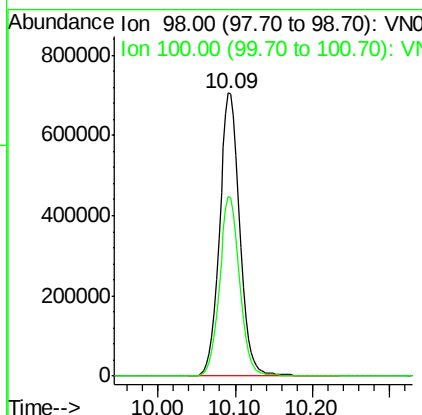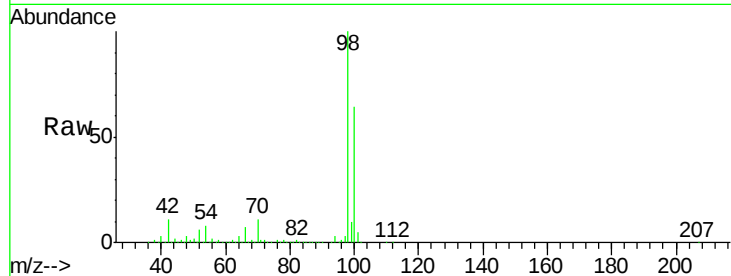

#59
2-Hexanone
Concen: 4.69 ug/l
RT: 10.77 min Scan# 2854
Delta R.T. 0.01 min
Lab File: VN049878.D
Acq: 18 Jul 2018 17:37

Tgt Ion: 43 Resp: 22560
Ion Ratio Lower Upper
43 100
58 27.4 27.8 83.4#

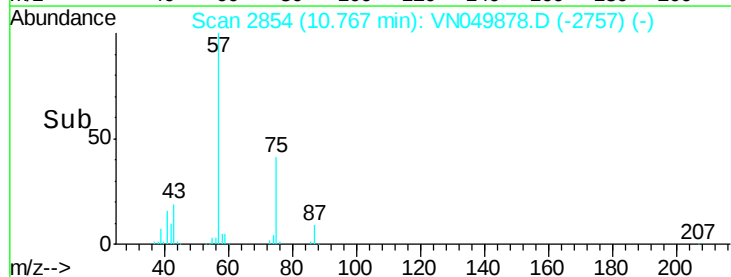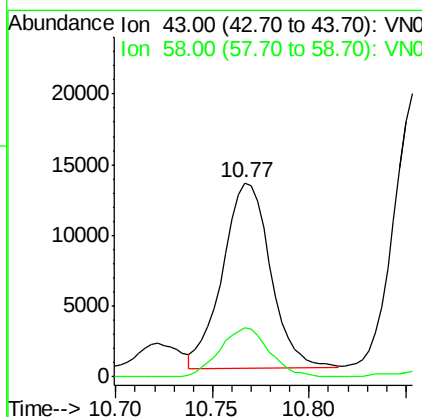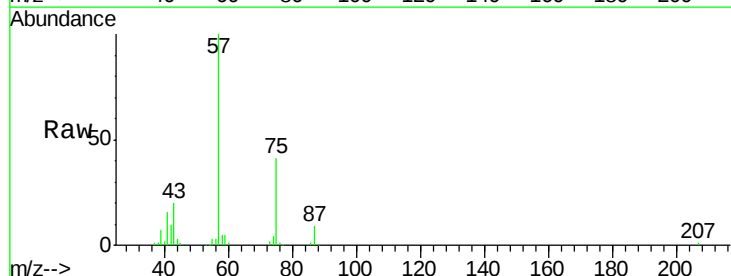

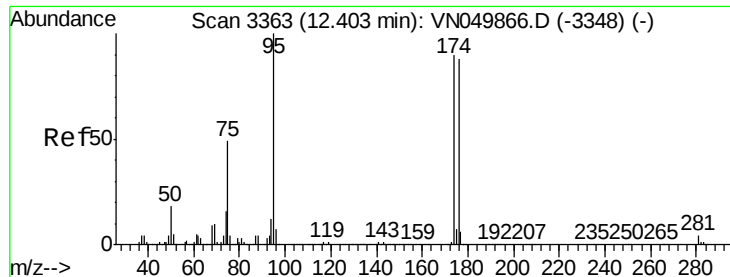

#62

4-Bromofluorobenzene

Concen: 35.50 ug/l

RT: 12.40 min Scan# 3363

Delta R.T. 0.00 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37

Instrument :

MSVOA_N

ClientSampleId :

PB111206ZHE#10


Tot Ion: 95 Resp: 359417

Ion Ratio Lower Upper

95 100

174 92.1 0.0 179.6




176 88.4 0.0 174.0



Abundance Ion 94.90 (94.60 to 95.60): VN049866.D (-3348) (-)

Ion 173.80 (173.50 to 174.50): VN049866.D (-3348) (-)

Ion 175.80 (175.50 to 176.50): VN049866.D (-3348) (-)

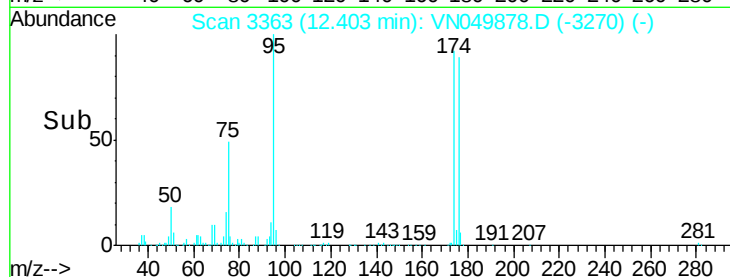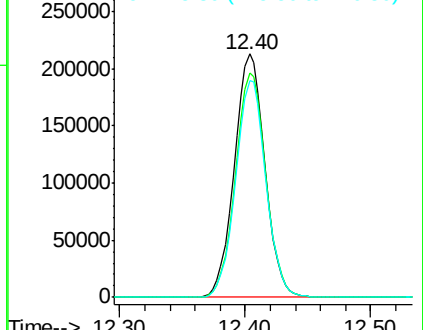

#63

Chlorobenzene-d5

Concen: 50.00 ug/l

RT: 11.41 min Scan# 3054

Delta R.T. 0.00 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37


Tgt Ion: 117 Resp: 812354

Ion Ratio Lower Upper

117 100

82 54.4 41.9 62.9



119 32.3 25.4 38.2




Abundance Ion 116.90 (116.60 to 117.60): VN049866.D (-3038) (-)

Ion 82.00 (81.70 to 82.70): VN049866.D (-3038) (-)

Ion 118.90 (118.60 to 119.60): VN049866.D (-3038) (-)

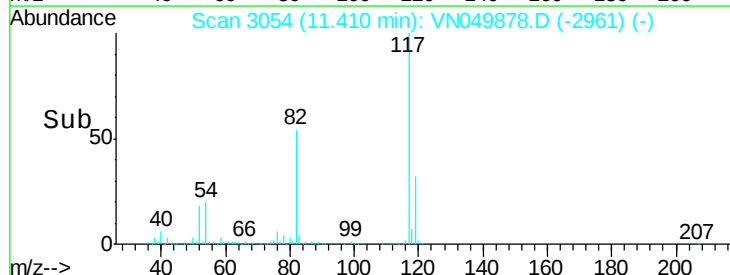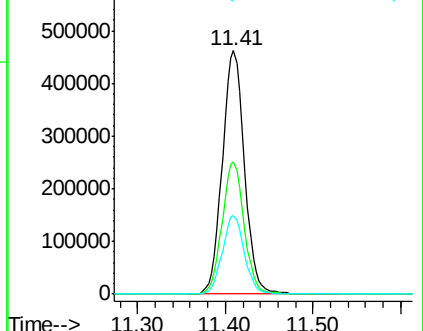

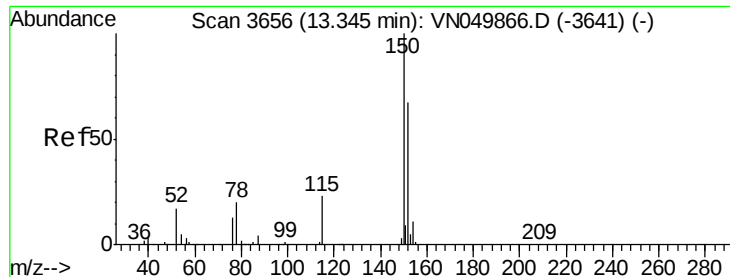

#72

1,4-Dichlorobenzene-d4

Concen: 50.00 ug/l

RT: 13.35 min Scan# 3656

Delta R.T. 0.00 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37

Instrument :

MSVOA_N

ClientSampleId :

PB111206ZHE#10


Tot Ion:152 Resp: 313564

Ion Ratio Lower Upper

152 100

115 56.4 28.1 84.2




150 157.6 0.0 347.6



Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

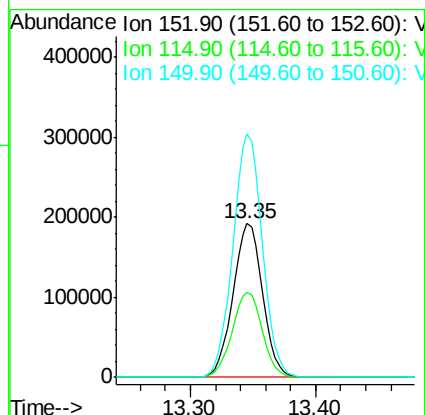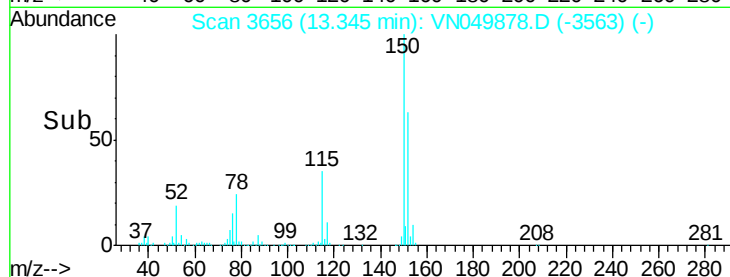

#95

Naphthalene

Concen: 4.88 ug/l

RT: 15.14 min Scan# 4213

Delta R.T. 0.00 min

Lab File: VN049878.D

Acq: 18 Jul 2018 17:37


Tgt Ion:128 Resp: 6305

Ion Ratio Lower Upper

128 100

127 13.1 10.4 15.6

129 11.3 8.6 13.0



Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

