


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071819\
 Data File : VN056800.D
 Acq On : 18 Jul 2019 8:22
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N071319W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Fri Jul 12 23:58:13 2019

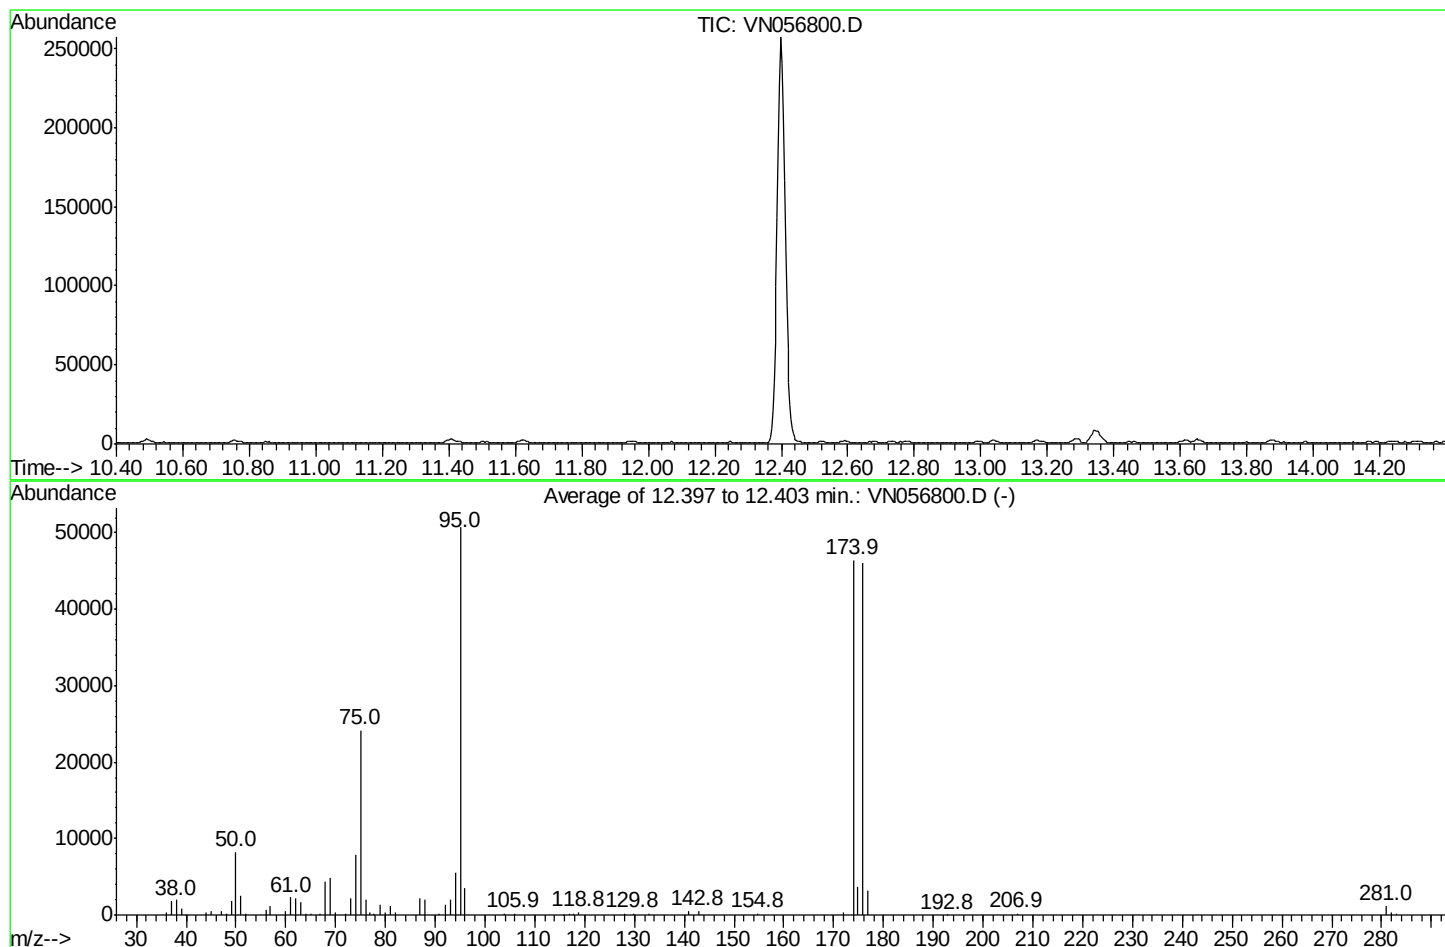

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.3	8242	PASS
75	95	30	60	47.6	24122	PASS
95	95	100	100	100.0	50720	PASS
96	95	5	9	7.1	3586	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	91.6	46469	PASS
175	174	5	9	8.0	3732	PASS
176	174	95	101	99.0	45997	PASS
177	176	5	9	6.8	3118	PASS