


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN071819\
Data File : VN056810.D
Acq On : 18 Jul 2019 13:49
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N071319W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Fri Jul 12 23:58:13 2019

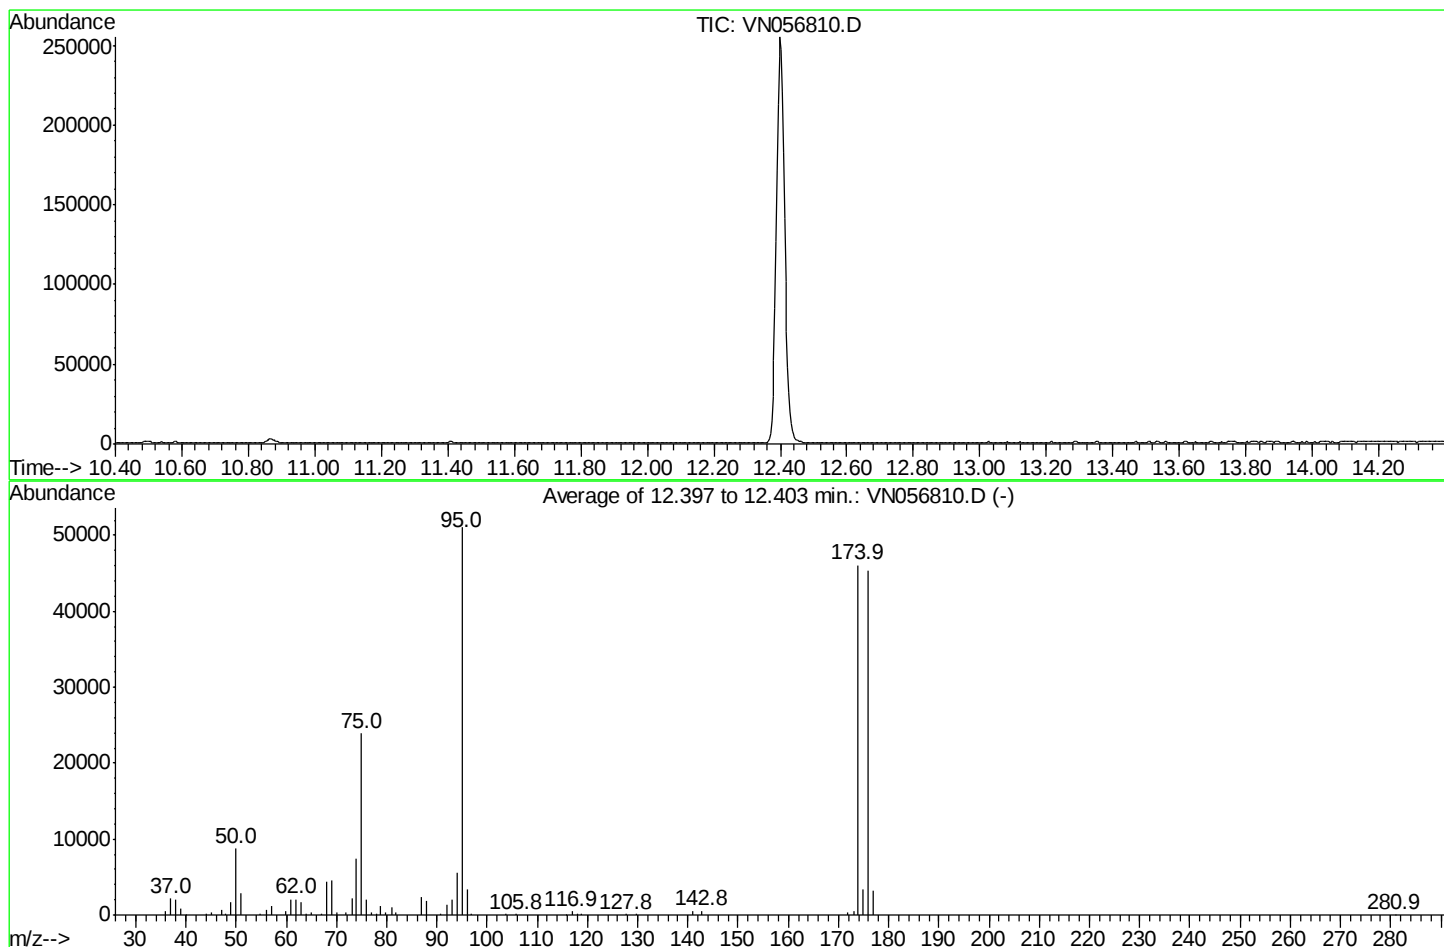

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8697	PASS
75	95	30	60	46.7	23864	PASS
95	95	100	100	100.0	51048	PASS
96	95	5	9	6.6	3371	PASS
173	174	0.00	2	1.2	534	PASS
174	95	50	100	90.3	46098	PASS
175	174	5	9	7.5	3460	PASS
176	174	95	101	98.2	45280	PASS
177	176	5	9	7.2	3247	PASS