

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071822\
 Data File : VN073497.D
 Acq On : 18 Jul 2022 14:26
 Operator : JC\MD
 Sample : N3711-05
 Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PSC124035

Quant Time: Jul 18 15:31:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 29 01:54:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.004	168	259915	50.000	ug/l	-0.01
34) 1,4-Difluorobenzene	8.898	114	444802	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.686	117	438761	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.616	152	212099	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.363	65	170103	45.335	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	90.660%
35) Dibromofluoromethane	7.945	113	139066	46.992	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	93.980%
50) Toluene-d8	10.380	98	482742	45.929	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.860%
62) 4-Bromofluorobenzene	12.674	95	215433	53.336	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	106.680%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071822\
Data File : VN073497.D
Acq On : 18 Jul 2022 14:26
Operator : JC\MD
Sample : N3711-05
Misc : 5.03g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PSC124035

Quant Time: Jul 18 15:31:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Quant Title : SW846 8260
QLast Update : Wed Jun 29 01:54:03 2022
Response via : Initial Calibration




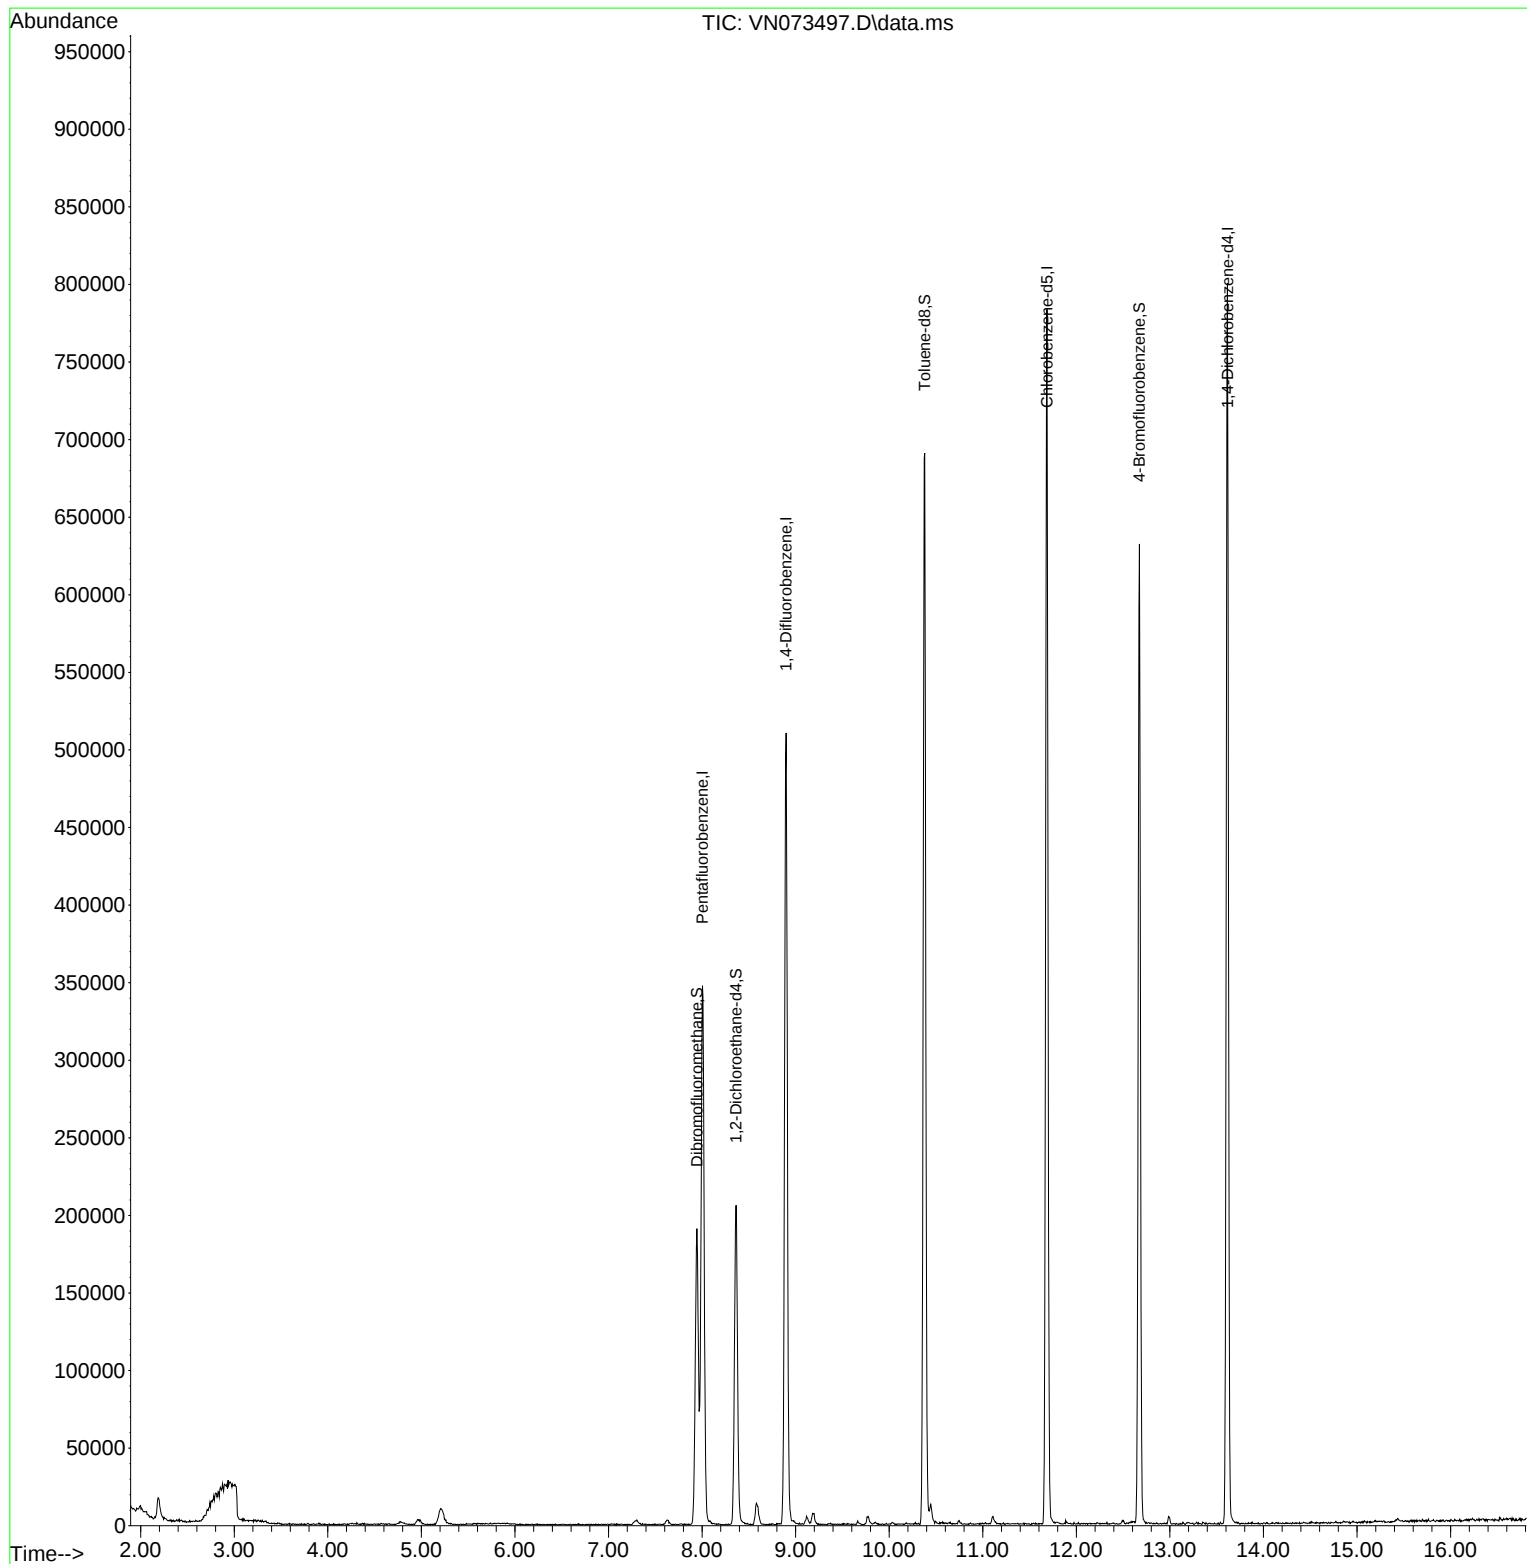


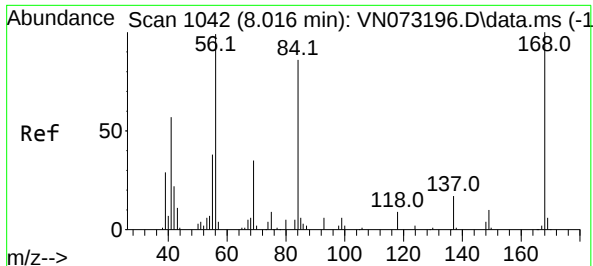

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.004 min Scan# 1101
Delta R.T. -0.012 min
Lab File: VN073497.D
Acq: 18 Jul 2022 14:26




Instrument :
MSVOA_N
ClientSampleId :
PSC124035

Tgt Ion:168 Resp: 259915
Ion Ratio Lower Upper
168 100
99 57.8 42.3 63.5

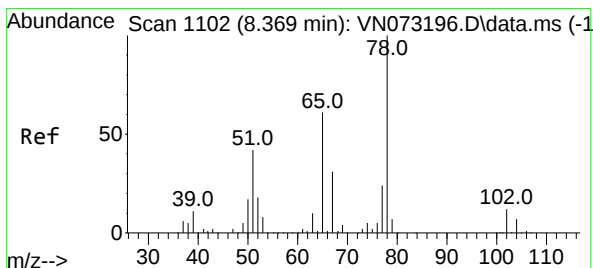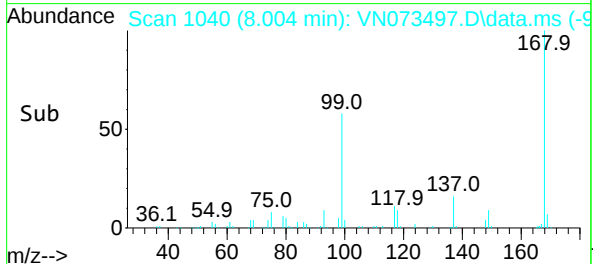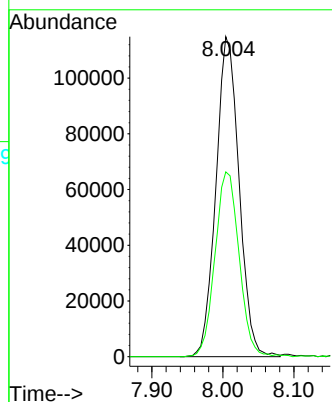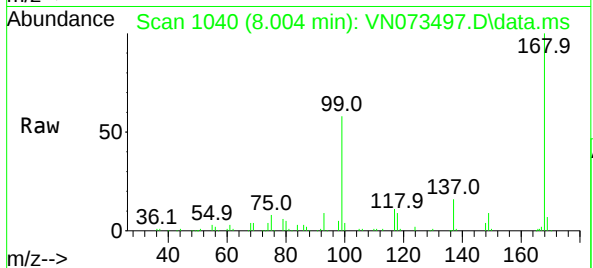

#33
1,2-Dichloroethane-d4
Concen: 45.335 ug/l
RT: 8.363 min Scan# 1101
Delta R.T. -0.006 min
Lab File: VN073497.D
Acq: 18 Jul 2022 14:26

Tgt Ion: 65 Resp: 170103
Ion Ratio Lower Upper
65 100
67 52.3 0.0 104.8

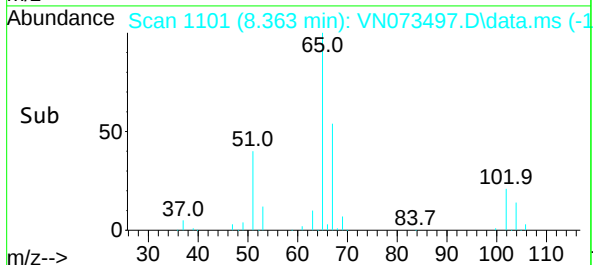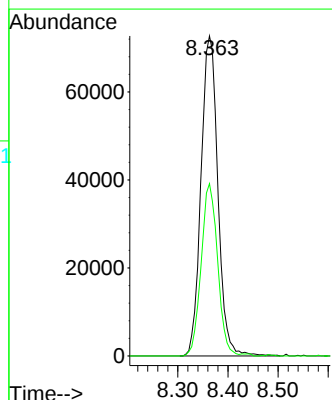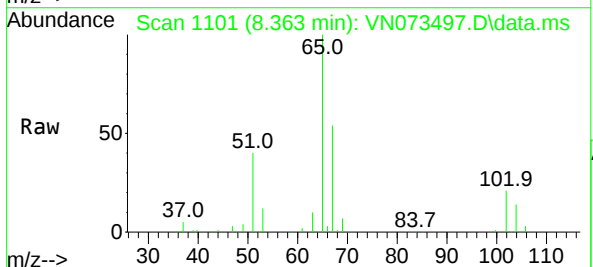



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.898 min Scan# 1192

Delta R.T. 0.000 min

Lab File: VN073497.D

Acq: 18 Jul 2022 14:26

Instrument :

MSVOA_N

ClientSampleId :

PSC124035





Tgt Ion:114 Resp: 444802

Ion Ratio Lower Upper

114 100

63 21.5 0.0 40.0

88 16.7 0.0 32.6

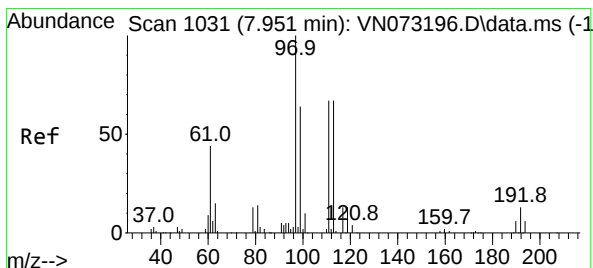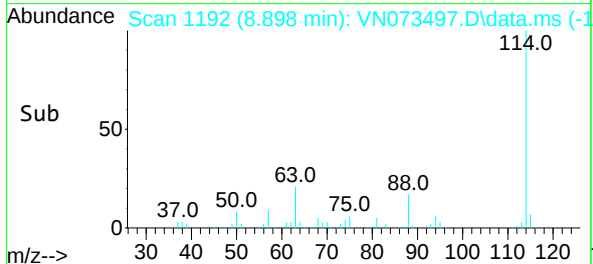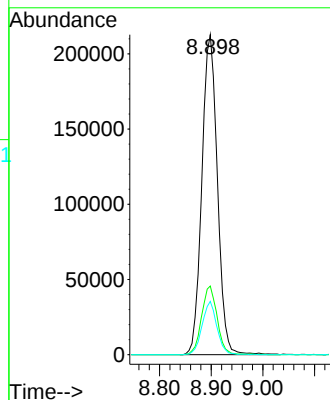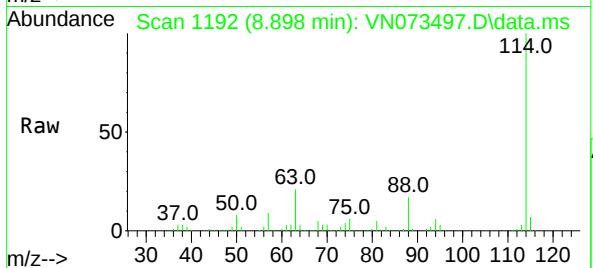

#35

Dibromofluoromethane

Concen: 46.992 ug/l

RT: 7.945 min Scan# 1030

Delta R.T. -0.006 min

Lab File: VN073497.D

Acq: 18 Jul 2022 14:26




Tgt Ion:113 Resp: 139066


Ion Ratio Lower Upper

113 100

111 105.2 81.4 122.0

192 18.6 17.0 25.6

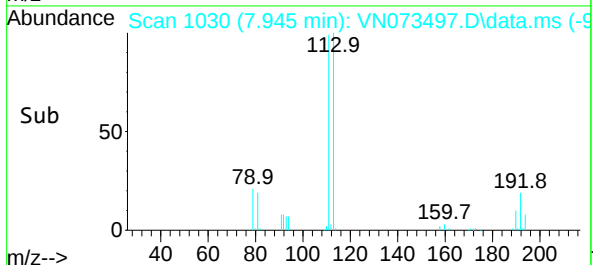
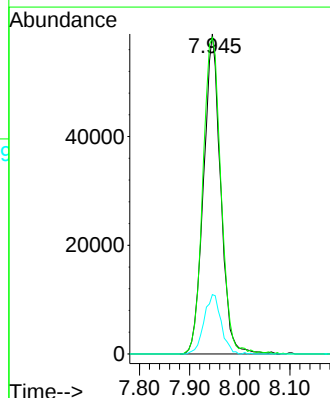
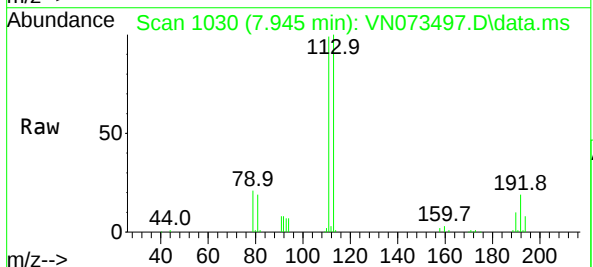


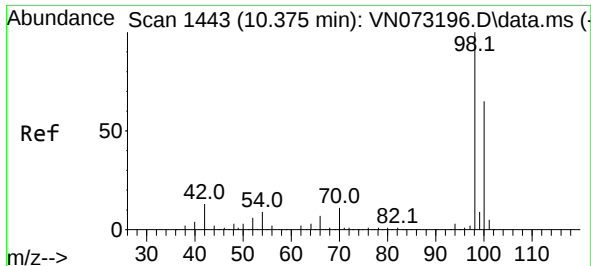

#50
Toluene-d8
Concen: 45.929 ug/l
RT: 10.380 min Scan# 1443
Delta R.T. 0.005 min
Lab File: VN073497.D
Acq: 18 Jul 2022 14:26




Instrument :
MSVOA_N
ClientSampleId :
PSC124035


Tgt Ion: 98 Resp: 482742
Ion Ratio Lower Upper
98 100
100 65.7 52.6 78.8

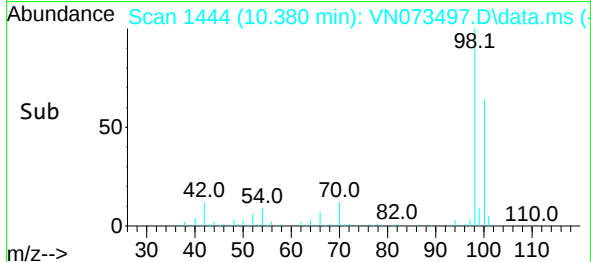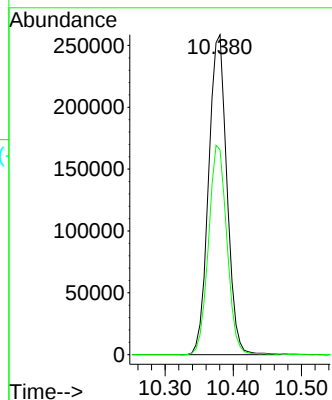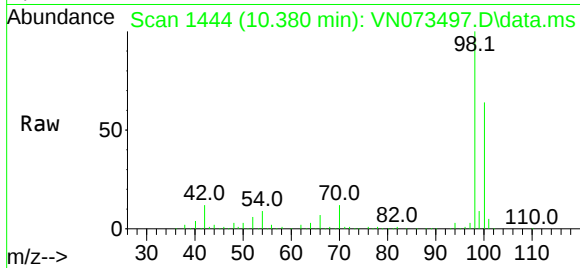

#62
4-Bromofluorobenzene
Concen: 53.336 ug/l
RT: 12.674 min Scan# 1834
Delta R.T. 0.005 min
Lab File: VN073497.D
Acq: 18 Jul 2022 14:26

Tgt Ion: 95 Resp: 215433
Ion Ratio Lower Upper
95 100
174 75.0 0.0 167.6
176 72.7 0.0 163.4

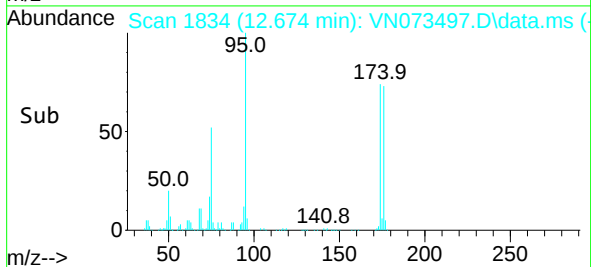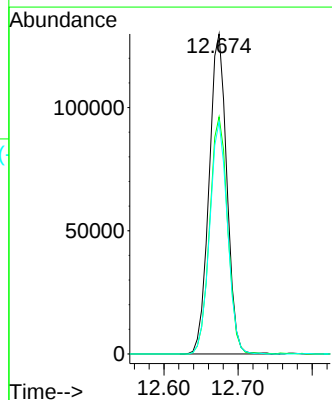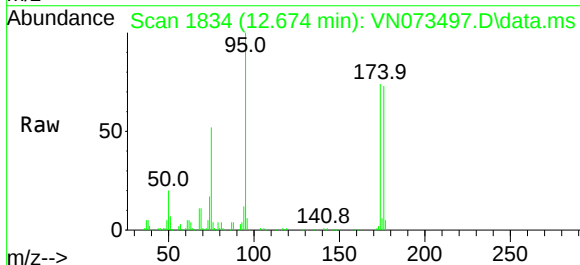

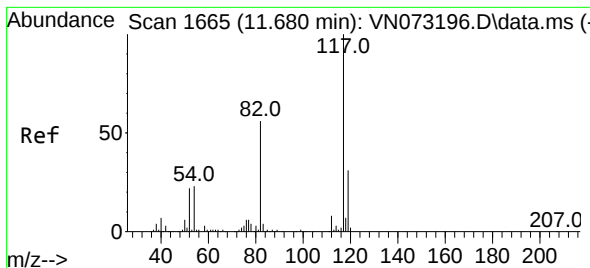

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.686 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN073497.D

Acq: 18 Jul 2022 14:26

Instrument :

MSVOA_N

ClientSampleId :

PSC124035





Tgt Ion:117 Resp: 438761

Ion Ratio Lower Upper

117 100

82 56.6 44.2 66.2

119 33.1 25.4 38.0

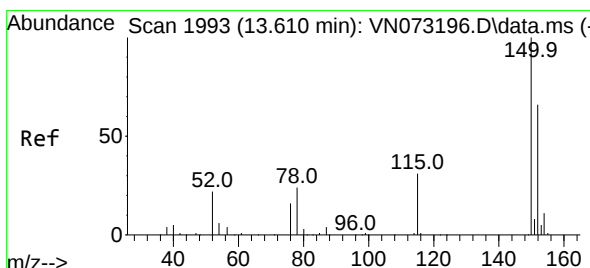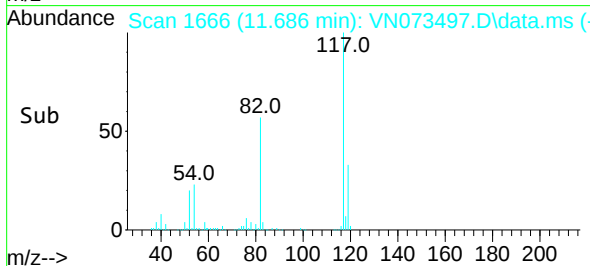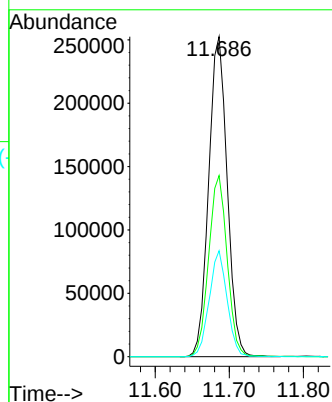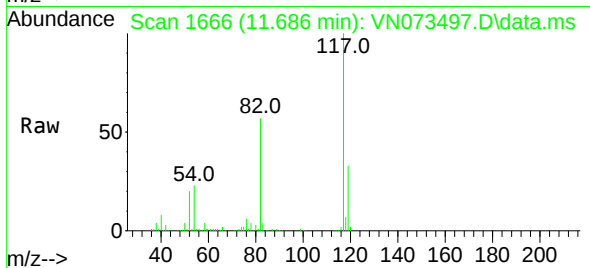

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.616 min Scan# 1994

Delta R.T. 0.006 min

Lab File: VN073497.D

Acq: 18 Jul 2022 14:26

Tgt Ion:152 Resp: 212099

Ion Ratio Lower Upper

152 100

115 60.0 28.9 86.7

150 157.8 0.0 356.2

