
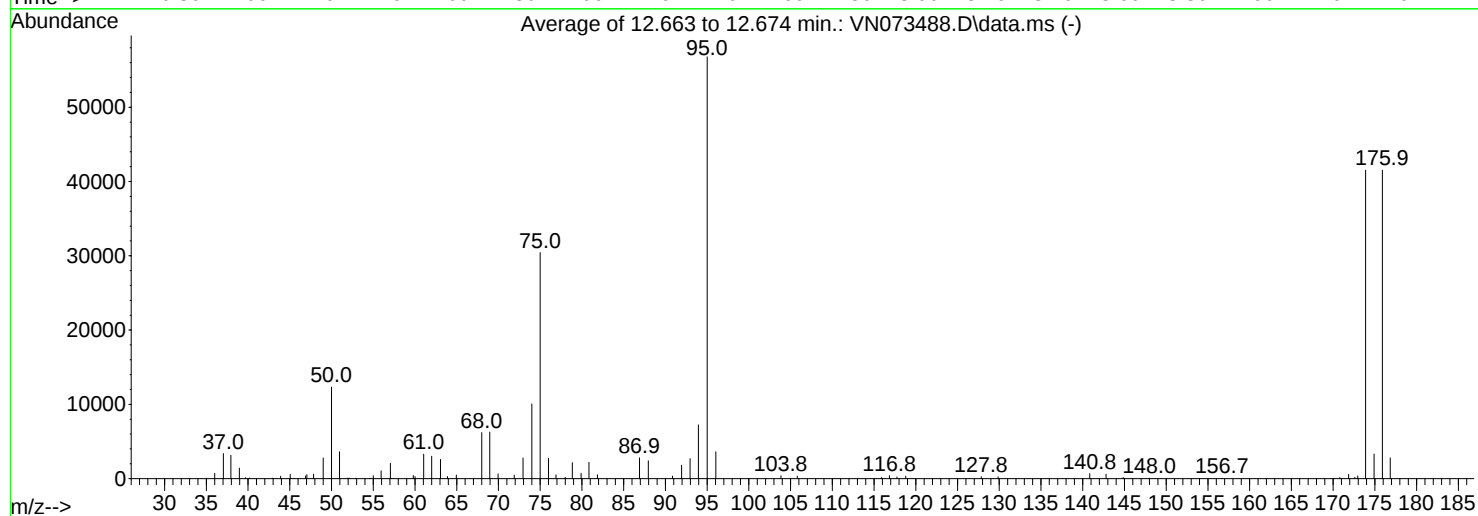


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071822\
 Data File : VN073488.D
 Acq On : 18 Jul 2022 10:08
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
 Title : SW846 8260
 Last Update : Wed Jun 29 01:54:03 2022

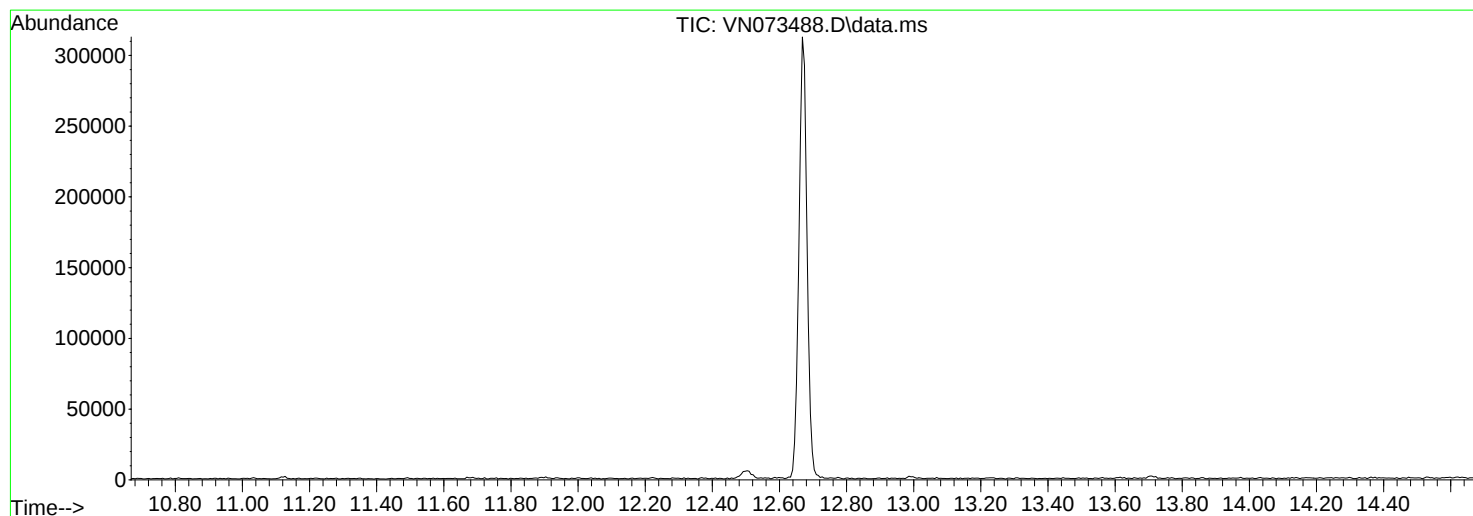

AutoFind: Scans 1832, 1833, 1834; Background Corrected with Scan 1823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	12312	PASS
75	95	30	60	53.6	30437	PASS
95	95	100	100	100.0	56781	PASS
96	95	5	9	6.4	3614	PASS
173	174	0.00	2	0.9	363	PASS
174	95	50	100	73.1	41520	PASS
175	174	5	9	8.0	3326	PASS
176	174	95	101	100.0	41520	PASS
177	176	5	9	6.7	2792	PASS