

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071823\
 Data File : VN078568.D
 Acq On : 18 Jul 2023 18:04
 Operator : JC\MD
 Sample : 03654-02RE
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 72-12016

Quant Time: Jul 19 01:54:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	398284	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	755943	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	719475	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	259253	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	267758	50.147	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 100.300%			
35) Dibromofluoromethane	8.177	113	268517	52.326	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 104.660%			
50) Toluene-d8	10.571	98	894377	46.136	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 92.280%			
62) 4-Bromofluorobenzene	12.853	95	311863	52.228	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery = 104.460%			
Target Compounds						Qvalue
3) Chloromethane	2.365	50	1403	0.264	ug/l #	74
5) Bromomethane	2.971	94	1349	Below Cal		82
6) Chloroethane	3.077	64	683	Below Cal #		59
11) Tert butyl alcohol	5.541	59	177	0.215	ug/l #	72
16) Acetone	4.453	43	67836	40.786	ug/l	96
18) Methyl Acetate	5.036	43	6435	0.914	ug/l #	57
20) Methylene Chloride	5.283	84	18871	2.801	ug/l	91
25) 2-Butanone	7.506	43	42461	16.218	ug/l #	72
29) Tetrahydrofuran	7.859	42	510	0.297	ug/l #	20
31) Cyclohexane	8.235	56	8865	1.229	ug/l #	1
36) 1,1-Dichloropropene	8.230	75	32994	4.453	ug/l #	48
37) Ethyl Acetate	7.571	43	12587	2.038	ug/l #	95
38) Carbon Tetrachloride	8.230	117	43796	5.438	ug/l #	15
42) 1,2-Dichloroethane	8.694	62	2195	0.294	ug/l #	73
43) Isopropyl Acetate	8.700	43	421928	41.491	ug/l #	75
45) 1,2-Dichloropropane	9.753	63	3170	0.570	ug/l #	45
48) Methyl methacrylate	9.676	41	7056	1.498	ug/l #	35
49) 1,4-Dioxane	9.747	88	434	4.224	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	145849	24.112	ug/l	94
53) t-1,3-Dichloropropene	10.729	75	1847	0.230	ug/l #	86
54) cis-1,3-Dichloropropene	10.365	75	107141	12.508	ug/l #	68
57) 1,3-Dichloropropane	11.206	76	12879	1.413	ug/l #	42
58) 2-Chloroethyl Vinyl ether	10.171	63	2372	0.888	ug/l #	87
59) 2-Hexanone	11.176	43	230057	53.515	ug/l #	19
71) Bromoform	12.853	173	2485	0.593	ug/l #	28
75) 1,1,2,2-Tetrachloroethane	12.894	83	156	Below Cal #		26
76) 1,2,3-Trichloropropane	12.853	75	165357	26.388	ug/l #	1
77) Bromobenzene	12.853	156	139	Below Cal #		1
81) trans-1,4-Dichloro-2-b...	12.853	75	165357	69.342	ug/l #	15
90) Hexachloroethane	14.323	117	155	Below Cal #		21


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071823\
Data File : VN078568.D
Acq On : 18 Jul 2023 18:04
Operator : JC\MD
Sample : 03654-02RE
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
72-12016

Quant Time: Jul 19 01:54:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration

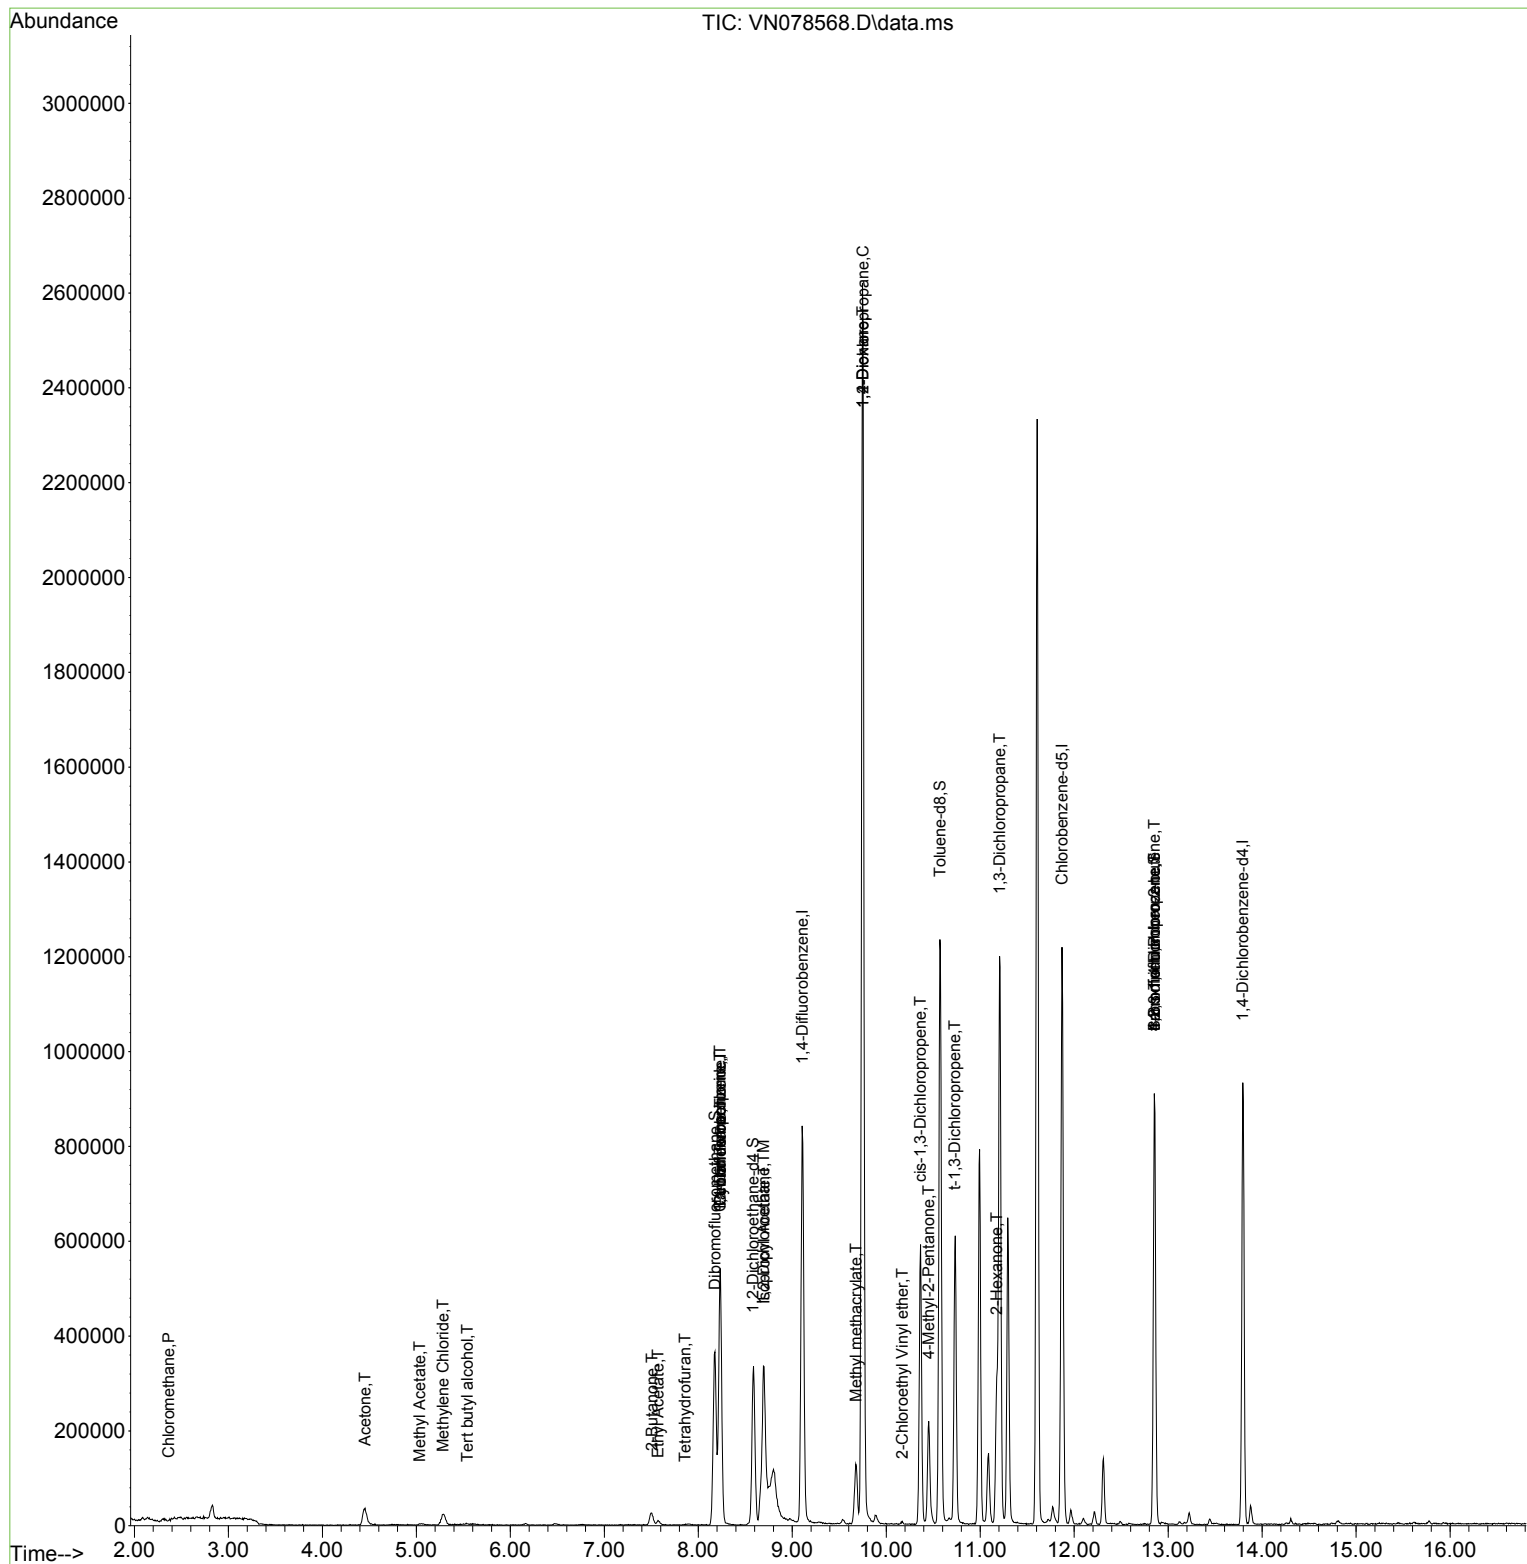

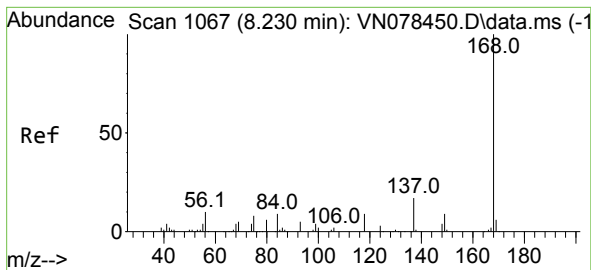

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.235 min Scan# 1

Delta R.T. 0.005 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :





72-12016

Tgt Ion:168 Resp: 398284

Ion Ratio Lower Upper

168 100

99 55.9 53.0 79.6

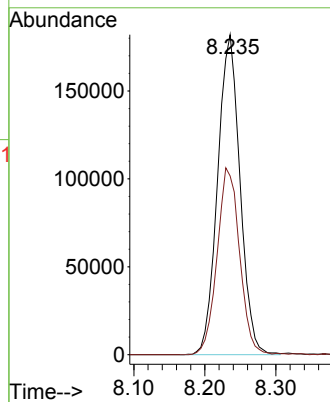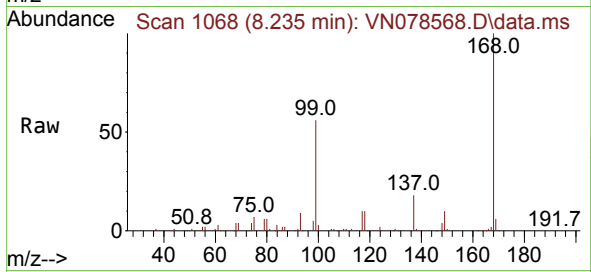

#3

Chloromethane

Concen: 0.264 ug/l

RT: 2.365 min Scan# 70

Delta R.T. -0.006 min

Lab File: VN078568.D




Acq: 18 Jul 2023 18:04


Tgt Ion: 50 Resp: 1403

Ion Ratio Lower Upper

50 100

52 18.5 26.5 39.7#


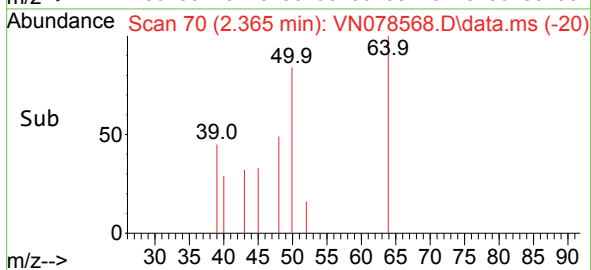
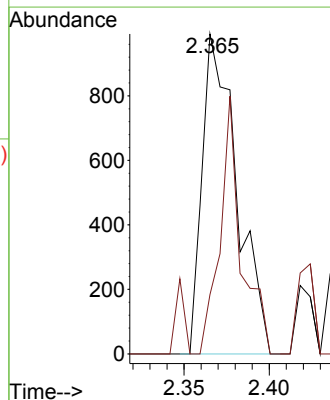





#5
Bromomethane
Concen: Below Cal
RT: 2.971 min Scan# 11
Delta R.T. 0.017 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 94 Resp: 1349
Ion Ratio Lower Upper
94 100
96 74.0 73.1 109.7



#6
Chloroethane
Concen: Below Cal
RT: 3.077 min Scan# 191
Delta R.T. -0.041 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 64 Resp: 683
Ion Ratio Lower Upper
64 100
66 8.7 25.4 38.2#


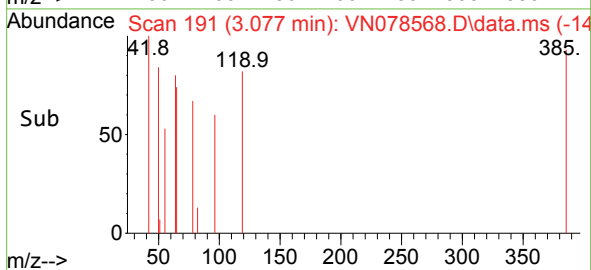






#11
Tert butyl alcohol
Concen: 0.215 ug/l
RT: 5.541 min Scan# 611
Delta R.T. 0.005 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 59 Resp: 177
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#



#16
Acetone
Concen: 40.786 ug/l
RT: 4.453 min Scan# 425
Delta R.T. 0.011 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 43 Resp: 67836
Ion Ratio Lower Upper
43 100
58 32.8 28.0 42.0


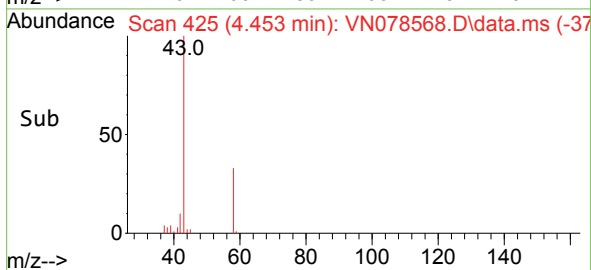






#18
Methyl Acetate
Concen: 0.914 ug/l
RT: 5.036 min Scan# 51
Delta R.T. -0.000 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 43 Resp: 6435
Ion Ratio Lower Upper
43 100
74 8.5 26.2 39.4#



#20
Methylene Chloride
Concen: 2.801 ug/l
RT: 5.283 min Scan# 566
Delta R.T. -0.000 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 84 Resp: 18871
Ion Ratio Lower Upper
84 100
49 94.1 79.7 119.5
51 26.9 25.2 37.8
86 54.4 53.3 79.9


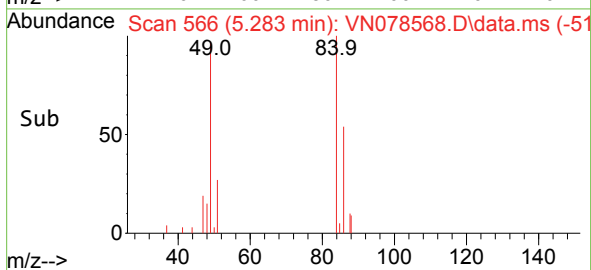






#25
2-Butanone
Concen: 16.218 ug/l
RT: 7.506 min Scan# 941
Delta R.T. 0.017 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 43 Resp: 42461
Ion Ratio Lower Upper
43 100
72 20.9 30.2 45.2#

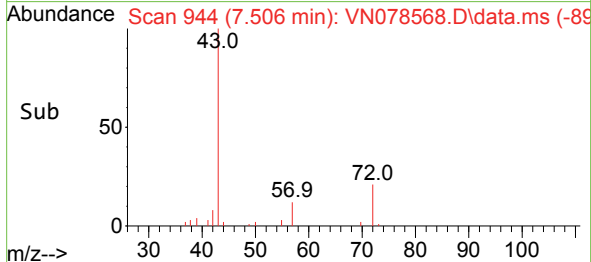

#29
Tetrahydrofuran
Concen: 0.297 ug/l
RT: 7.859 min Scan# 1004
Delta R.T. 0.012 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 42 Resp: 510
Ion Ratio Lower Upper
42 100
72 0.0 49.8 74.6#
71 0.0 47.4 71.2#




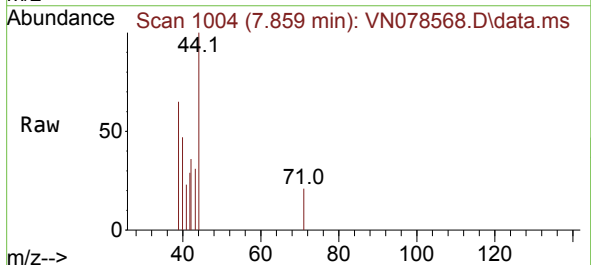




#31
Cyclohexane
Concen: 1.229 ug/l
RT: 8.235 min Scan# 1068
Delta R.T. -0.030 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 56 Resp: 8865
Ion Ratio Lower Upper
56 100
69 179.3 26.8 40.2#
84 151.4 81.8 122.6#



#33
1,2-Dichloroethane-d4
Concen: 50.147 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.001 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 65 Resp: 267758
Ion Ratio Lower Upper
65 100
67 51.1 0.0 106.6





#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

72-12016





Tgt Ion:114 Resp: 755943

Ion Ratio Lower Upper

114 100

63 19.6 0.0 36.4

88 15.0 0.0 30.6



#35

Dibromofluoromethane

Concen: 52.326 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04




Tgt Ion:113 Resp: 268517


Ion Ratio Lower Upper

113 100

111 101.9 82.6 123.8

192 17.4 12.7 19.1



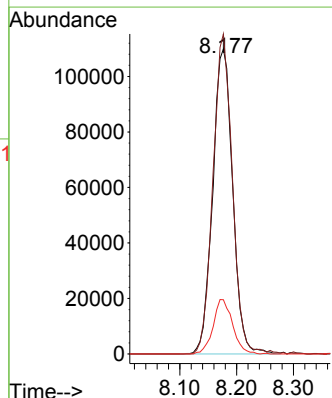





#36
1,1-Dichloropropene
Concen: 4.453 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.147 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 75 Resp: 32994
Ion Ratio Lower Upper
75 100
110 9.4 19.1 57.3#
77 0.0 25.0 37.4#

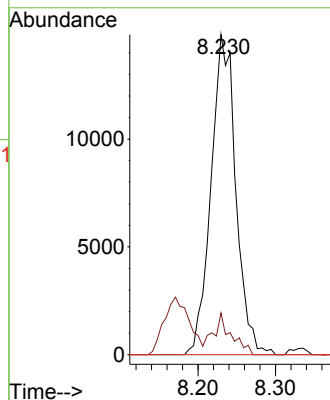

#37
Ethyl Acetate
Concen: 2.038 ug/l
RT: 7.571 min Scan# 955
Delta R.T. -0.000 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 43 Resp: 12587
Ion Ratio Lower Upper
43 100
61 16.8 13.2 19.8
70 10.0 11.3 16.9#

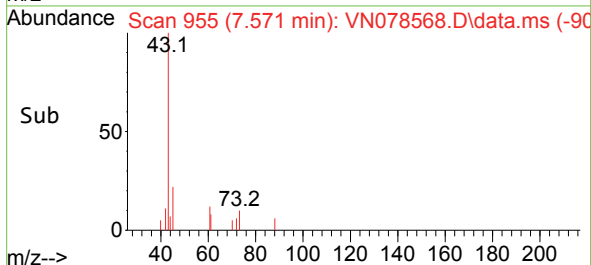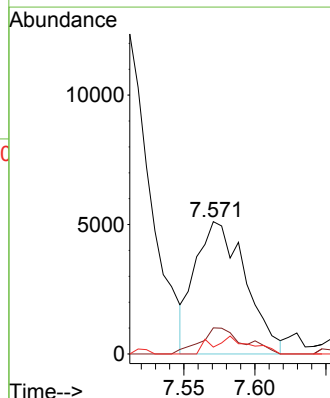

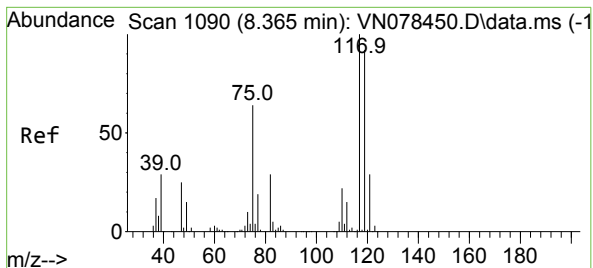

#38

Carbon Tetrachloride

Concen: 5.438 ug/l

RT: 8.230 min Scan# 1067

Delta R.T. -0.135 min

Lab File: VN078568.D


Acq: 18 Jul 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

72-12016

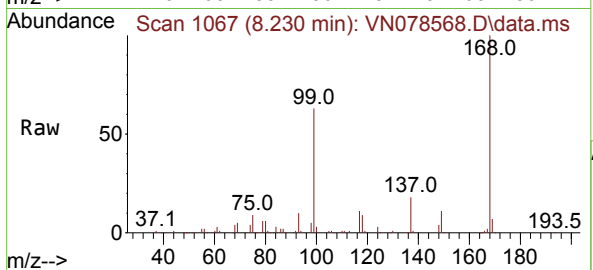




Tgt Ion:117 Resp: 43796

Ion Ratio Lower Upper

117 100

119 4.4 77.3 115.9#

121 0.0 23.3 34.9#

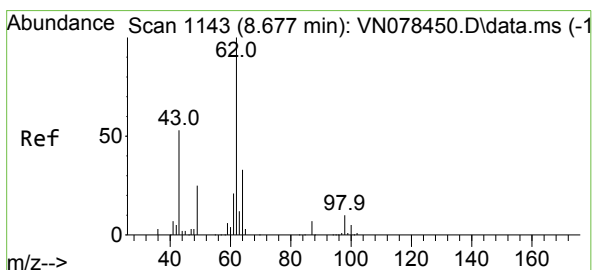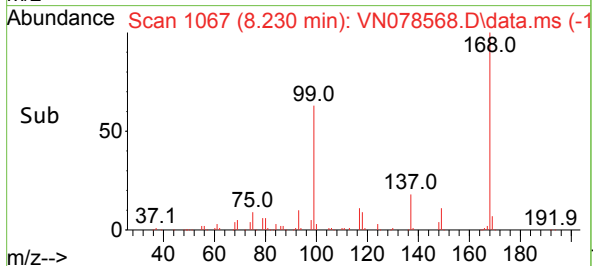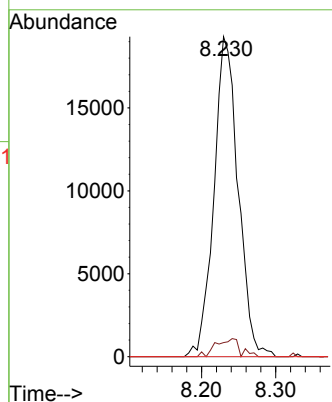

#42

1,2-Dichloroethane

Concen: 0.294 ug/l

RT: 8.694 min Scan# 1146

Delta R.T. 0.017 min

Lab File: VN078568.D




Acq: 18 Jul 2023 18:04


Tgt Ion: 62 Resp: 2195

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8


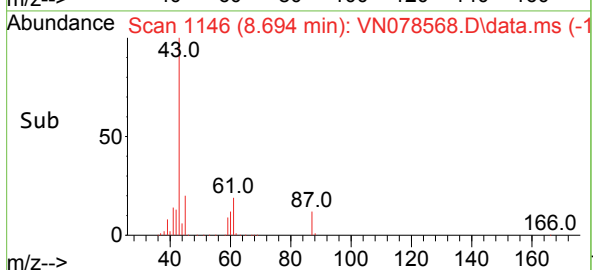

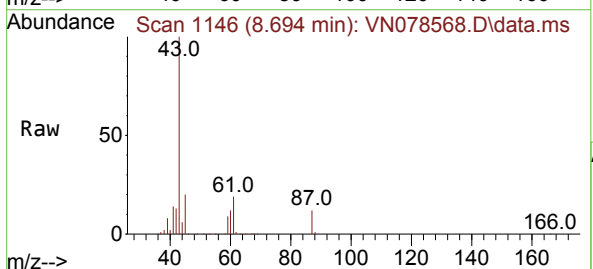




#43
Isopropyl Acetate
Concen: 41.491 ug/l
RT: 8.700 min Scan# 1146
Delta R.T. 0.006 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 43 Resp: 421928
Ion Ratio Lower Upper
43 100
61 14.7 24.7 37.1#
87 9.9 14.6 21.8#

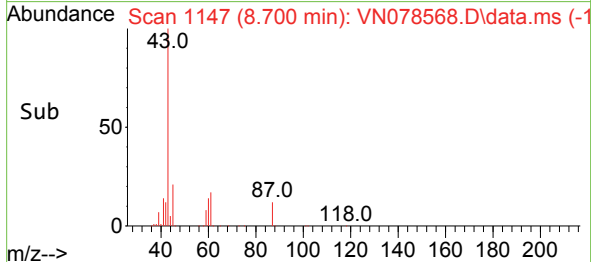

#45
1,2-Dichloropropane
Concen: 0.570 ug/l
RT: 9.753 min Scan# 1326
Delta R.T. 0.123 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 63 Resp: 3170
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#

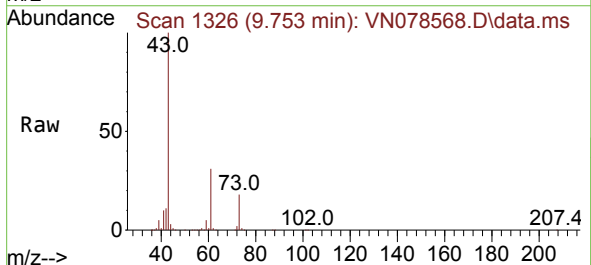



#48

Methyl methacrylate

Concen: 1.498 ug/l

RT: 9.676 min Scan# 1

Delta R.T. -0.012 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

72-12016





Tgt Ion: 41 Resp: 7056

Ion Ratio Lower Upper

41 100

69 0.9 90.4 135.6#

39 67.6 54.6 81.8

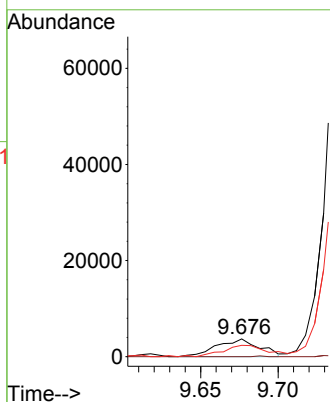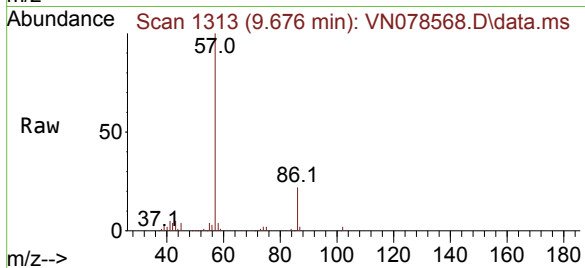

#49

1,4-Dioxane

Concen: 4.224 ug/l

RT: 9.747 min Scan# 1325

Delta R.T. 0.047 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04




Tgt Ion: 88 Resp: 434


Ion Ratio Lower Upper

88 100

43 558965.9 17.0 25.6#

58 3087.6 47.0 70.4#



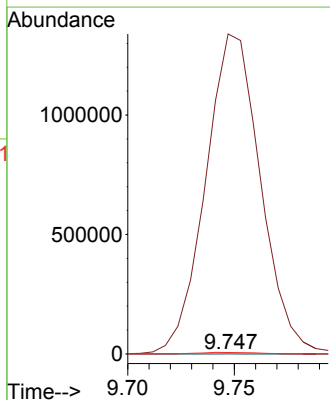
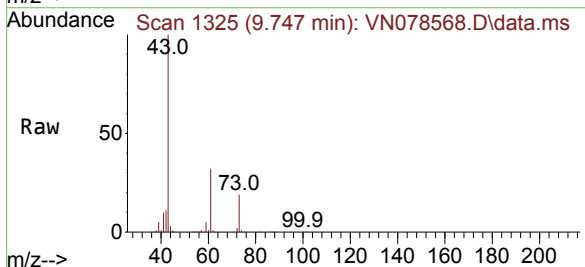




#50
Toluene-d8
Concen: 46.136 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 98 Resp: 894377
Ion Ratio Lower Upper
98 100
100 63.1 52.0 78.0

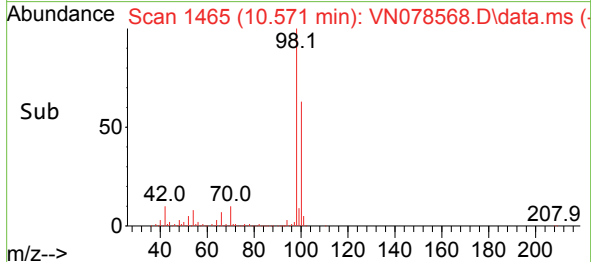

#51
4-Methyl-2-Pentanone
Concen: 24.112 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 43 Resp: 145849
Ion Ratio Lower Upper
43 100
58 41.9 36.6 54.8




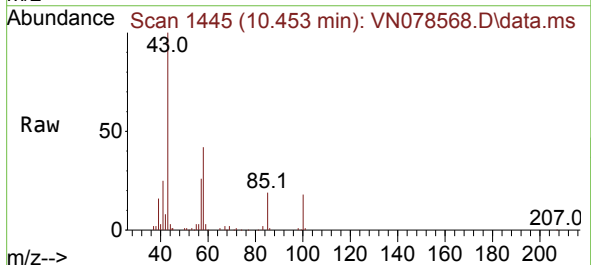


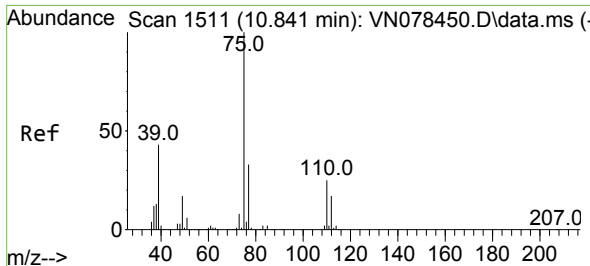

#53
 t-1,3-Dichloropropene
 Concen: 0.230 ug/l
 RT: 10.729 min Scan# 141
 Delta R.T. -0.112 min
 Lab File: VN078568.D
 Acq: 18 Jul 2023 18:04




Instrument :
 MSVOA_N
 ClientSampleId :
 72-12016


Tgt Ion: 75 Resp: 1847
 Ion Ratio Lower Upper
 75 100
 77 24.0 25.4 38.0#

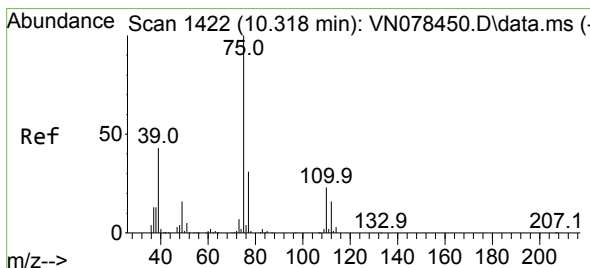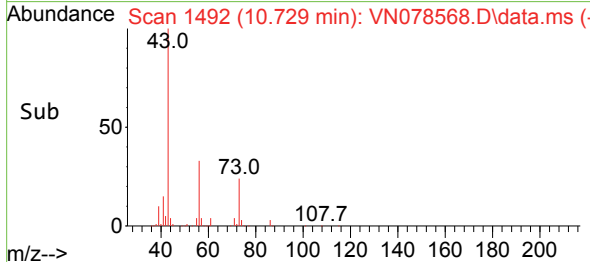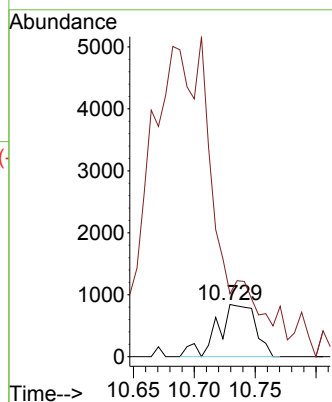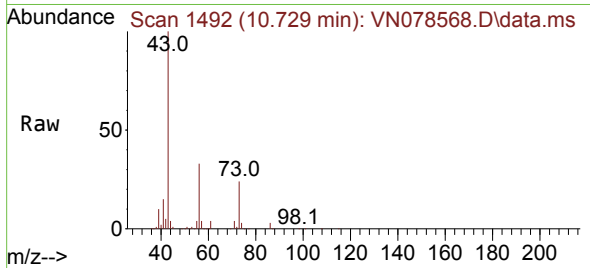

#54
 cis-1,3-Dichloropropene
 Concen: 12.508 ug/l
 RT: 10.365 min Scan# 1430
 Delta R.T. 0.047 min
 Lab File: VN078568.D
 Acq: 18 Jul 2023 18:04

Tgt Ion: 75 Resp: 107141
 Ion Ratio Lower Upper
 75 100
 77 0.7 26.1 39.1#
 39 32.4 31.6 47.4


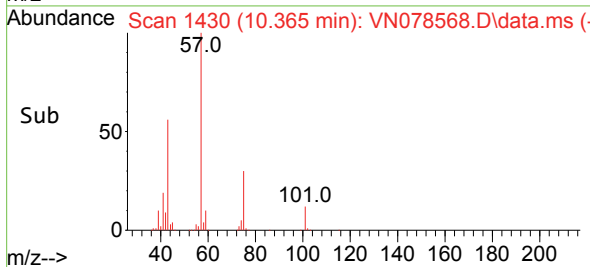

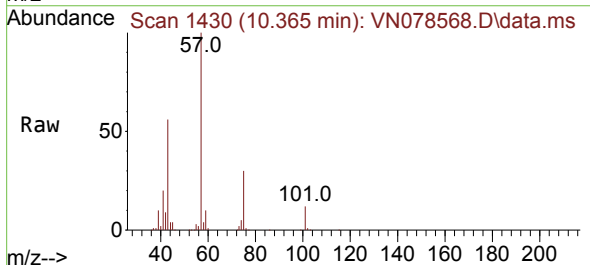


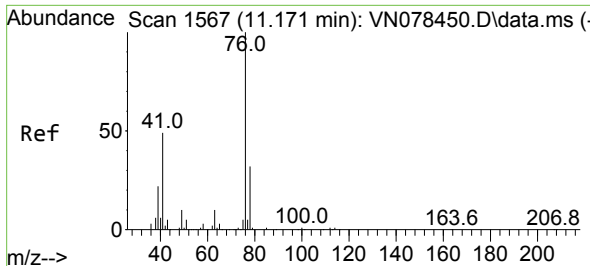

#57
1,3-Dichloropropane
Concen: 1.413 ug/l
RT: 11.206 min Scan# 11
Delta R.T. 0.035 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 76 Resp: 12879
Ion Ratio Lower Upper
76 100
78 0.0 26.1 39.1#

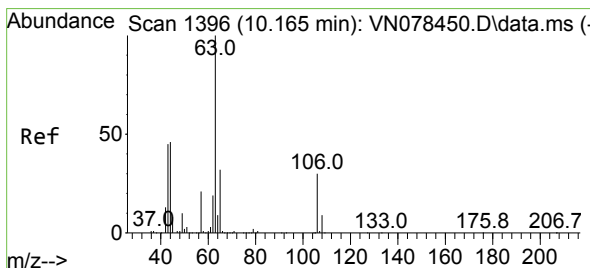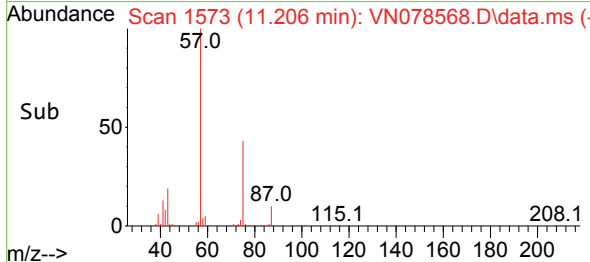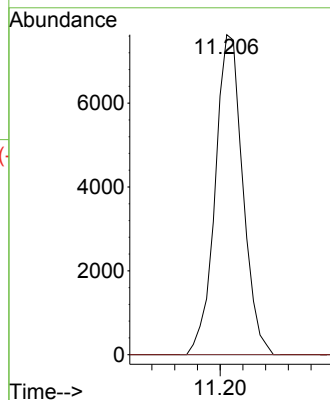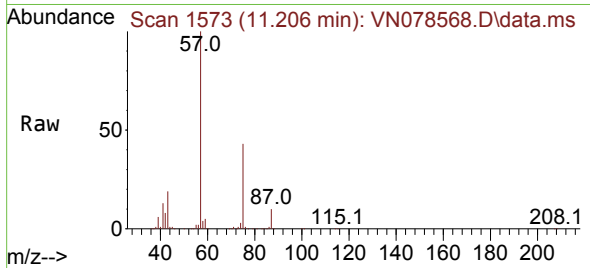

#58
2-Chloroethyl Vinyl ether
Concen: 0.888 ug/l
RT: 10.171 min Scan# 1397
Delta R.T. 0.006 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 63 Resp: 2372
Ion Ratio Lower Upper
63 100
106 25.2 26.2 39.4#


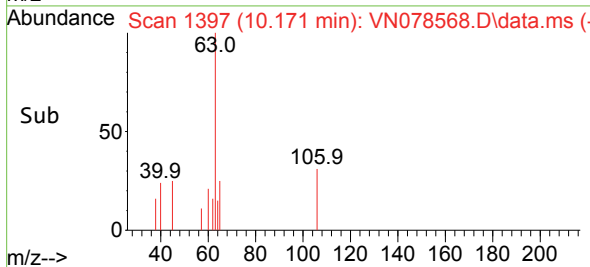
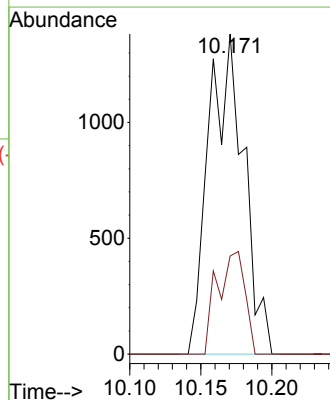
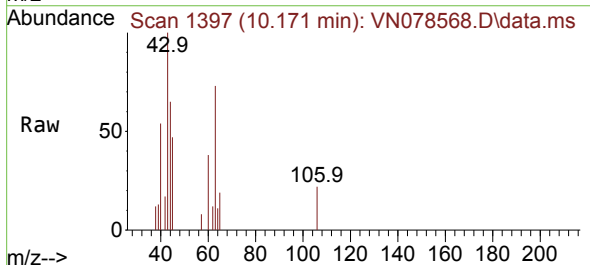




#59
2-Hexanone
Concen: 53.515 ug/l
RT: 11.176 min Scan# 11176
Delta R.T. -0.024 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 43 Resp: 230057
Ion Ratio Lower Upper
43 100
58 0.0 31.7 95.1#

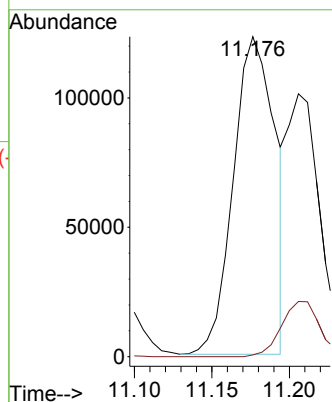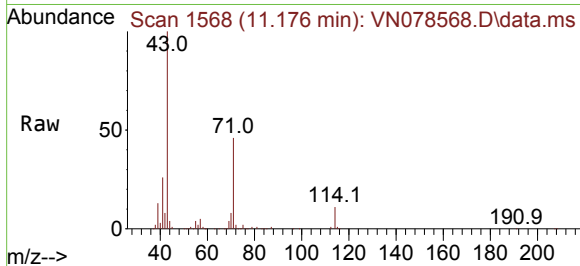

#62
4-Bromofluorobenzene
Concen: 52.228 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 95 Resp: 311863
Ion Ratio Lower Upper
95 100
174 79.2 0.0 143.8
176 76.8 0.0 135.8

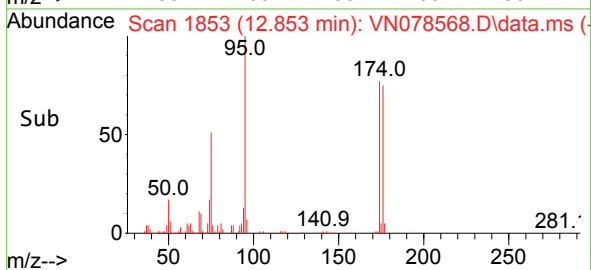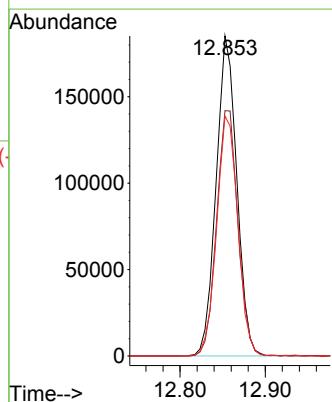

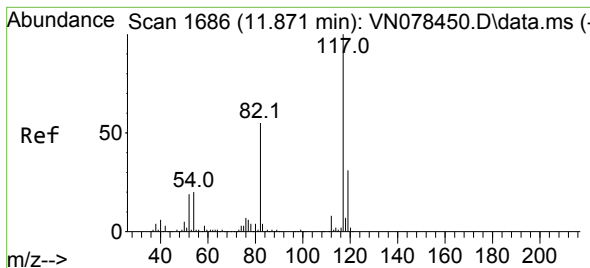

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.870 min Scan# 1

Delta R.T. -0.001 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

72-12016





Tgt Ion:117 Resp: 719475

Ion Ratio Lower Upper

117 100

82 55.7 44.0 66.0

119 31.5 25.6 38.4

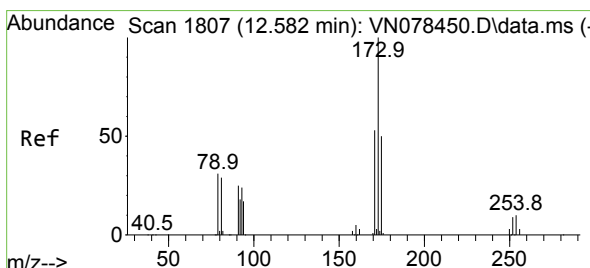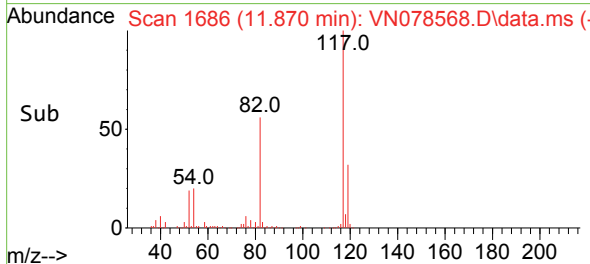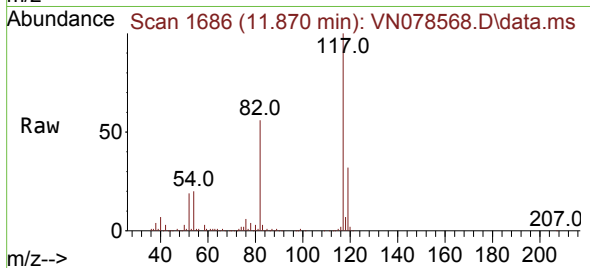

#71

Bromoform

Concen: 0.593 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.271 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04




Tgt Ion:173 Resp: 2485


Ion Ratio Lower Upper

173 100

175 0.0 24.3 73.0#

254 0.0 0.0 0.0

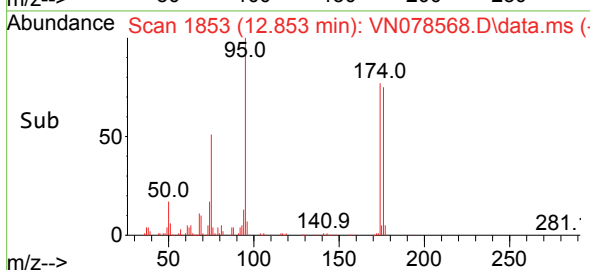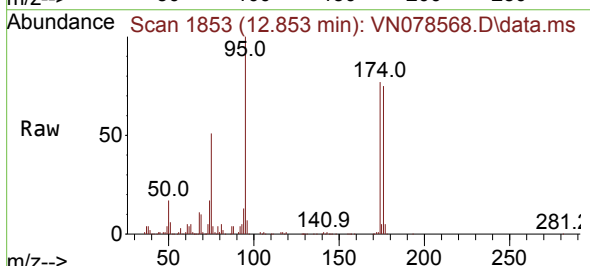

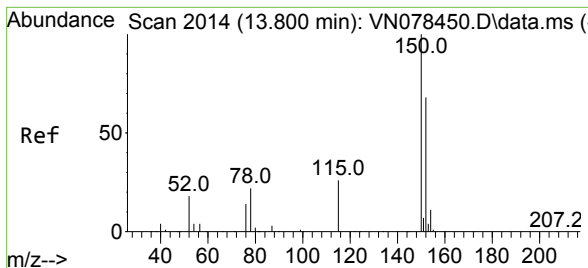

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 20

Delta R.T. -0.006 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04

Instrument :

MSVOA_N

ClientSampleId :

72-12016





Tgt Ion:152 Resp: 259253

Ion Ratio Lower Upper

152 100

115 59.0 32.3 96.8

150 156.4 0.0 355.8

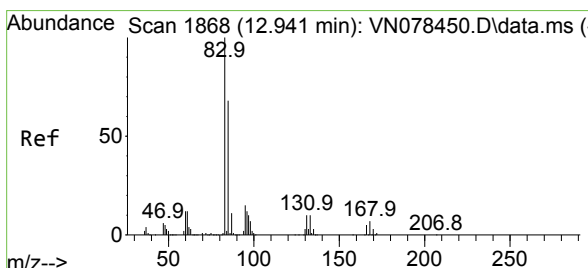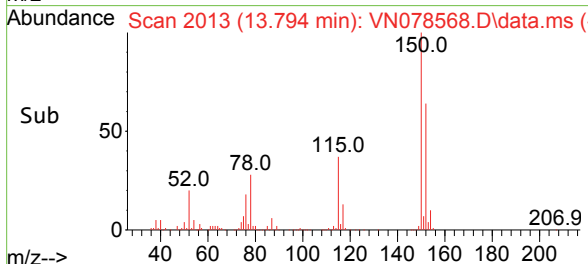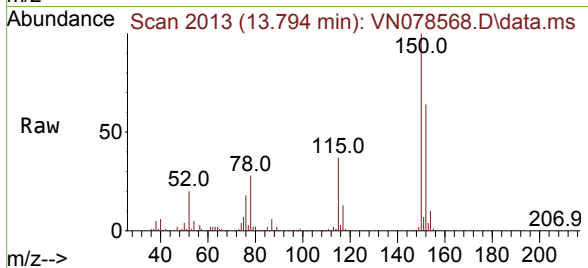

#75

1,1,2,2-Tetrachloroethane

Concen: Below Cal

RT: 12.894 min Scan# 1860

Delta R.T. -0.047 min

Lab File: VN078568.D

Acq: 18 Jul 2023 18:04




Tgt Ion: 83 Resp: 156


Ion Ratio Lower Upper

83 100

131 0.0 5.0 15.0#

85 0.0 31.9 95.7#


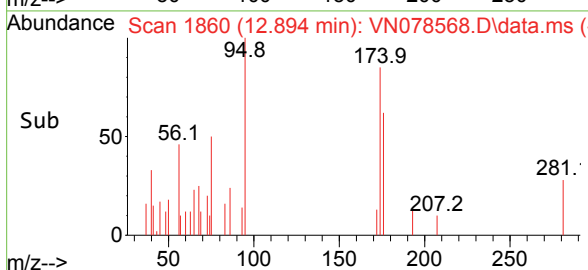

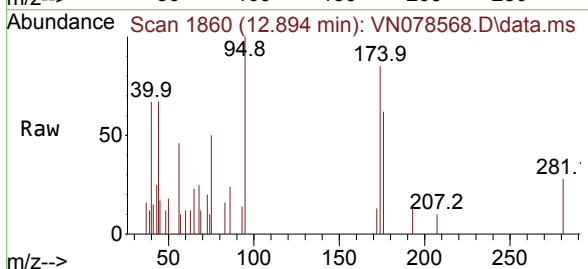




#76
1,2,3-Trichloropropane
Concen: 26.388 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04




Instrument :
MSVOA_N
ClientSampleId :
72-12016


Tgt Ion: 75 Resp: 165357
Ion Ratio Lower Upper
75 100
77 1.4 84.5 253.5#

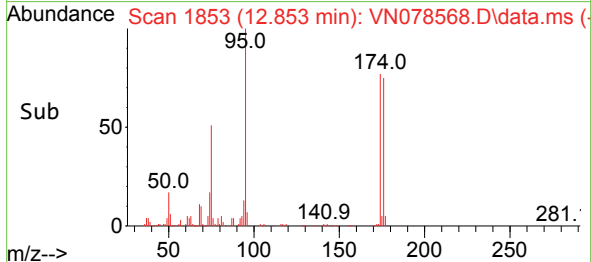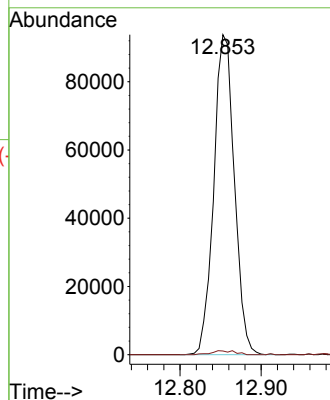

#77
Bromobenzene
Concen: Below Cal
RT: 12.853 min Scan# 1853
Delta R.T. -0.135 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion:156 Resp: 139
Ion Ratio Lower Upper
156 100
77 1671.2 107.7 323.3#
158 0.0 48.4 145.3#



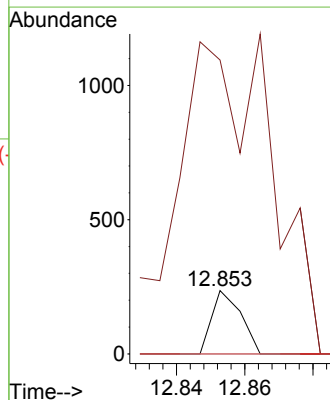
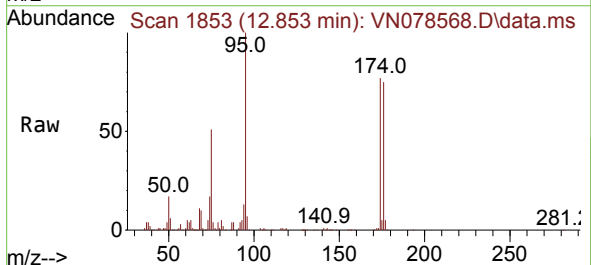


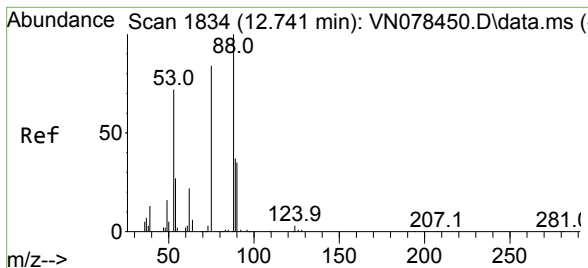

#81
trans-1,4-Dichloro-2-butene
Concen: 69.342 ug/l
RT: 12.853 min Scan# 11
Delta R.T. 0.112 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Instrument :
MSVOA_N
ClientSampleId :
72-12016

Tgt Ion: 75 Resp: 165357
Ion Ratio Lower Upper
75 100
53 0.3 67.4 101.2#
89 0.0 38.8 58.2#

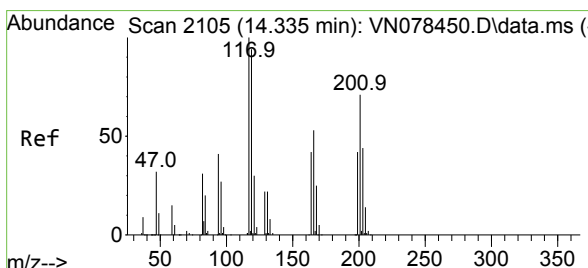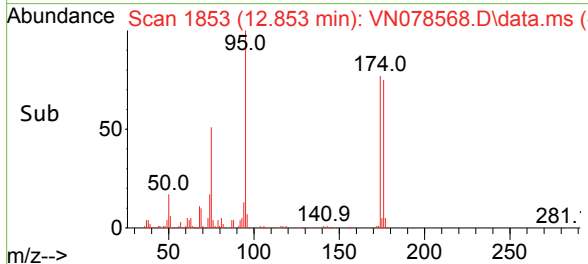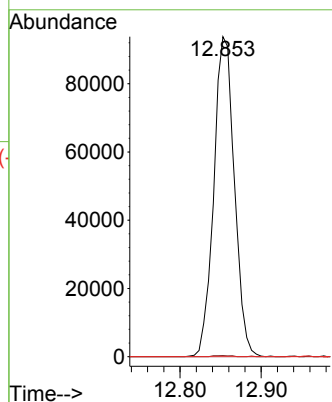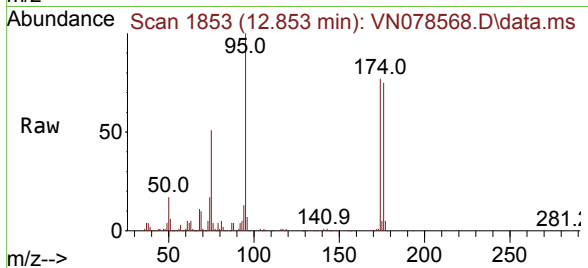

#90
Hexachloroethane
Concen: Below Cal
RT: 14.323 min Scan# 2103
Delta R.T. -0.012 min
Lab File: VN078568.D
Acq: 18 Jul 2023 18:04

Tgt Ion: 117 Resp: 155
Ion Ratio Lower Upper
117 100
201 0.0 29.3 88.0#

