

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071823\
 Data File : VN078551.D
 Acq On : 18 Jul 2023 11:03
 Operator : JC\MD
 Sample : VN0718MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0718MBL01

Quant Time: Jul 19 01:44:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.229	168	406941	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	714817	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	641541	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	220434	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	258263	47.340	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	94.680%
35) Dibromofluoromethane	8.177	113	270537	55.753	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	111.500%
50) Toluene-d8	10.570	98	818157	44.633	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	89.260%
62) 4-Bromofluorobenzene	12.853	95	276153	48.909	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.820%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071823\
Data File : VN078551.D
Acq On : 18 Jul 2023 11:03
Operator : JC\MD
Sample : VN0718MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0718MBL01

Quant Time: Jul 19 01:44:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration




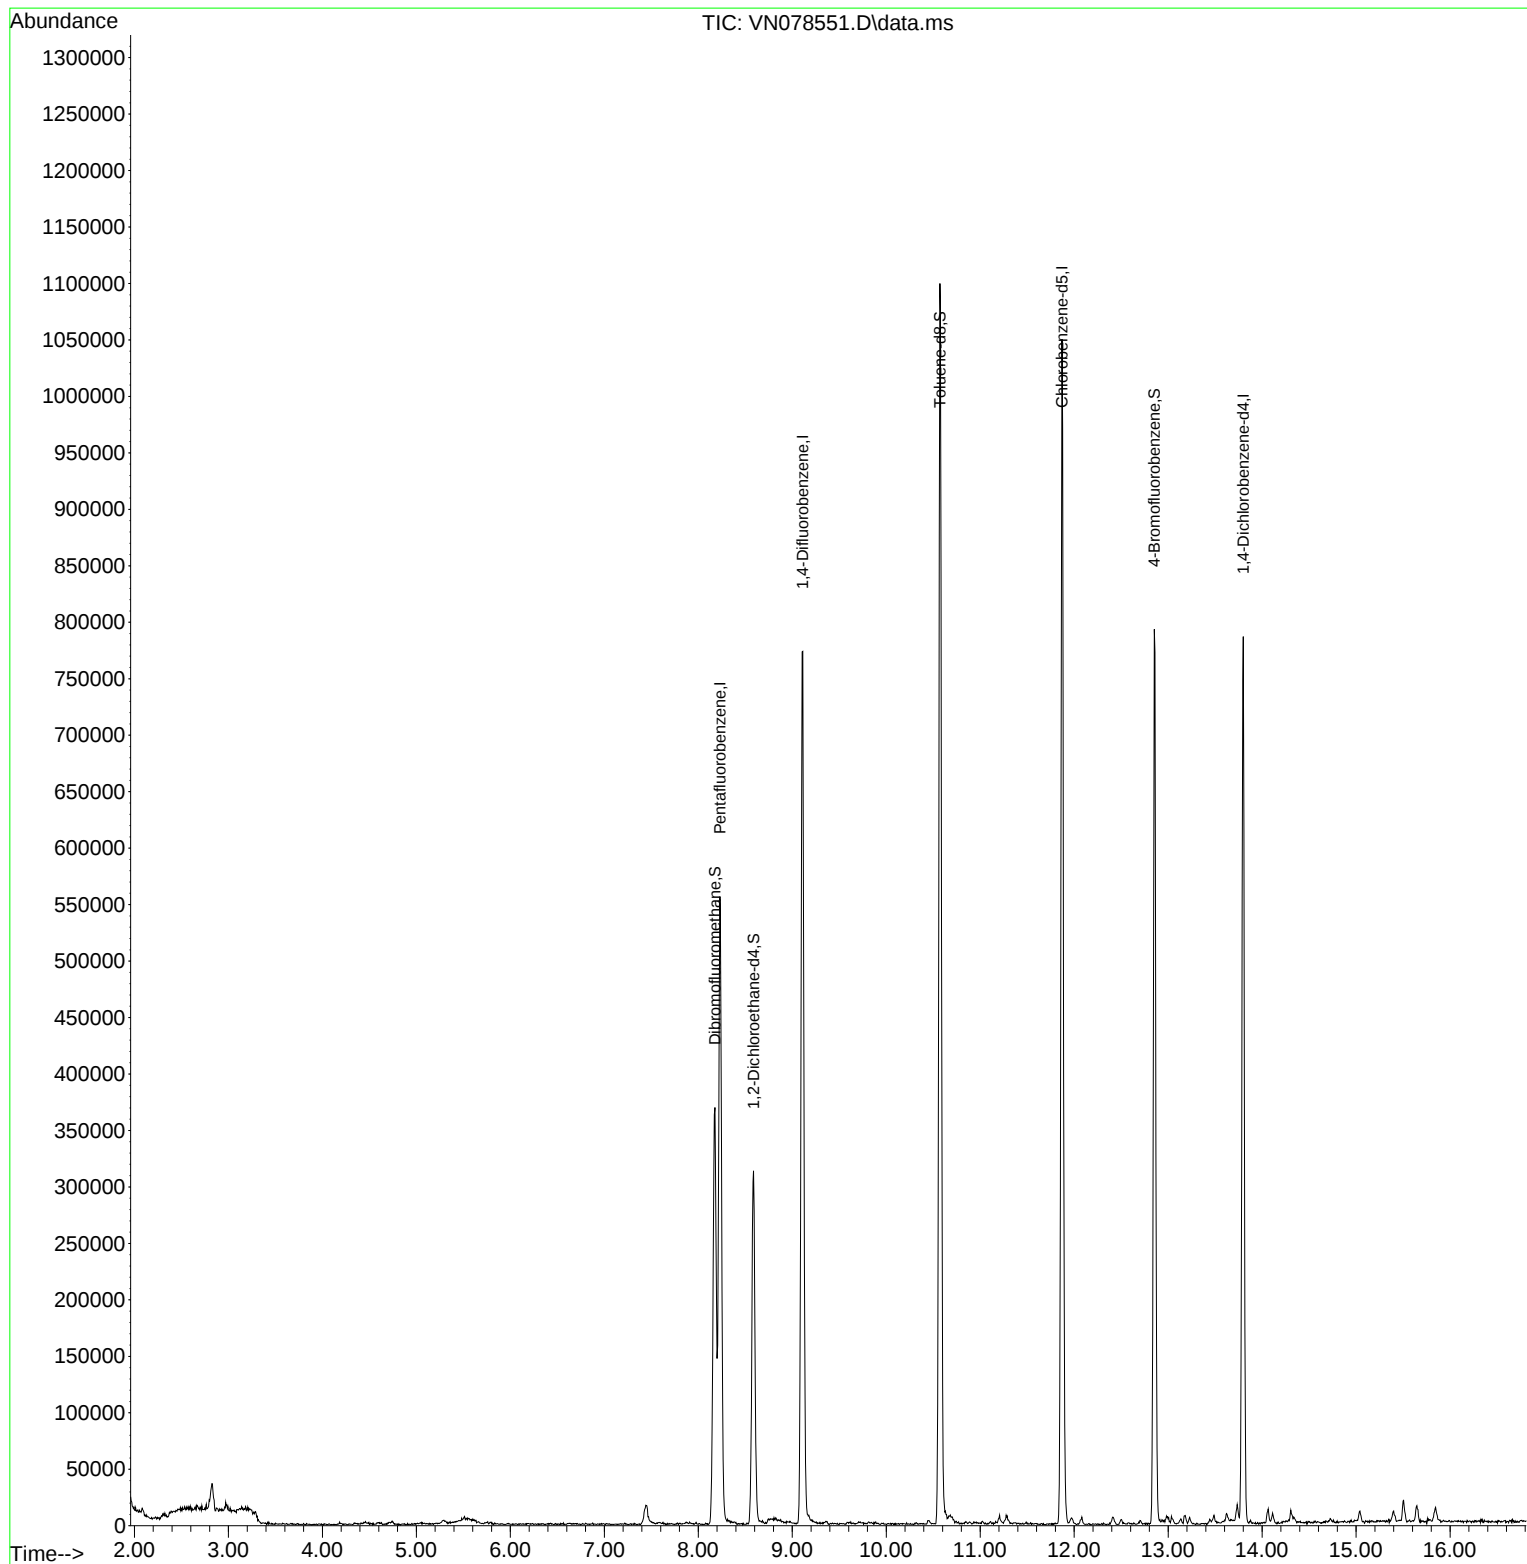


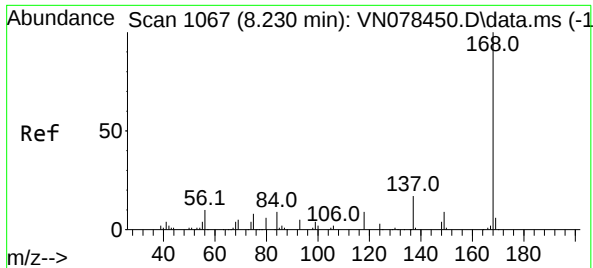

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.001 min
Lab File: VN078551.D
Acq: 18 Jul 2023 11:03




Instrument :
MSVOA_N
ClientSampleId :
VN0718MBL01


Tgt Ion:168 Resp: 406941
Ion Ratio Lower Upper
168 100
99 60.5 53.0 79.6

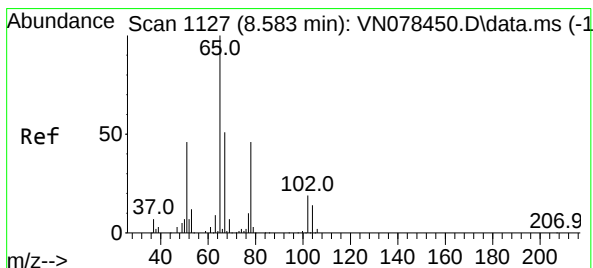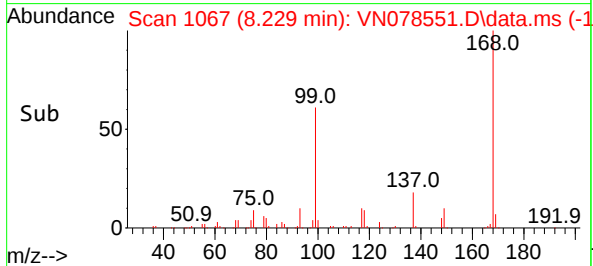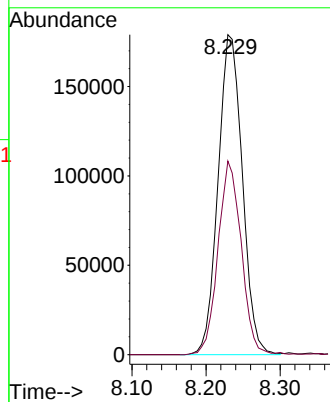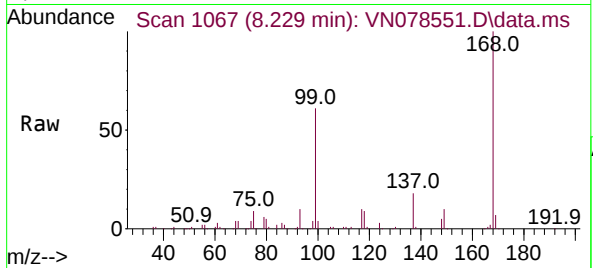

#33
1,2-Dichloroethane-d4
Concen: 47.340 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.005 min
Lab File: VN078551.D
Acq: 18 Jul 2023 11:03

Tgt Ion: 65 Resp: 258263
Ion Ratio Lower Upper
65 100
67 53.8 0.0 106.6

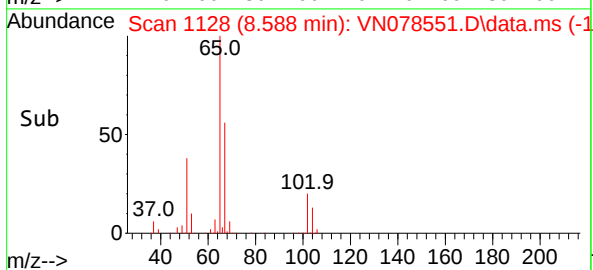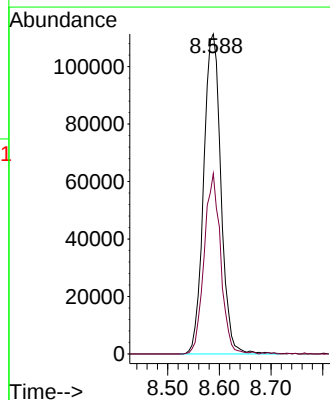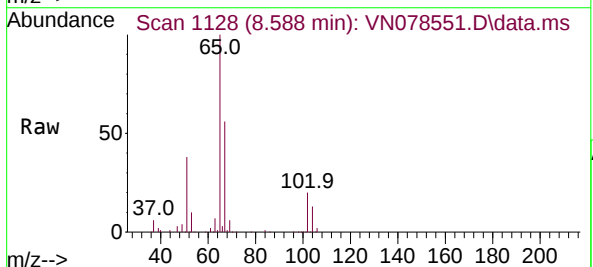

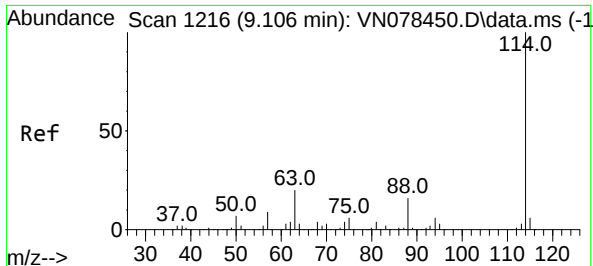

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN078551.D

Acq: 18 Jul 2023 11:03

Instrument :

MSVOA_N

ClientSampleId :

VN0718MBL01





Tgt Ion:114 Resp: 714817

Ion Ratio Lower Upper

114 100

63 17.4 0.0 36.4

88 13.5 0.0 30.6

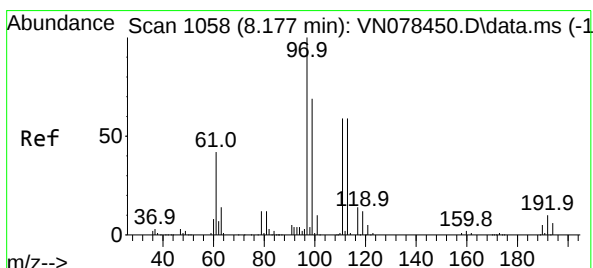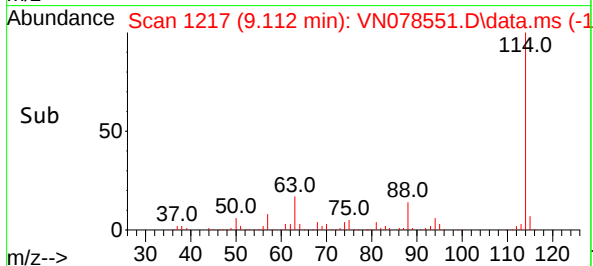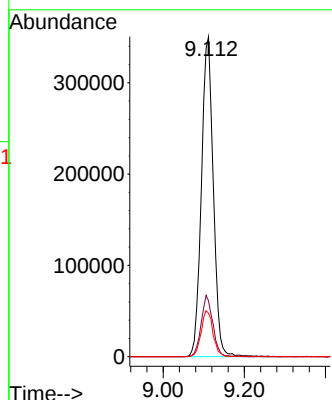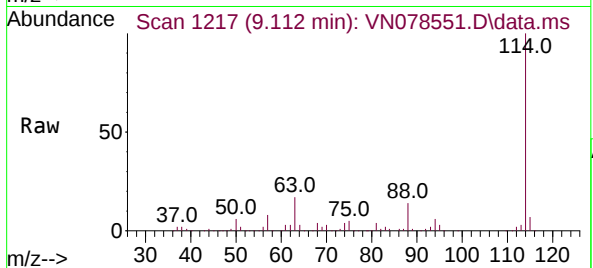

#35

Dibromofluoromethane

Concen: 55.753 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078551.D

Acq: 18 Jul 2023 11:03




Tgt Ion:113 Resp: 270537


Ion Ratio Lower Upper

113 100

111 104.1 82.6 123.8

192 18.2 12.7 19.1


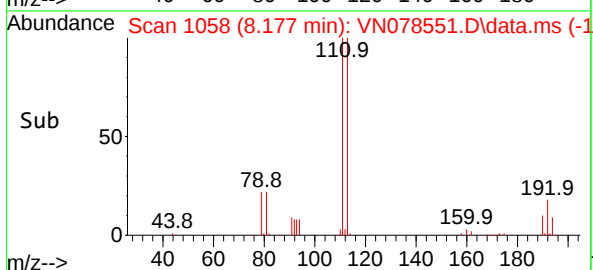
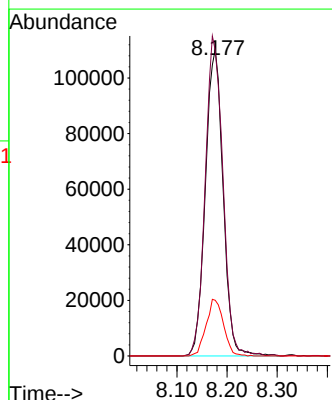
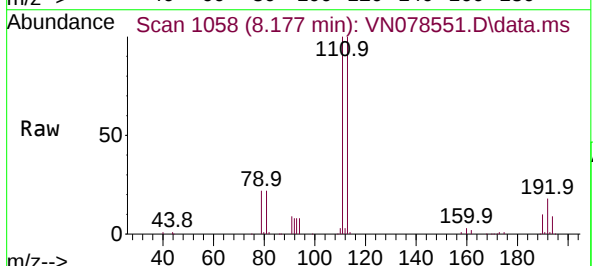


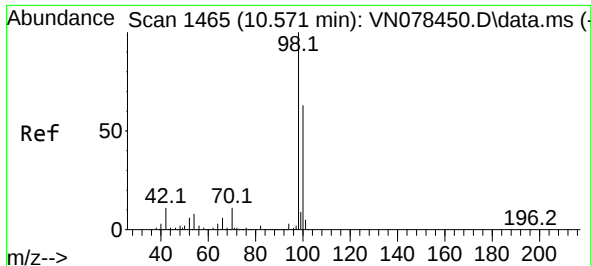

#50
Toluene-d8
Concen: 44.633 ug/l
RT: 10.570 min Scan# 1465
Delta R.T. -0.001 min
Lab File: VN078551.D
Acq: 18 Jul 2023 11:03




Instrument :
MSVOA_N
ClientSampleId :
VN0718MBL01


Tgt Ion: 98 Resp: 818157
Ion Ratio Lower Upper
98 100
100 62.5 52.0 78.0

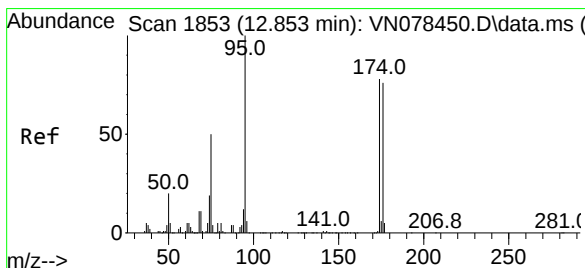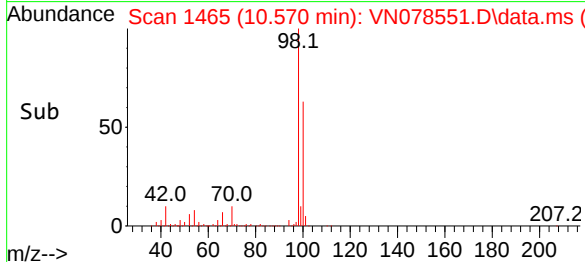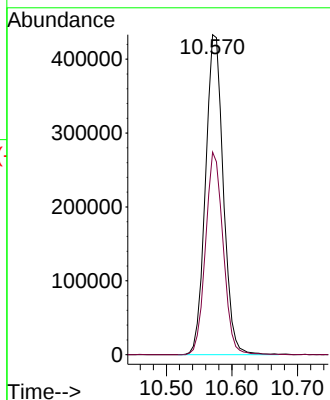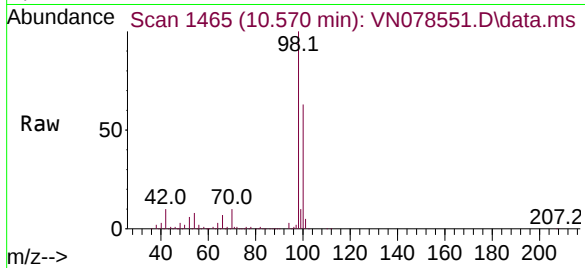

#62
4-Bromofluorobenzene
Concen: 48.909 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078551.D
Acq: 18 Jul 2023 11:03

Tgt Ion: 95 Resp: 276153
Ion Ratio Lower Upper
95 100
174 81.8 0.0 143.8
176 78.5 0.0 135.8


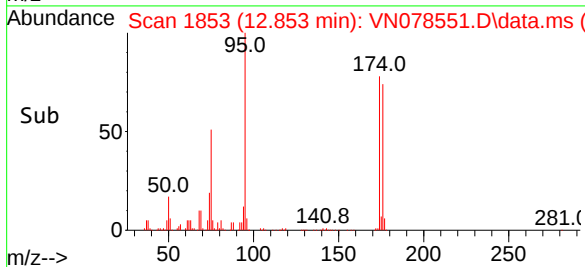
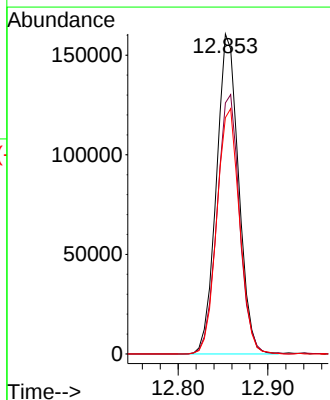
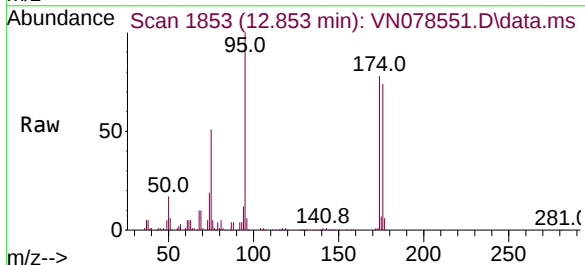


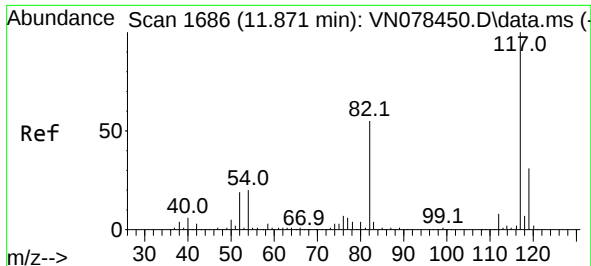

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.870 min Scan# 11
Delta R.T. -0.001 min
Lab File: VN078551.D
Acq: 18 Jul 2023 11:03

Instrument :
MSVOA_N
ClientSampleId :
VN0718MBL01

Tgt Ion:117 Resp: 641541
Ion Ratio Lower Upper
117 100
82 55.5 44.0 66.0
119 32.3 25.6 38.4

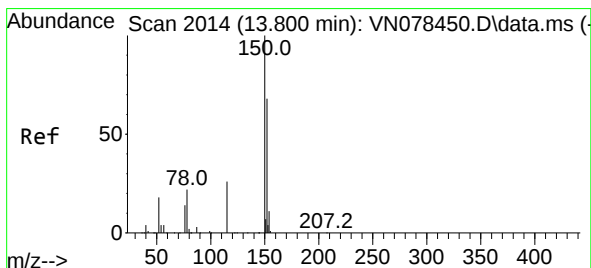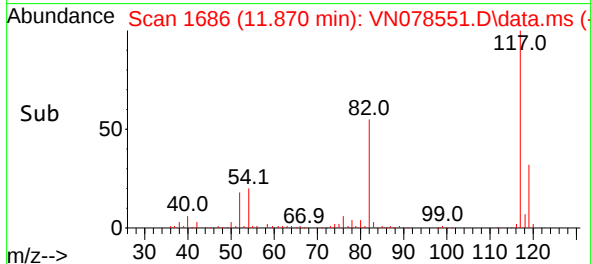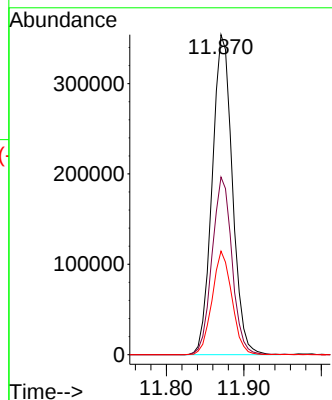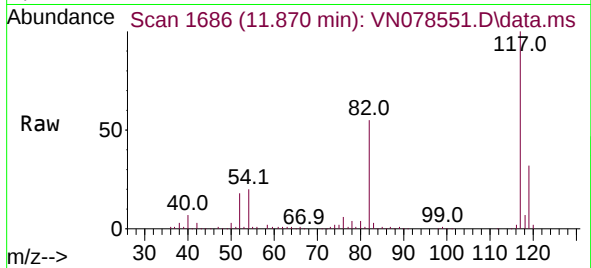

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.800 min Scan# 2014
Delta R.T. -0.000 min
Lab File: VN078551.D
Acq: 18 Jul 2023 11:03

Tgt Ion:152 Resp: 220434
Ion Ratio Lower Upper
152 100
115 61.3 32.3 96.8
150 158.7 0.0 355.8

