
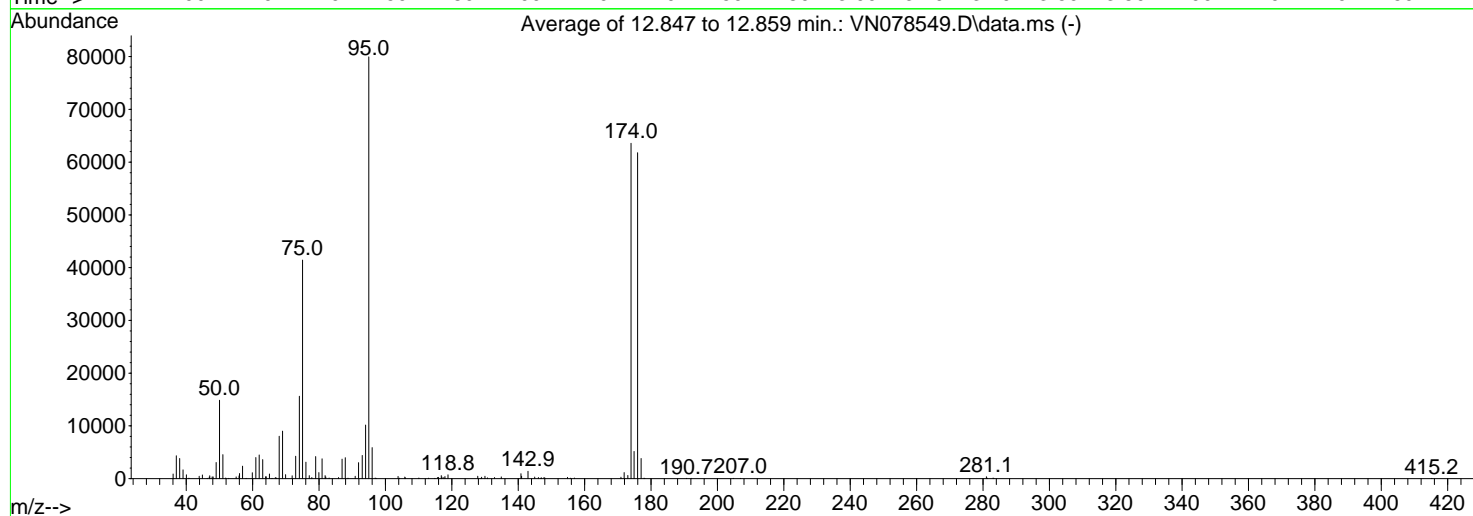


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071823\
 Data File : VN078549.D
 Acq On : 18 Jul 2023 09:55
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Title : SW846 8260
 Last Update : Mon Jul 10 16:13:53 2023

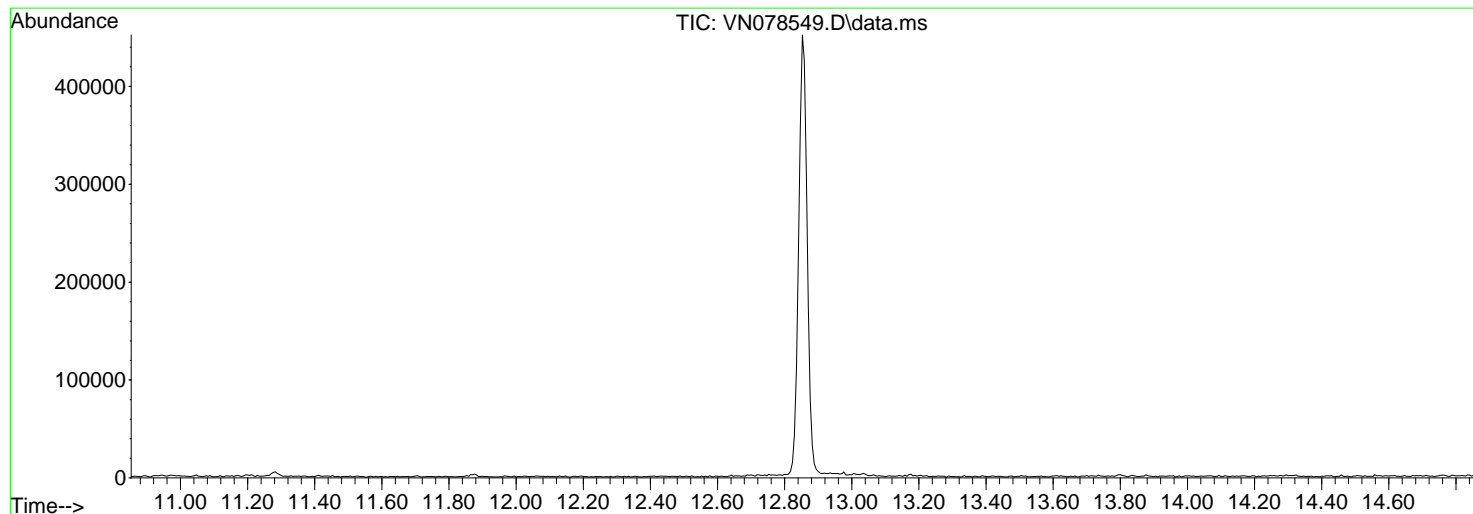

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result
50	95	15	40	18.6	14875	PASS
75	95	30	60	51.8	41448	PASS
95	95	100	100	100.0	79960	PASS
96	95	5	9	7.4	5897	PASS
173	174	0.00	2	0.9	601	PASS
174	95	50	100	79.5	63581	PASS
175	174	5	9	8.1	5145	PASS
176	174	95	101	97.2	61792	PASS
177	176	5	9	6.2	3831	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	888	47.80	326	58.00	60	68.00	805
37.00	4355	48.10	340	59.90	1117	69.00	900
38.00	3837	49.00	3076	60.95	4002	69.90	75
39.00	1666	50.00	14875	61.95	4487	71.90	56
40.05	731	51.00	4565	63.00	3623	72.95	4242
40.80	80	51.90	114	63.90	359	74.05	15633
43.90	455	52.80	69	64.10	379	75.00	41448
44.85	689	55.00	320	65.05	891	76.05	3117
46.30	53	55.90	508	65.80	50	77.05	569
46.90	310	56.05	966	66.85	205	77.80	200
47.05	544	56.95	2380	67.20	131	78.95	4200

Average of 12.847 to 12.859 min.: VN078549.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	1163	93.00	4398	113.00	81	128.95	280
80.90	3775	94.00	10171	114.90	69	129.95	448
81.80	579	95.00	79960	115.65	217	130.75	159
82.00	341	96.00	5897	116.00	236	132.85	211
83.00	120	96.90	121	116.80	564	134.90	331
85.85	215	97.20	74	117.00	293	140.80	930
86.95	3711	103.80	442	117.60	222	141.00	455
87.90	3971	104.20	80	117.90	407	142.95	1405
88.70	100	105.80	306	118.85	720	144.95	313
90.90	458	106.00	158	127.80	452	146.05	209
91.90	3036	110.05	135	128.70	75	146.80	74

Average of 12.847 to 12.859 min.: VN078549.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
146.95	182	175.95	61792	283.30	66		
147.75	200	177.00	3831	415.20	60		
148.00	143	177.90	89				
154.85	253	178.10	52				
155.70	82	190.70	50				
156.90	133	192.10	51				
170.95	268	204.80	62				
171.90	1141	207.00	67				
173.00	601	281.05	361				
174.00	63581	281.30	92				
174.90	5145	283.05	112				

Instrument :

MSVOA_N

ClientSampleId :

BFB