
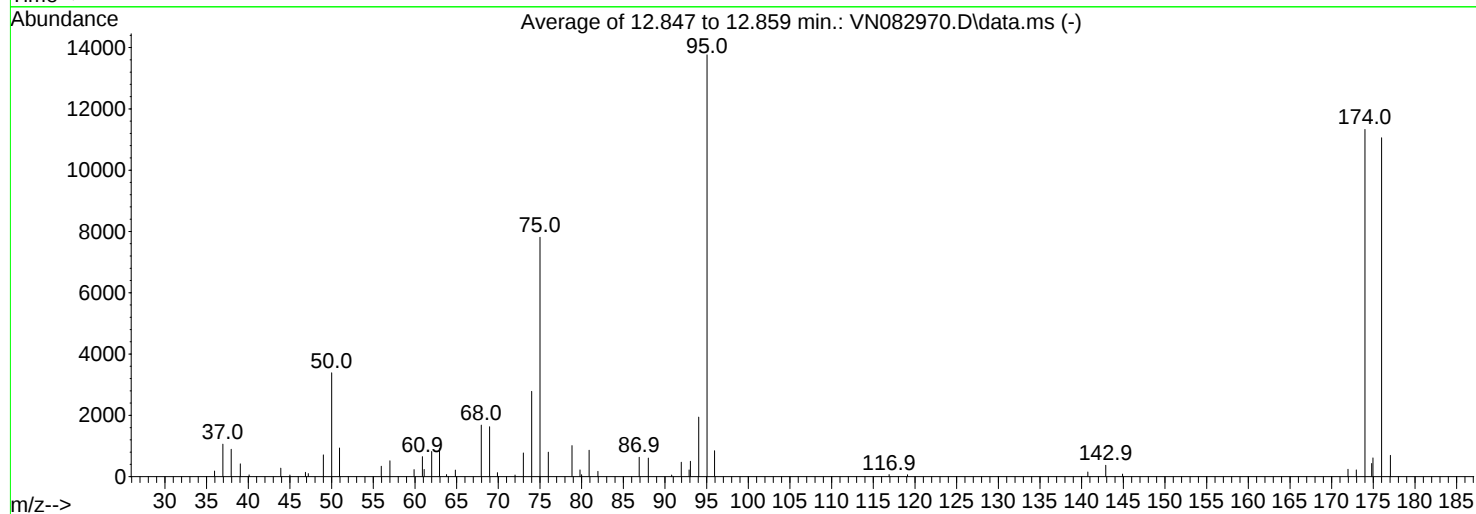


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071824\
Data File : VN082970.D
Acq On : 18 Jul 2024 11:40
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

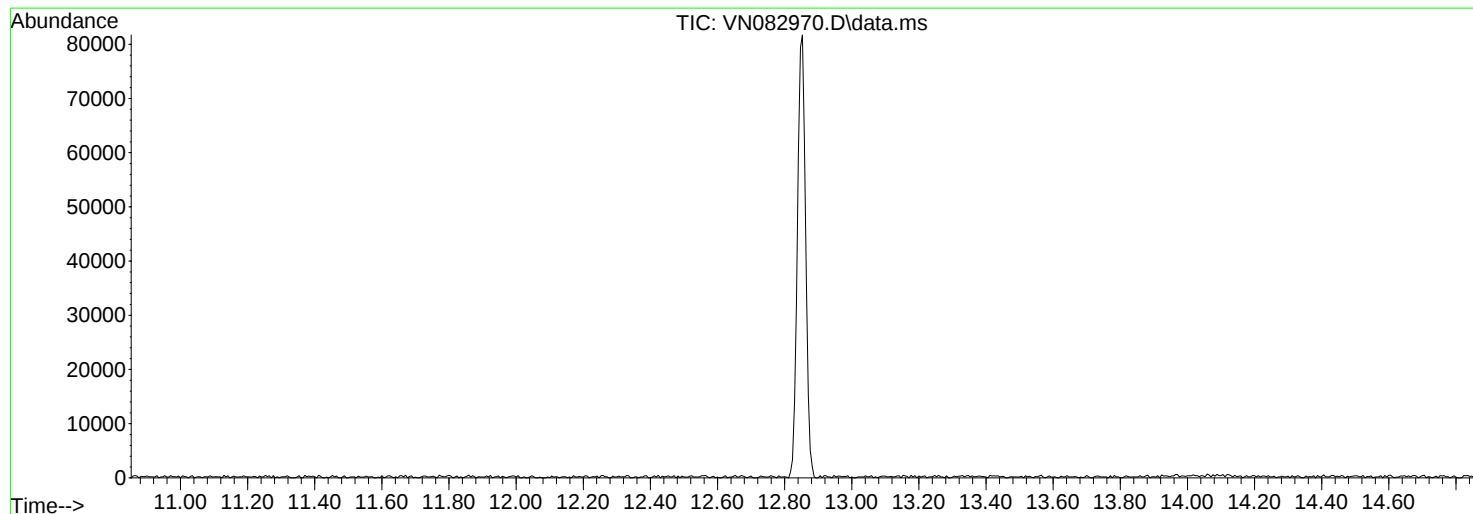

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	3386	PASS
75	95	30	60	56.8	7812	PASS
95	95	100	100	100.0	13763	PASS
96	95	5	9	6.1	845	PASS
173	174	0.00	2	1.9	218	PASS
174	95	50	100	82.3	11329	PASS
175	174	5	9	5.4	610	PASS
176	174	95	101	97.6	11058	PASS
177	176	5	9	6.3	696	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	185	50.95	933	68.95	1631	81.95	171
36.95	1060	55.95	339	69.90	132	86.90	63
37.95	892	57.00	515	72.00	53	88.00	60
39.05	420	59.90	230	73.00	772	90.80	5
40.10	55	60.90	653	74.00	2781	91.95	469
43.90	279	61.10	237	75.00	7812	92.90	218
45.00	51	62.00	819	76.00	801	93.05	501
46.85	142	62.95	917	78.85	1013	94.05	1942
47.20	100	63.80	69	79.80	219	95.05	13763
49.00	708	64.85	213	80.00	65	95.95	845
50.00	3386	67.95	1680	80.90	864	116.90	70

Average of 12.847 to 12.859 min.: VN082970.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
119.10	65						
140.75	149						
142.90	371						
144.90	83						
171.95	240						
172.95	218						
174.00	11329						
174.80	429						
174.95	610						
176.00	11058						
177.05	696						

Instrument :

MSVOA_N

ClientSampleId :

BFB