


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071918\
Data File : VN049904.D
Acq On : 19 Jul 2018 9:01
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Title : SW846 8260
Last Update : Thu Jul 19 01:58:39 2018

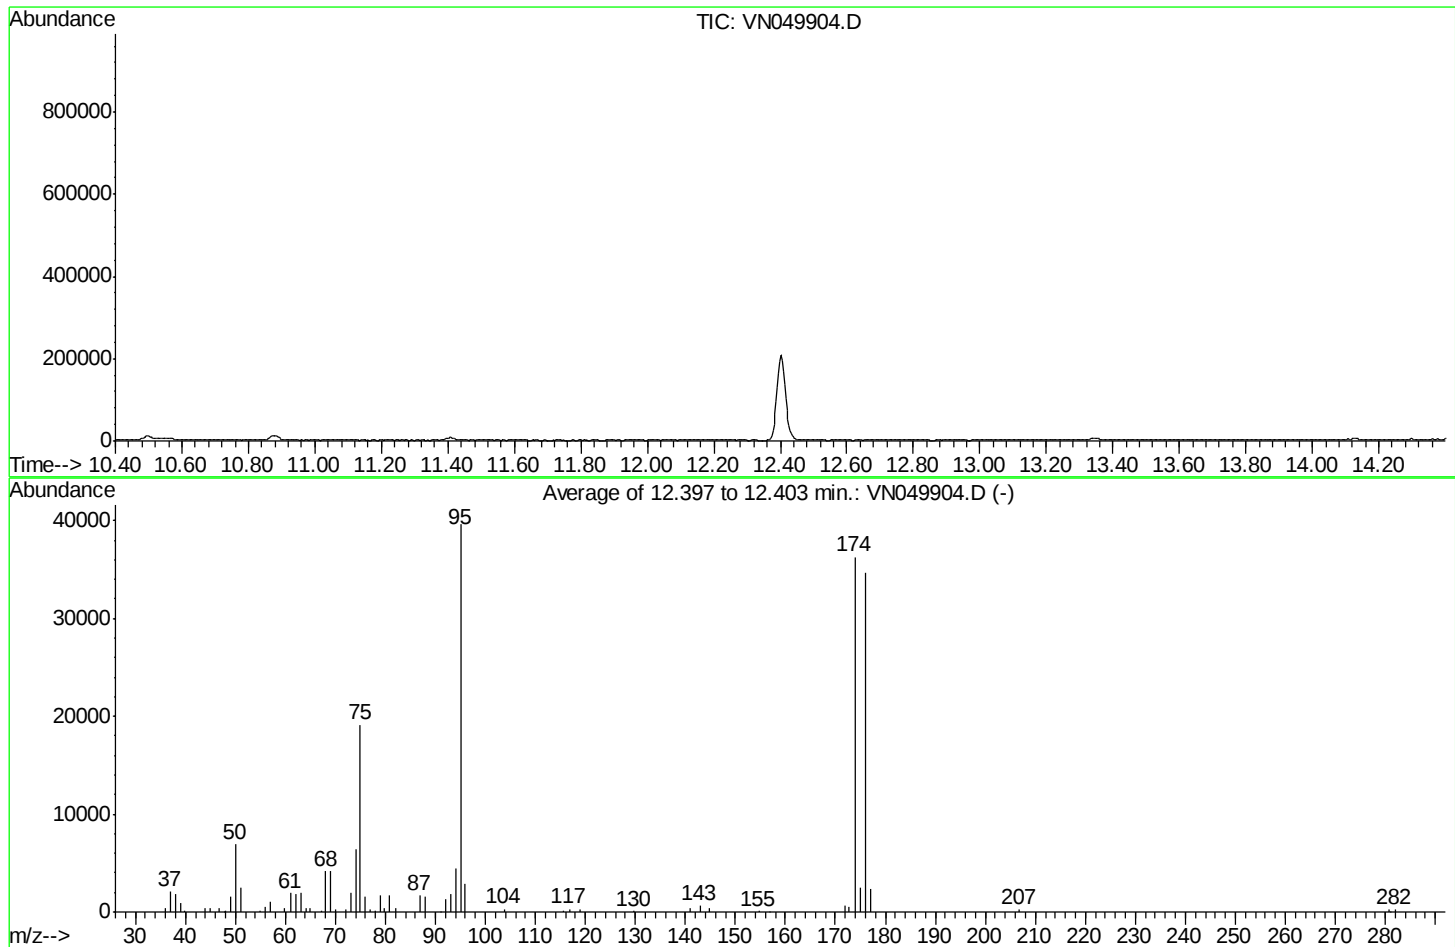

AutoFind: Scans 3361, 3362, 3363; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	6926	PASS
75	95	30	60	48.3	19130	PASS
95	95	100	100	100.0	39618	PASS
96	95	5	9	7.3	2903	PASS
173	174	0.00	2	1.4	525	PASS
174	95	50	100	91.5	36242	PASS
175	174	5	9	6.9	2516	PASS
176	174	95	101	95.6	34664	PASS
177	176	5	9	6.7	2318	PASS