


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN071918\
Data File : VN049930.D
Acq On : 19 Jul 2018 21:37
Operator : MD\SY
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
Title : SW846 8260
Last Update : Thu Jul 19 01:58:39 2018

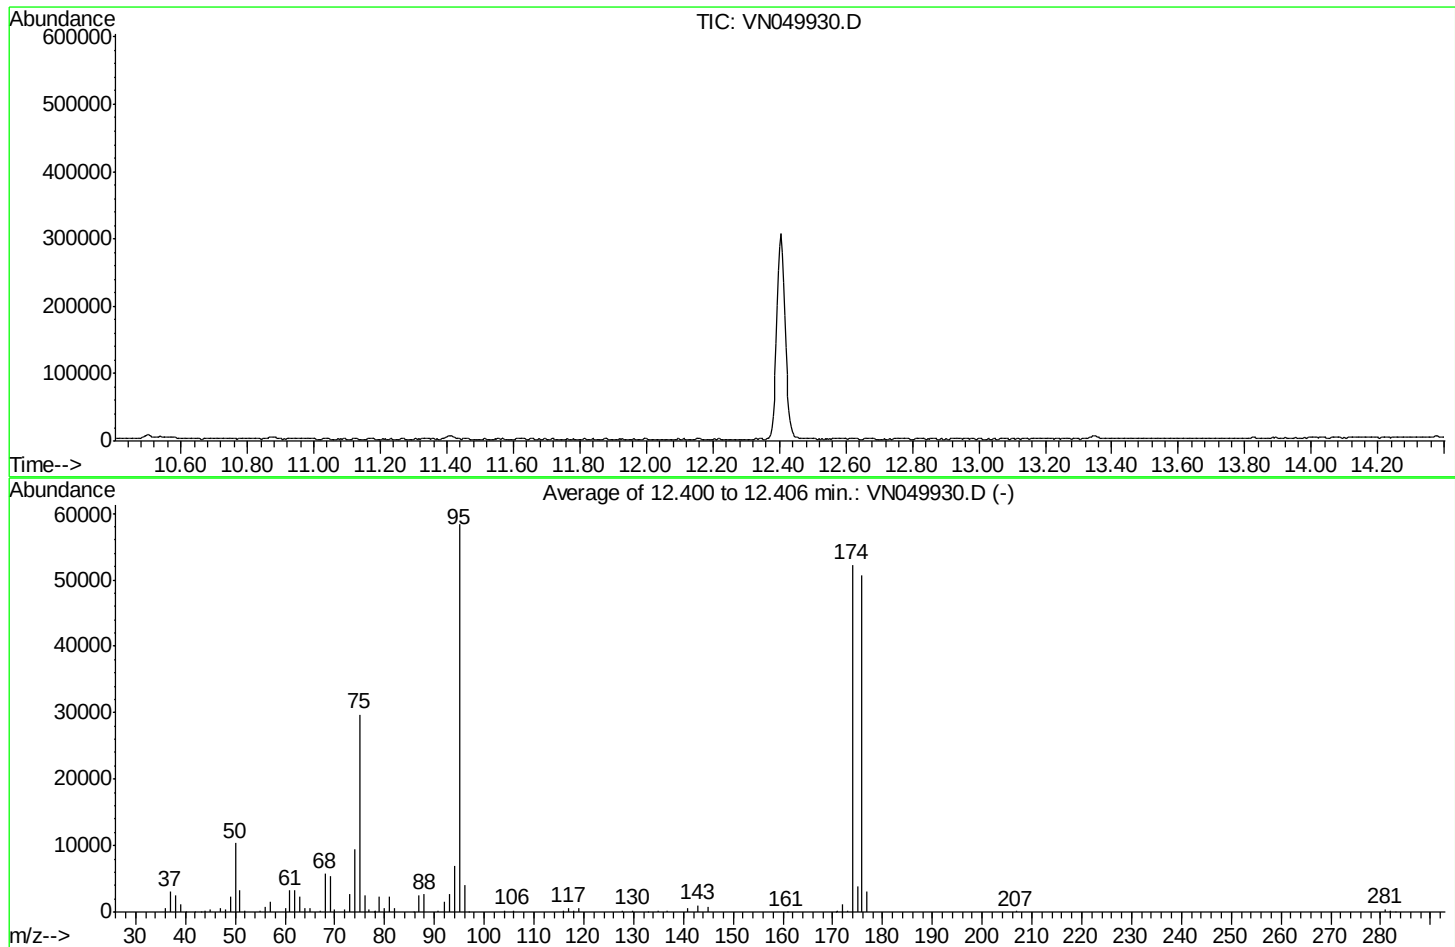

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3348

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	10341	PASS
75	95	30	60	50.9	29717	PASS
95	95	100	100	100.0	58365	PASS
96	95	5	9	6.8	3959	PASS
173	174	0.00	2	0.6	288	PASS
174	95	50	100	89.6	52282	PASS
175	174	5	9	7.5	3898	PASS
176	174	95	101	97.0	50706	PASS
177	176	5	9	6.2	3156	PASS