

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071921\
 Data File : VN067799.D
 Acq On : 19 Jul 2021 17:36
 Operator : JC/MD
 Sample : M3088-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 20 04:53:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	314214	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	585842	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	611991	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	223291	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	245327	51.662	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 103.320%	
35) Dibromofluoromethane	8.024	113	181027	51.145	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 102.280%	
50) Toluene-d8	10.443	98	768469	51.869	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 103.740%	
62) 4-Bromofluorobenzene	12.734	95	266277	50.878	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 101.760%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.824	94	229	Below Cal	#	4
6) Chloroethane	3.001	64	53	Below Cal	#	44
11) Tert butyl alcohol	5.390	59	279	0.409	ug/l	# 71
13) Acrolein	4.052	56	256	Below Cal	#	64
16) Acetone	4.296	43	35664	23.868	ug/l	# 88
18) Methyl Acetate	4.867	43	3232	0.770	ug/l	# 78
20) Methylene Chloride	5.087	84	28585	7.605	ug/l	89
25) 2-Butanone	7.351	43	9554	3.851	ug/l	92
29) Tetrahydrofuran	7.702	42	4326	2.651	ug/l	96
31) Cyclohexane	8.088	56	8748	1.314	ug/l	# 42
36) 1,1-Dichloropropene	8.094	75	28984	5.326	ug/l	# 46
37) Ethyl Acetate	7.351	43	9554	1.812	ug/l	# 78
38) Carbon Tetrachloride	8.086	117	35532	6.619	ug/l	# 18
41) Methacrylonitrile	7.702	41	1925	0.710	ug/l	# 38
43) Isopropyl Acetate	8.563	43	38694	4.172	ug/l	# 91
45) 1,2-Dichloropropane	9.628	63	2491	0.604	ug/l	# 44
48) Methyl methacrylate	9.550	41	9567	2.332	ug/l	# 12
49) 1,4-Dioxane	9.631	88	206	34.576	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.339	43	11867	2.083	ug/l	98
53) t-1,3-Dichloropropene	10.438	75	50	1.751	ug/l	# 56
54) cis-1,3-Dichloropropene	10.247	75	65214	10.250	ug/l	# 62
57) 1,3-Dichloropropane	11.095	76	38549	5.498	ug/l	# 43
59) 2-Hexanone	11.095	43	585233	147.141	ug/l	# 54
60) Dibromochloromethane	11.492	129	275	2.409	ug/l	# 11
71) Bromoform	12.718	173	205	3.225	ug/l	# 29
74) N-amyl acetate	12.200	43	22041	3.372	ug/l	# 53
76) 1,2,3-Trichloropropane	12.734	75	148968	32.668	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.734	75	148968	105.326	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.263	180	222	2.731	ug/l	73
95) Naphthalene	15.509	128	3133	3.282	ug/l	# 88
96) 1,2,3-Trichlorobenzene	15.697	180	329	2.720	ug/l	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071921\
Data File : VN067799.D
Acq On : 19 Jul 2021 17:36
Operator : JC/MD
Sample : M3088-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 20 04:53:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




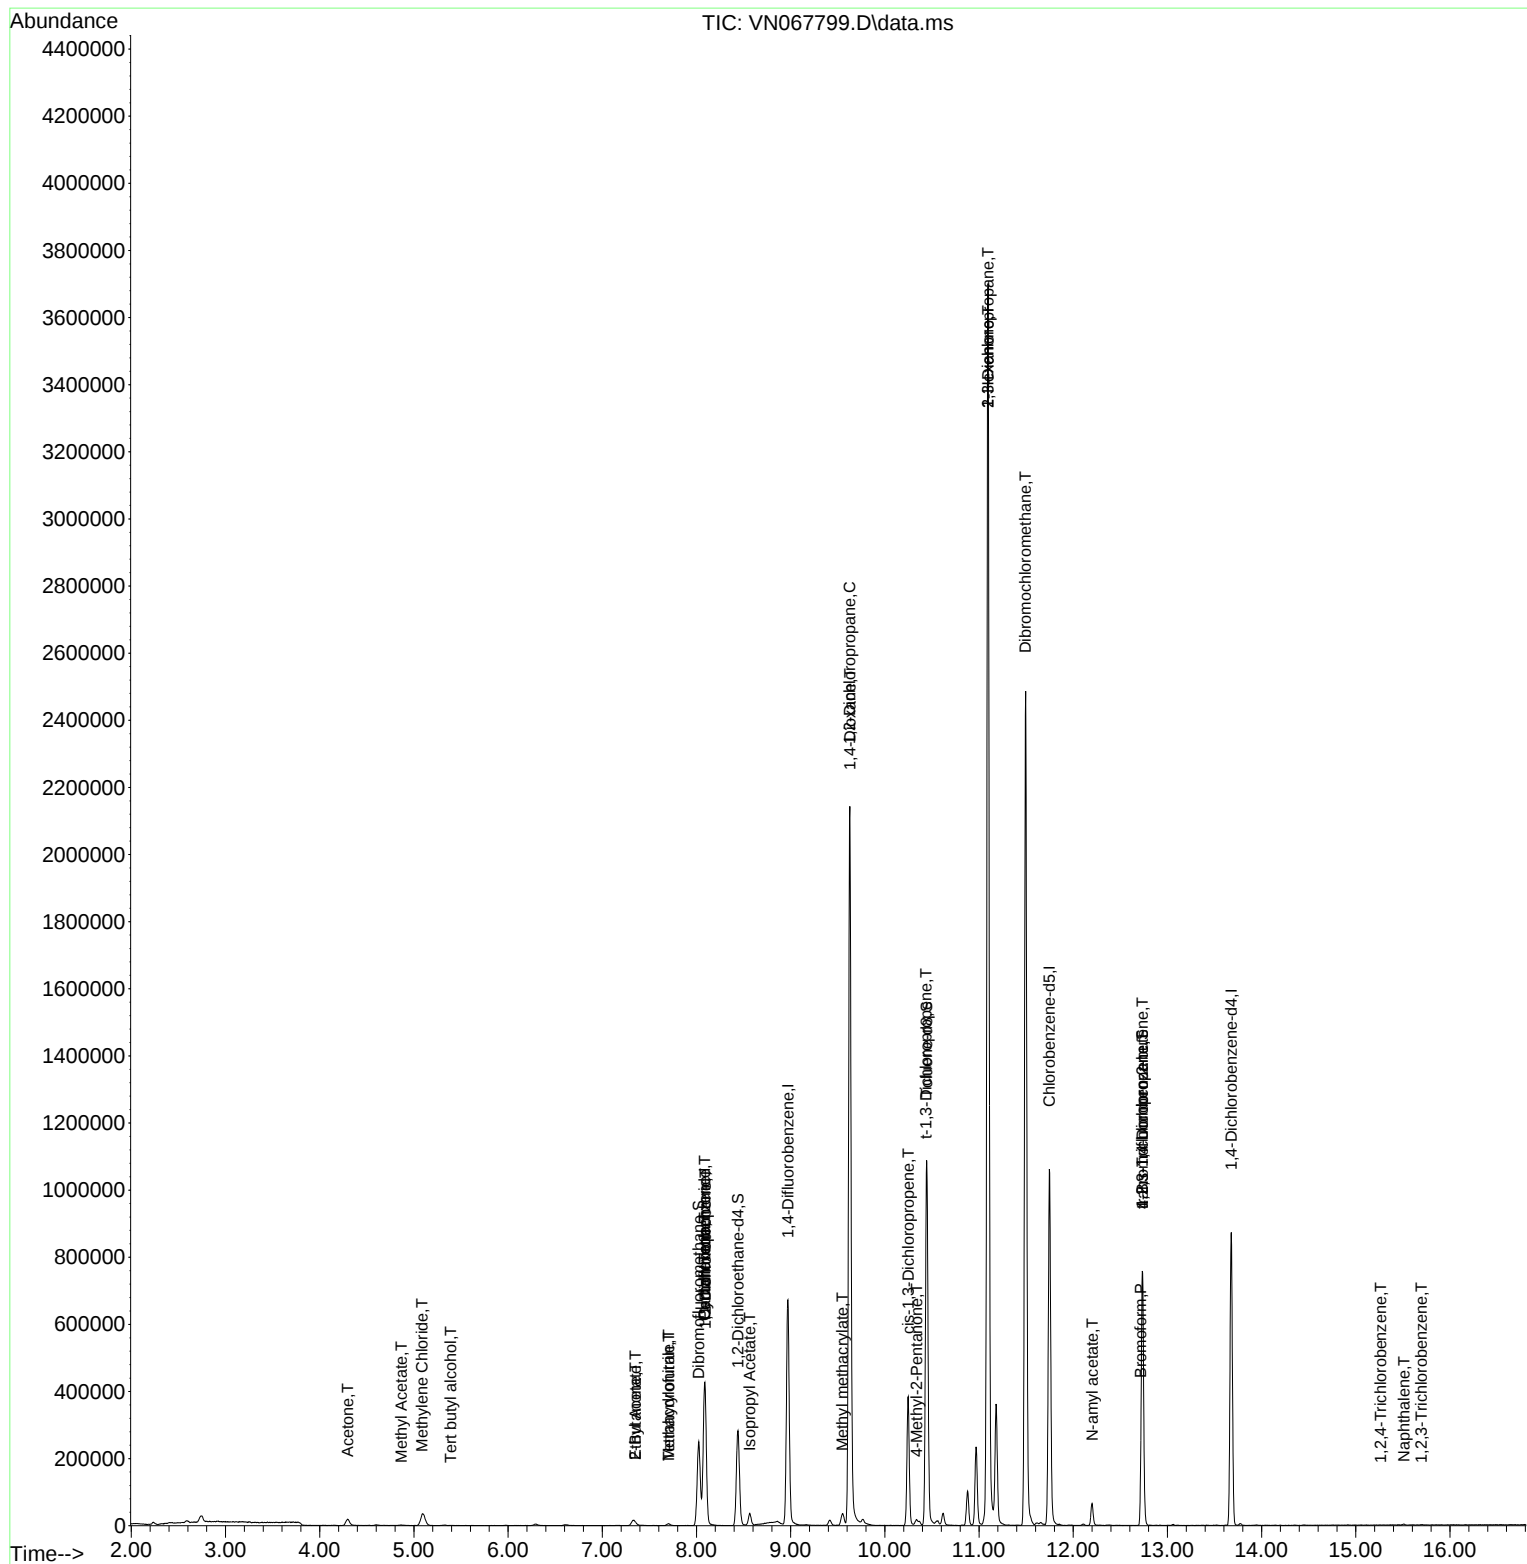




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 314214
Ion Ratio Lower Upper
168 100
99 62.7 62.9 94.3#

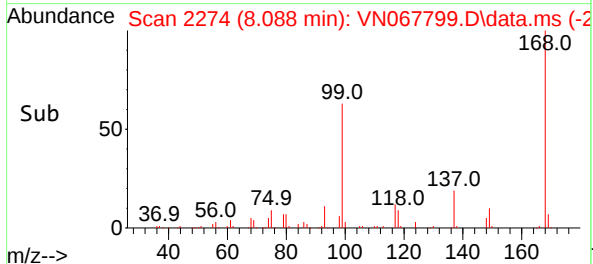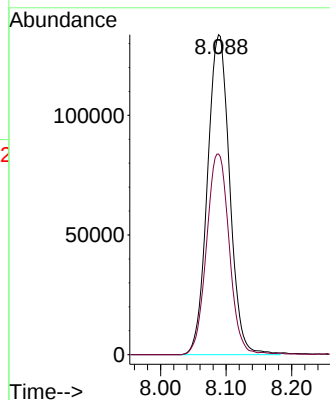

#5
Bromomethane
Concen: Below Cal
RT: 2.824 min Scan# 311
Delta R.T. -0.008 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 94 Resp: 229
Ion Ratio Lower Upper
94 100
96 0.0 73.7 110.5#


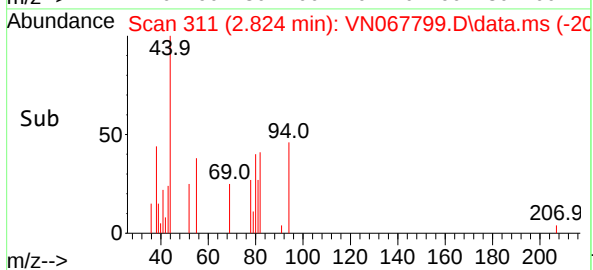
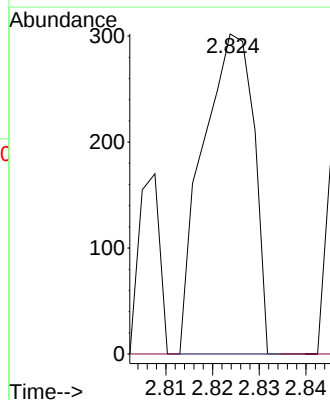





#6
Chloroethane
Concen: Below Cal
RT: 3.001 min Scan# 377
Delta R.T. -0.005 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 64 Resp: 53
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

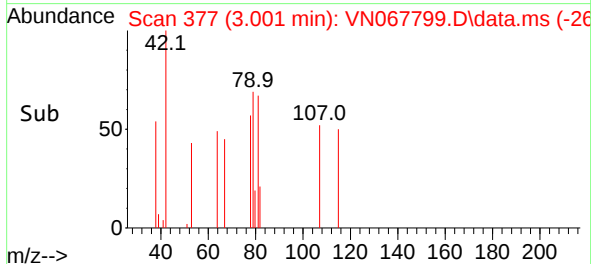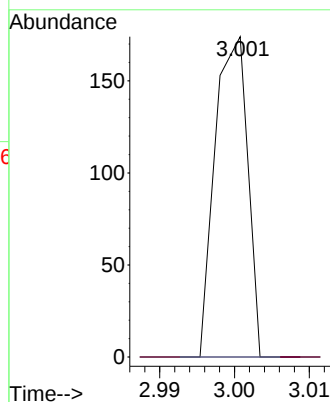

#11
Tert butyl alcohol
Concen: 0.409 ug/l
RT: 5.390 min Scan# 1268
Delta R.T. 0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 59 Resp: 279
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


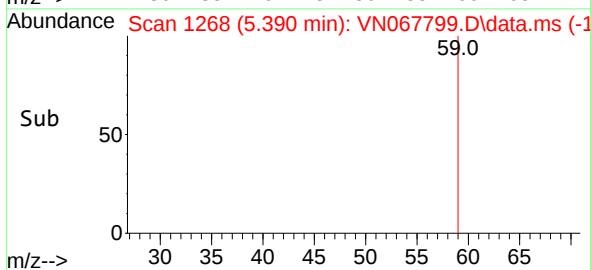
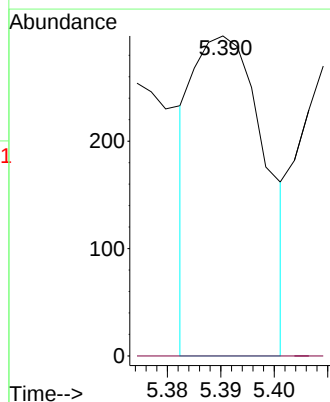
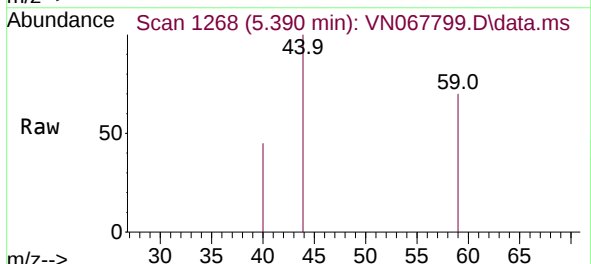


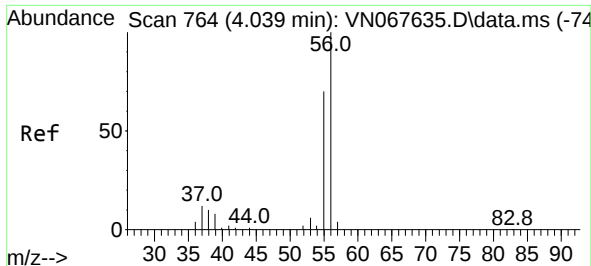

#13
Acrolein
Concen: Below Cal
RT: 4.052 min Scan# 769
Delta R.T. 0.013 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 256
Ion Ratio Lower Upper
56 100
55 42.2 57.4 86.0#

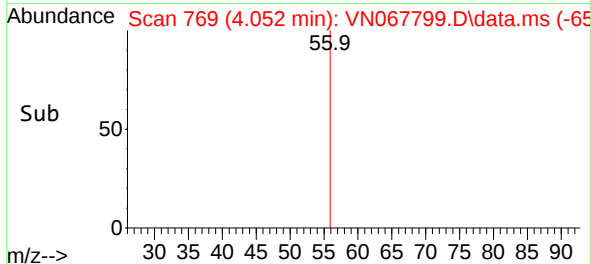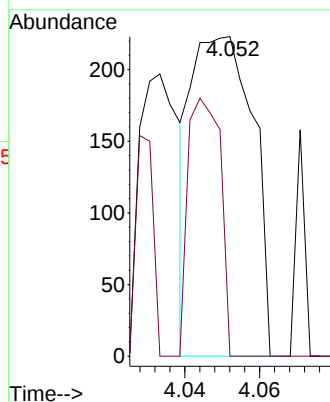

#16
Acetone
Concen: 23.868 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 43 Resp: 35664
Ion Ratio Lower Upper
43 100
58 32.6 21.2 31.8#


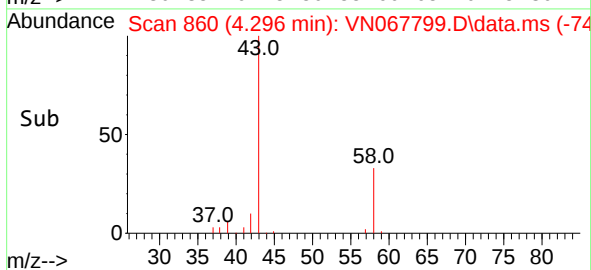
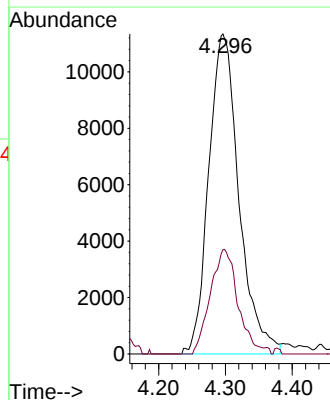
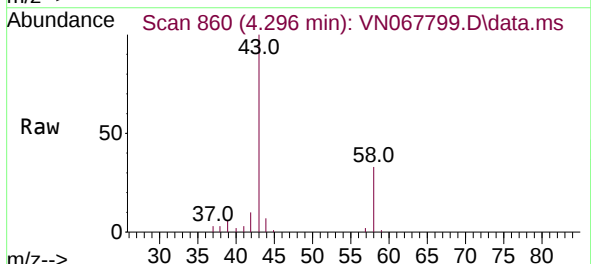




#18
Methyl Acetate
Concen: 0.770 ug/l
RT: 4.867 min Scan# 1073
Delta R.T. 0.010 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 3232
Ion Ratio Lower Upper
43 100
74 11.4 17.4 26.0#

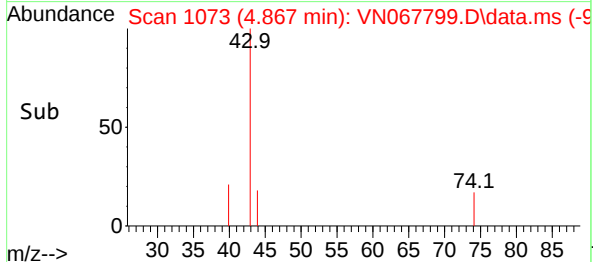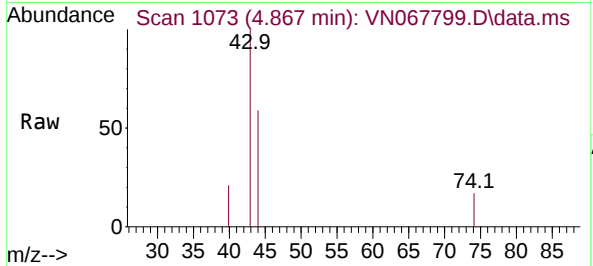

#20
Methylene Chloride
Concen: 7.605 ug/l
RT: 5.087 min Scan# 1155
Delta R.T. -0.003 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 84 Resp: 28585
Ion Ratio Lower Upper
84 100
49 118.6 110.9 166.3
51 36.4 32.6 49.0
86 62.2 51.6 77.4




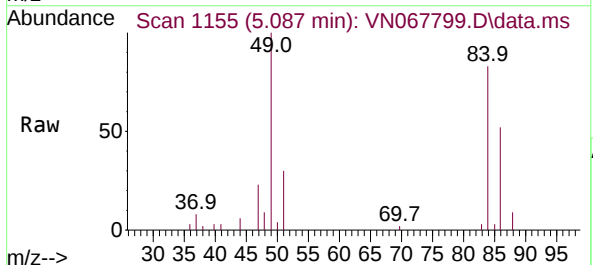


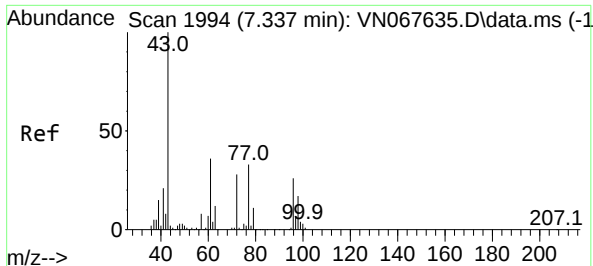

#25
2-Butanone
Concen: 3.851 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.014 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 9554
Ion Ratio Lower Upper
43 100
72 28.7 19.7 29.5

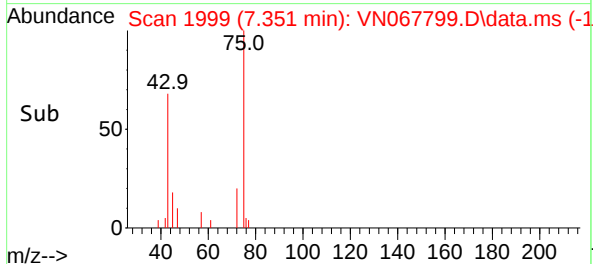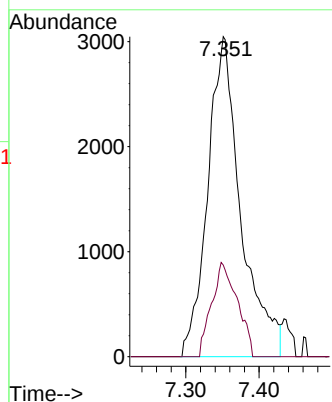

#29
Tetrahydrofuran
Concen: 2.651 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.013 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 42 Resp: 4326
Ion Ratio Lower Upper
42 100
72 41.3 32.8 49.2
71 34.3 31.2 46.8









#31
Cyclohexane
Concen: 1.314 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.006 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 8748
Ion Ratio Lower Upper
56 100
69 139.2 27.3 40.9#
84 86.1 64.9 97.3

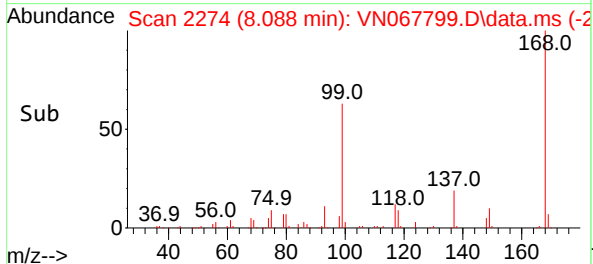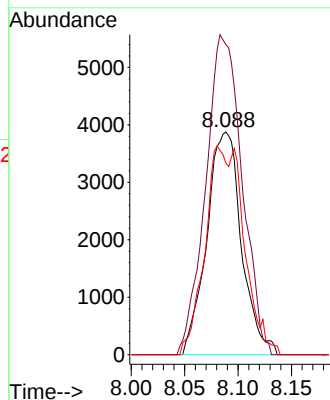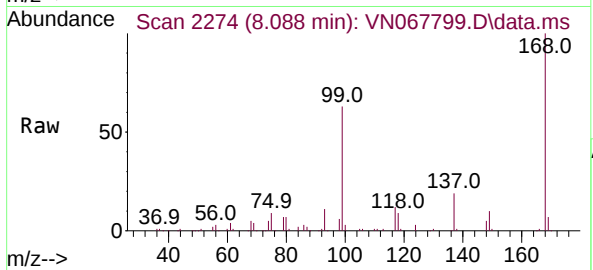

#33
1,2-Dichloroethane-d4
Concen: 51.662 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 65 Resp: 245327
Ion Ratio Lower Upper
65 100
67 51.3 0.0 98.6

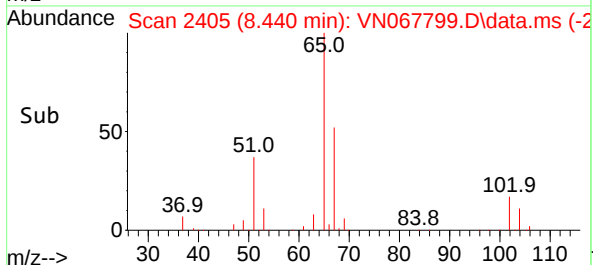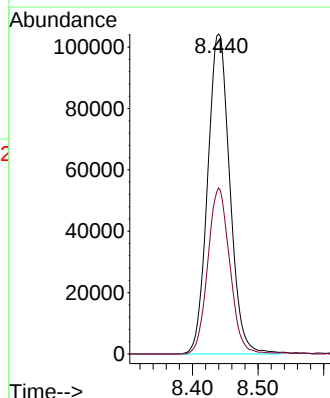




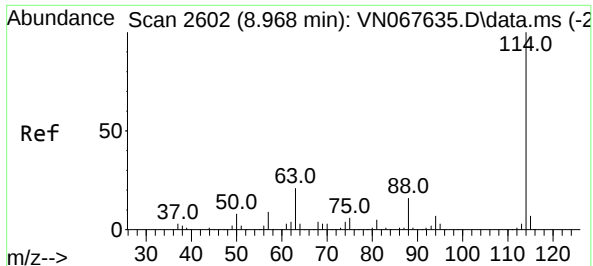


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion:114 Resp: 585842
Ion Ratio Lower Upper
114 100
63 20.7 0.0 49.0
88 15.7 0.0 36.6

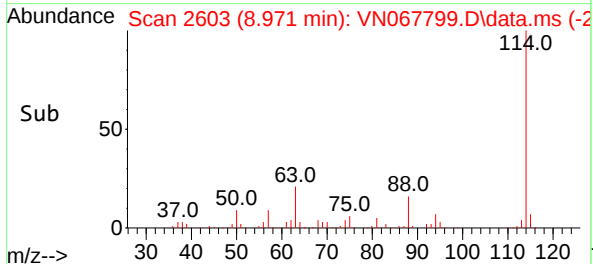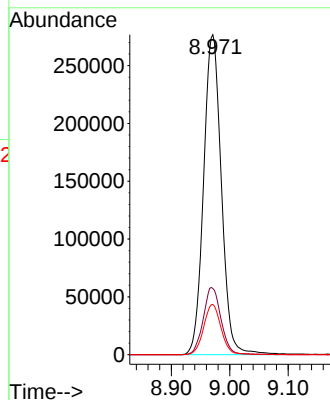


#35

Dibromofluoromethane
Concen: 51.145 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36


Tgt Ion:113 Resp: 181027
Ion Ratio Lower Upper
113 100
111 101.9 83.8 125.8
192 15.8 13.4 20.0

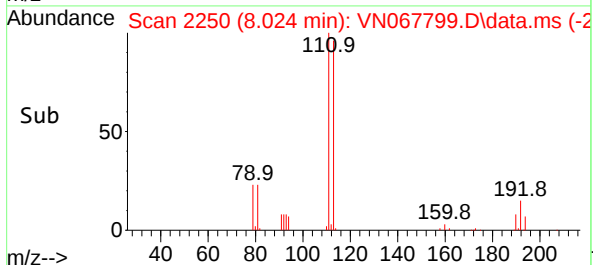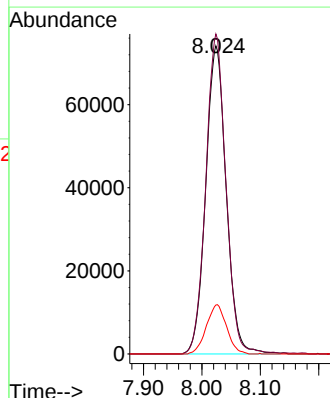



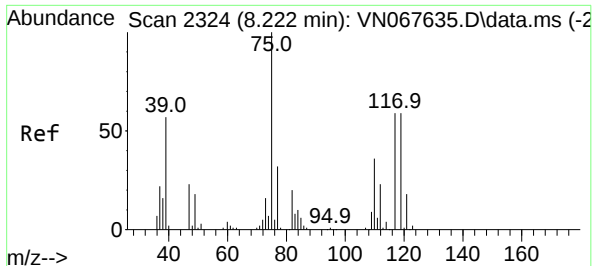


#36
1,1-Dichloropropene
Concen: 5.326 ug/l
RT: 8.094 min Scan# 2276
Delta R.T. -0.128 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Instrument :
MSVOA_N
ClientSampled :



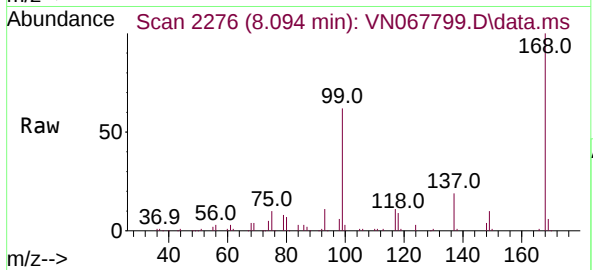



Tgt Ion: 75 Resp: 28984
Ion Ratio Lower Upper
75 100
110 2.4 15.7 47.0#
77 0.0 24.6 37.0#

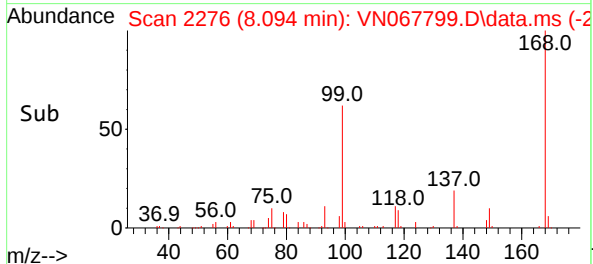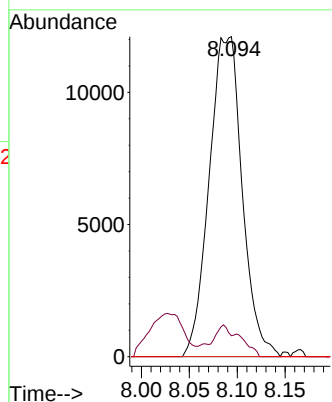

#37
Ethyl Acetate
Concen: 1.812 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.067 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36


Tgt Ion: 43 Resp: 9554
Ion Ratio Lower Upper
43 100
61 6.3 10.6 16.0#
70 0.0 8.1 12.1#

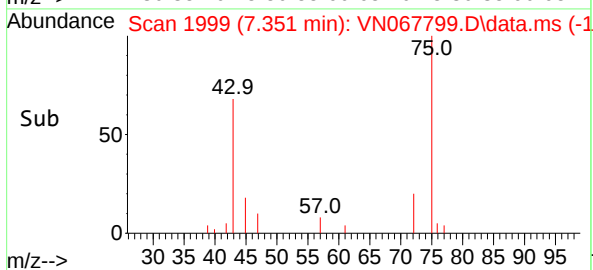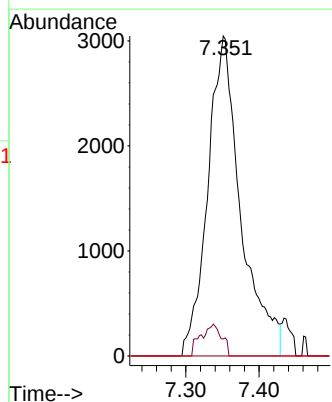



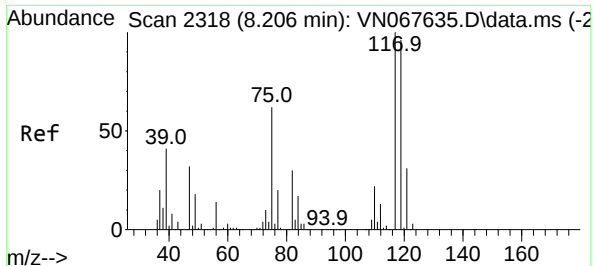


#38
Carbon Tetrachloride
Concen: 6.619 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36


Instrument :
MSVOA_N
ClientSampled :

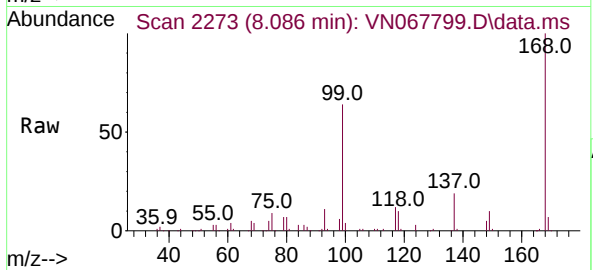



Tgt Ion:117 Resp: 35532
Ion Ratio Lower Upper
117 100
119 6.3 75.4 113.2#
121 0.0 23.5 35.3#

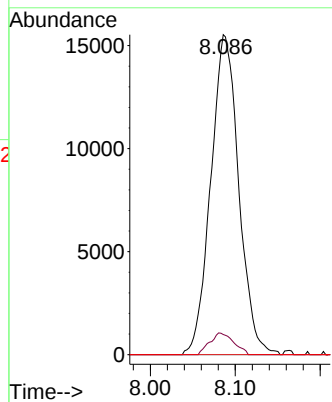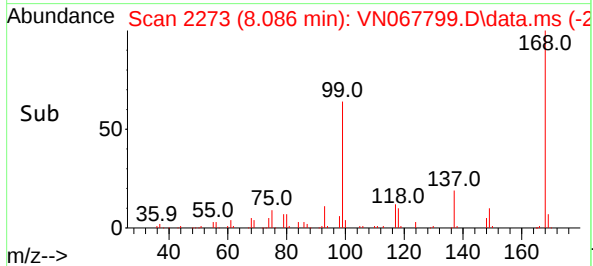


#41
Methacrylonitrile
Concen: 0.710 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.062 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36



Tgt Ion: 41 Resp: 1925
Ion Ratio Lower Upper
41 100
39 85.7 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#




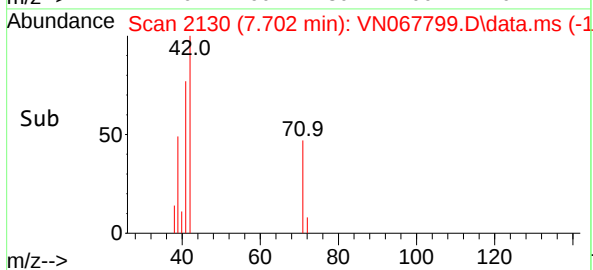


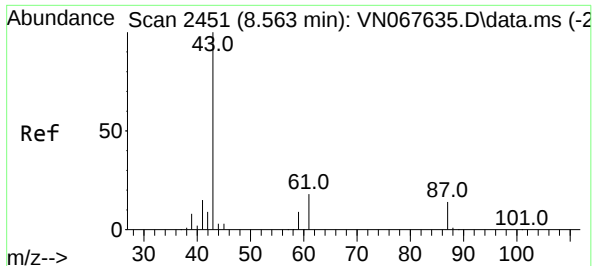

#43
Isopropyl Acetate
Concen: 4.172 ug/l
RT: 8.563 min Scan# 2451
Delta R.T. 0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion	Ratio	Lower	Upper
43	100		
61	18.3	19.0	28.4#
87	13.6	9.5	14.3

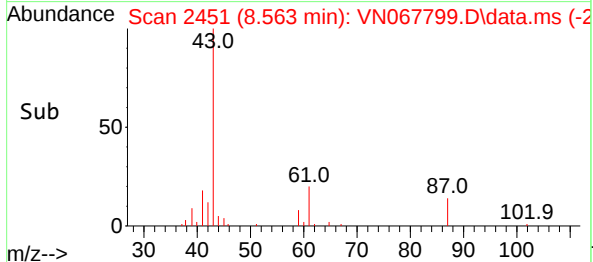

#45
1,2-Dichloropropane
Concen: 0.604 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion	Ratio	Lower	Upper
63	100		
65	0.0	24.3	36.5#




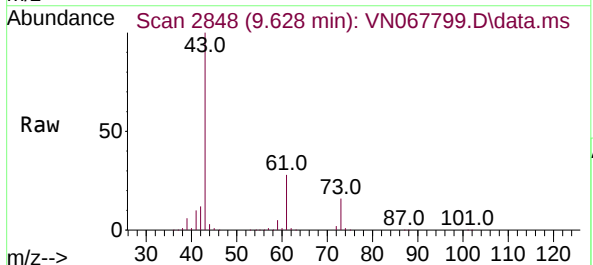


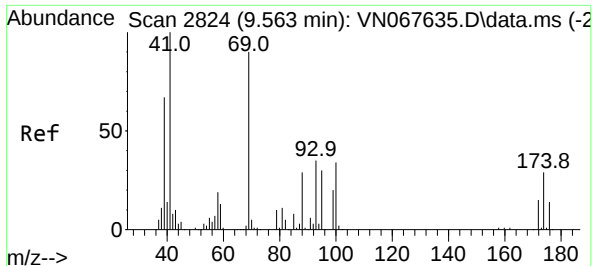

#48
Methyl methacrylate
Concen: 2.332 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.013 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 9567
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

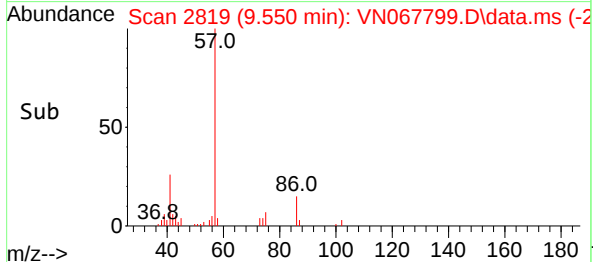

#49
1,4-Dioxane
Concen: 34.576 ug/l
RT: 9.631 min Scan# 2849
Delta R.T. 0.060 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 88 Resp: 206
Ion Ratio Lower Upper
88 100
43 1025646.1 28.8 43.2#
58 4488.3 60.4 90.6#




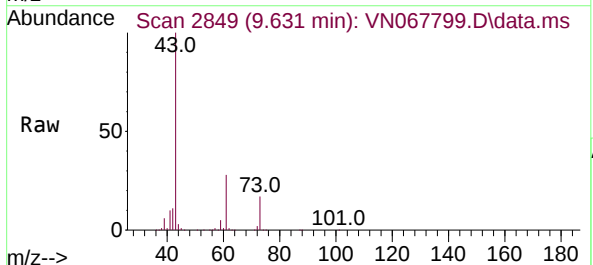




#50
Toluene-d8
Concen: 51.869 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 768469
Ion Ratio Lower Upper
98 100
100 63.5 51.7 77.5

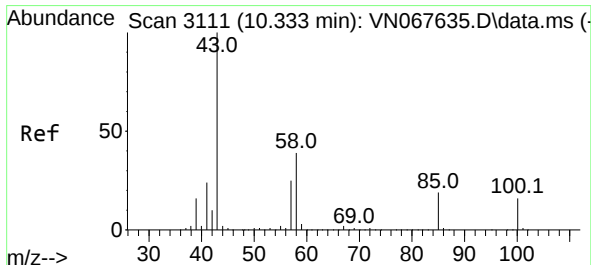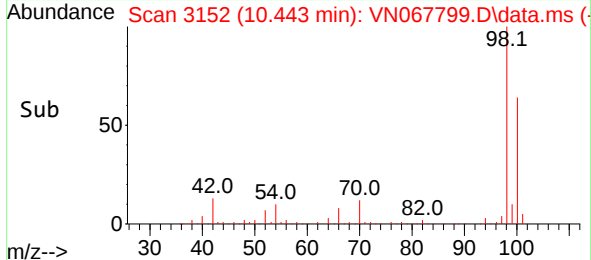

#51
4-Methyl-2-Pentanone
Concen: 2.083 ug/l
RT: 10.339 min Scan# 3113
Delta R.T. 0.006 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 43 Resp: 11867
Ion Ratio Lower Upper
43 100
58 34.5 28.6 43.0


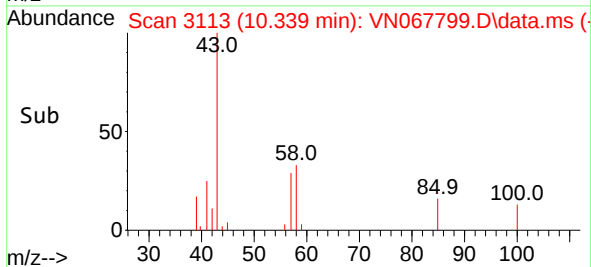

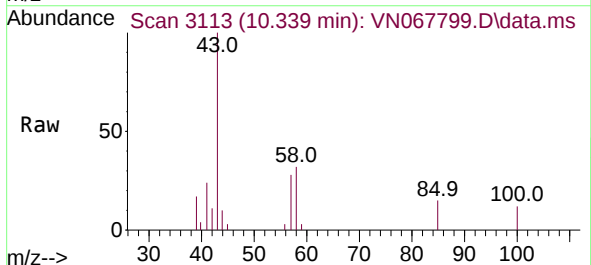


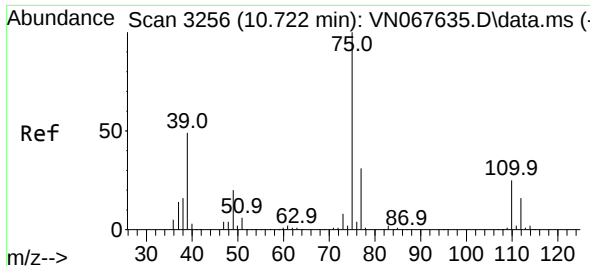

#53
t-1,3-Dichloropropene
Concen: 1.751 ug/l
RT: 10.438 min Scan# 3150
Delta R.T. -0.284 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 50
Ion Ratio Lower Upper
75 100
77 7.0 25.1 37.7#

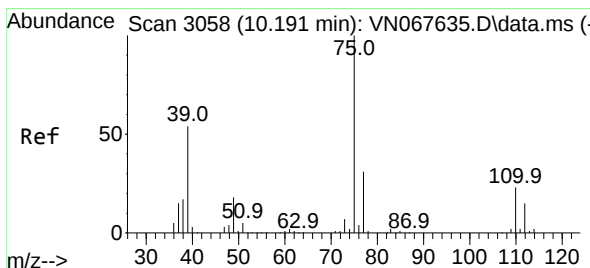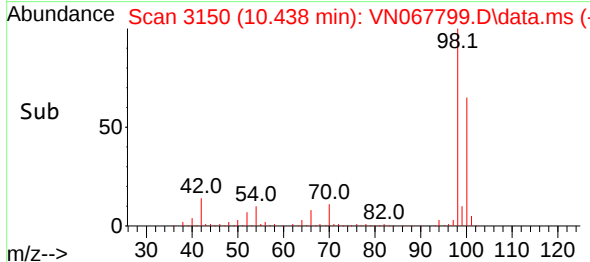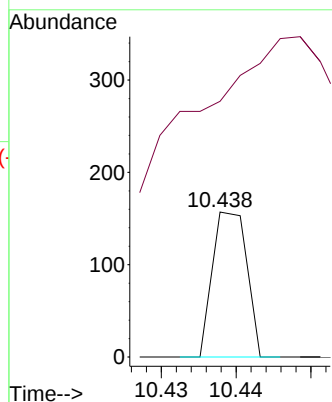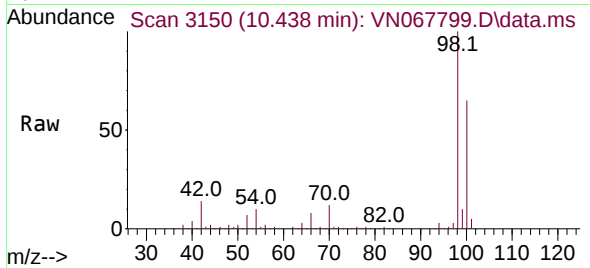

#54
cis-1,3-Dichloropropene
Concen: 10.250 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 75 Resp: 65214
Ion Ratio Lower Upper
75 100
77 0.8 24.6 37.0#
39 40.0 50.7 76.1#


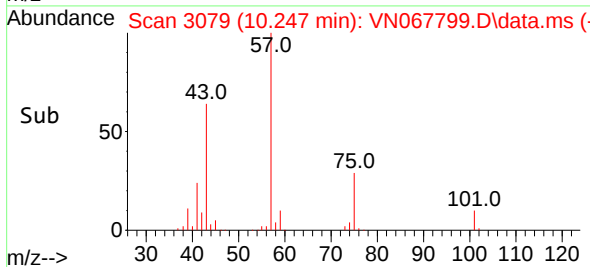

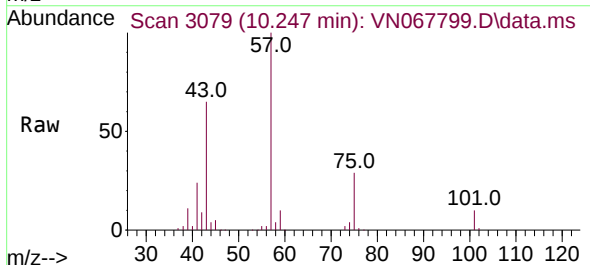




#57
1,3-Dichloropropane
Concen: 5.498 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 38549
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#

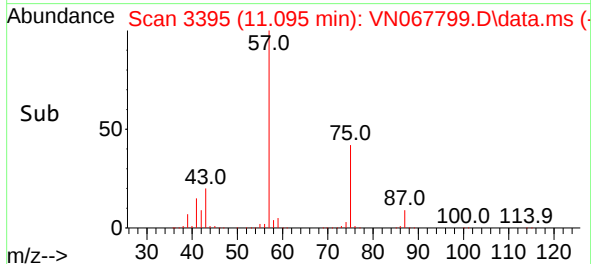

#59
2-Hexanone
Concen: 147.141 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36


Tgt Ion: 43 Resp: 585233
Ion Ratio Lower Upper
43 100
58 17.7 24.7 74.1#

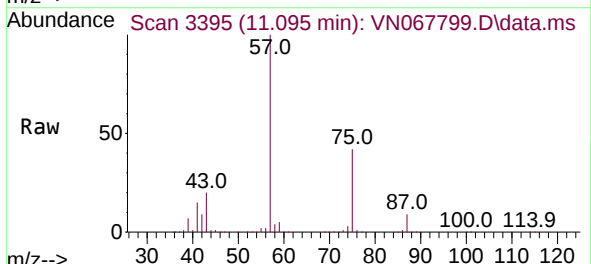



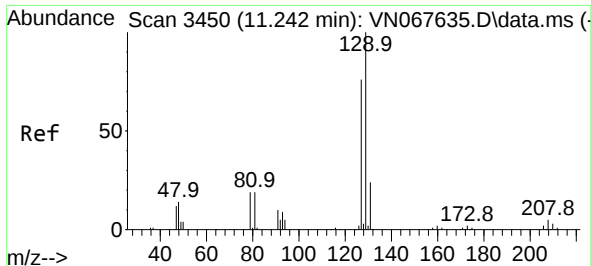


#60
Dibromochloromethane
Concen: 2.409 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.250 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion:129 Resp: 275
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

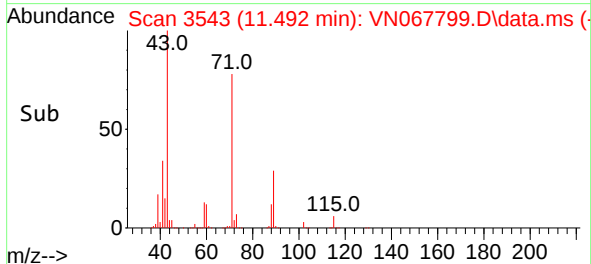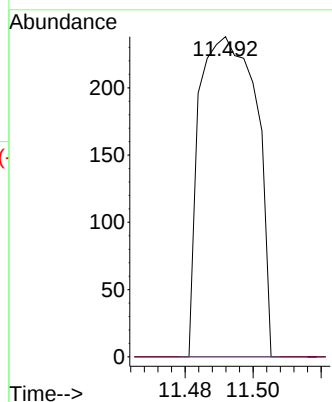

#62
4-Bromofluorobenzene
Concen: 50.878 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 95 Resp: 266277
Ion Ratio Lower Upper
95 100
174 71.5 0.0 122.0
176 68.0 0.0 117.6


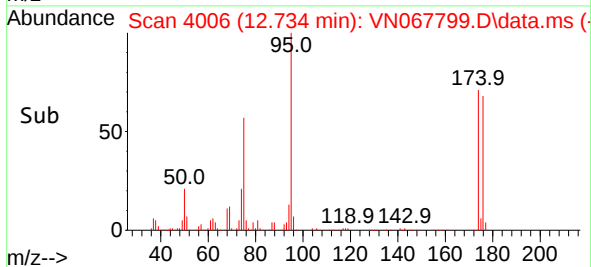
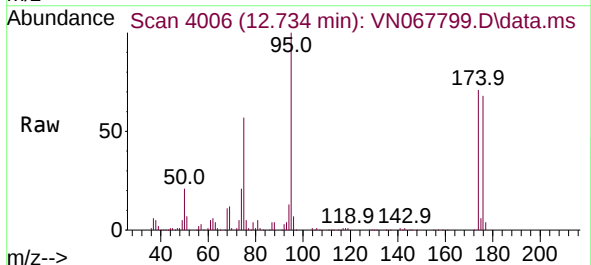





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 611991
Ion Ratio Lower Upper
117 100
82 56.5 53.1 79.7
119 32.0 25.5 38.3

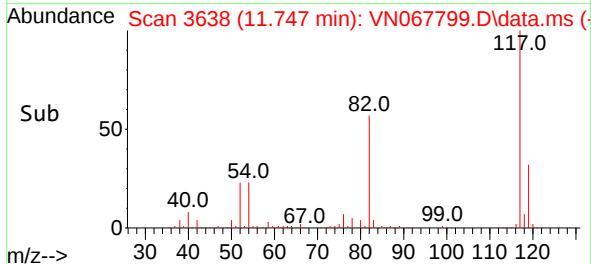

#71
Bromoform
Concen: 3.225 ug/l
RT: 12.718 min Scan# 4000
Delta R.T. 0.258 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion:173 Resp: 205
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0


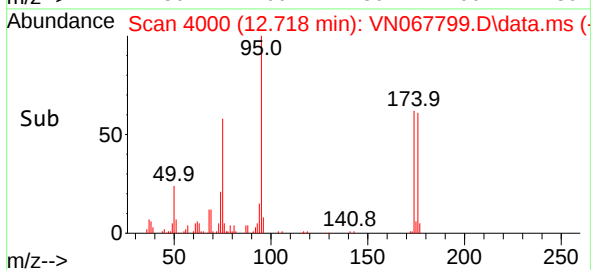

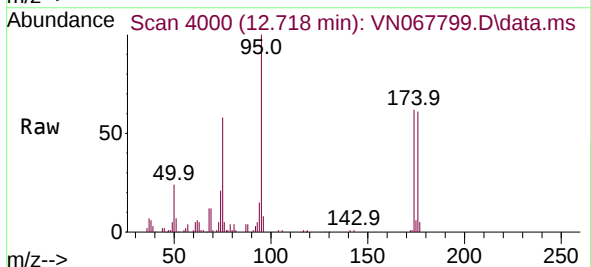




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:152 Resp: 223291
Ion Ratio Lower Upper
152 100
115 63.8 36.1 108.5
150 160.5 0.0 351.8

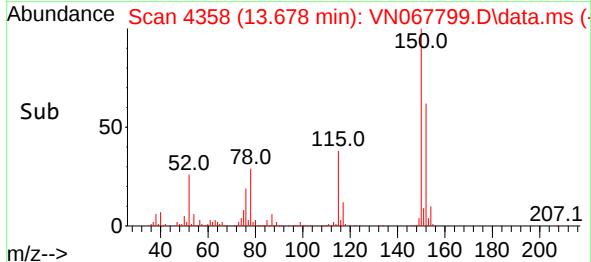

#74
N-ethyl acetate
Concen: 3.372 ug/l
RT: 12.200 min Scan# 3807
Delta R.T. -0.190 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

Tgt Ion: 43 Resp: 22041
Ion Ratio Lower Upper
43 100
70 1.0 29.4 44.2#
55 5.3 17.0 25.4#
61 4.7 17.6 26.4#


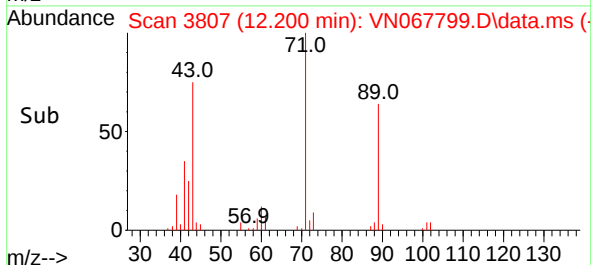
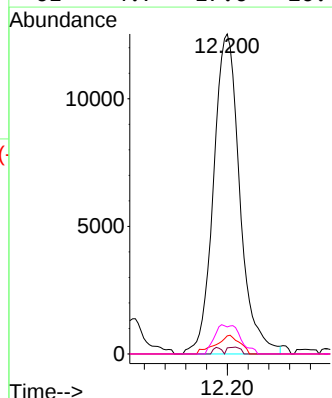
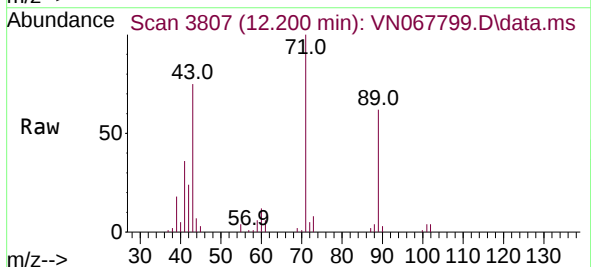


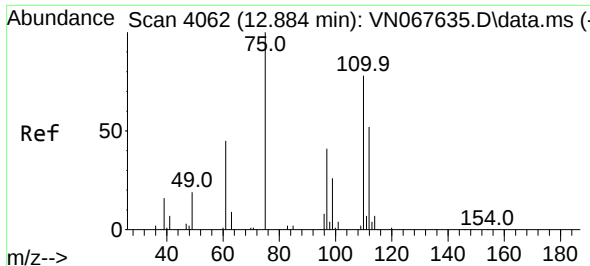

#76
1,2,3-Trichloropropane
Concen: 32.668 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 148968
Ion Ratio Lower Upper
75 100
77 1.0 0.0 0.0#

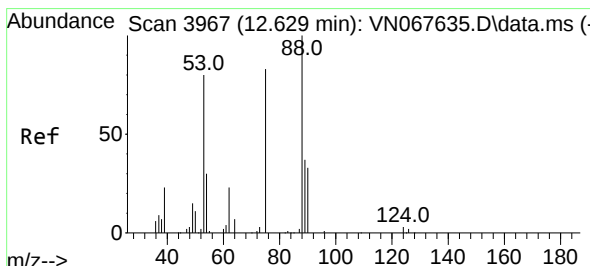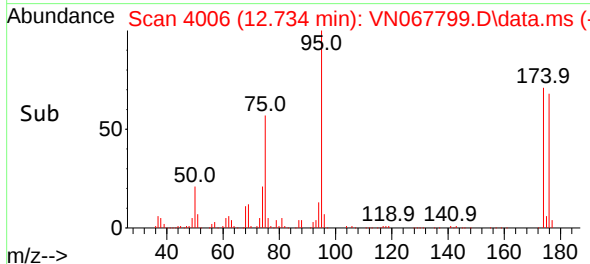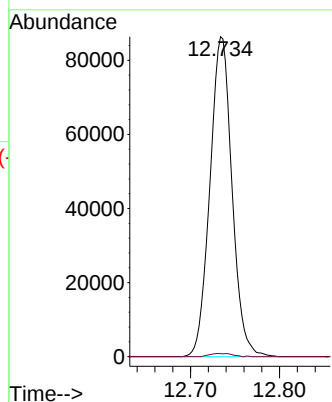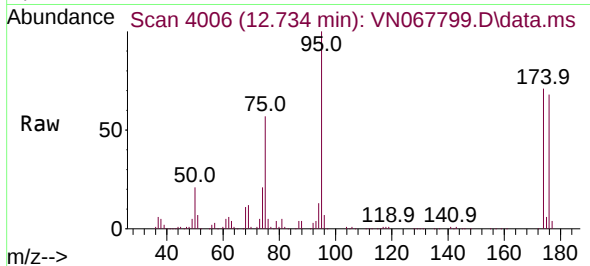

#81
trans-1,4-Dichloro-2-butene
Concen: 105.326 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36


Tgt Ion: 75 Resp: 148968
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

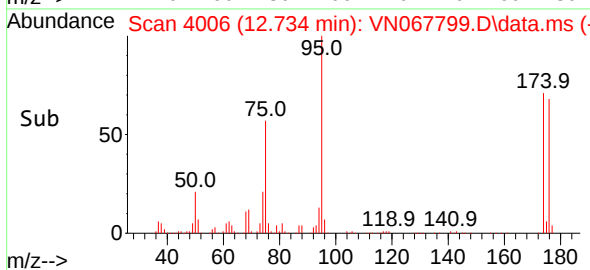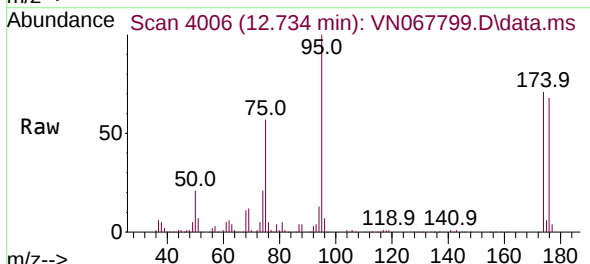






#93
1,2,4-Trichlorobenzene
Concen: 2.731 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.002 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:180 Resp: 222
Ion Ratio Lower Upper
180 100
182 124.3 47.5 142.5
145 23.9 17.2 51.6

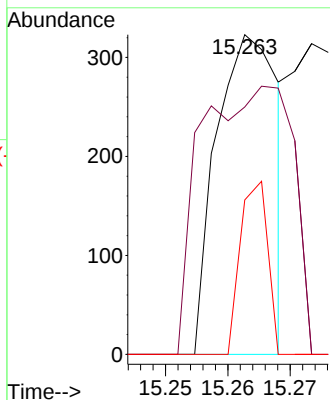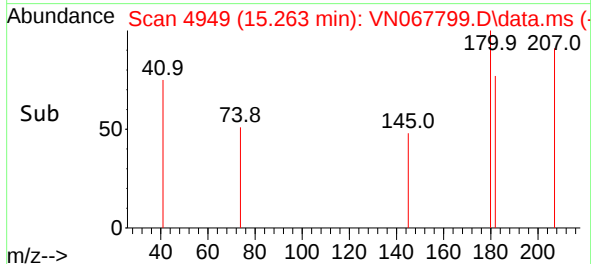


#95
Naphthalene
Concen: 3.282 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN067799.D
Acq: 19 Jul 2021 17:36

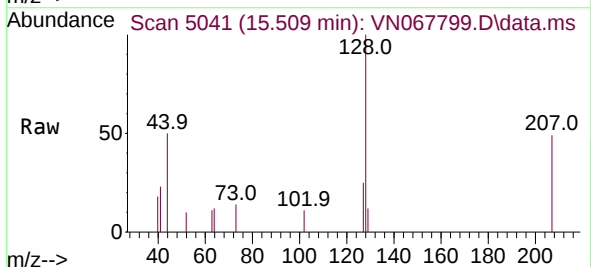


Tgt Ion:128 Resp: 3133
Ion Ratio Lower Upper
128 100
127 10.1 10.6 15.8#
129 4.1 8.6 12.8#

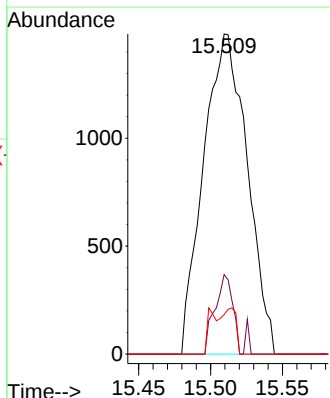



#96
 1,2,3-Trichlorobenzene
 Concen: 2.720 ug/l
 RT: 15.697 min Scan# 5111
 Delta R.T. -0.005 min
 Lab File: VN067799.D
 Acq: 19 Jul 2021 17:36

Instrument :
 MSVOA_N
 ClientSampled :

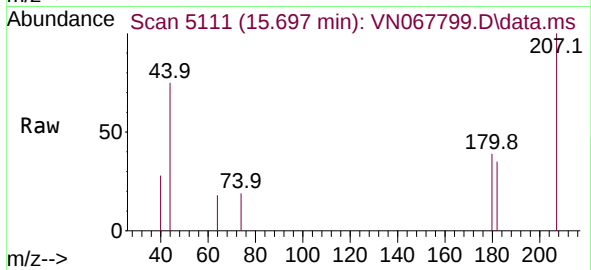

Tgt Ion:180 Resp: 329
 Ion Ratio Lower Upper
 180 100
 182 81.5 47.8 143.3
 145 28.0 18.2 54.6

