

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071921\
 Data File : VN067801.D
 Acq On : 19 Jul 2021 18:25
 Operator : JC/MD
 Sample : M3088-06
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 20 04:53:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	311028	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	595532	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	614801	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	220956	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	249958	53.176	ug/l	0.00
Spiked Amount	50.000	Range 61 - 141	Recovery	= 106.360%		
35) Dibromofluoromethane	8.024	113	180342	50.122	ug/l	0.00
Spiked Amount	50.000	Range 69 - 133	Recovery	= 100.240%		
50) Toluene-d8	10.446	98	790525	52.490	ug/l	0.00
Spiked Amount	50.000	Range 65 - 126	Recovery	= 104.980%		
62) 4-Bromofluorobenzene	12.734	95	268372	50.444	ug/l	0.00
Spiked Amount	50.000	Range 58 - 135	Recovery	= 100.880%		
Target Compounds						
					Qvalue	
5) Bromomethane	2.834	94	76	Below Cal	#	4
6) Chloroethane	3.044	64	25	Below Cal	#	44
11) Tert butyl alcohol	5.396	59	626	0.927	ug/l #	71
13) Acrolein	4.047	56	210	Below Cal	#	14
16) Acetone	4.301	43	34922	23.611	ug/l	100
18) Methyl Acetate	4.857	43	4410	1.062	ug/l #	68
20) Methylene Chloride	5.098	84	27964	7.507	ug/l	92
25) 2-Butanone	7.354	43	7931	3.229	ug/l	94
29) Tetrahydrofuran	7.697	42	2071	1.282	ug/l #	32
31) Cyclohexane	8.086	56	8399	1.274	ug/l #	19
36) 1,1-Dichloropropene	8.083	75	29563	5.344	ug/l #	52
37) Ethyl Acetate	7.354	43	7931	1.480	ug/l #	69
38) Carbon Tetrachloride	8.086	117	34008	6.232	ug/l #	18
41) Methacrylonitrile	7.705	41	2736	0.993	ug/l #	49
43) Isopropyl Acetate	8.569	43	40456	4.291	ug/l #	89
45) 1,2-Dichloropropane	9.628	63	2594	0.619	ug/l #	44
48) Methyl methacrylate	9.550	41	9965	2.390	ug/l #	12
49) 1,4-Dioxane	9.628	88	293	35.551	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	9618	1.660	ug/l	88
53) t-1,3-Dichloropropene	10.454	75	184	1.770	ug/l #	1
54) cis-1,3-Dichloropropene	10.247	75	66246	10.243	ug/l #	60
57) 1,3-Dichloropropane	11.095	76	38598	5.415	ug/l #	43
59) 2-Hexanone	11.095	43	581261	143.764	ug/l #	53
60) Dibromochloromethane	11.495	129	248	2.403	ug/l #	11
71) Bromoform	12.712	173	86	3.196	ug/l #	29
76) 1,2,3-Trichloropropane	12.734	75	147329	32.650	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	147329	105.268	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.260	180	124	2.706	ug/l #	22
95) Naphthalene	15.509	128	1007	3.100	ug/l #	86
96) 1,2,3-Trichlorobenzene	15.697	180	83	2.655	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071921\
Data File : VN067801.D
Acq On : 19 Jul 2021 18:25
Operator : JC/MD
Sample : M3088-06
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 20 04:53:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




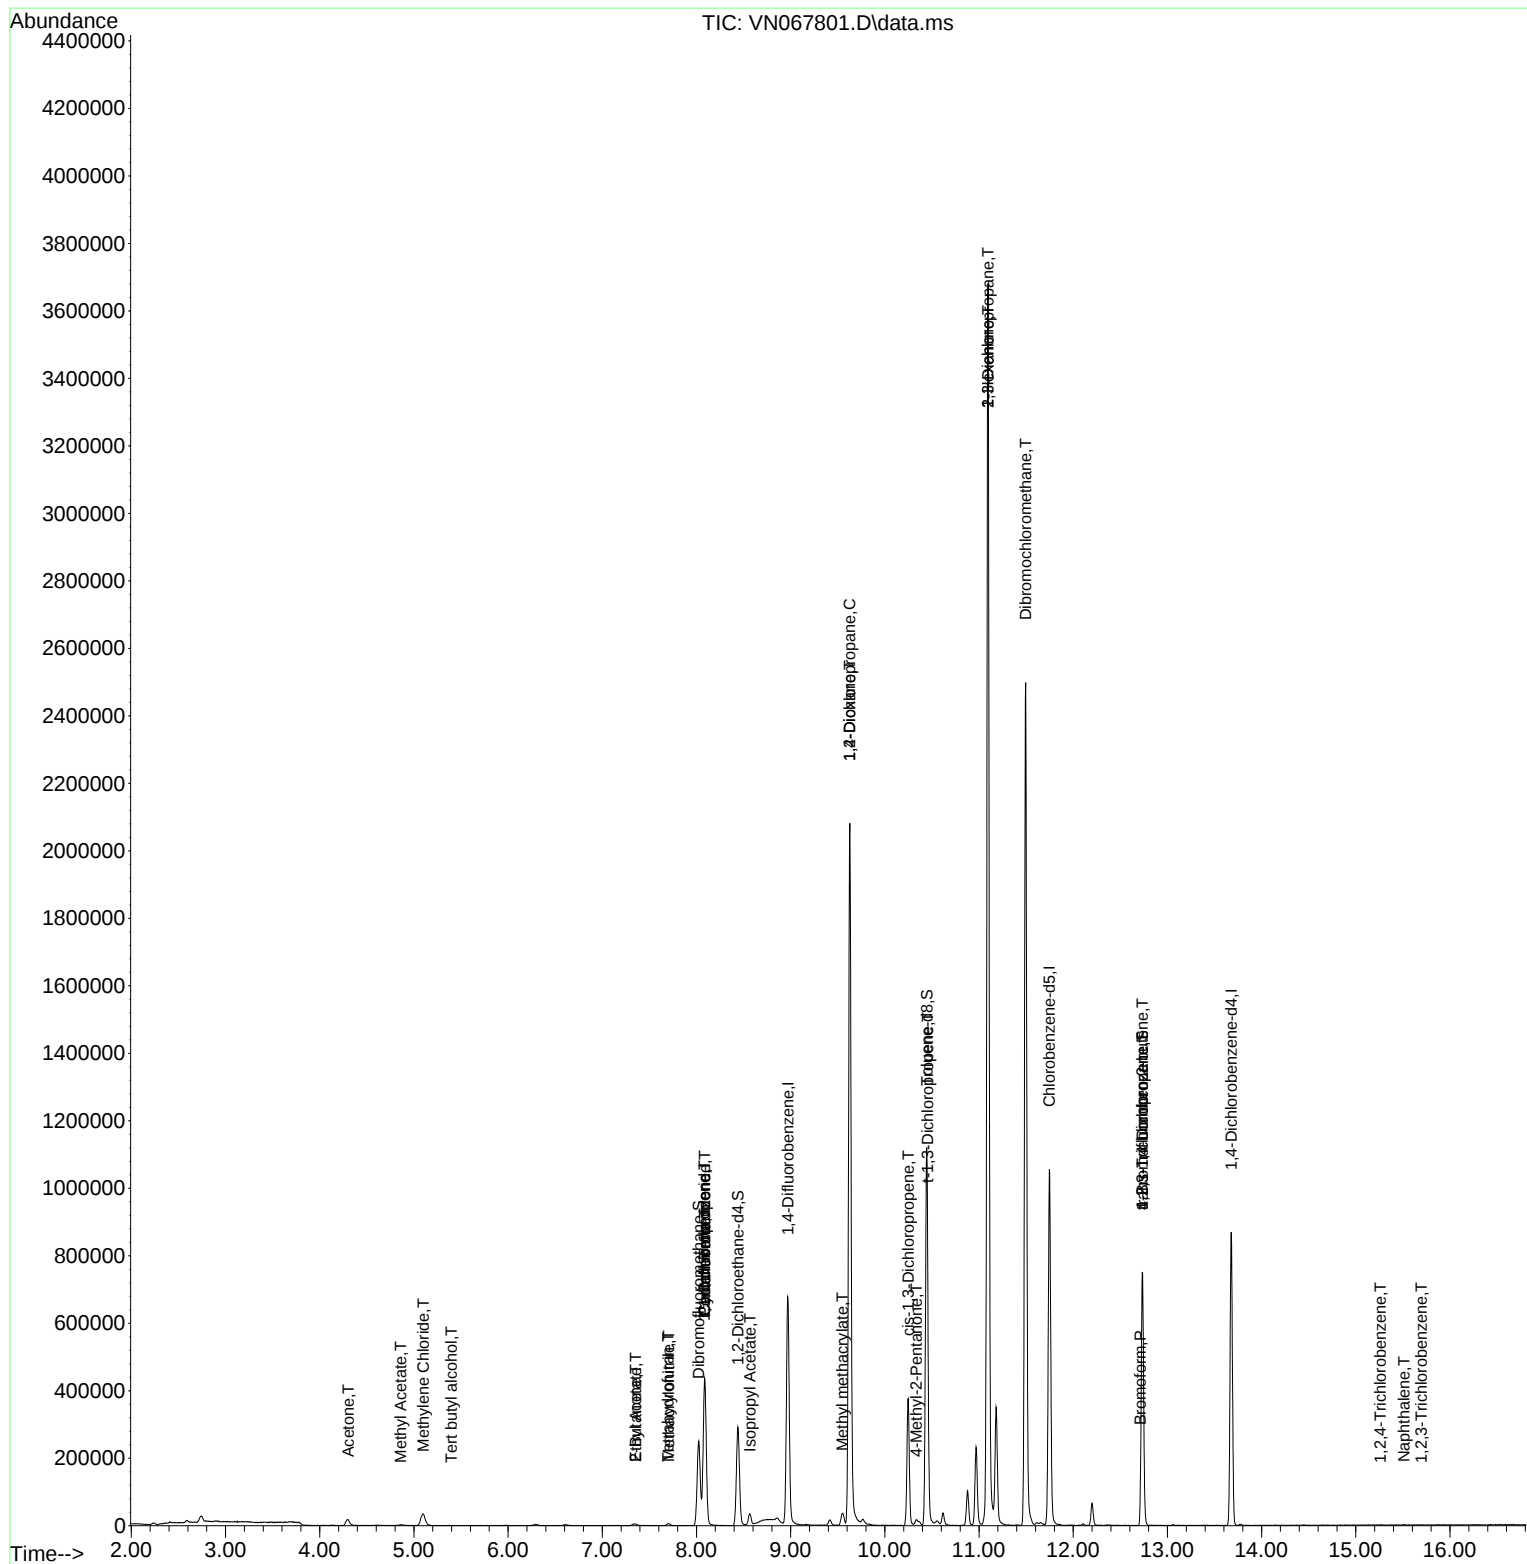




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:168 Resp: 311028
Ion Ratio Lower Upper
168 100
99 64.0 62.9 94.3

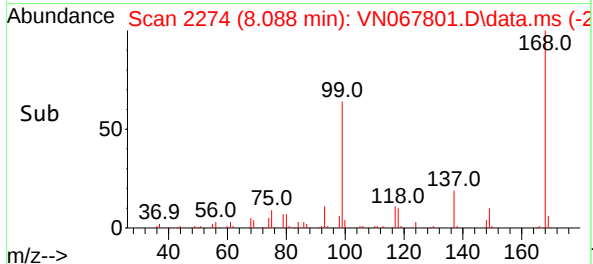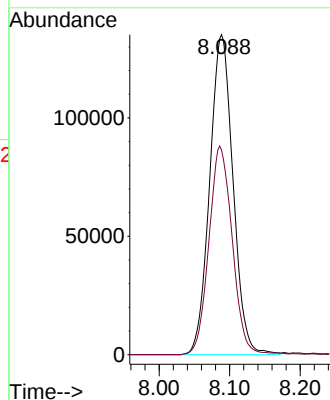

#5
Bromomethane
Concen: Below Cal
RT: 2.834 min Scan# 315
Delta R.T. 0.002 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 94 Resp: 76
Ion Ratio Lower Upper
94 100
96 0.0 73.7 110.5#


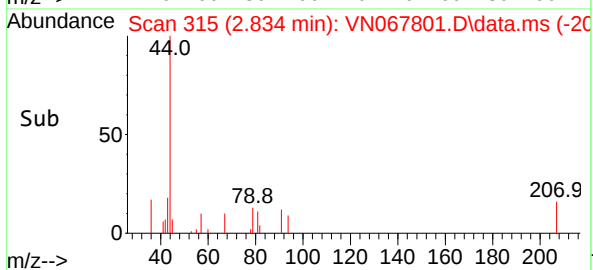
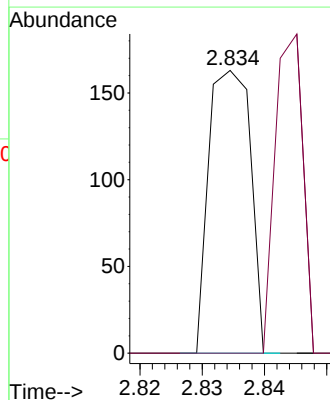
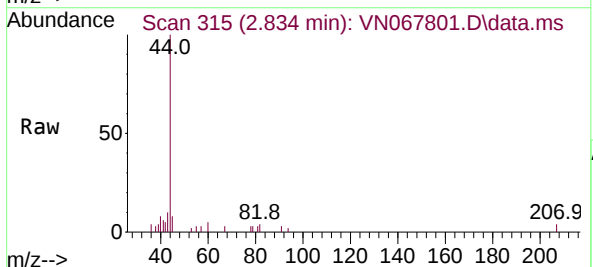


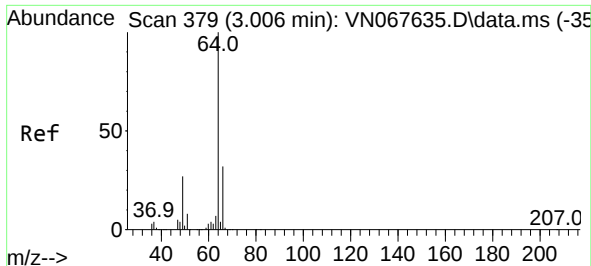

#6
Chloroethane
Concen: Below Cal
RT: 3.044 min Scan# 393
Delta R.T. 0.038 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 64 Resp: 25
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#

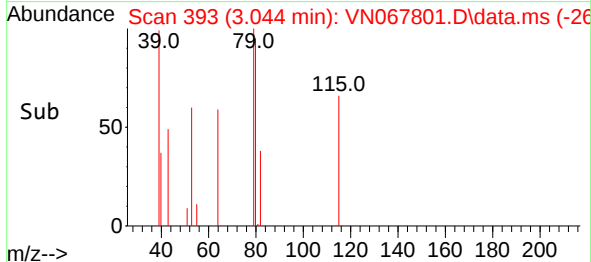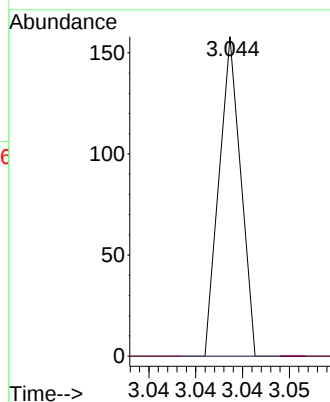

#11
Tert butyl alcohol
Concen: 0.927 ug/l
RT: 5.396 min Scan# 1270
Delta R.T. 0.006 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 59 Resp: 626
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#


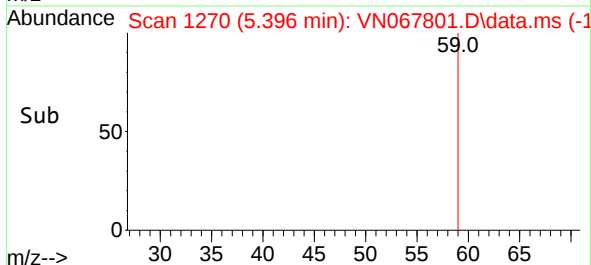
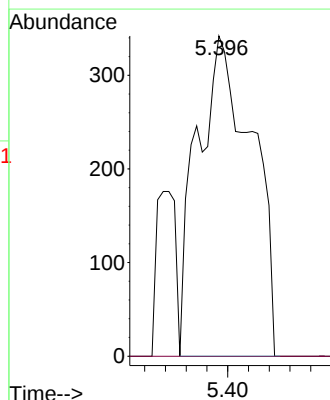
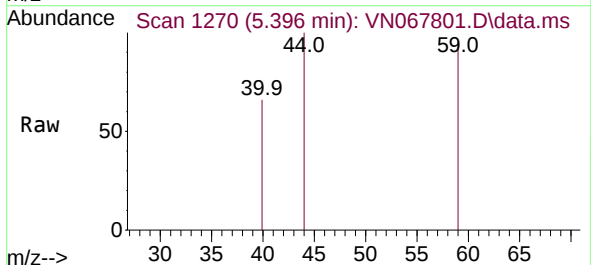


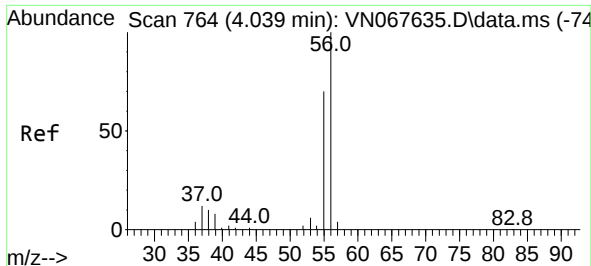

#13
Acrolein
Concen: Below Cal
RT: 4.047 min Scan# 767
Delta R.T. 0.008 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 210
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#

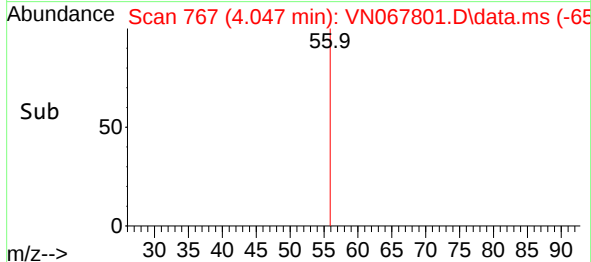

#16
Acetone
Concen: 23.611 ug/l
RT: 4.301 min Scan# 862
Delta R.T. 0.013 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 43 Resp: 34922
Ion Ratio Lower Upper
43 100
58 26.5 21.2 31.8

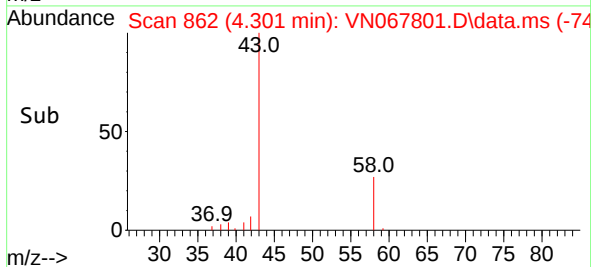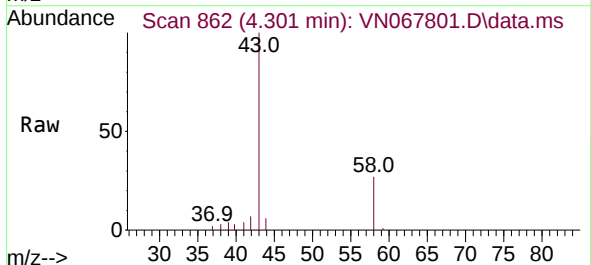

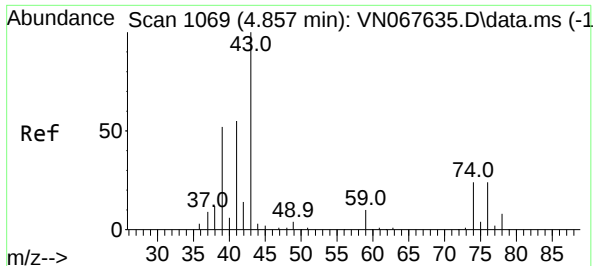

#18

Methyl Acetate

Concen: 1.062 ug/l

RT: 4.857 min Scan# 1069





Delta R.T. -0.000 min

Lab File: VN067801.D

Acq: 19 Jul 2021 18:25

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion: 43 Resp: 4410
Ion Ratio Lower Upper
43 100
74 6.4 17.4 26.0#

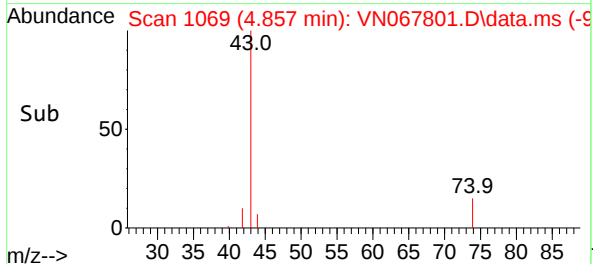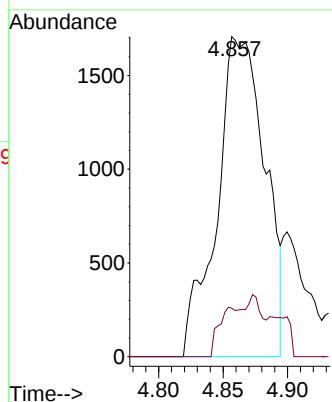

#20

Methylene Chloride

Concen: 7.507 ug/l




RT: 5.098 min Scan# 1159


Delta R.T. 0.008 min

Lab File: VN067801.D

Acq: 19 Jul 2021 18:25

Tgt Ion: 84 Resp: 27964
Ion Ratio Lower Upper
84 100
49 125.0 110.9 166.3
51 37.6 32.6 49.0
86 62.5 51.6 77.4


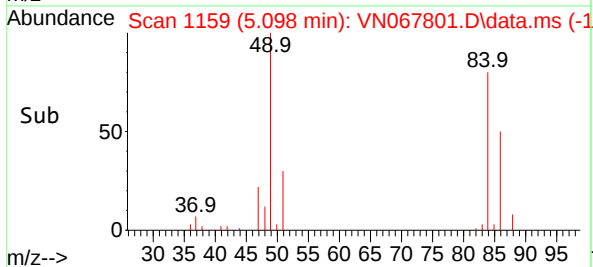

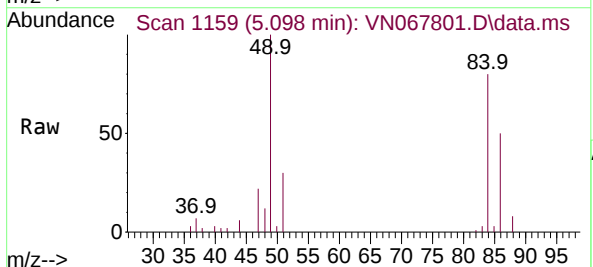


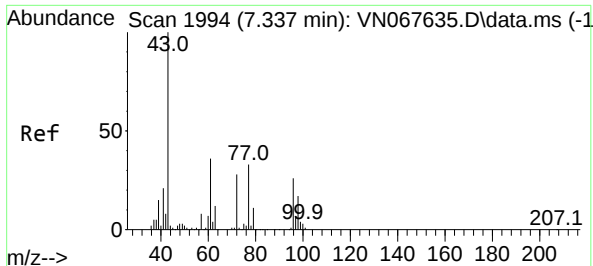

#25
2-Butanone
Concen: 3.229 ug/l
RT: 7.354 min Scan# 2000
Delta R.T. 0.017 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 7931
Ion Ratio Lower Upper
43 100
72 21.4 19.7 29.5

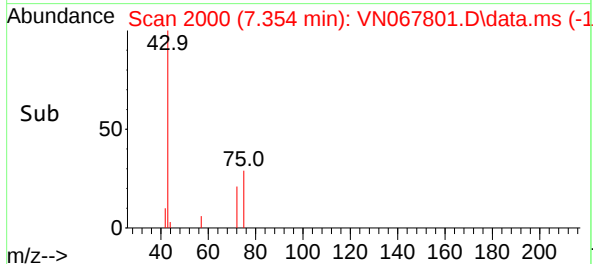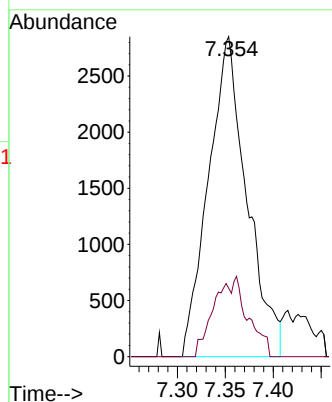

#29
Tetrahydrofuran
Concen: 1.282 ug/l
RT: 7.697 min Scan# 2128
Delta R.T. 0.008 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 42 Resp: 2071
Ion Ratio Lower Upper
42 100
72 86.9 32.8 49.2#
71 76.7 31.2 46.8#


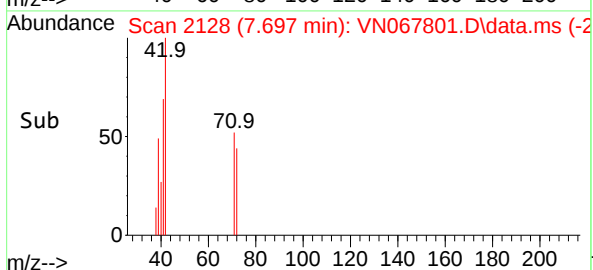

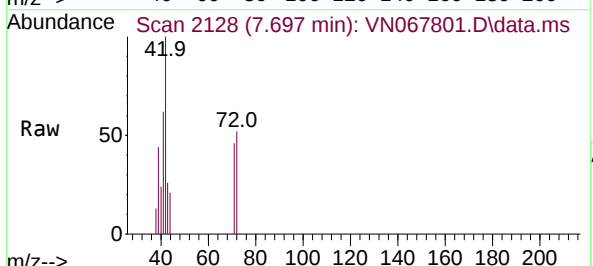


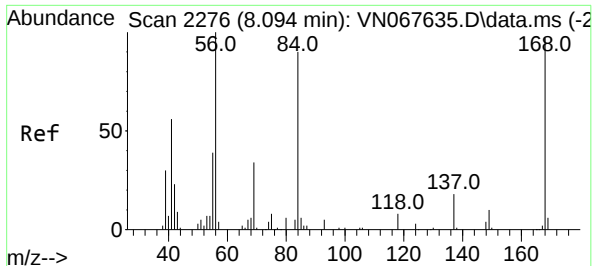

#31
Cyclohexane
Concen: 1.274 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.008 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 8399
Ion Ratio Lower Upper
56 100
69 152.3 27.3 40.9#
84 106.4 64.9 97.3#

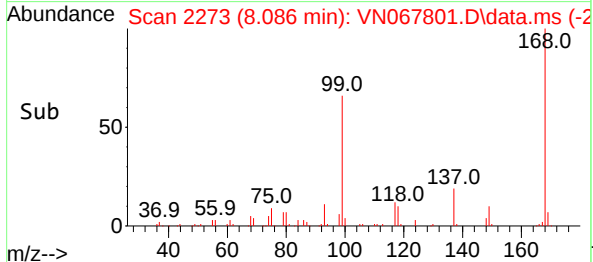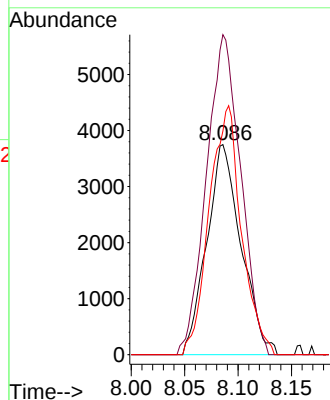

#33
1,2-Dichloroethane-d4
Concen: 53.176 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 65 Resp: 249958
Ion Ratio Lower Upper
65 100
67 50.4 0.0 98.6

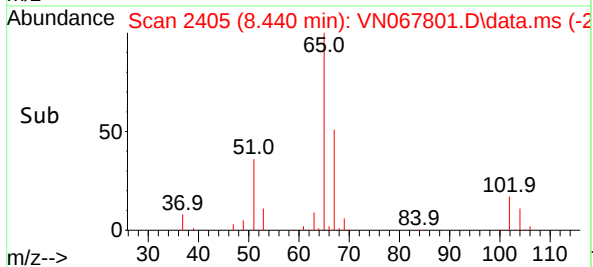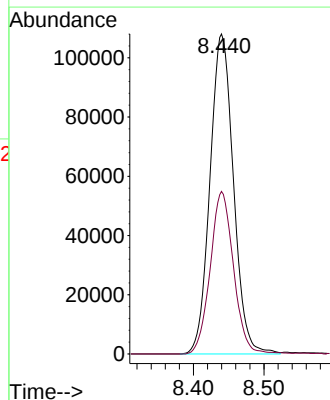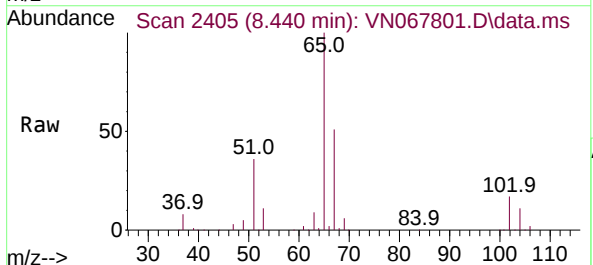




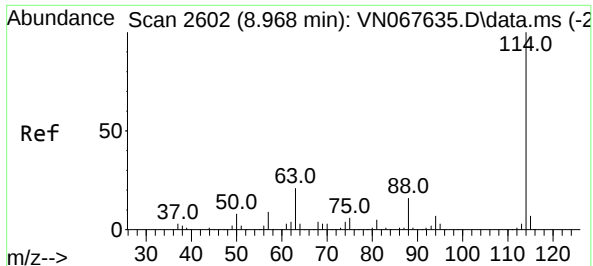


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion:114 Resp: 595532
Ion Ratio Lower Upper
114 100
63 21.4 0.0 49.0
88 15.6 0.0 36.6

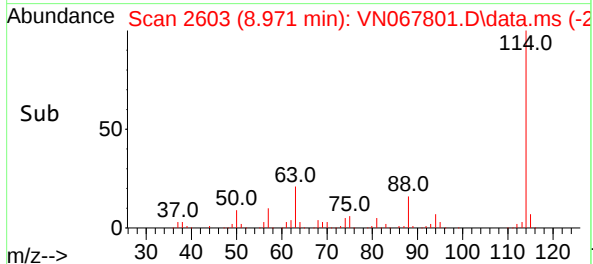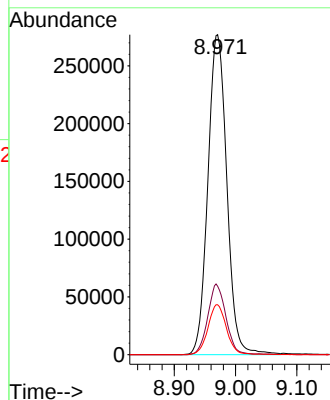


#35

Dibromofluoromethane
Concen: 50.122 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion:113 Resp: 180342
Ion Ratio Lower Upper
113 100
111 103.9 83.8 125.8
192 16.2 13.4 20.0

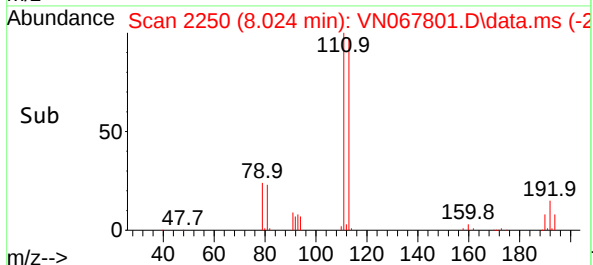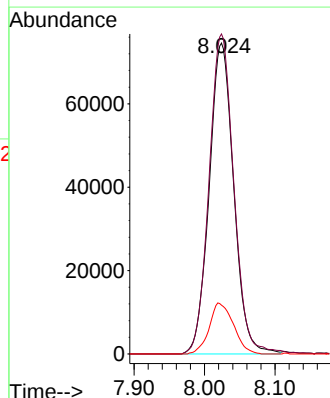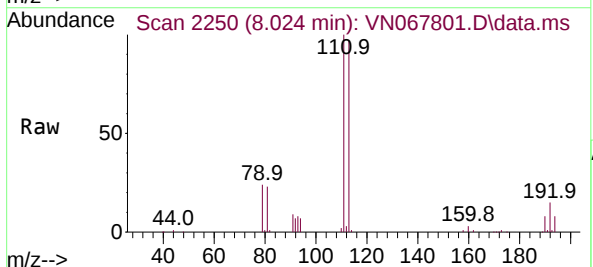


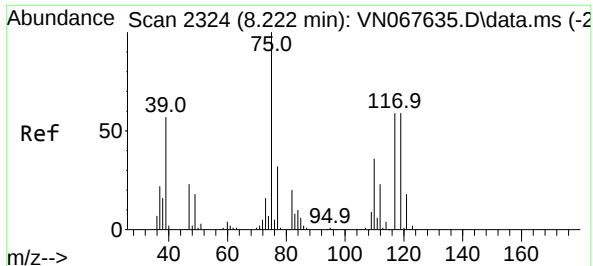




#36

1,1-Dichloropropene
Concen: 5.344 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.139 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Instrument :
MSVOA_N
ClientSampled :






Tgt Ion:	75	Resp:	29563
Ion Ratio	Lower	Upper	
75	100		
110	9.6	15.7	47.0#
77	0.0	24.6	37.0#

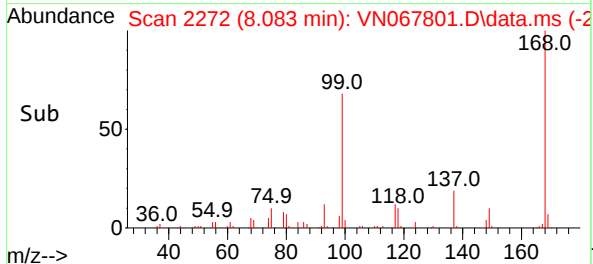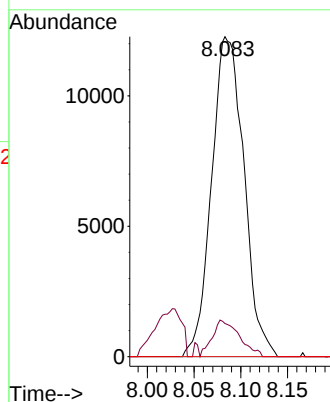


#37

Ethyl Acetate
Concen: 1.480 ug/l
RT: 7.354 min Scan# 2000
Delta R.T. -0.064 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25


Tgt Ion:	43	Resp:	7931
Ion Ratio	Lower	Upper	
43	100		
61	0.0	10.6	16.0#
70	0.0	8.1	12.1#

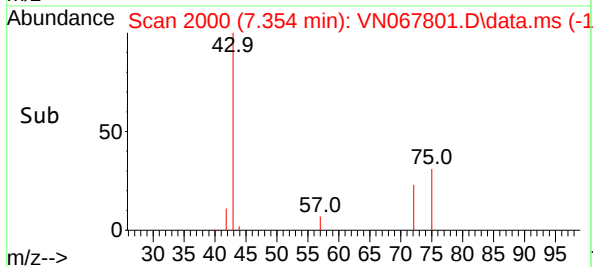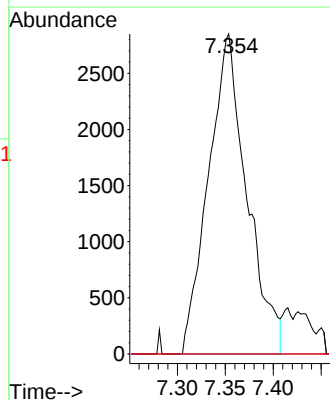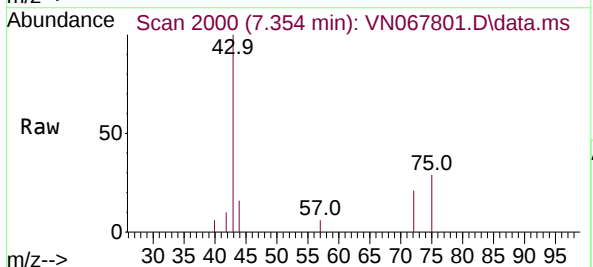



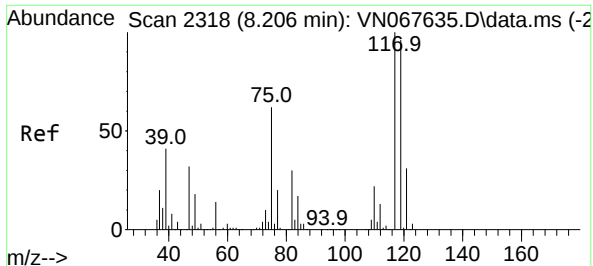


#38
Carbon Tetrachloride
Concen: 6.232 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25


Instrument :
MSVOA_N
ClientSampleId :

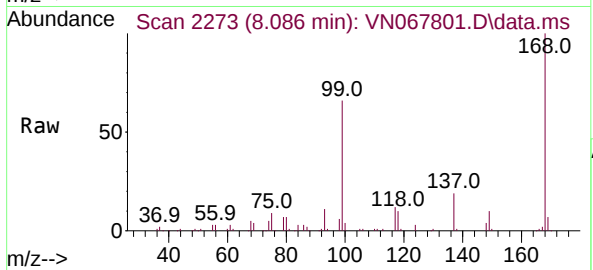



Tgt Ion: 117 Resp: 34008
Ion Ratio Lower Upper
117 100
119 6.2 75.4 113.2#
121 0.0 23.5 35.3#

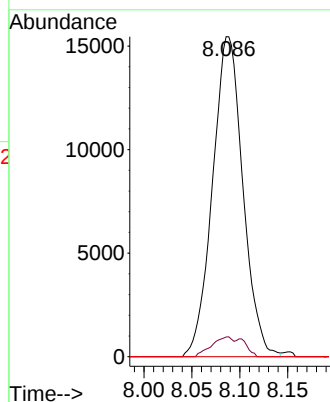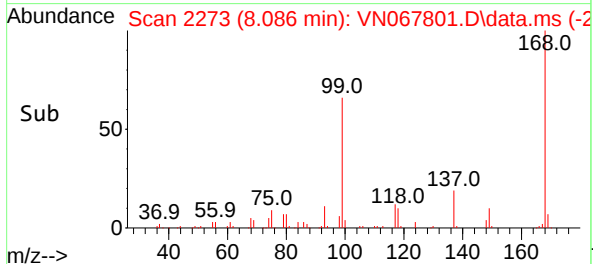


#41
Methacrylonitrile
Concen: 0.993 ug/l
RT: 7.705 min Scan# 2131
Delta R.T. 0.065 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

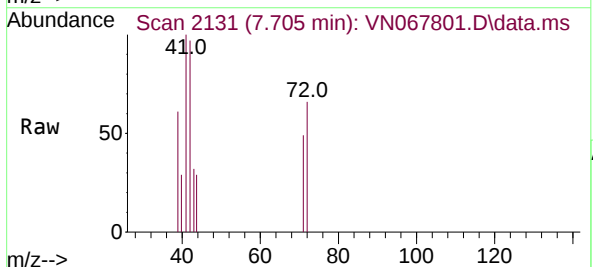

Tgt Ion: 41 Resp: 2736
Ion Ratio Lower Upper
41 100
39 62.9 47.6 71.4
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#



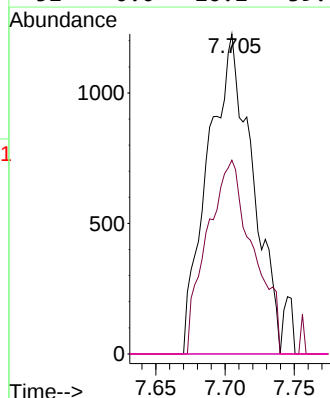





#43
Isopropyl Acetate
Concen: 4.291 ug/l
RT: 8.569 min Scan# 2453
Delta R.T. 0.006 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion	Ratio	Lower	Upper
43	100		
61	18.2	19.0	28.4#
87	7.9	9.5	14.3#

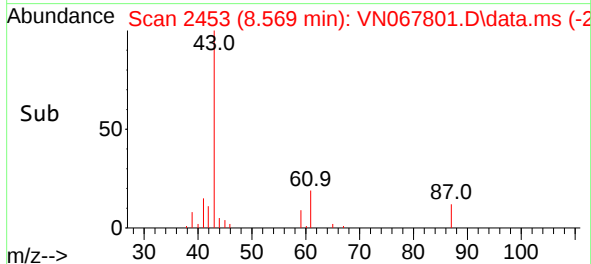

#45
1,2-Dichloropropane
Concen: 0.619 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion	Ratio	Lower	Upper
63	100		
65	0.0	24.3	36.5#


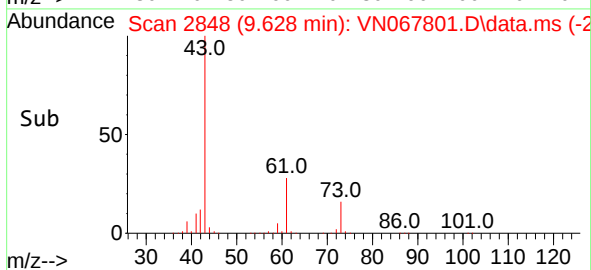

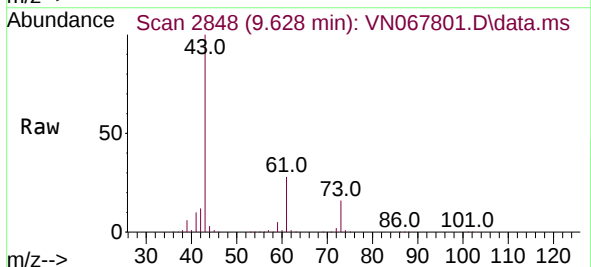


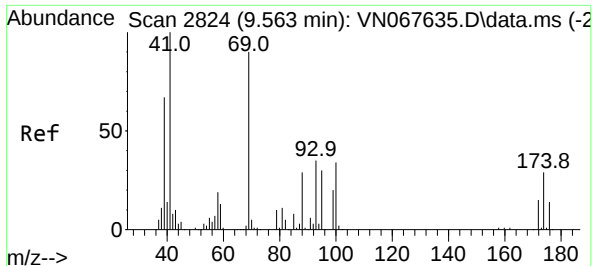

#48
Methyl methacrylate
Concen: 2.390 ug/l
RT: 9.550 min Scan# 2819
Delta R.T. -0.013 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 9965
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

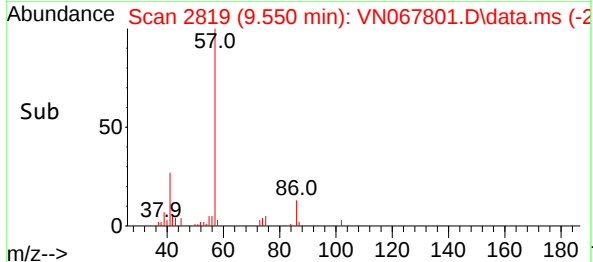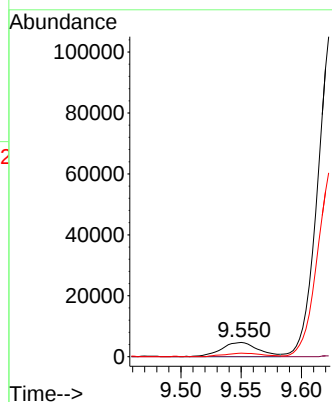

#49
1,4-Dioxane
Concen: 35.551 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.057 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 88 Resp: 293
Ion Ratio Lower Upper
88 100
43 708123.2 28.8 43.2#
58 2991.8 60.4 90.6#


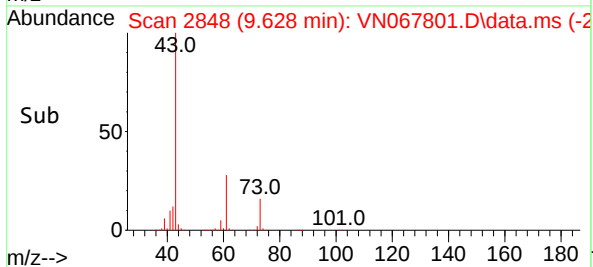

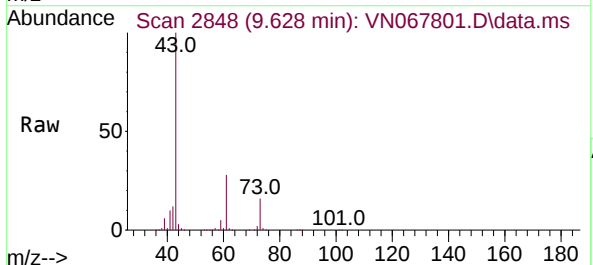


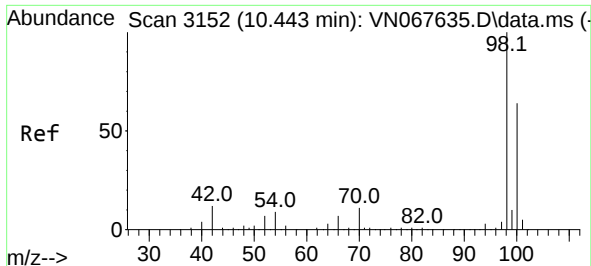

#50
Toluene-d8
Concen: 52.490 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. 0.003 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 790525
Ion Ratio Lower Upper
98 100
100 62.8 51.7 77.5

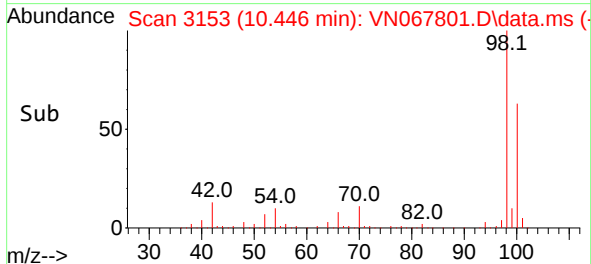

#51
4-Methyl-2-Pentanone
Concen: 1.660 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 43 Resp: 9618
Ion Ratio Lower Upper
43 100
58 42.7 28.6 43.0


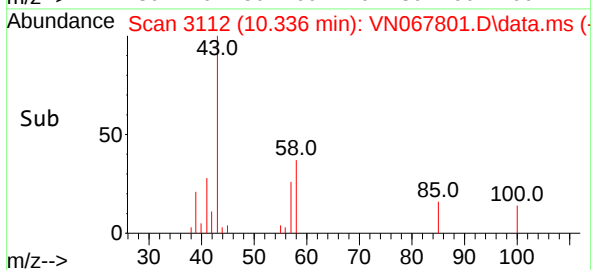

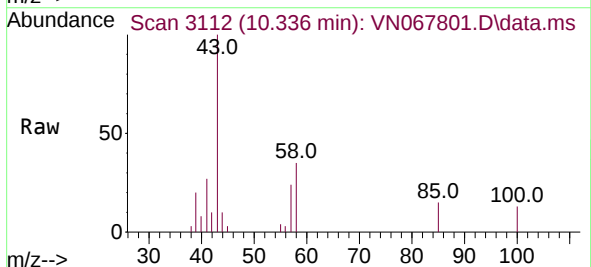


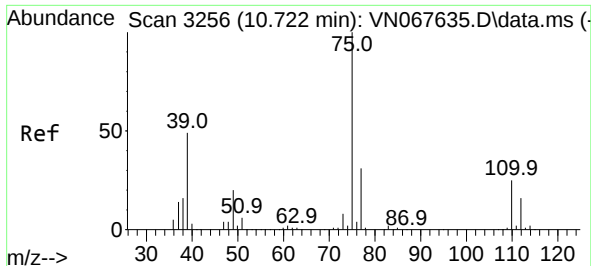

#53
t-1,3-Dichloropropene
Concen: 1.770 ug/l
RT: 10.454 min Scan# 3156
Delta R.T. -0.268 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 184
Ion Ratio Lower Upper
75 100
77 120.9 25.1 37.7#

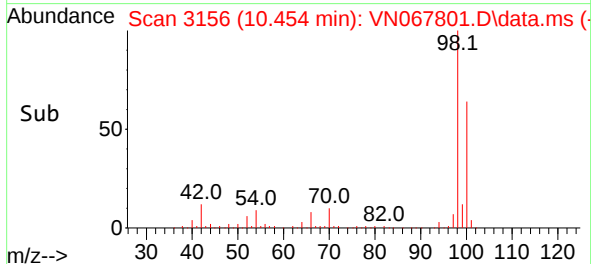

#54
cis-1,3-Dichloropropene
Concen: 10.243 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 75 Resp: 66246
Ion Ratio Lower Upper
75 100
77 0.6 24.6 37.0#
39 38.4 50.7 76.1#


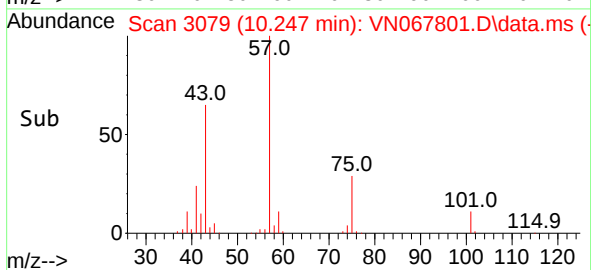

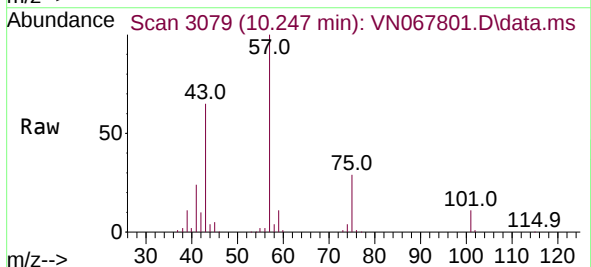


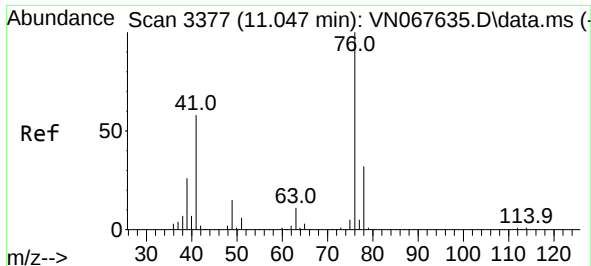

#57
1,3-Dichloropropane
Concen: 5.415 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 38598
Ion Ratio Lower Upper
76 100
78 0.1 25.7 38.5#

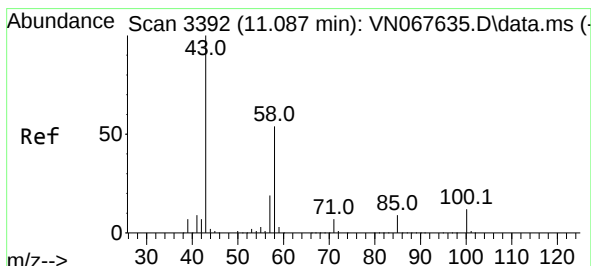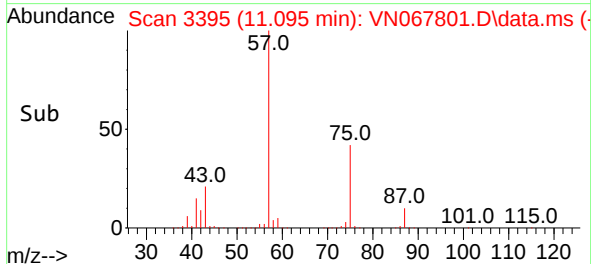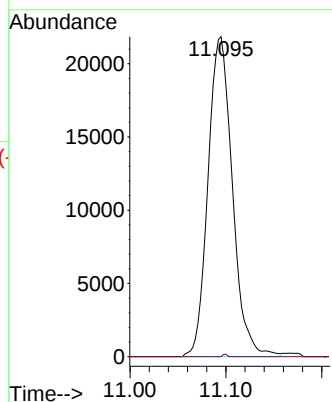

#59
2-Hexanone
Concen: 143.764 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 43 Resp: 581261
Ion Ratio Lower Upper
43 100
58 17.5 24.7 74.1#




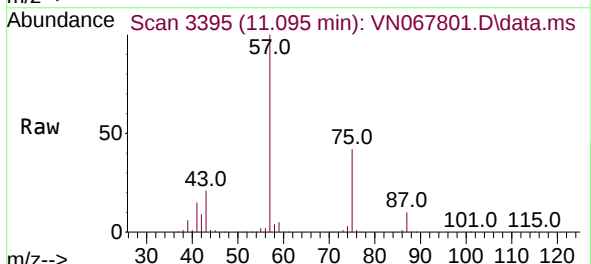


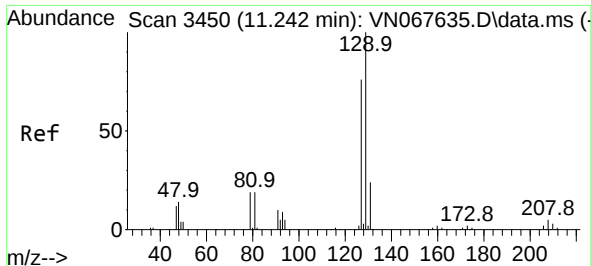

#60
Dibromochloromethane
Concen: 2.403 ug/l
RT: 11.495 min Scan# 3544
Delta R.T. 0.253 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 248
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

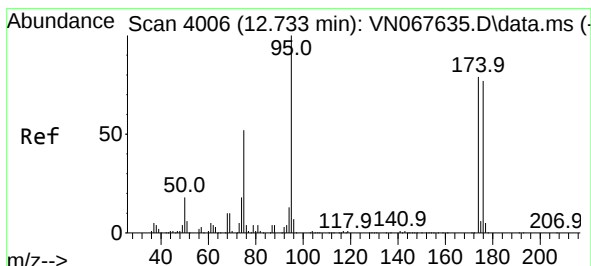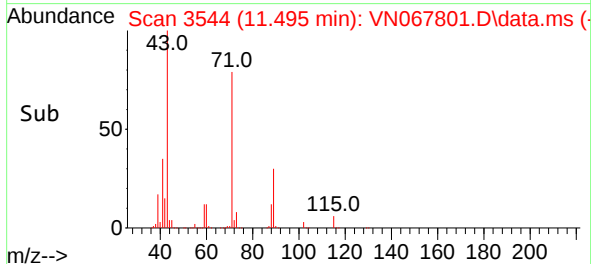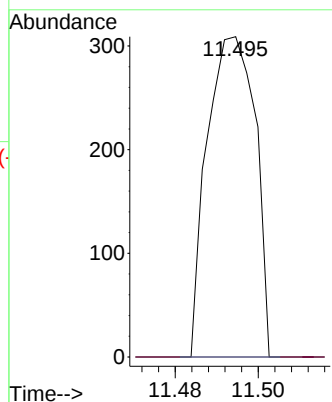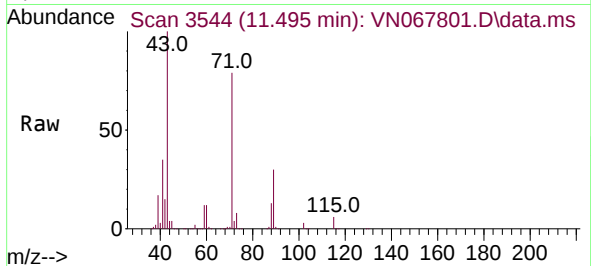

#62
4-Bromofluorobenzene
Concen: 50.444 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion: 95 Resp: 268372
Ion Ratio Lower Upper
95 100
174 70.3 0.0 122.0
176 67.5 0.0 117.6




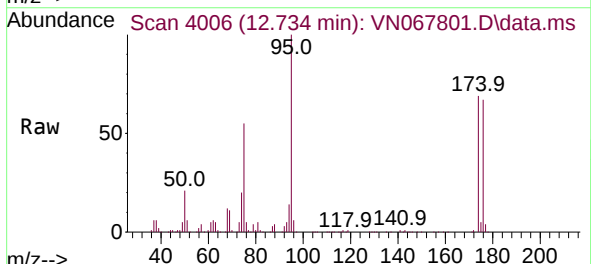




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 614801
Ion Ratio Lower Upper
117 100
82 57.1 53.1 79.7
119 32.5 25.5 38.3

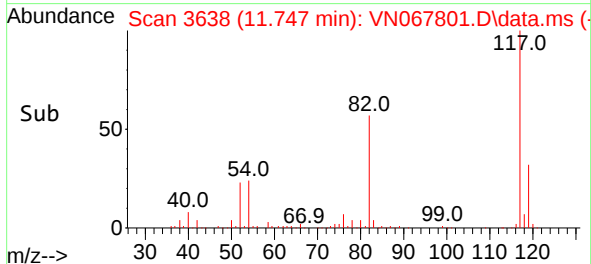

#71
Bromoform
Concen: 3.196 ug/l
RT: 12.712 min Scan# 3998
Delta R.T. 0.252 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion:173 Resp: 86
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0


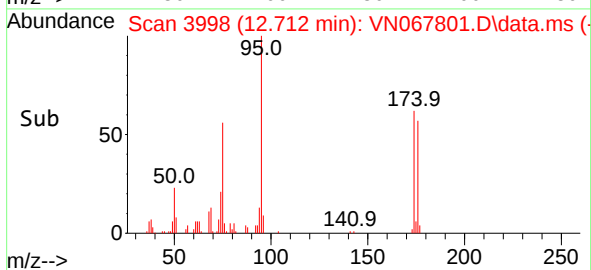

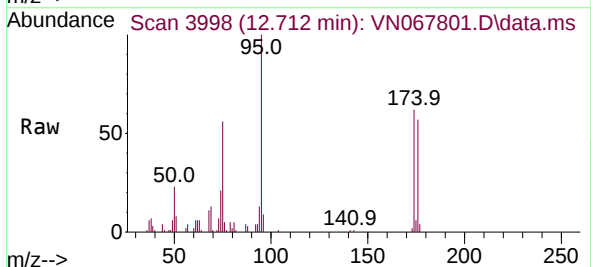


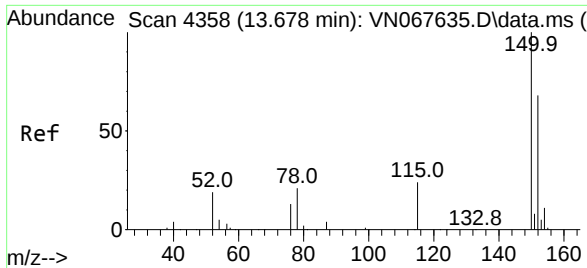

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 4358
 Delta R.T. 0.000 min
 Lab File: VN067801.D
 Acq: 19 Jul 2021 18:25




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion:152 Resp: 220956
 Ion Ratio Lower Upper
 152 100
 115 63.4 36.1 108.5
 150 159.7 0.0 351.8

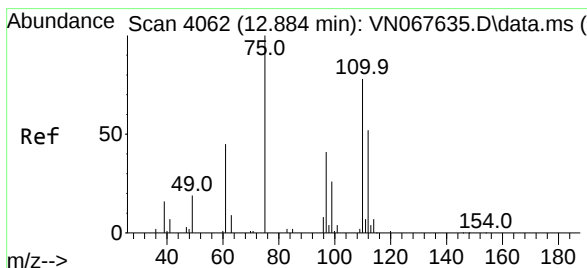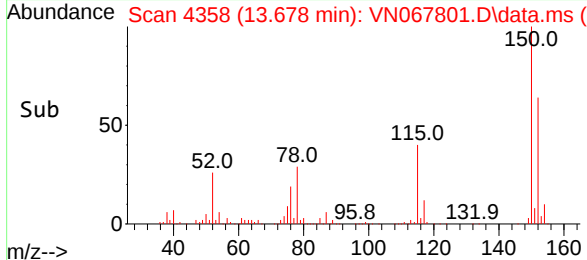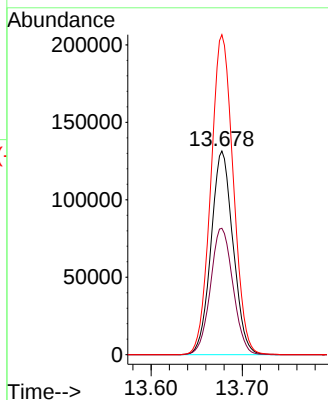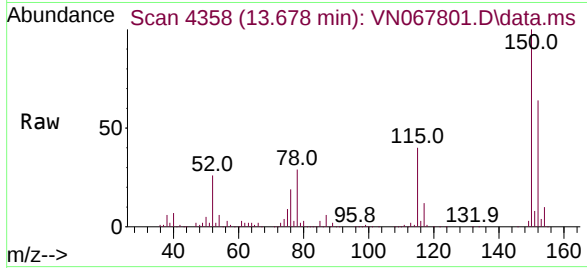

#76
 1,2,3-Trichloropropane
 Concen: 32.650 ug/l
 RT: 12.734 min Scan# 4006
 Delta R.T. -0.150 min
 Lab File: VN067801.D
 Acq: 19 Jul 2021 18:25


Tgt Ion: 75 Resp: 147329
 Ion Ratio Lower Upper
 75 100
 77 1.1 0.0 0.0#

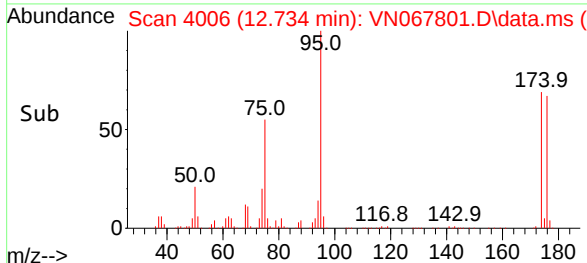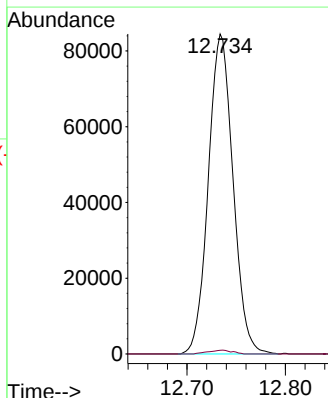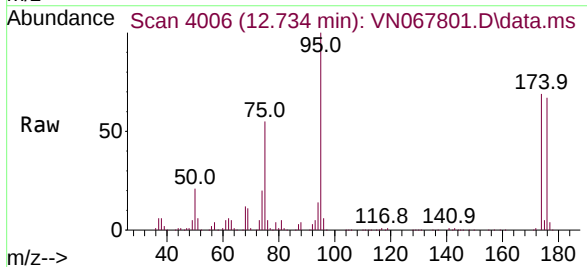






#81
trans-1,4-Dichloro-2-butene
Concen: 105.268 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25


Instrument :
MSVOA_N
ClientSampled :

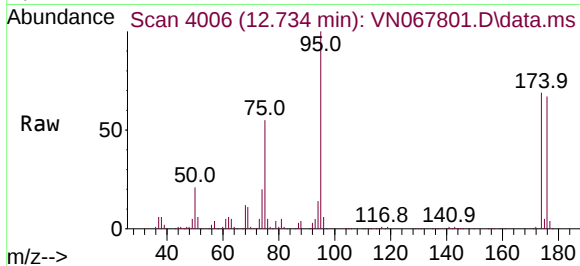



Tgt Ion: 75 Resp: 147329
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

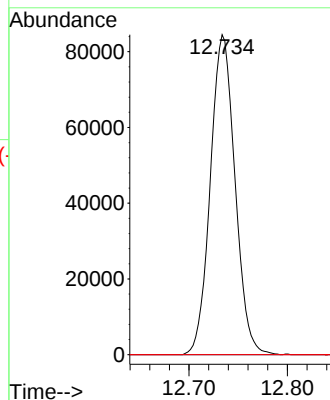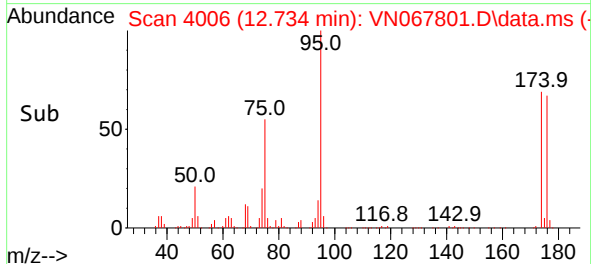


#93
1,2,4-Trichlorobenzene
Concen: 2.706 ug/l
RT: 15.260 min Scan# 4948
Delta R.T. -0.005 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

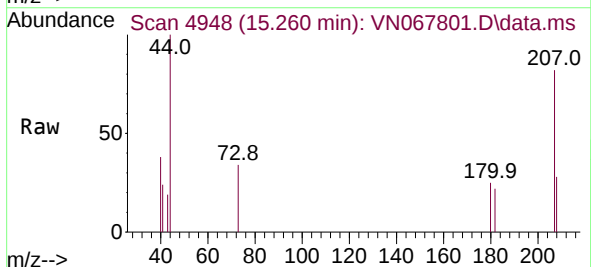

Tgt Ion:180 Resp: 124
Ion Ratio Lower Upper
180 100
182 177.4 47.5 142.5#
145 0.0 17.2 51.6#



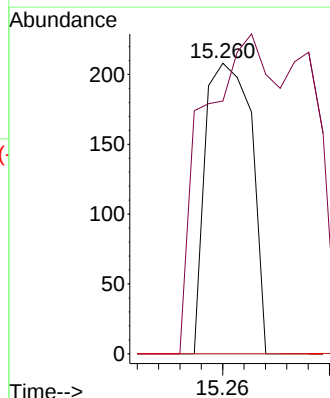



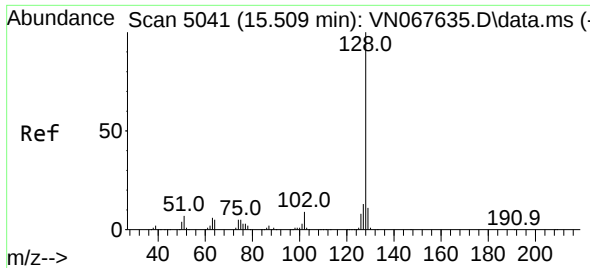

#95
Naphthalene
Concen: 3.100 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion:128	Resp:	1007
Ion Ratio	Lower	Upper
128	100	
127	5.5	10.6 15.8#
129	8.3	8.6 12.8#

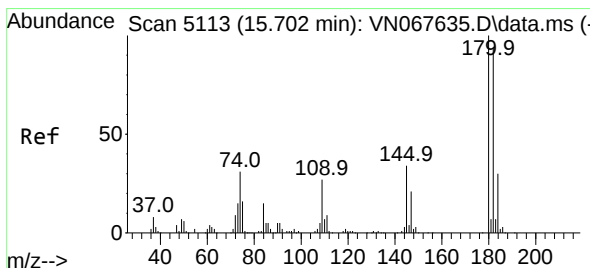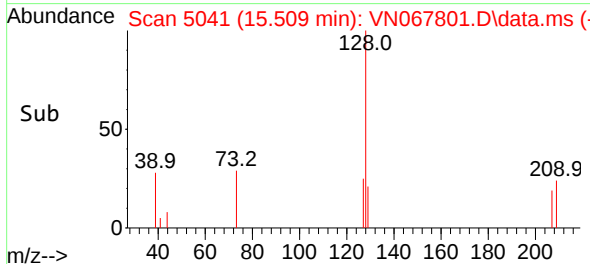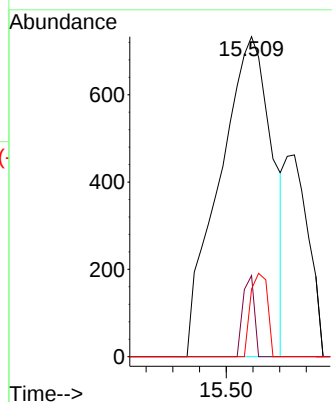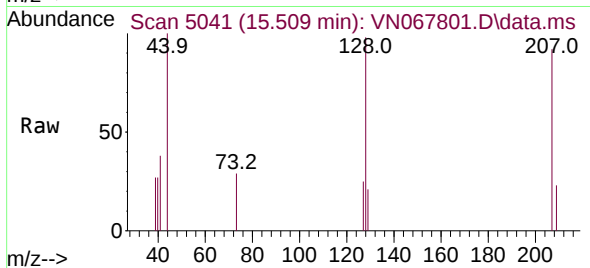

#96
1,2,3-Trichlorobenzene
Concen: 2.655 ug/l
RT: 15.697 min Scan# 5111
Delta R.T. -0.005 min
Lab File: VN067801.D
Acq: 19 Jul 2021 18:25

Tgt Ion:180	Resp:	83
Ion Ratio	Lower	Upper
180	100	
182	0.0	47.8 143.3#
145	0.0	18.2 54.6#

