
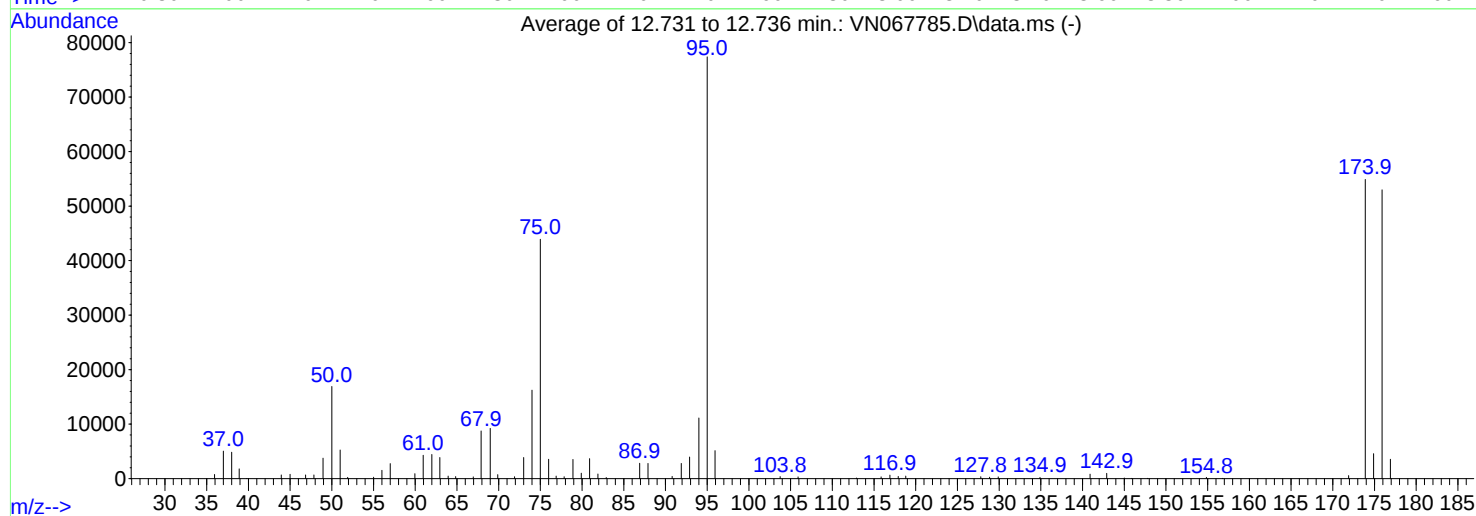


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071921\
 Data File : VN067785.D
 Acq On : 19 Jul 2021 10:01
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Title : SW846 8260
 Last Update : Wed Jul 07 16:18:53 2021

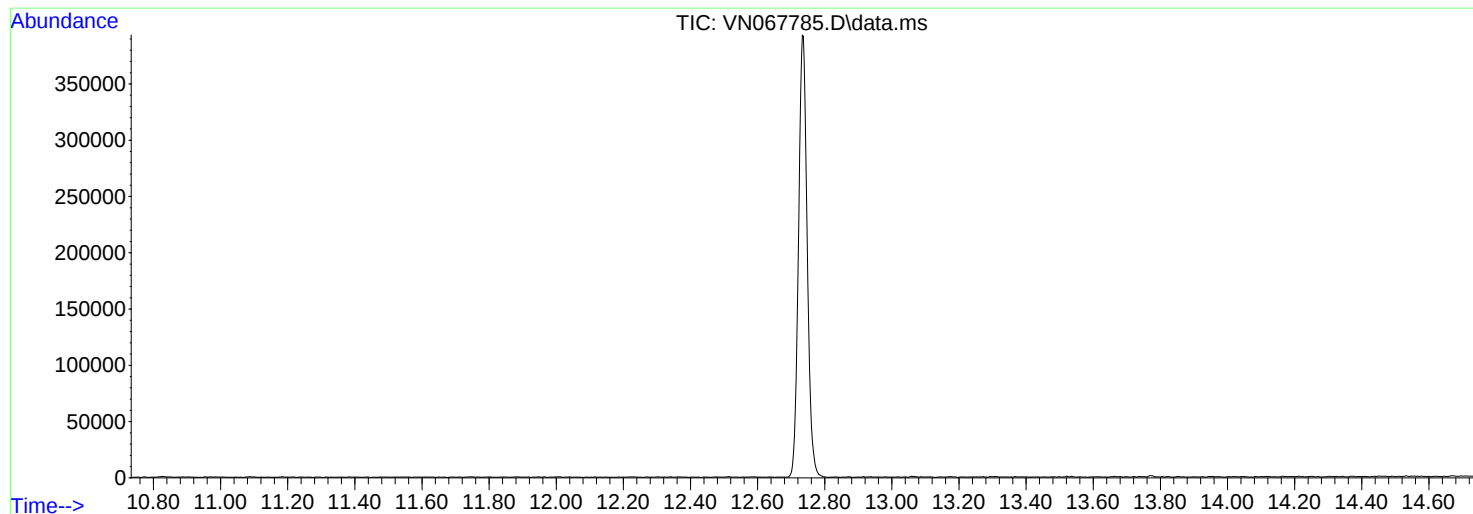

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	16915	PASS
75	95	30	60	56.7	43901	PASS
95	95	100	100	100.0	77379	PASS
96	95	5	9	6.6	5145	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.9	54893	PASS
175	174	5	9	8.4	4594	PASS
176	174	95	101	96.5	52971	PASS
177	176	5	9	6.7	3548	PASS