
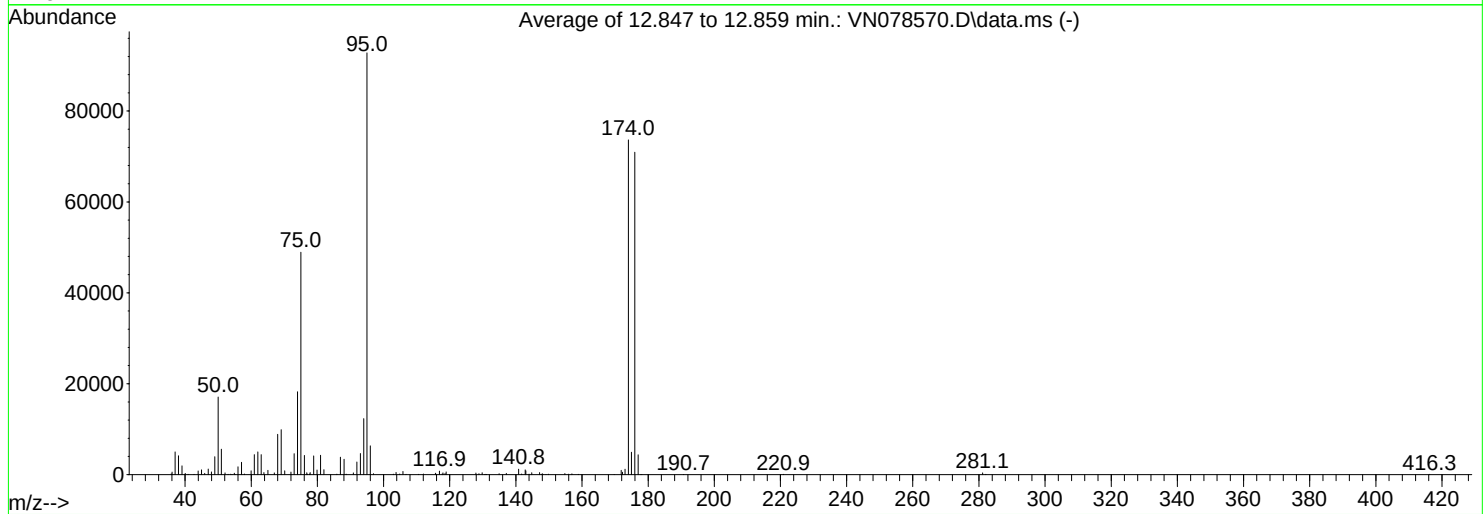


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071923\
Data File : VN078570.D
Acq On : 19 Jul 2023 09:56
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

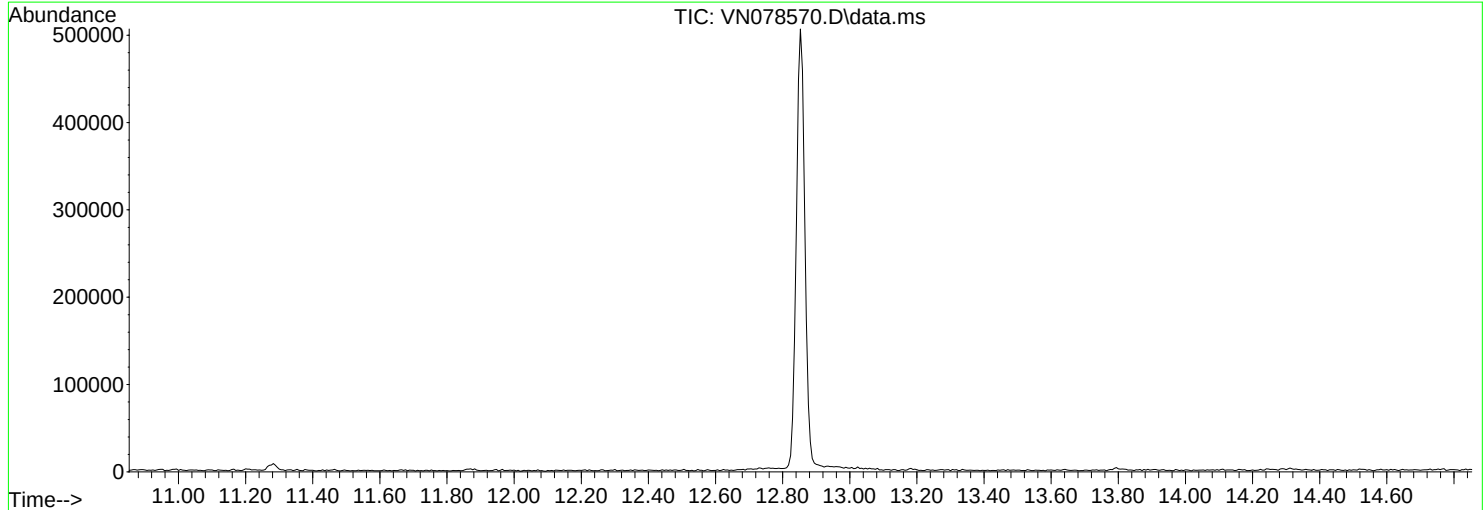

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	17069	PASS
75	95	30	60	52.7	48920	PASS
95	95	100	100	100.0	92803	PASS
96	95	5	9	6.8	6320	PASS
173	174	0.00	2	1.6	1210	PASS
174	95	50	100	79.4	73645	PASS
175	174	5	9	6.7	4913	PASS
176	174	95	101	96.3	70949	PASS
177	176	5	9	6.1	4357	PASS

Average of 12.847 to 12.859 min.: VN078570.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	171	45.95	280	55.10	50	68.00	887
36.05	551	47.00	1224	56.00	1720	69.05	987
37.00	5019	47.95	618	57.05	2716	70.10	85
38.00	4159	49.00	3936	57.95	135	72.00	54
39.05	1925	50.00	17069	59.95	834	72.95	4618
39.90	126	50.95	5610	60.95	4415	74.00	18221
40.10	256	52.05	387	62.00	5019	75.00	48920
40.90	56	53.00	85	63.00	4409	76.05	4213
42.70	72	53.80	120	63.85	467	76.80	412
43.95	830	54.20	52	65.05	951	77.00	95
44.95	1071	54.90	304	66.95	375	77.60	159

Average of 12.847 to 12.859 min.: VN078570.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
77.80	452	93.00	4661	112.05	141	130.60	55
78.85	4132	94.00	12339	115.70	311	130.90	85
79.90	1020	95.00	92803	115.90	126	131.10	52
80.95	4248	96.00	6320	116.90	786	134.95	215
81.95	1093	96.95	198	117.70	145	137.10	280
85.90	98	102.95	110	117.95	386	140.85	1198
86.95	3847	103.80	496	118.60	243	141.75	130
88.05	3377	104.90	156	118.95	588	142.80	1062
88.70	113	105.85	693	127.90	360	143.00	837
90.85	397	106.80	78	128.85	196	144.00	97
91.95	2784	110.60	56	129.80	443	144.80	441

Average of 12.847 to 12.859 min.: VN078570.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.20	458	171.85	951	281.10	394		
147.70	85	172.25	541	282.10	72		
148.00	199	173.00	1210	416.30	56		
148.20	79	174.00	73645				
149.10	51	174.95	4913				
149.85	112	175.95	70949				
154.80	234	176.95	4357				
155.90	92	177.80	53				
156.95	185	178.10	53				
158.90	74	190.70	53				
169.70	51	220.90	70				