
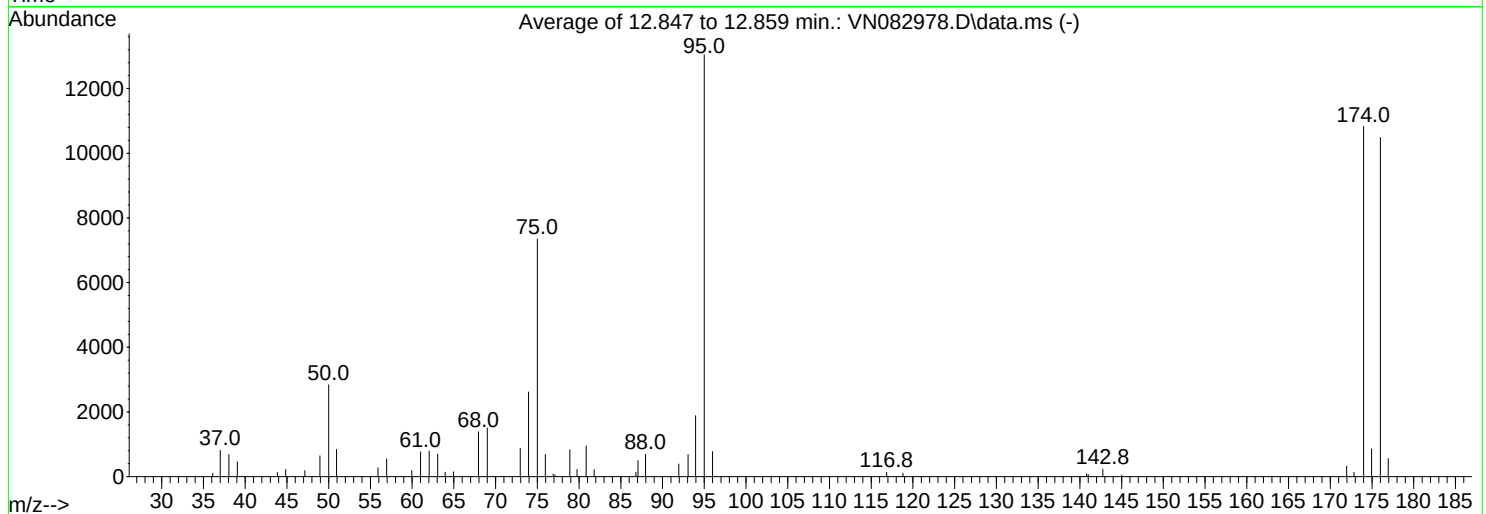


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN071924\
Data File : VN082978.D
Acq On : 19 Jul 2024 09:42
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070824W.M
Title : SW846 8260
Last Update : Mon Jul 08 13:46:04 2024

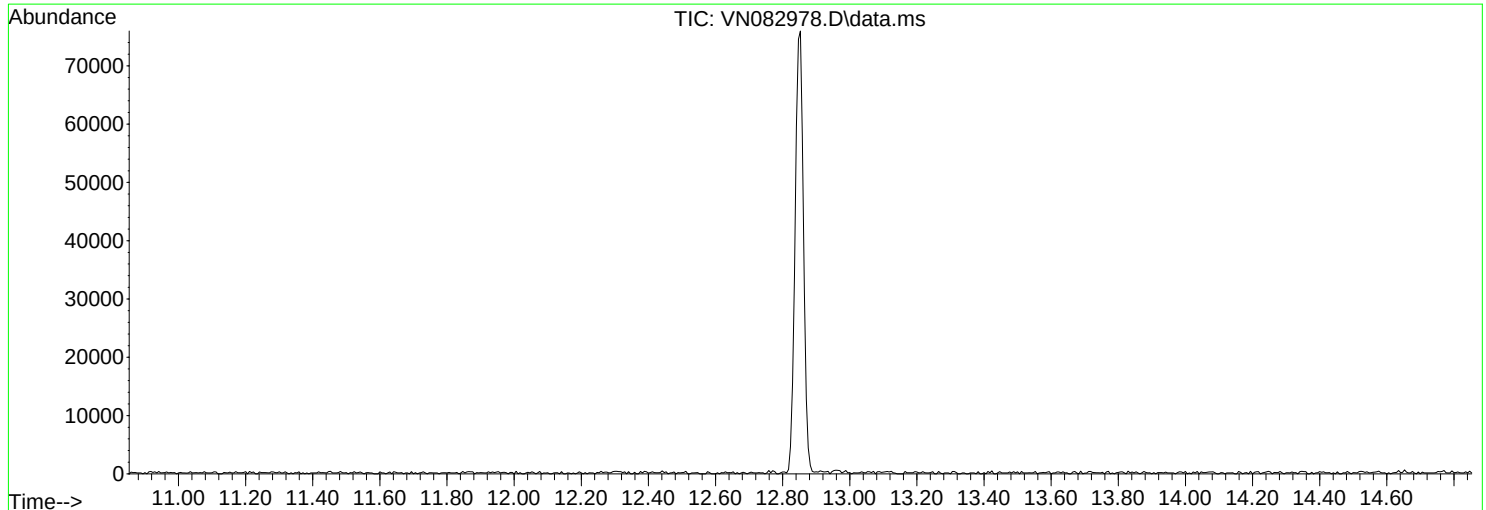

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	2839	PASS
75	95	30	60	56.4	7352	PASS
95	95	100	100	100.0	13041	PASS
96	95	5	9	5.9	773	PASS
173	174	0.00	2	1.2	134	PASS
174	95	50	100	83.0	10823	PASS
175	174	5	9	7.9	854	PASS
176	174	95	101	96.9	10490	PASS
177	176	5	9	5.3	559	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.10	102	56.95	548	75.00	7352	91.95	381
37.00	814	59.95	188	75.95	688	93.05	681
38.05	682	61.00	766	76.90	78	93.95	188
39.05	460	62.05	791	77.10	55	95.00	1304
43.85	130	63.05	700	78.90	833	96.00	773
44.85	223	63.95	141	79.75	221	116.85	134
47.15	188	64.95	151	80.85	952	118.80	109
48.95	644	67.95	1386	81.80	217	140.80	85
50.00	2839	69.00	1502	86.80	138	141.00	63
50.95	842	72.95	874	87.05	495	142.75	226
55.90	271	73.95	2615	87.95	695	145.00	50

Average of 12.847 to 12.859 min.: VN082978.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
171.95	323						
172.85	134						
174.00	10823						
174.95	854						
176.00	10490						
176.95	559						

Instrument :

MSVOA_N

ClientSampleId :

BFB