


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN072018\
 Data File : VN049981.D
 Acq On : 21 Jul 2018 00:44
 Operator : MD\SY
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N071818W.M
 Title : SW846 8260
 Last Update : Thu Jul 19 01:58:39 2018

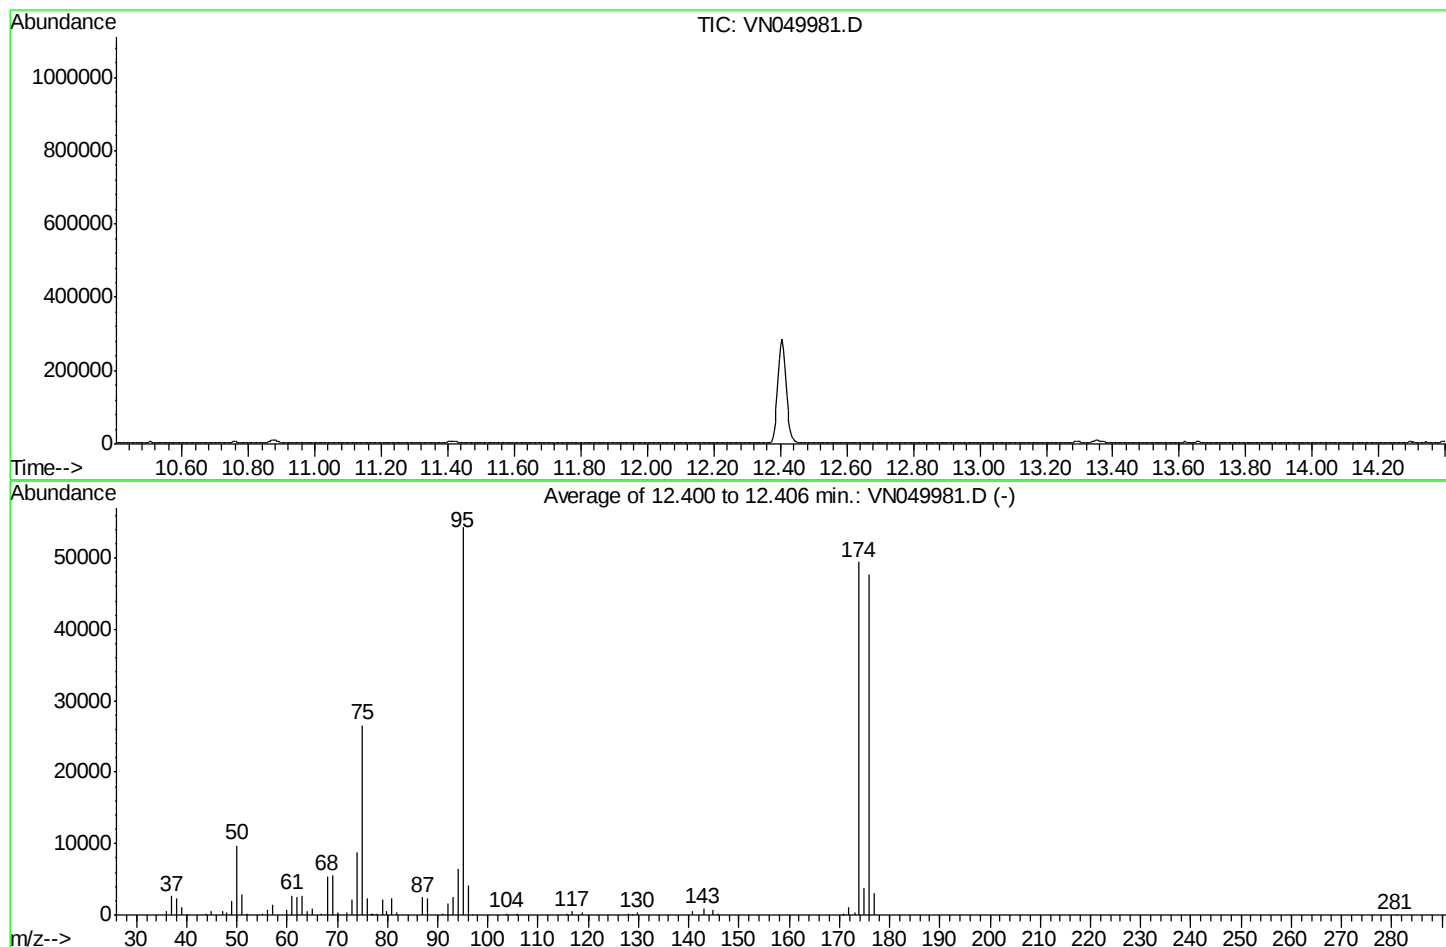

AutoFind: Scans 3362, 3363, 3364; Background Corrected with Scan 3349

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	9765	PASS
75	95	30	60	49.0	26589	PASS
95	95	100	100	100.0	54290	PASS
96	95	5	9	7.5	4052	PASS
173	174	0.00	2	0.7	352	PASS
174	95	50	100	91.1	49437	PASS
175	174	5	9	7.5	3707	PASS
176	174	95	101	96.5	47693	PASS
177	176	5	9	6.4	3042	PASS