

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072020\
 Data File : VN062560.D
 Acq On : 20 Jul 2020 14:28
 Operator : JC/MD
 Sample : IBLK
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 IBLK

Quant Time: Jul 21 01:27:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N071320W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Tue Jul 14 00:52:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Bromochloromethane	7.15	128	44651	30.00	ug/l	0.00
28) 1,4-Difluorobenzene	8.55	114	237321	30.00	ug/l	0.00
57) Chlorobenzene-d5	11.38	117	216483	30.00	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	7.99	65	118453	30.88	ug/l	0.00
Spiked Amount	30.000	Range	50 - 169	Recovery	=	102.93%
60) 4-Bromofluorobenzene	12.38	95	96093	26.08	ug/l	0.00
Spiked Amount	30.000	Range	56 - 143	Recovery	=	86.93%
63) Toluene-d8	10.06	98	307035	30.01	ug/l	0.00
Spiked Amount	30.000	Range	66 - 137	Recovery	=	100.03%


Target Compounds	Ovalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN072020\
Data File : VN062560.D
Acq On : 20 Jul 2020 14:28
Operator : JC/MD
Sample : IBLK
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
IBLK

Quant Time: Jul 21 01:27:00 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA N\METHODS\624N071320W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Tue Jul 14 00:52:57 2020
Response via : Initial Calibration

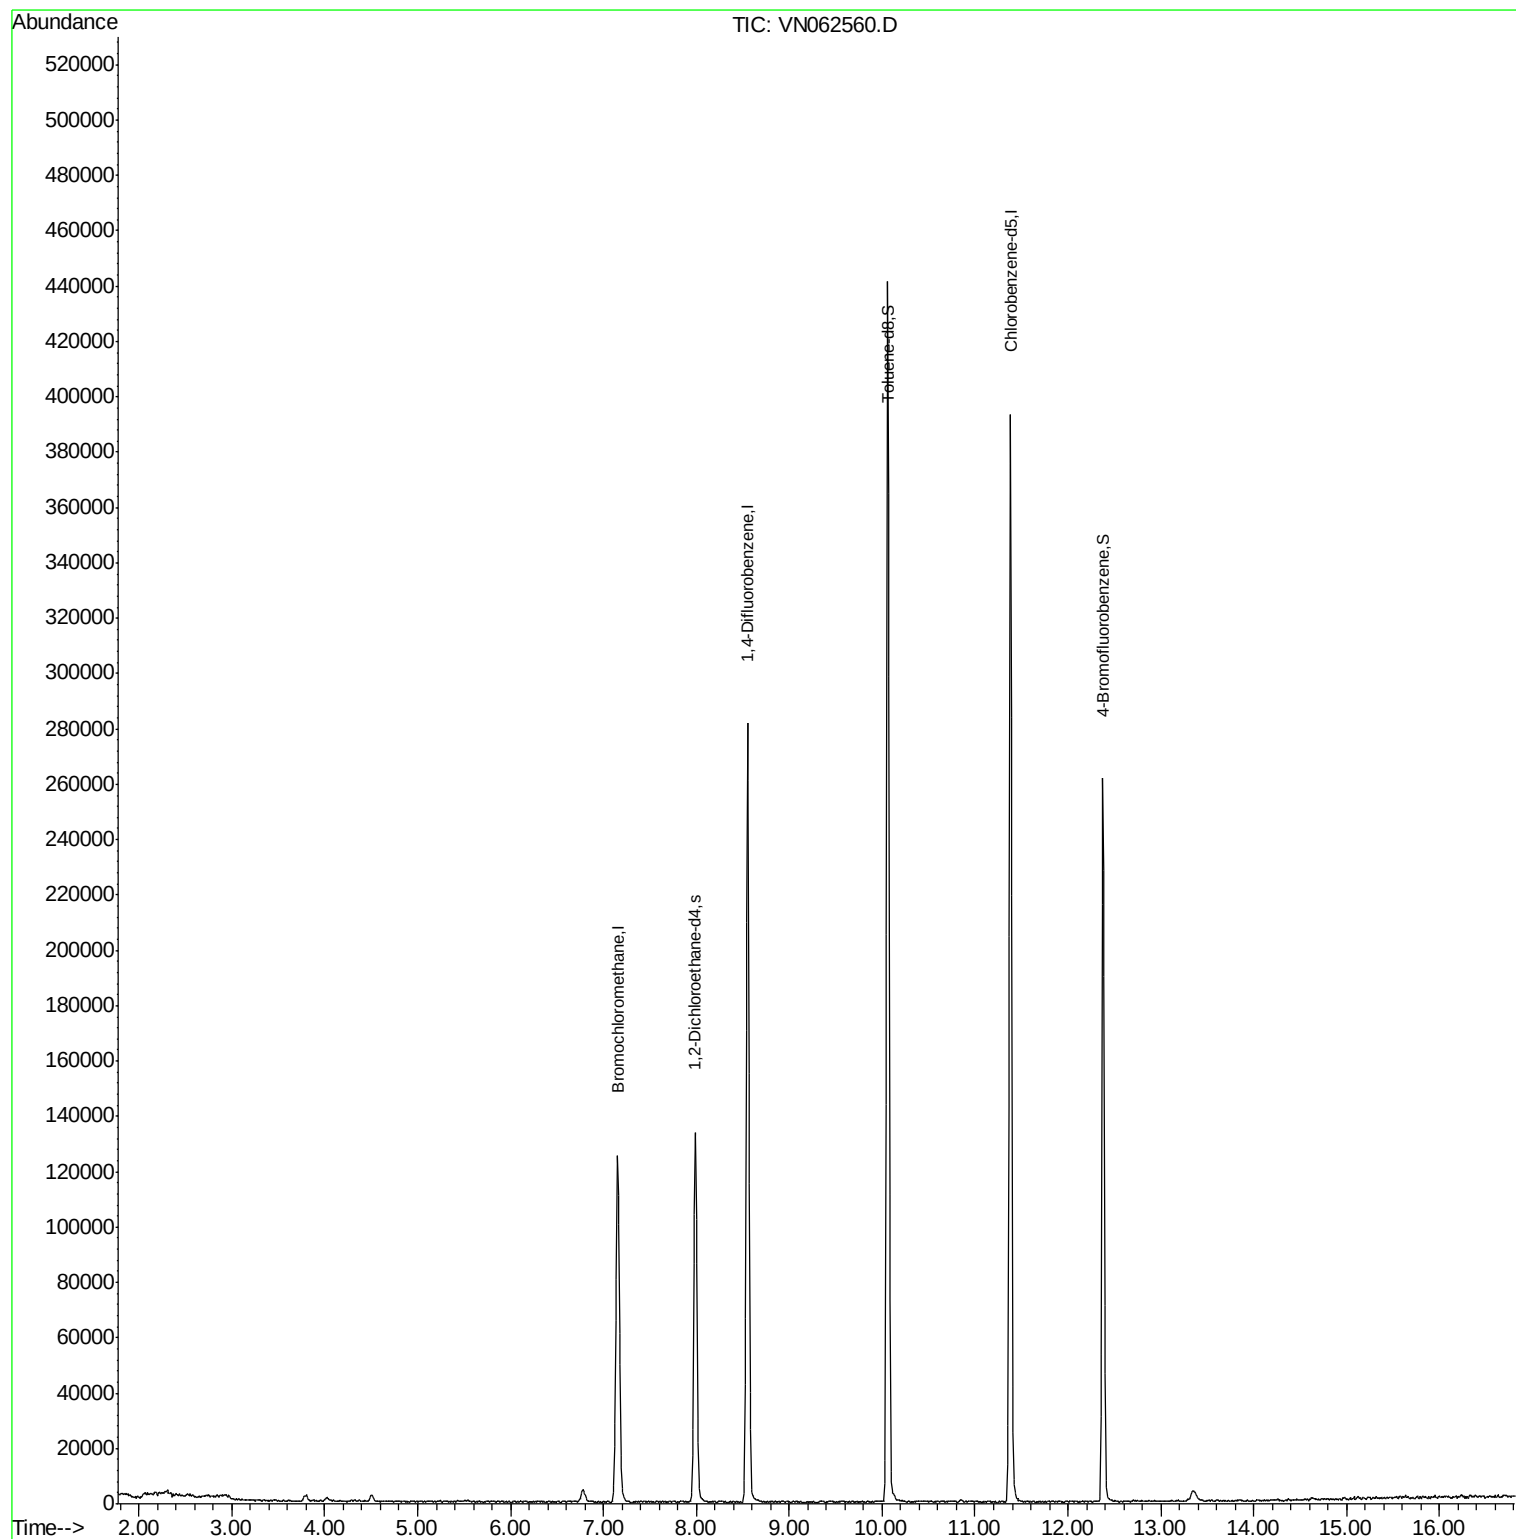

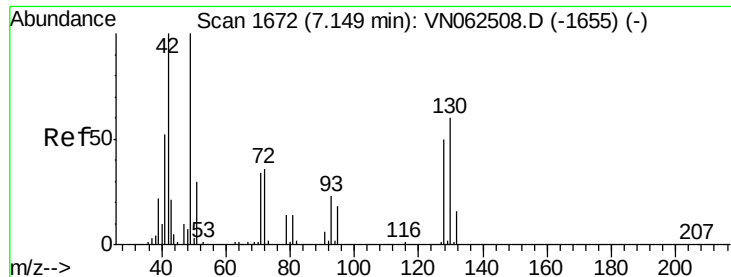

#1

Bromochloromethane

Concen: 30.000 ug/l

RT: 7.15 min Scan# 1673

Delta R.T. 0.00 min

Lab File: VN062560.D

Acq: 20 Jul 2020 14:28

Instrument :

MSVOA_N

ClientSampled :

IBLK


Tot Ion:128 Resp: 44651

Ion Ratio Lower Upper

128 100

49 208.3 0.0 525.0




130 131.4 0.0 319.8

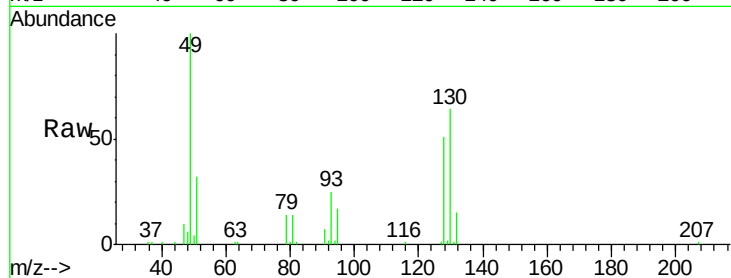

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 49.00 (48.70 to 49.70): VN0

Ion 130.00 (129.70 to 130.70): V

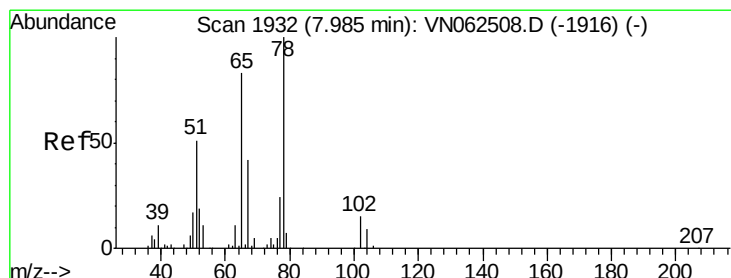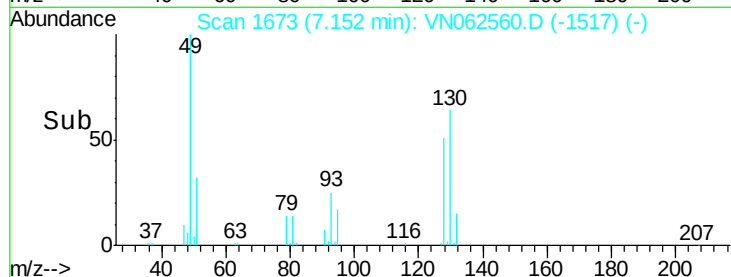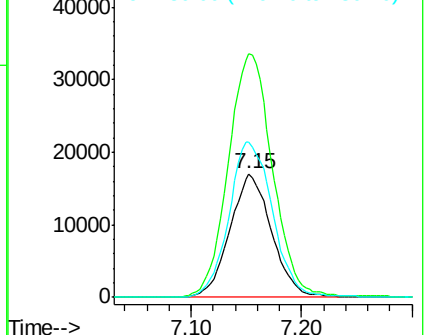

#27

1,2-Dichloroethane-d4

Concen: 30.881 ug/l

RT: 7.99 min Scan# 1933

Delta R.T. 0.00 min

Lab File: VN062560.D


Acq: 20 Jul 2020 14:28

Tgt Ion: 65 Resp: 118453

Ion Ratio Lower Upper



65 100


67 52.3 41.7 62.5

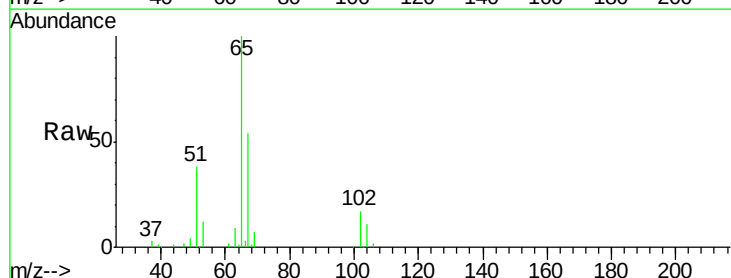

Abundance Ion 65.00 (64.70 to 65.70): VN0

Ion 67.00 (66.70 to 67.70): VN0



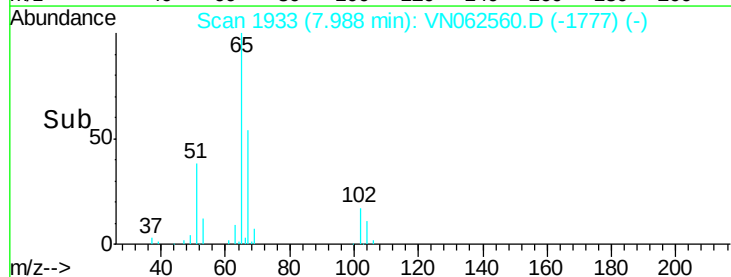
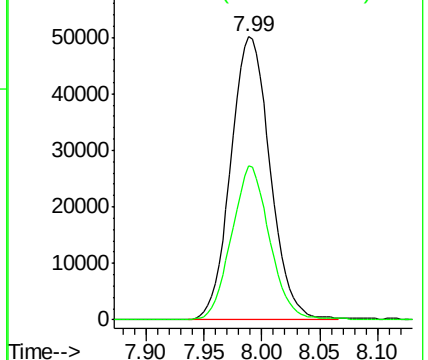


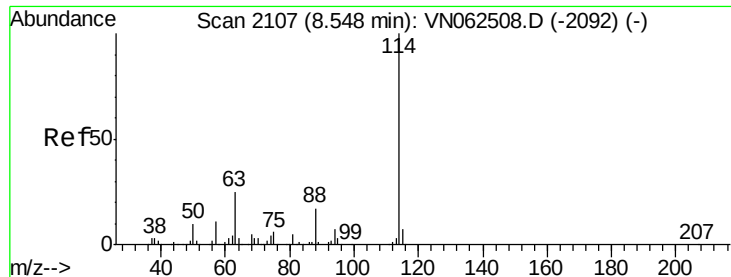

#28
 1,4-Difluorobenzene
 Concen: 30.000 ug/l
 RT: 8.55 min Scan# 2108
 Delta R.T. 0.00 min
 Lab File: VN062560.D
 Acq: 20 Jul 2020 14:28




Instrument :
 MSVOA_N
 ClientSampled :
 IBLK


Tot Ion	Ratio	Lower	Upper
114	100		
63	24.0	19.4	29.0
88	17.3	13.5	20.3

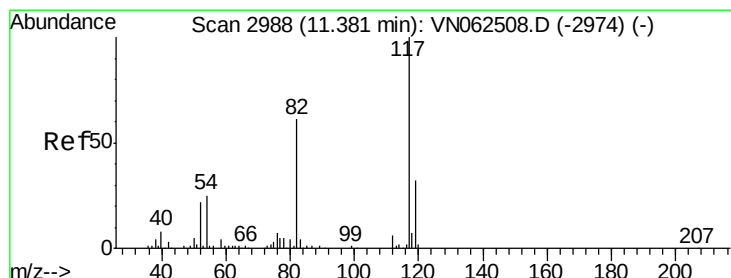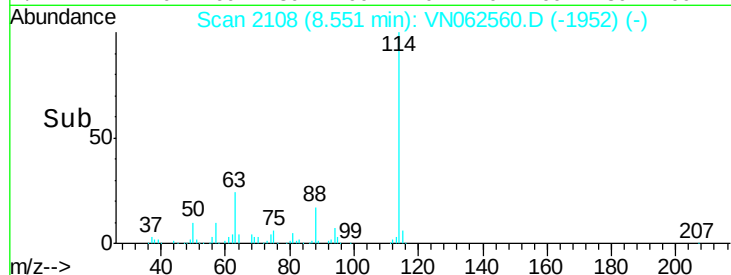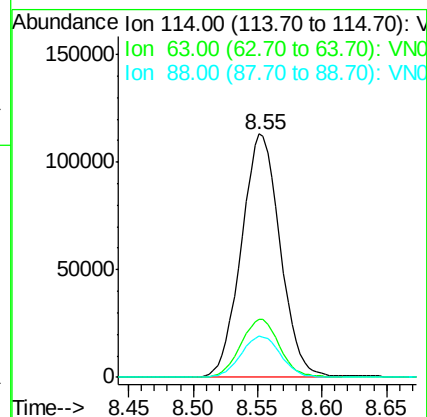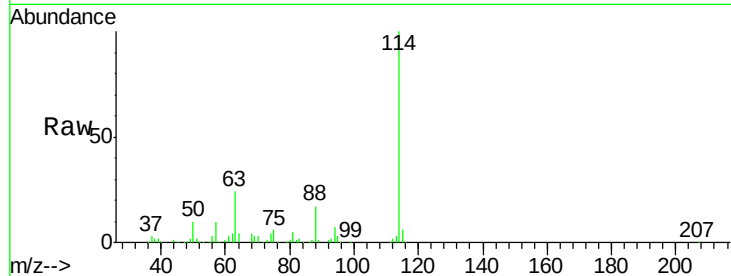

#57
 Chlorobenzene-d5
 Concen: 30.000 ug/l
 RT: 11.38 min Scan# 2988
 Delta R.T. -0.00 min
 Lab File: VN062560.D
 Acq: 20 Jul 2020 14:28

Tgt Ion	Ratio	Lower	Upper
117	100		
82	61.5	49.0	73.6
119	31.9	25.6	38.4


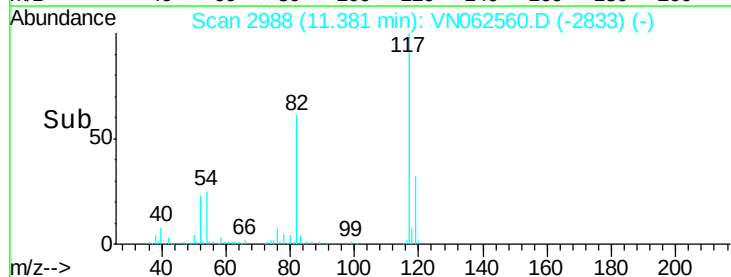
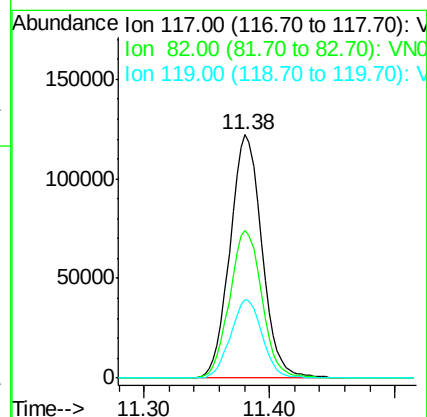
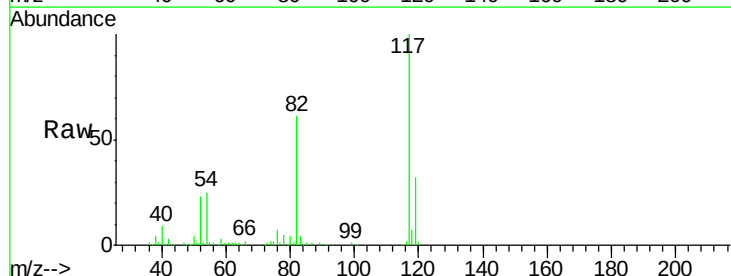


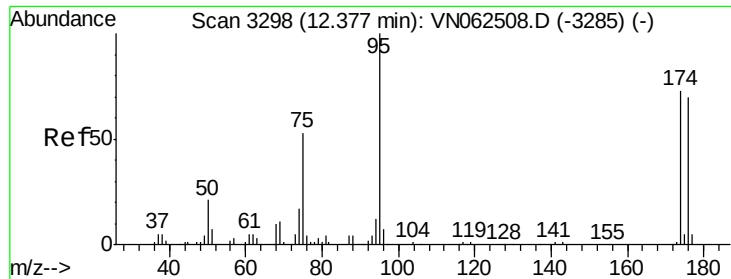

#60
 4-Bromofluorobenzene
 Concen: 26.084 ug/l
 RT: 12.38 min Scan# 3298
 Delta R.T. -0.00 min
 Lab File: VN062560.D
 Acq: 20 Jul 2020 14:28

Instrument :
 MSVOA_N
 ClientSampled :
 IBLK

Tot Ion: 95 Resp: 96093
 Ion Ratio Lower Upper
 95 100
 174 71.8 57.5 86.3
 176 69.9 56.3 84.5

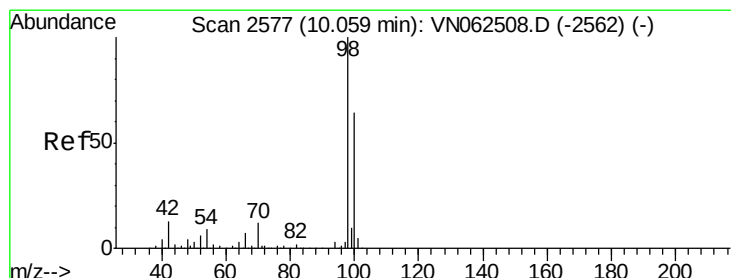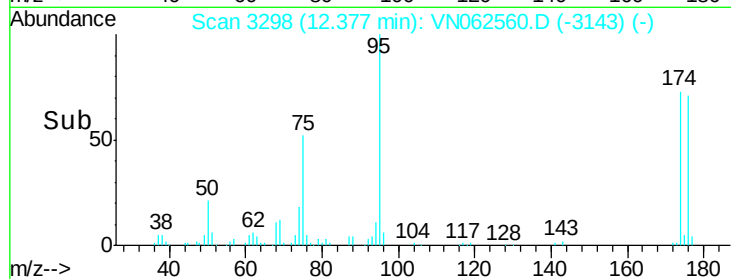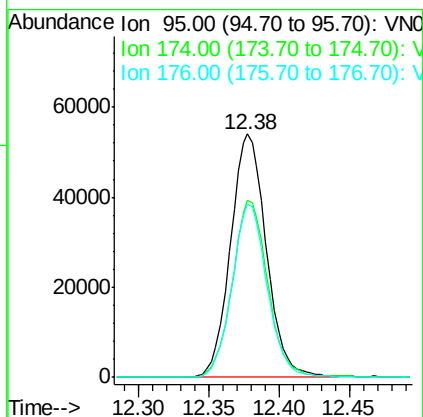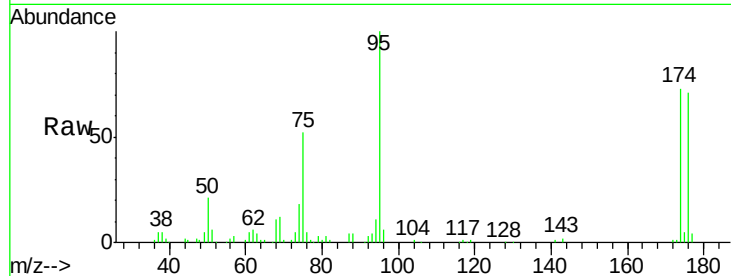

#63
 Toluene-d8
 Concen: 30.015 ug/l
 RT: 10.06 min Scan# 2578
 Delta R.T. 0.00 min
 Lab File: VN062560.D
 Acq: 20 Jul 2020 14:28

Tgt Ion: 98 Resp: 307035
 Ion Ratio Lower Upper
 98 100
 100 62.4 50.4 75.6

