

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072021\
 Data File : VN067820.D
 Acq On : 20 Jul 2021 16:23
 Operator : JC/MD
 Sample : PB137795ZHE#01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 21 05:08:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	333493	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.971	114	634420	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	649566	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	229930	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	262032	51.989	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 103.980%	
35) Dibromofluoromethane	8.024	113	191993	50.089	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 100.180%	
50) Toluene-d8	10.443	98	820615	51.148	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 102.300%	
62) 4-Bromofluorobenzene	12.734	95	282480	49.841	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 99.680%	


Target Compounds			Qvalue			
5) Bromomethane	2.840	94	206	Below Cal	#	4
6) Chloroethane	3.038	64	56	Below Cal	#	44
7) Trichlorofluoromethane	3.376	101	25	Below Cal	#	18
13) Acrolein	4.036	56	145	Below Cal	#	75
16) Acetone	4.293	43	25204	15.892	ug/l	# 87
18) Methyl Acetate	4.867	43	3124	0.701	ug/l	# 70
20) Methylene Chloride	5.093	84	27401	6.800	ug/l	90
25) 2-Butanone	7.356	43	5622	2.135	ug/l	97
29) Tetrahydrofuran	7.694	42	1003	0.579	ug/l	# 65
31) Cyclohexane	8.083	56	8814	1.247	ug/l	# 18
36) 1,1-Dichloropropene	8.088	75	30565	5.187	ug/l	# 45
37) Ethyl Acetate	7.356	43	5622	0.985	ug/l	# 69
38) Carbon Tetrachloride	8.086	117	38384	6.603	ug/l	# 16
41) Methacrylonitrile	7.697	41	601	0.205	ug/l	# 41
43) Isopropyl Acetate	8.566	43	41250	4.107	ug/l	# 92
45) 1,2-Dichloropropane	9.628	63	2593	0.581	ug/l	# 44
48) Methyl methacrylate	9.545	41	9215	2.074	ug/l	# 12
49) 1,4-Dioxane	9.620	88	215	34.488	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.336	43	7422	1.203	ug/l	# 66
53) t-1,3-Dichloropropene	10.719	75	89	1.756	ug/l	# 43
54) cis-1,3-Dichloropropene	10.247	75	70537	10.238	ug/l	# 62
57) 1,3-Dichloropropane	11.095	76	44237	5.826	ug/l	# 43
59) 2-Hexanone	11.095	43	653668	151.763	ug/l	# 54
60) Dibromochloromethane	11.478	129	52	2.366	ug/l	# 11
71) Bromoform	12.712	173	124	3.204	ug/l	# 29
74) N-amyl acetate	12.390	43	1576	0.234	ug/l	# 72
76) 1,2,3-Trichloropropane	12.734	75	156814	33.396	ug/l	# 100
80) 1,3,5-Trimethylbenzene	13.061	105	3899	0.259	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.734	75	156814	107.672	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.265	180	1229	2.978	ug/l	87
95) Naphthalene	15.509	128	8226	3.699	ug/l	# 86
96) 1,2,3-Trichlorobenzene	15.711	180	657	2.802	ug/l	# 10


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072021\
Data File : VN067820.D
Acq On : 20 Jul 2021 16:23
Operator : JC/MD
Sample : PB137795ZHE#01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 21 05:08:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

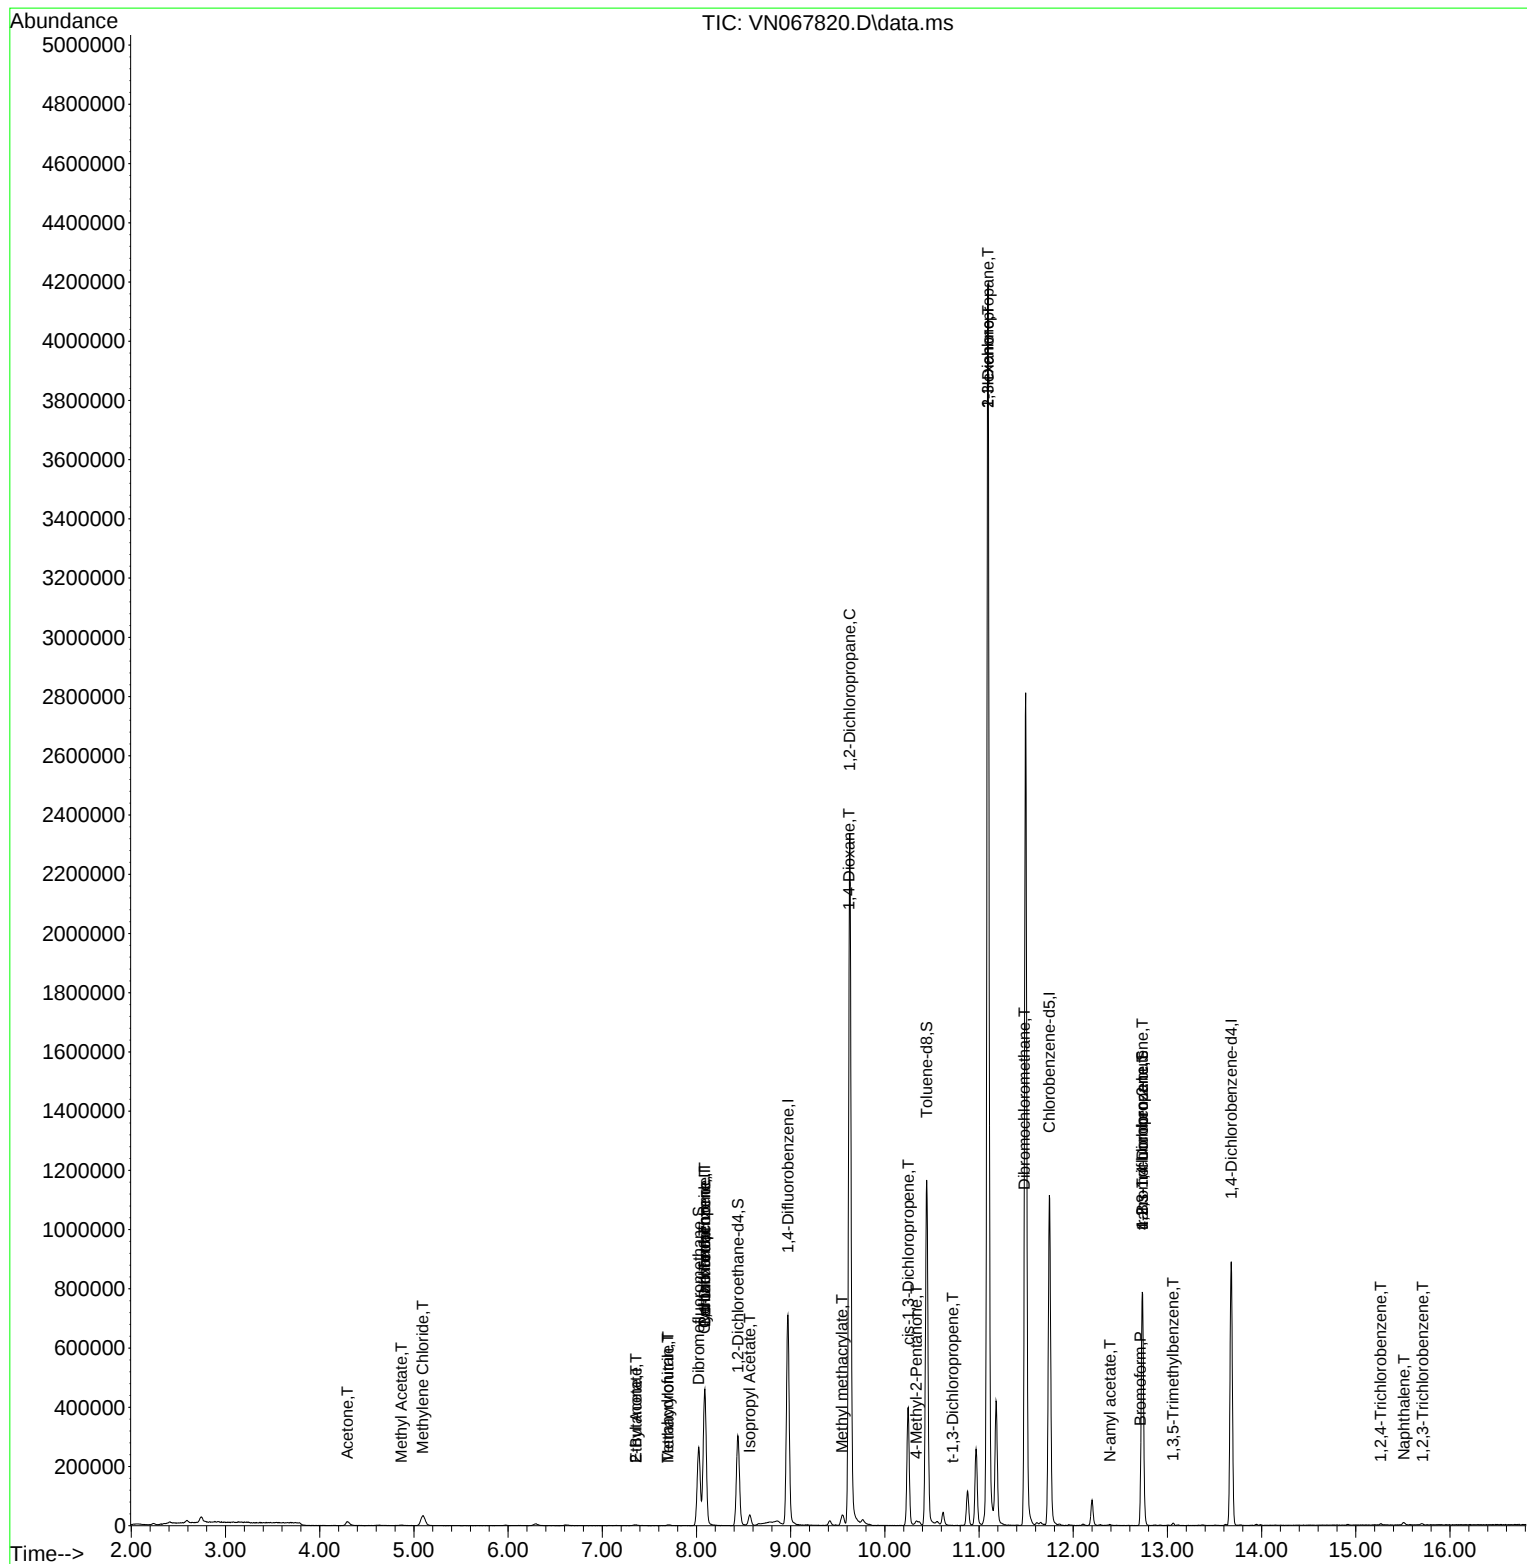

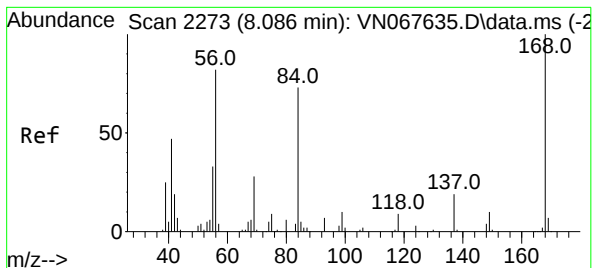

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067820.D





Acq: 20 Jul 2021 16:23

Tgt Ion:168 Resp: 333493

Ion Ratio Lower Upper

168 100

99 62.5 62.9 94.3#

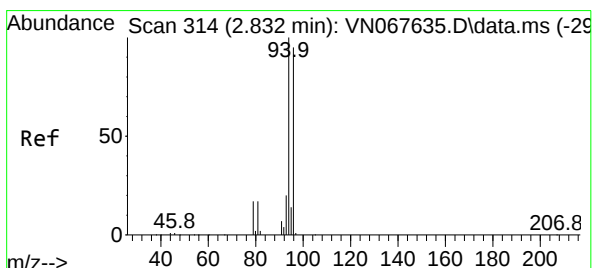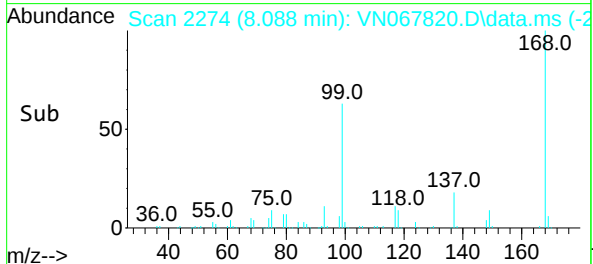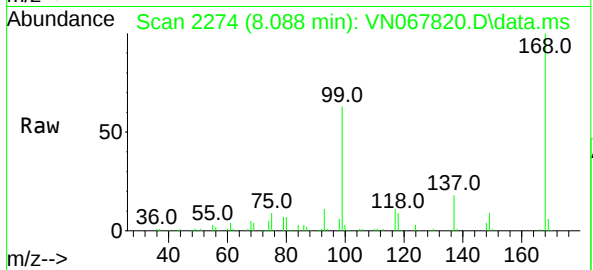

#5

Bromomethane

Concen: Below Cal

RT: 2.840 min Scan# 317

Delta R.T. 0.008 min

Lab File: VN067820.D




Acq: 20 Jul 2021 16:23


Tgt Ion: 94 Resp: 206

Ion Ratio Lower Upper

94 100


96 0.0 73.7 110.5#

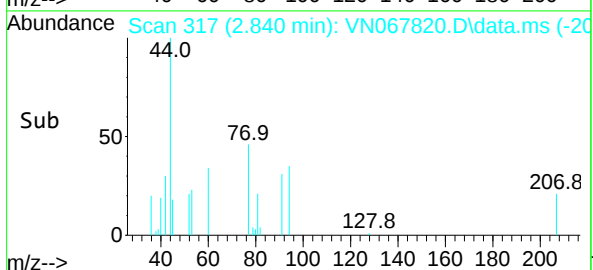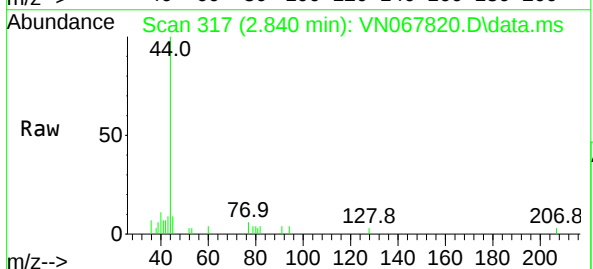






#6
Chloroethane
Concen: Below Cal
RT: 3.038 min Scan# 391
Delta R.T. 0.032 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 64 Resp: 56
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#



#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.376 min Scan# 517
Delta R.T. 0.011 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 101 Resp: 25
Ion Ratio Lower Upper
101 100
103 0.0 51.2 76.8#









#13
Acrolein
Concen: Below Cal
RT: 4.036 min Scan# 763
Delta R.T. -0.003 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 145
Ion Ratio Lower Upper
56 100
55 92.4 57.4 86.0#



#16
Acetone
Concen: 15.892 ug/l
RT: 4.293 min Scan# 859
Delta R.T. 0.005 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 43 Resp: 25204
Ion Ratio Lower Upper
43 100
58 33.2 21.2 31.8#


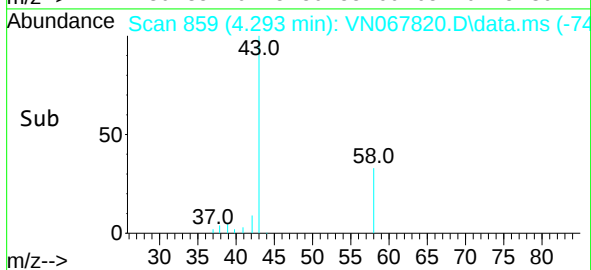




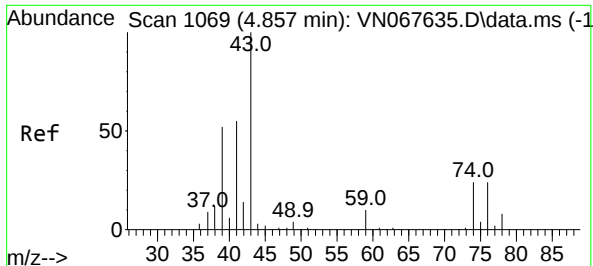

#18
Methyl Acetate
Concen: 0.701 ug/l
RT: 4.867 min Scan# 1073
Delta R.T. 0.010 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 43 Resp: 3124
Ion Ratio Lower Upper
43 100
74 7.7 17.4 26.0#

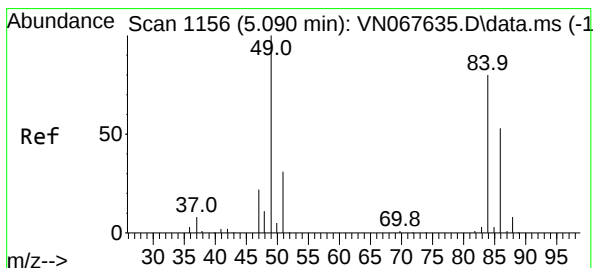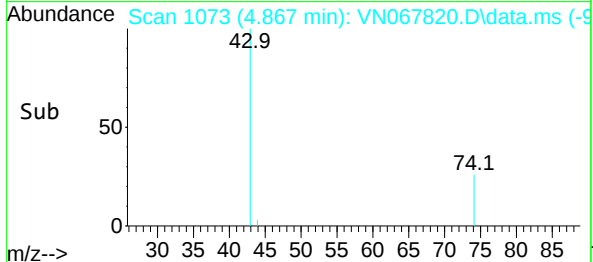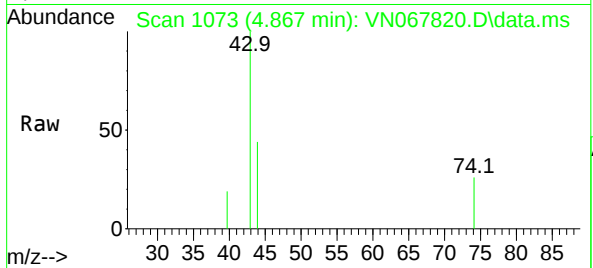

#20
Methylene Chloride
Concen: 6.800 ug/l
RT: 5.093 min Scan# 1157
Delta R.T. 0.003 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 84 Resp: 27401
Ion Ratio Lower Upper
84 100
49 119.9 110.9 166.3
51 38.0 32.6 49.0
86 66.1 51.6 77.4


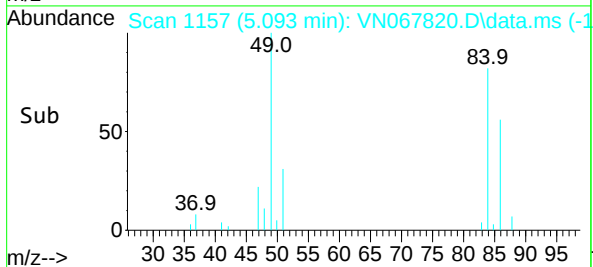

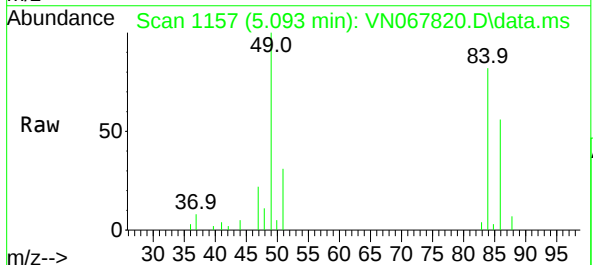


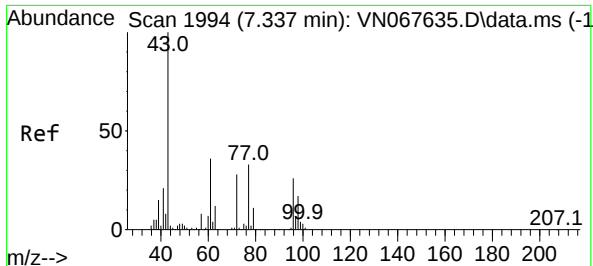

#25
2-Butanone
Concen: 2.135 ug/l
RT: 7.356 min Scan# 2001
Delta R.T. 0.019 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 5622
Ion Ratio Lower Upper
43 100
72 26.3 19.7 29.5

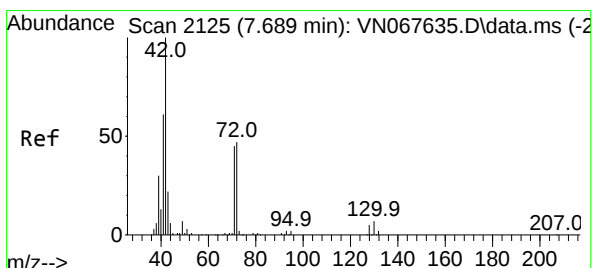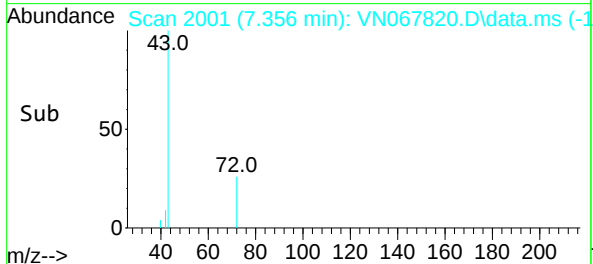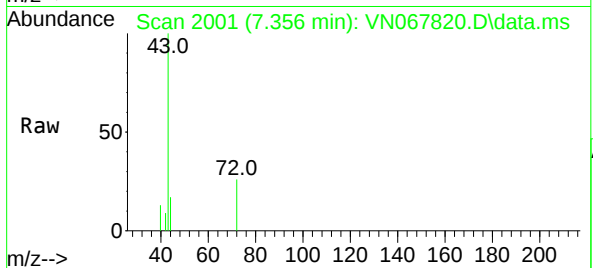

#29
Tetrahydrofuran
Concen: 0.579 ug/l
RT: 7.694 min Scan# 2127
Delta R.T. 0.005 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 42 Resp: 1003
Ion Ratio Lower Upper
42 100
72 23.4 32.8 49.2#
71 13.3 31.2 46.8#


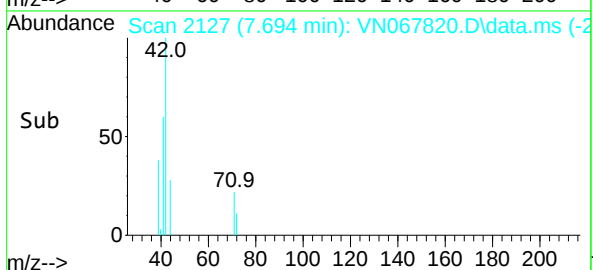

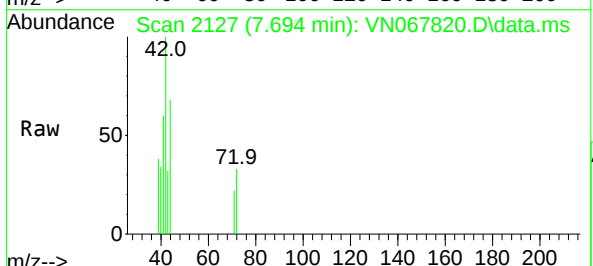




#31
Cyclohexane
Concen: 1.247 ug/l
RT: 8.083 min Scan# 2272
Delta R.T. -0.011 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 56 Resp: 8814
Ion Ratio Lower Upper
56 100
69 147.5 27.3 40.9#
84 110.4 64.9 97.3#



#33
1,2-Dichloroethane-d4
Concen: 51.989 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 65 Resp: 262032
Ion Ratio Lower Upper
65 100
67 50.0 0.0 98.6


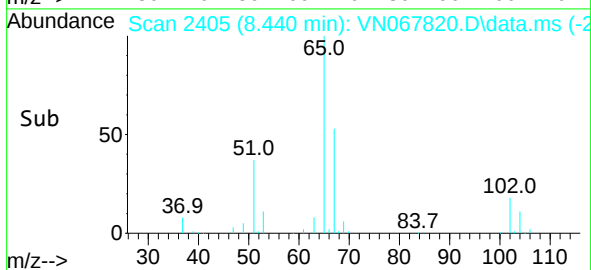






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:114 Resp: 634420
Ion Ratio Lower Upper
114 100
63 20.8 0.0 49.0
88 15.0 0.0 36.6

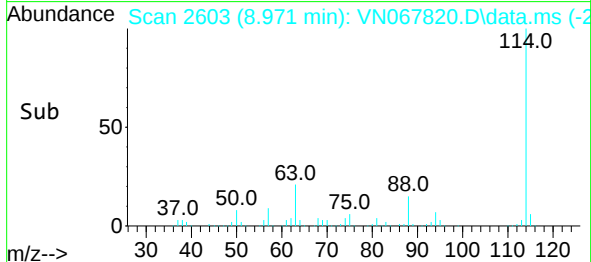

#35
Dibromofluoromethane
Concen: 50.089 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23


Tgt Ion:113 Resp: 191993
Ion Ratio Lower Upper
113 100
111 102.2 83.8 125.8
192 15.3 13.4 20.0

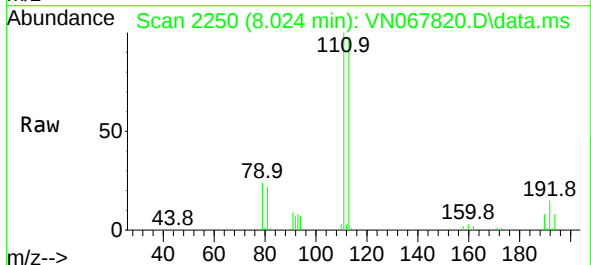






#36
1,1-Dichloropropene
Concen: 5.187 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Instrument :
MSVOA_N
ClientSampleId :



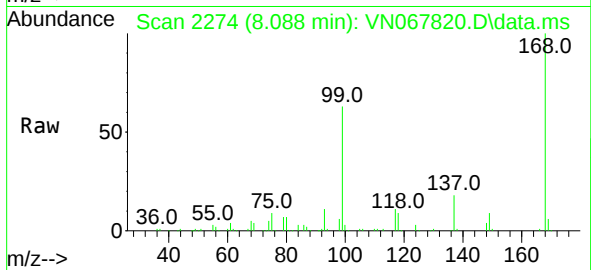



Tgt Ion: 75 Resp: 30565
Ion Ratio Lower Upper
75 100
110 2.0 15.7 47.0#
77 0.0 24.6 37.0#



#37
Ethyl Acetate
Concen: 0.985 ug/l
RT: 7.356 min Scan# 2001
Delta R.T. -0.062 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23


Tgt Ion: 43 Resp: 5622
Ion Ratio Lower Upper
43 100
61 0.0 10.6 16.0#
70 0.0 8.1 12.1#

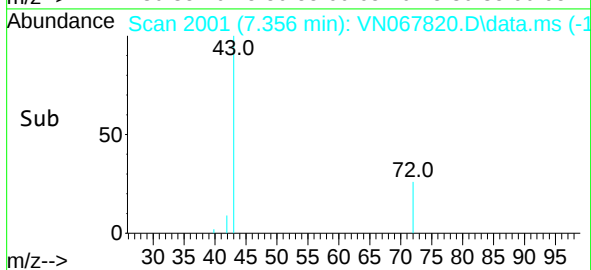






#38
Carbon Tetrachloride
Concen: 6.603 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion:117 Resp: 38384
Ion Ratio Lower Upper
117 100
119 4.1 75.4 113.2#
121 0.0 23.5 35.3#




#41
Methacrylonitrile
Concen: 0.205 ug/l
RT: 7.697 min Scan# 2128
Delta R.T. 0.057 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Tgt Ion: 41 Resp: 601
Ion Ratio Lower Upper
41 100
39 39.8 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#

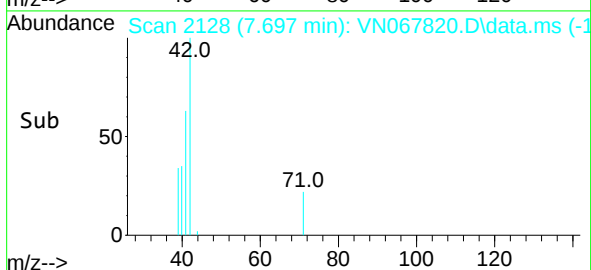






#43
Isopropyl Acetate
Concen: 4.107 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23


Instrument :
MSVOA_N
ClientSampleId :

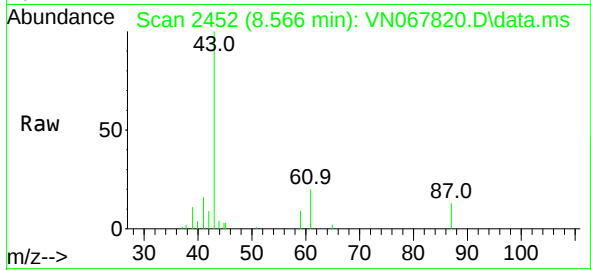



Tgt Ion: 43 Resp: 41250
Ion Ratio Lower Upper
43 100
61 18.2 19.0 28.4#
87 12.6 9.5 14.3




#45
1,2-Dichloropropane
Concen: 0.581 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23



Tgt Ion: 63 Resp: 2593
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#



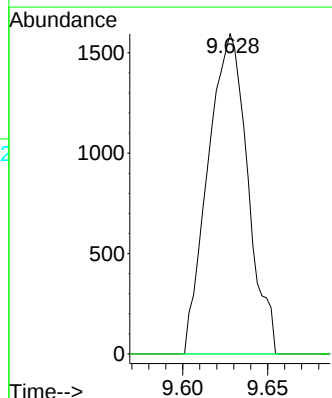





#48
Methyl methacrylate
Concen: 2.074 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.018 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 9215
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#



#49
1,4-Dioxane
Concen: 34.488 ug/l
RT: 9.620 min Scan# 2845
Delta R.T. 0.049 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 88 Resp: 215
Ion Ratio Lower Upper
88 100
43 1076325.6 28.8 43.2#
58 4802.8 60.4 90.6#









#50
Toluene-d8
Concen: 51.148 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 820615
Ion Ratio Lower Upper
98 100
100 64.0 51.7 77.5

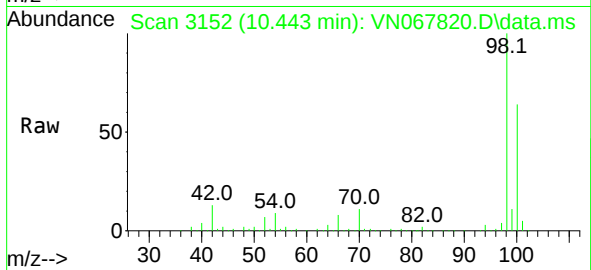

#51
4-Methyl-2-Pentanone
Concen: 1.203 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 43 Resp: 7422
Ion Ratio Lower Upper
43 100
58 55.7 28.6 43.0#









#53
 t-1,3-Dichloropropene
 Concen: 1.756 ug/l
 RT: 10.719 min Scan# 3255
 Delta R.T. -0.003 min
 Lab File: VN067820.D
 Acq: 20 Jul 2021 16:23




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 75 Resp: 89
 Ion Ratio Lower Upper
 75 100
 77 0.0 25.1 37.7#



#54
 cis-1,3-Dichloropropene
 Concen: 10.238 ug/l
 RT: 10.247 min Scan# 3079
 Delta R.T. 0.056 min
 Lab File: VN067820.D
 Acq: 20 Jul 2021 16:23

Tgt Ion: 75 Resp: 70537
 Ion Ratio Lower Upper
 75 100
 77 0.5 24.6 37.0#
 39 40.2 50.7 76.1#


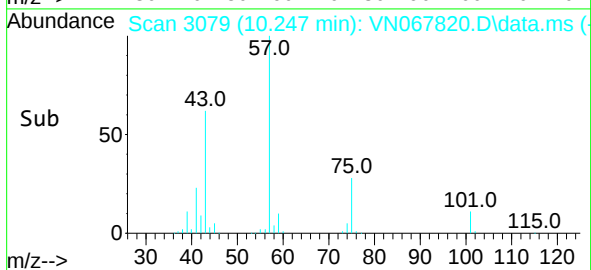




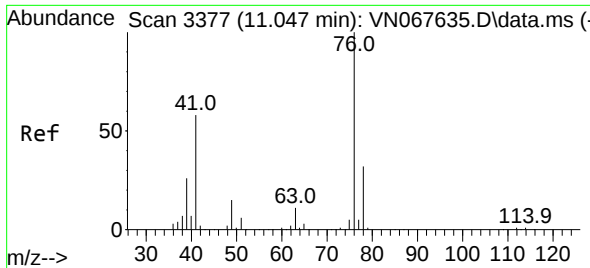

#57
1,3-Dichloropropane
Concen: 5.826 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 44237
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#

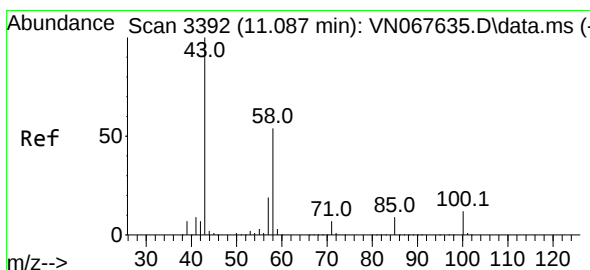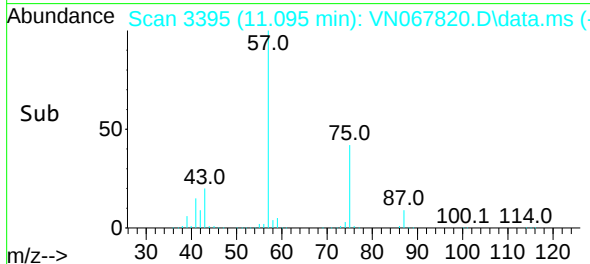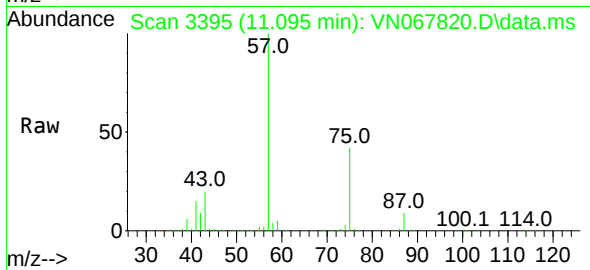

#59
2-Hexanone
Concen: 151.763 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 43 Resp: 653668
Ion Ratio Lower Upper
43 100
58 18.1 24.7 74.1#


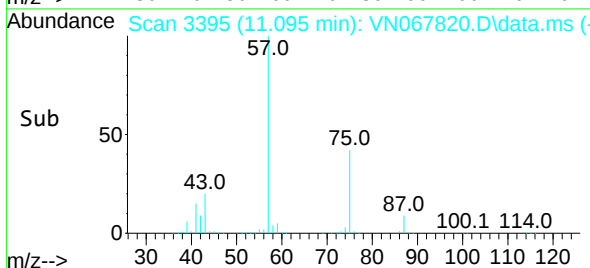

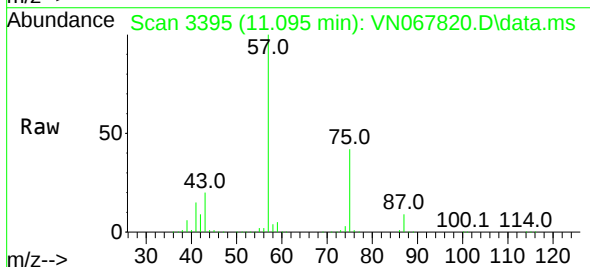




#60
Dibromochloromethane
Concen: 2.366 ug/l
RT: 11.478 min Scan# 3538
Delta R.T. 0.236 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 52
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

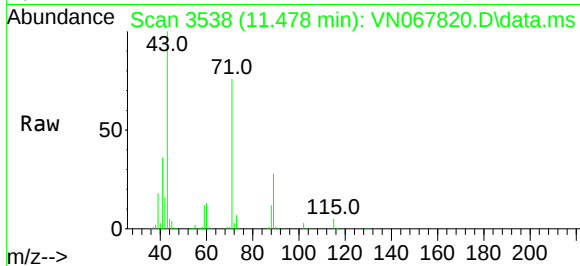

#62
4-Bromofluorobenzene
Concen: 49.841 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 95 Resp: 282480
Ion Ratio Lower Upper
95 100
174 70.1 0.0 122.0
176 67.9 0.0 117.6




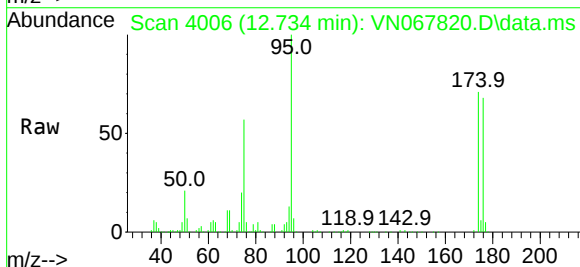


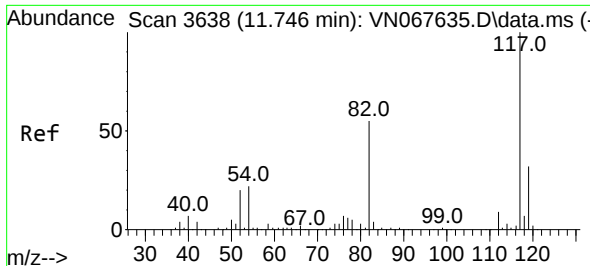

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:117 Resp: 649566
Ion Ratio Lower Upper
117 100
82 56.3 53.1 79.7
119 32.7 25.5 38.3

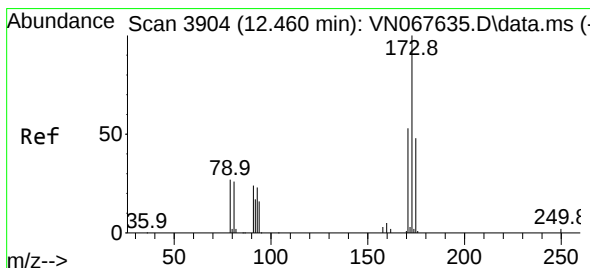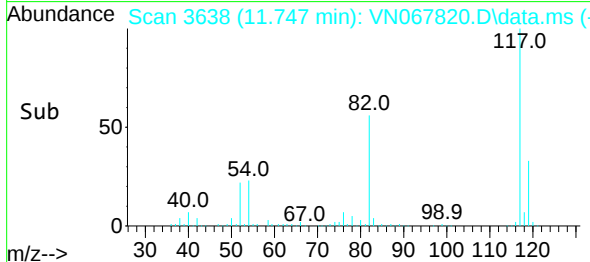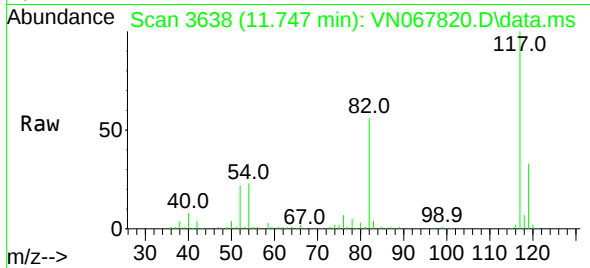

#71
Bromoform
Concen: 3.204 ug/l
RT: 12.712 min Scan# 3998
Delta R.T. 0.252 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion:173 Resp: 124
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0


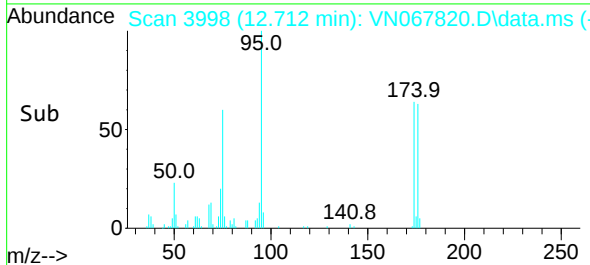

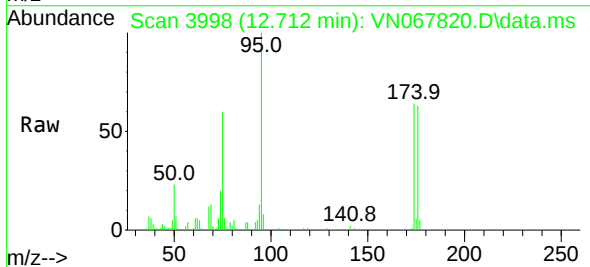


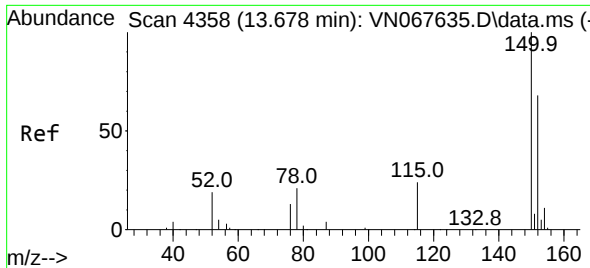

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 229930
Ion Ratio Lower Upper
152 100
115 63.5 36.1 108.5
150 160.3 0.0 351.8

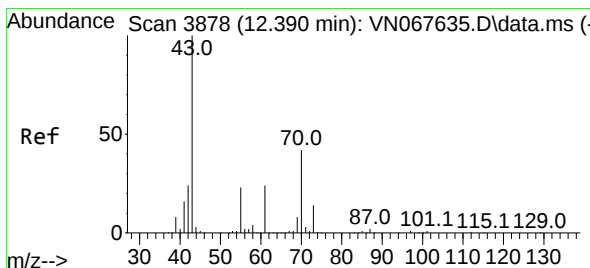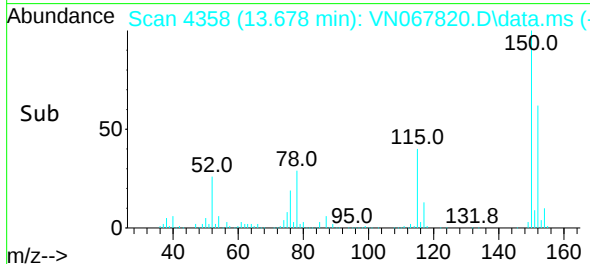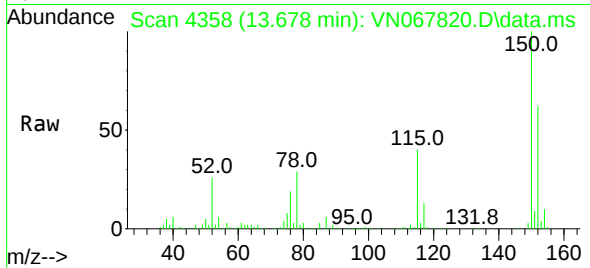

#74
N-ethyl acetate
Concen: 0.234 ug/l
RT: 12.390 min Scan# 3878
Delta R.T. 0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion: 43 Resp: 1576
Ion Ratio Lower Upper
43 100
70 23.4 29.4 44.2#
55 12.5 17.0 25.4#
61 0.0 17.6 26.4#

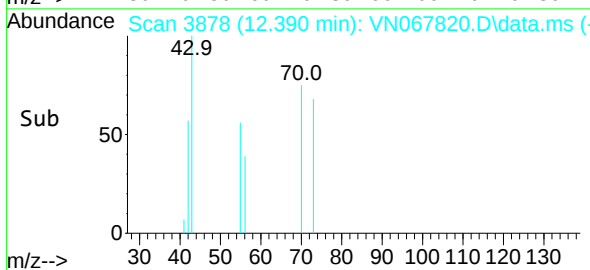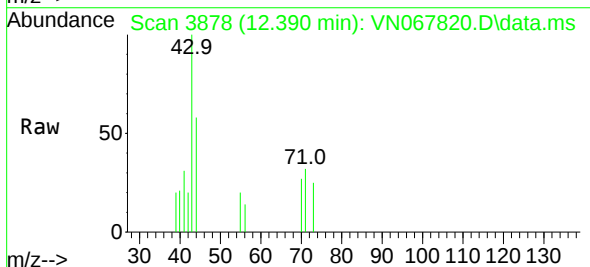

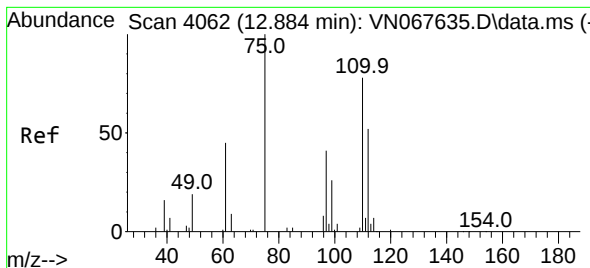

#76

1,2,3-Trichloropropane

Concen: 33.396 ug/l

RT: 12.734 min Scan# 4006

Delta R.T. -0.150 min

Lab File: VN067820.D





Acq: 20 Jul 2021 16:23

Tgt Ion: 75 Resp: 156814

Ion Ratio Lower Upper

75 100

77 1.0 0.0 0.0#

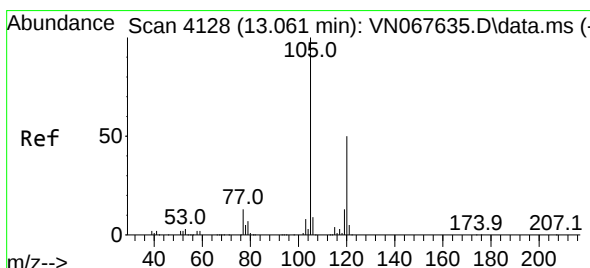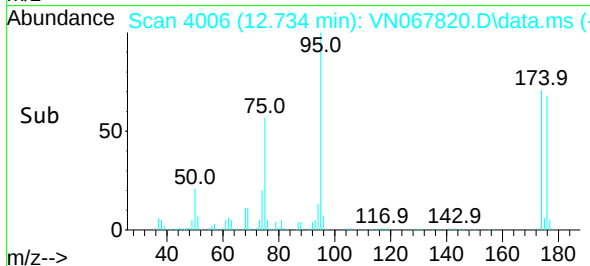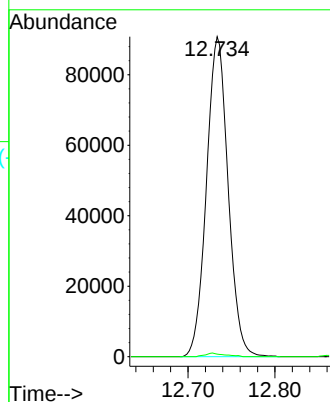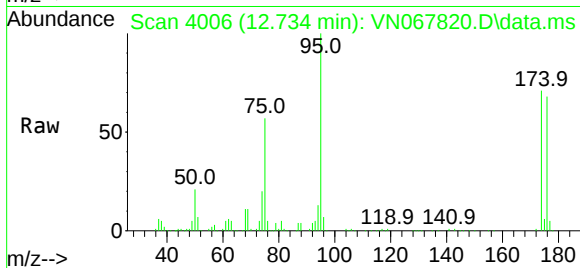

#80

1,3,5-Trimethylbenzene

Concen: 0.259 ug/l

RT: 13.061 min Scan# 4128

Delta R.T. -0.000 min

Lab File: VN067820.D




Acq: 20 Jul 2021 16:23


Tgt Ion:105 Resp: 3899

Ion Ratio Lower Upper

105 100

120 39.3 22.2 66.6


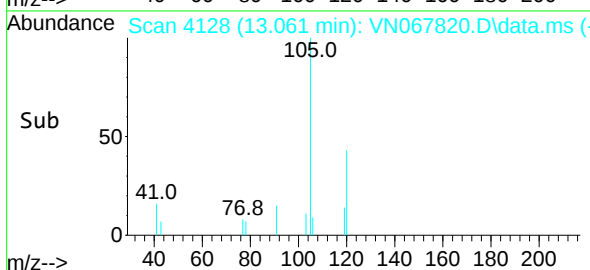
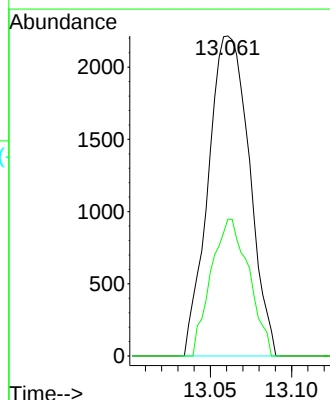
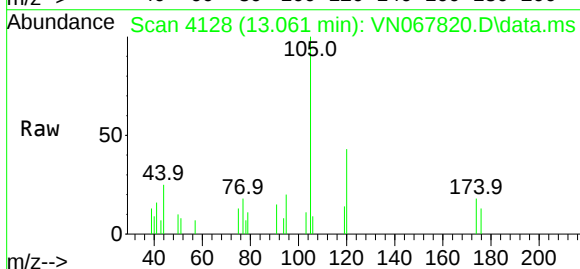




#81
trans-1,4-Dichloro-2-butene
Concen: 107.672 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 156814
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

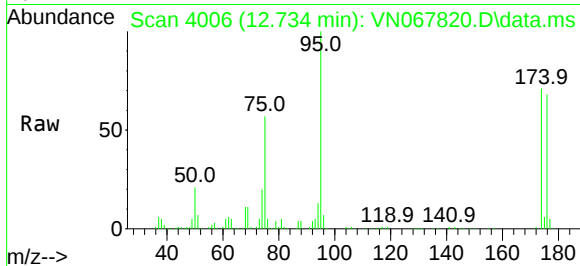

#93
1,2,4-Trichlorobenzene
Concen: 2.978 ug/l
RT: 15.265 min Scan# 4950
Delta R.T. 0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion:180 Resp: 1229
Ion Ratio Lower Upper
180 100
182 112.2 47.5 142.5
145 34.7 17.2 51.6




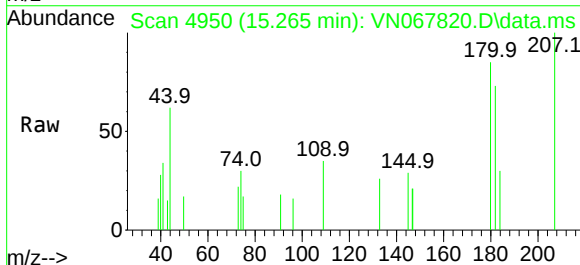




#95
Naphthalene
Concen: 3.699 ug/l
RT: 15.509 min Scan# 5041
Delta R.T. 0.000 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion:128 Resp: 8226
Ion Ratio Lower Upper
128 100
127 5.8 10.6 15.8#
129 13.5 8.6 12.8#

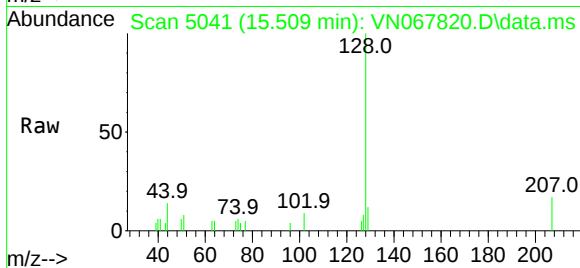

#96
1,2,3-Trichlorobenzene
Concen: 2.802 ug/l
RT: 15.711 min Scan# 5116
Delta R.T. 0.009 min
Lab File: VN067820.D
Acq: 20 Jul 2021 16:23

Tgt Ion:180 Resp: 657
Ion Ratio Lower Upper
180 100
182 191.5 47.8 143.3#
145 76.1 18.2 54.6#

