

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072021\
 Data File : VN067821.D
 Acq On : 20 Jul 2021 16:47
 Operator : JC/MD
 Sample : PB137795ZHE#02
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 21 05:09:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	321854	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	607866	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.746	117	631544	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	232908	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	247260	50.833	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 101.660%	
35) Dibromofluoromethane	8.024	113	184397	50.209	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 100.420%	
50) Toluene-d8	10.443	98	793266	51.603	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 103.200%	
62) 4-Bromofluorobenzene	12.733	95	274005	50.457	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 100.920%	


Target Compounds			Qvalue			
5) Bromomethane	2.824	94	51	Below Cal	#	4
6) Chloroethane	3.135	64	24	Below Cal	#	44
13) Acrolein	4.047	56	269	Below Cal	#	39
16) Acetone	4.296	43	25178	16.450	ug/l	98
18) Methyl Acetate	4.848	43	1030	0.240	ug/l	97
20) Methylene Chloride	5.095	84	25778	6.611	ug/l	# 90
25) 2-Butanone	7.348	43	5739	2.258	ug/l	# 81
29) Tetrahydrofuran	7.702	42	1914	1.145	ug/l	# 56
31) Cyclohexane	8.088	56	8534	1.251	ug/l	# 22
36) 1,1-Dichloropropene	8.086	75	28286	5.009	ug/l	# 51
37) Ethyl Acetate	7.348	43	5739	1.049	ug/l	# 69
38) Carbon Tetrachloride	8.086	117	37050	6.652	ug/l	# 16
41) Methacrylonitrile	7.699	41	724	0.257	ug/l	# 45
43) Isopropyl Acetate	8.566	43	41010	4.261	ug/l	93
45) 1,2-Dichloropropane	9.628	63	2746	0.642	ug/l	# 44
48) Methyl methacrylate	9.545	41	10077	2.367	ug/l	# 12
49) 1,4-Dioxane	9.622	88	241	34.888	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.333	43	8441	1.428	ug/l	89
53) t-1,3-Dichloropropene	10.623	75	27	1.748	ug/l	# 58
54) cis-1,3-Dichloropropene	10.247	75	71136	10.776	ug/l	# 61
57) 1,3-Dichloropropane	11.095	76	44492	6.115	ug/l	# 43
59) 2-Hexanone	11.095	43	665618	161.288	ug/l	# 53
60) Dibromochloromethane	11.492	129	263	2.405	ug/l	# 11
71) Bromoform	12.725	173	939	3.393	ug/l	# 1
74) N-amyl acetate	12.197	43	26619	3.905	ug/l	# 56
76) 1,2,3-Trichloropropane	12.733	75	150013	31.539	ug/l	# 100
80) 1,3,5-Trimethylbenzene	13.061	105	3646	0.239	ug/l	97
81) trans-1,4-Dichloro-2-b...	12.733	75	150013	101.685	ug/l	# 6
93) 1,2,4-Trichlorobenzene	15.273	180	679	2.840	ug/l	95
95) Naphthalene	15.509	128	4404	3.375	ug/l	# 88
96) 1,2,3-Trichlorobenzene	15.700	180	773	2.829	ug/l	# 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072021\
Data File : VN067821.D
Acq On : 20 Jul 2021 16:47
Operator : JC/MD
Sample : PB137795ZHE#02
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 21 05:09:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

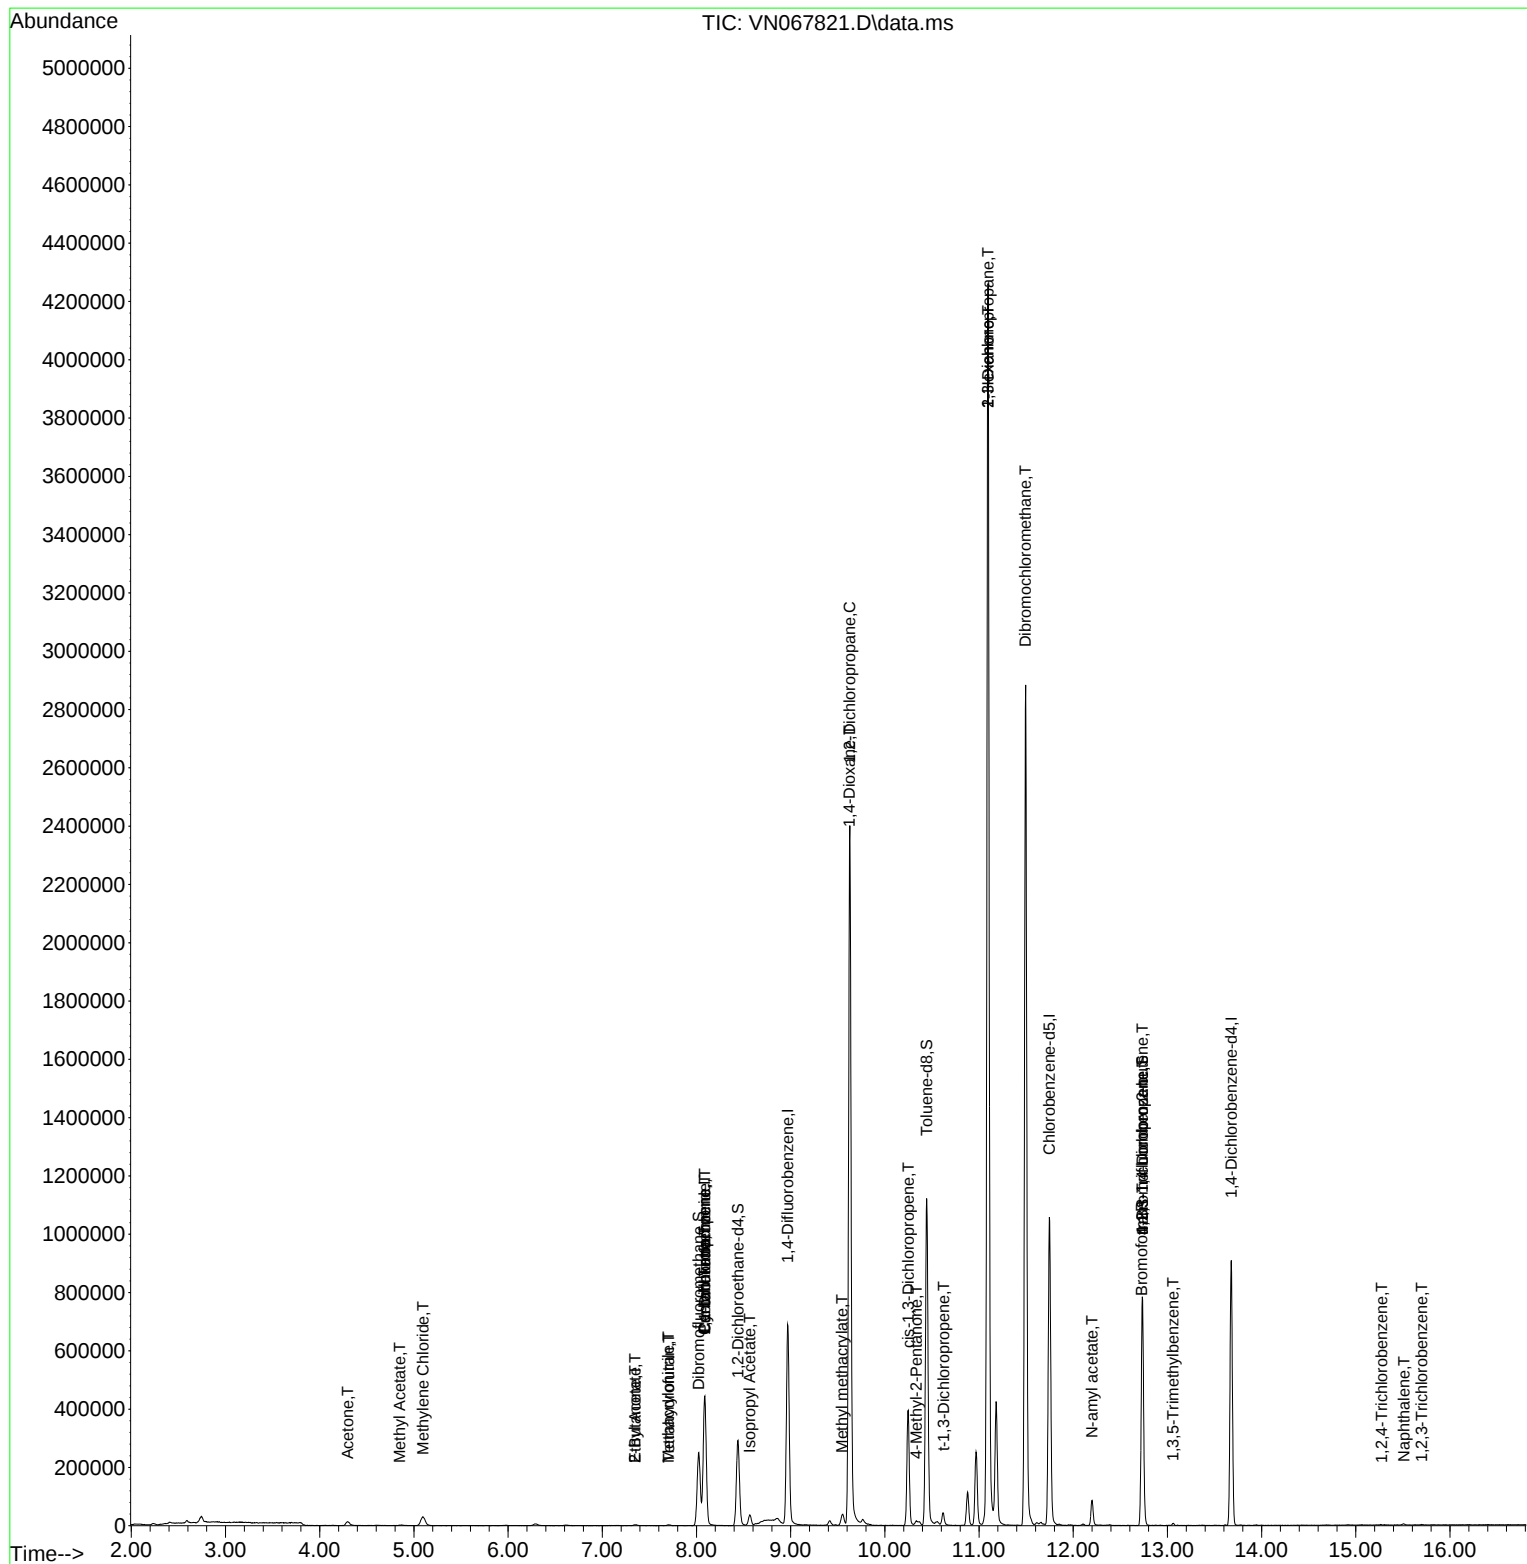

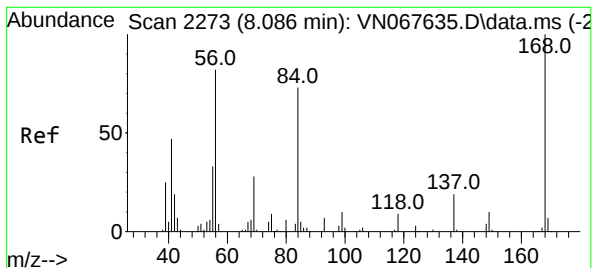

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067821.D





Acq: 20 Jul 2021 16:47

Tgt Ion:168 Resp: 321854

Ion Ratio Lower Upper

168 100

99 64.0 62.9 94.3

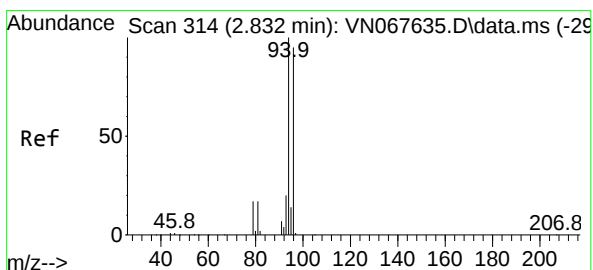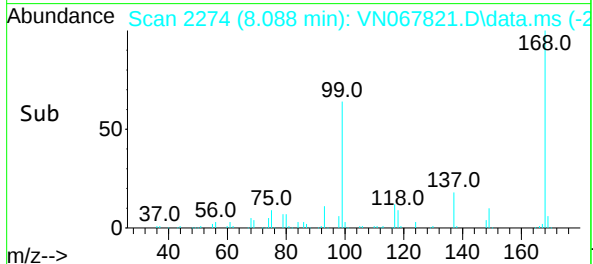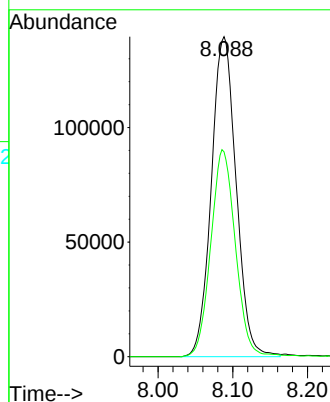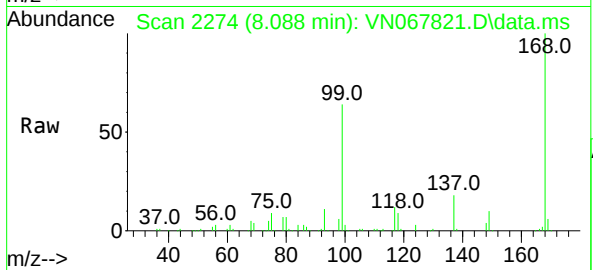

#5

Bromomethane

Concen: Below Cal

RT: 2.824 min Scan# 311

Delta R.T. -0.008 min

Lab File: VN067821.D




Acq: 20 Jul 2021 16:47


Tgt Ion: 94 Resp: 51

Ion Ratio Lower Upper

94 100

96 0.0 73.7 110.5#


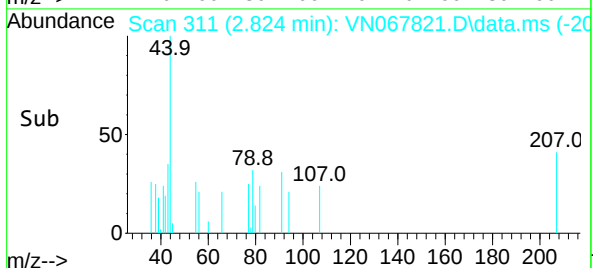
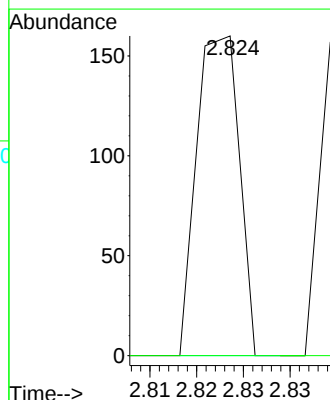
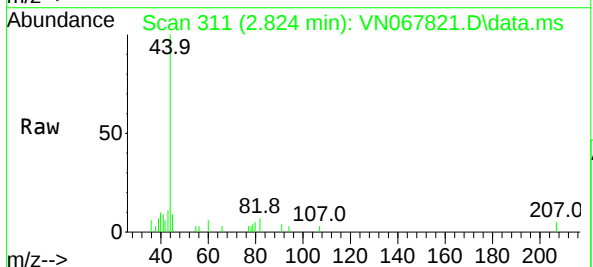




#6
Chloroethane
Concen: Below Cal
RT: 3.135 min Scan# 427
Delta R.T. 0.129 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 64 Resp: 24
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#



#13
Acrolein
Concen: Below Cal
RT: 4.047 min Scan# 767
Delta R.T. 0.008 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 56 Resp: 269
Ion Ratio Lower Upper
56 100
55 20.8 57.4 86.0#


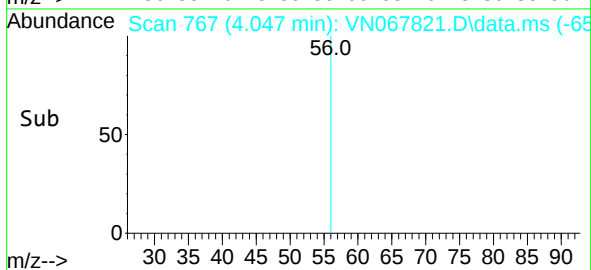






#16
Acetone
Concen: 16.450 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 25178
Ion Ratio Lower Upper
43 100
58 25.5 21.2 31.8



#18
Methyl Acetate
Concen: 0.240 ug/l
RT: 4.848 min Scan# 1066
Delta R.T. -0.009 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 43 Resp: 1030
Ion Ratio Lower Upper
43 100
74 20.3 17.4 26.0


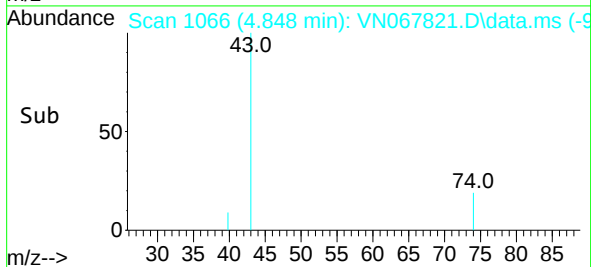

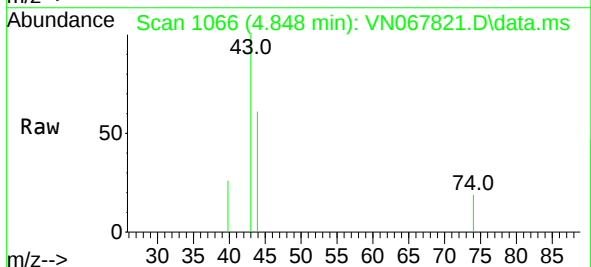


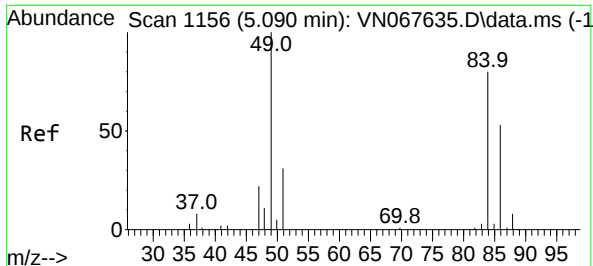

#20
Methylene Chloride
Concen: 6.611 ug/l
RT: 5.095 min Scan# 1158
Delta R.T. 0.005 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:	84	Resp:	25778
Ion	Ratio	Lower	Upper
84	100		
49	124.6	110.9	166.3
51	30.3	32.6	49.0#
86	62.2	51.6	77.4

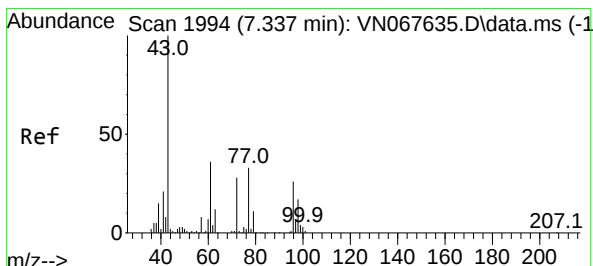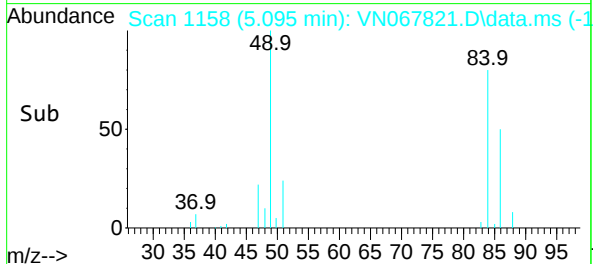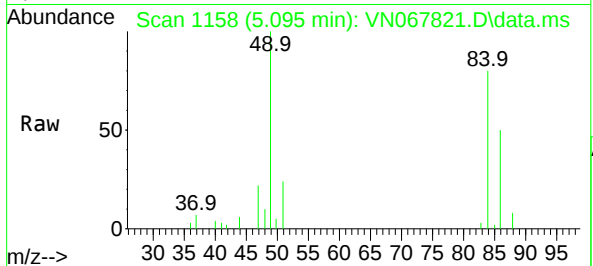

#25
2-Butanone
Concen: 2.258 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. 0.011 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion:	43	Resp:	5739
Ion	Ratio	Lower	Upper
43	100		
72	15.0	19.7	29.5#

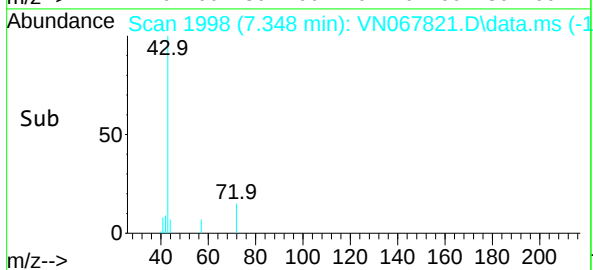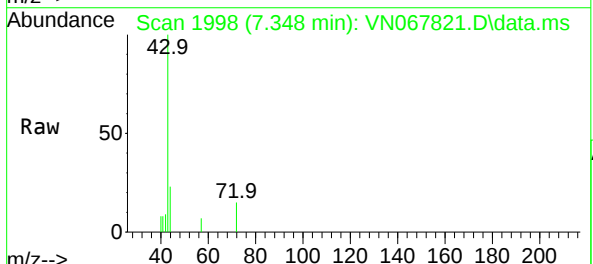



#29

Tetrahydrofuran

Concen: 1.145 ug/l


RT: 7.702 min Scan# 2130

Delta R.T. 0.013 min




Lab File: VN067821.D

Acq: 20 Jul 2021 16:47

Instrument :
MSVOA_N
ClientSampled :

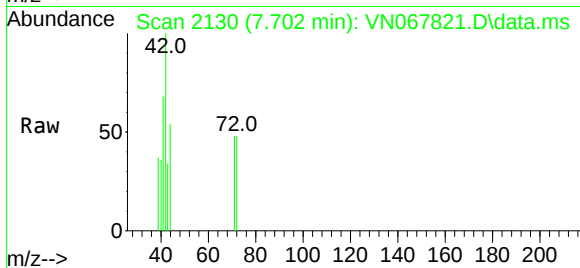

Tgt Ion:	42	Resp:	1914
Ion	Ratio	Lower	Upper
42	100		
72	20.0	32.8	49.2#
71	5.6	31.2	46.8#



#31

Cyclohexane


Concen: 1.251 ug/l

RT: 8.088 min Scan# 2274



Delta R.T. -0.006 min


Lab File: VN067821.D

Acq: 20 Jul 2021 16:47

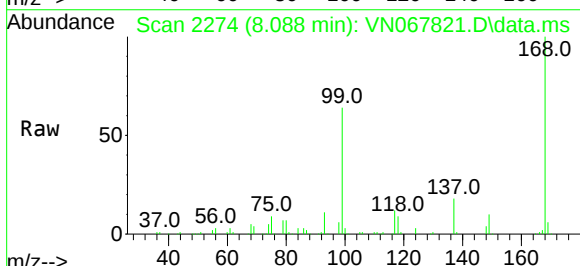

Tgt Ion:	56	Resp:	8534
Ion	Ratio	Lower	Upper
56	100		
69	150.0	27.3	40.9#
84	103.5	64.9	97.3#



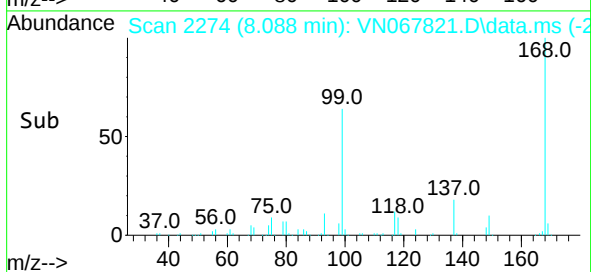





#33
 1,2-Dichloroethane-d4
 Concen: 50.833 ug/l
 RT: 8.440 min Scan# 2405
 Delta R.T. -0.000 min
 Lab File: VN067821.D
 Acq: 20 Jul 2021 16:47




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 65 Resp: 247260
 Ion Ratio Lower Upper
 65 100
 67 52.3 0.0 98.6



#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.968 min Scan# 2602
 Delta R.T. -0.000 min
 Lab File: VN067821.D
 Acq: 20 Jul 2021 16:47

Tgt Ion: 114 Resp: 607866
 Ion Ratio Lower Upper
 114 100
 63 20.8 0.0 49.0
 88 14.8 0.0 36.6


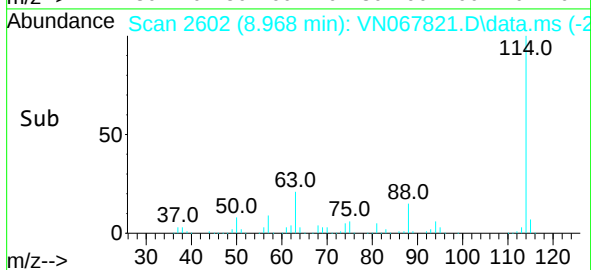

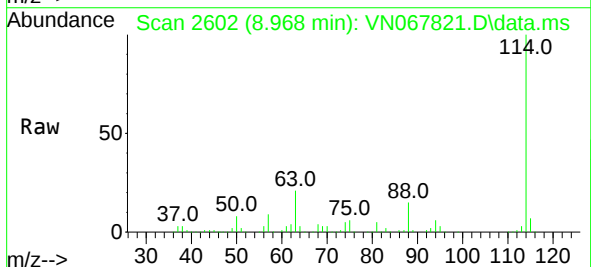




#35
Dibromofluoromethane
Concen: 50.209 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:113 Resp: 184397
Ion Ratio Lower Upper
113 100
111 101.9 83.8 125.8
192 15.2 13.4 20.0

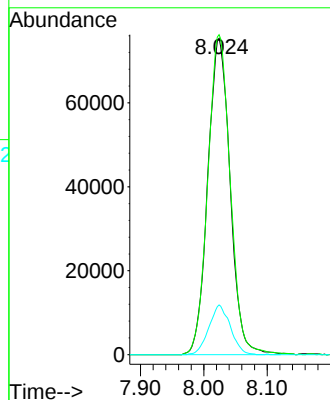

#36
1,1-Dichloropropene
Concen: 5.009 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.136 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47


Tgt Ion: 75 Resp: 28286
Ion Ratio Lower Upper
75 100
110 8.4 15.7 47.0#
77 0.0 24.6 37.0#

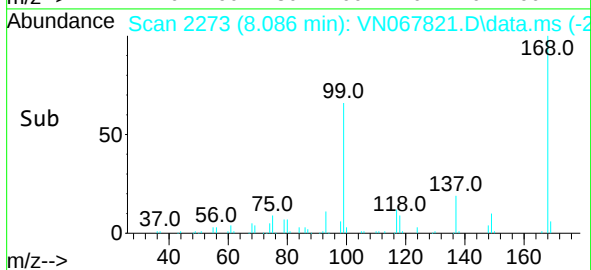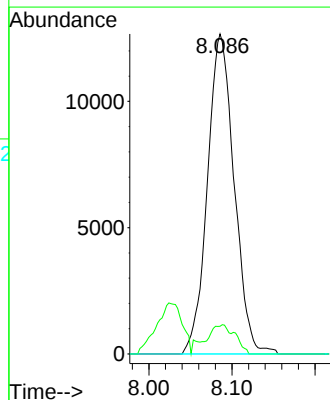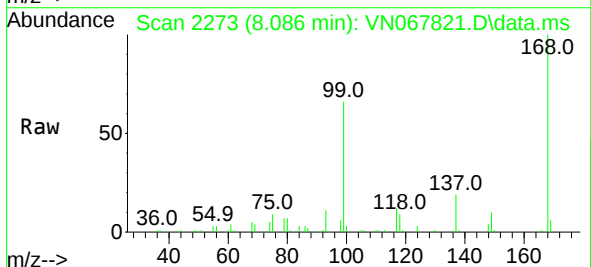



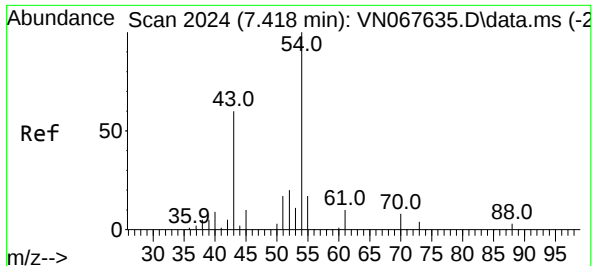


#37
Ethyl Acetate
Concen: 1.049 ug/l
RT: 7.348 min Scan# 1998
Delta R.T. -0.070 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Instrument :
MSVOA_N
ClientSampleId :



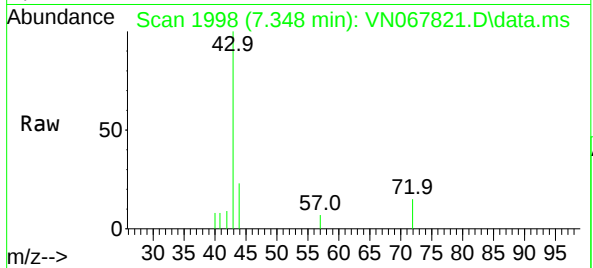



Tgt Ion:	43	Resp:	5739
Ion	Ratio	Lower	Upper
43	100		
61	0.0	10.6	16.0#
70	0.0	8.1	12.1#

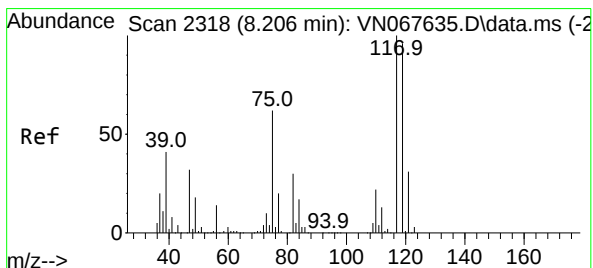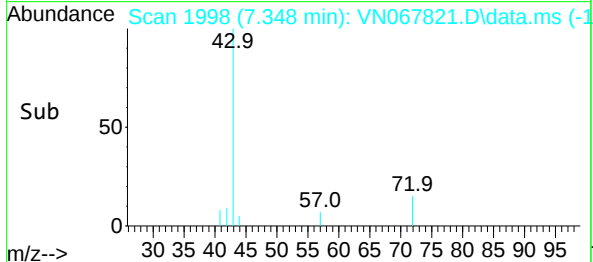

#38
Carbon Tetrachloride
Concen: 6.652 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47


Tgt Ion:	117	Resp:	37050
Ion	Ratio	Lower	Upper
117	100		
119	4.7	75.4	113.2#
121	0.0	23.5	35.3#

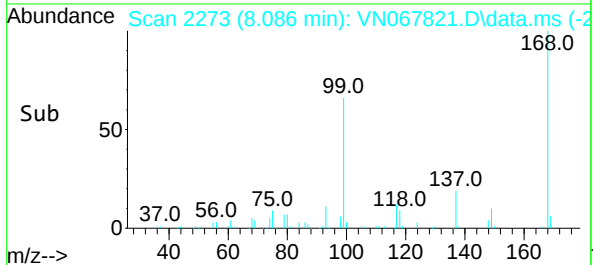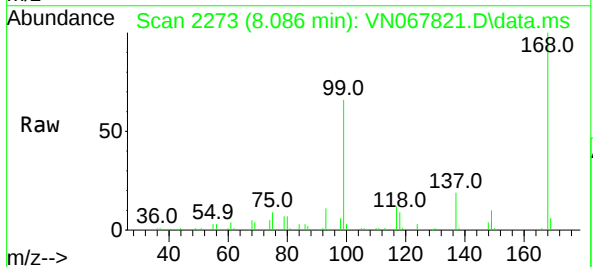



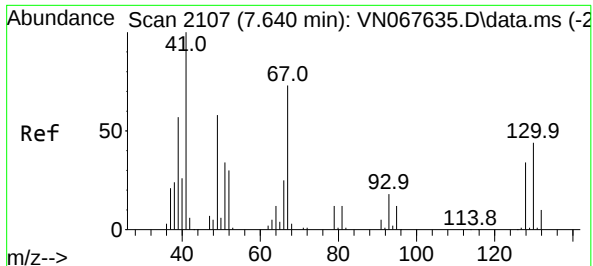


#41
Methacrylonitrile
Concen: 0.257 ug/l
RT: 7.699 min Scan# 2129
Delta R.T. 0.059 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47


Instrument :
MSVOA_N
ClientSampled :

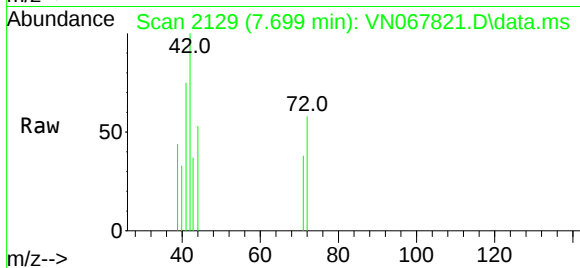



Tgt Ion:	41	Resp:	724
Ion	Ratio	Lower	Upper
41	100		
39	71.8	47.6	71.4#
67	0.0	57.7	86.5#
52	0.0	26.2	39.4#

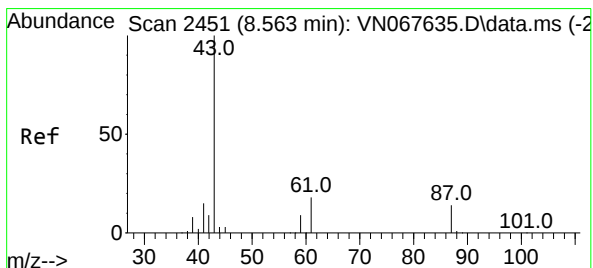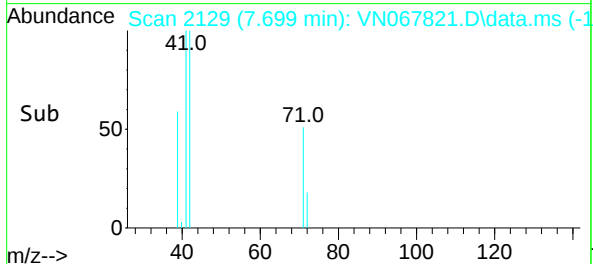


#43
Isopropyl Acetate
Concen: 4.261 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

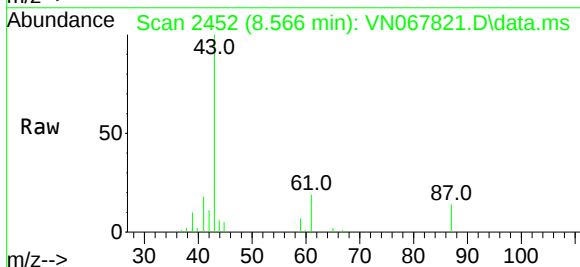

Tgt Ion:	43	Resp:	41010
Ion	Ratio	Lower	Upper
43	100		
61	19.0	19.0	28.4
87	12.4	9.5	14.3

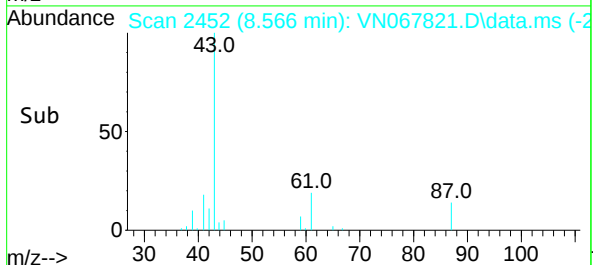




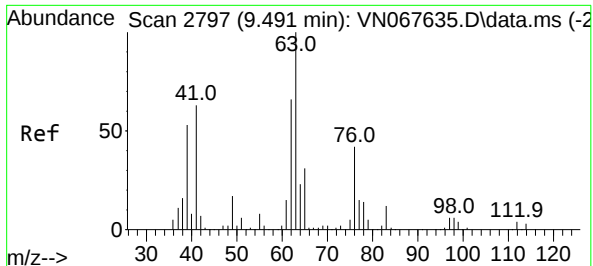


#45

1,2-Dichloropropane
Concen: 0.642 ug/l
RT: 9.628 min Scan# 2848
Delta R.T. 0.137 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 63 Resp: 2746
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#

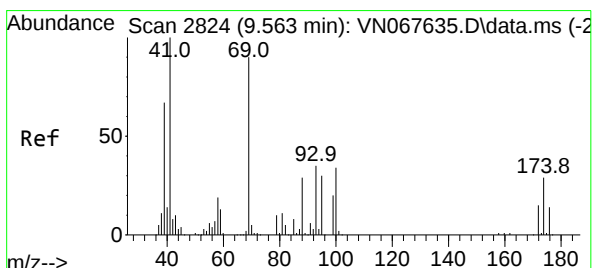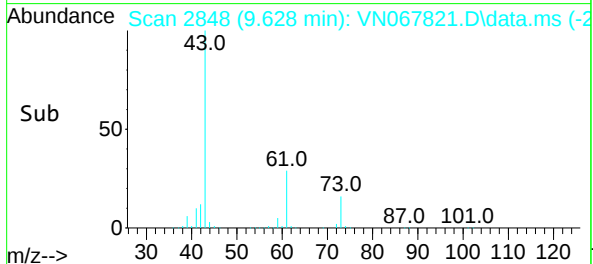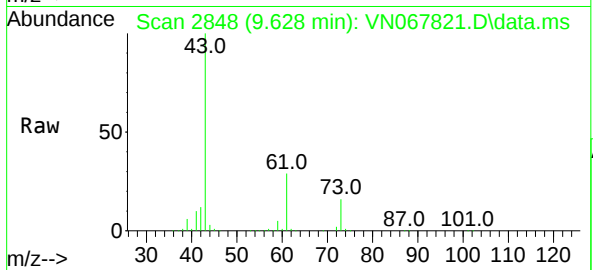


#48

Methyl methacrylate
Concen: 2.367 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.018 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 41 Resp: 10077
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

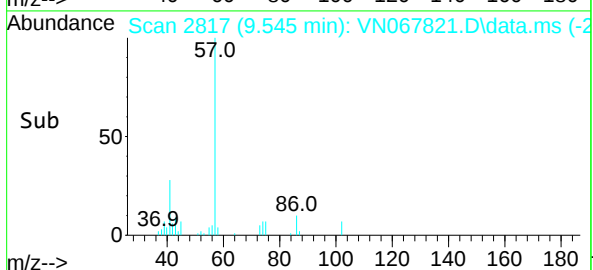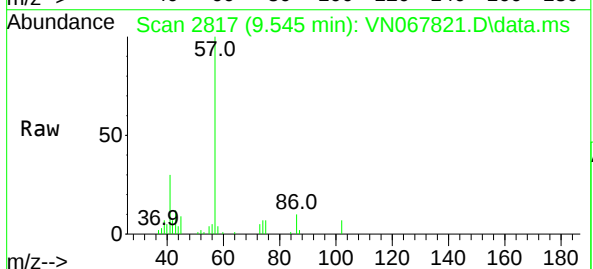



#49

1,4-Dioxane

Concen: 34.888 ug/l

RT: 9.622 min Scan# 2846

Delta R.T. 0.051 min

Lab File: VN067821.D

Acq: 20 Jul 2021 16:47





Tgt Ion: 88 Resp: 241

Ion Ratio Lower Upper

88 100

43 980297.9 28.8 43.2#

58 4142.3 60.4 90.6#

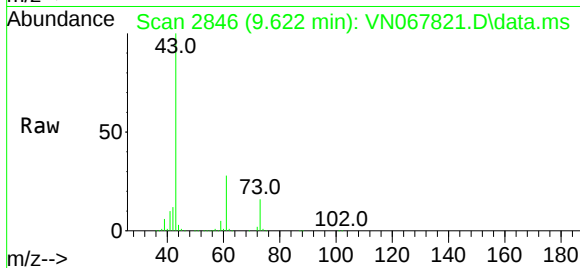

#50

Toluene-d8

Concen: 51.603 ug/l

RT: 10.443 min Scan# 3152

Delta R.T. 0.000 min

Lab File: VN067821.D




Acq: 20 Jul 2021 16:47


Tgt Ion: 98 Resp: 793266

Ion Ratio Lower Upper

98 100

100 63.2 51.7 77.5


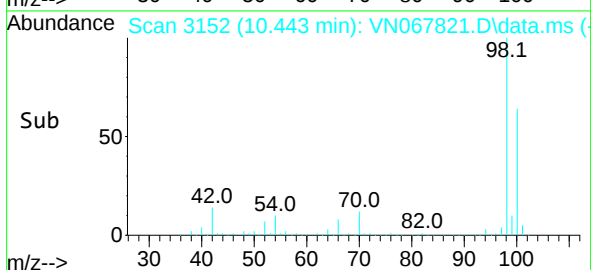

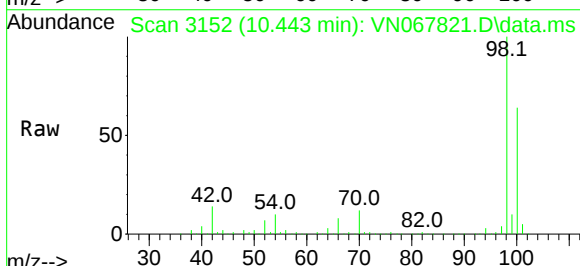




#51
4-Methyl-2-Pentanone
Concen: 1.428 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 8441
Ion Ratio Lower Upper
43 100
58 42.2 28.6 43.0



#53
t-1,3-Dichloropropene
Concen: 1.748 ug/l
RT: 10.623 min Scan# 3219
Delta R.T. -0.099 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 75 Resp: 27
Ion Ratio Lower Upper
75 100
77 8.3 25.1 37.7#


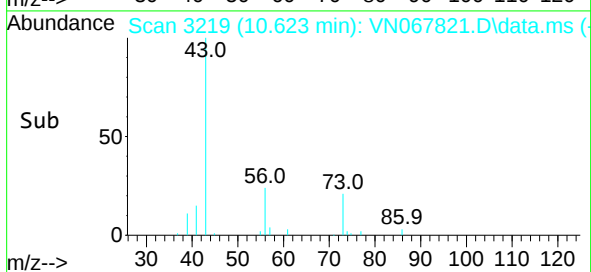






#54
 cis-1,3-Dichloropropene
 Concen: 10.776 ug/l
 RT: 10.247 min Scan# 3079
 Delta R.T. 0.056 min
 Lab File: VN067821.D
 Acq: 20 Jul 2021 16:47




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion: 75 Resp: 71136
 Ion Ratio Lower Upper
 75 100
 77 0.5 24.6 37.0#
 39 38.7 50.7 76.1#



#57
 1,3-Dichloropropane
 Concen: 6.115 ug/l
 RT: 11.095 min Scan# 3395
 Delta R.T. 0.048 min
 Lab File: VN067821.D
 Acq: 20 Jul 2021 16:47

Tgt Ion: 76 Resp: 44492
 Ion Ratio Lower Upper
 76 100
 78 0.2 25.7 38.5#


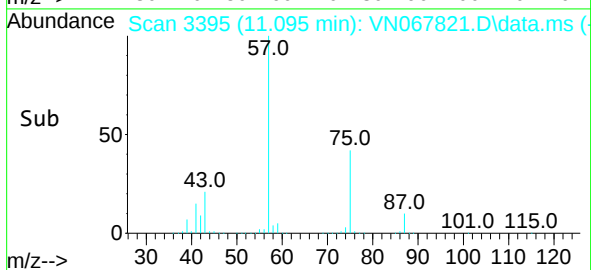






#59
2-Hexanone
Concen: 161.288 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 665618
Ion Ratio Lower Upper
43 100
58 17.4 24.7 74.1#

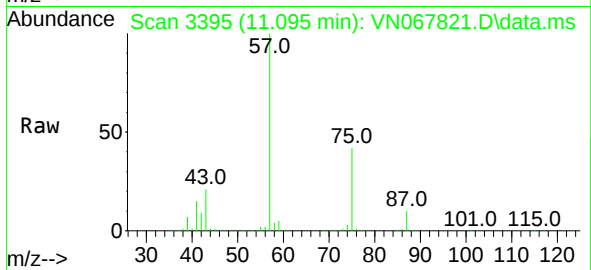

#60
Dibromochloromethane
Concen: 2.405 ug/l
RT: 11.492 min Scan# 3543
Delta R.T. 0.250 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 129 Resp: 263
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#


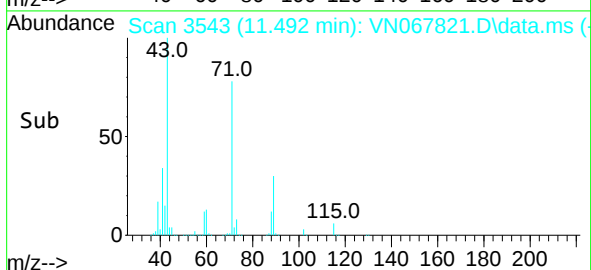

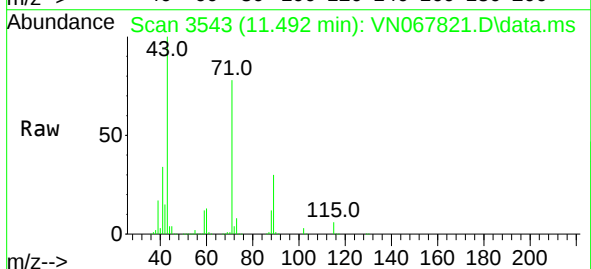


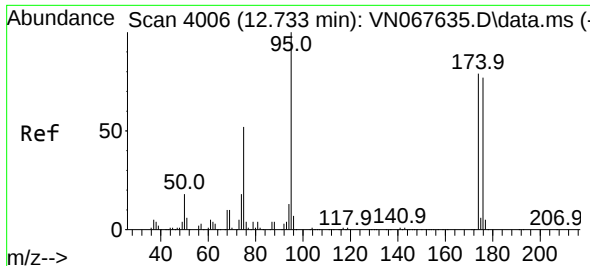

#62
4-Bromofluorobenzene
Concen: 50.457 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.000 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 95 Resp: 274005
Ion Ratio Lower Upper
95 100
174 71.4 0.0 122.0
176 69.3 0.0 117.6

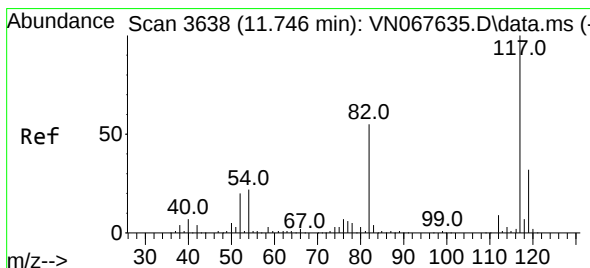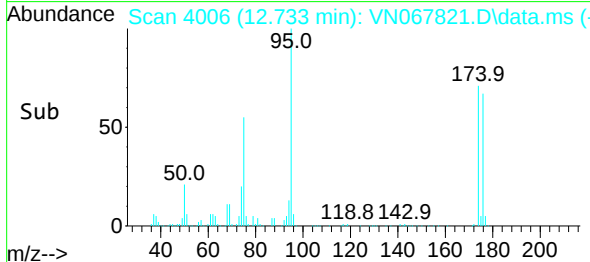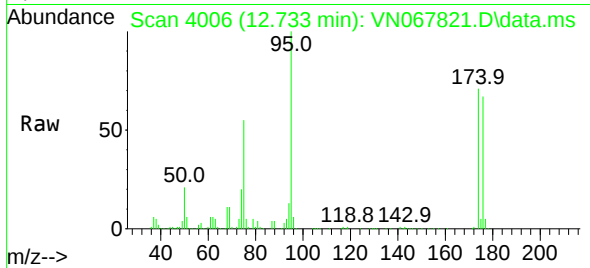

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.746 min Scan# 3638
Delta R.T. -0.000 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 117 Resp: 631544
Ion Ratio Lower Upper
117 100
82 56.1 53.1 79.7
119 31.8 25.5 38.3


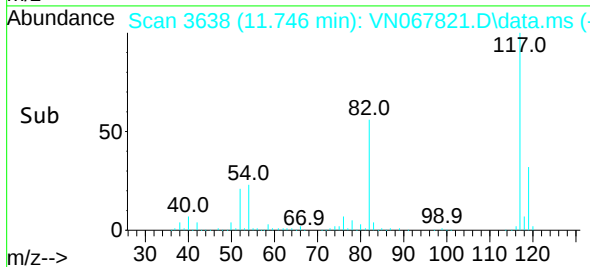

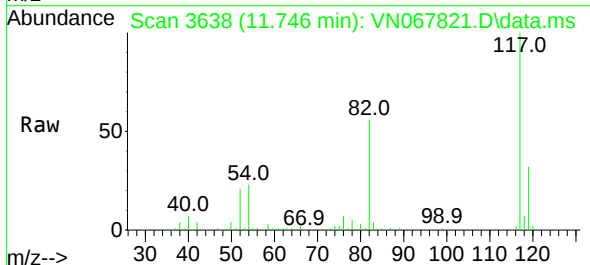


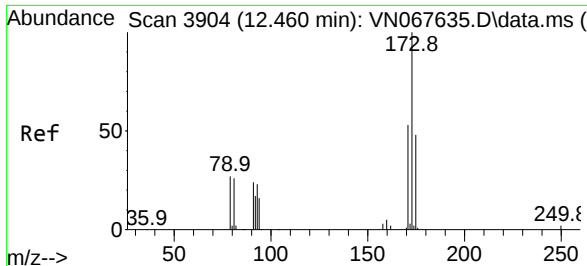

#71
Bromoform
Concen: 3.393 ug/l
RT: 12.725 min Scan# 4003
Delta R.T. 0.265 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 939
Ion Ratio Lower Upper
173 100
175 1488.1 23.9 71.8#
254 0.0 0.0 0.0

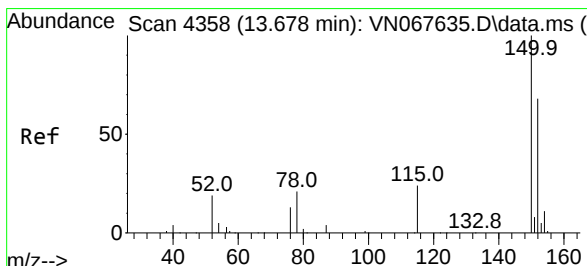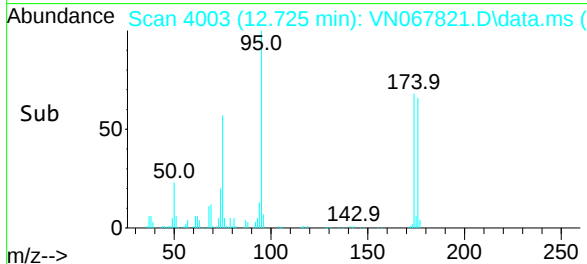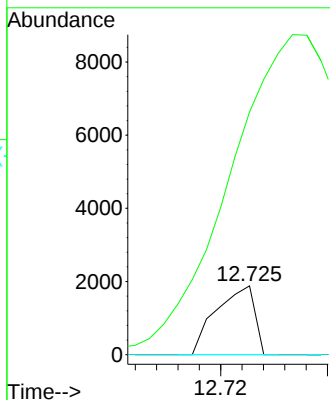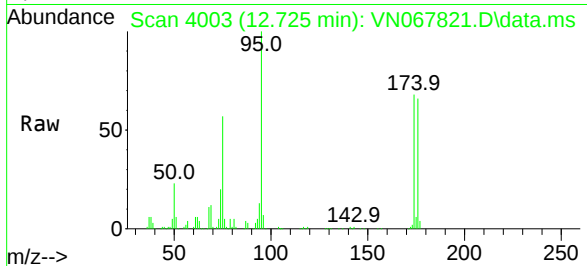

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. -0.000 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47


Tgt Ion:152 Resp: 232908
Ion Ratio Lower Upper
152 100
115 63.1 36.1 108.5
150 158.2 0.0 351.8

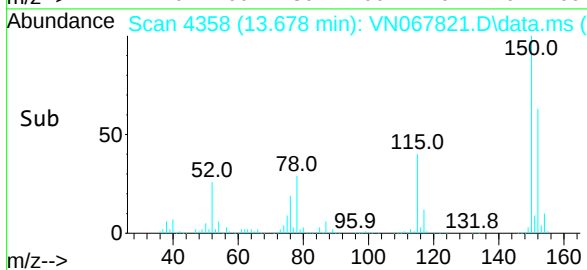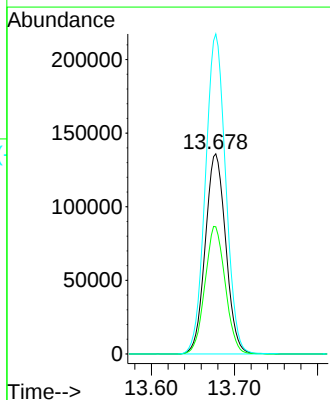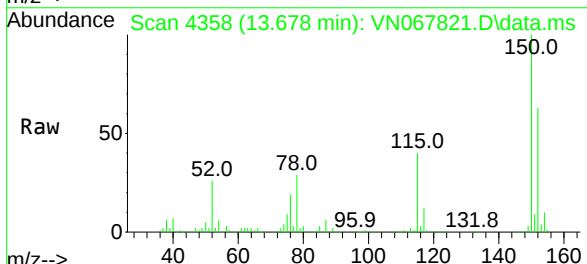






#74
N-amy1 acetate
Concen: 3.905 ug/l
RT: 12.197 min Scan# 3806
Delta R.T. -0.193 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Instrument :
MSVOA_N
ClientSampleId :



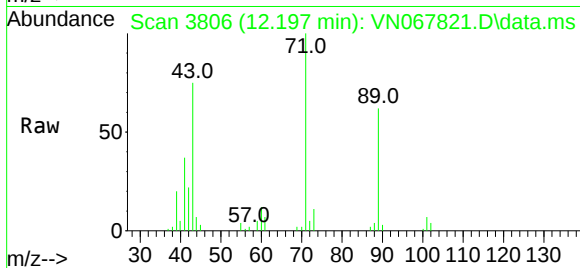



Tgt Ion:	43	Resp:	26619
Ion Ratio	100	Lower	29.4
Upper	44.2#	Lower	17.0
Upper	25.4#	Lower	17.6
Upper	26.4#		



#76
1,2,3-Trichloropropane
Concen: 31.539 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. -0.151 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion:	75	Resp:	150013
Ion Ratio	100	Lower	0.0
Upper	0.0#	Lower	0.0#
Upper			




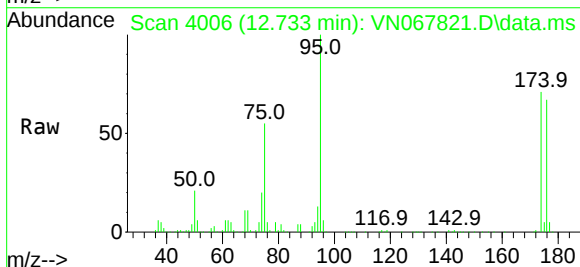


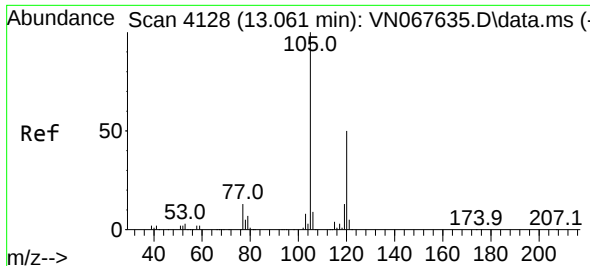

#80
1,3,5-Trimethylbenzene
Concen: 0.239 ug/l
RT: 13.061 min Scan# 4128
Delta R.T. -0.000 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:105 Resp: 3646
Ion Ratio Lower Upper
105 100
120 46.1 22.2 66.6

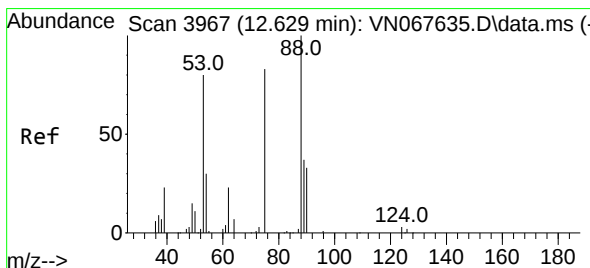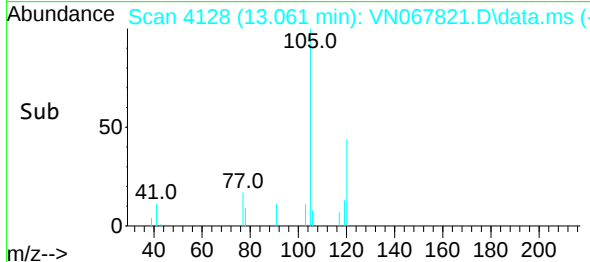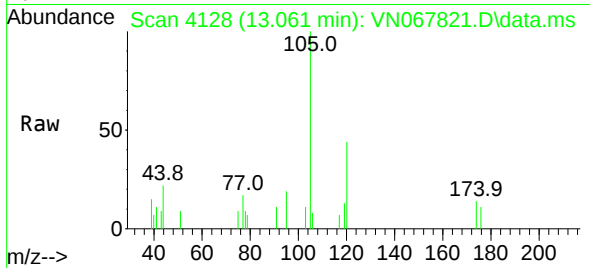

#81
trans-1,4-Dichloro-2-butene
Concen: 101.685 ug/l
RT: 12.733 min Scan# 4006
Delta R.T. 0.104 min
Lab File: VN067821.D
Acq: 20 Jul 2021 16:47

Tgt Ion: 75 Resp: 150013
Ion Ratio Lower Upper
75 100
53 0.1 87.6 131.4#
89 0.0 37.8 56.8#

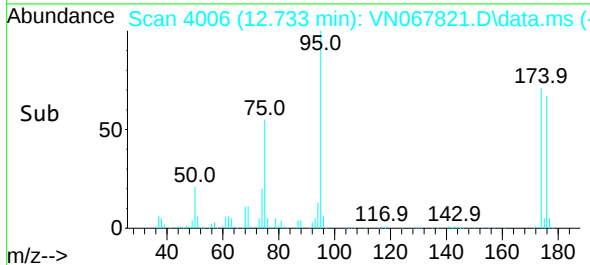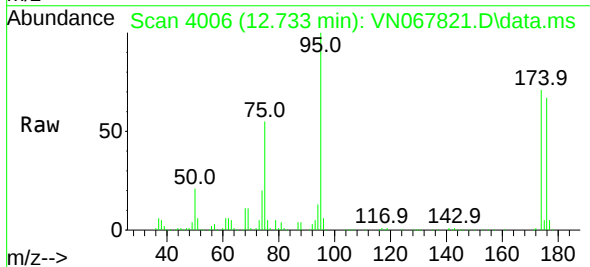

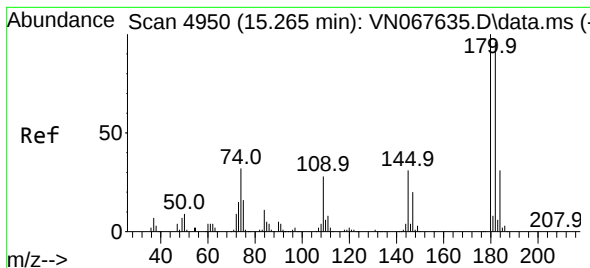

#93

1,2,4-Trichlorobenzene

Concen: 2.840 ug/l

RT: 15.273 min Scan# 4953

Delta R.T. 0.008 min

Lab File: VN067821.D

Acq: 20 Jul 2021 16:47





Tgt Ion:180 Resp: 679

Ion Ratio Lower Upper

180 100

182 91.2 47.5 142.5

145 29.7 17.2 51.6

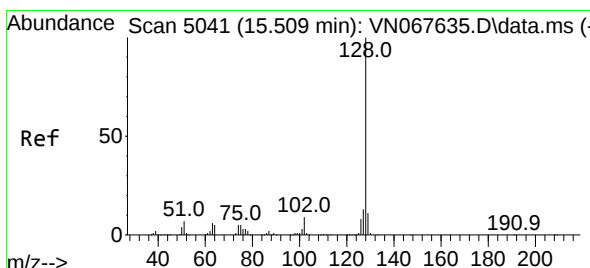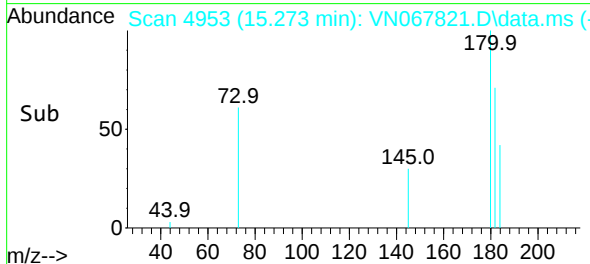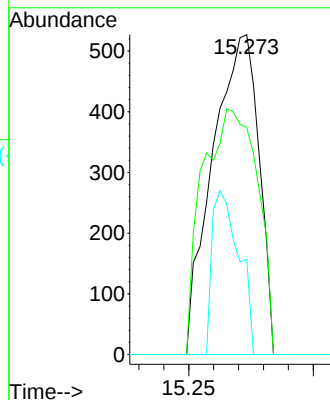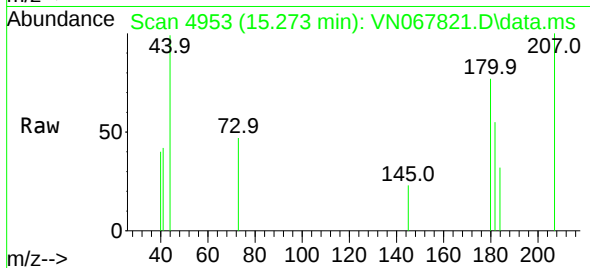

#95

Naphthalene

Concen: 3.375 ug/l

RT: 15.509 min Scan# 5041

Delta R.T. 0.000 min

Lab File: VN067821.D

Acq: 20 Jul 2021 16:47




Tgt Ion:128 Resp: 4404


Ion Ratio Lower Upper

128 100

127 15.2 10.6 15.8


129 3.1 8.6 12.8#

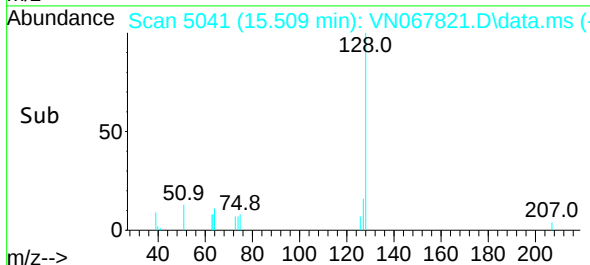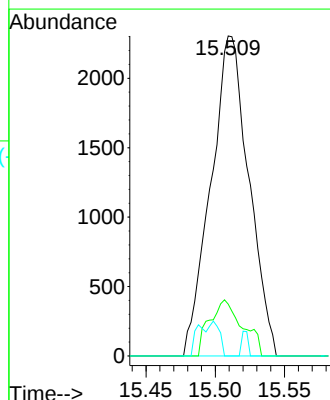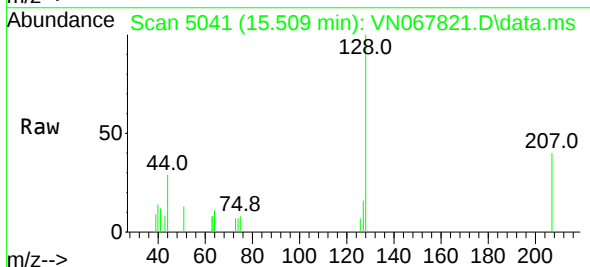

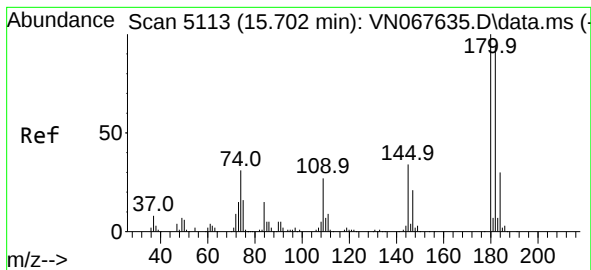

#96
 1,2,3-Trichlorobenzene
 Concen: 2.829 ug/l
 RT: 15.700 min Scan# 5112
 Delta R.T. -0.002 min
 Lab File: VN067821.D
 Acq: 20 Jul 2021 16:47

Instrument :
 MSVOA_N
 ClientSampled :

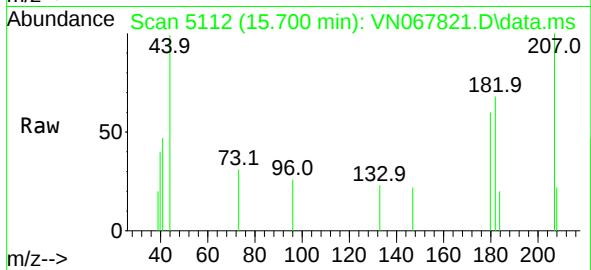

Tgt Ion:	180	Resp:	773
Ion	Ratio	Lower	Upper
180	100		
182	102.5	47.8	143.3
145	3.1	18.2	54.6#

