

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072023\
 Data File : VN078585.D
 Acq On : 20 Jul 2023 11:09
 Operator : JC\MD
 Sample : VN0720MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0720MBL01

Quant Time: Jul 21 06:08:04 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.235	168	394252	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	723771	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	663958	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	234548	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.588	65	271379	51.345	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	102.700%
35) Dibromofluoromethane	8.177	113	274143	55.797	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	111.600%
50) Toluene-d8	10.571	98	849100	45.748	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	91.500%
62) 4-Bromofluorobenzene	12.853	95	293214	51.288	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	102.580%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072023\
Data File : VN078585.D
Acq On : 20 Jul 2023 11:09
Operator : JC\MD
Sample : VN0720MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0720MBL01

Quant Time: Jul 21 06:08:04 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration




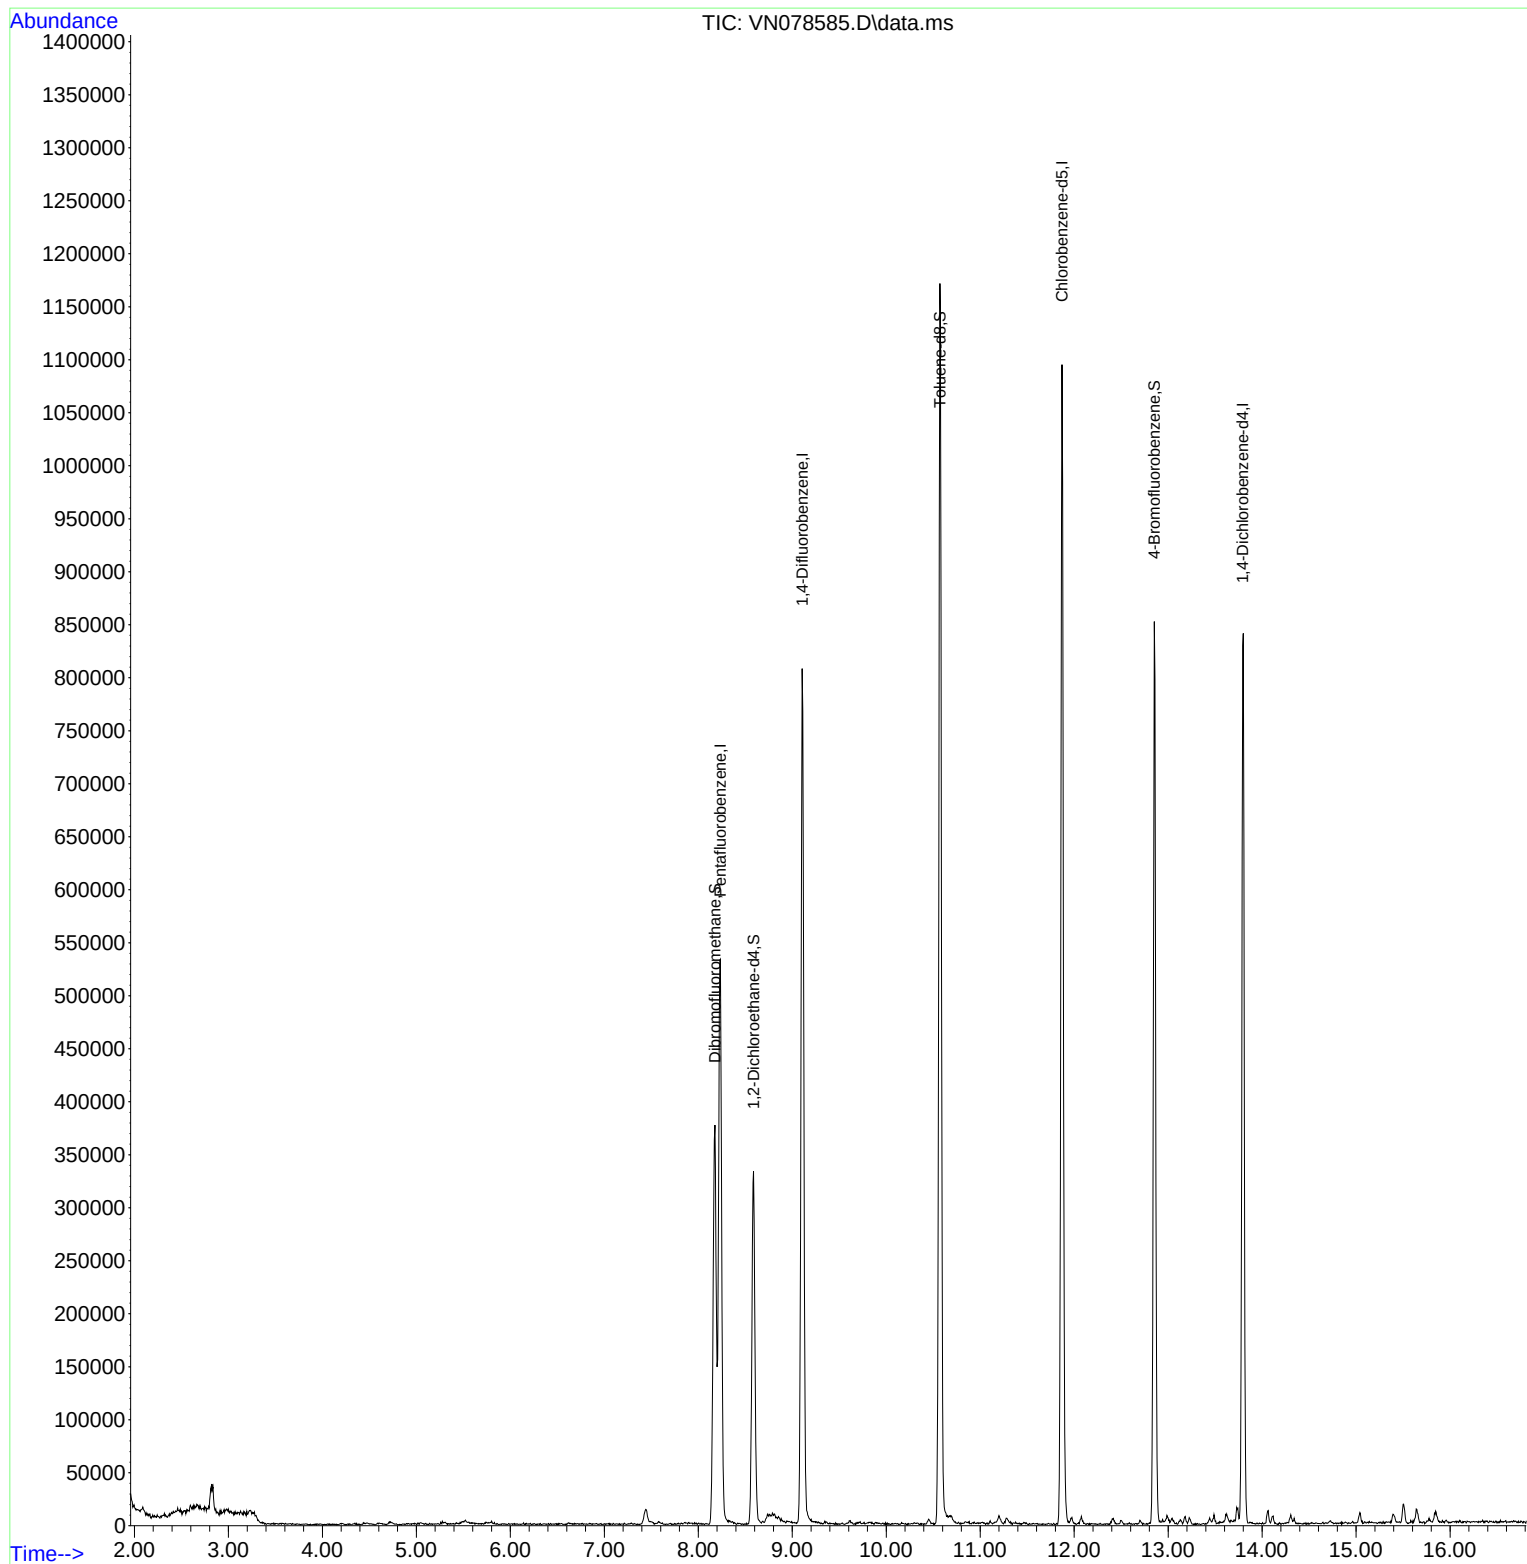


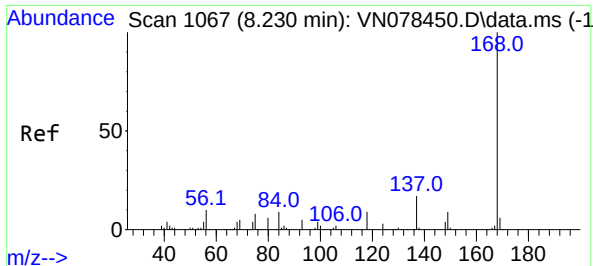

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.235 min Scan# 1067
Delta R.T. 0.005 min
Lab File: VN078585.D
Acq: 20 Jul 2023 11:09




Instrument :
MSVOA_N
ClientSampleId :
VN0720MBL01


Tgt Ion:168 Resp: 394252
Ion Ratio Lower Upper
168 100
99 58.7 53.0 79.6

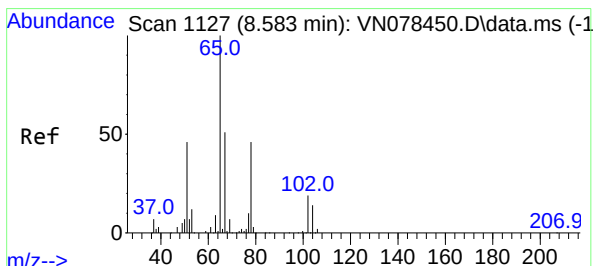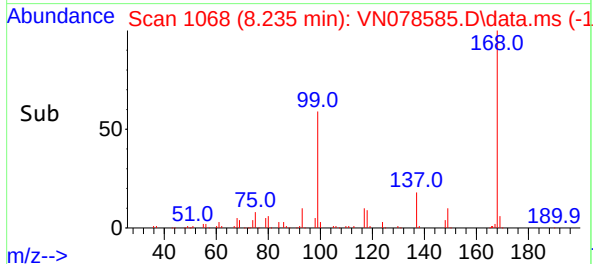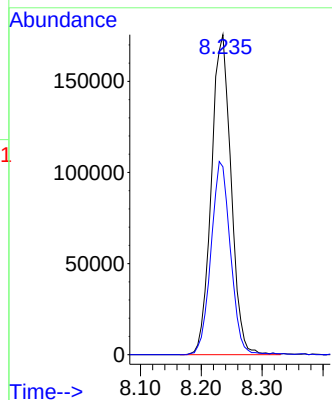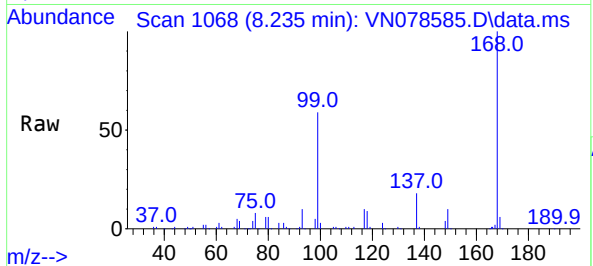

#33
1,2-Dichloroethane-d4
Concen: 51.345 ug/l
RT: 8.588 min Scan# 1128
Delta R.T. 0.005 min
Lab File: VN078585.D
Acq: 20 Jul 2023 11:09

Tgt Ion: 65 Resp: 271379
Ion Ratio Lower Upper
65 100
67 51.6 0.0 106.6

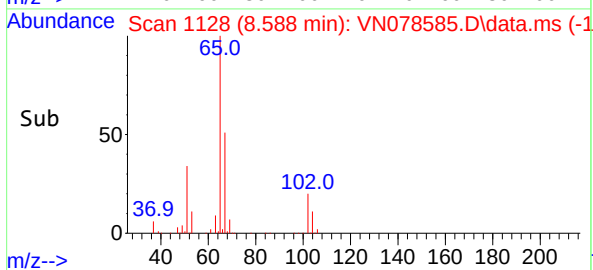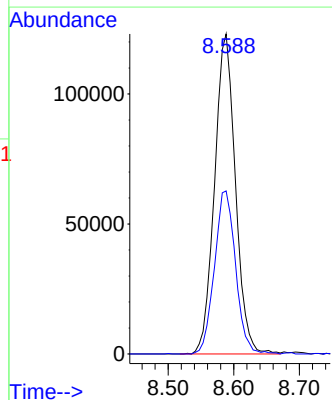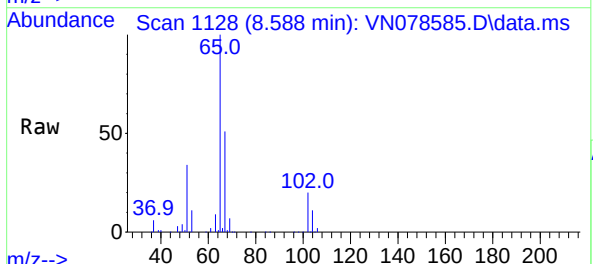

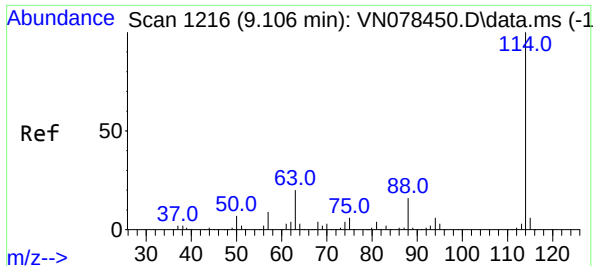

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.106 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN078585.D

Acq: 20 Jul 2023 11:09

Instrument :

MSVOA_N

ClientSampleId :

VN0720MBL01





Tgt Ion:114 Resp: 723771

Ion Ratio Lower Upper

114 100

63 19.0 0.0 36.4

88 13.9 0.0 30.6

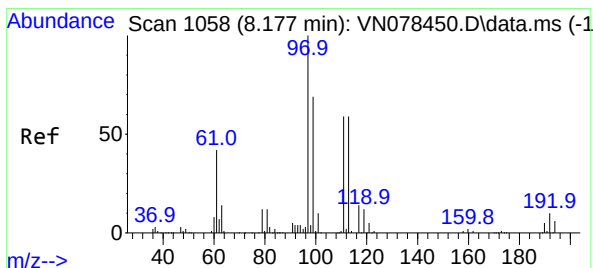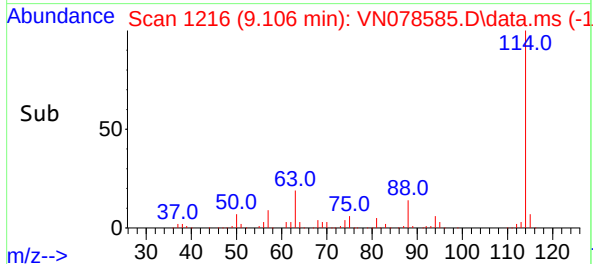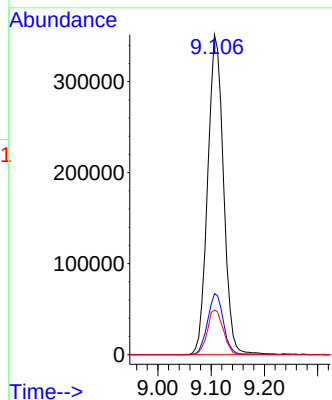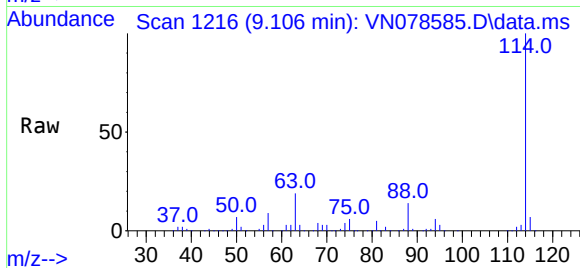

#35

Dibromofluoromethane

Concen: 55.797 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078585.D

Acq: 20 Jul 2023 11:09




Tgt Ion:113 Resp: 274143


Ion Ratio Lower Upper

113 100

111 101.5 82.6 123.8

192 17.4 12.7 19.1


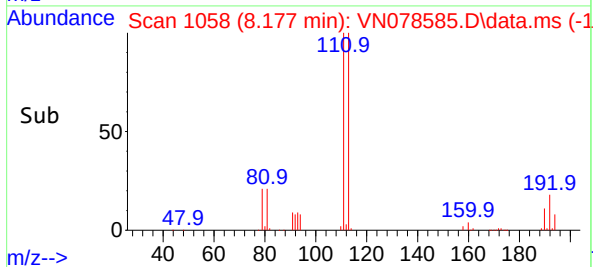
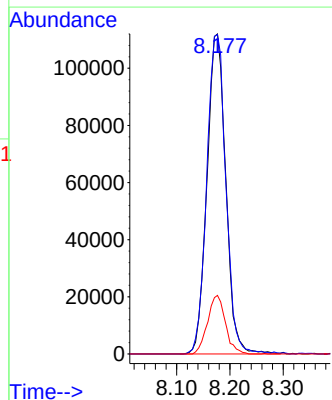
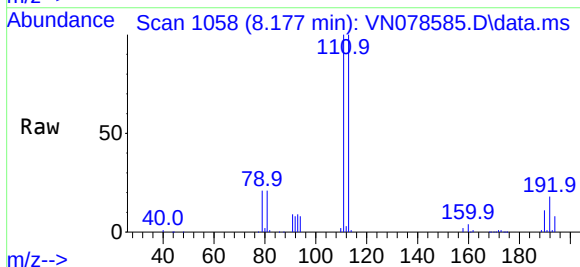


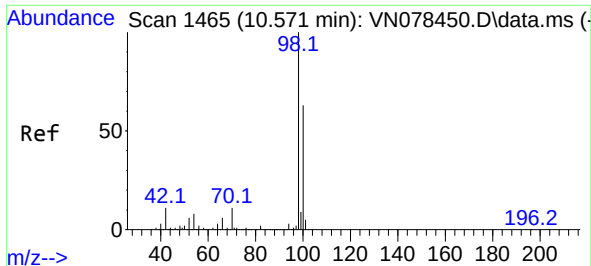

#50
Toluene-d8
Concen: 45.748 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078585.D
Acq: 20 Jul 2023 11:09




Instrument :
MSVOA_N
ClientSampleId :
VN0720MBL01


Tgt Ion: 98 Resp: 849100
Ion Ratio Lower Upper
98 100
100 62.5 52.0 78.0

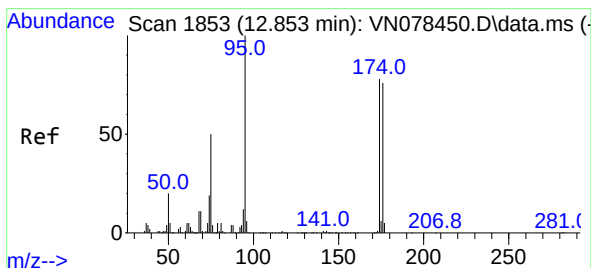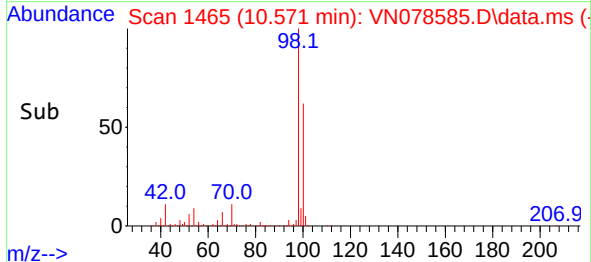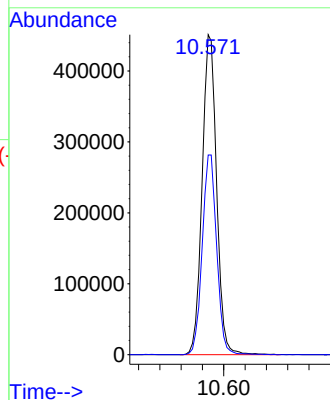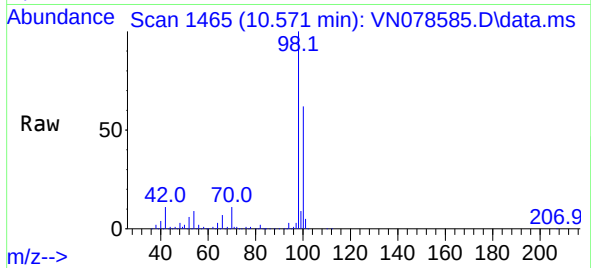

#62
4-Bromofluorobenzene
Concen: 51.288 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.000 min
Lab File: VN078585.D
Acq: 20 Jul 2023 11:09

Tgt Ion: 95 Resp: 293214
Ion Ratio Lower Upper
95 100
174 78.6 0.0 143.8
176 73.7 0.0 135.8


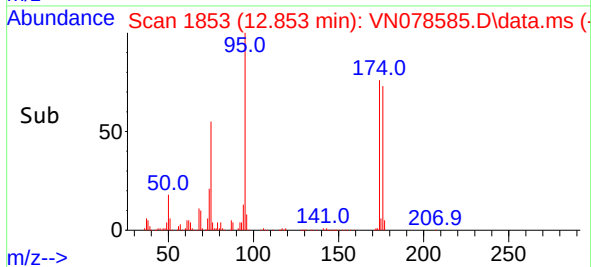
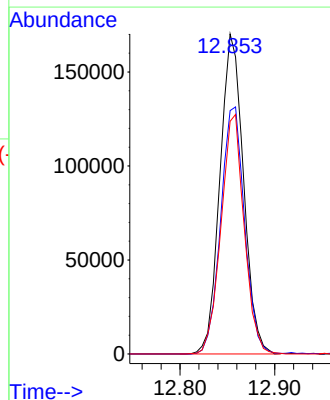
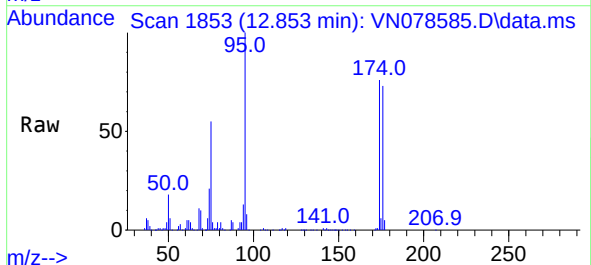


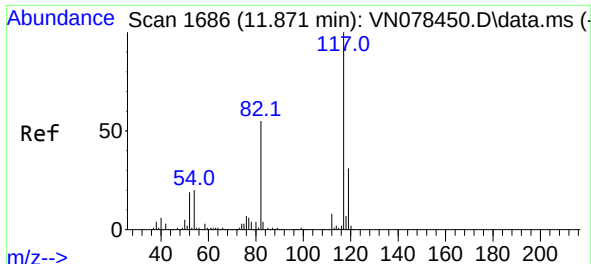

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1
Delta R.T. -0.001 min
Lab File: VN078585.D
Acq: 20 Jul 2023 11:09

Instrument :
MSVOA_N
ClientSampleId :
VN0720MBL01

Tgt Ion:117 Resp: 663958
Ion Ratio Lower Upper
117 100
82 53.3 44.0 66.0
119 31.9 25.6 38.4

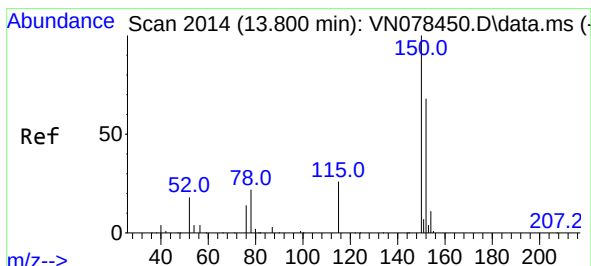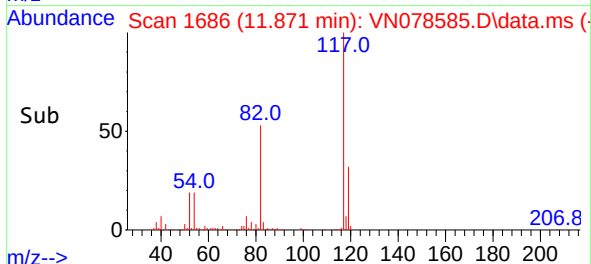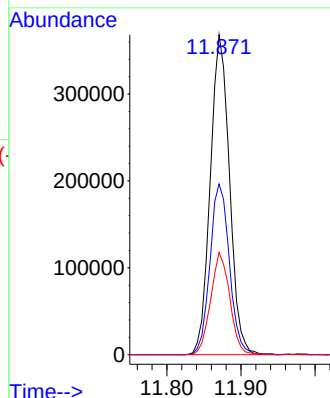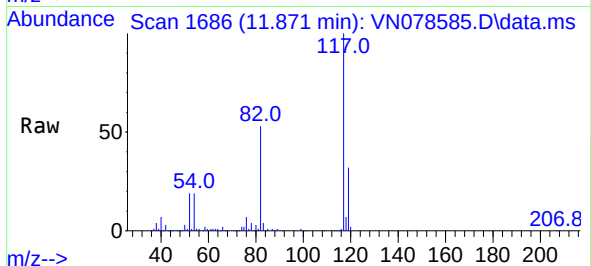

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. -0.006 min
Lab File: VN078585.D
Acq: 20 Jul 2023 11:09

Tgt Ion:152 Resp: 234548
Ion Ratio Lower Upper
152 100
115 61.6 32.3 96.8
150 157.7 0.0 355.8

