


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072023\
Data File : VN078583.D
Acq On : 20 Jul 2023 10:02
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

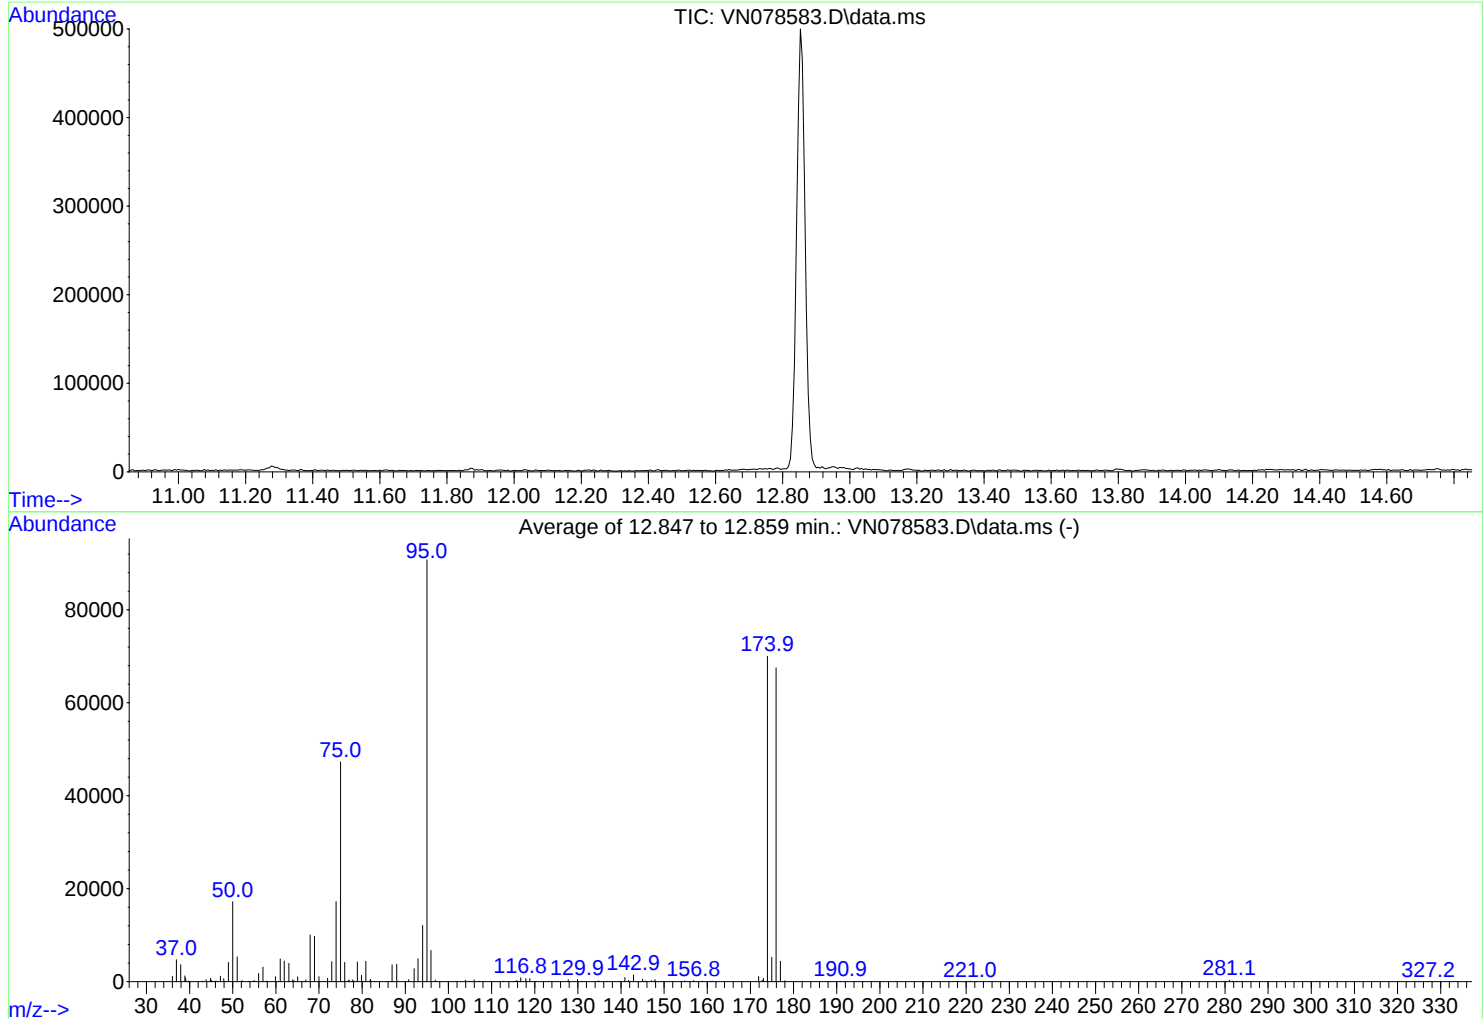

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	17181	PASS
75	95	30	60	52.1	47269	PASS
95	95	100	100	100.0	90752	PASS
96	95	5	9	7.4	6723	PASS
173	174	0.00	2	1.0	696	PASS
174	95	50	100	77.1	69995	PASS
175	174	5	9	7.5	5226	PASS
176	174	95	101	96.4	67493	PASS
177	176	5	9	6.5	4356	PASS

Average of 12.847 to 12.859 min.: VN078583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.00	1127	46.15	133	56.00	1771	67.95	1004
36.95	4706	47.15	1164	57.00	3131	68.95	976
37.95	3665	47.90	613	57.90	144	70.00	106
38.90	1256	49.00	4120	59.90	1061	72.00	72
39.10	769	50.00	17181	61.00	4896	72.95	4316
39.70	125	51.05	5340	61.95	4446	73.95	17208
42.90	102	51.90	53	63.00	3919	75.00	47269
43.85	402	52.15	237	63.90	415	75.95	4179
44.85	701	53.70	69	64.20	244	76.80	221
45.10	305	54.70	113	65.05	1030	76.95	379
45.70	81	55.00	243	66.95	394	77.80	370

Average of 12.847 to 12.859 min.: VN078583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
78.10	127	92.95	4932	115.10	52	135.00	66
78.90	4245	94.00	12082	115.60	64	136.70	52
79.85	1341	95.00	90752	115.85	273	139.70	68
80.85	4391	95.95	6723	116.75	818	140.10	52
81.80	255	96.95	309	117.95	656	140.90	899
81.95	512	103.80	110	118.85	675	141.75	269
82.80	51	104.00	311	126.00	62	142.90	1447
86.95	3602	104.90	65	127.75	420	145.00	555
88.00	3743	105.95	368	129.90	460	145.60	132
90.80	440	107.10	113	131.00	106	145.80	83
92.05	2779	112.70	59	134.70	132	147.10	244

Average of 12.847 to 12.859 min.: VN078583.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.85	433	175.95	67493				
154.75	158	176.95	4356				
156.85	256	178.00	202				
158.80	117	190.90	76				
160.80	85	221.00	57				
161.10	106	281.05	303				
171.90	1091	281.80	111				
172.70	313	282.80	113				
173.00	696	284.00	81				
173.95	69995	325.00	52				
174.95	5226	327.20	54				

Instrument :

MSVOA_N

ClientSampleId :

BFB