

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
 Data File : VN067830.D
 Acq On : 21 Jul 2021 11:33
 Operator : JC/MD
 Sample : VN0721MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 21 15:08:54 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	403863	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.968	114	745212	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.749	117	676940	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	245164	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	289268	47.393	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	94.780%		
35) Dibromofluoromethane	8.024	113	217019	48.201	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	96.400%		
50) Toluene-d8	10.443	98	881839	46.792	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	93.580%		
62) 4-Bromofluorobenzene	12.734	95	289202	43.441	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	86.880%		
Target Compounds						Qvalue
3) Chloromethane	2.303	50	1097	0.202	ug/l #	80
5) Bromomethane	2.824	94	60	Below Cal	#	4
6) Chloroethane	3.001	64	59	Below Cal	#	44
7) Trichlorofluoromethane	3.376	101	84	Below Cal	#	18
13) Acrolein	4.044	56	560	Below Cal	#	76
16) Acetone	4.296	43	2270	1.182	ug/l #	82
18) Methyl Acetate	4.857	43	1485	0.275	ug/l #	54
20) Methylene Chloride	5.093	84	7271	0.939	ug/l	98
25) 2-Butanone	7.354	43	680	0.213	ug/l #	51
31) Cyclohexane	8.088	56	10051	1.174	ug/l #	19
36) 1,1-Dichloropropene	8.088	75	35445	5.120	ug/l #	52
38) Carbon Tetrachloride	8.088	117	44546	6.524	ug/l #	17
49) 1,4-Dioxane	9.577	88	96	33.028	ug/l #	35
51) 4-Methyl-2-Pentanone	10.333	43	3547	0.489	ug/l	95
53) t-1,3-Dichloropropene	10.717	75	348	1.783	ug/l #	43
58) 2-Chloroethyl Vinyl ether	10.046	63	615	17.282	ug/l #	78
59) 2-Hexanone	11.089	43	7257	1.434	ug/l	100
60) Dibromochloromethane	10.988	129	49	2.364	ug/l #	11
71) Bromoform	12.463	173	24	3.181	ug/l #	29
74) N-amyl acetate	12.396	43	3865	0.539	ug/l #	85
76) 1,2,3-Trichloropropane	12.734	75	161353	32.228	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	161353	103.905	ug/l #	6
82) 4-Chlorotoluene	13.109	91	2834	0.212	ug/l	98
87) 1,3-Dichlorobenzene	13.616	146	1907	0.235	ug/l	91
88) 1,4-Dichlorobenzene	13.616	146	1907	0.229	ug/l	93
89) n-Butylbenzene	13.943	91	5220	0.399	ug/l	96
92) 1,2-Dibromo-3-Chloropr...	14.606	75	432	0.433	ug/l #	62
93) 1,2,4-Trichlorobenzene	15.268	180	3875	3.572	ug/l	94
94) Hexachlorobutadiene	15.370	225	937	0.569	ug/l #	28
95) Naphthalene	15.507	128	21251	4.676	ug/l	99
96) 1,2,3-Trichlorobenzene	15.705	180	5497	3.963	ug/l	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
Data File : VN067830.D
Acq On : 21 Jul 2021 11:33
Operator : JC/MD
Sample : VN0721MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampled :

Quant Time: Jul 21 15:08:54 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration




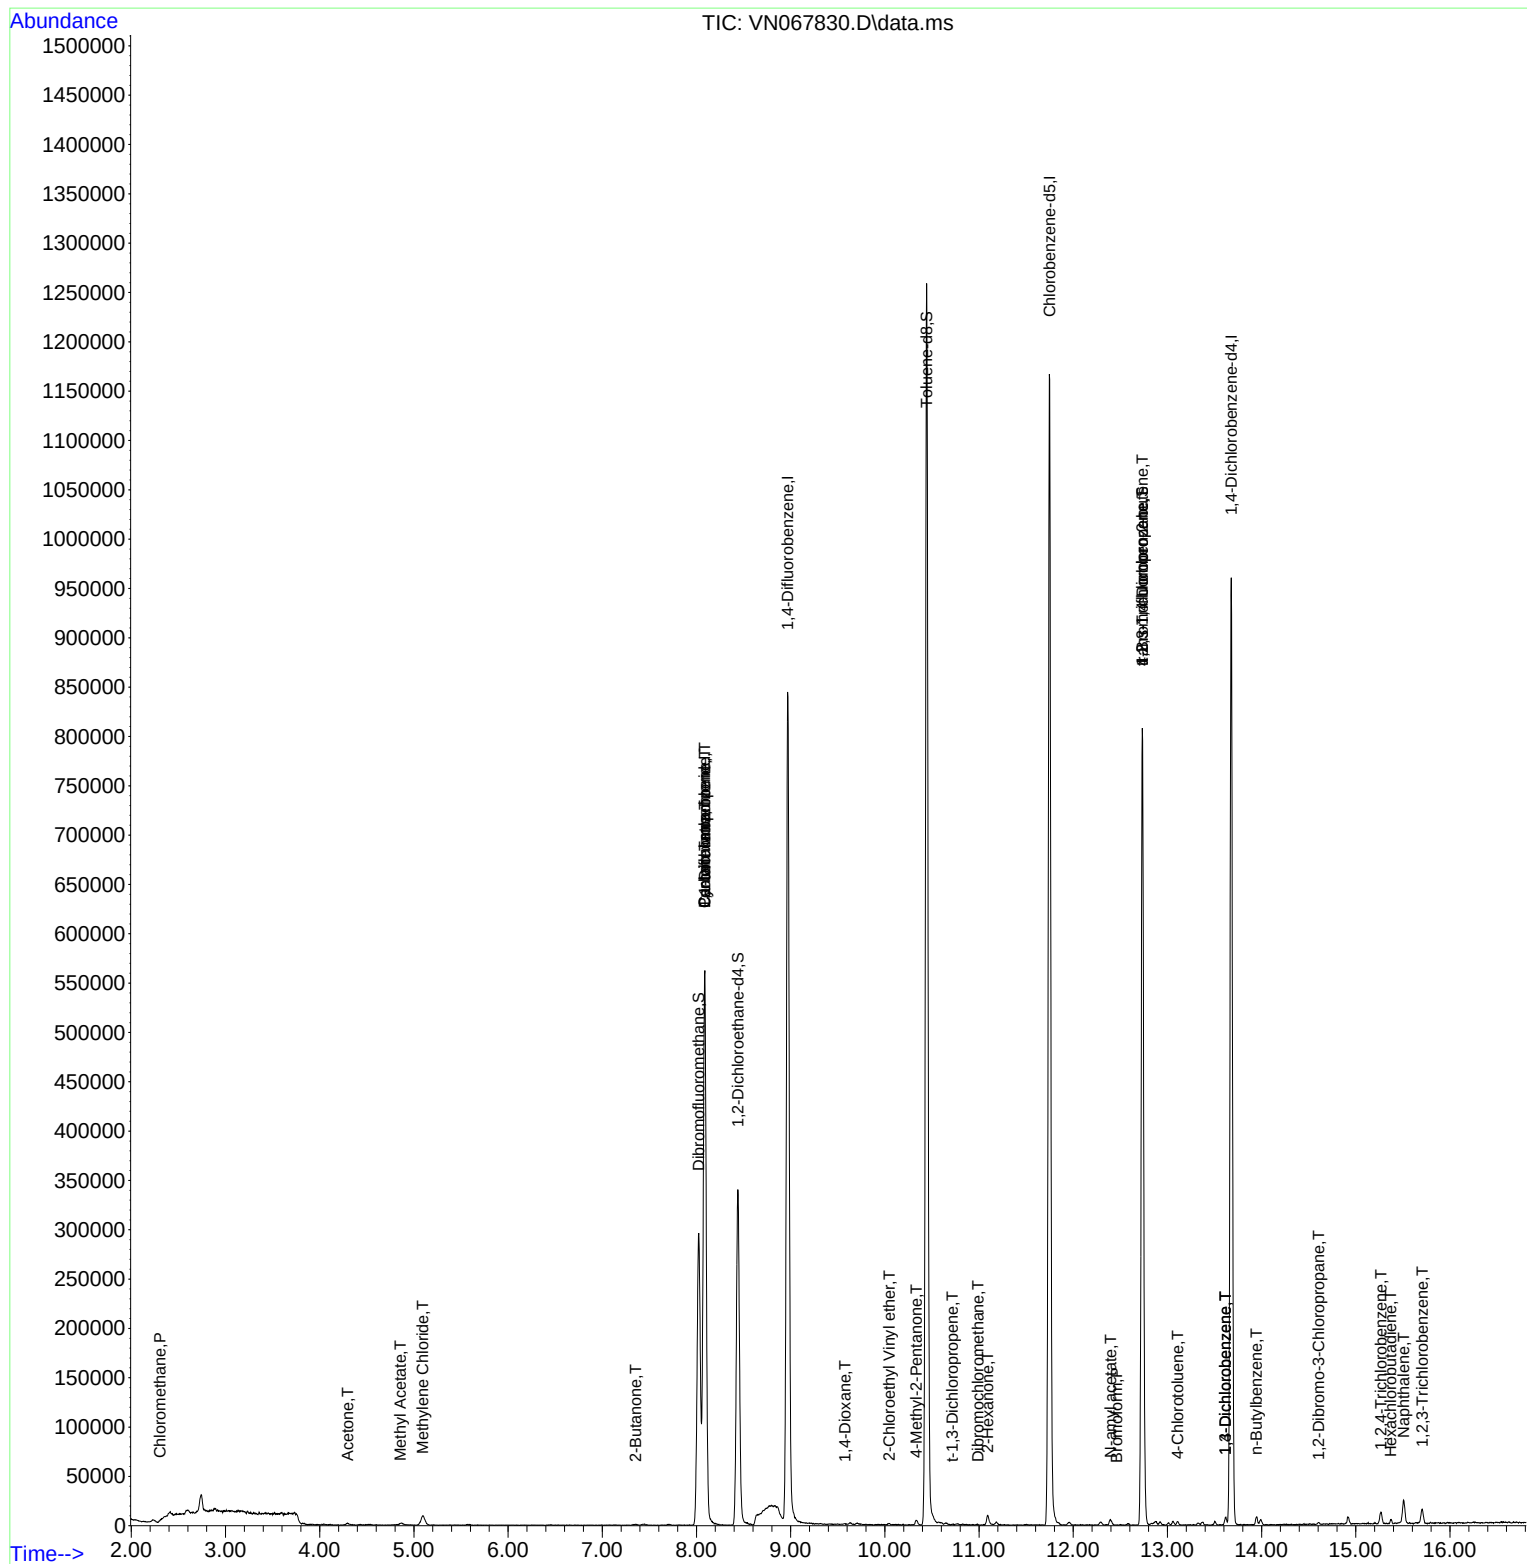




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. 0.002 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:168 Resp: 403863
Ion Ratio Lower Upper
168 100
99 63.9 62.9 94.3

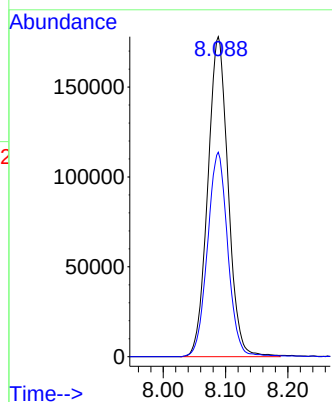

#3
Chloromethane
Concen: 0.202 ug/l
RT: 2.303 min Scan# 117
Delta R.T. 0.002 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 50 Resp: 1097
Ion Ratio Lower Upper
50 100
52 20.6 25.6 38.4#


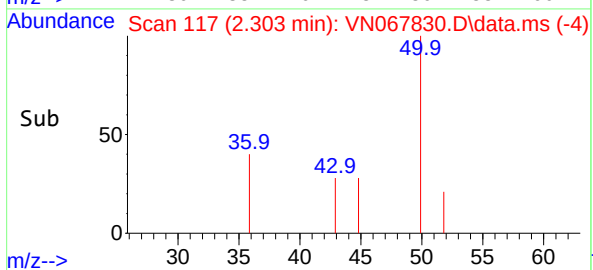
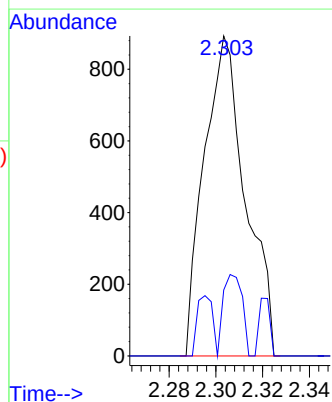





#5
Bromomethane
Concen: Below Cal
RT: 2.824 min Scan# 311
Delta R.T. -0.008 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 94 Resp: 60
Ion Ratio Lower Upper
94 100
96 0.0 73.7 110.5#

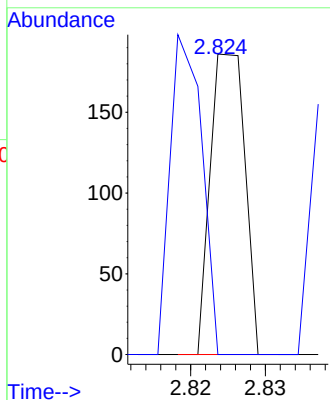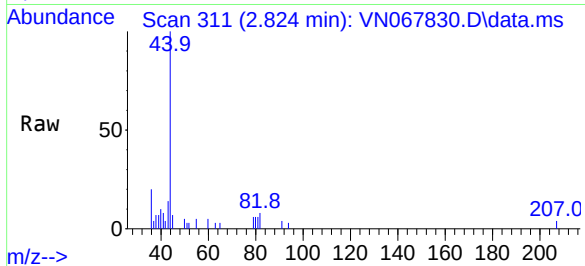

#6
Chloroethane
Concen: Below Cal
RT: 3.001 min Scan# 377
Delta R.T. -0.005 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 64 Resp: 59
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#


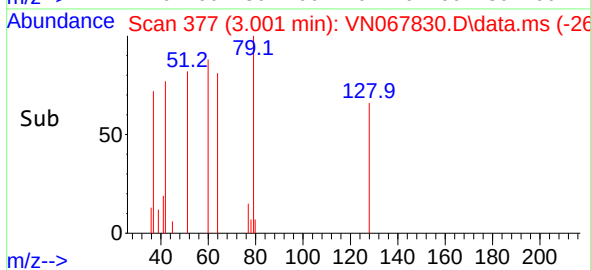
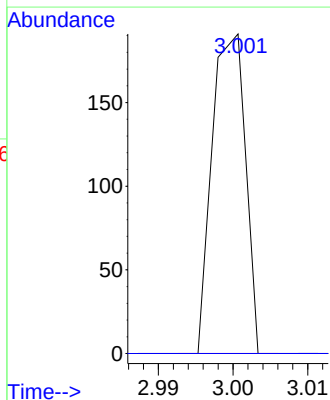
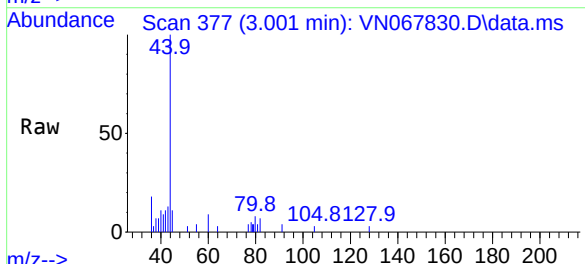




#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.376 min Scan# 517
Delta R.T. 0.011 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:101 Resp: 84
Ion Ratio Lower Upper
101 100
103 0.0 51.2 76.8#

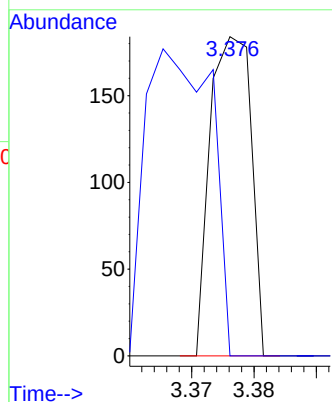

#13
Acrolein
Concen: Below Cal
RT: 4.044 min Scan# 766
Delta R.T. 0.005 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 56 Resp: 560
Ion Ratio Lower Upper
56 100
55 51.4 57.4 86.0#


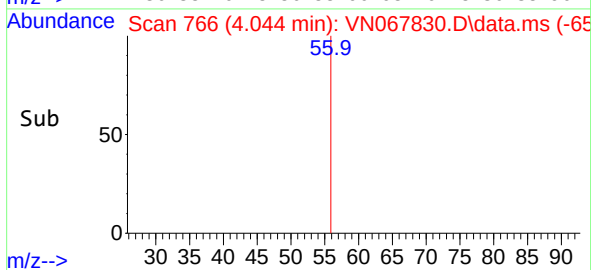
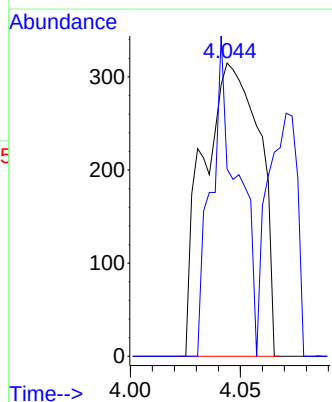





#16
Acetone
Concen: 1.182 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 2270
Ion Ratio Lower Upper
43 100
58 35.8 21.2 31.8#



#18
Methyl Acetate
Concen: 0.275 ug/l
RT: 4.857 min Scan# 1069
Delta R.T. -0.000 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 43 Resp: 1485
Ion Ratio Lower Upper
43 100
74 0.0 17.4 26.0#

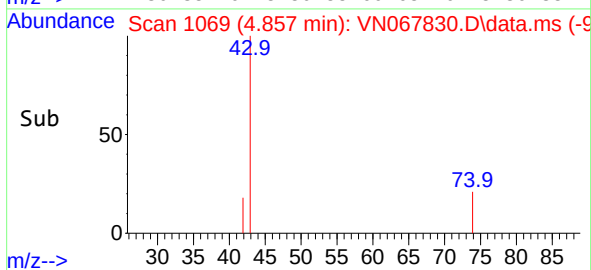







#20
Methylene Chloride
Concen: 0.939 ug/l
RT: 5.093 min Scan# 1157
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Instrument :
MSVOA_N
ClientSampled :

Tgt Ion: 84 Resp: 7271




Ion	Ratio	Lower	Upper
84	100		
49	139.3	110.9	166.3
51	47.4	32.6	49.0
86	65.3	51.6	77.4




#25
2-Butanone
Concen: 0.213 ug/l
RT: 7.354 min Scan# 2000
Delta R.T. 0.017 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 43 Resp: 680

Ion	Ratio	Lower	Upper
43	100		
72	0.0	19.7	29.5#


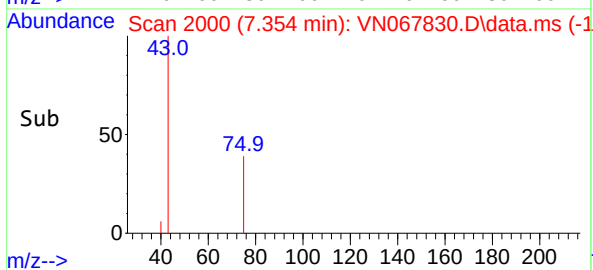






#31
Cyclohexane
Concen: 1.174 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.006 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 10051
Ion Ratio Lower Upper
56 100
69 156.4 27.3 40.9#
84 103.2 64.9 97.3#

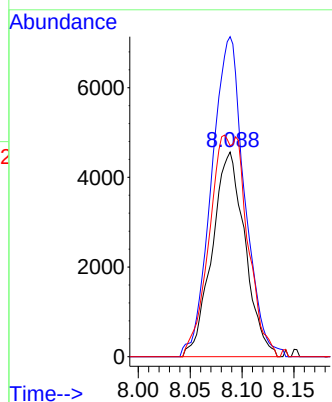

#33
1,2-Dichloroethane-d4
Concen: 47.393 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 65 Resp: 289268
Ion Ratio Lower Upper
65 100
67 50.9 0.0 98.6


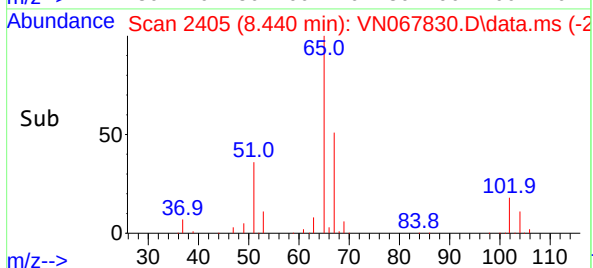






#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.968 min Scan# 2602
Delta R.T. 0.000 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:114 Resp: 745212
Ion Ratio Lower Upper
114 100
63 20.8 0.0 49.0
88 15.6 0.0 36.6

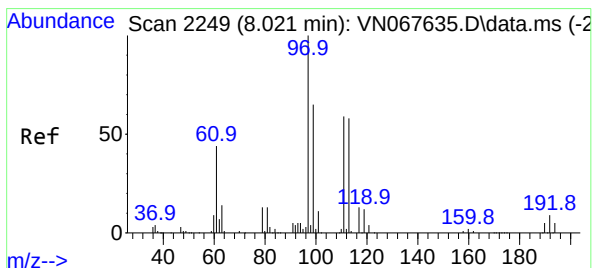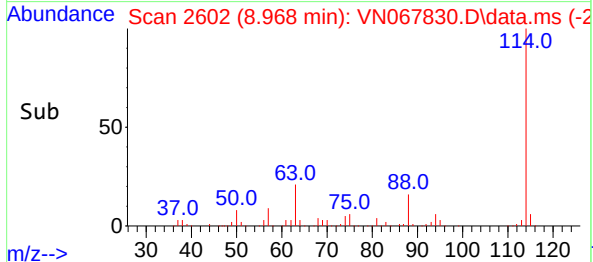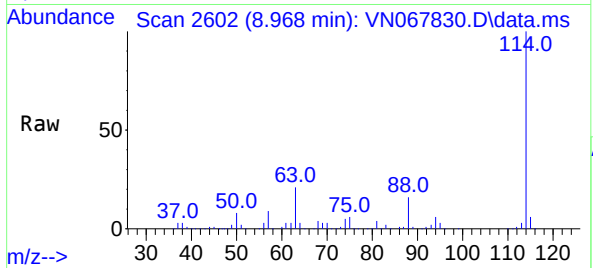

#35
Dibromofluoromethane
Concen: 48.201 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion:113 Resp: 217019
Ion Ratio Lower Upper
113 100
111 103.9 83.8 125.8
192 15.9 13.4 20.0


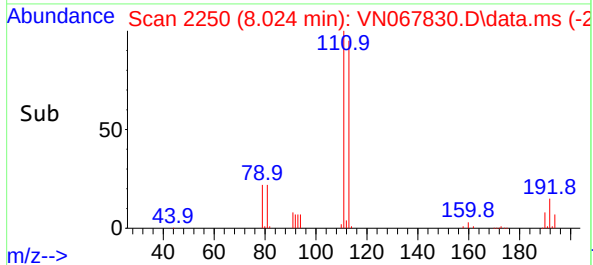

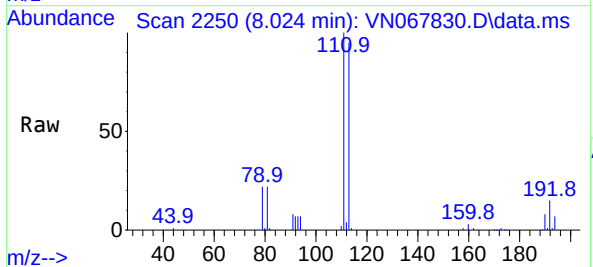




#36
1,1-Dichloropropene
Concen: 5.120 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 35445
Ion Ratio Lower Upper
75 100
110 9.0 15.7 47.0#
77 0.0 24.6 37.0#

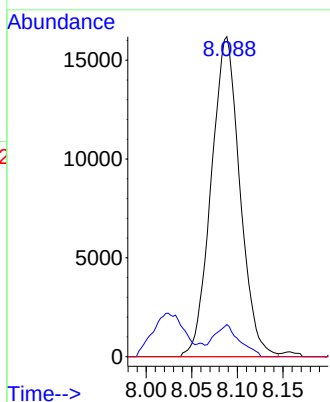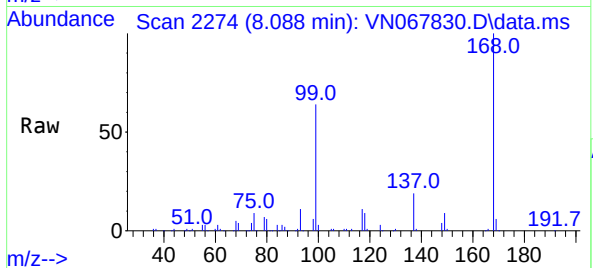

#38
Carbon Tetrachloride
Concen: 6.524 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 117 Resp: 44546
Ion Ratio Lower Upper
117 100
119 5.2 75.4 113.2#
121 0.0 23.5 35.3#


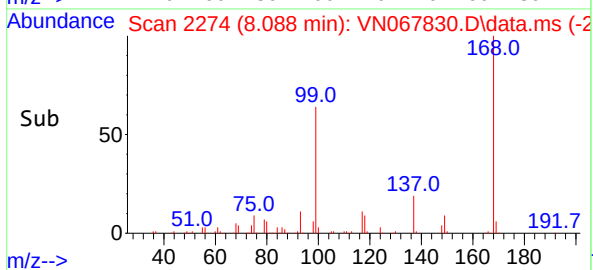
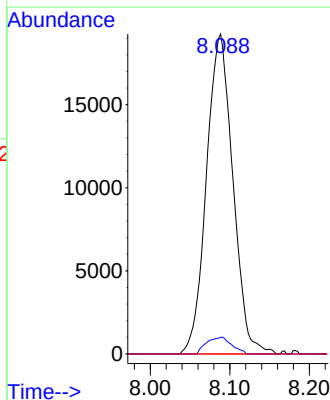





#49
1,4-Dioxane
Concen: 33.028 ug/l
RT: 9.577 min Scan# 2829
Delta R.T. 0.006 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 88 Resp: 96
Ion Ratio Lower Upper
88 100
43 45.8 28.8 43.2#
58 0.0 60.4 90.6#



#50
Toluene-d8
Concen: 46.792 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 98 Resp: 881839
Ion Ratio Lower Upper
98 100
100 63.9 51.7 77.5


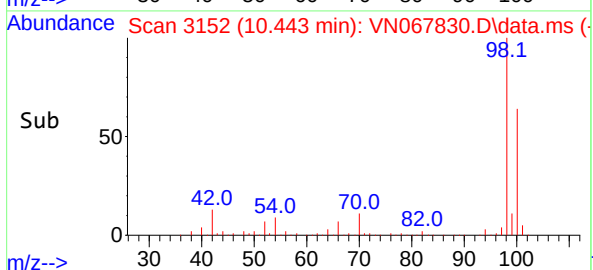






#51
4-Methyl-2-Pentanone
Concen: 0.489 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 3547
Ion Ratio Lower Upper
43 100
58 33.1 28.6 43.0

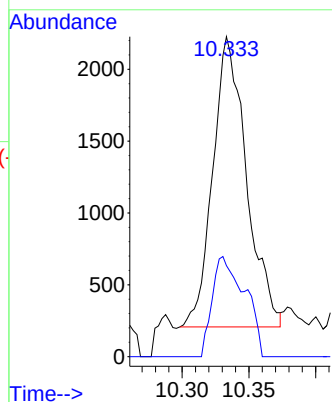

#53
t-1,3-Dichloropropene
Concen: 1.783 ug/l
RT: 10.717 min Scan# 3254
Delta R.T. -0.005 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 75 Resp: 348
Ion Ratio Lower Upper
75 100
77 0.0 25.1 37.7#









#58
2-Chloroethyl Vinyl ether
Concen: 17.282 ug/l
RT: 10.046 min Scan# 3004
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 63 Resp: 615
Ion Ratio Lower Upper
63 100
106 13.8 19.8 29.8#

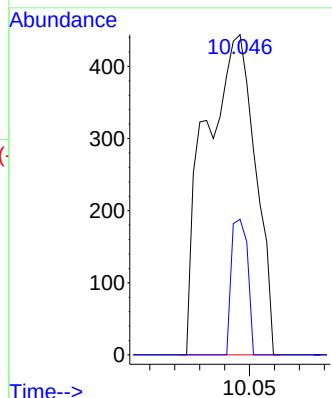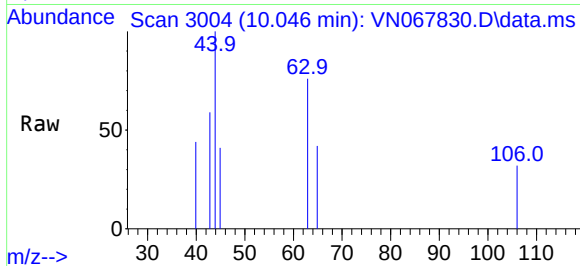

#59
2-Hexanone
Concen: 1.434 ug/l
RT: 11.089 min Scan# 3393
Delta R.T. 0.002 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 43 Resp: 7257
Ion Ratio Lower Upper
43 100
58 49.3 24.7 74.1




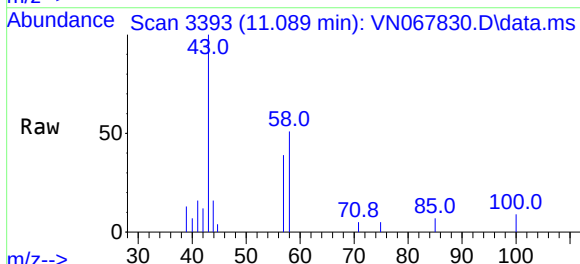




#60
Dibromochloromethane
Concen: 2.364 ug/l
RT: 10.988 min Scan# 3355
Delta R.T. -0.254 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 49
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

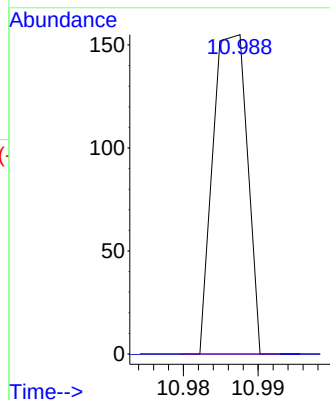

#62
4-Bromofluorobenzene
Concen: 43.441 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 95 Resp: 289202
Ion Ratio Lower Upper
95 100
174 71.8 0.0 122.0
176 68.1 0.0 117.6



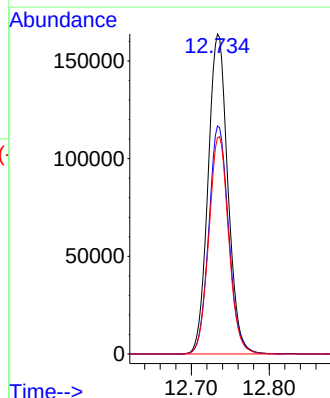





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.749 min Scan# 3639
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 676940
Ion Ratio Lower Upper
117 100
82 57.1 53.1 79.7
119 31.9 25.5 38.3

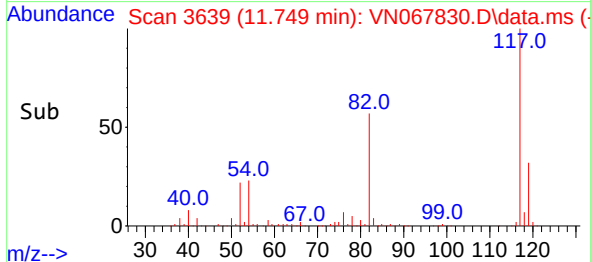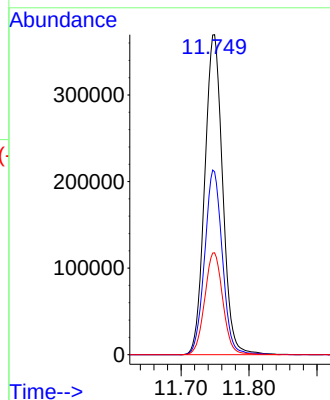

#71
Bromoform
Concen: 3.181 ug/l
RT: 12.463 min Scan# 3905
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion:173 Resp: 24
Ion Ratio Lower Upper
173 100
175 0.0 23.9 71.8#
254 0.0 0.0 0.0



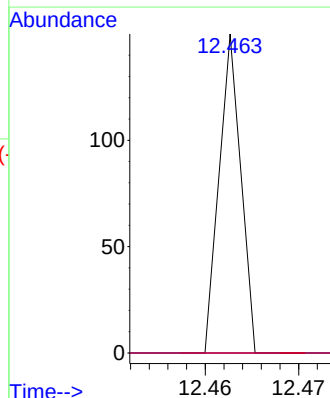





#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:152 Resp: 245164
Ion Ratio Lower Upper
152 100
115 63.0 36.1 108.5
150 160.0 0.0 351.8

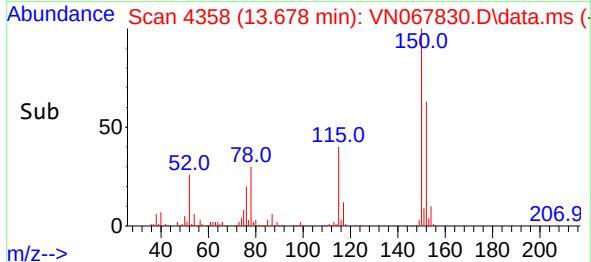

#74
N-ethyl acetate
Concen: 0.539 ug/l
RT: 12.396 min Scan# 3880
Delta R.T. 0.006 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 43 Resp: 3865
Ion Ratio Lower Upper
43 100
70 21.5 29.4 44.2#
55 21.9 17.0 25.4
61 17.9 17.6 26.4


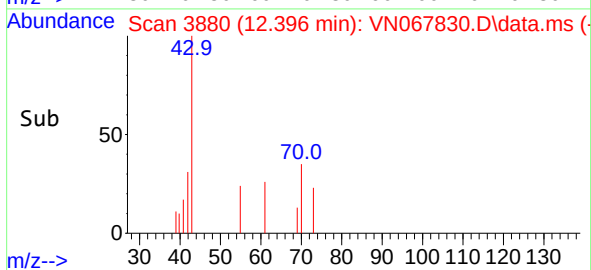






#76
1,2,3-Trichloropropane
Concen: 32.228 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 161353
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

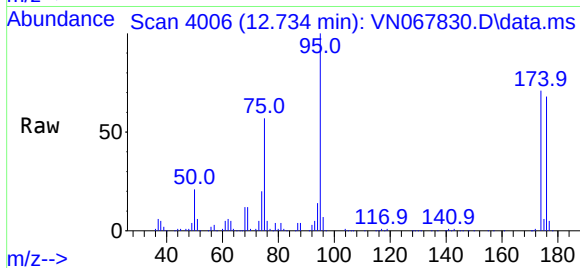

#81
trans-1,4-Dichloro-2-butene
Concen: 103.905 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 75 Resp: 161353
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#


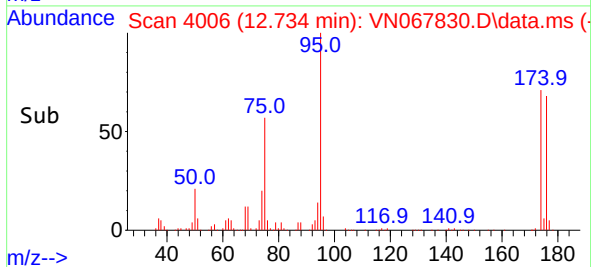

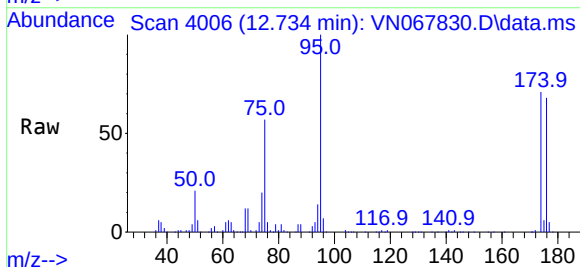




#82
4-Chlorotoluene
Concen: 0.212 ug/l
RT: 13.109 min Scan# 4146
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 91 Resp: 2834
Ion Ratio Lower Upper
91 100
126 30.8 14.8 44.4



#87
1,3-Dichlorobenzene
Concen: 0.235 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33


Tgt Ion:146 Resp: 1907
Ion Ratio Lower Upper
146 100
111 43.3 24.3 72.8
148 56.7 32.0 96.0

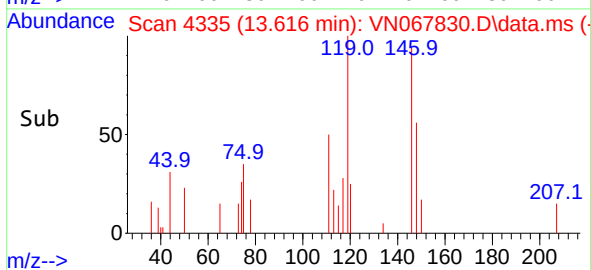






#88
1,4-Dichlorobenzene
Concen: 0.229 ug/l
RT: 13.616 min Scan# 4335
Delta R.T. -0.080 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion:146 Resp: 1907
Ion Ratio Lower Upper
146 100
111 43.3 23.4 70.2
148 56.7 31.8 95.3




#89
n-Butylbenzene
Concen: 0.399 ug/l
RT: 13.943 min Scan# 4457
Delta R.T. -0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33



Tgt Ion: 91 Resp: 5220
Ion Ratio Lower Upper
91 100
92 53.2 25.7 77.1
134 25.3 11.2 33.6



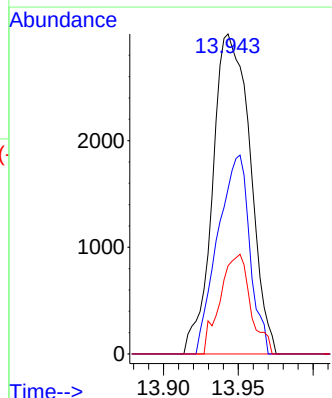





#92
1,2-Dibromo-3-Chloropropane
Concen: 0.433 ug/l
RT: 14.606 min Scan# 4704
Delta R.T. 0.001 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 432
Ion Ratio Lower Upper
75 100
155 43.8 29.8 89.5
157 31.7 37.6 112.8#

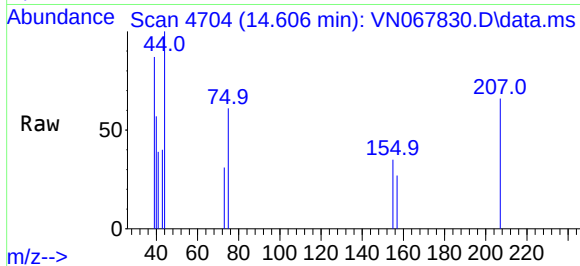

#93
1,2,4-Trichlorobenzene
Concen: 3.572 ug/l
RT: 15.268 min Scan# 4951
Delta R.T. 0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33

Tgt Ion: 180 Resp: 3875
Ion Ratio Lower Upper
180 100
182 90.0 47.5 142.5
145 28.9 17.2 51.6


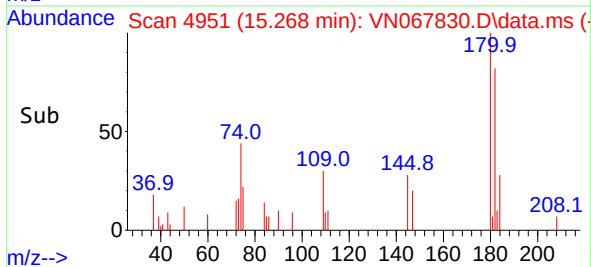

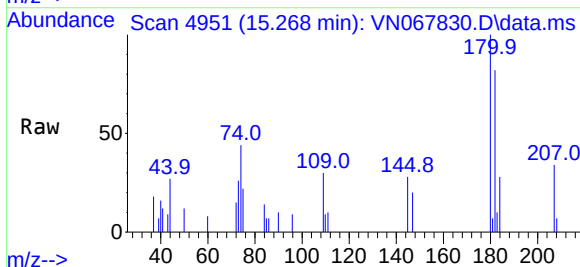




#94
Hexachlorobutadiene
Concen: 0.569 ug/l
RT: 15.370 min Scan# 4989
Delta R.T. -0.003 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:225 Resp: 937
Ion Ratio Lower Upper
225 100
223 13.4 31.4 94.0#
227 0.0 31.2 93.6#

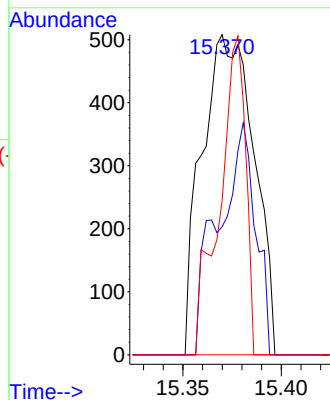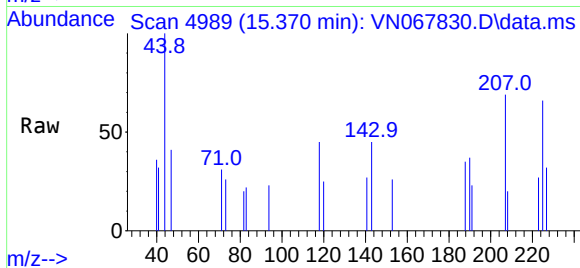

#95
Naphthalene
Concen: 4.676 ug/l
RT: 15.507 min Scan# 5040
Delta R.T. -0.002 min
Lab File: VN067830.D
Acq: 21 Jul 2021 11:33


Tgt Ion:128 Resp: 21251
Ion Ratio Lower Upper
128 100
127 12.8 10.6 15.8
129 10.9 8.6 12.8

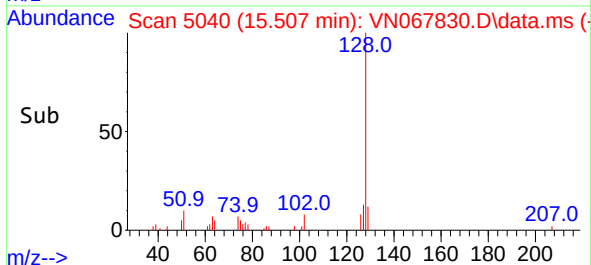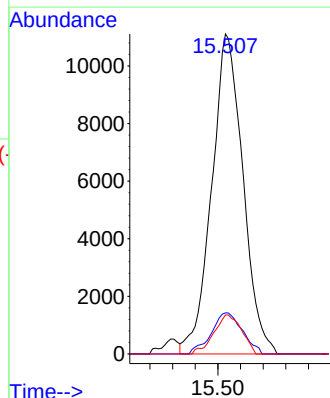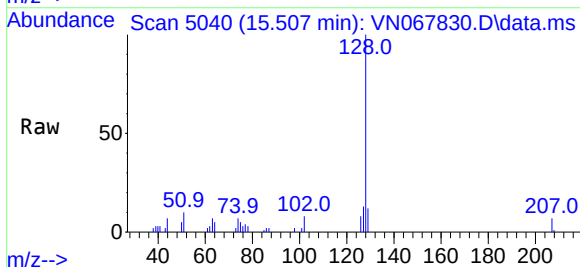



#96
 1,2,3-Trichlorobenzene
 Concen: 3.963 ug/l
 RT: 15.705 min Scan# 5114
 Delta R.T. 0.003 min
 Lab File: VN067830.D
 Acq: 21 Jul 2021 11:33

Instrument :
 MSVOA_N
 ClientSampleId :



Tgt Ion:	180	Resp:	5497
Ion Ratio	Lower	Upper	
180	100		
182	81.5	47.8	143.3
145	34.8	18.2	54.6

