

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
 Data File : VN067843.D
 Acq On : 21 Jul 2021 17:03
 Operator : JC/MD
 Sample : M3089-15
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 22 02:13:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.088	168	316485	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	601025	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	620235	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	232244	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	248607	51.977	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 103.960%	
35) Dibromofluoromethane	8.024	113	182091	50.146	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 100.300%	
50) Toluene-d8	10.443	98	786408	51.739	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 103.480%	
62) 4-Bromofluorobenzene	12.734	95	270570	50.392	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 100.780%	
Target Compounds						
					Qvalue	
5) Bromomethane	2.883	94	1040	Below Cal		87
6) Chloroethane	2.767	64	50	Below Cal	#	1
11) Tert butyl alcohol	5.396	59	243	0.354	ug/l #	71
13) Acrolein	4.041	56	24	Below Cal	#	14
16) Acetone	4.296	43	40162	26.685	ug/l	95
18) Methyl Acetate	4.865	43	7700	1.821	ug/l #	59
20) Methylene Chloride	5.101	84	32462	8.664	ug/l	88
25) 2-Butanone	7.351	43	8524	3.411	ug/l	94
29) Tetrahydrofuran	7.702	42	4452	2.709	ug/l #	67
31) Cyclohexane	8.086	56	8475	1.264	ug/l #	31
36) 1,1-Dichloropropene	8.088	75	28955	5.186	ug/l #	52
37) Ethyl Acetate	7.351	43	8524	1.576	ug/l #	70
38) Carbon Tetrachloride	8.088	117	34227	6.215	ug/l #	17
41) Methacrylonitrile	7.700	41	2716	0.977	ug/l #	26
43) Isopropyl Acetate	8.566	43	34720	3.649	ug/l #	91
45) 1,2-Dichloropropane	9.623	63	2099	0.496	ug/l #	44
48) Methyl methacrylate	9.545	41	8943	2.125	ug/l #	12
49) 1,4-Dioxane	9.636	88	160	33.983	ug/l #	1
51) 4-Methyl-2-Pentanone	10.336	43	8459	1.447	ug/l #	78
53) t-1,3-Dichloropropene	10.446	75	125	1.762	ug/l	90
54) cis-1,3-Dichloropropene	10.247	75	60621	9.288	ug/l #	61
57) 1,3-Dichloropropane	11.095	76	33549	4.664	ug/l #	43
59) 2-Hexanone	11.095	43	503450	123.381	ug/l #	54
60) Dibromochloromethane	11.497	129	204	2.395	ug/l #	11
71) Bromoform	12.723	173	389	3.267	ug/l #	1
76) 1,2,3-Trichloropropane	12.734	75	148985	31.413	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	148985	101.277	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.263	180	57	2.688	ug/l #	81
95) Naphthalene	15.512	128	1476	3.134	ug/l #	75
96) 1,2,3-Trichlorobenzene	15.705	180	228	2.691	ug/l #	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
Data File : VN067843.D
Acq On : 21 Jul 2021 17:03
Operator : JC/MD
Sample : M3089-15
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 22 02:13:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

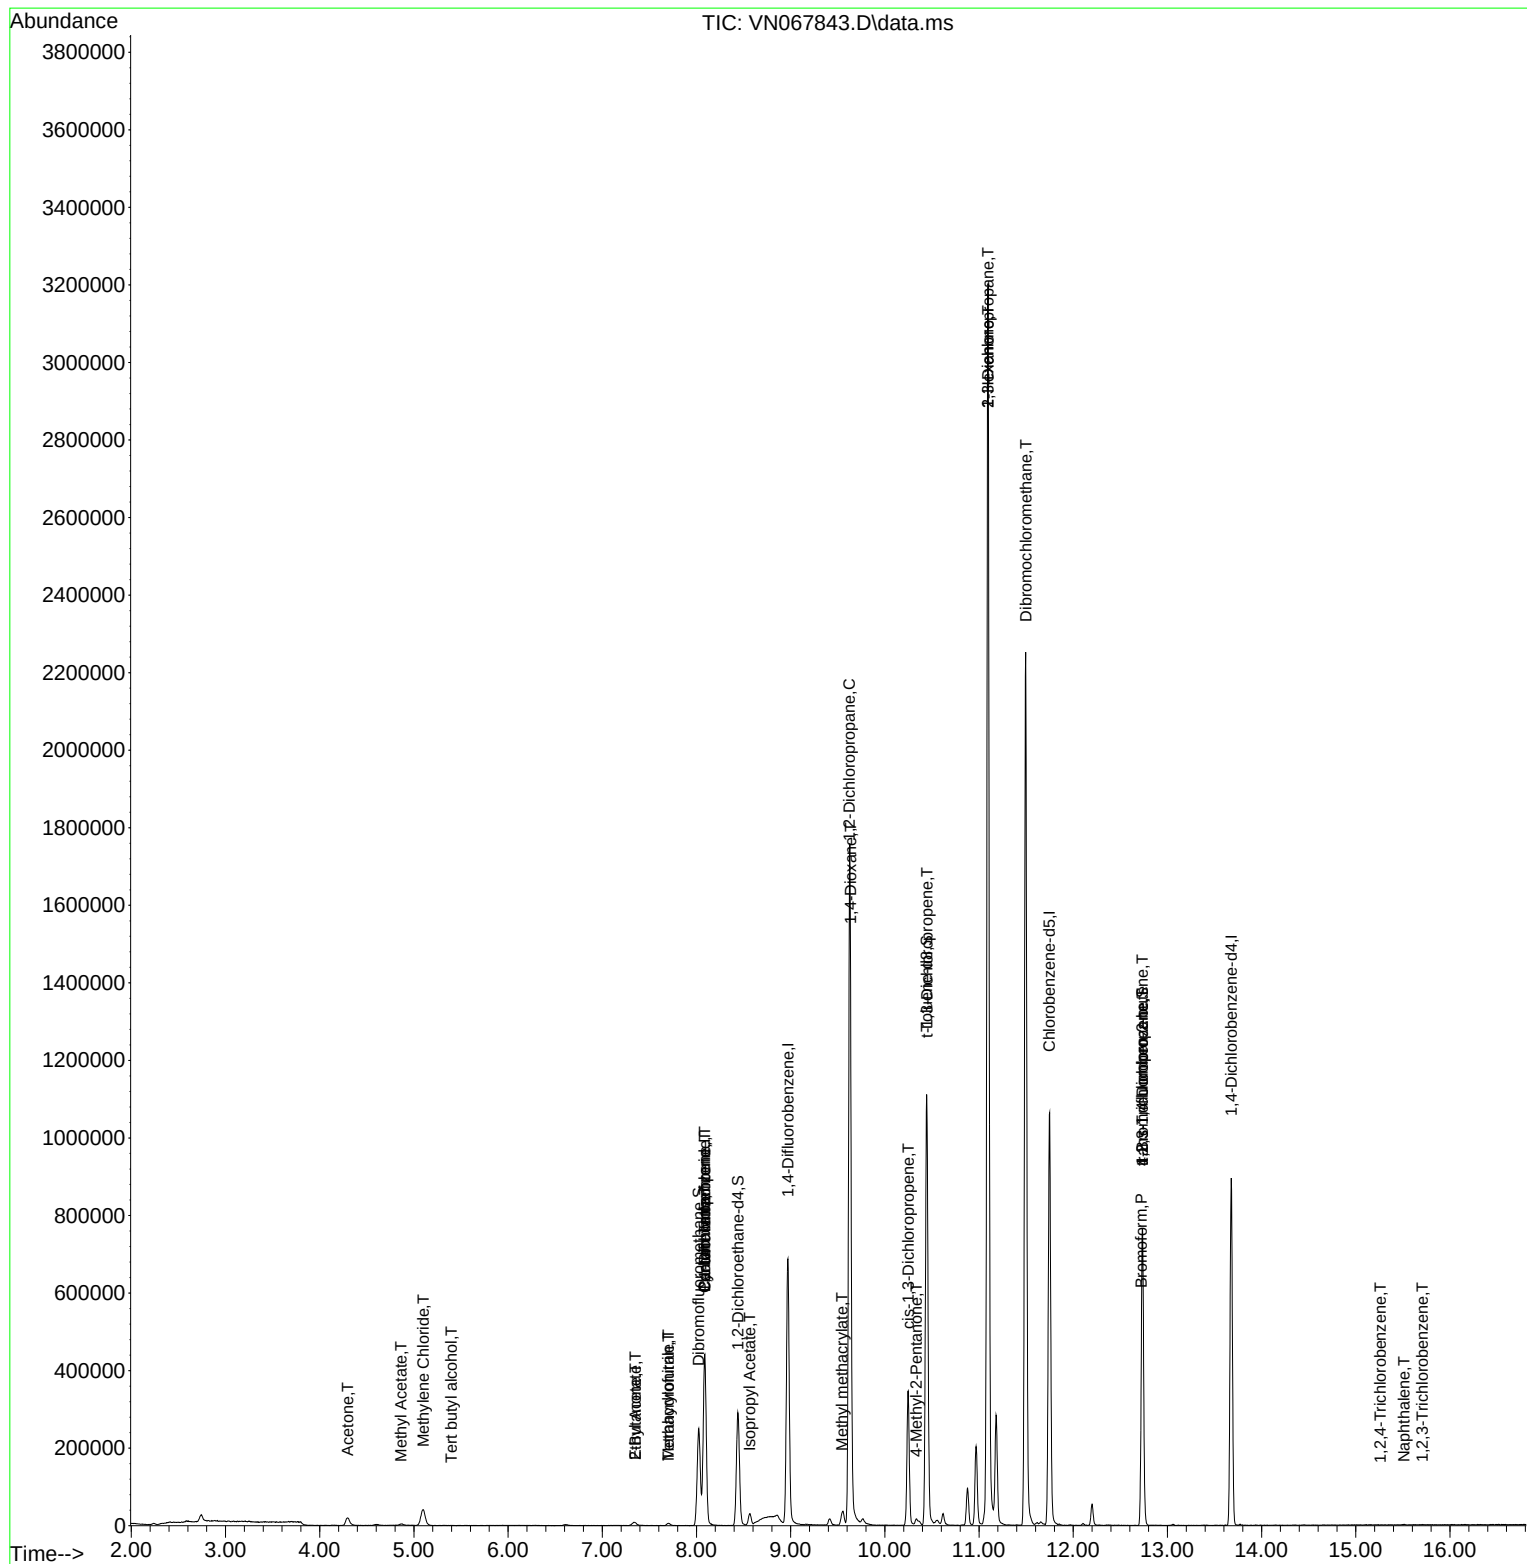



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067843.D





Acq: 21 Jul 2021 17:03

Tgt Ion:168 Resp: 316485

Ion Ratio Lower Upper

168 100

99 63.8 62.9 94.3

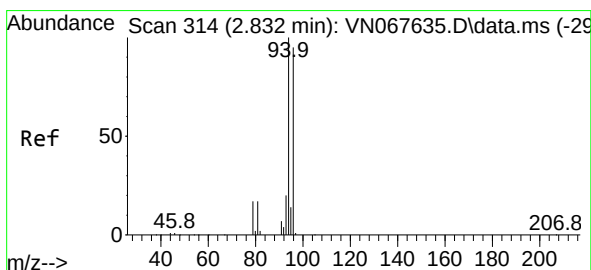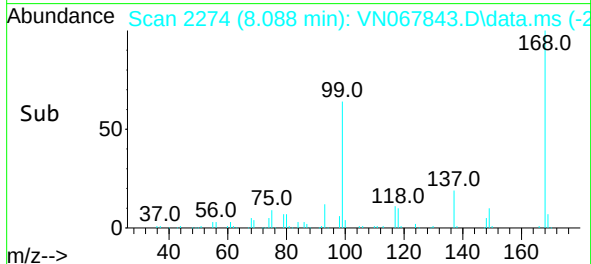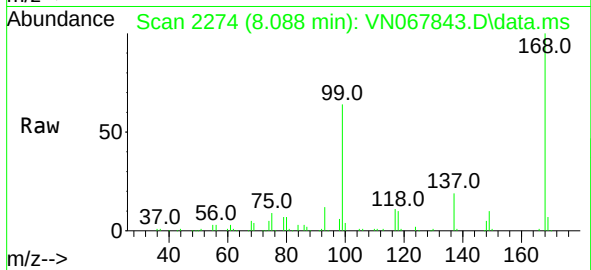

#5

Bromomethane

Concen: Below Cal

RT: 2.883 min Scan# 333

Delta R.T. 0.051 min

Lab File: VN067843.D




Acq: 21 Jul 2021 17:03


Tgt Ion: 94 Resp: 1040

Ion Ratio Lower Upper

94 100

96 79.7 73.7 110.5


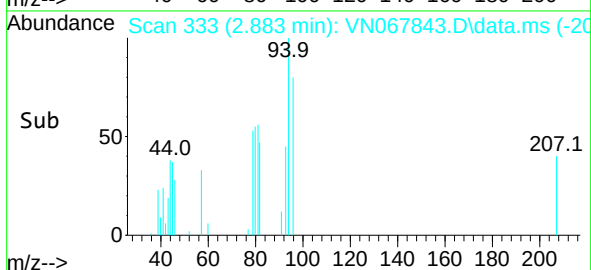

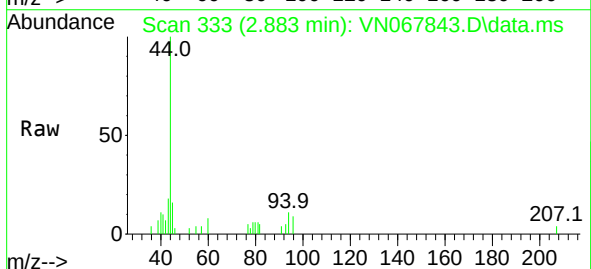




#6
Chloroethane
Concen: Below Cal
RT: 2.767 min Scan# 290
Delta R.T. -0.239 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 64 Resp: 50
Ion Ratio Lower Upper
64 100
66 119.1 24.7 37.1#

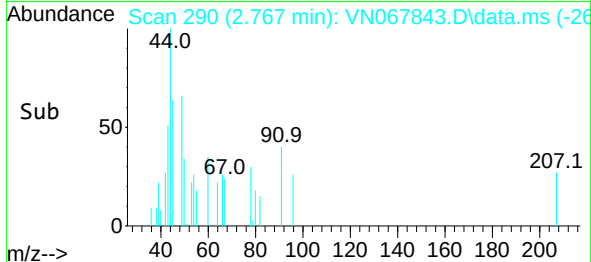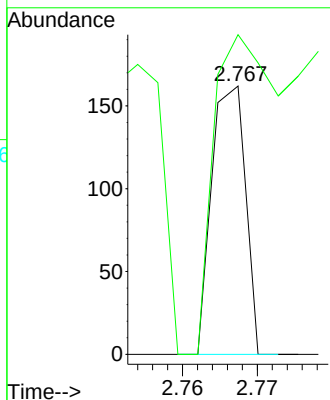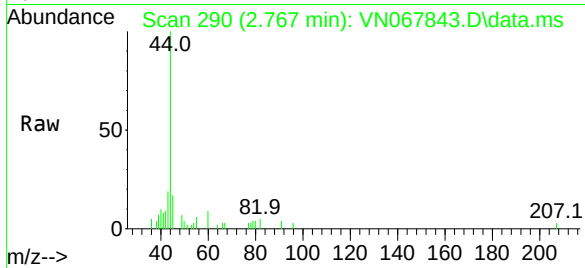

#11
Tert butyl alcohol
Concen: 0.354 ug/l
RT: 5.396 min Scan# 1270
Delta R.T. 0.006 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 59 Resp: 243
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#



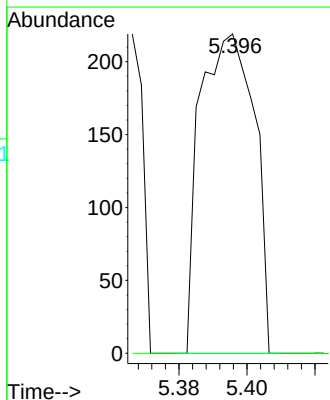
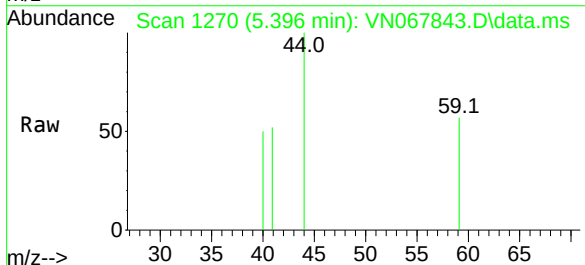




#13
Acrolein
Concen: Below Cal
RT: 4.041 min Scan# 765
Delta R.T. 0.002 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 24
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.0#

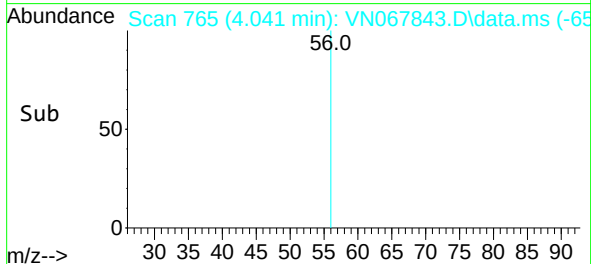

#16
Acetone
Concen: 26.685 ug/l
RT: 4.296 min Scan# 860
Delta R.T. 0.008 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 43 Resp: 40162
Ion Ratio Lower Upper
43 100
58 28.9 21.2 31.8







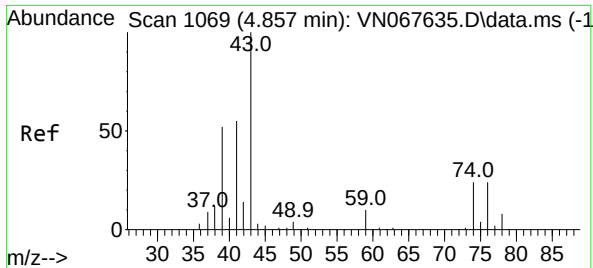

#18
Methyl Acetate
Concen: 1.821 ug/l
RT: 4.865 min Scan# 1072
Delta R.T. 0.008 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 7700
Ion Ratio Lower Upper
43 100
74 2.1 17.4 26.0#

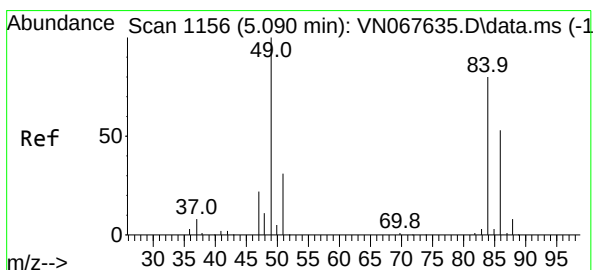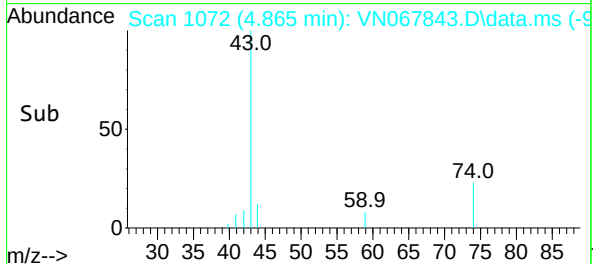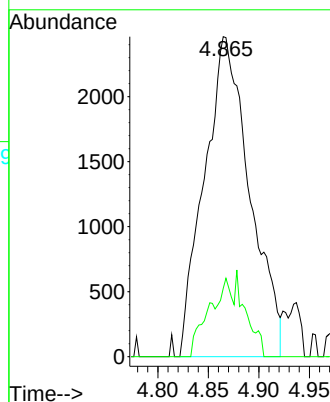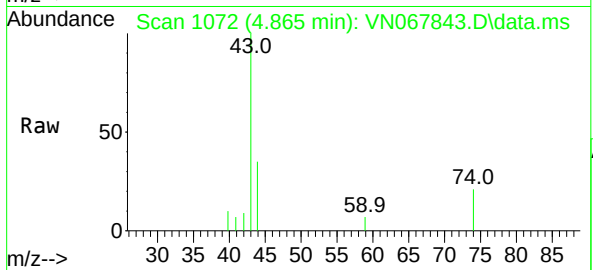

#20
Methylene Chloride
Concen: 8.664 ug/l
RT: 5.101 min Scan# 1160
Delta R.T. 0.011 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03


Tgt Ion: 84 Resp: 32462
Ion Ratio Lower Upper
84 100
49 117.5 110.9 166.3
51 41.8 32.6 49.0
86 69.1 51.6 77.4

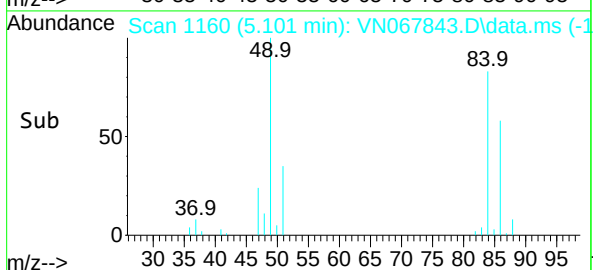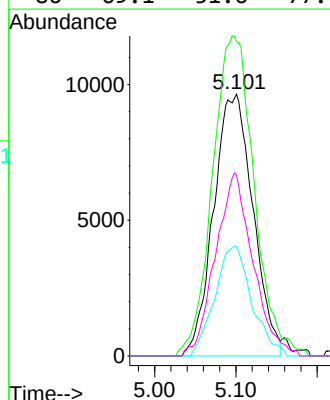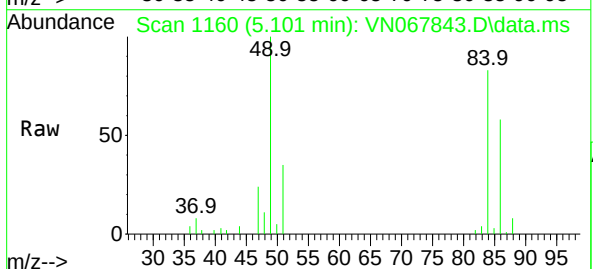



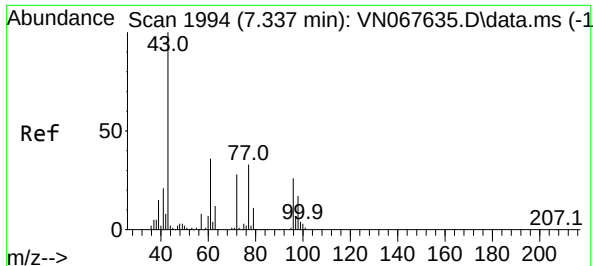


#25
2-Butanone
Concen: 3.411 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. 0.014 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Instrument :
MSVOA_N
ClientSampled :



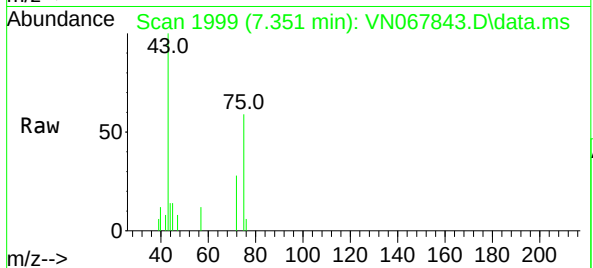



Tgt Ion: 43 Resp: 8524
Ion Ratio Lower Upper
43 100
72 27.5 19.7 29.5

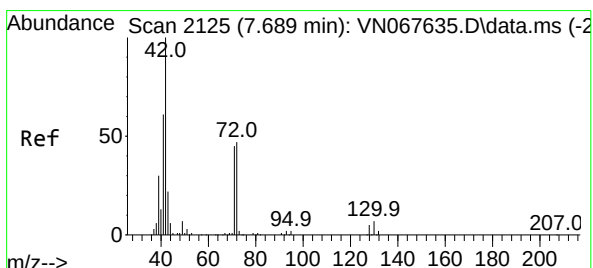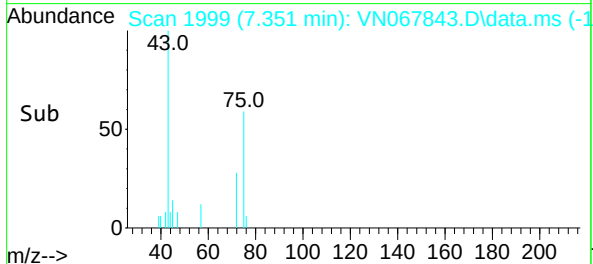

#29
Tetrahydrofuran
Concen: 2.709 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.013 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 42 Resp: 4452
Ion Ratio Lower Upper
42 100
72 16.0 32.8 49.2#
71 23.7 31.2 46.8#


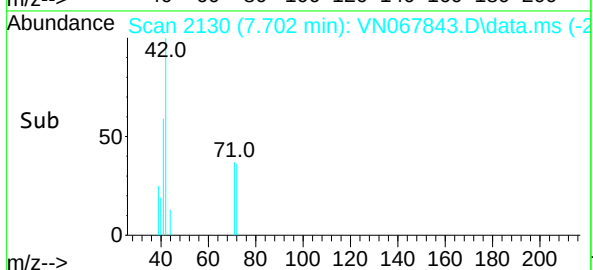

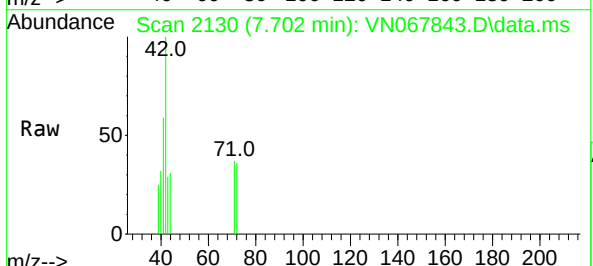




#31
Cyclohexane
Concen: 1.264 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.008 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 56 Resp: 8475
Ion Ratio Lower Upper
56 100
69 136.2 27.3 40.9#
84 101.2 64.9 97.3#

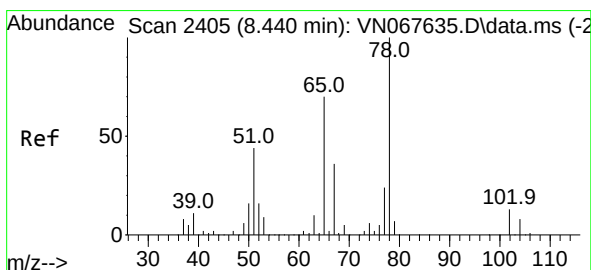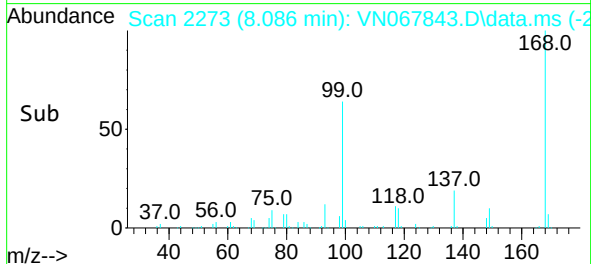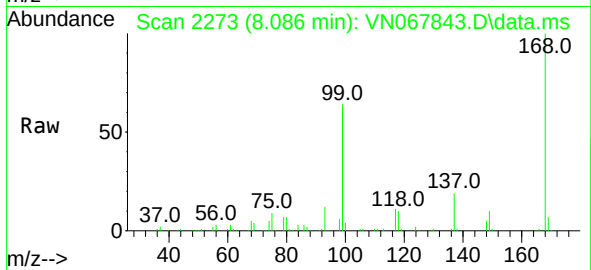

#33
1,2-Dichloroethane-d4
Concen: 51.977 ug/l
RT: 8.440 min Scan# 2405
Delta R.T. -0.000 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 65 Resp: 248607
Ion Ratio Lower Upper
65 100
67 51.3 0.0 98.6









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.971 min Scan# 2603
Delta R.T. 0.003 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:114 Resp: 601025
Ion Ratio Lower Upper
114 100
63 21.2 0.0 49.0
88 15.5 0.0 36.6

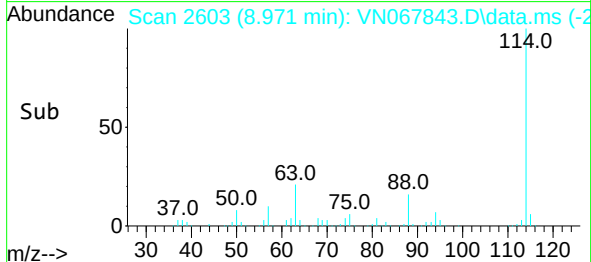

#35
Dibromofluoromethane
Concen: 50.146 ug/l
RT: 8.024 min Scan# 2250
Delta R.T. 0.003 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion:113 Resp: 182091
Ion Ratio Lower Upper
113 100
111 103.8 83.8 125.8
192 15.4 13.4 20.0




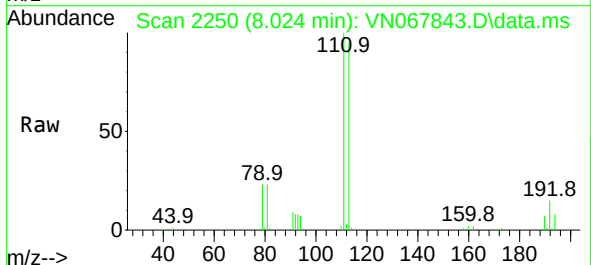




#36
1,1-Dichloropropene
Concen: 5.186 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.134 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion: 75 Resp: 28955
Ion Ratio Lower Upper
75 100
110 8.9 15.7 47.0#
77 0.0 24.6 37.0#

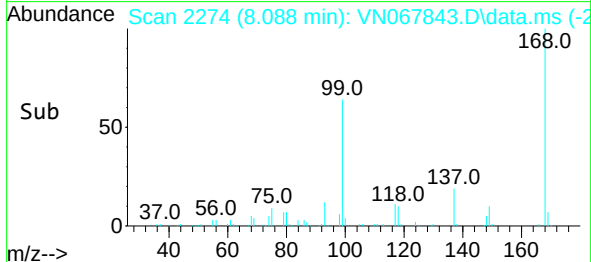

#37
Ethyl Acetate
Concen: 1.576 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.067 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03


Tgt Ion: 43 Resp: 8524
Ion Ratio Lower Upper
43 100
61 0.3 10.6 16.0#
70 0.0 8.1 12.1#

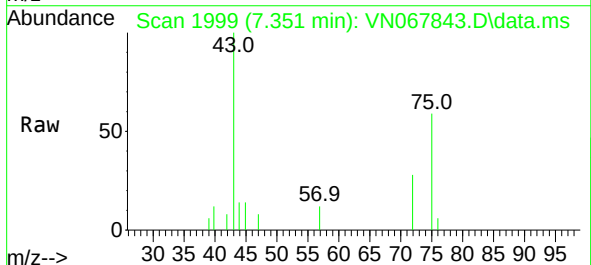



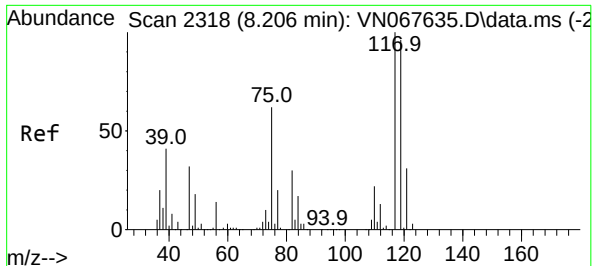


#38
Carbon Tetrachloride
Concen: 6.215 ug/l
RT: 8.088 min Scan# 2274
Delta R.T. -0.118 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Instrument :
MSVOA_N
ClientSampleId :



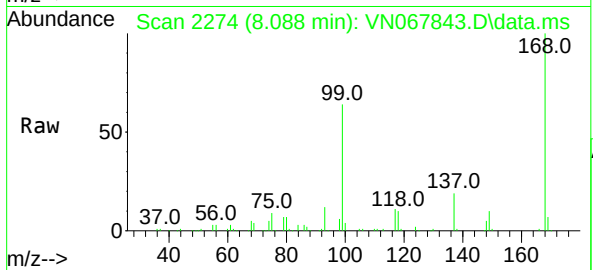



Tgt Ion:117 Resp: 34227
Ion Ratio Lower Upper
117 100
119 5.5 75.4 113.2#
121 0.0 23.5 35.3#

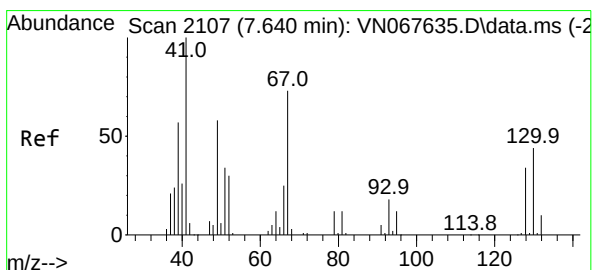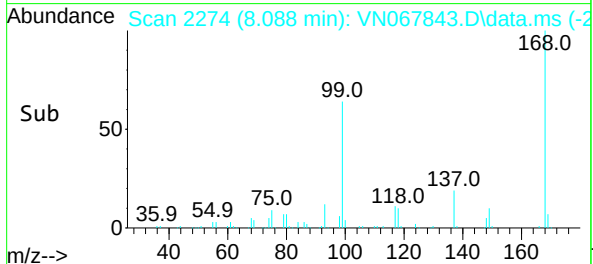

#41
Methacrylonitrile
Concen: 0.977 ug/l
RT: 7.700 min Scan# 2129
Delta R.T. 0.060 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03


Tgt Ion: 41 Resp: 2716
Ion Ratio Lower Upper
41 100
39 8.4 47.6 71.4#
67 0.0 57.7 86.5#
52 0.0 26.2 39.4#

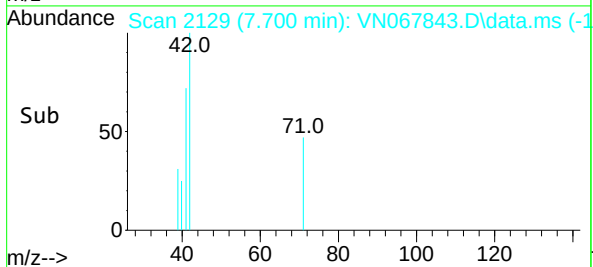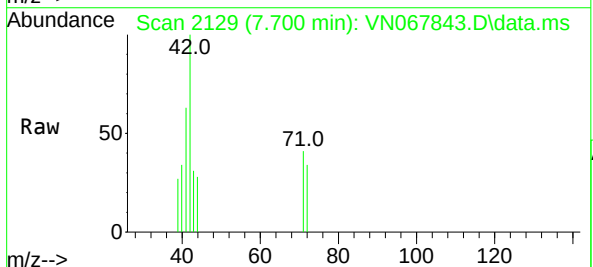






#43
Isopropyl Acetate
Concen: 3.649 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03


Instrument :
MSVOA_N
ClientSampled :





Tgt Ion: 43 Resp: 34720
Ion Ratio Lower Upper
43 100
61 17.9 19.0 28.4#
87 13.6 9.5 14.3




#45
1,2-Dichloropropane
Concen: 0.496 ug/l
RT: 9.623 min Scan# 2846
Delta R.T. 0.132 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03



Tgt Ion: 63 Resp: 2099
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#



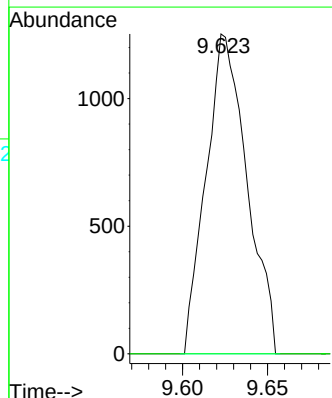





#48
Methyl methacrylate
Concen: 2.125 ug/l
RT: 9.545 min Scan# 2817
Delta R.T. -0.018 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41 Resp: 8943
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

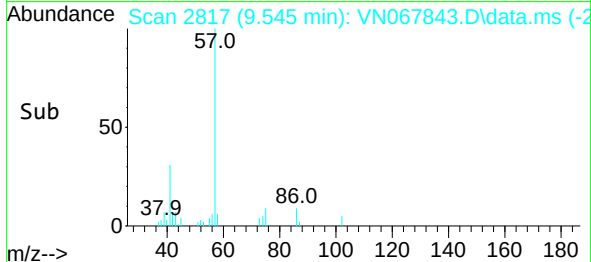

#49
1,4-Dioxane
Concen: 33.983 ug/l
RT: 9.636 min Scan# 2851
Delta R.T. 0.065 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 88 Resp: 160
Ion Ratio Lower Upper
88 100
43 1096436.3 28.8 43.2#
58 5015.0 60.4 90.6#



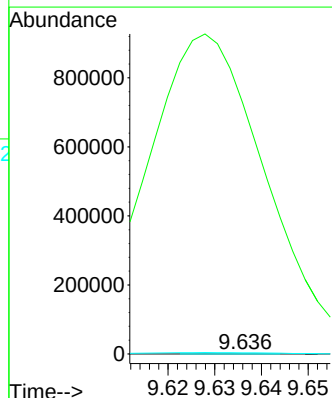
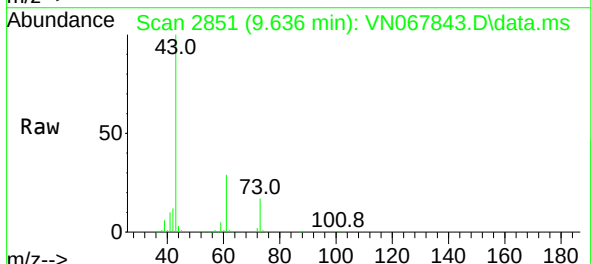




#50
Toluene-d8
Concen: 51.739 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 98 Resp: 786408
Ion Ratio Lower Upper
98 100
100 63.3 51.7 77.5

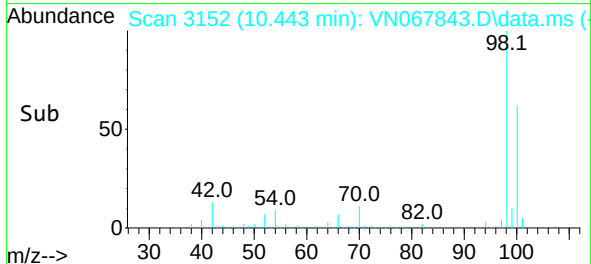

#51
4-Methyl-2-Pentanone
Concen: 1.447 ug/l
RT: 10.336 min Scan# 3112
Delta R.T. 0.003 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 43 Resp: 8459
Ion Ratio Lower Upper
43 100
58 48.5 28.6 43.0#


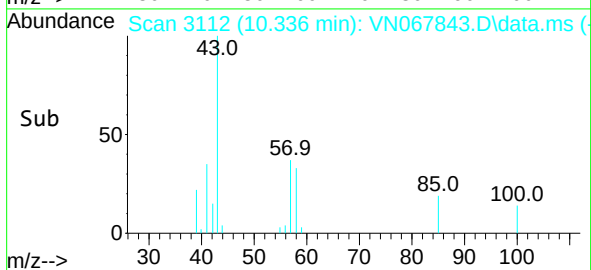




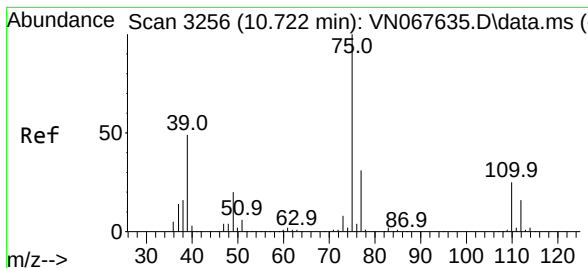

#53
t-1,3-Dichloropropene
Concen: 1.762 ug/l
RT: 10.446 min Scan# 3153
Delta R.T. -0.276 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 125
Ion Ratio Lower Upper
75 100
77 26.0 25.1 37.7

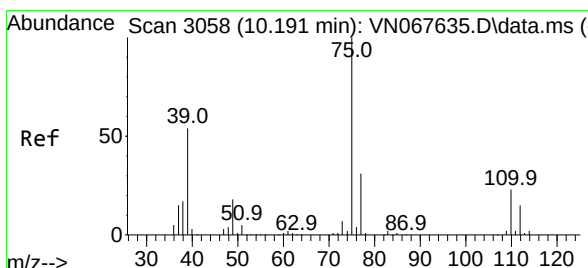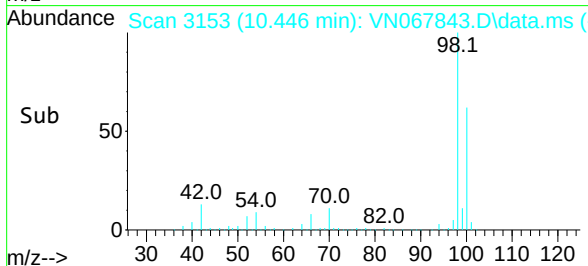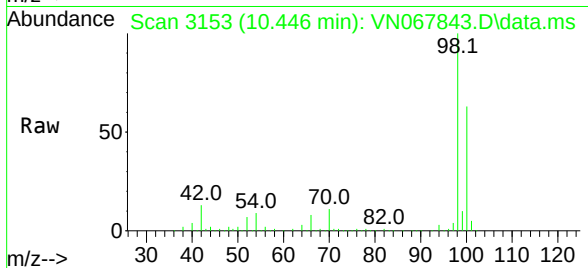

#54
cis-1,3-Dichloropropene
Concen: 9.288 ug/l
RT: 10.247 min Scan# 3079
Delta R.T. 0.056 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 75 Resp: 60621
Ion Ratio Lower Upper
75 100
77 0.0 24.6 37.0#
39 39.1 50.7 76.1#


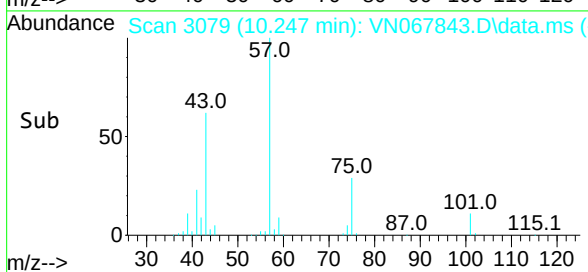

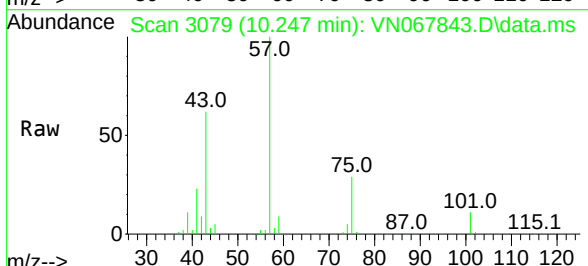




#57
1,3-Dichloropropane
Concen: 4.664 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.048 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 76 Resp: 33549
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#

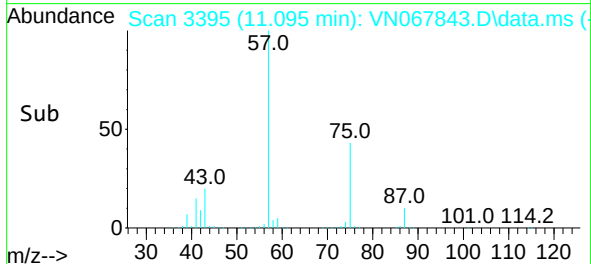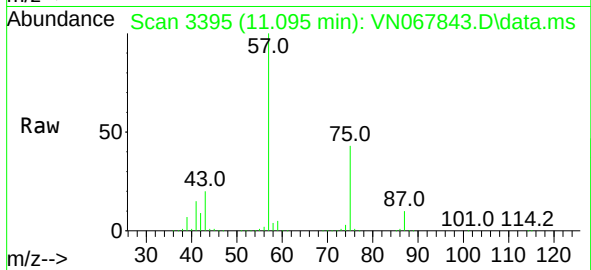

#59
2-Hexanone
Concen: 123.381 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 43 Resp: 503450
Ion Ratio Lower Upper
43 100
58 18.2 24.7 74.1#


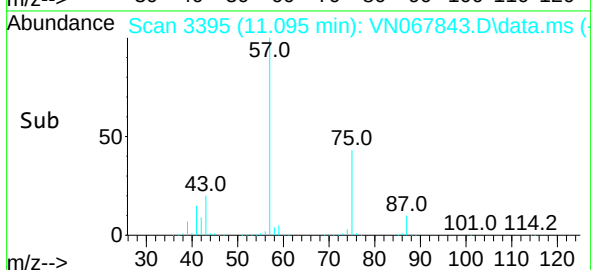






#60
Dibromochloromethane
Concen: 2.395 ug/l
RT: 11.497 min Scan# 3545
Delta R.T. 0.255 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion:129 Resp: 204
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#

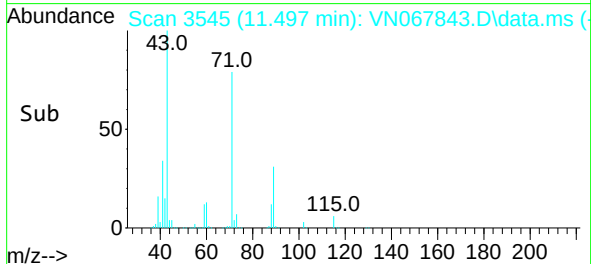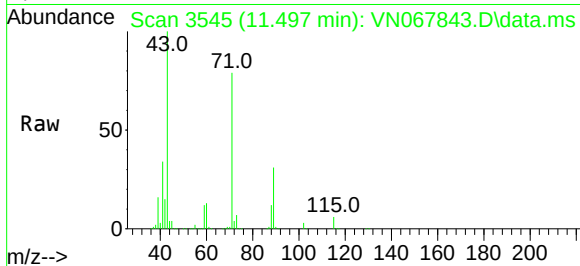

#62
4-Bromofluorobenzene
Concen: 50.392 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion: 95 Resp: 270570
Ion Ratio Lower Upper
95 100
174 70.7 0.0 122.0
176 67.7 0.0 117.6




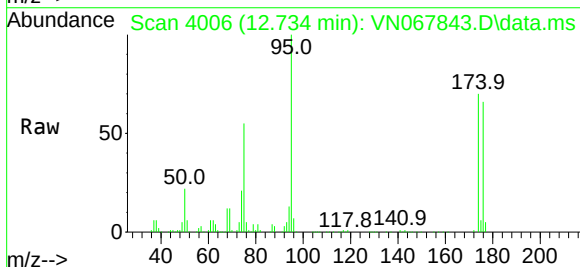


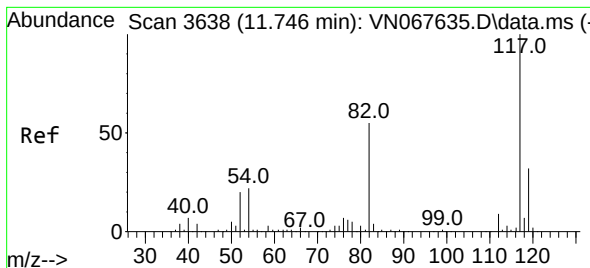

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:117 Resp: 620235
Ion Ratio Lower Upper
117 100
82 55.2 53.1 79.7
119 31.2 25.5 38.3

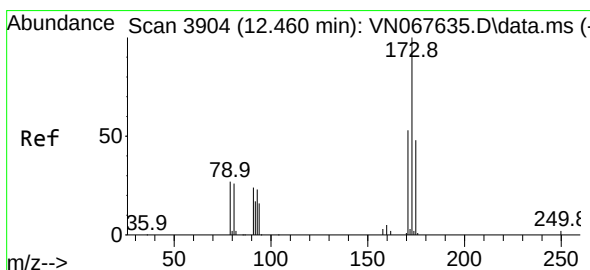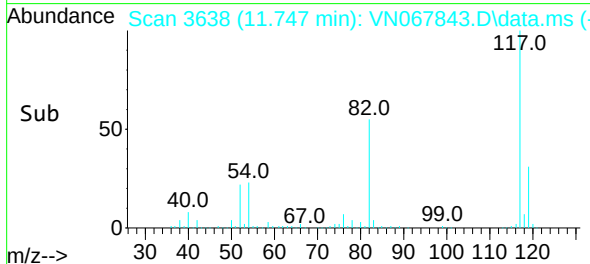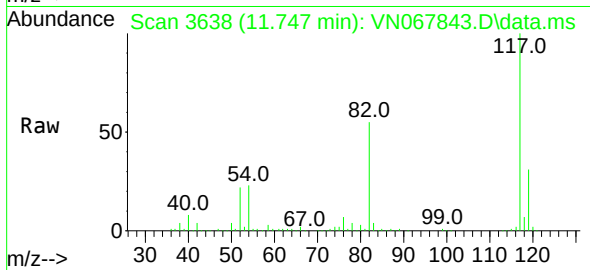

#71
Bromoform
Concen: 3.267 ug/l
RT: 12.723 min Scan# 4002
Delta R.T. 0.263 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

Tgt Ion:173 Resp: 389
Ion Ratio Lower Upper
173 100
175 3707.2 23.9 71.8#
254 0.0 0.0 0.0


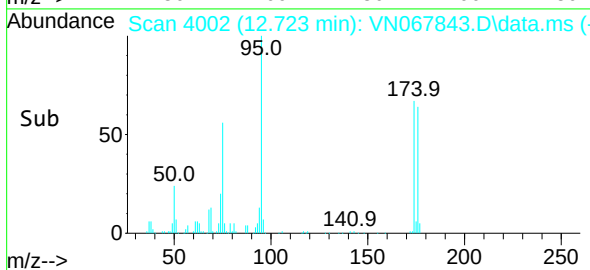

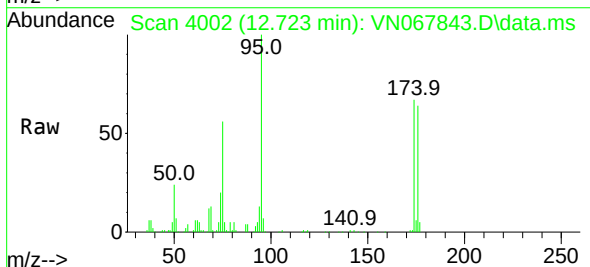




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.678 min Scan# 4358
 Delta R.T. 0.000 min
 Lab File: VN067843.D
 Acq: 21 Jul 2021 17:03




Instrument :
 MSVOA_N
 ClientSampleId :


Tgt Ion:152 Resp: 232244
 Ion Ratio Lower Upper
 152 100
 115 63.6 36.1 108.5
 150 157.5 0.0 351.8

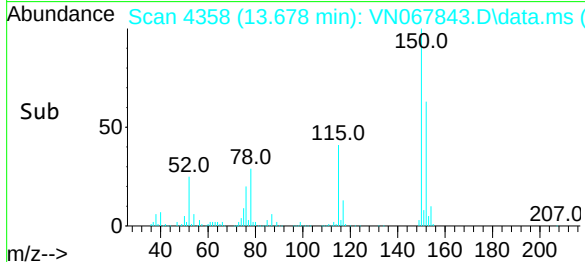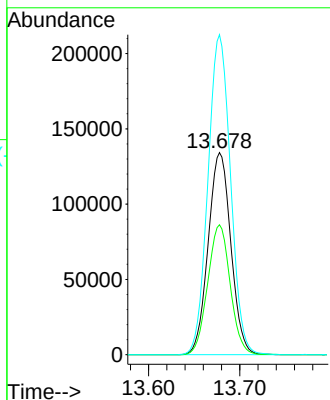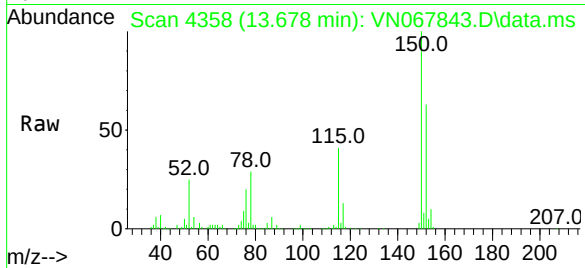

#76
 1,2,3-Trichloropropane
 Concen: 31.413 ug/l
 RT: 12.734 min Scan# 4006
 Delta R.T. -0.150 min
 Lab File: VN067843.D
 Acq: 21 Jul 2021 17:03

Tgt Ion: 75 Resp: 148985
 Ion Ratio Lower Upper
 75 100
 77 1.1 0.0 0.0#


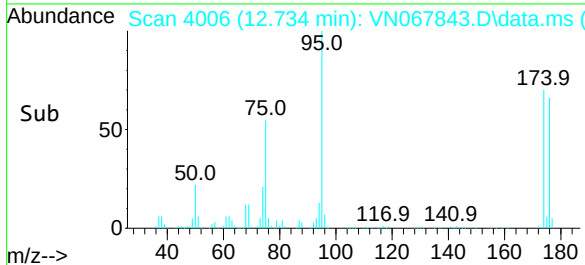
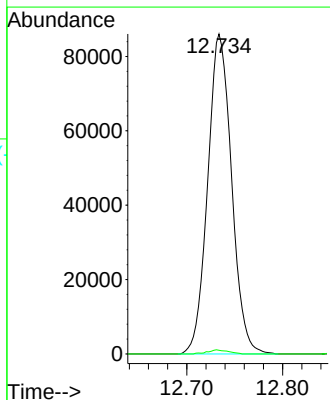
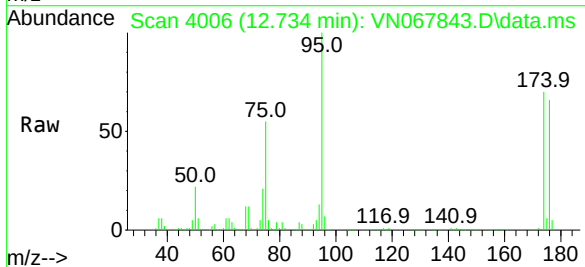




#81
trans-1,4-Dichloro-2-butene
Concen: 101.277 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 148985
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

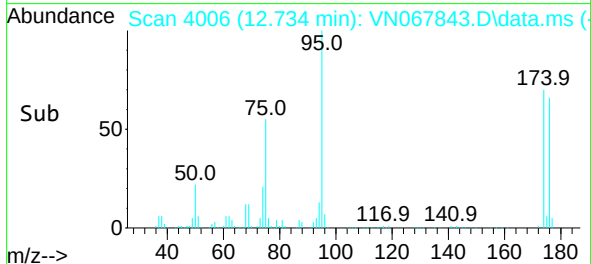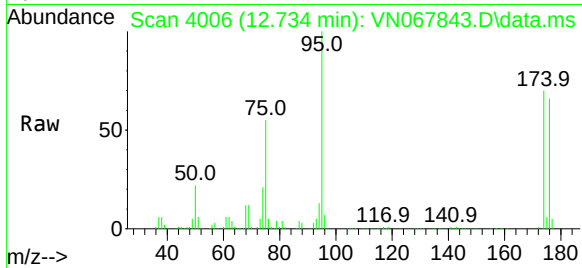

#93
1,2,4-Trichlorobenzene
Concen: 2.688 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.002 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03


Tgt Ion:180 Resp: 57
Ion Ratio Lower Upper
180 100
182 91.2 47.5 142.5
145 0.0 17.2 51.6#

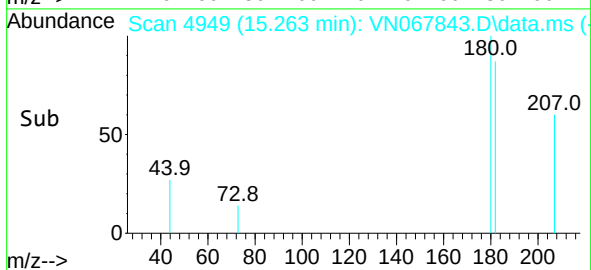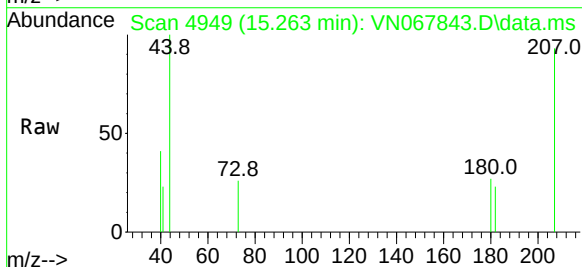






#95
Naphthalene
Concen: 3.134 ug/l
RT: 15.512 min Scan# 5042
Delta R.T. 0.003 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03


Instrument :
MSVOA_N
ClientSampled :

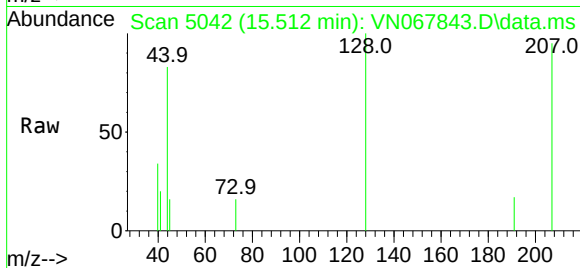

Tgt Ion:128 Resp: 1476
Ion Ratio Lower Upper
128 100
127 4.1 10.6 15.8#
129 0.0 8.6 12.8#

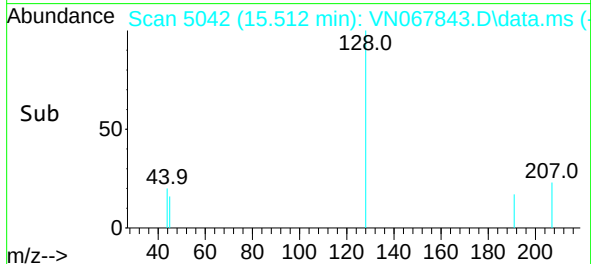

#96
1,2,3-Trichlorobenzene
Concen: 2.691 ug/l
RT: 15.705 min Scan# 5114
Delta R.T. 0.003 min
Lab File: VN067843.D
Acq: 21 Jul 2021 17:03

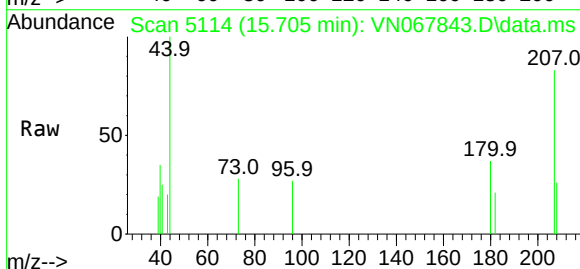

Tgt Ion:180 Resp: 228
Ion Ratio Lower Upper
180 100
182 87.3 47.8 143.3
145 0.0 18.2 54.6#

