

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
 Data File : VN067844.D
 Acq On : 21 Jul 2021 17:28
 Operator : JC/MD
 Sample : M3089-16
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Jul 22 02:13:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 07 16:18:53 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.088	168	318203	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.971	114	614712	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.747	117	636299	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.678	152	231843	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.440	65	258161	53.683	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	= 107.360%	
35) Dibromofluoromethane	8.024	113	184359	49.640	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	= 99.280%	
50) Toluene-d8	10.443	98	798633	51.374	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	= 102.740%	
62) 4-Bromofluorobenzene	12.734	95	276064	50.270	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	= 100.540%	


Target Compounds				Qvalue		
5) Bromomethane	2.872	94	719	Below Cal	#	71
6) Chloroethane	3.046	64	24	Below Cal	#	44
7) Trichlorofluoromethane	3.245	101	25	Below Cal	#	18
11) Tert butyl alcohol	5.385	59	238	0.344	ug/l #	71
13) Acrolein	4.044	56	321	Below Cal		88
16) Acetone	4.299	43	41229	27.246	ug/l	93
18) Methyl Acetate	4.867	43	7769	1.828	ug/l #	74
20) Methylene Chloride	5.087	84	14243	3.383	ug/l	92
25) 2-Butanone	7.351	43	8780	3.494	ug/l	93
29) Tetrahydrofuran	7.700	42	4272	2.585	ug/l #	81
31) Cyclohexane	8.088	56	8623	1.279	ug/l #	14
36) 1,1-Dichloropropene	8.086	75	28821	5.047	ug/l #	52
37) Ethyl Acetate	7.351	43	8780	1.587	ug/l #	75
38) Carbon Tetrachloride	8.086	117	36120	6.413	ug/l #	17
41) Methacrylonitrile	7.702	41	2906	1.022	ug/l #	46
43) Isopropyl Acetate	8.566	43	39854	4.095	ug/l #	90
45) 1,2-Dichloropropane	9.623	63	2618	0.605	ug/l #	44
48) Methyl methacrylate	9.547	41	9804	2.278	ug/l #	12
49) 1,4-Dioxane	9.625	88	232	34.755	ug/l #	1
51) 4-Methyl-2-Pentanone	10.333	43	11087	1.854	ug/l	97
53) t-1,3-Dichloropropene	10.438	75	173	1.768	ug/l #	1
54) cis-1,3-Dichloropropene	10.247	75	65309	9.783	ug/l #	62
57) 1,3-Dichloropropane	11.095	76	38446	5.225	ug/l #	43
59) 2-Hexanone	11.095	43	570341	136.662	ug/l #	54
60) Dibromochloromethane	11.489	129	265	2.405	ug/l #	11
71) Bromoform	12.726	173	813	3.362	ug/l #	1
74) N-amyl acetate	12.197	43	19990	2.946	ug/l #	50
76) 1,2,3-Trichloropropane	12.734	75	156957	33.151	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.734	75	156957	106.881	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.263	180	204	2.724	ug/l #	12
95) Naphthalene	15.515	128	959	3.092	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.695	180	77	2.652	ug/l #	12


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
Data File : VN067844.D
Acq On : 21 Jul 2021 17:28
Operator : JC/MD
Sample : M3089-16
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Jul 22 02:13:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
Quant Title : SW846 8260
QLast Update : Wed Jul 07 16:18:53 2021
Response via : Initial Calibration

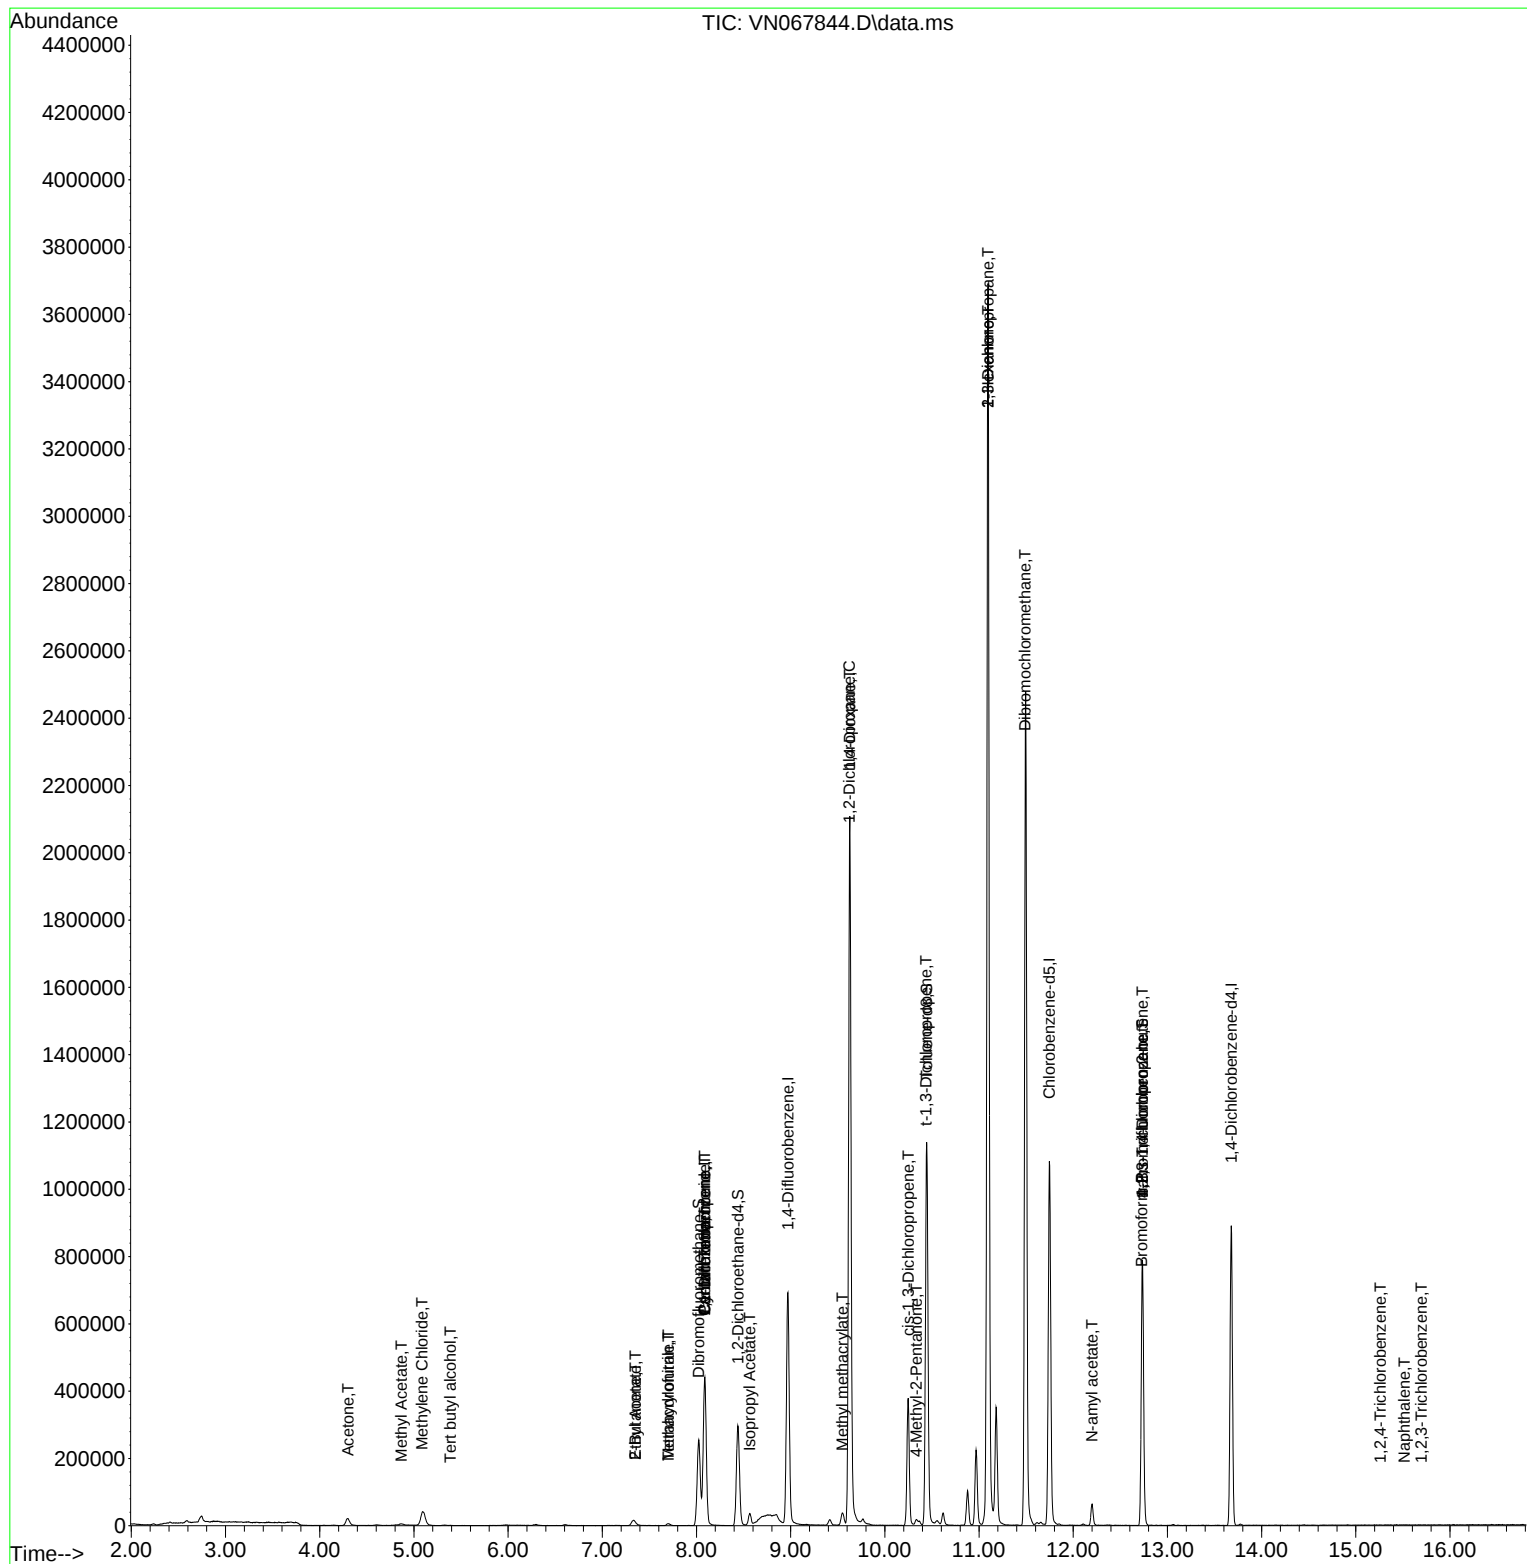



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.088 min Scan# 2274

Delta R.T. 0.002 min

Lab File: VN067844.D





Acq: 21 Jul 2021 17:28

Tgt Ion:168 Resp: 318203

Ion Ratio Lower Upper

168 100

99 65.1 62.9 94.3

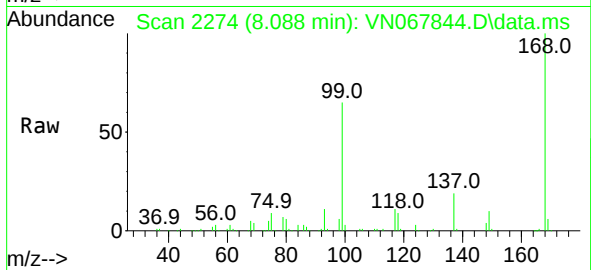

#5

Bromomethane

Concen: Below Cal

RT: 2.872 min Scan# 329

Delta R.T. 0.040 min

Lab File: VN067844.D




Acq: 21 Jul 2021 17:28


Tgt Ion: 94 Resp: 719

Ion Ratio Lower Upper

94 100

96 64.3 73.7 110.5#


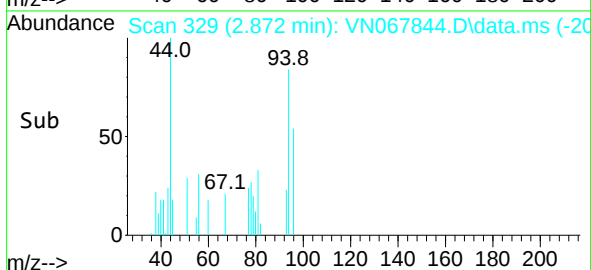

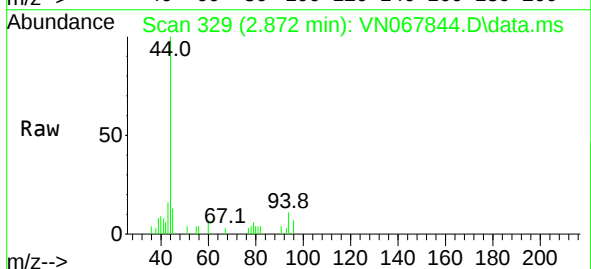




#6
Chloroethane
Concen: Below Cal
RT: 3.046 min Scan# 394
Delta R.T. 0.040 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 64 Resp: 24
Ion Ratio Lower Upper
64 100
66 0.0 24.7 37.1#



#7
Trichlorofluoromethane
Concen: Below Cal
RT: 3.245 min Scan# 468
Delta R.T. -0.120 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion:101 Resp: 25
Ion Ratio Lower Upper
101 100
103 0.0 51.2 76.8#

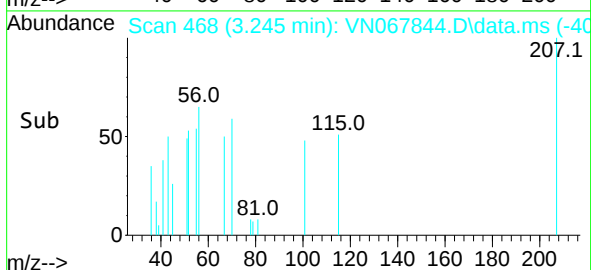




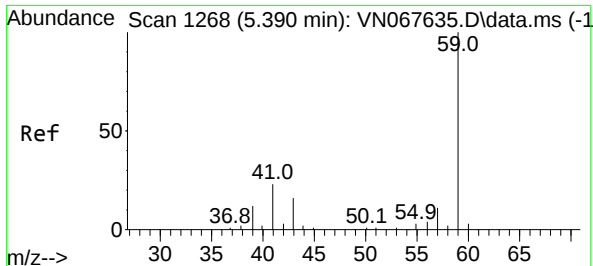


#11

Tert butyl alcohol
Concen: 0.344 ug/l
RT: 5.385 min Scan# 1266
Delta R.T. -0.005 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampled :




Tgt Ion: 59 Resp: 238
Ion Ratio Lower Upper
59 100
57 0.0 8.7 13.1#

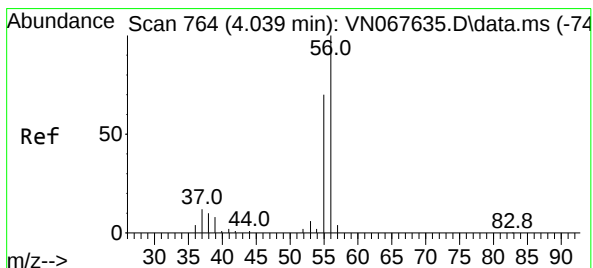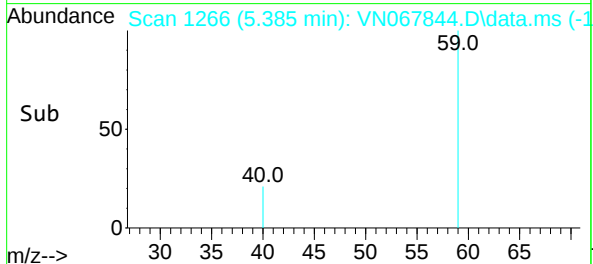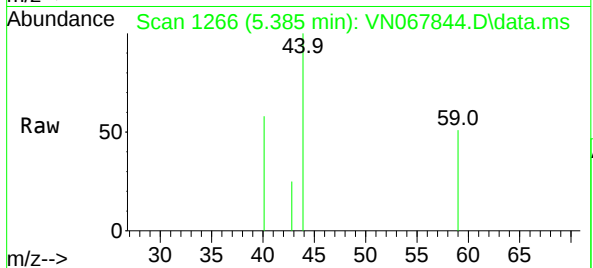


#13

Acrolein
Concen: Below Cal
RT: 4.044 min Scan# 766
Delta R.T. 0.005 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28


Tgt Ion: 56 Resp: 321
Ion Ratio Lower Upper
56 100
55 62.0 57.4 86.0

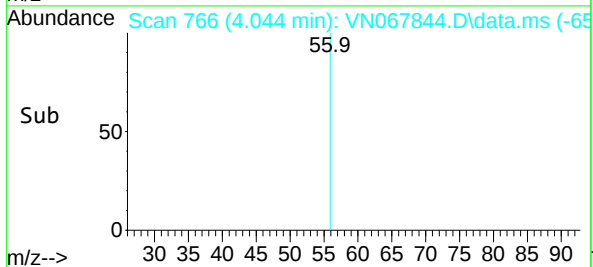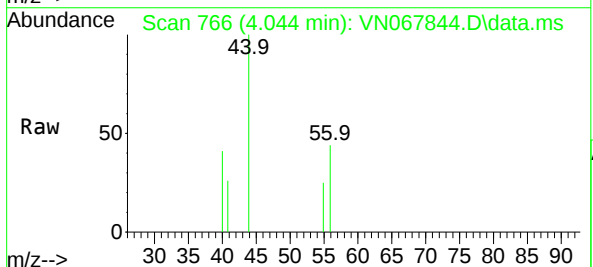






#16
Acetone
Concen: 27.246 ug/l
RT: 4.299 min Scan# 861
Delta R.T. 0.011 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 43 Resp: 41229
Ion Ratio Lower Upper
43 100
58 30.3 21.2 31.8



#18
Methyl Acetate
Concen: 1.828 ug/l
RT: 4.867 min Scan# 1073
Delta R.T. 0.010 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion: 43 Resp: 7769
Ion Ratio Lower Upper
43 100
74 9.2 17.4 26.0#

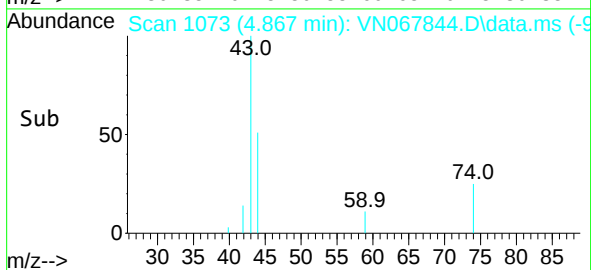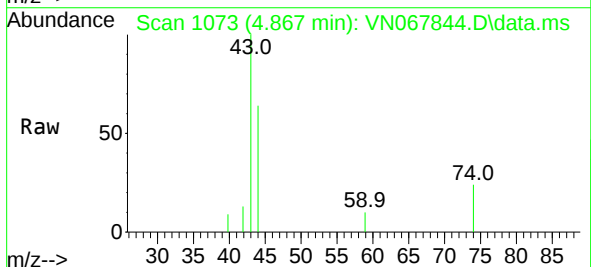

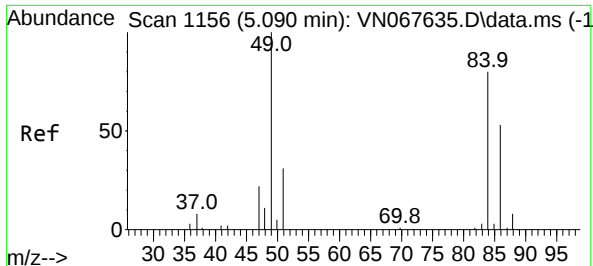

#20

Methylene Chloride

Concen: 3.383 ug/l

RT: 5.087 min Scan# 1155

Delta R.T. -0.003 min

Lab File: VN067844.D

Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampleId :

Tgt Ion: 84 Resp: 14243





Ion Ratio Lower Upper

84 100

49 126.6 110.9 166.3

51 42.4 32.6 49.0

86 60.1 51.6 77.4

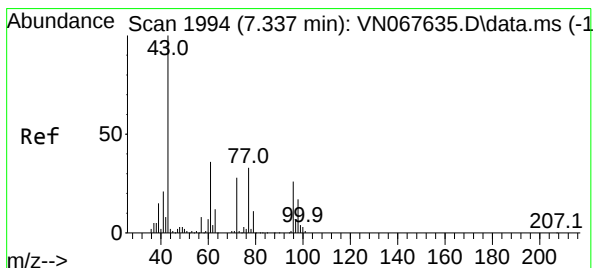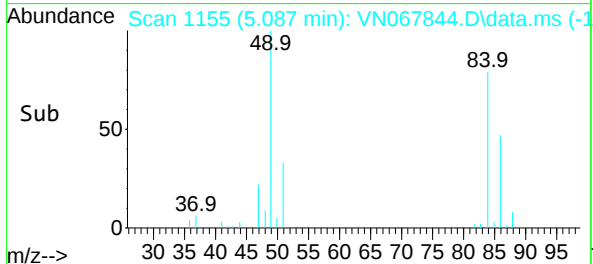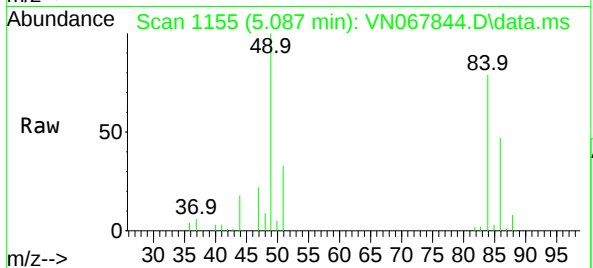

#25

2-Butanone

Concen: 3.494 ug/l

RT: 7.351 min Scan# 1999

Delta R.T. 0.014 min

Lab File: VN067844.D




Acq: 21 Jul 2021 17:28


Tgt Ion: 43 Resp: 8780

Ion Ratio Lower Upper

43 100

72 28.1 19.7 29.5

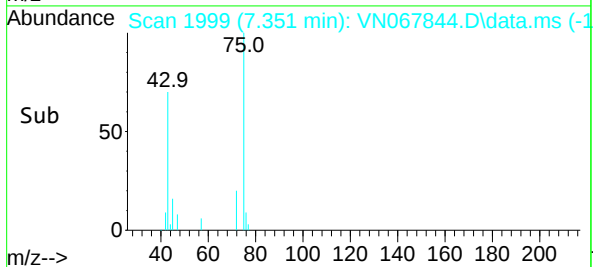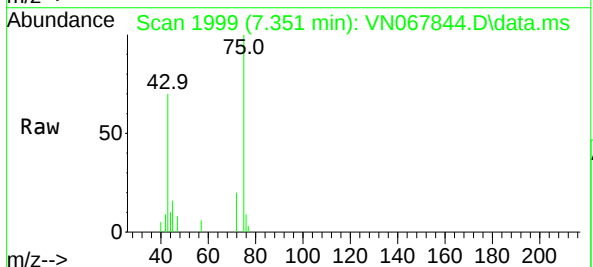



#29

Tetrahydrofuran

Concen: 2.585 ug/l


RT: 7.700 min Scan# 2129

Delta R.T. 0.011 min




Lab File: VN067844.D

Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampled :

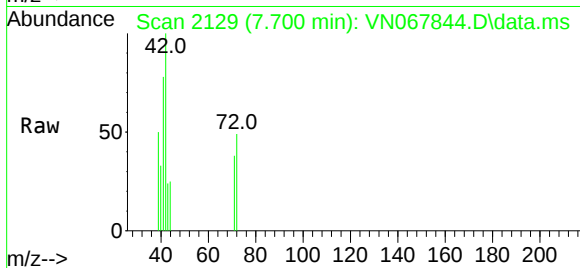

Tgt Ion:	42	Resp:	4272
Ion	Ratio	Lower	Upper
42	100		
72	44.6	32.8	49.2
71	18.8	31.2	46.8#

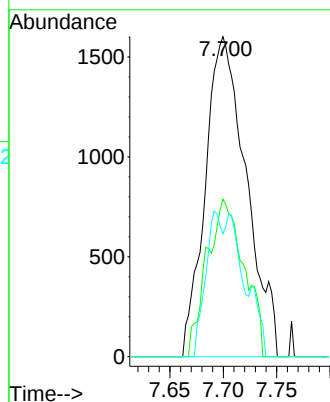

#31

Cyclohexane

Concen: 1.279 ug/l




RT: 8.088 min Scan# 2274


Delta R.T. -0.006 min

Lab File: VN067844.D

Acq: 21 Jul 2021 17:28

Tgt Ion:	56	Resp:	8623
Ion	Ratio	Lower	Upper
56	100		
69	152.2	27.3	40.9#
84	112.1	64.9	97.3#

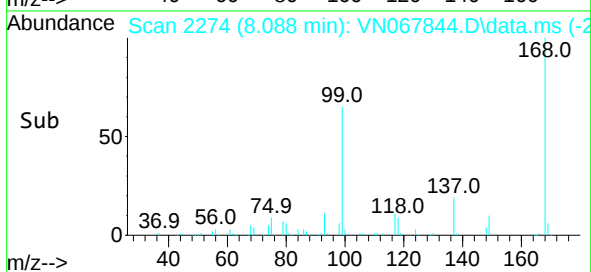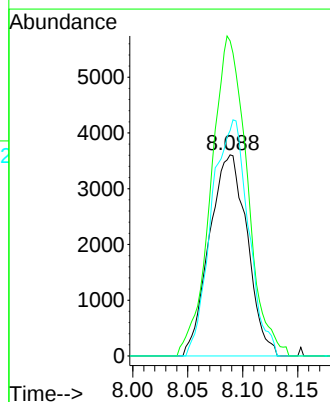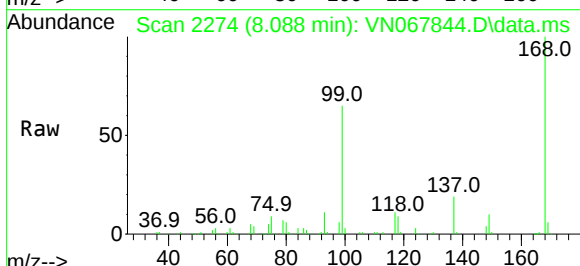



#33

1,2-Dichloroethane-d4

Concen: 53.683 ug/l

RT: 8.440 min Scan# 2405

Delta R.T. -0.000 min

Lab File: VN067844.D





Acq: 21 Jul 2021 17:28

Tgt Ion: 65 Resp: 258161

Ion Ratio Lower Upper

65 100

67 50.7 0.0 98.6



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.971 min Scan# 2603

Delta R.T. 0.003 min

Lab File: VN067844.D

Acq: 21 Jul 2021 17:28




Tgt Ion: 114 Resp: 614712


Ion Ratio Lower Upper

114 100

63 20.7 0.0 49.0

88 15.0 0.0 36.6

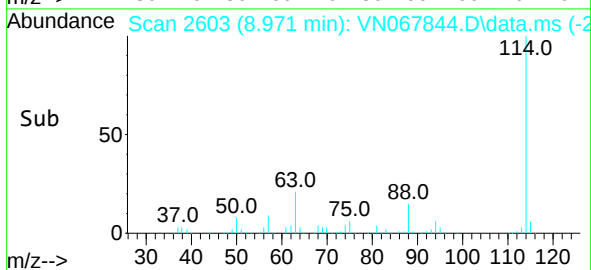



#35

Dibromofluoromethane

Concen: 49.640 ug/l

RT: 8.024 min Scan# 2250

Delta R.T. 0.003 min

Lab File: VN067844.D

Acq: 21 Jul 2021 17:28





Tgt Ion:113 Resp: 184359

Ion Ratio Lower Upper

113 100

111 103.2 83.8 125.8

192 16.5 13.4 20.0



#36

1,1-Dichloropropene

Concen: 5.047 ug/l

RT: 8.086 min Scan# 2273

Delta R.T. -0.136 min

Lab File: VN067844.D

Acq: 21 Jul 2021 17:28




Tgt Ion: 75 Resp: 28821


Ion Ratio Lower Upper

75 100

110 9.5 15.7 47.0#


77 0.0 24.6 37.0#

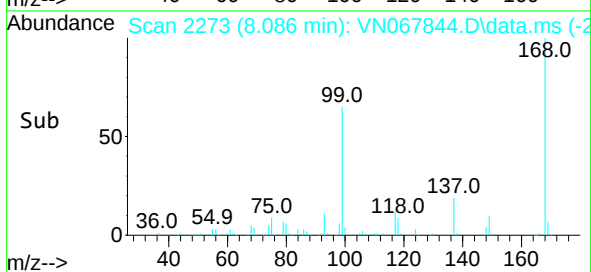






#37
Ethyl Acetate
Concen: 1.587 ug/l
RT: 7.351 min Scan# 1999
Delta R.T. -0.067 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28


Instrument :
MSVOA_N
ClientSampleId :





Tgt Ion: 43 Resp: 8780
Ion Ratio Lower Upper
43 100
61 3.6 10.6 16.0#
70 0.0 8.1 12.1#




#38
Carbon Tetrachloride
Concen: 6.413 ug/l
RT: 8.086 min Scan# 2273
Delta R.T. -0.120 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

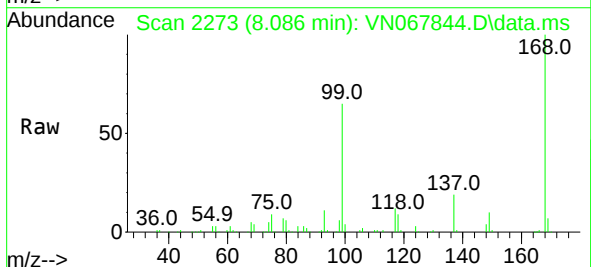

Tgt Ion: 117 Resp: 36120
Ion Ratio Lower Upper
117 100
119 5.9 75.4 113.2#
121 0.0 23.5 35.3#







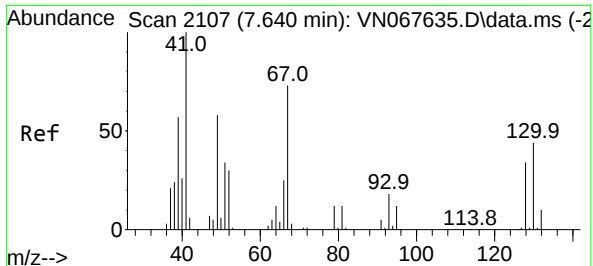

#41
Methacrylonitrile
Concen: 1.022 ug/l
RT: 7.702 min Scan# 2130
Delta R.T. 0.062 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 41	Resp: 2906
Ion Ratio	Lower Upper
41 100	
39 68.0	47.6 71.4
67 0.0	57.7 86.5#
52 0.0	26.2 39.4#

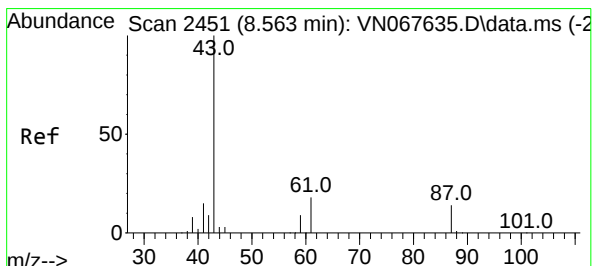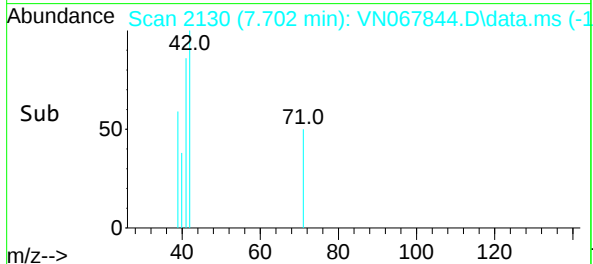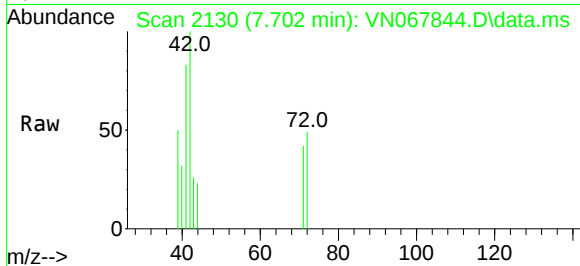

#43
Isopropyl Acetate
Concen: 4.095 ug/l
RT: 8.566 min Scan# 2452
Delta R.T. 0.003 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion: 43	Resp: 39854
Ion Ratio	Lower Upper
43 100	
61 17.3	19.0 28.4#
87 13.6	9.5 14.3


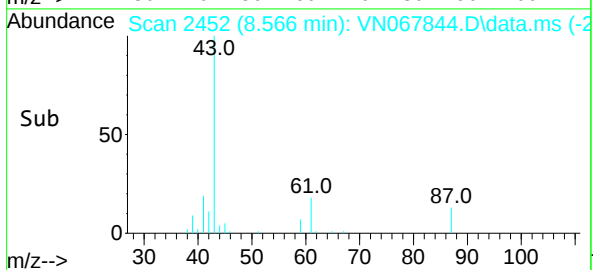

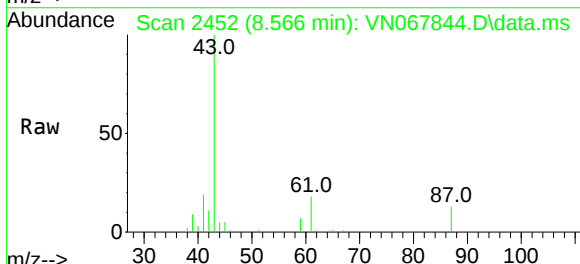


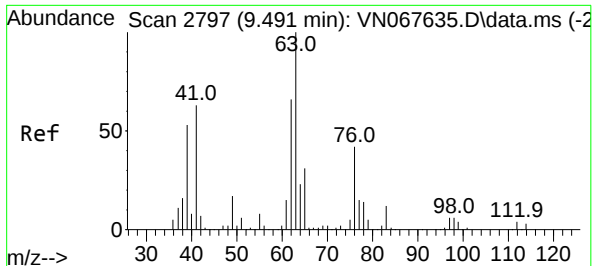

#45
1,2-Dichloropropane
Concen: 0.605 ug/l
RT: 9.623 min Scan# 2846
Delta R.T. 0.132 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 63 Resp: 2618
Ion Ratio Lower Upper
63 100
65 0.0 24.3 36.5#

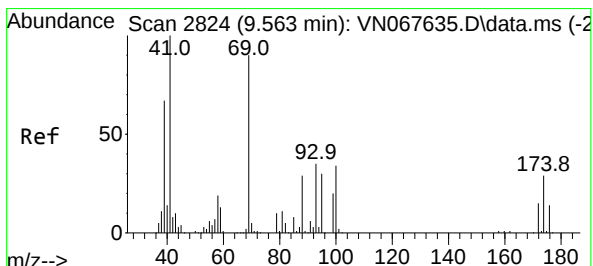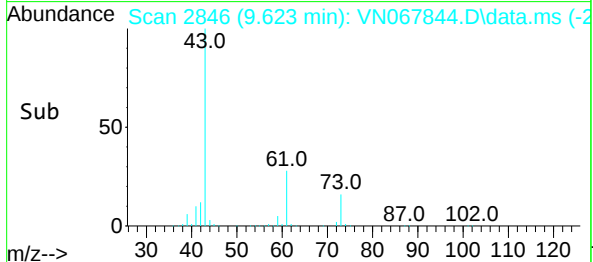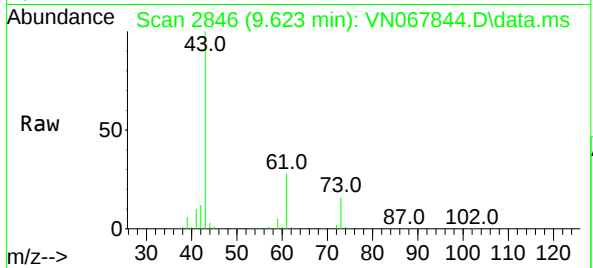

#48
Methyl methacrylate
Concen: 2.278 ug/l
RT: 9.547 min Scan# 2818
Delta R.T. -0.016 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28


Tgt Ion: 41 Resp: 9804
Ion Ratio Lower Upper
41 100
69 0.0 64.6 96.8#
39 0.0 53.3 79.9#

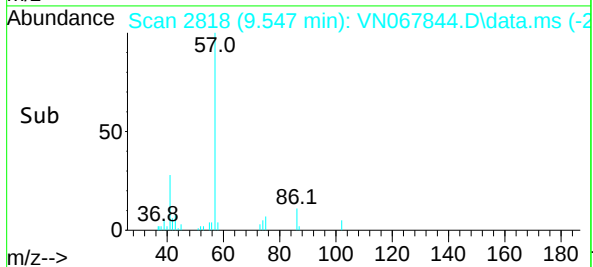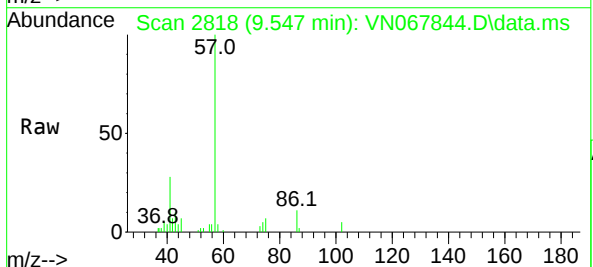






#49
1,4-Dioxane
Concen: 34.755 ug/l
RT: 9.625 min Scan# 2847
Delta R.T. 0.054 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampled :







Tgt Ion: 88 Resp: 232
Ion Ratio Lower Upper
88 100
43 888605.6 28.8 43.2#
58 3984.5 60.4 90.6#



#50
Toluene-d8
Concen: 51.374 ug/l
RT: 10.443 min Scan# 3152
Delta R.T. 0.000 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion: 98 Resp: 798633
Ion Ratio Lower Upper
98 100
100 63.6 51.7 77.5


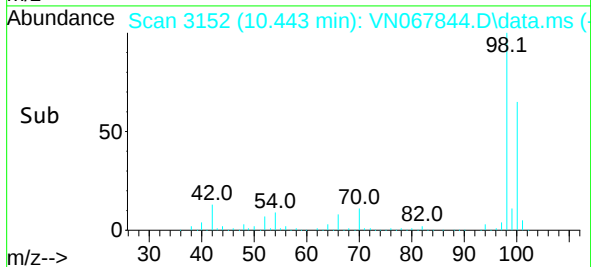

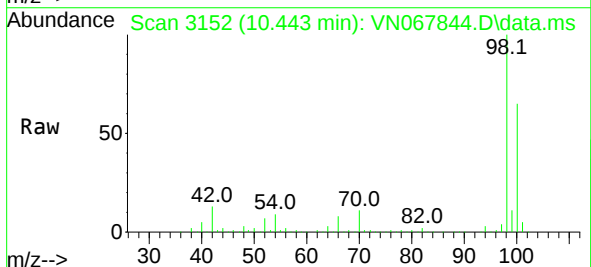




#51
4-Methyl-2-Pentanone
Concen: 1.854 ug/l
RT: 10.333 min Scan# 3111
Delta R.T. 0.000 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 11087
Ion Ratio Lower Upper
43 100
58 37.5 28.6 43.0

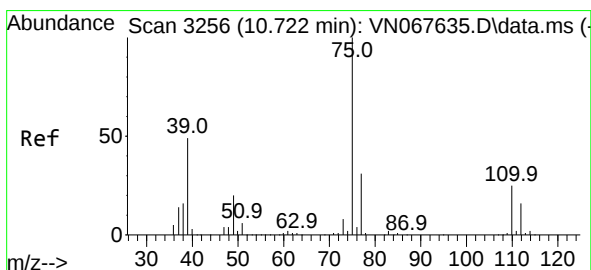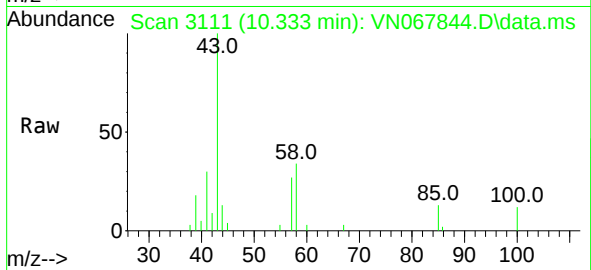

#53
t-1,3-Dichloropropene
Concen: 1.768 ug/l
RT: 10.438 min Scan# 3150
Delta R.T. -0.284 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion: 75 Resp: 173
Ion Ratio Lower Upper
75 100
77 130.2 25.1 37.7#


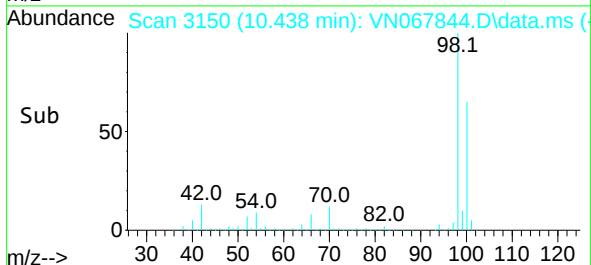

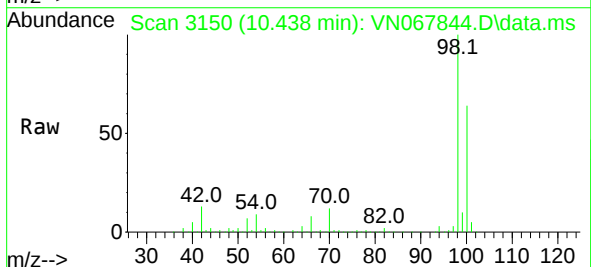




#54
 cis-1,3-Dichloropropene
 Concen: 9.783 ug/l
 RT: 10.247 min Scan# 3079
 Delta R.T. 0.056 min
 Lab File: VN067844.D
 Acq: 21 Jul 2021 17:28




Instrument :
 MSVOA_N
 ClientSampled :


Tgt Ion: 75 Resp: 65309
 Ion Ratio Lower Upper
 75 100
 77 0.6 24.6 37.0#
 39 40.3 50.7 76.1#



#57
 1,3-Dichloropropane
 Concen: 5.225 ug/l
 RT: 11.095 min Scan# 3395
 Delta R.T. 0.048 min
 Lab File: VN067844.D
 Acq: 21 Jul 2021 17:28

Tgt Ion: 76 Resp: 38446
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.7 38.5#









#59
2-Hexanone
Concen: 136.662 ug/l
RT: 11.095 min Scan# 3395
Delta R.T. 0.008 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 43 Resp: 570341
Ion Ratio Lower Upper
43 100
58 17.8 24.7 74.1#



#60
Dibromochloromethane
Concen: 2.405 ug/l
RT: 11.489 min Scan# 3542
Delta R.T. 0.247 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion:129 Resp: 265
Ion Ratio Lower Upper
129 100
127 0.0 38.6 115.8#


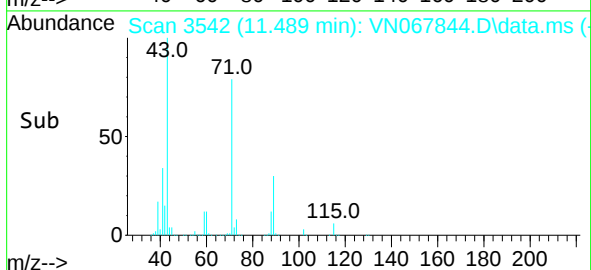




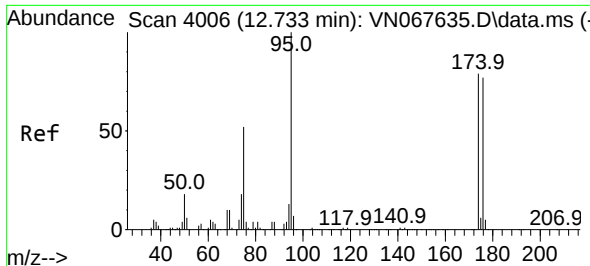

#62
4-Bromofluorobenzene
Concen: 50.270 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.001 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 95 Resp: 276064
Ion Ratio Lower Upper
95 100
174 71.5 0.0 122.0
176 69.6 0.0 117.6

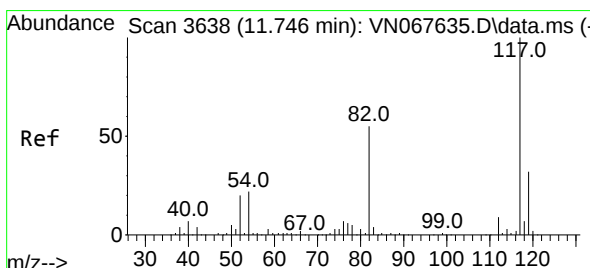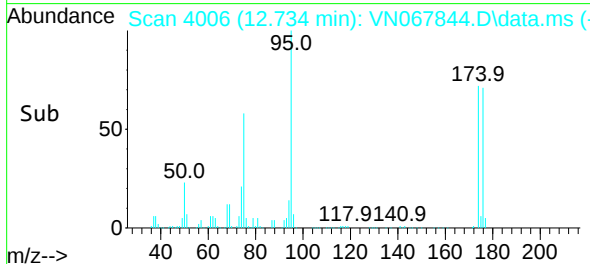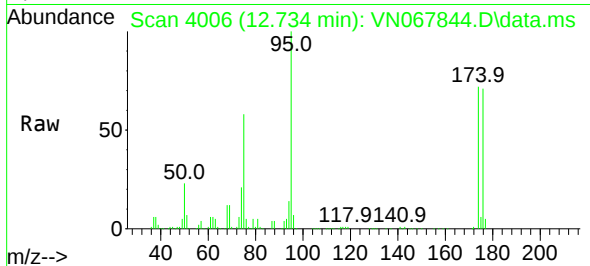

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.747 min Scan# 3638
Delta R.T. 0.000 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion: 117 Resp: 636299
Ion Ratio Lower Upper
117 100
82 57.2 53.1 79.7
119 32.5 25.5 38.3


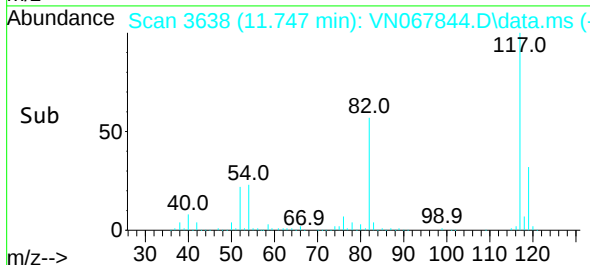

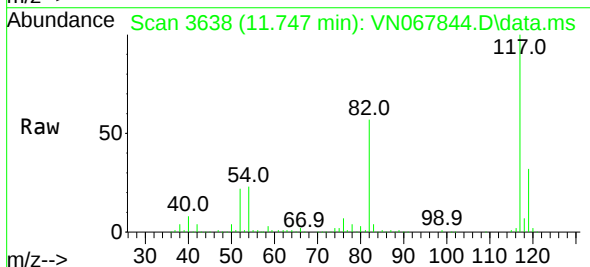


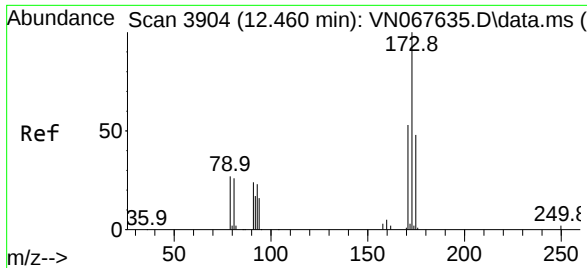

#71
Bromoform
Concen: 3.362 ug/l
RT: 12.726 min Scan# 4003
Delta R.T. 0.266 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampleId :


Tgt Ion:173 Resp: 813
Ion Ratio Lower Upper
173 100
175 1728.4 23.9 71.8#
254 0.0 0.0 0.0

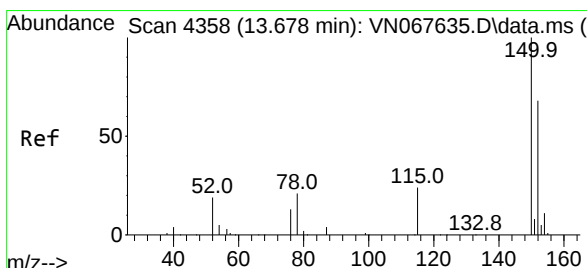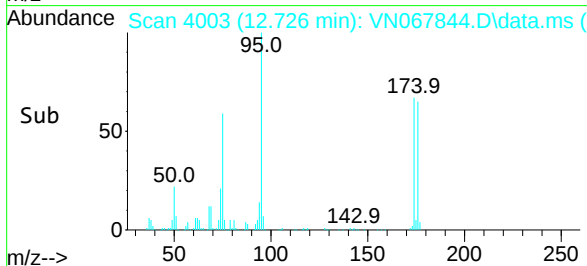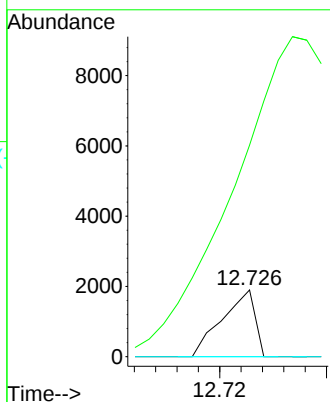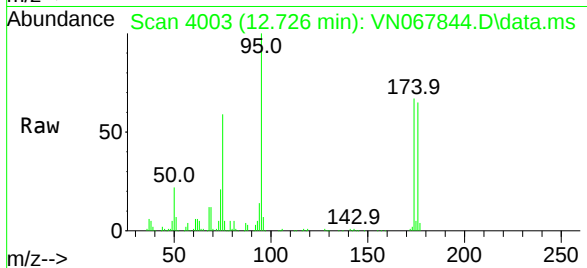

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.678 min Scan# 4358
Delta R.T. 0.000 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28


Tgt Ion:152 Resp: 231843
Ion Ratio Lower Upper
152 100
115 63.4 36.1 108.5
150 157.1 0.0 351.8

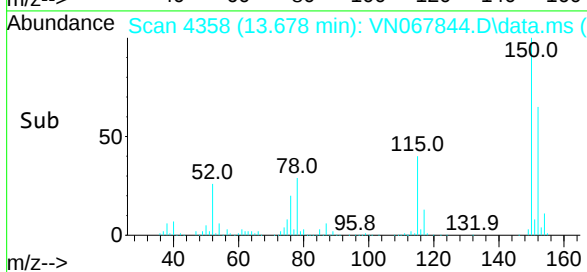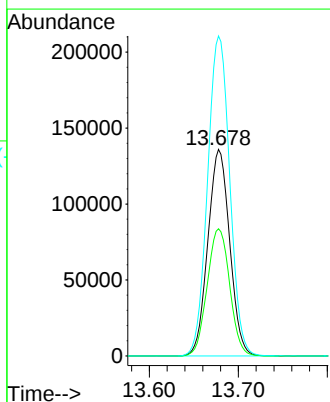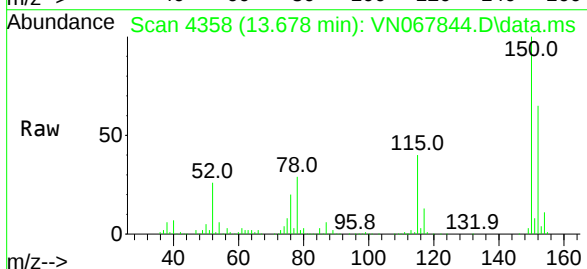






#74
N-amy1 acetate
Concen: 2.946 ug/l
RT: 12.197 min Scan# 3806
Delta R.T. -0.193 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampleId :



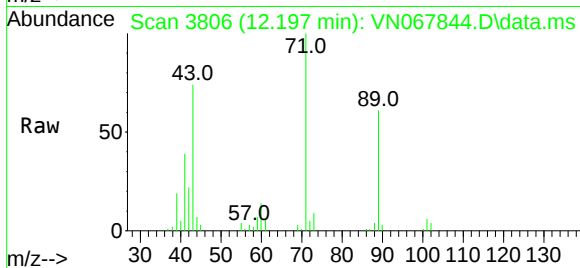



Tgt Ion	Ratio	Lower	Upper
43	100		
70	0.4	29.4	44.2#
55	5.0	17.0	25.4#
61	0.0	17.6	26.4#



#76
1,2,3-Trichloropropane
Concen: 33.151 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. -0.150 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion	Ratio	Lower	Upper
75	100		
77	1.0	0.0	0.0#


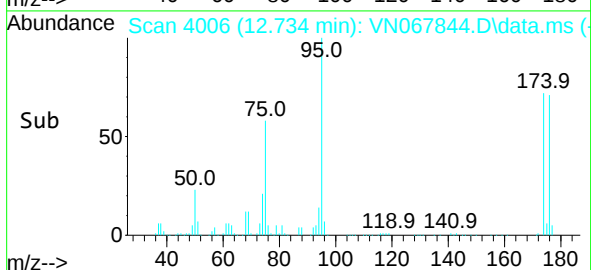

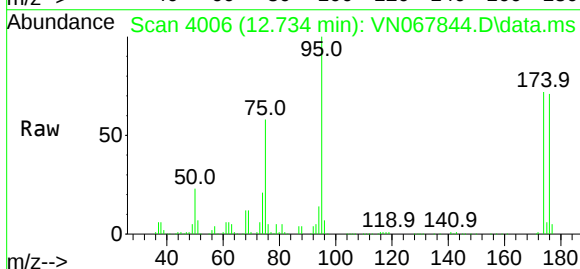




#81
trans-1,4-Dichloro-2-butene
Concen: 106.881 ug/l
RT: 12.734 min Scan# 4006
Delta R.T. 0.105 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28




Instrument :
MSVOA_N
ClientSampled :


Tgt Ion: 75 Resp: 156957
Ion Ratio Lower Upper
75 100
53 0.0 87.6 131.4#
89 0.0 37.8 56.8#

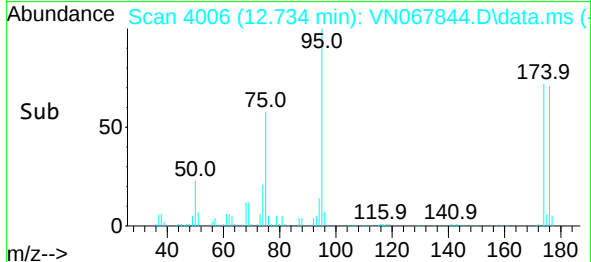

#93
1,2,4-Trichlorobenzene
Concen: 2.724 ug/l
RT: 15.263 min Scan# 4949
Delta R.T. -0.002 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28


Tgt Ion:180 Resp: 204
Ion Ratio Lower Upper
180 100
182 0.0 47.5 142.5#
145 0.0 17.2 51.6#

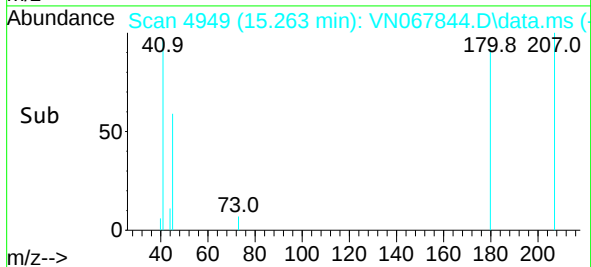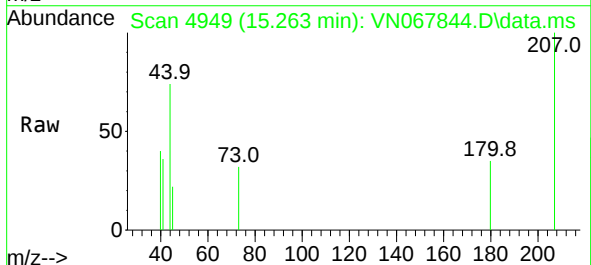






#95
Naphthalene
Concen: 3.092 ug/l
RT: 15.515 min Scan# 5043
Delta R.T. 0.006 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Instrument :
MSVOA_N
ClientSampled :



Tgt Ion:128 Resp: 959
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.6 12.8#



#96
1,2,3-Trichlorobenzene
Concen: 2.652 ug/l
RT: 15.695 min Scan# 5110
Delta R.T. -0.007 min
Lab File: VN067844.D
Acq: 21 Jul 2021 17:28

Tgt Ion:180 Resp: 77
Ion Ratio Lower Upper
180 100
182 0.0 47.8 143.3#
145 0.0 18.2 54.6#

