


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072121\
 Data File : VN067828.D
 Acq On : 21 Jul 2021 9:55
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N070721W.M
 Title : SW846 8260
 Last Update : Wed Jul 07 16:18:53 2021

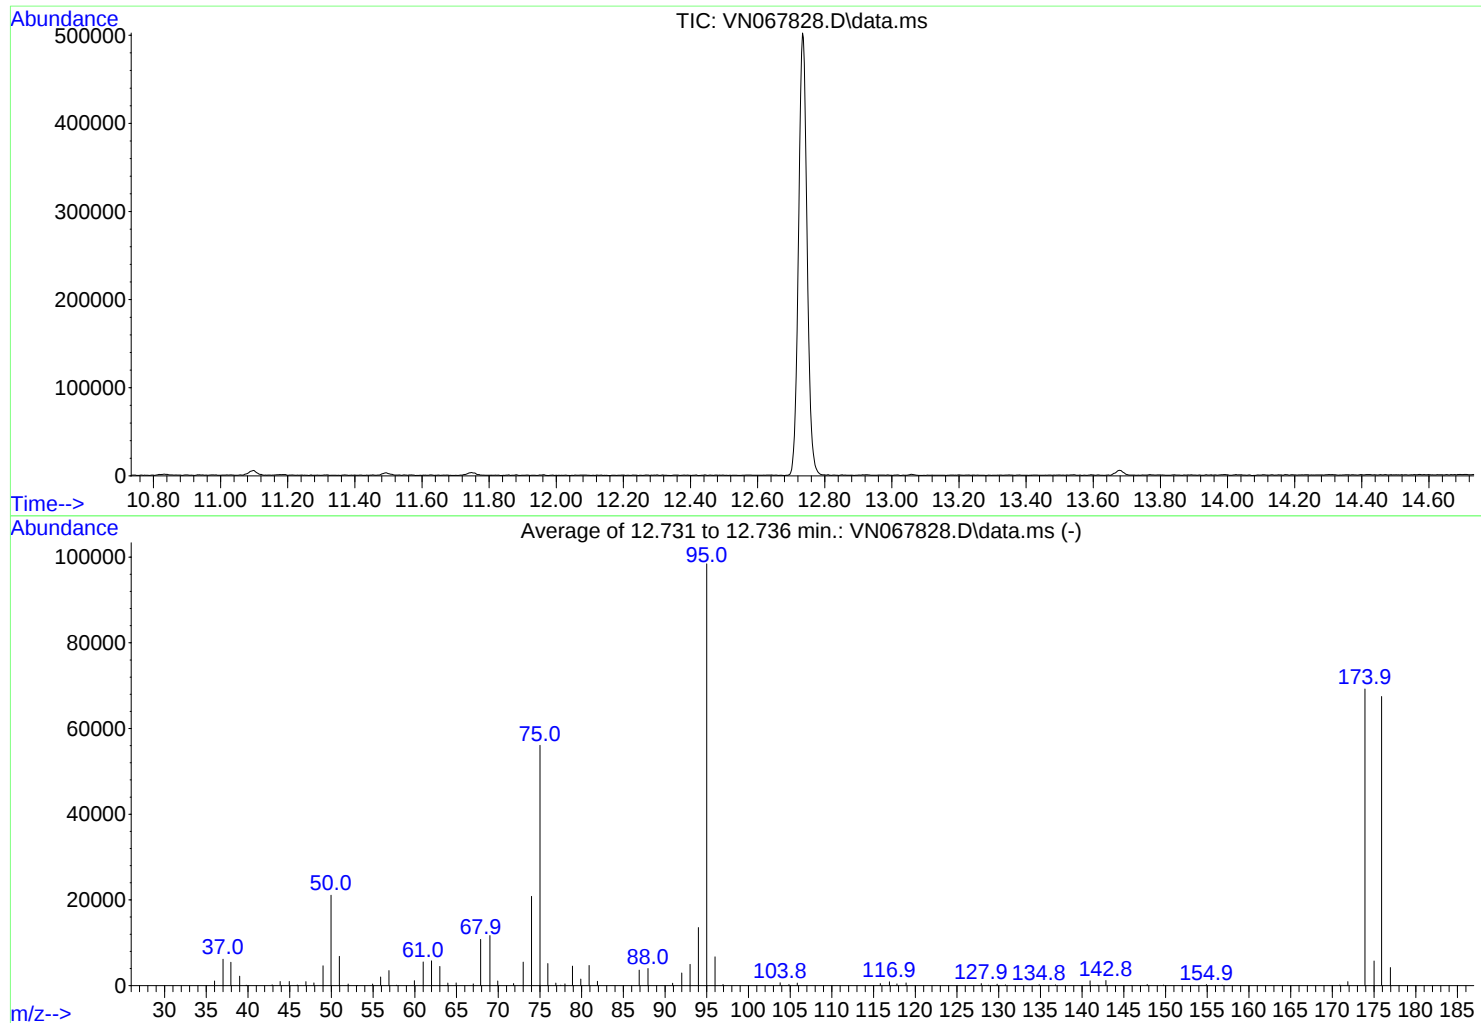

AutoFind: Scans 4005, 4006, 4007; Background Corrected with Scan 3988

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	21083	PASS
75	95	30	60	57.0	56075	PASS
95	95	100	100	100.0	98429	PASS
96	95	5	9	6.8	6720	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.3	69237	PASS
175	174	5	9	8.3	5766	PASS
176	174	95	101	97.5	67485	PASS
177	176	5	9	6.3	4219	PASS