
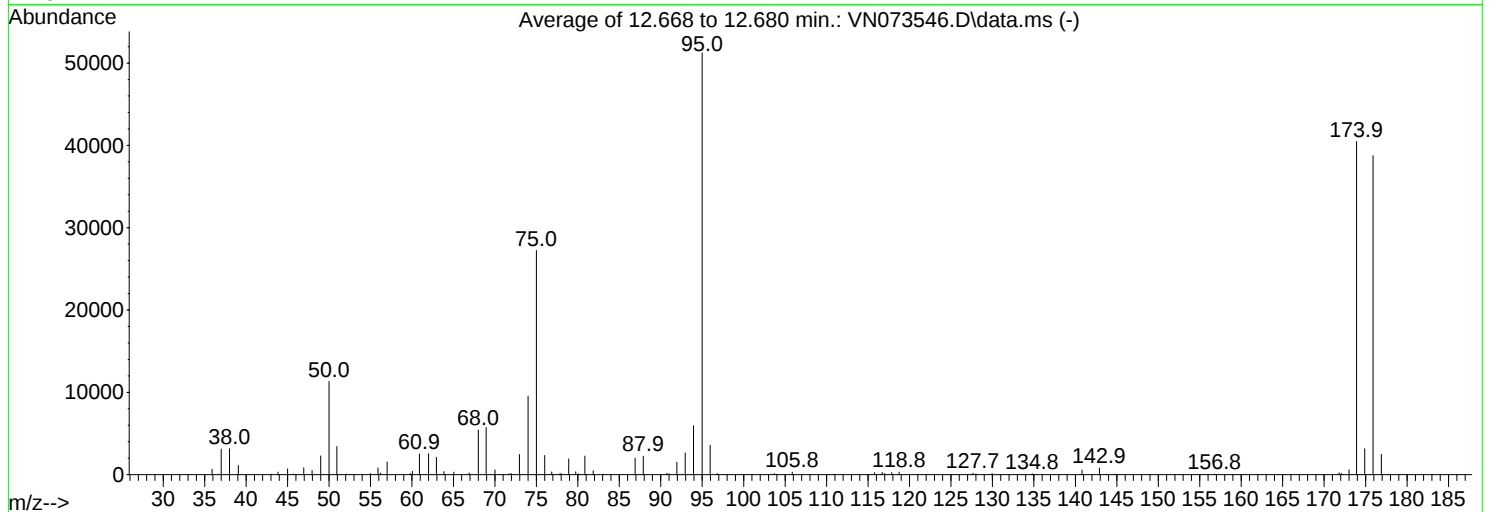


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072122\
Data File : VN073546.D
Acq On : 21 Jul 2022 09:16
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N062822W.M
Title : SW846 8260
Last Update : Wed Jun 29 01:54:03 2022

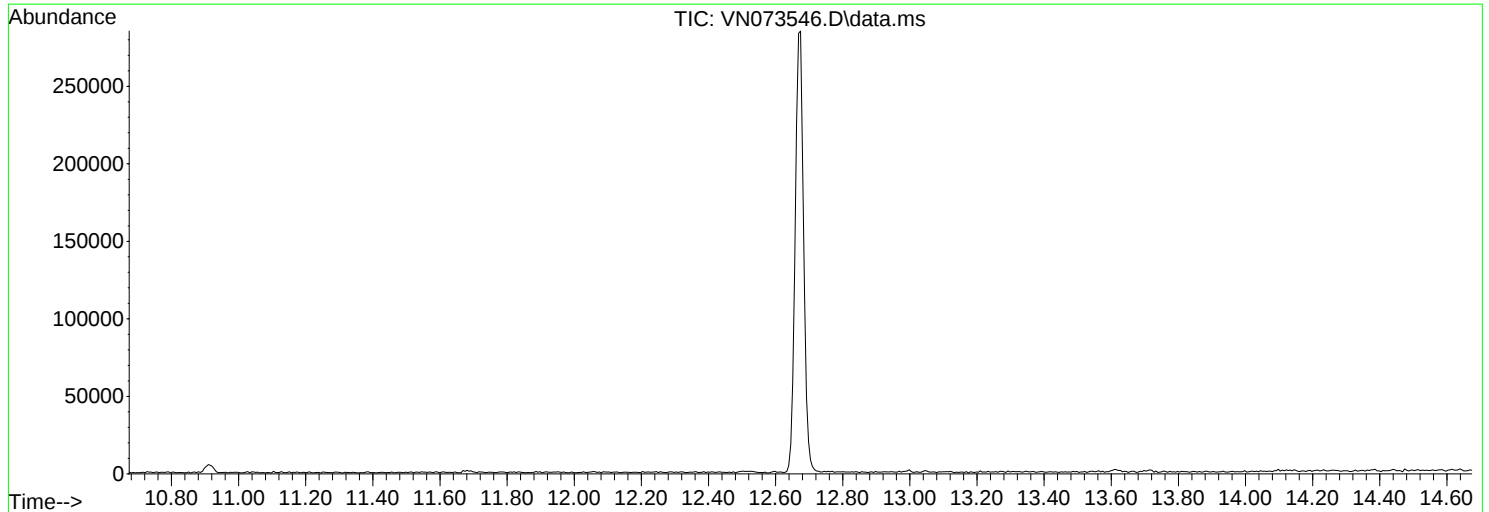

AutoFind: Scans 1833, 1834, 1835; Background Corrected with Scan 1824

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.1	11329	PASS
75	95	30	60	53.1	27232	PASS
95	95	100	100	100.0	51240	PASS
96	95	5	9	6.9	3556	PASS
173	174	0.00	2	1.4	583	PASS
174	95	50	100	79.0	40467	PASS
175	174	5	9	7.8	3159	PASS
176	174	95	101	95.8	38760	PASS
177	176	5	9	6.4	2469	PASS