

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072123\
 Data File : VN078621.D
 Acq On : 21 Jul 2023 18:13
 Operator : JC\MD
 Sample : 03680-02
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3

Quant Time: Jul 21 23:28:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
 Quant Title : SW846 8260
 QLast Update : Mon Jul 10 16:13:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.235	168	404089	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.112	114	756491	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.870	117	737525	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.800	152	258137	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.582	65	278572	51.423	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 102.840%	
35) Dibromofluoromethane	8.177	113	280141	54.552	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 109.100%	
50) Toluene-d8	10.571	98	929768	47.927	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 95.860%	
62) 4-Bromofluorobenzene	12.853	95	316705	53.001	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 106.000%	
Target Compounds						
					Qvalue	
3) Chloromethane	2.377	50	2005	0.372	ug/l	94
5) Bromomethane	2.977	94	2316	Below Cal	#	67
6) Chloroethane	3.106	64	1860	Below Cal	#	43
11) Tert butyl alcohol	5.541	59	430	0.515	ug/l #	72
16) Acetone	4.441	43	68585	40.644	ug/l	94
18) Methyl Acetate	5.059	43	7268	1.017	ug/l #	82
20) Methylene Chloride	5.283	84	19903	2.962	ug/l #	92
25) 2-Butanone	7.506	43	44471	16.742	ug/l	88
29) Tetrahydrofuran	7.871	42	1366	0.784	ug/l #	39
31) Cyclohexane	8.229	56	9628	1.315	ug/l #	26
36) 1,1-Dichloropropene	8.229	75	31602	4.262	ug/l #	49
37) Ethyl Acetate	7.571	43	15393	2.490	ug/l #	93
38) Carbon Tetrachloride	8.229	117	43991	5.459	ug/l #	15
42) 1,2-Dichloroethane	8.700	62	1878	0.251	ug/l #	73
43) Isopropyl Acetate	8.694	43	299676	29.448	ug/l #	84
45) 1,2-Dichloropropane	9.753	63	3897	0.700	ug/l #	45
48) Methyl methacrylate	9.747	41	256660	54.438	ug/l #	29
49) 1,4-Dioxane	9.747	88	378	3.676	ug/l #	1
51) 4-Methyl-2-Pentanone	10.453	43	149405	24.682	ug/l	90
54) cis-1,3-Dichloropropene	10.365	75	113416	13.231	ug/l #	69
56) Ethyl methacrylate	10.988	69	4546	0.606	ug/l #	1
57) 1,3-Dichloropropane	11.206	76	14771	1.620	ug/l #	42
59) 2-Hexanone	11.206	43	165338	38.433	ug/l #	50
74) N-amyl acetate	12.488	43	3261	0.390	ug/l #	37
75) 1,1,2,2-Tetrachloroethane	12.941	83	142	Below Cal	#	63
76) 1,2,3-Trichloropropane	12.853	75	167155	26.790	ug/l #	1
77) Bromobenzene	12.864	156	60	Below Cal	#	1
81) trans-1,4-Dichloro-2-b...	12.853	75	167155	70.399	ug/l #	15
92) 1,2-Dibromo-3-Chloropr...	14.817	75	57	Below Cal	#	4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072123\
Data File : VN078621.D
Acq On : 21 Jul 2023 18:13
Operator : JC\MD
Sample : 03680-02
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-3

Quant Time: Jul 21 23:28:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Quant Title : SW846 8260
QLast Update : Mon Jul 10 16:13:53 2023
Response via : Initial Calibration

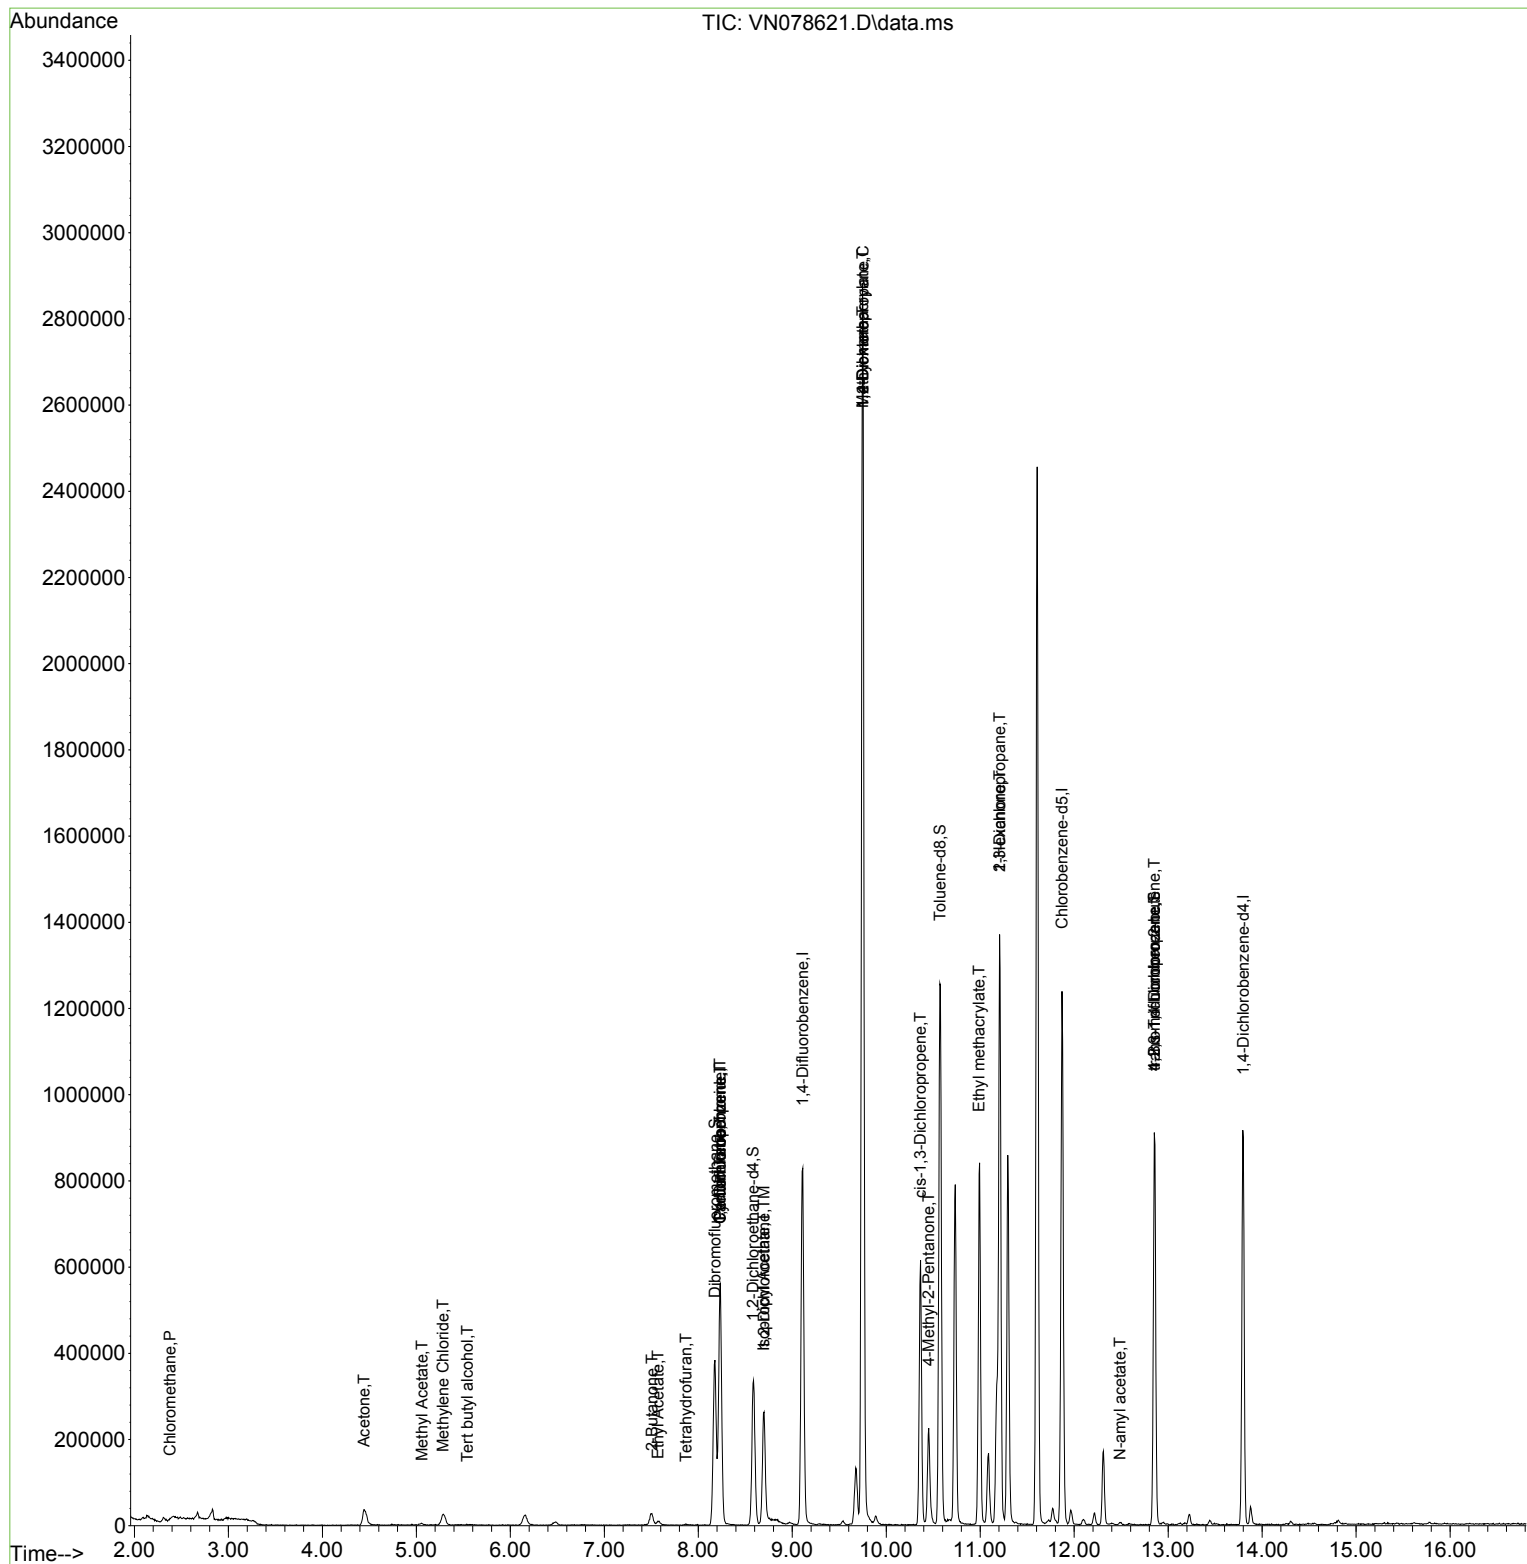



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 8.235 min Scan# 1

Delta R.T. 0.005 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Instrument :

MSVOA_N

ClientSampleId :





TP-3

Tgt Ion:168 Resp: 404089

Ion Ratio Lower Upper

168 100

99 58.2 53.0 79.6

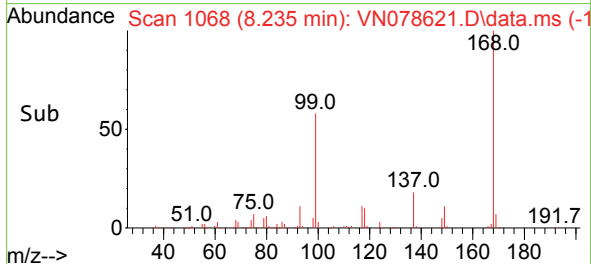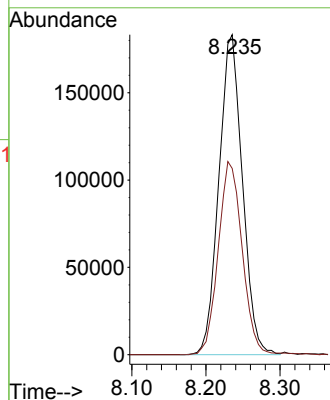

#3

Chloromethane

Concen: 0.372 ug/l

RT: 2.377 min Scan# 72

Delta R.T. 0.006 min

Lab File: VN078621.D




Acq: 21 Jul 2023 18:13


Tgt Ion: 50 Resp: 2005

Ion Ratio Lower Upper

50 100

52 29.5 26.5 39.7



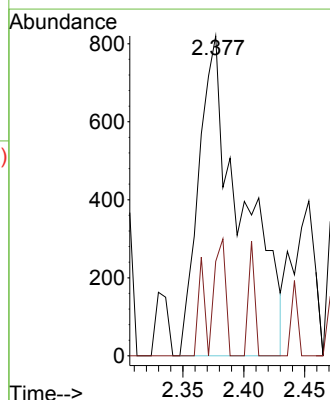
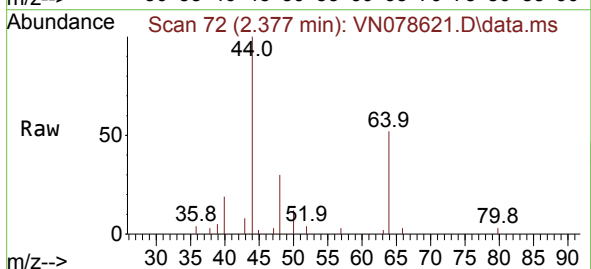


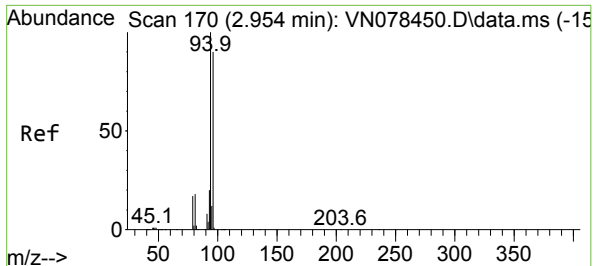

#5
Bromomethane
Concen: Below Cal
RT: 2.977 min Scan# 11
Delta R.T. 0.023 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 94 Resp: 2316
Ion Ratio Lower Upper
94 100
96 60.0 73.1 109.7#

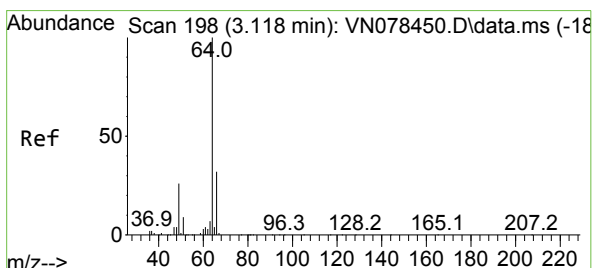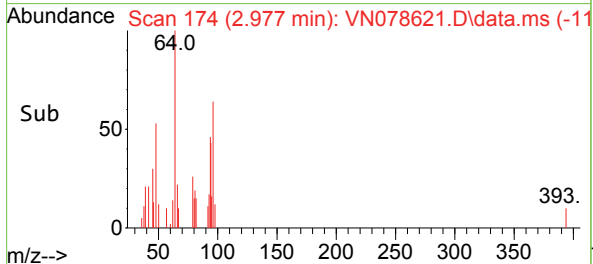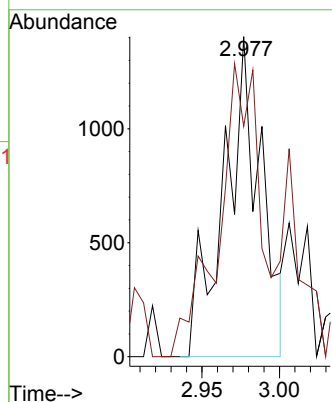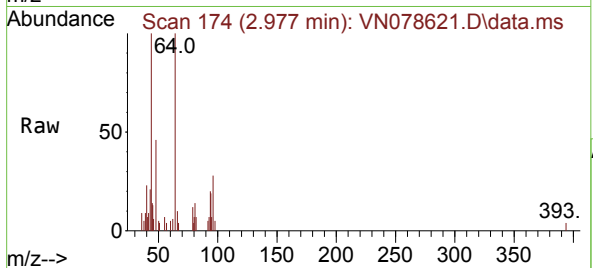

#6
Chloroethane
Concen: Below Cal
RT: 3.106 min Scan# 196
Delta R.T. -0.012 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 64 Resp: 1860
Ion Ratio Lower Upper
64 100
66 0.0 25.4 38.2#


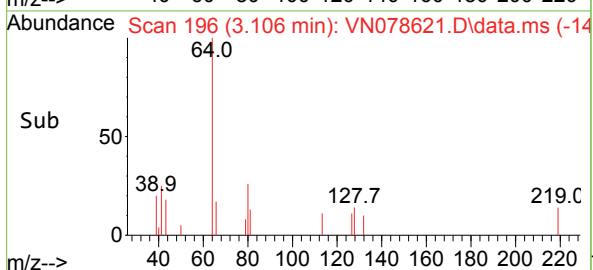

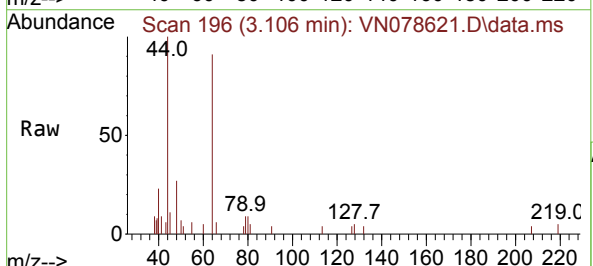




#11
Tert butyl alcohol
Concen: 0.515 ug/l
RT: 5.541 min Scan# 610
Delta R.T. 0.005 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 59 Resp: 430
Ion Ratio Lower Upper
59 100
57 0.0 8.2 12.4#

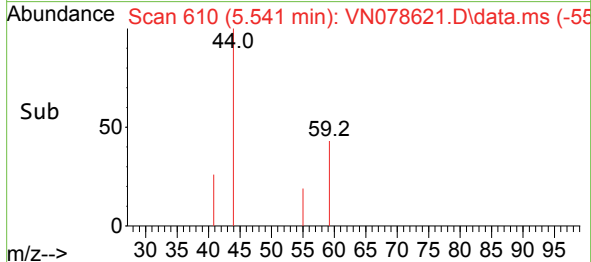

#16
Acetone
Concen: 40.644 ug/l
RT: 4.441 min Scan# 423
Delta R.T. -0.001 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 43 Resp: 68585
Ion Ratio Lower Upper
43 100
58 31.4 28.0 42.0


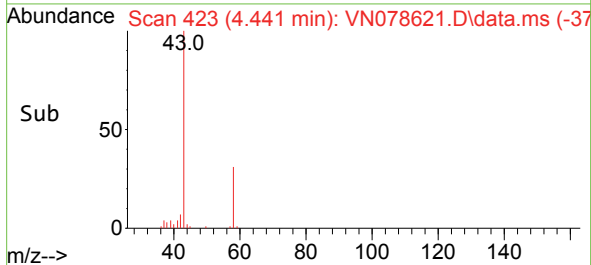

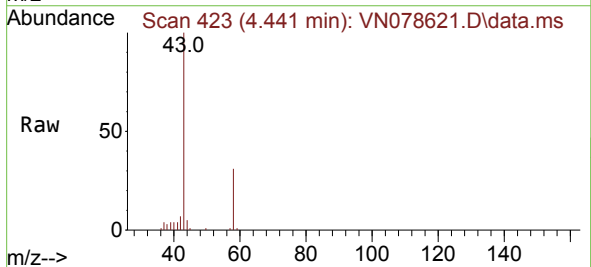




#18
Methyl Acetate
Concen: 1.017 ug/l
RT: 5.059 min Scan# 51
Delta R.T. 0.023 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 43 Resp: 7268
Ion Ratio Lower Upper
43 100
74 22.4 26.2 39.4#

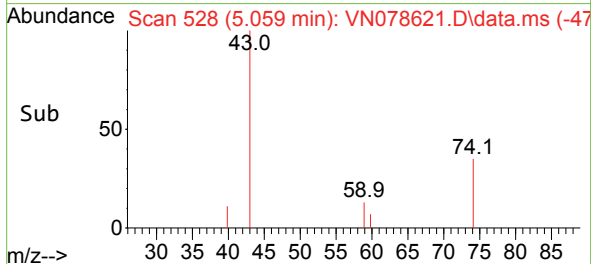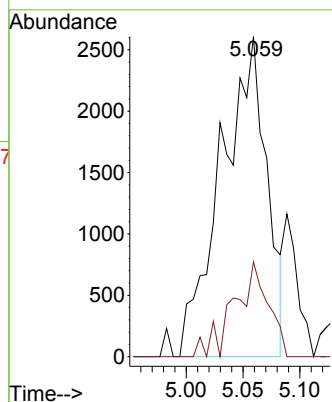

#20
Methylene Chloride
Concen: 2.962 ug/l
RT: 5.283 min Scan# 566
Delta R.T. -0.000 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 84 Resp: 19903
Ion Ratio Lower Upper
84 100
49 106.6 79.7 119.5
51 43.6 25.2 37.8#
86 64.9 53.3 79.9


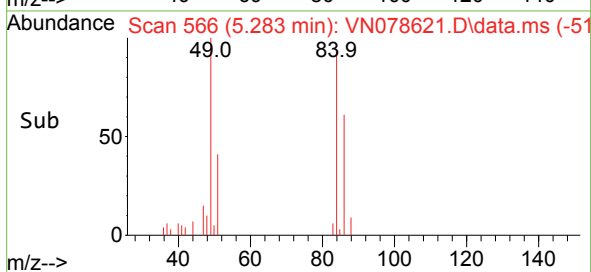

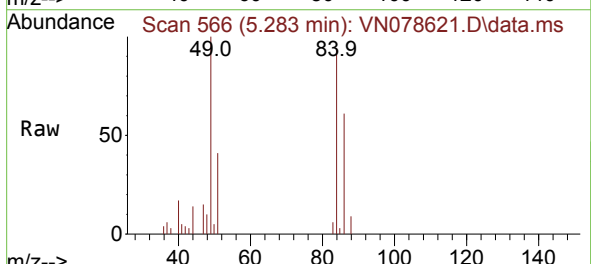


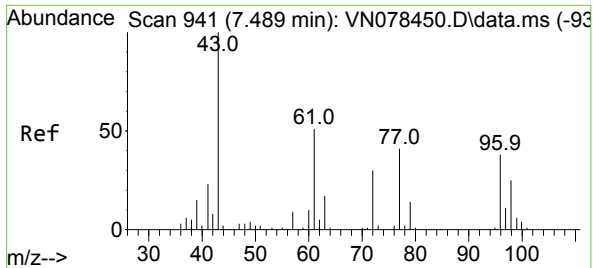

#25
2-Butanone
Concen: 16.742 ug/l
RT: 7.506 min Scan# 941
Delta R.T. 0.017 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 43 Resp: 44471
Ion Ratio Lower Upper
43 100
72 30.5 30.2 45.2

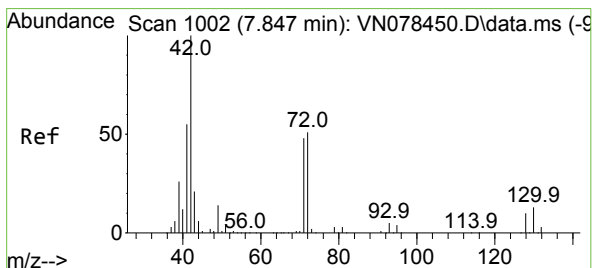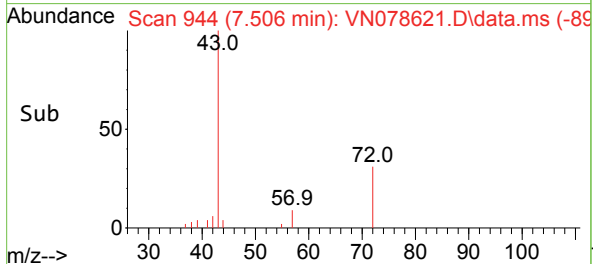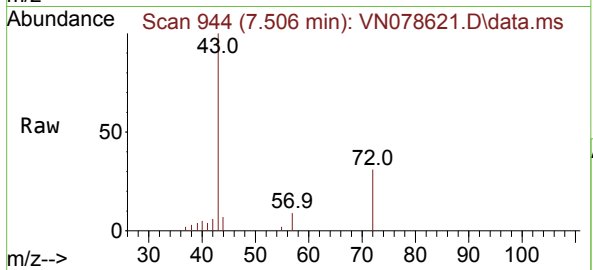

#29
Tetrahydrofuran
Concen: 0.784 ug/l
RT: 7.871 min Scan# 1006
Delta R.T. 0.024 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 42 Resp: 1366
Ion Ratio Lower Upper
42 100
72 0.0 49.8 74.6#
71 29.4 47.4 71.2#


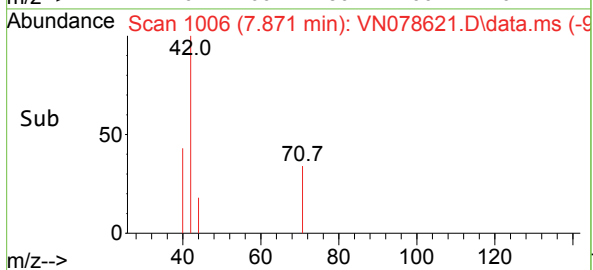

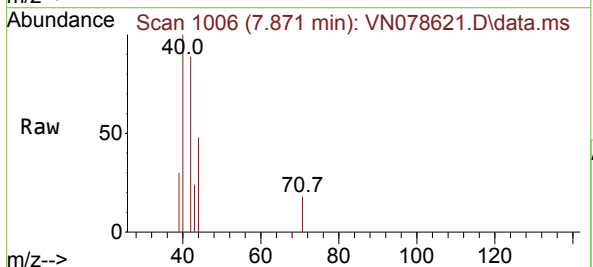




#31
Cyclohexane
Concen: 1.315 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.036 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 56 Resp: 9628
Ion Ratio Lower Upper
56 100
69 154.7 26.8 40.2#
84 130.9 81.8 122.6#

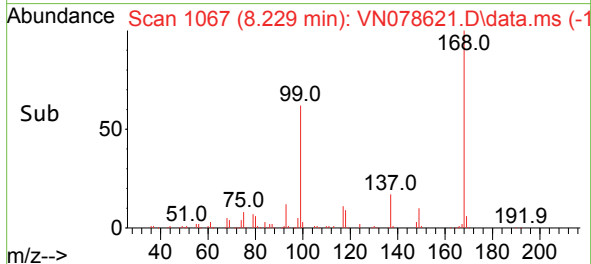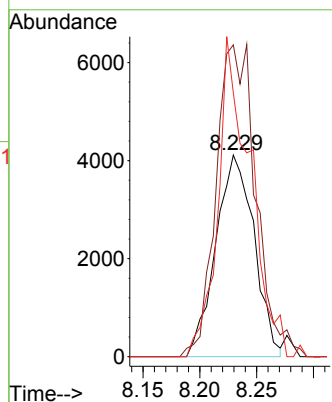

#33
1,2-Dichloroethane-d4
Concen: 51.423 ug/l
RT: 8.582 min Scan# 1127
Delta R.T. -0.001 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 65 Resp: 278572
Ion Ratio Lower Upper
65 100
67 52.2 0.0 106.6

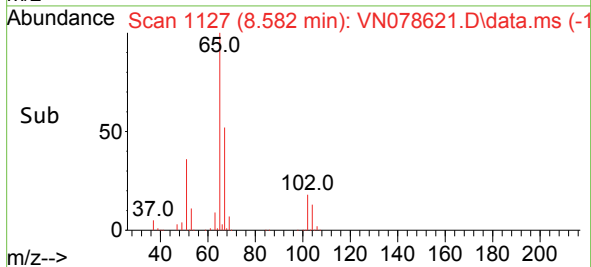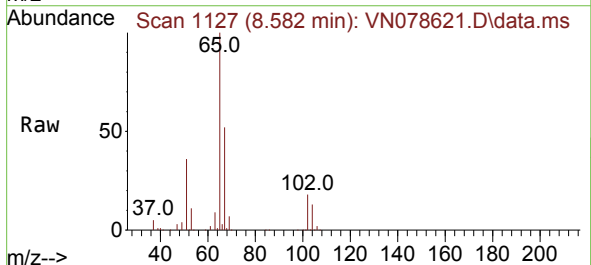



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.112 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Instrument :

MSVOA_N

ClientSampleId :

TP-3





Tgt Ion:114 Resp: 756491

Ion Ratio Lower Upper

114 100

63 19.2 0.0 36.4

88 15.4 0.0 30.6

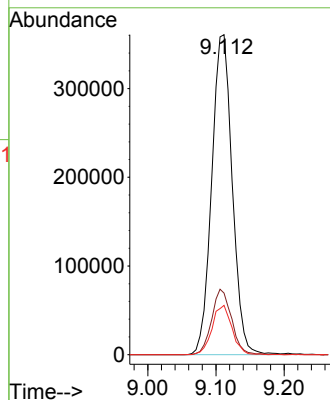

#35

Dibromofluoromethane

Concen: 54.552 ug/l

RT: 8.177 min Scan# 1058

Delta R.T. -0.000 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13




Tgt Ion:113 Resp: 280141


Ion Ratio Lower Upper

113 100

111 100.9 82.6 123.8


192 16.8 12.7 19.1

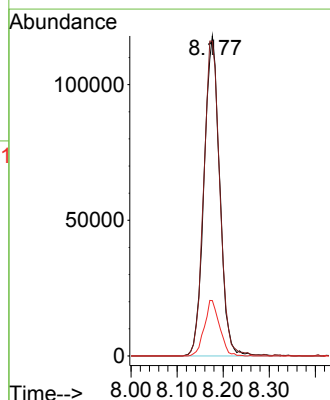






#36
1,1-Dichloropropene
Concen: 4.262 ug/l
RT: 8.229 min Scan# 1067
Delta R.T. -0.148 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Instrument :
MSVOA_N
ClientSampleId :
TP-3







Tgt Ion: 75 Resp: 31602
Ion Ratio Lower Upper
75 100
110 10.0 19.1 57.3#
77 0.0 25.0 37.4#

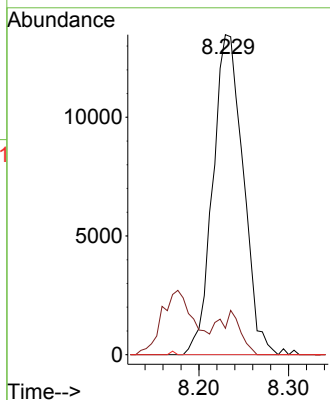

#37
Ethyl Acetate
Concen: 2.490 ug/l
RT: 7.571 min Scan# 955
Delta R.T. -0.000 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 43 Resp: 15393
Ion Ratio Lower Upper
43 100
61 13.2 13.2 19.8
70 11.2 11.3 16.9#

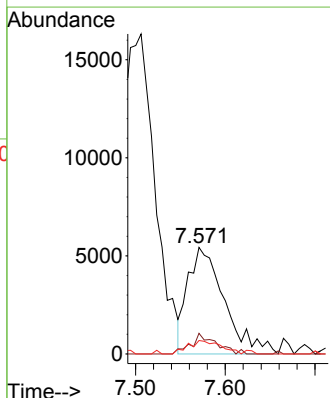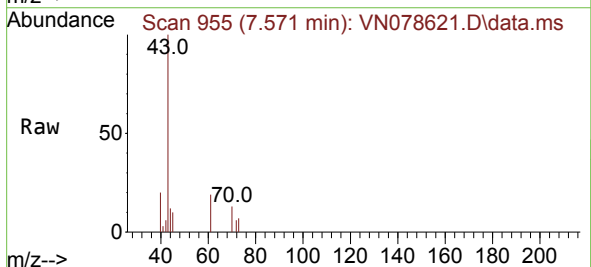



#38

Carbon Tetrachloride

Concen: 5.459 ug/l

RT: 8.229 min Scan# 1067

Delta R.T. -0.136 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Instrument :

MSVOA_N

ClientSampleId :

TP-3





Tgt Ion:117 Resp: 43991

Ion Ratio Lower Upper

117 100

119 4.1 77.3 115.9#

121 0.0 23.3 34.9#

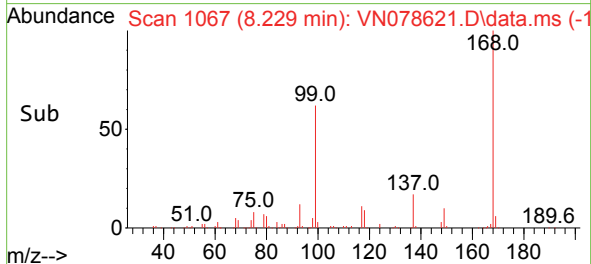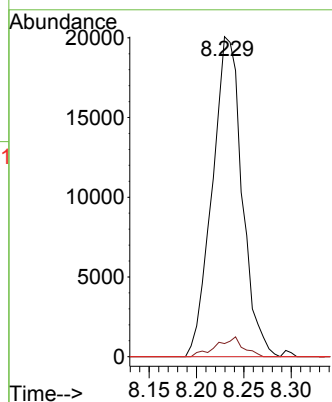

#42

1,2-Dichloroethane

Concen: 0.251 ug/l

RT: 8.700 min Scan# 1147

Delta R.T. 0.023 min

Lab File: VN078621.D




Acq: 21 Jul 2023 18:13


Tgt Ion: 62 Resp: 1878

Ion Ratio Lower Upper

62 100

98 0.0 0.0 19.8




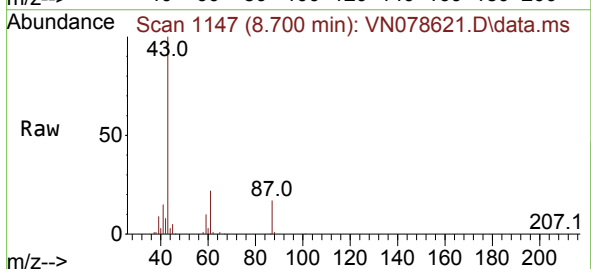




#43
Isopropyl Acetate
Concen: 29.448 ug/l
RT: 8.694 min Scan# 1146
Delta R.T. 0.000 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 43 Resp: 299676
Ion Ratio Lower Upper
43 100
61 19.6 24.7 37.1#
87 14.3 14.6 21.8#

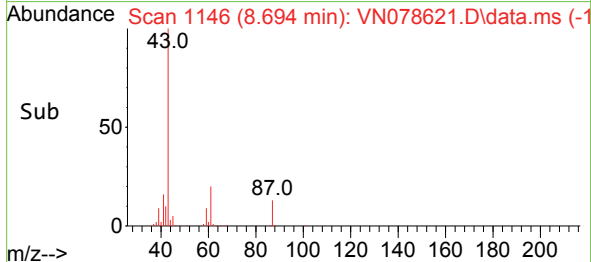

#45
1,2-Dichloropropane
Concen: 0.700 ug/l
RT: 9.753 min Scan# 1326
Delta R.T. 0.123 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 63 Resp: 3897
Ion Ratio Lower Upper
63 100
65 0.0 23.9 35.9#



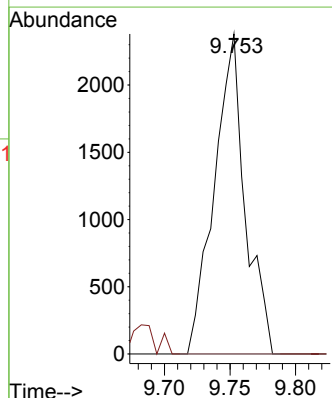
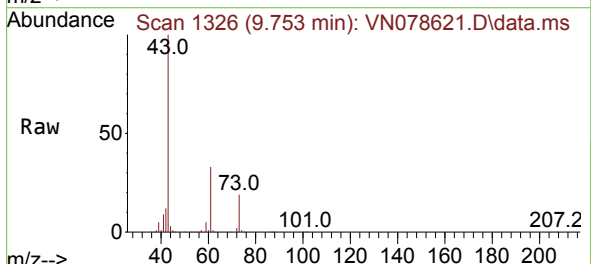




#48
Methyl methacrylate
Concen: 54.438 ug/l
RT: 9.747 min Scan# 11
Delta R.T. 0.059 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 41 Resp: 256660
Ion Ratio Lower Upper
41 100
69 0.1 90.4 135.6#
39 57.2 54.6 81.8

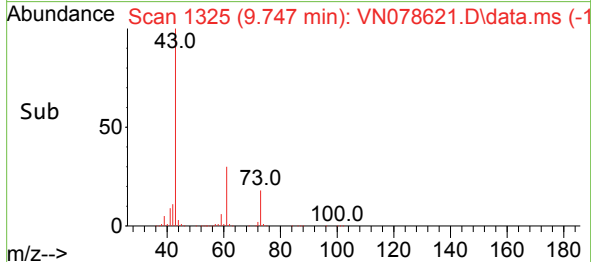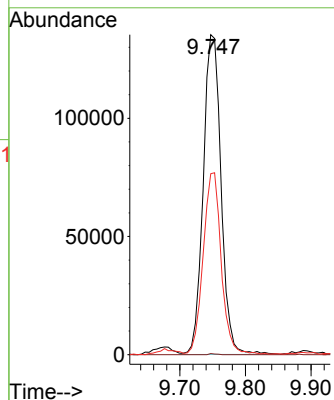

#49
1,4-Dioxane
Concen: 3.676 ug/l
RT: 9.747 min Scan# 1325
Delta R.T. 0.047 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 88 Resp: 378
Ion Ratio Lower Upper
88 100
43 721788.4 17.0 25.6#
58 3867.5 47.0 70.4#


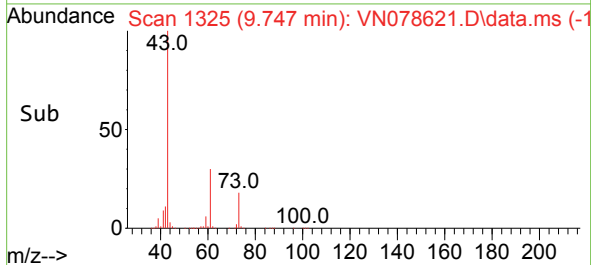
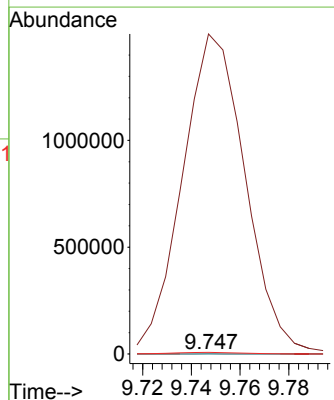
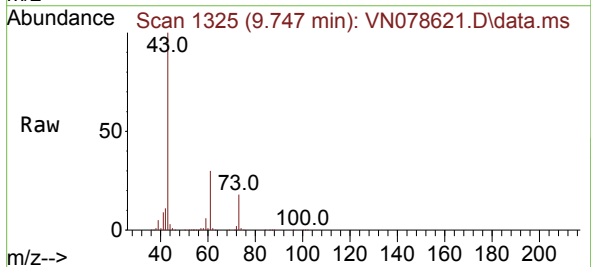




#50
Toluene-d8
Concen: 47.927 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. -0.000 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 98 Resp: 929768
Ion Ratio Lower Upper
98 100
100 62.5 52.0 78.0

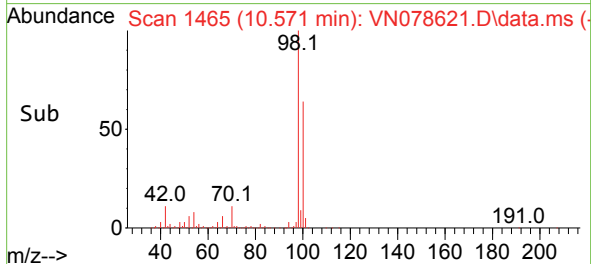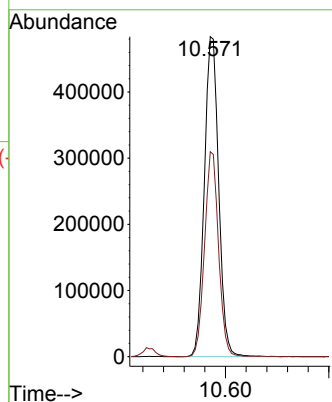

#51
4-Methyl-2-Pentanone
Concen: 24.682 ug/l
RT: 10.453 min Scan# 1445
Delta R.T. -0.000 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 43 Resp: 149405
Ion Ratio Lower Upper
43 100
58 39.4 36.6 54.8



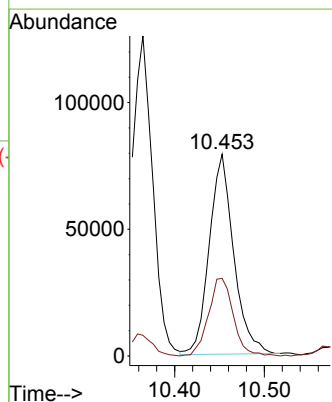
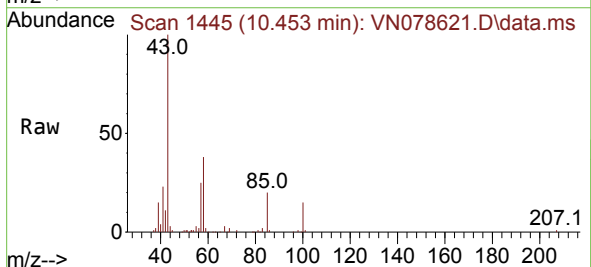


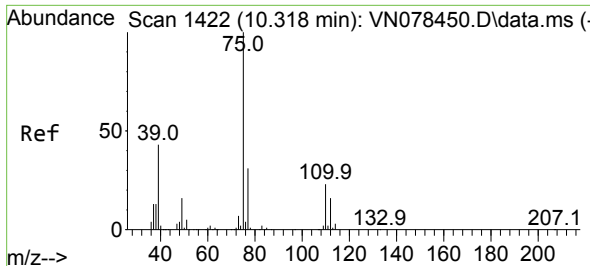

#54
 cis-1,3-Dichloropropene
 Concen: 13.231 ug/l
 RT: 10.365 min Scan# 14
 Delta R.T. 0.047 min
 Lab File: VN078621.D
 Acq: 21 Jul 2023 18:13




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3


Tgt Ion: 75 Resp: 113416
 Ion Ratio Lower Upper
 75 100
 77 0.3 26.1 39.1#
 39 33.4 31.6 47.4

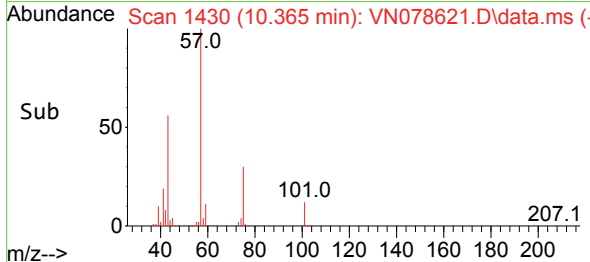

#56
 Ethyl methacrylate
 Concen: 0.606 ug/l
 RT: 10.988 min Scan# 1536
 Delta R.T. 0.106 min
 Lab File: VN078621.D
 Acq: 21 Jul 2023 18:13

Tgt Ion: 69 Resp: 4546
 Ion Ratio Lower Upper
 69 100
 41 3392.3 39.6 59.4#
 39 1544.3 28.6 43.0#

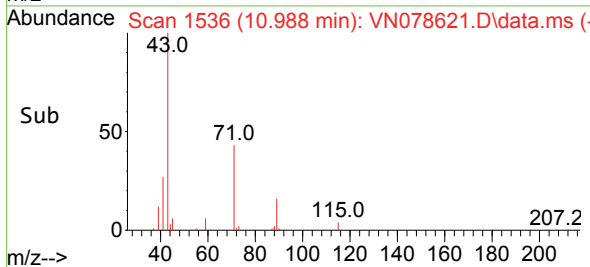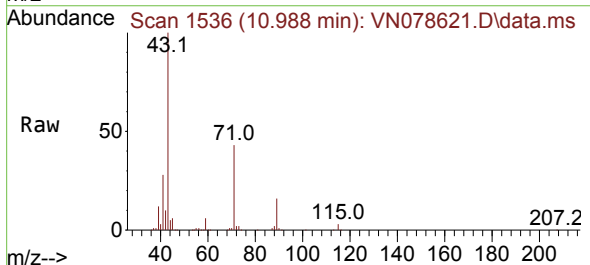

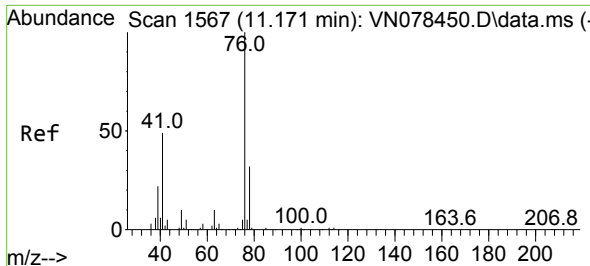

#57

1,3-Dichloropropane

Concen: 1.620 ug/l

RT: 11.206 min Scan# 1573

Delta R.T. 0.035 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Instrument :

MSVOA_N

ClientSampleId :





TP-3

Tgt Ion: 76 Resp: 14771

Ion Ratio Lower Upper

76 100

78 0.0 26.1 39.1#

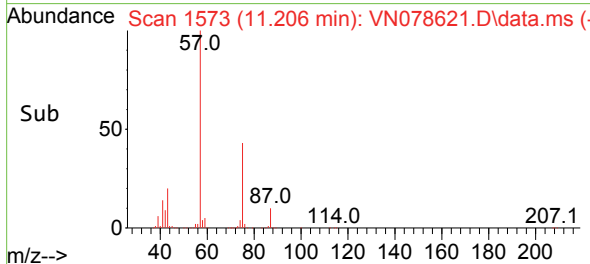

#59

2-Hexanone

Concen: 38.433 ug/l

RT: 11.206 min Scan# 1573

Delta R.T. 0.006 min

Lab File: VN078621.D




Acq: 21 Jul 2023 18:13


Tgt Ion: 43 Resp: 165338

Ion Ratio Lower Upper

43 100

58 24.4 31.7 95.1#


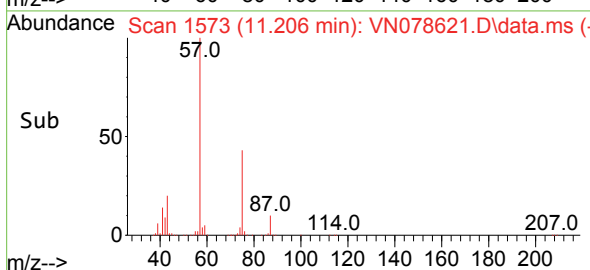

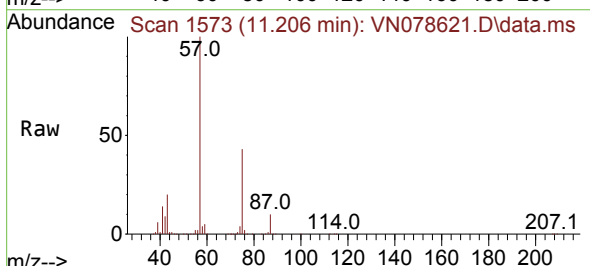


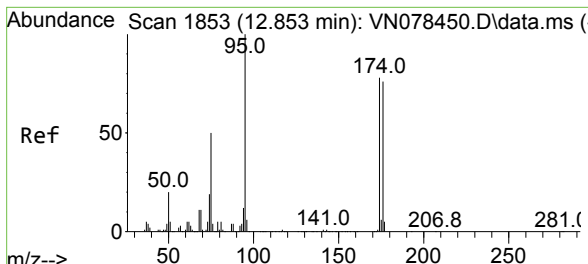

#62
 4-Bromofluorobenzene
 Concen: 53.001 ug/l
 RT: 12.853 min Scan# 1853
 Delta R.T. -0.000 min
 Lab File: VN078621.D
 Acq: 21 Jul 2023 18:13




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3


Tgt Ion:	95	Resp:	316705
Ion	Ratio	Lower	Upper
95	100		
174	79.4	0.0	143.8
176	75.4	0.0	135.8

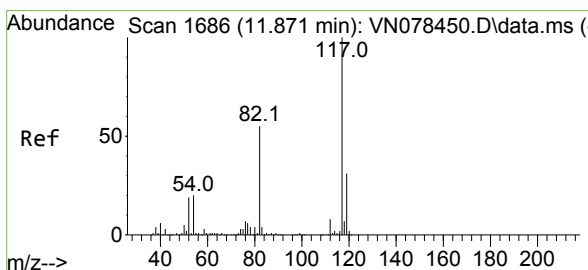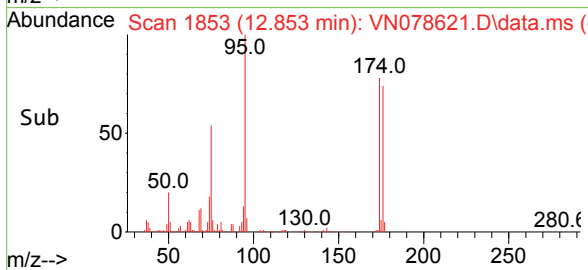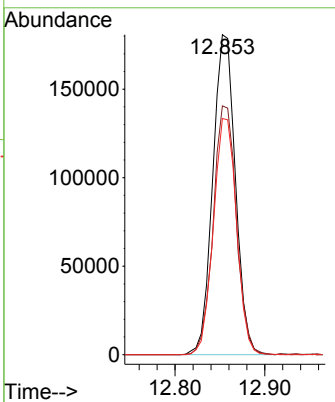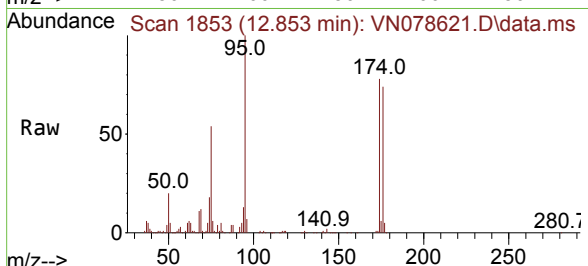

#63
 Chlorobenzene-d5
 Concen: 50.000 ug/l
 RT: 11.870 min Scan# 1686
 Delta R.T. -0.001 min
 Lab File: VN078621.D
 Acq: 21 Jul 2023 18:13

Tgt Ion:	117	Resp:	737525
Ion	Ratio	Lower	Upper
117	100		
82	53.7	44.0	66.0
119	31.4	25.6	38.4

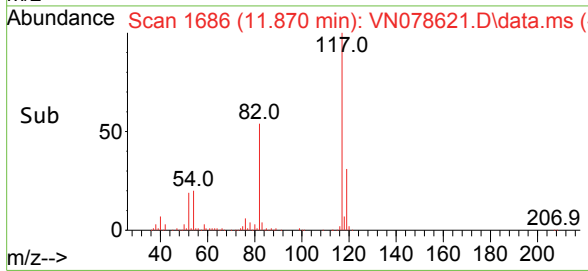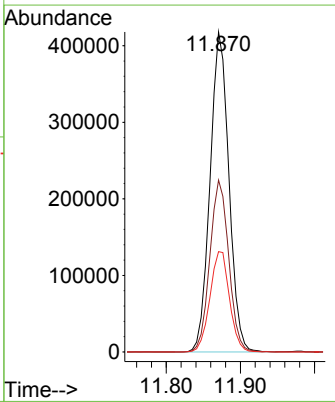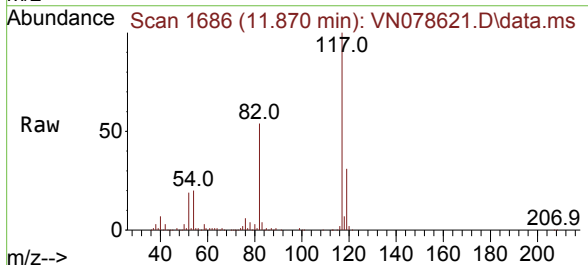



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.800 min Scan# 2014

Delta R.T. -0.000 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Instrument :

MSVOA_N

ClientSampleId :

TP-3





Tgt Ion:152 Resp: 258137

Ion Ratio Lower Upper

152 100

115 58.3 32.3 96.8

150 156.4 0.0 355.8

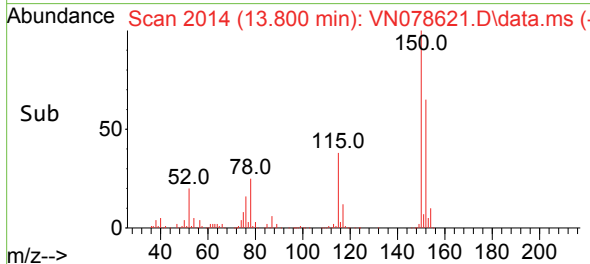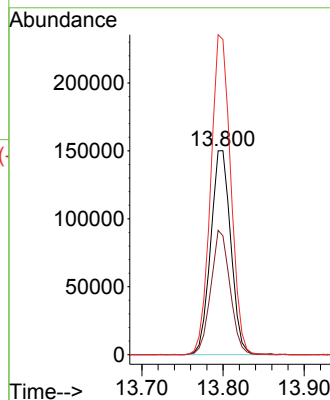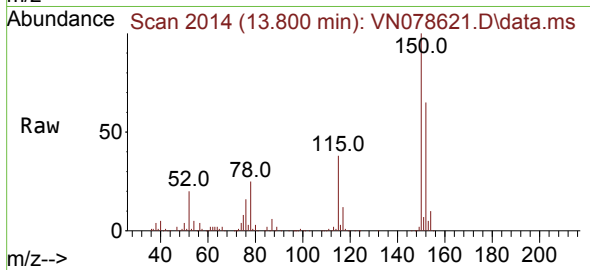

#74

N-ethyl acetate

Concen: 0.390 ug/l

RT: 12.488 min Scan# 1791

Delta R.T. -0.012 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Tgt Ion: 43 Resp: 3261




Ion Ratio Lower Upper


43 100

70 0.0 43.4 65.2#

55 2.7 21.4 32.0#

61 0.0 22.8 34.2#



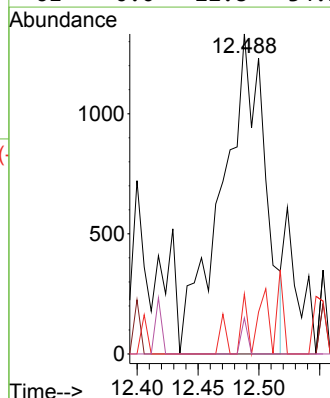
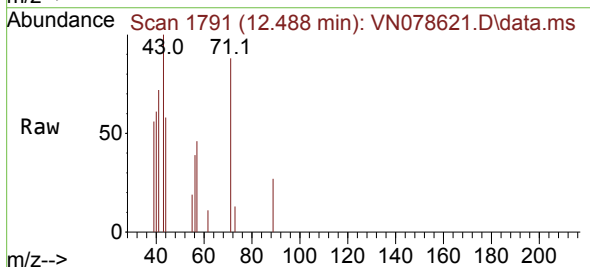




#75
1,1,2,2-Tetrachloroethane
Concen: Below Cal
RT: 12.941 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13




Instrument :
MSVOA_N
ClientSampleId :
TP-3


Tgt Ion: 83 Resp: 142
Ion Ratio Lower Upper
83 100
131 0.0 5.0 15.0#
85 93.7 31.9 95.7

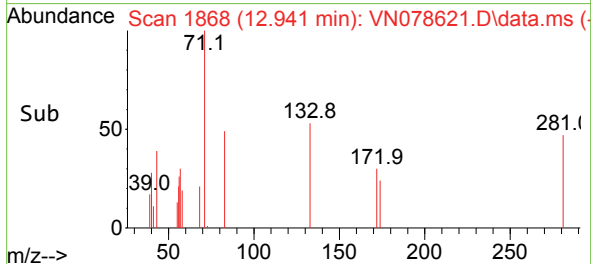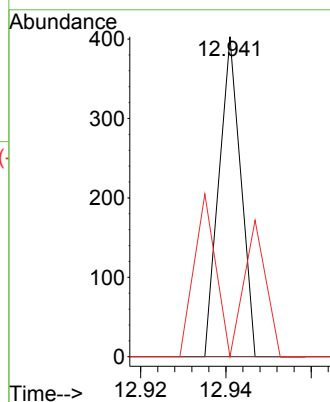

#76
1,2,3-Trichloropropane
Concen: 26.790 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. -0.147 min
Lab File: VN078621.D
Acq: 21 Jul 2023 18:13

Tgt Ion: 75 Resp: 167155
Ion Ratio Lower Upper
75 100
77 1.4 84.5 253.5#

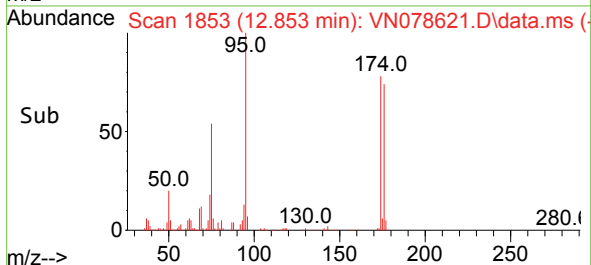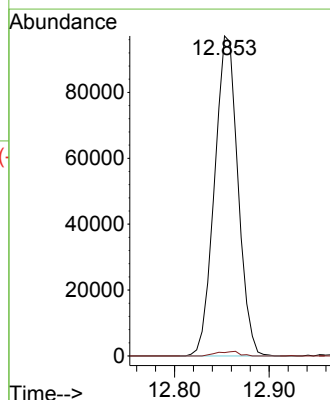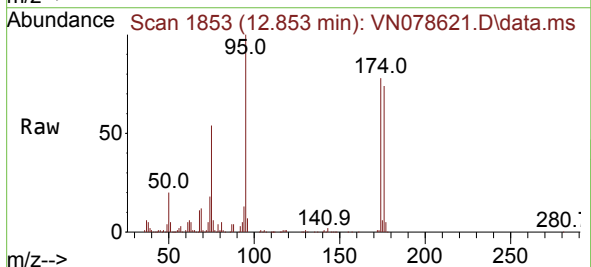



#77

Bromobenzene

Concen: Below Cal

RT: 12.864 min Scan# 1855

Delta R.T. -0.124 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13

Instrument :

MSVOA_N

ClientSampleId :

TP-3





Tgt Ion:156 Resp: 60

Ion Ratio Lower Upper

156 100

77 3833.3 107.7 323.3#

158 0.0 48.4 145.3#

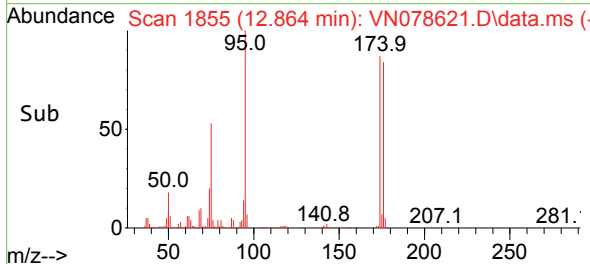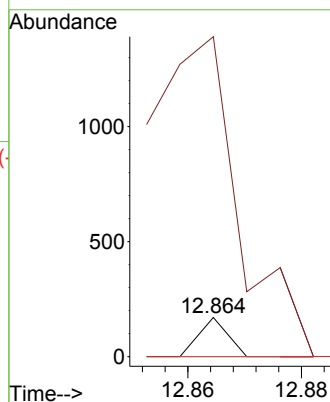

#81

trans-1,4-Dichloro-2-butene

Concen: 70.399 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN078621.D

Acq: 21 Jul 2023 18:13




Tgt Ion: 75 Resp: 167155


Ion Ratio Lower Upper

75 100

53 0.2 67.4 101.2#

89 0.0 38.8 58.2#

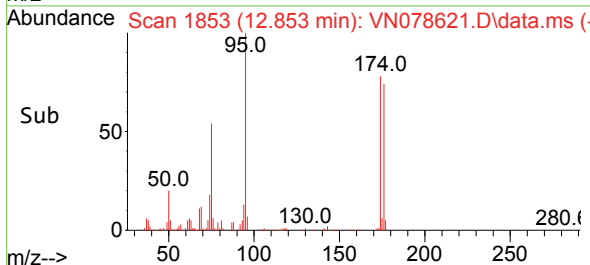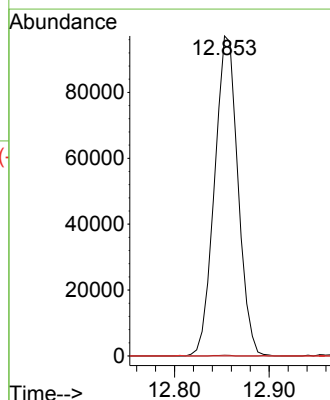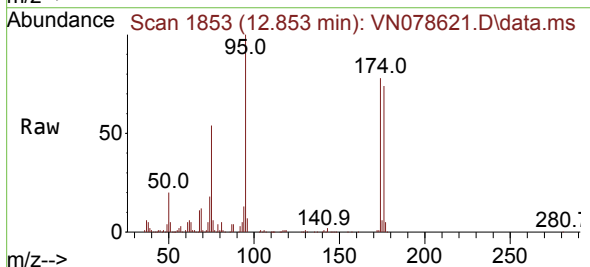



#92
 1,2-Dibromo-3-Chloropropane
 Concen: Below Cal
 RT: 14.817 min Scan# 21
 Delta R.T. 0.094 min
 Lab File: VN078621.D
 Acq: 21 Jul 2023 18:13

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-3

Tgt Ion: 75 Resp: 57
 Ion Ratio Lower Upper
 75 100
 155 0.0 39.1 117.2#
 157 0.0 50.3 150.9#

