
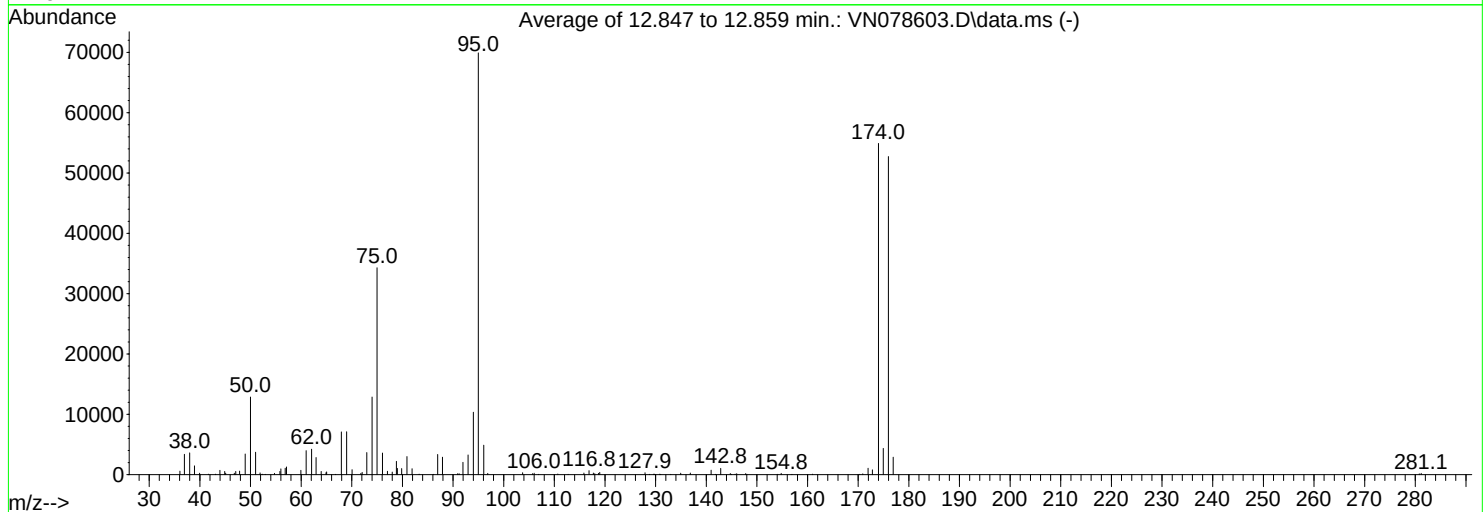


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072123\
Data File : VN078603.D
Acq On : 21 Jul 2023 09:18
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071023W.M
Title : SW846 8260
Last Update : Mon Jul 10 16:13:53 2023

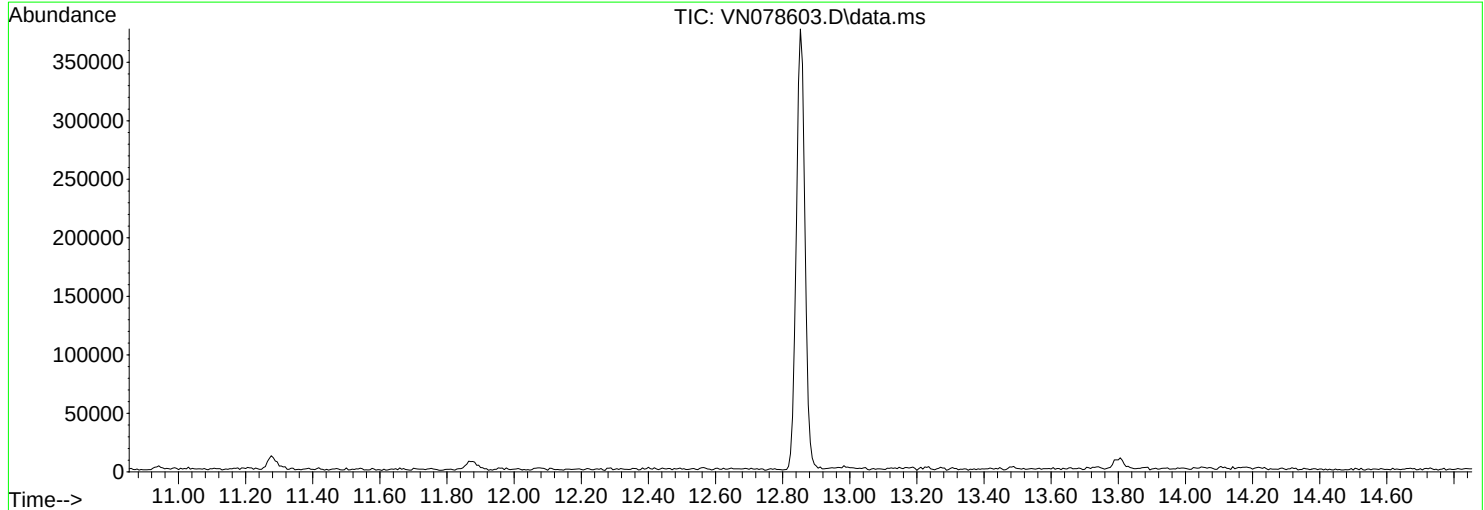

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.4	12872	PASS
75	95	30	60	49.1	34299	PASS
95	95	100	100	100.0	69923	PASS
96	95	5	9	7.0	4886	PASS
173	174	0.00	2	1.5	802	PASS
174	95	50	100	78.5	54896	PASS
175	174	5	9	7.9	4347	PASS
176	174	95	101	96.1	52731	PASS
177	176	5	9	5.5	2906	PASS

Average of 12.847 to 12.859 min.: VN078603.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	593	47.10	521	56.85	1055	69.00	712
36.95	3381	47.85	589	57.10	1272	70.05	811
38.00	3617	48.95	3434	59.95	715	71.80	205
38.95	1450	50.00	12872	61.00	3976	72.05	361
39.95	243	51.00	3720	62.05	4212	72.95	3662
41.70	87	51.90	302	62.95	2843	74.00	12869
43.10	89	52.30	84	63.95	538	75.00	34299
43.95	718	52.90	51	64.90	311	76.05	3592
44.90	539	54.75	212	65.05	465	77.05	568
45.10	246	55.80	536	66.80	60	78.00	413
46.80	243	56.00	944	67.95	7092	78.80	2192

Average of 12.847 to 12.859 min.: VN078603.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.00	1046	92.95	3270	115.85	257	131.00	57
79.85	1003	94.00	10348	116.85	675	133.00	65
80.90	2992	95.00	69923	117.70	273	134.95	249
81.90	990	96.05	4886	118.00	164	136.85	278
83.30	74	96.85	210	118.70	219	140.95	751
86.10	61	103.75	327	118.95	362	141.80	52
86.95	3349	105.70	171	127.90	309	142.85	1041
87.90	2890	106.00	237	128.80	54	144.75	193
90.90	166	106.90	53	129.60	84	145.00	59
91.20	157	110.70	105	129.80	75	145.70	75
91.95	2058	112.70	53	130.80	76	146.00	156

Average of 12.847 to 12.859 min.: VN078603.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.75	160	174.95	4347				
148.00	92	175.95	52731				
154.10	66	176.90	2906				
154.80	200	280.80	130				
156.90	59	281.15	208				
161.00	88						
170.30	59						
170.90	127						
171.95	1063						
172.80	802						
174.00	54896						

Instrument :

MSVOA_N

ClientSampleId :

BFB