


Instrument :
MSVOA_N
ClientSampleId :

Dichlorodifluoromethane


Response Ratio

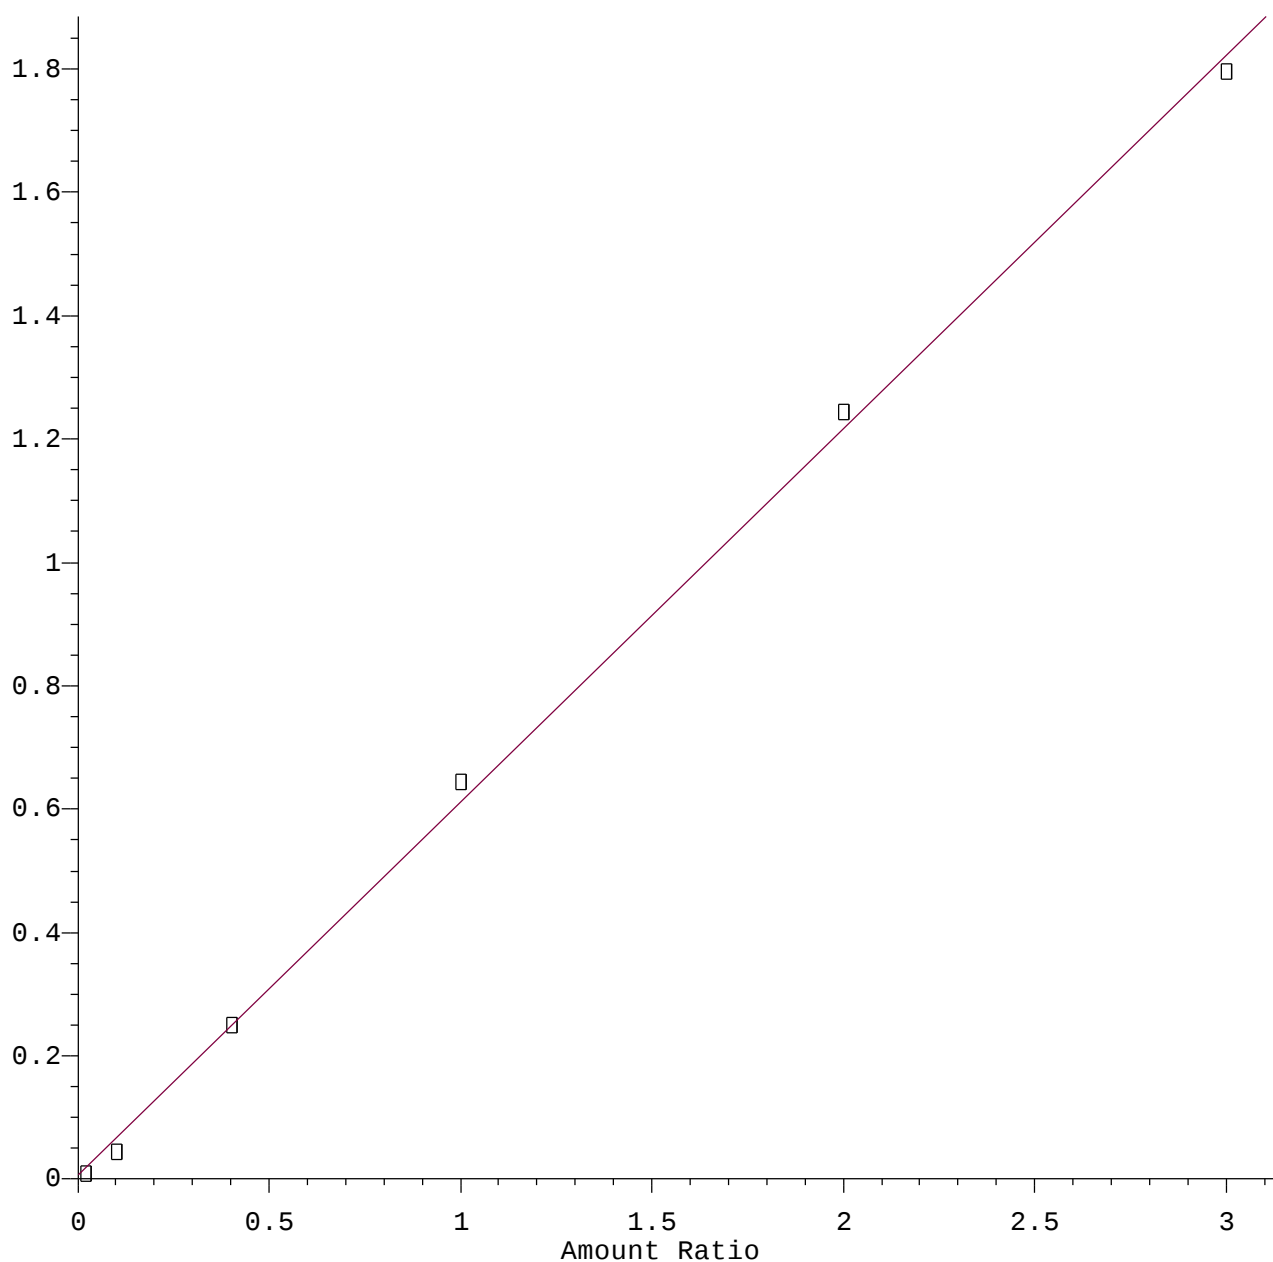

Resp Ratio = $6.06 \times 10^{-1} \times \text{Amt} + 5.54 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

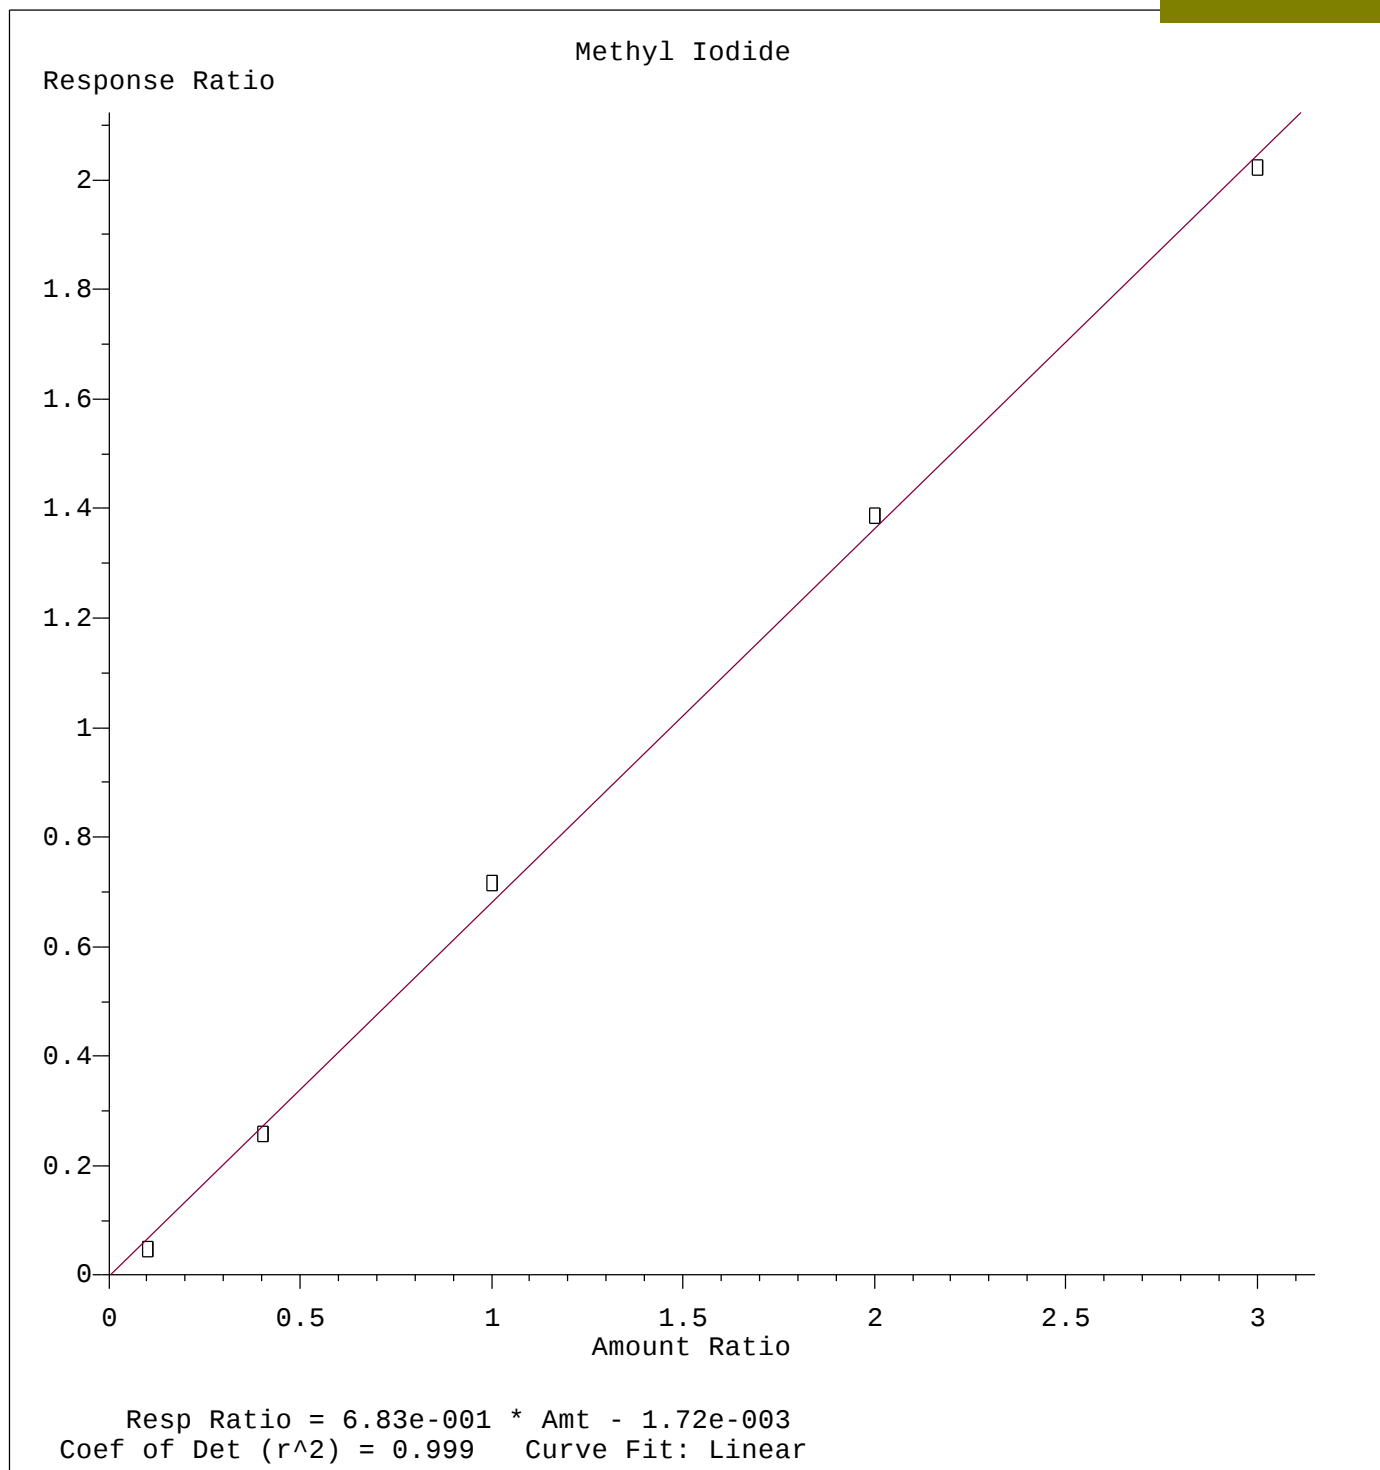


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

Methyl Acetate

Response Ratio

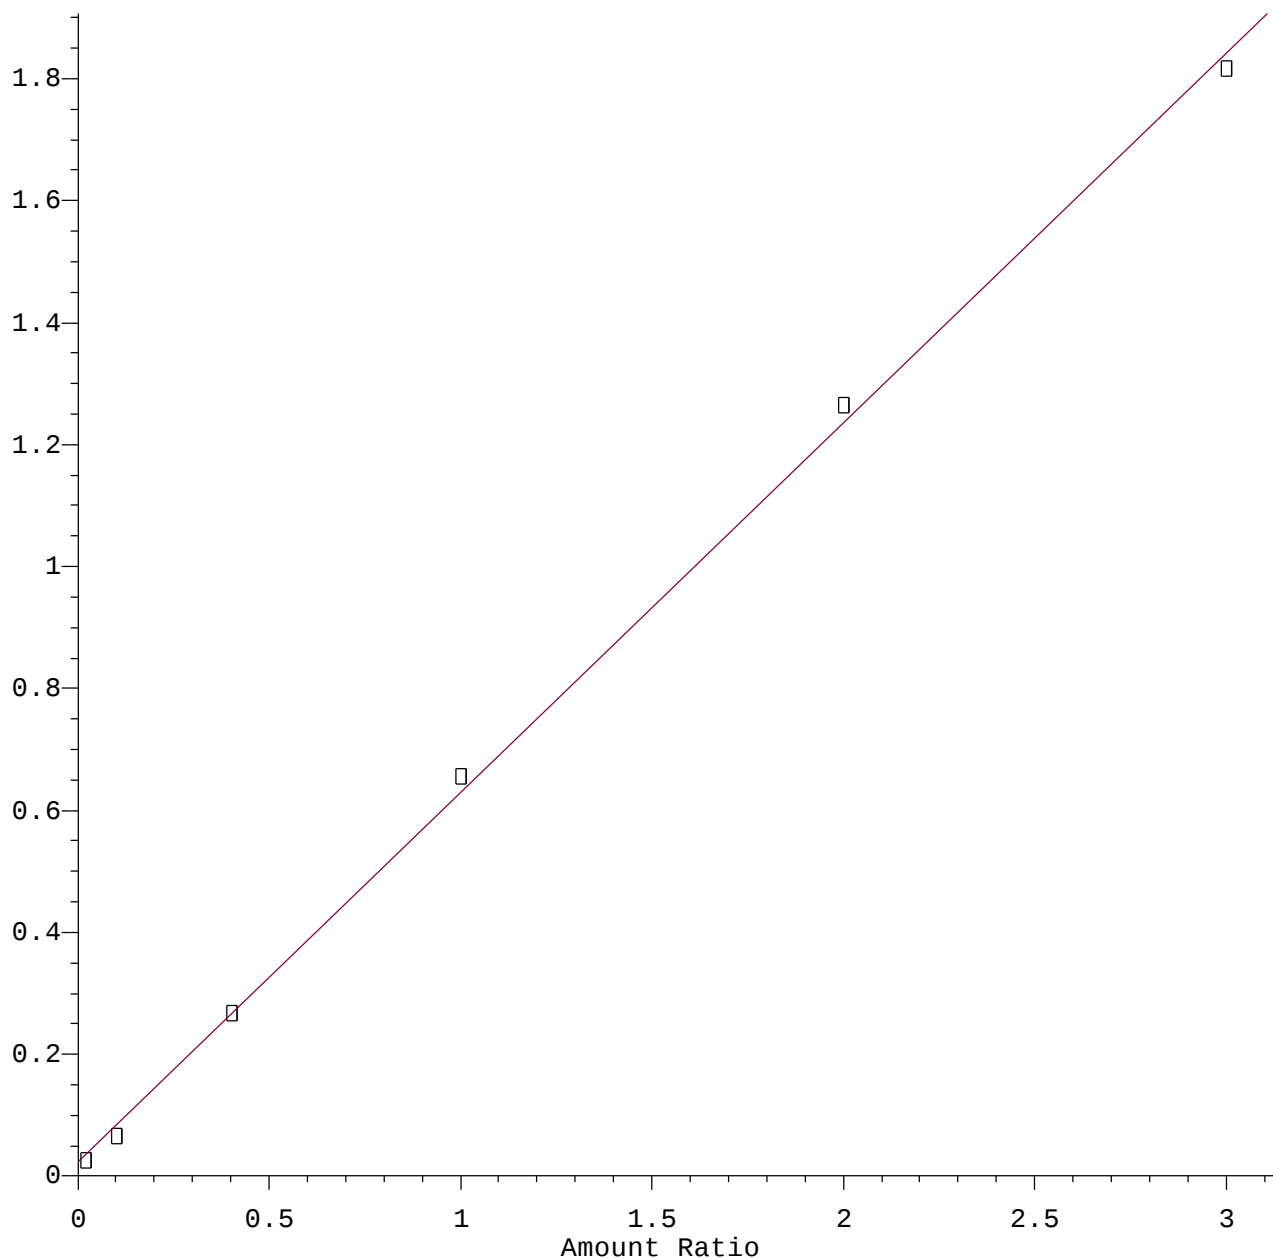


Resp Ratio = $6.06 \times 10^{-1} \times \text{Amt} + 2.31 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

2-Chloroethyl Vinyl ether


Response Ratio

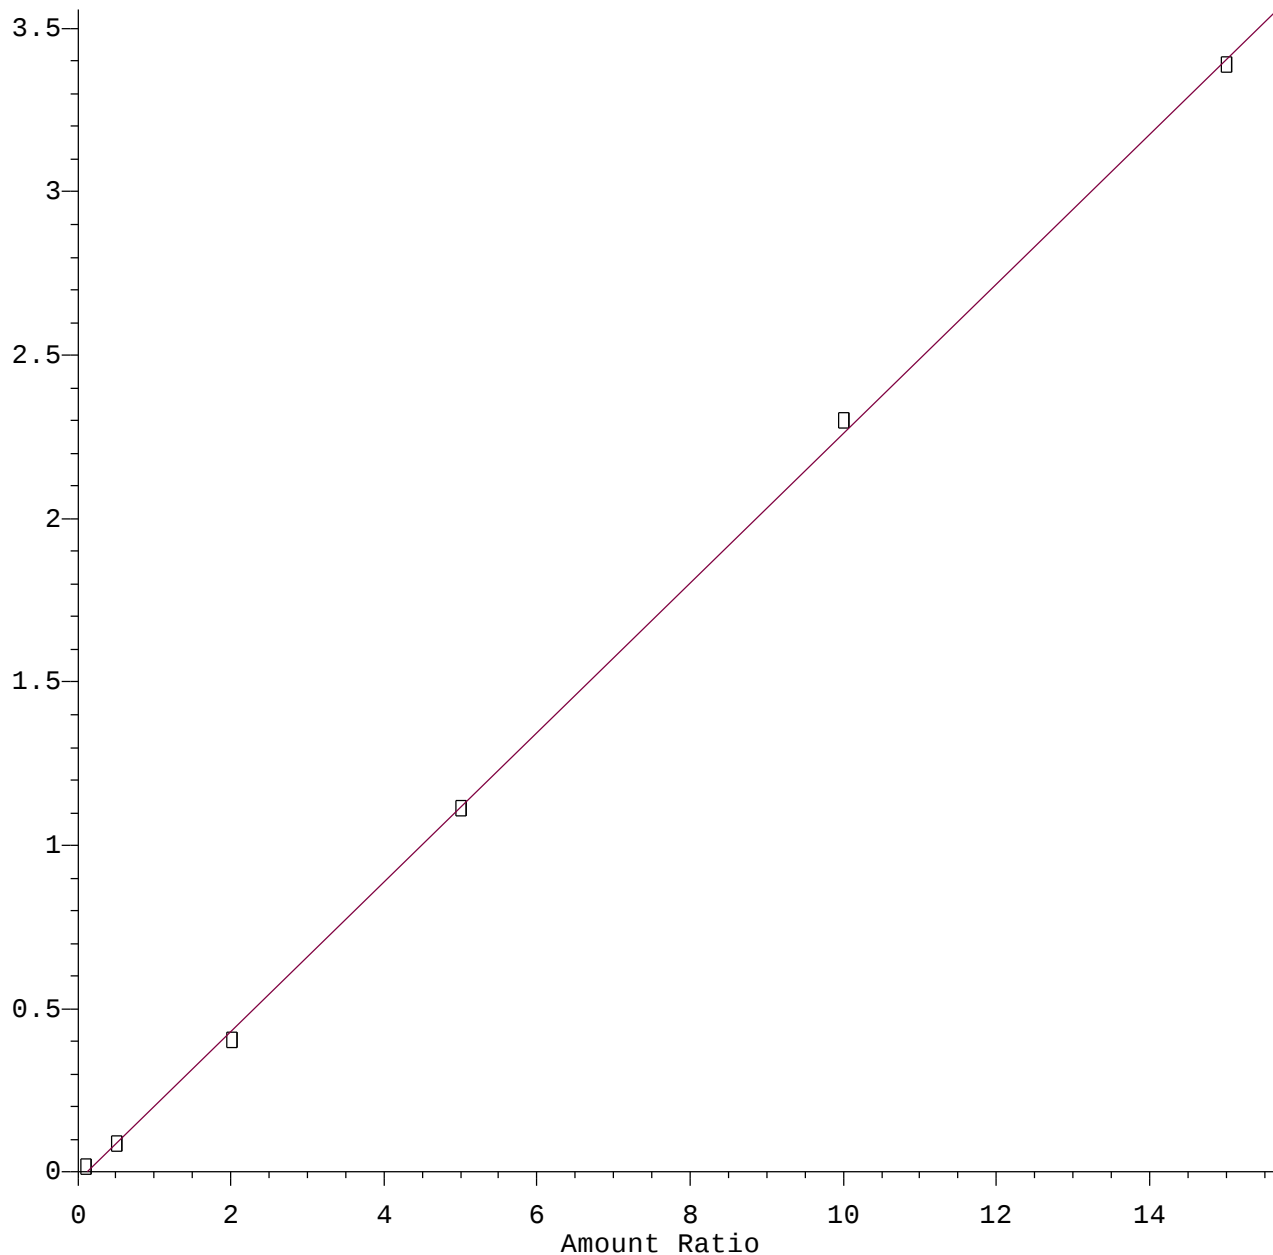

Resp Ratio = $2.29 \times 10^{-1} \times \text{Amt} - 2.61 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

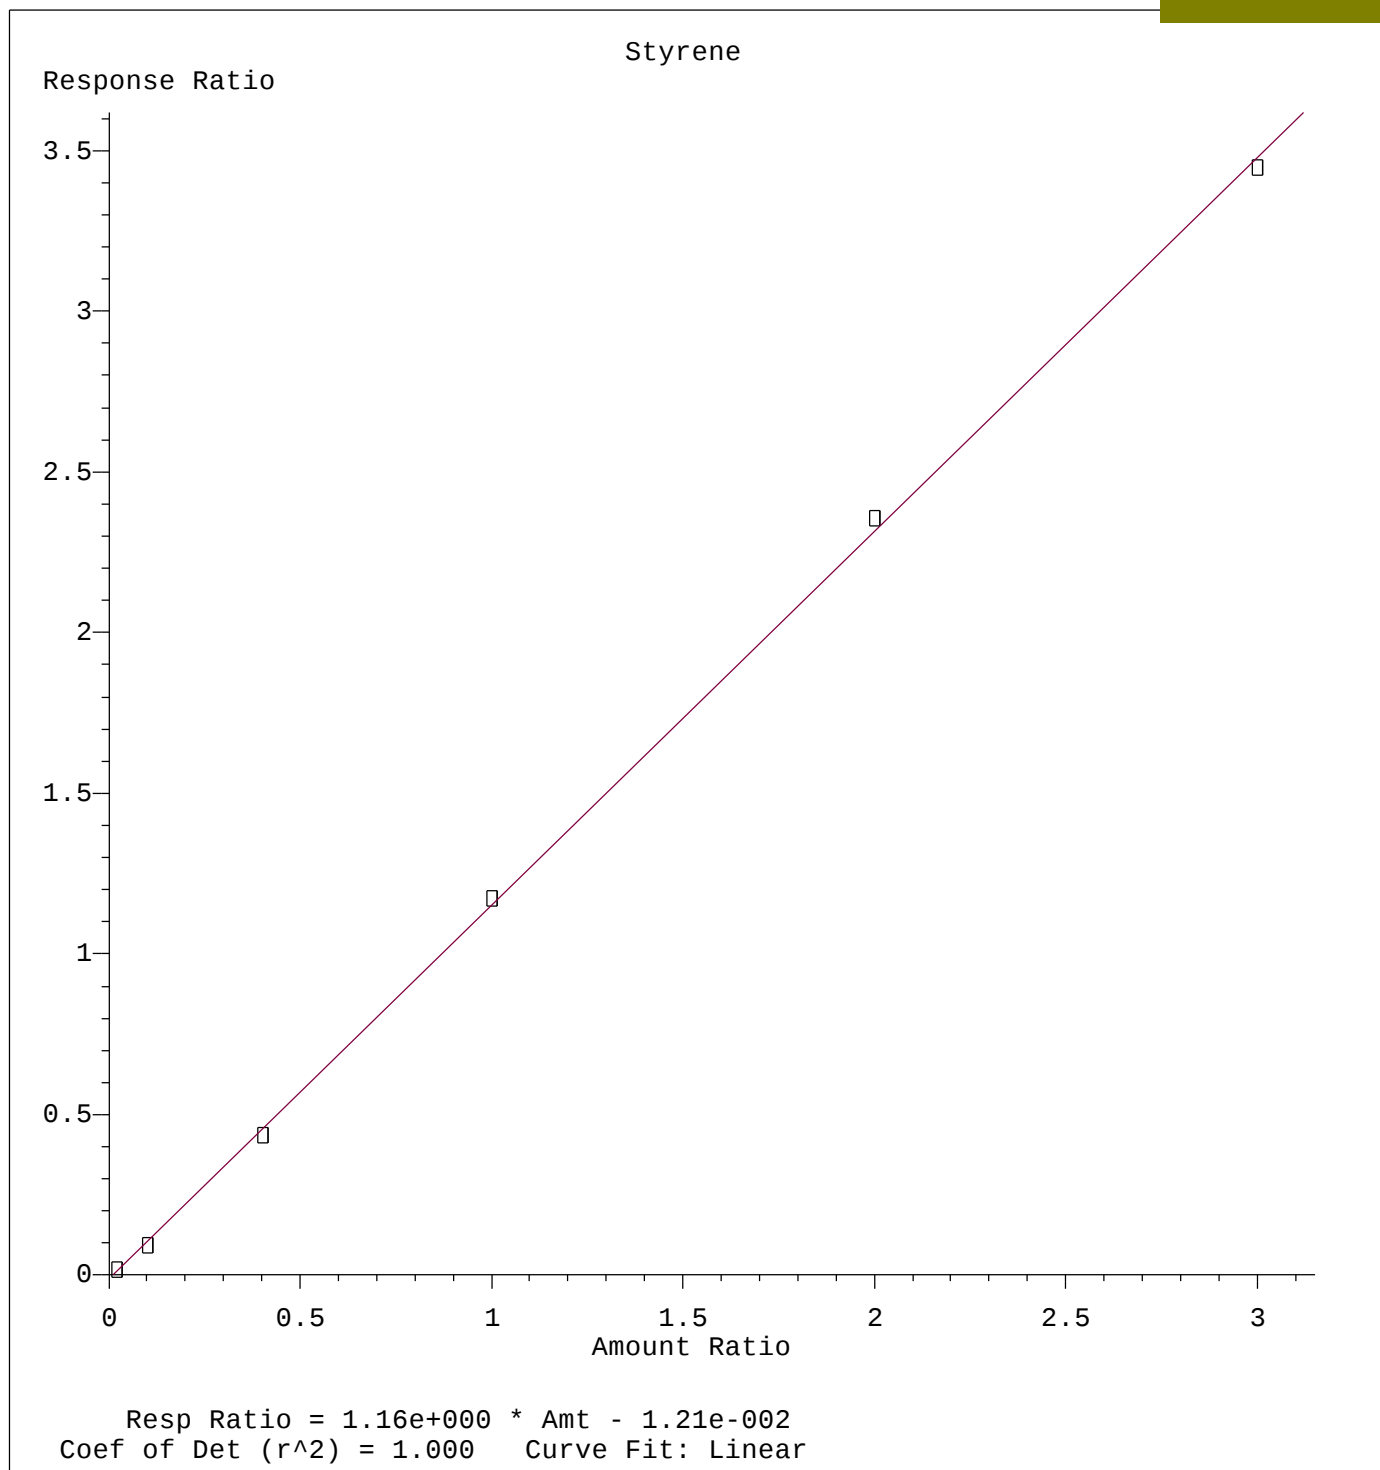

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

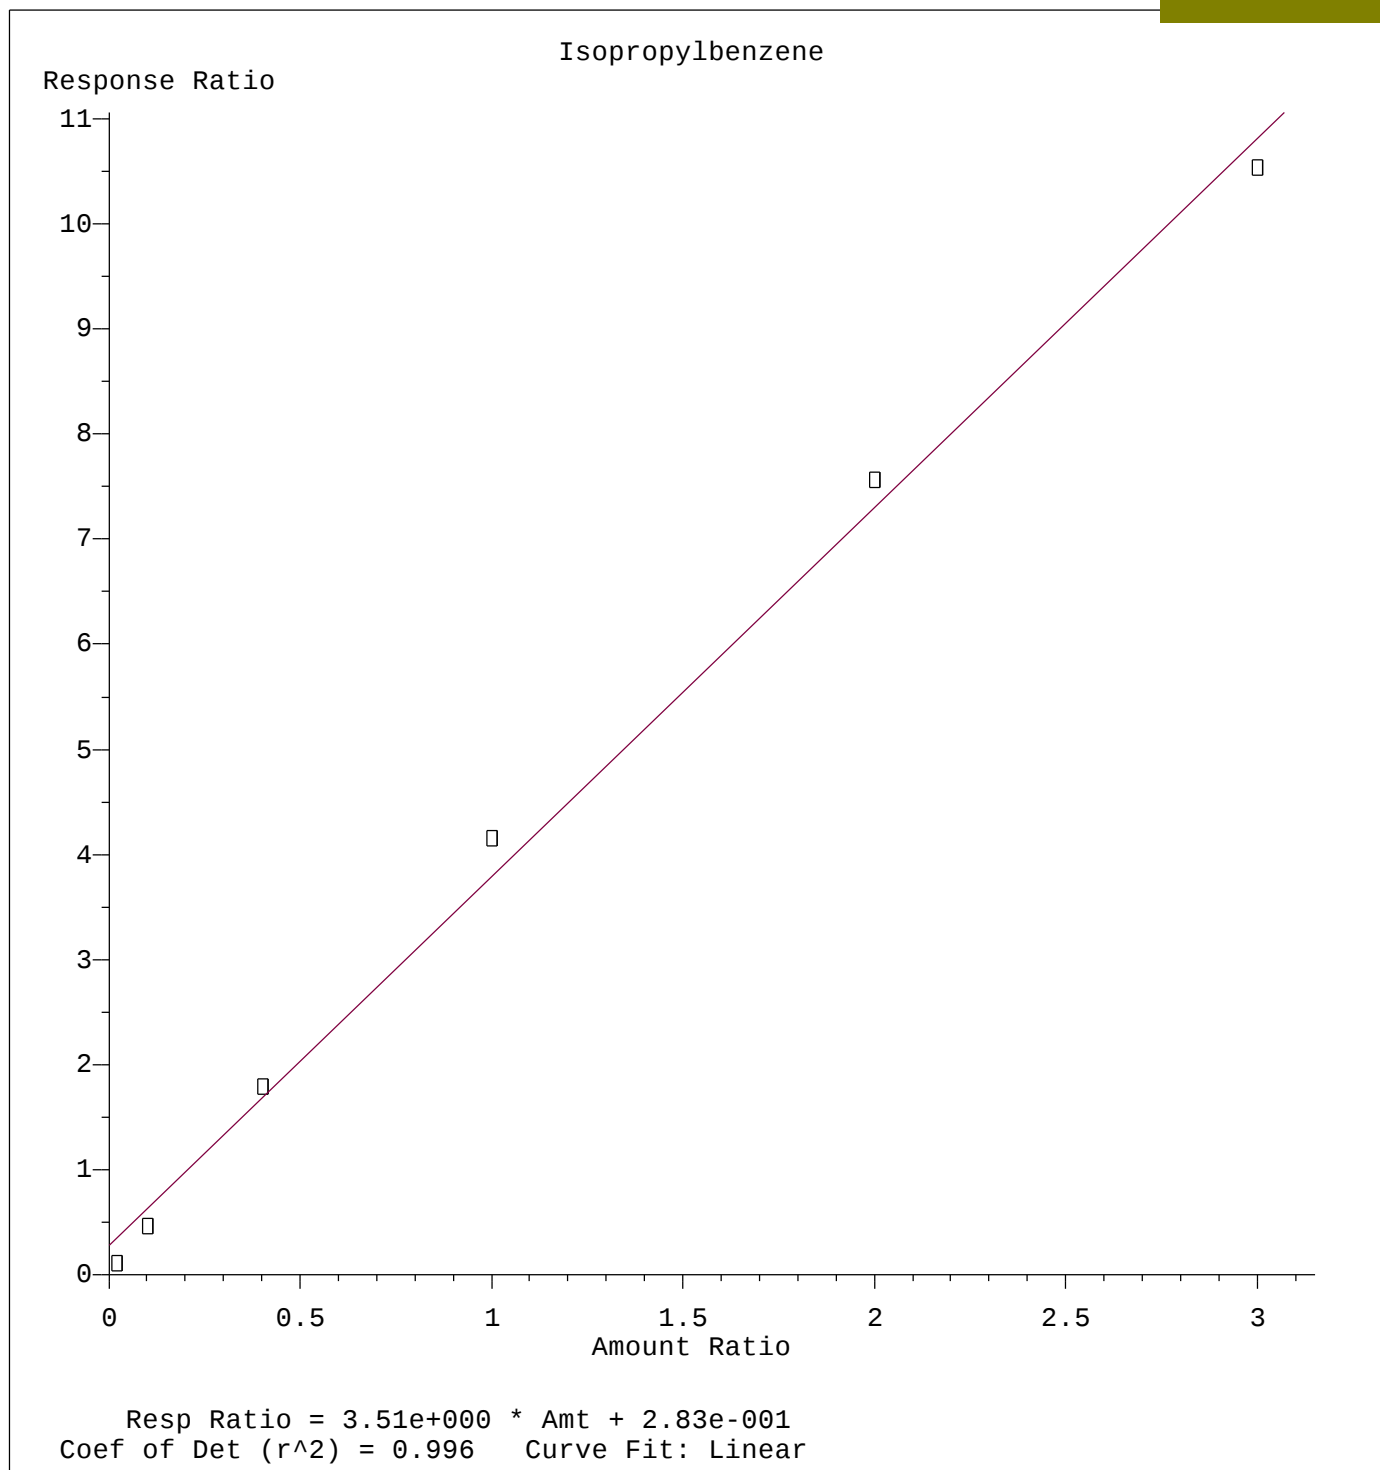


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

1,1,2,2-Tetrachloroethane

Response Ratio

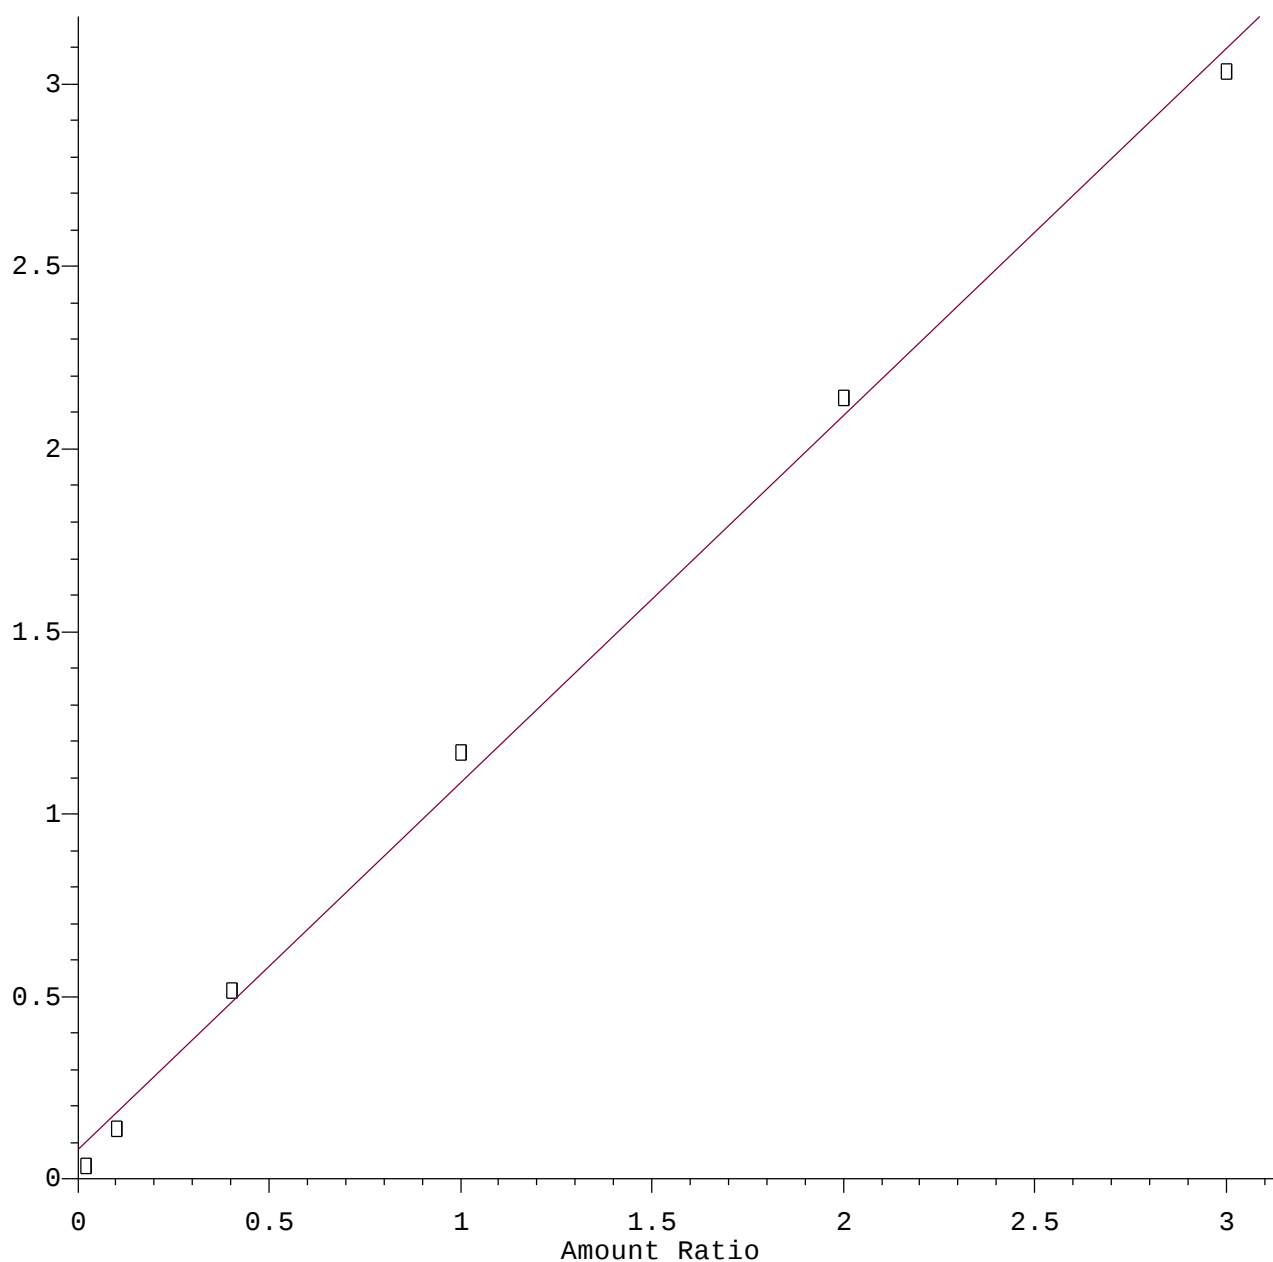


Resp Ratio = 1.01e+000 * Amt + 7.89e-002
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

2-Chlorotoluene

Response Ratio

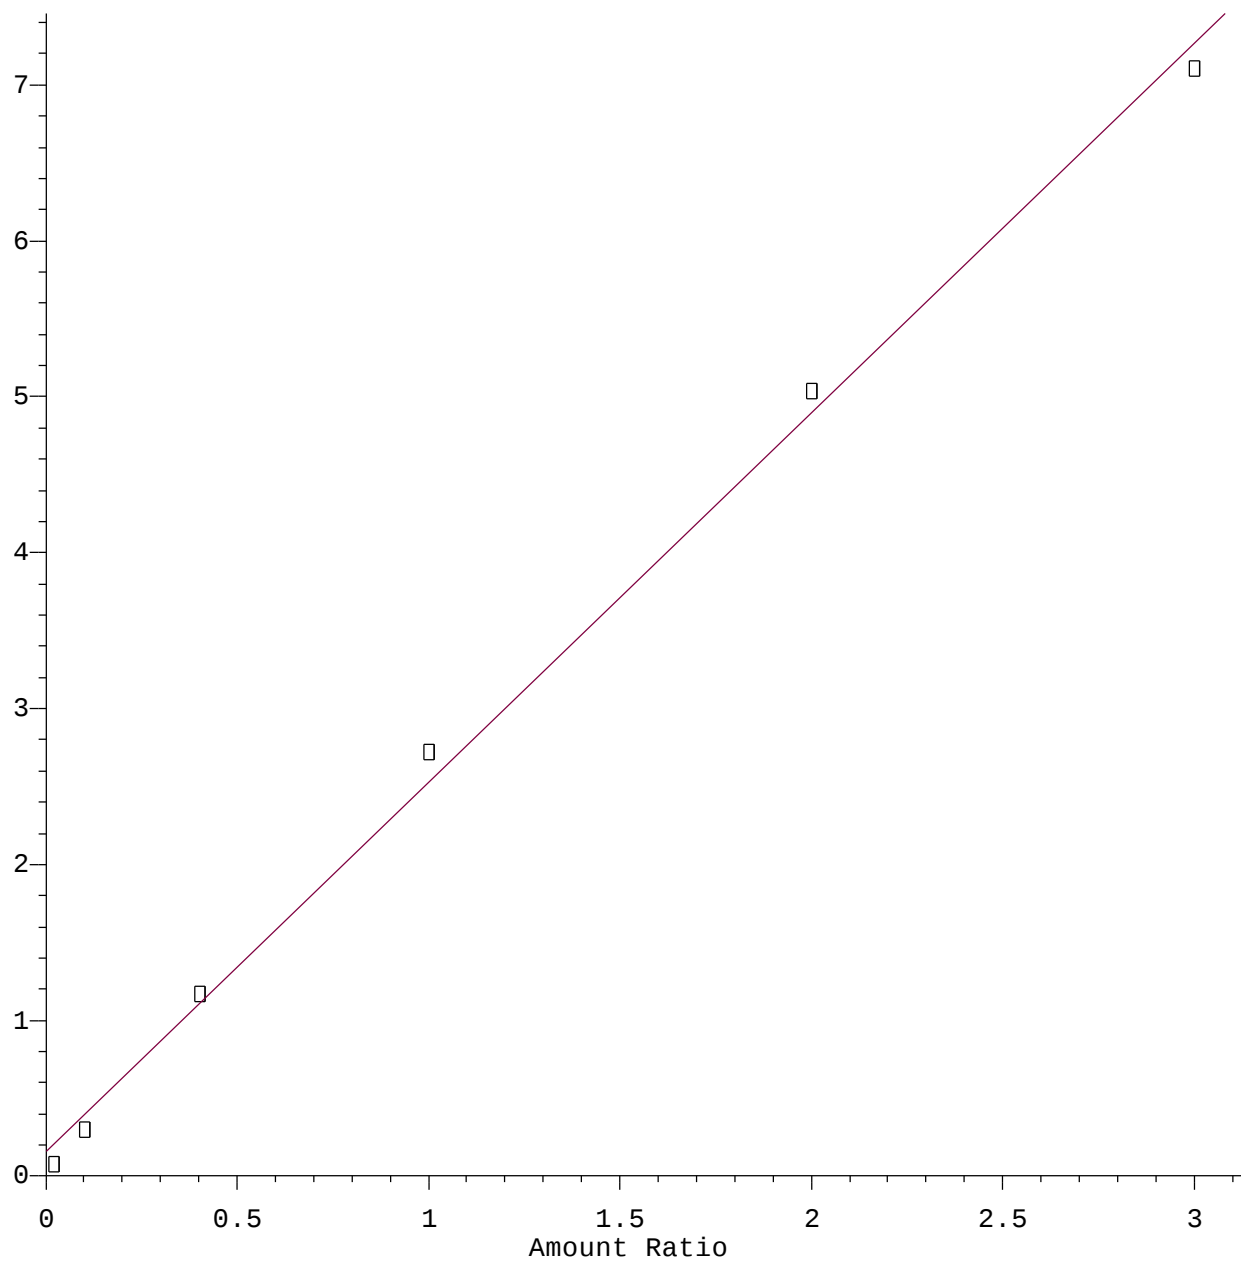


Resp Ratio = 2.37e+000 * Amt + 1.60e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

1,3,5-Trimethylbenzene

Response Ratio

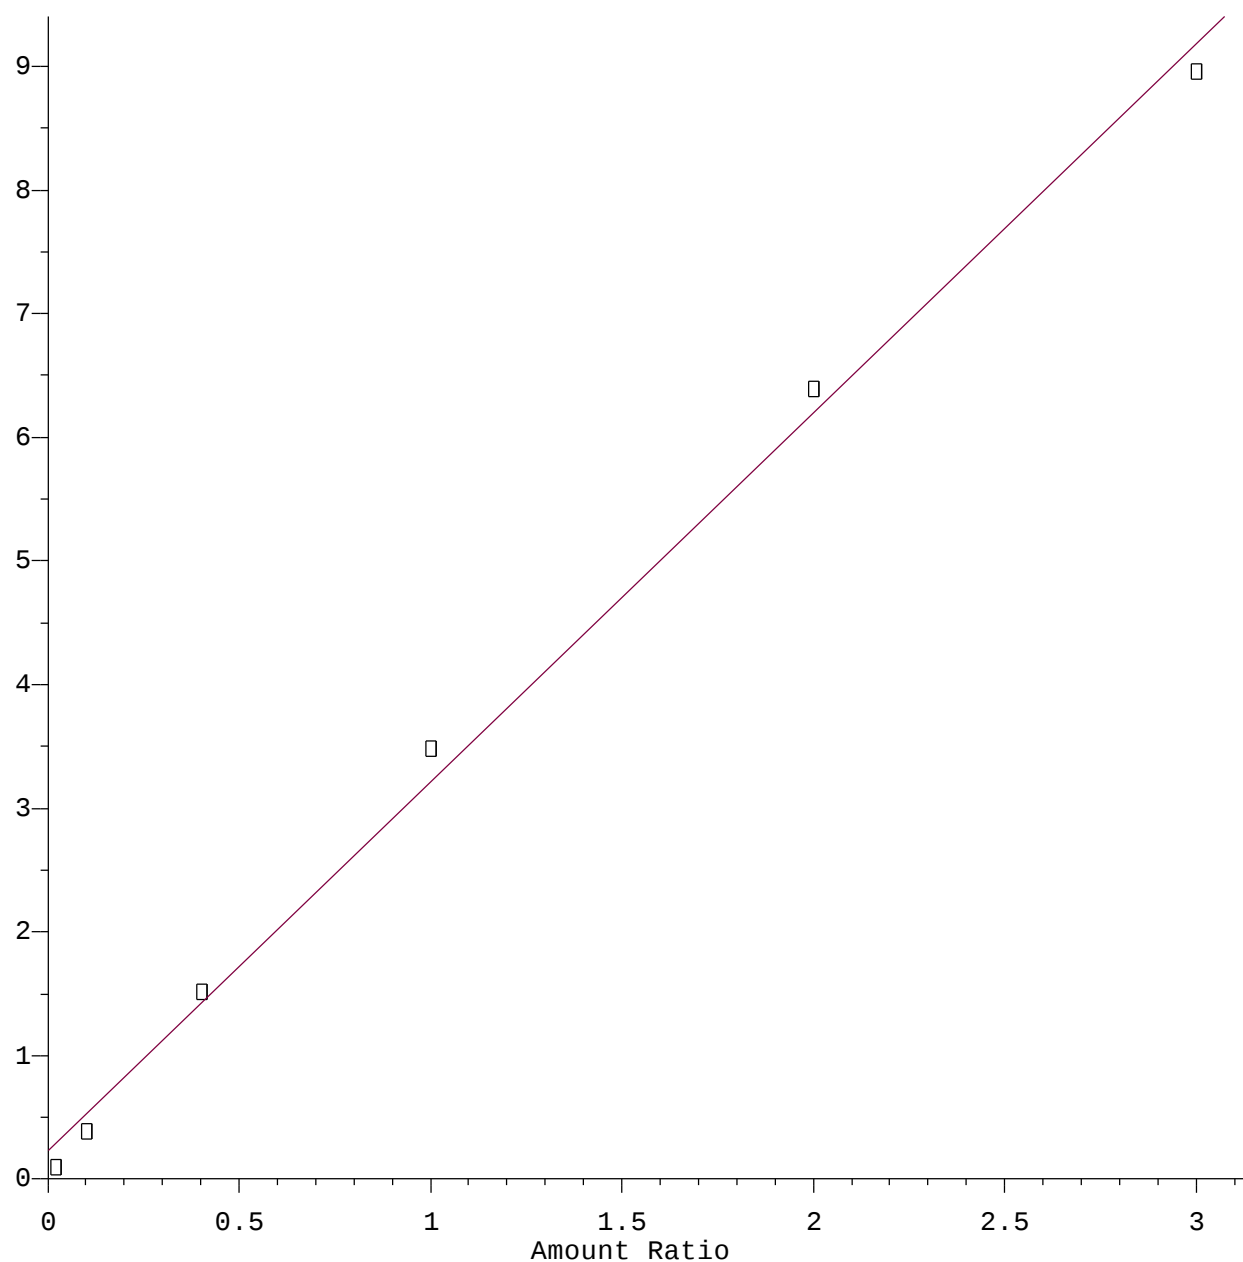


Resp Ratio = 2.99e+000 * Amt + 2.24e-001
Coef of Det (r^2) = 0.996 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

tert-Butylbenzene


Response Ratio

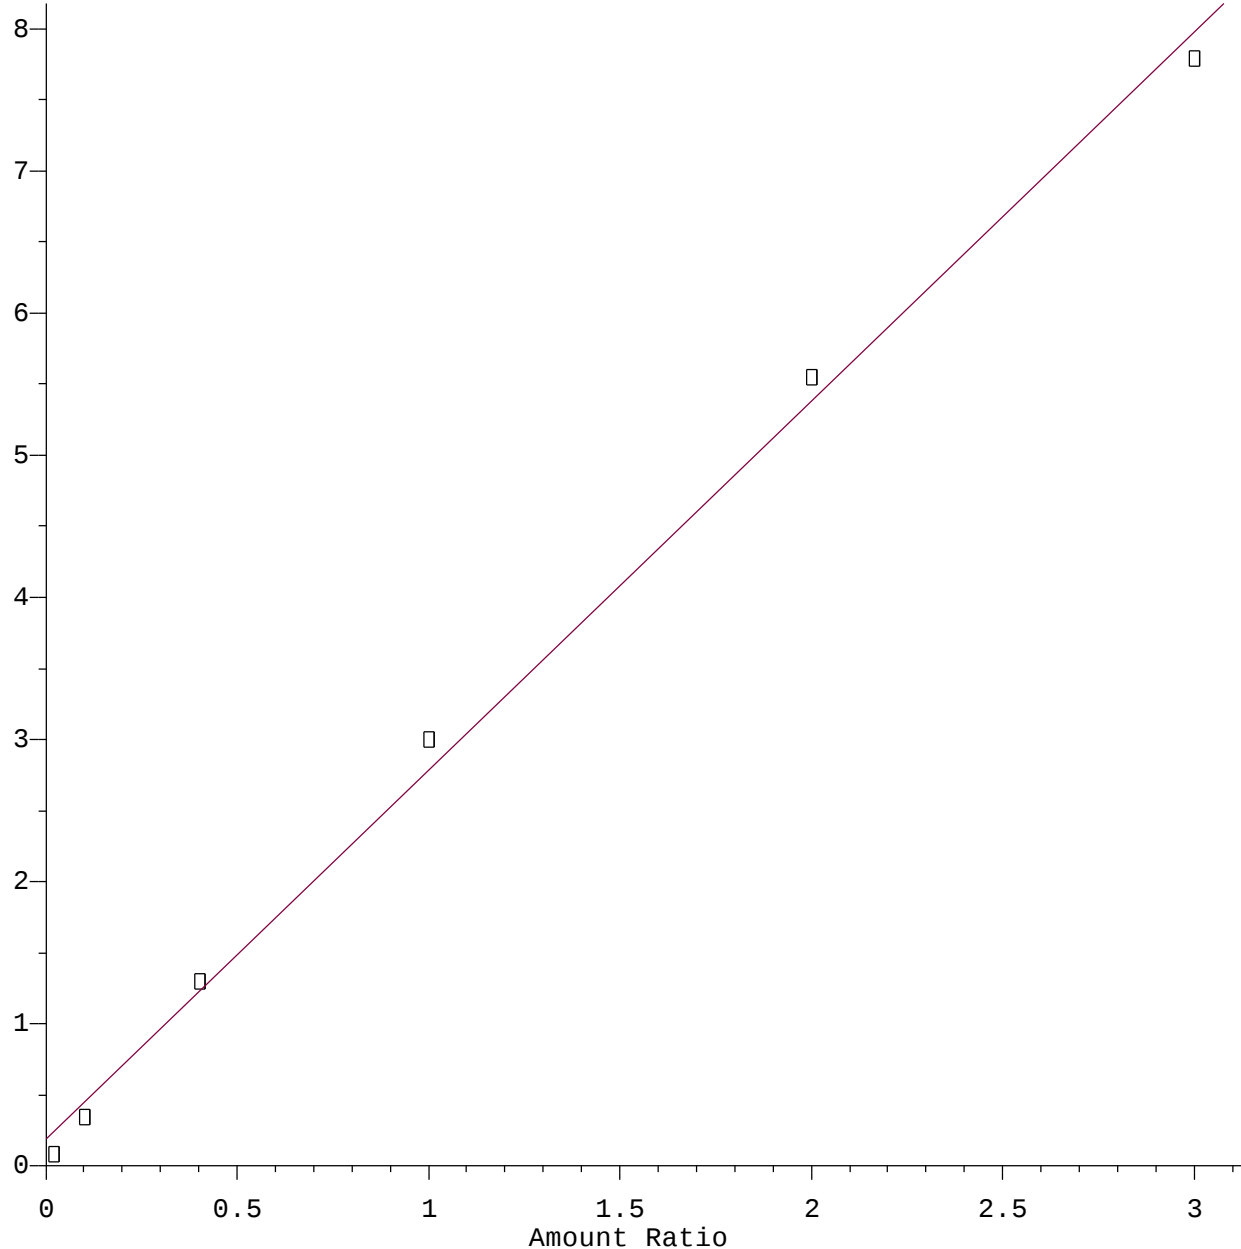

Resp Ratio = 2.59e+000 * Amt + 1.87e-001
Coef of Det (r^2) = 0.997 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

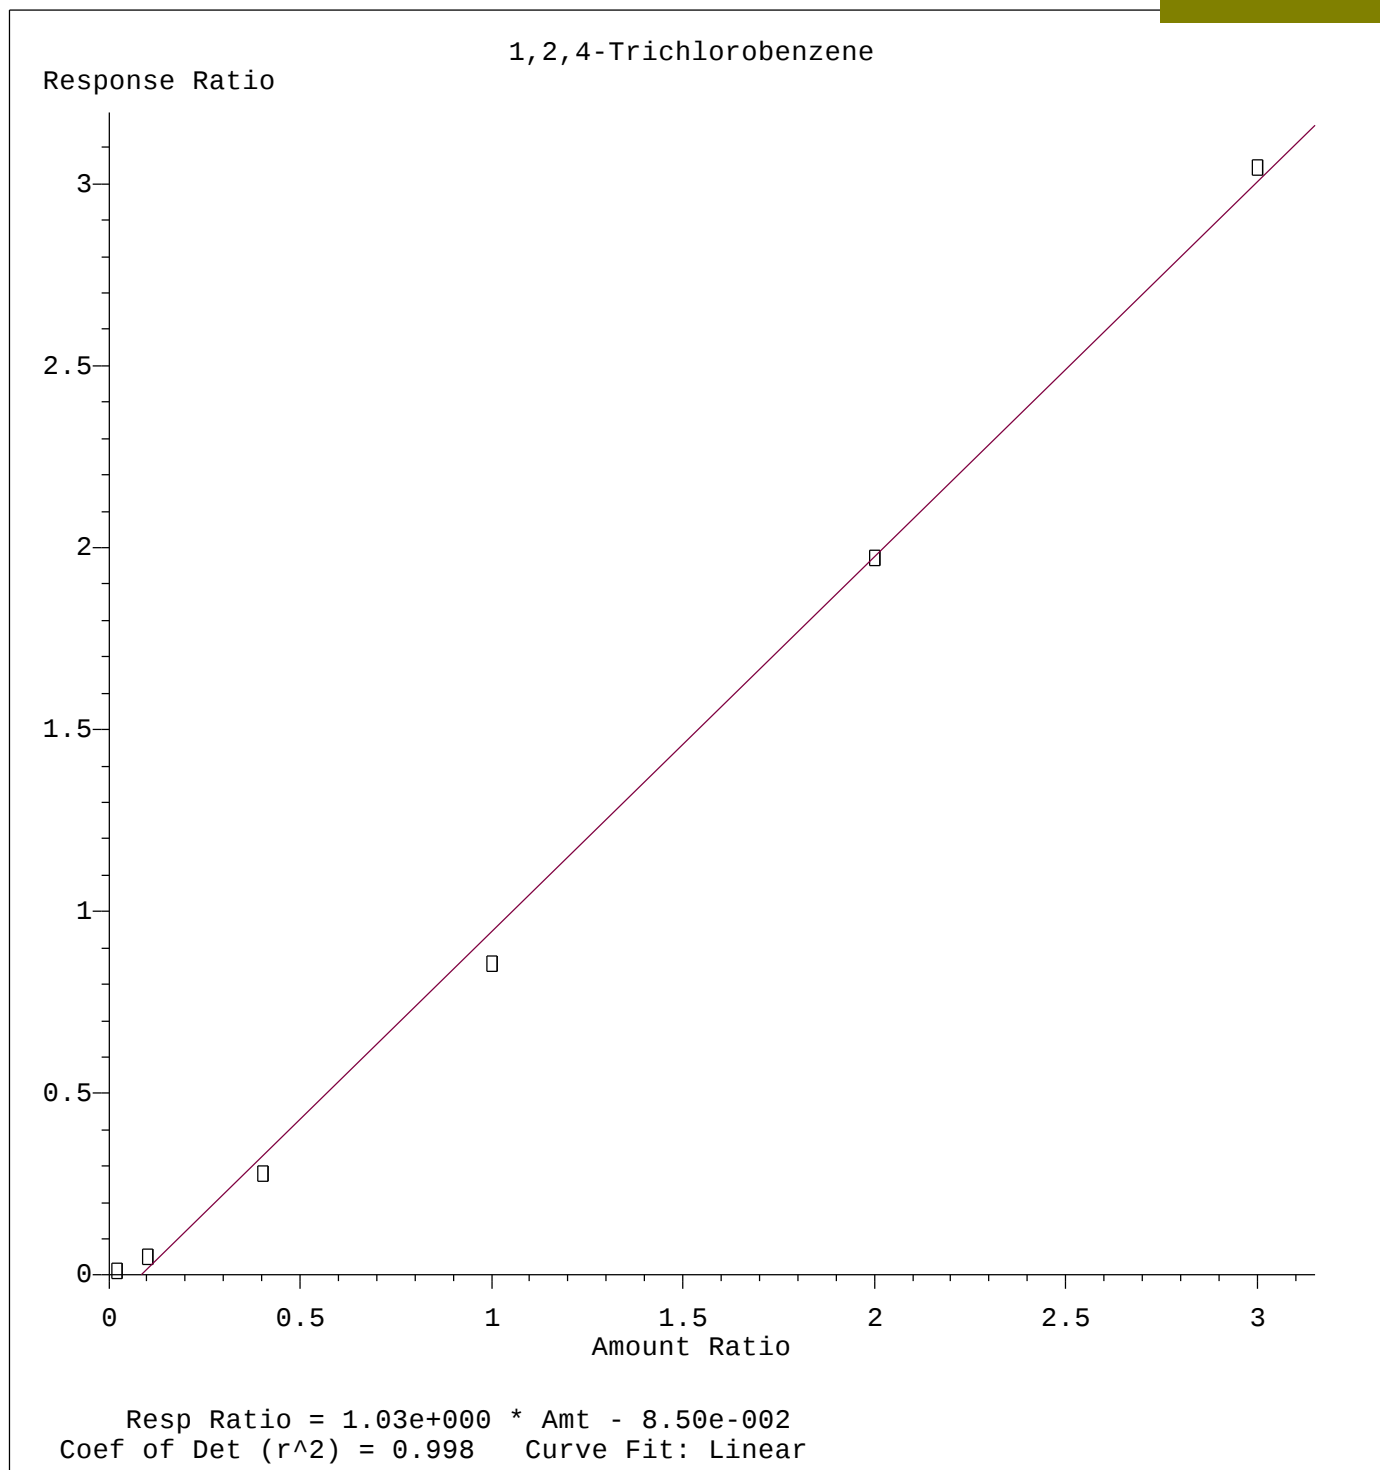

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

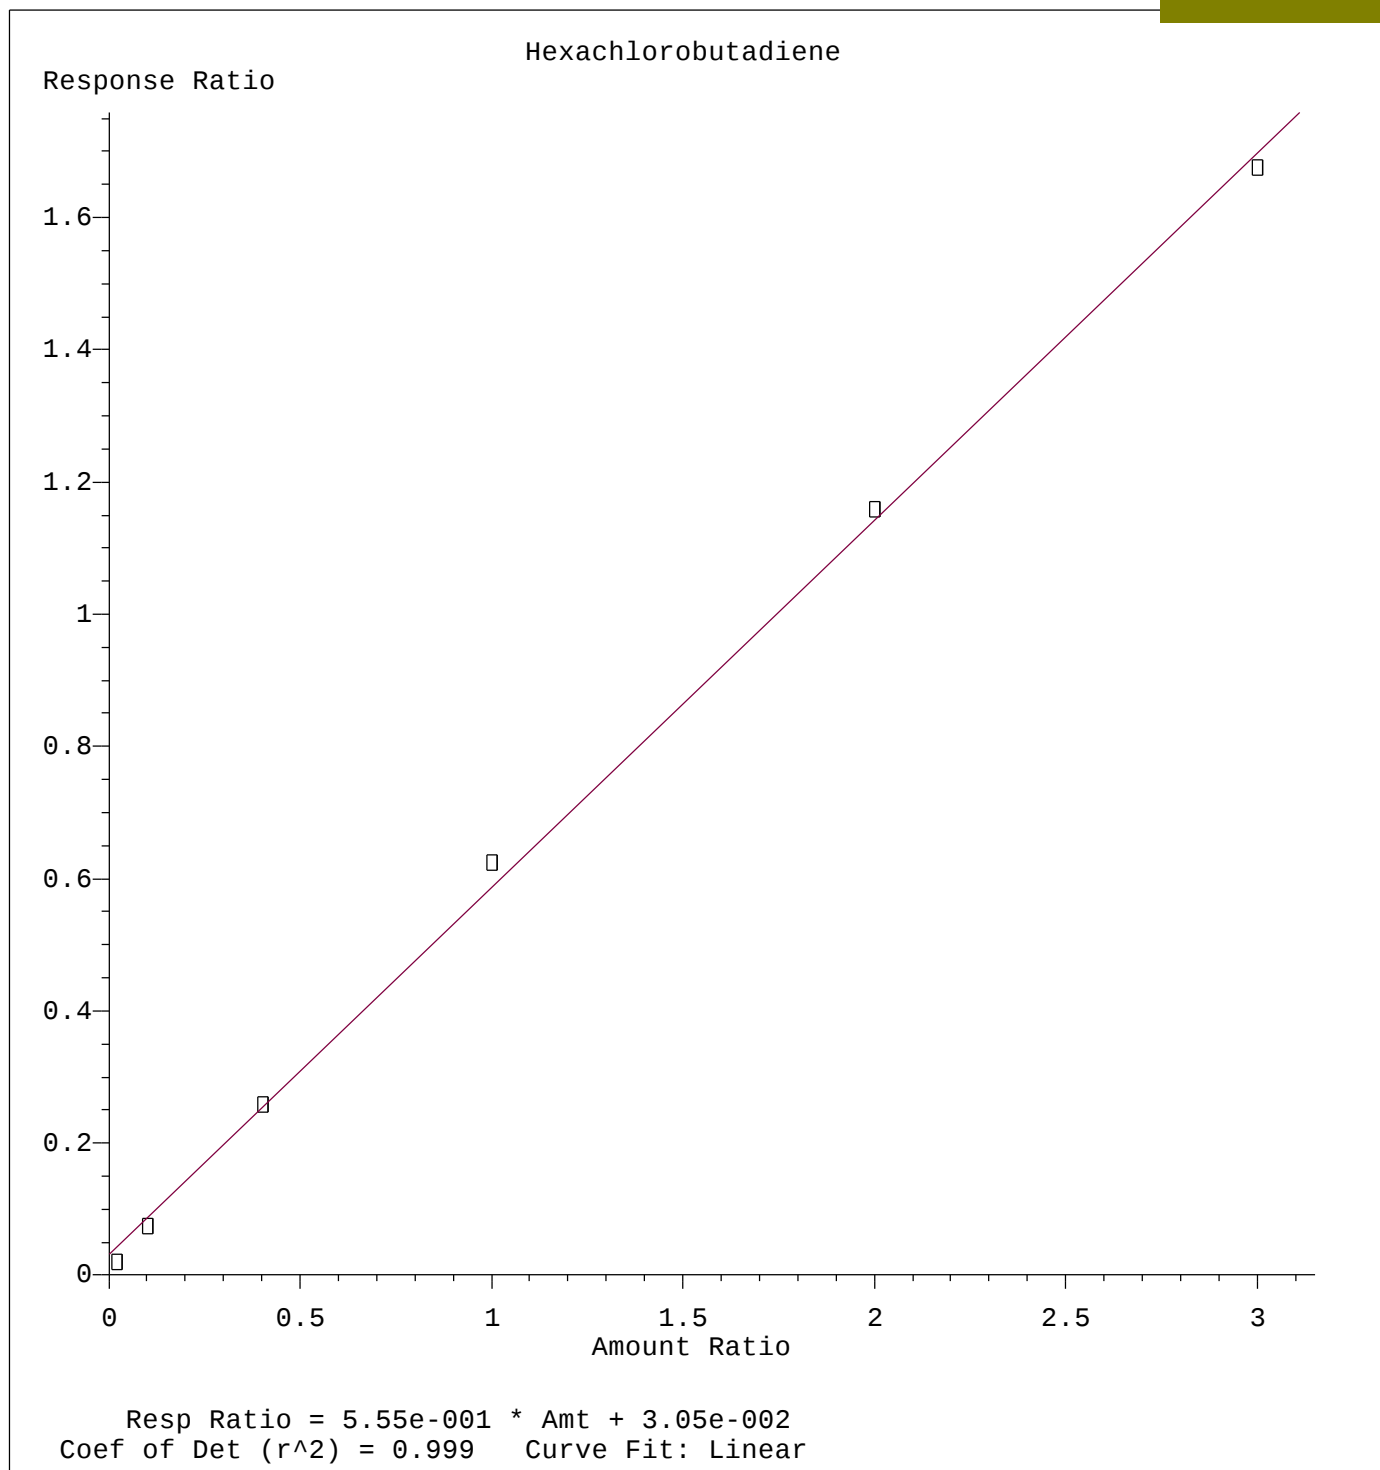


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

Naphthalene

Response Ratio

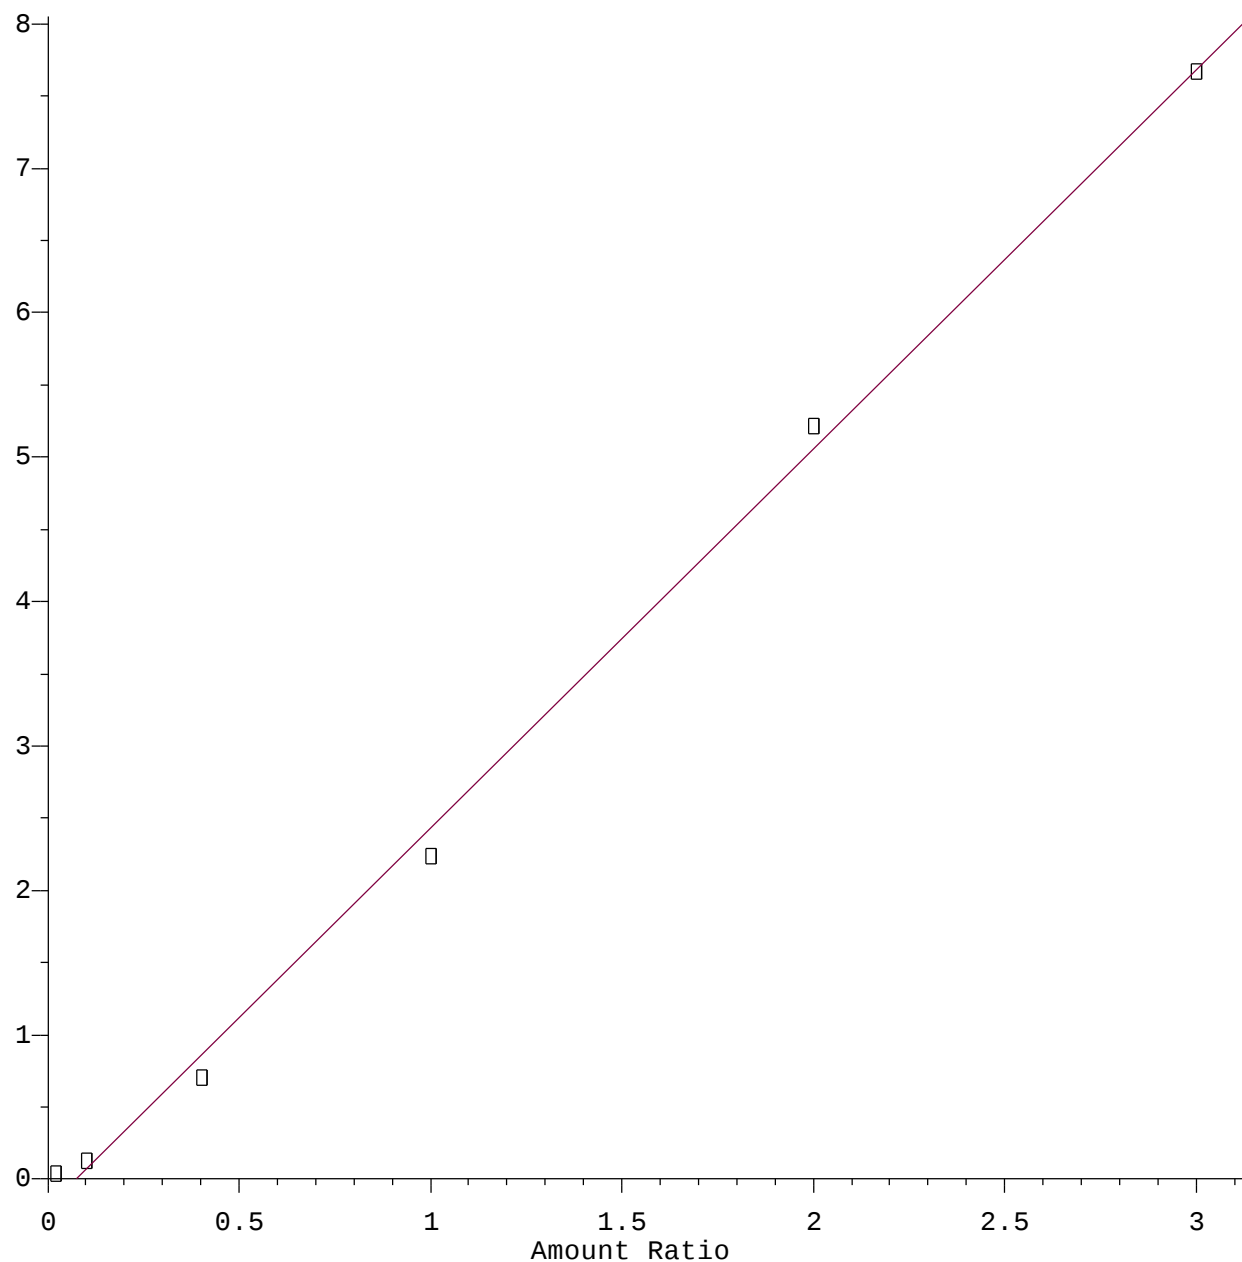


Resp Ratio = 2.62e+000 * Amt - 1.90e-001
Coef of Det (r^2) = 0.998 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019

Instrument :
MSVOA_N
ClientSampleId :

1,2,3-Trichlorobenzene

Response Ratio

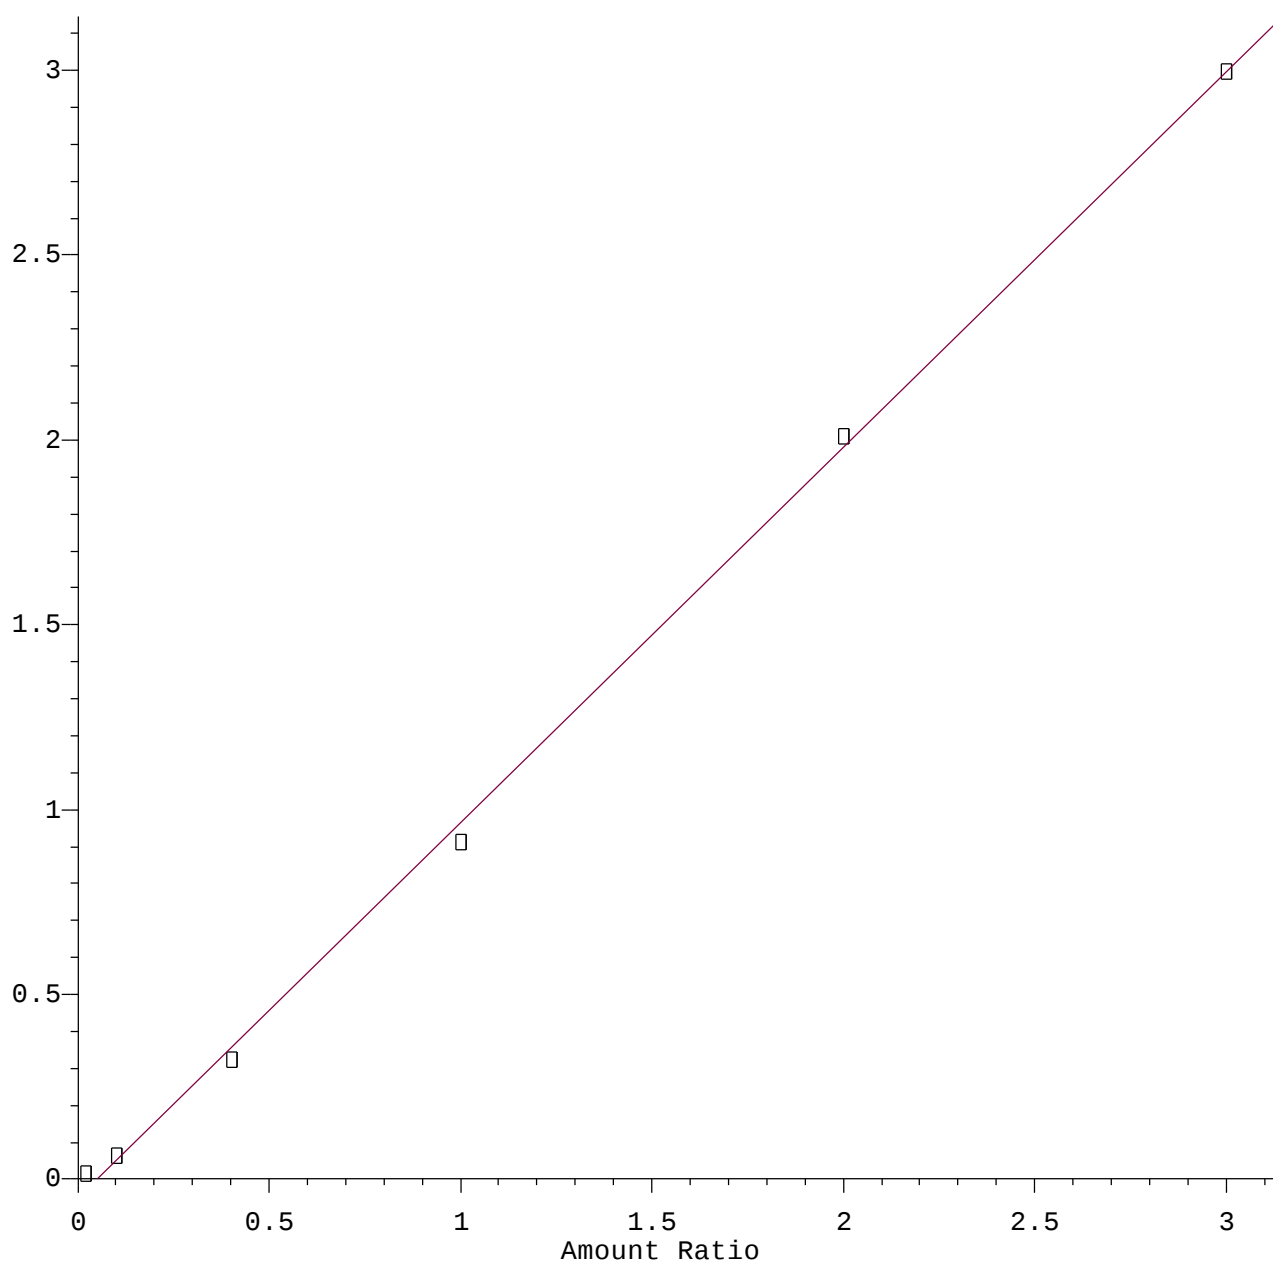

Resp Ratio = 1.01e+000 * Amt - 5.01e-002
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N072219W.M
Calibration Table Last Updated: Thu Jul 25 15:04:50 2019